

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
 Data File : PS001903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2018 11:32
 Operator : EI\SJ
 Sample : J5199-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 14:49:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.455	10.945	77507615	80753311	345.529	317.906
Target Compounds							
1) T	Dalapon	2.886	2.363	-2017365	25459584	N.D.	86.182
2) T	3,5-DICHL...	0.000	9.100	0	3883548	N.D.	12.304 #
6) T	MCP	12.123	0.000	23736123	0	37.249	N.D. #
12) T	2,4,5-T	0.000	14.568	0	3052316	N.D.	2.764 #
15) T	Picloram	16.973	16.880	19400284	30175975	11.142	17.743 #
16) T	DCPA	0.000	16.880	0	30175975	N.D.	16.361 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
Data File : PS001903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2018 11:32
Operator : EI\SJ
Sample : J5199-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 14:49:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

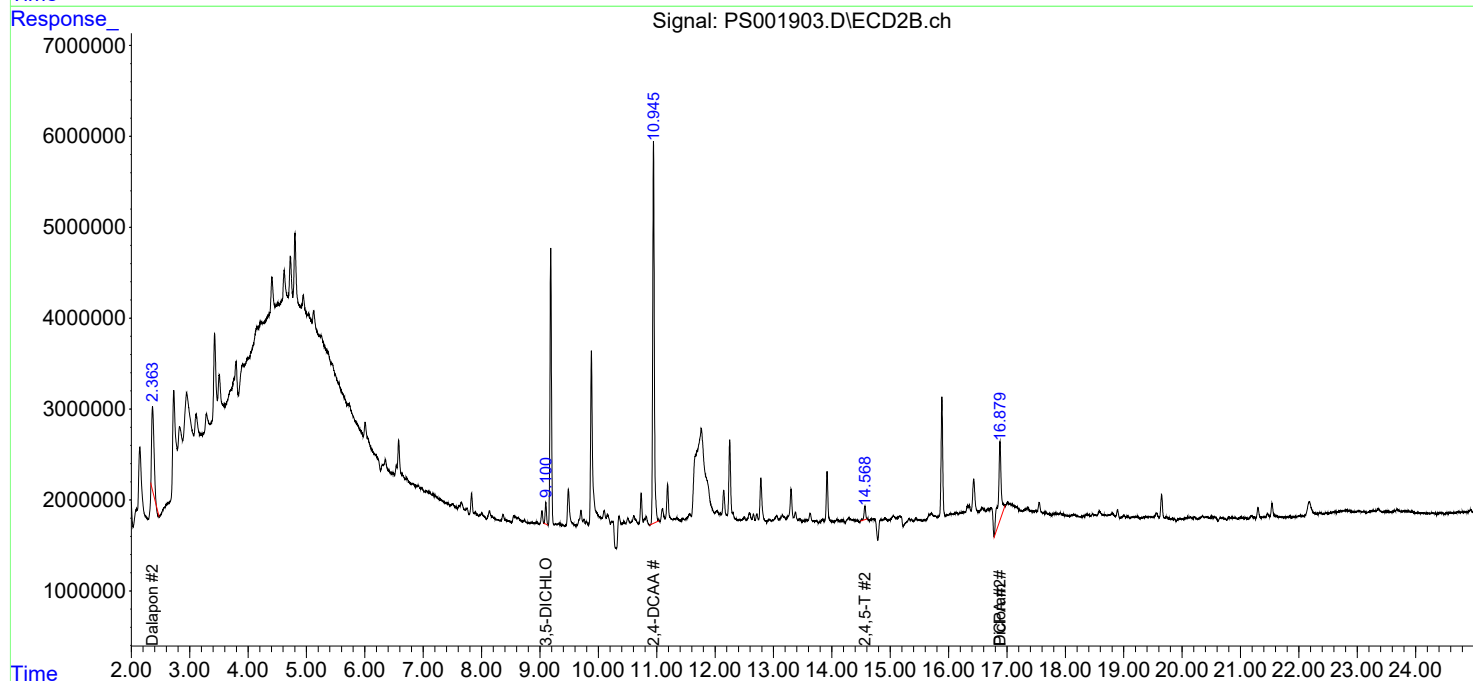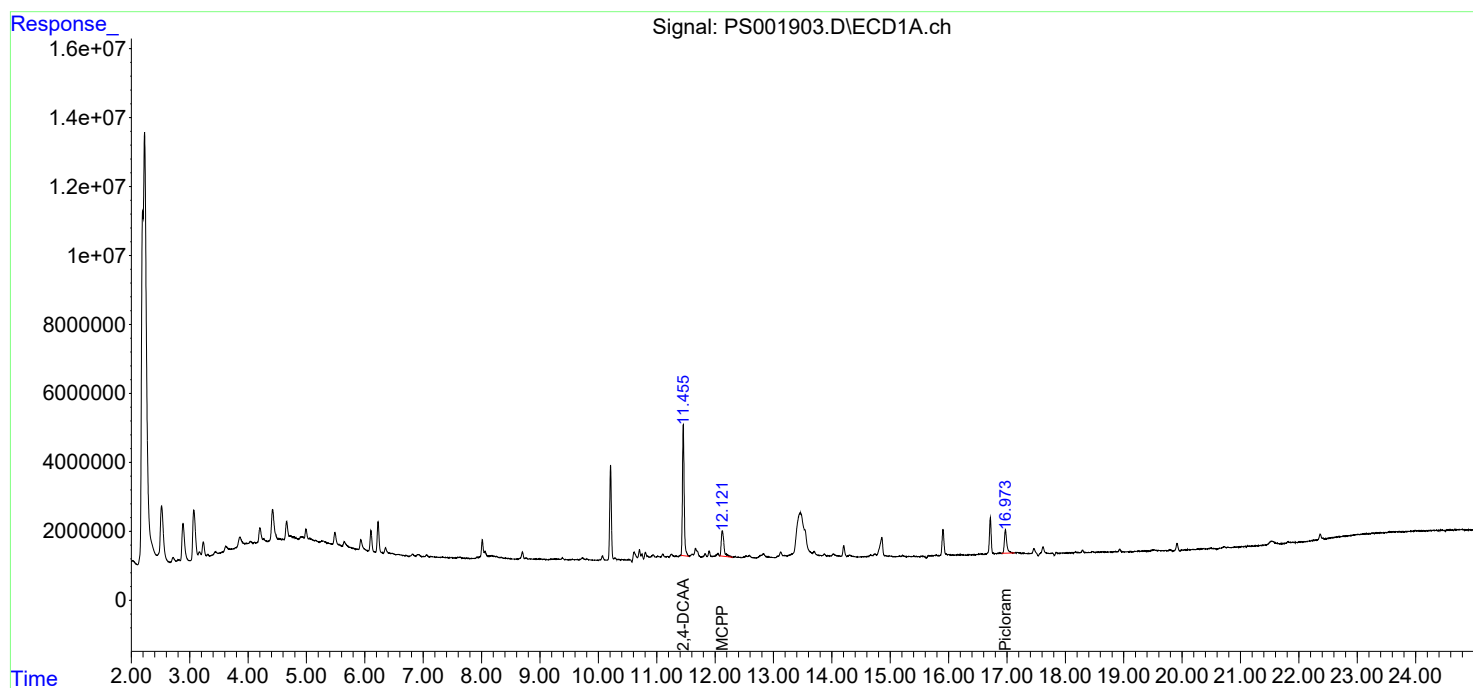


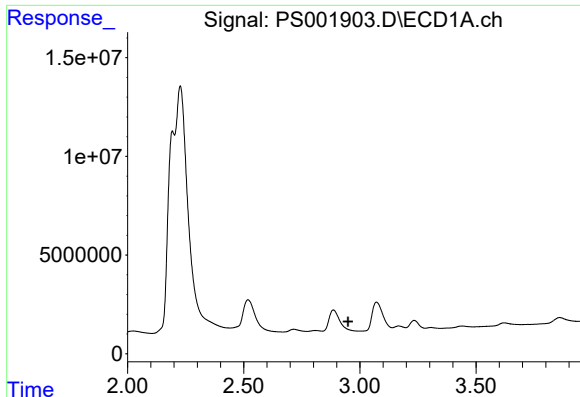

#1 Dalapon


R.T.: 2.886 min
Delta R.T.: -0.063 min
Response: -2017365
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

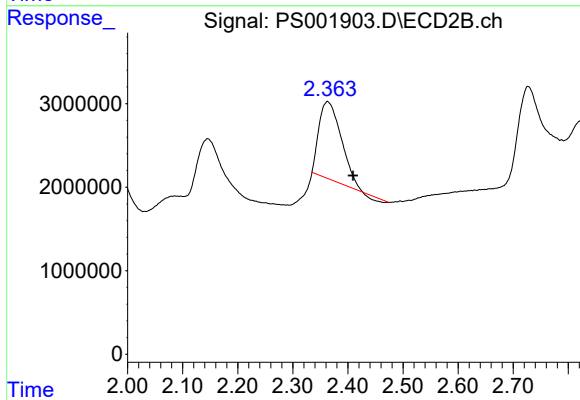


#1 Dalapon

R.T.: 2.363 min
Delta R.T.: -0.047 min
Response: 25459584
Conc: 86.18 ng/ml

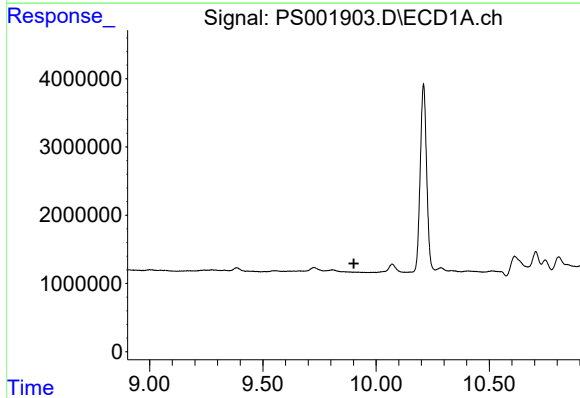


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.902 min
Response: 0
Conc: N.D.

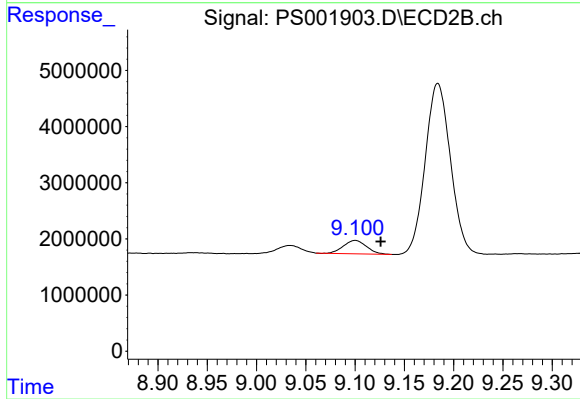

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.100 min
Delta R.T.: -0.026 min
Response: 3883548
Conc: 12.30 ng/ml

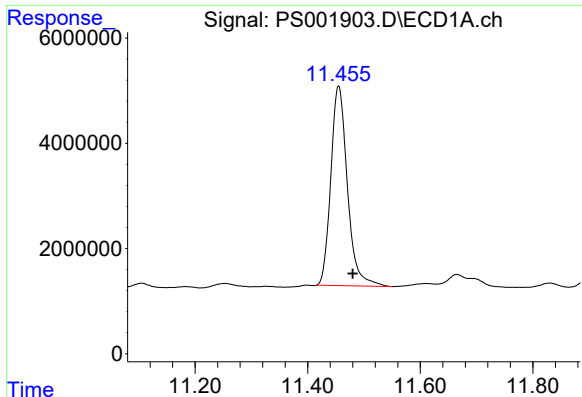

#4 2,4-DCAA


R.T.: 11.455 min
Delta R.T.: -0.025 min
Response: 77507615
Conc: 345.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

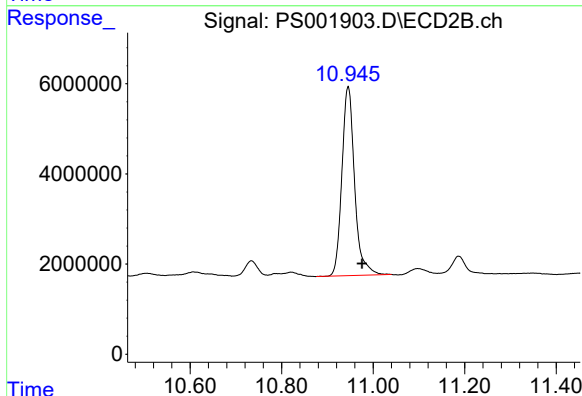


#4 2,4-DCAA

R.T.: 10.945 min
Delta R.T.: -0.031 min
Response: 80753311
Conc: 317.91 ng/ml

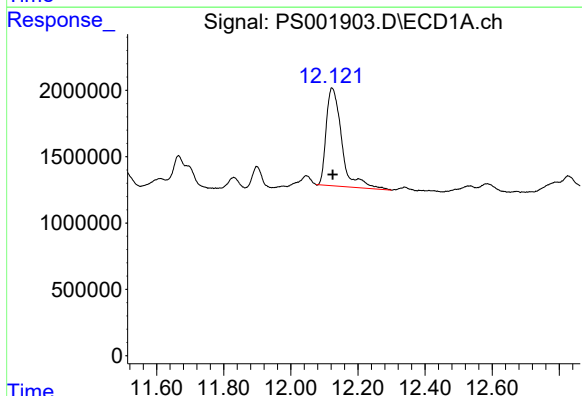


#6 MCP

R.T.: 12.123 min
Delta R.T.: -0.002 min
Response: 23736123
Conc: 37.25 ug/ml

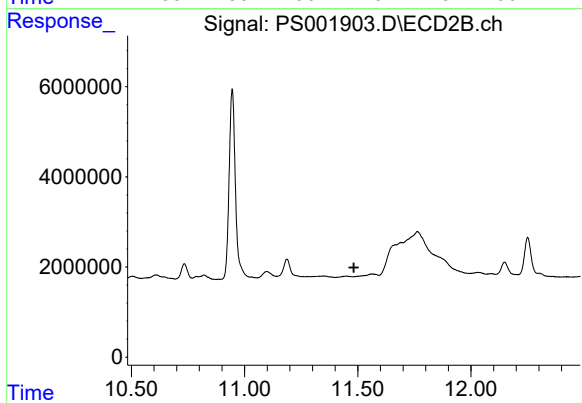

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

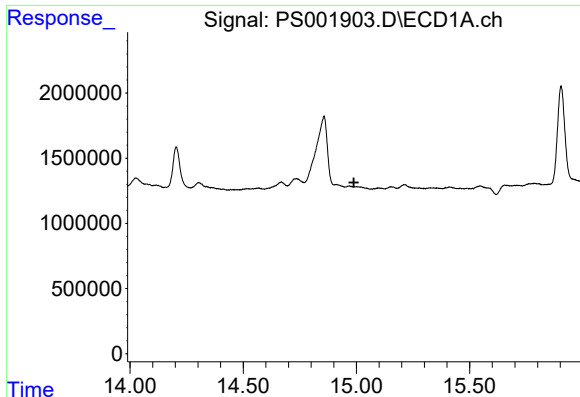

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

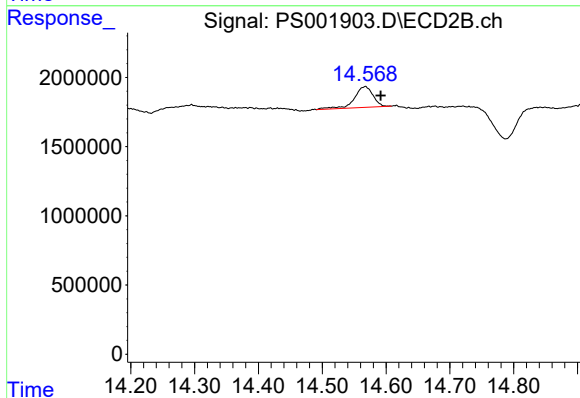


#12 2,4,5-T

R.T.: 14.568 min
Delta R.T.: -0.024 min
Response: 3052316
Conc: 2.76 ng/ml

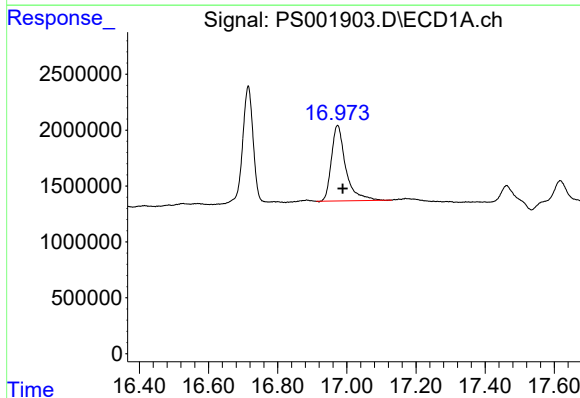


#15 Picloram

R.T.: 16.973 min
Delta R.T.: -0.015 min
Response: 19400284
Conc: 11.14 ng/ml

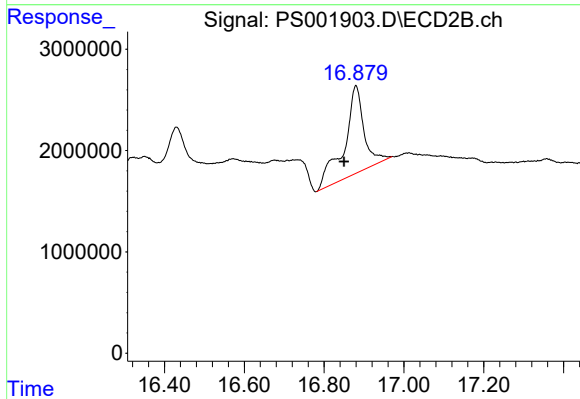

#15 Picloram


R.T.: 16.880 min
Delta R.T.: 0.030 min
Response: 30175975
Conc: 17.74 ng/ml

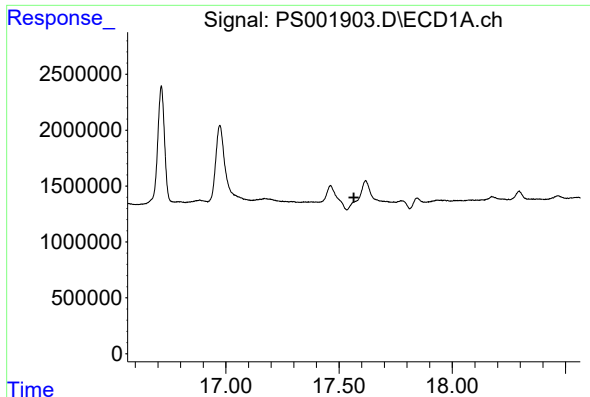

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

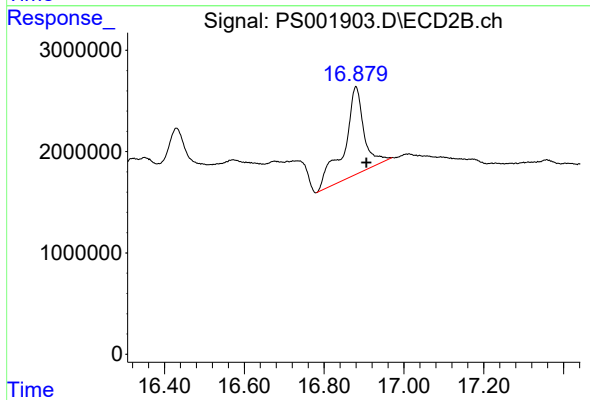

#16 DCPA

R.T.: 16.880 min
Delta R.T.: -0.026 min
Response: 30175975
Conc: 16.36 ng/ml