

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
 Data File : PS001906.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2018 13:05
 Operator : EI\SJ
 Sample : J5195-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 14:50:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.494	10.990	82844009	84373573	369.319	332.158
Target Compounds							
1) T	Dalapon	2.927	2.404	39175349	54031327	120.477	182.898 #
2) T	3,5-DICHL...	0.000	9.147	0	1758920	N.D.	5.573 #
5) T	DICAMBA	0.000	11.232	0	21989805	N.D.	24.656 #
6) T	MCP	12.179	0.000	20263634	0	31.799	N.D. #
9) T	2,4-D	0.000	12.824	0	5420300	N.D.	17.423 #
11) T	2,4,5-TP ...	0.000	13.977	0	18141624	N.D.	13.231 #
16) T	DCPA	0.000	16.920	0	1009699	N.D.	0.547 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
Data File : PS001906.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2018 13:05
Operator : EI\SJ
Sample : J5195-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 14:50:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

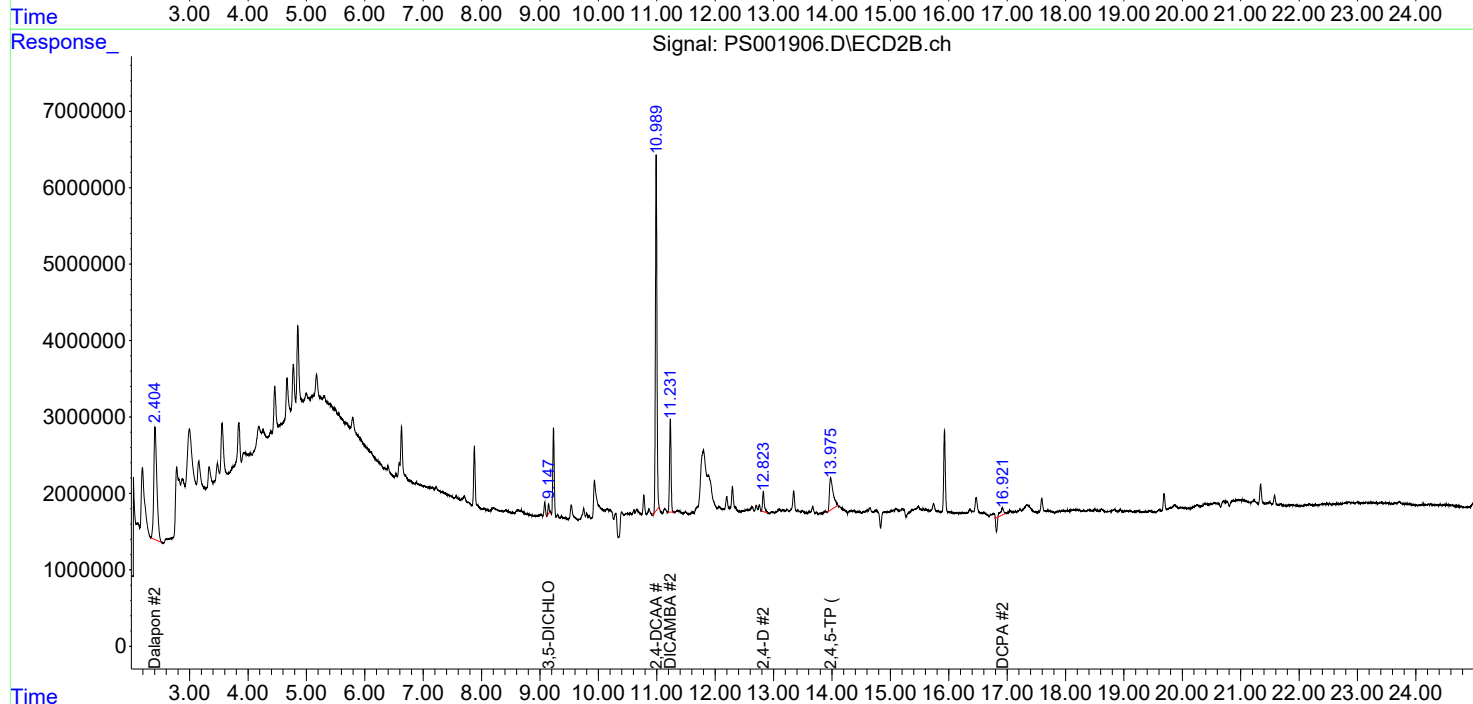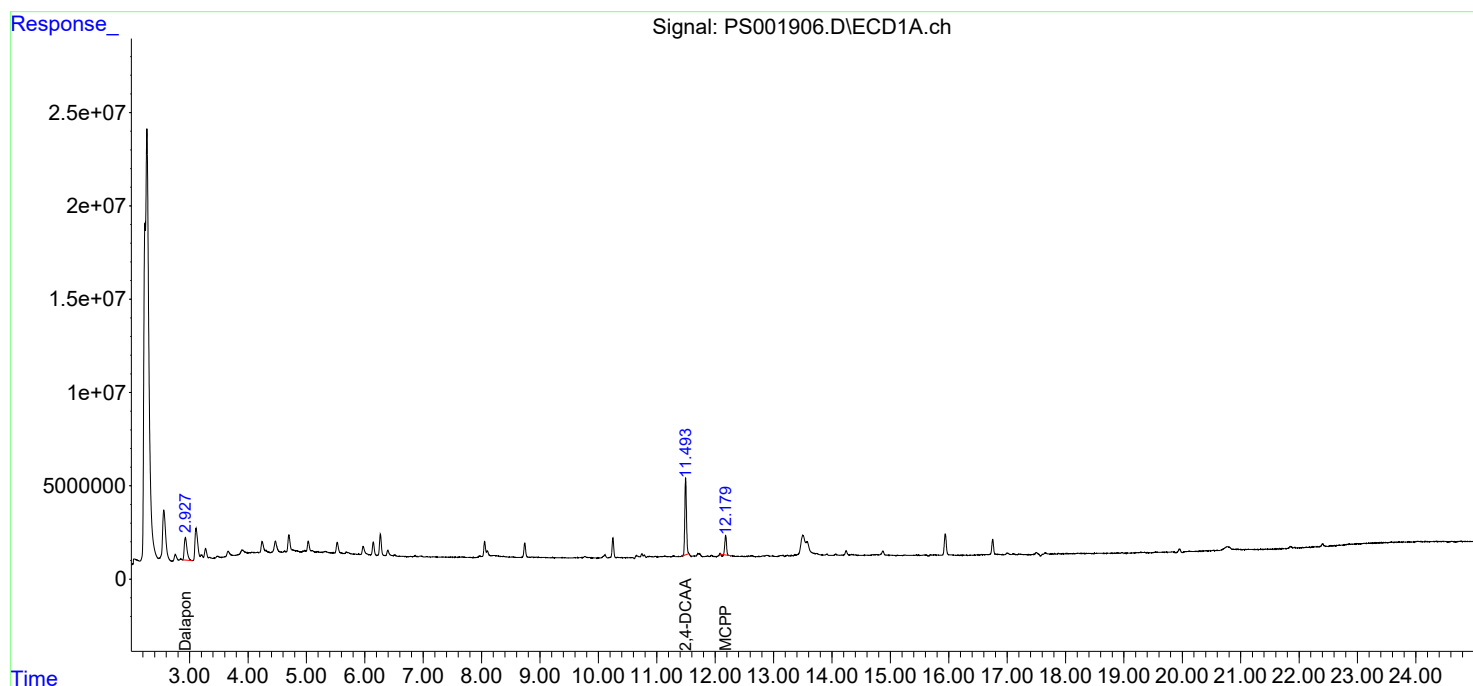


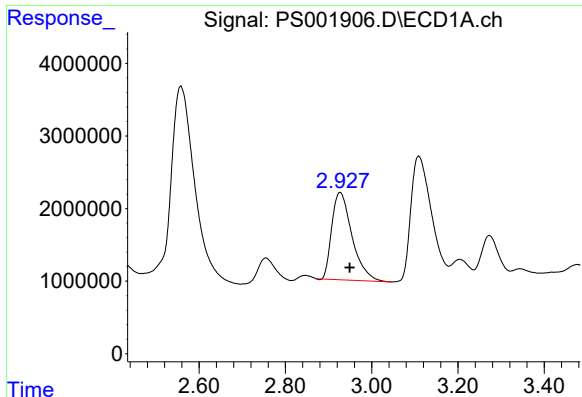

#1 Dalapon


R.T.: 2.927 min
Delta R.T.: -0.022 min
Response: 39175349
Conc: 120.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

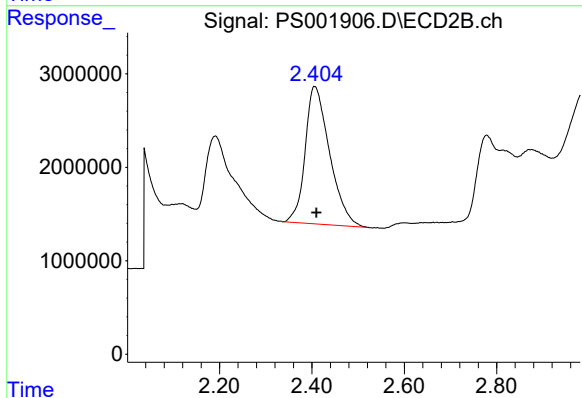


#1 Dalapon

R.T.: 2.404 min
Delta R.T.: -0.005 min
Response: 54031327
Conc: 182.90 ng/ml

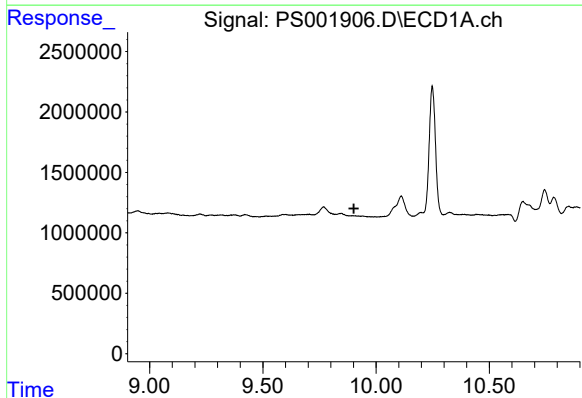


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.902 min
Response: 0
Conc: N.D.

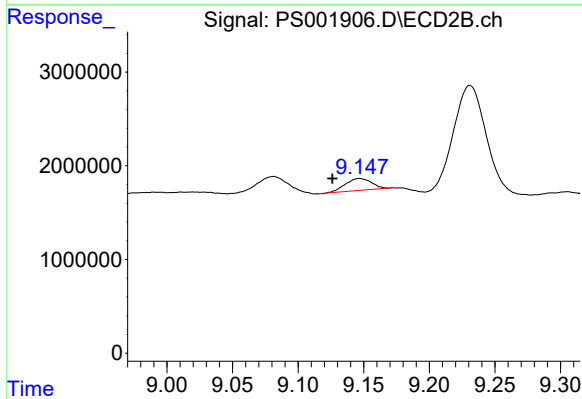

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.147 min
Delta R.T.: 0.021 min
Response: 1758920
Conc: 5.57 ng/ml

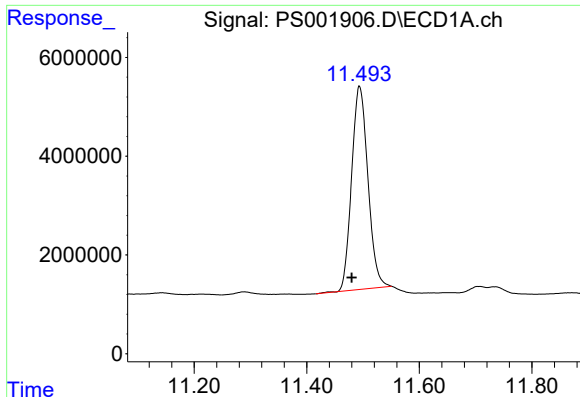

#4 2,4-DCAA


R.T.: 11.494 min
Delta R.T.: 0.014 min
Response: 82844009
Conc: 369.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

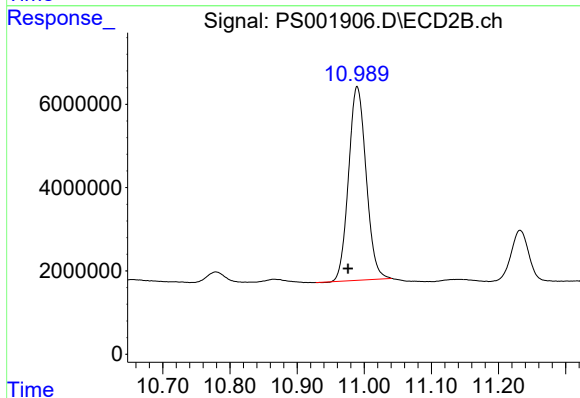


#4 2,4-DCAA

R.T.: 10.990 min
Delta R.T.: 0.014 min
Response: 84373573
Conc: 332.16 ng/ml

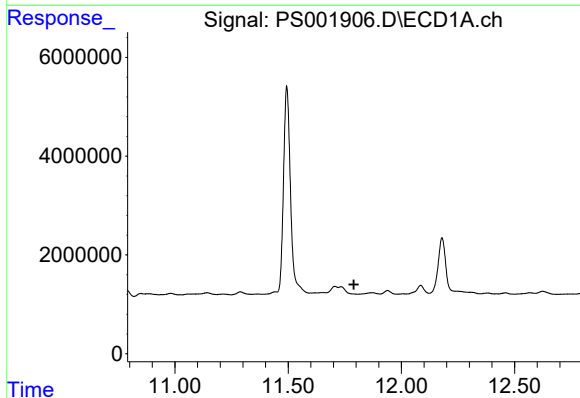


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.790 min
Response: 0
Conc: N.D.

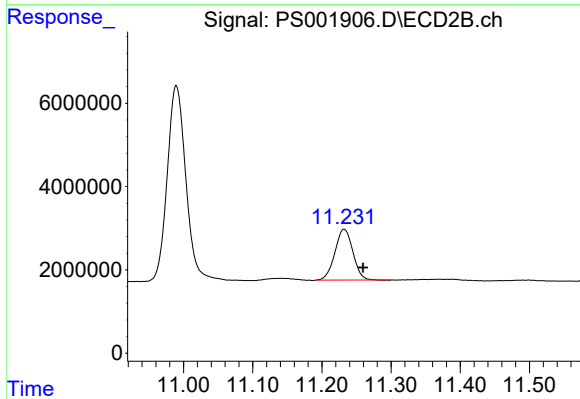

#5 DICAMBA


R.T.: 11.232 min
Delta R.T.: -0.028 min
Response: 21989805
Conc: 24.66 ng/ml

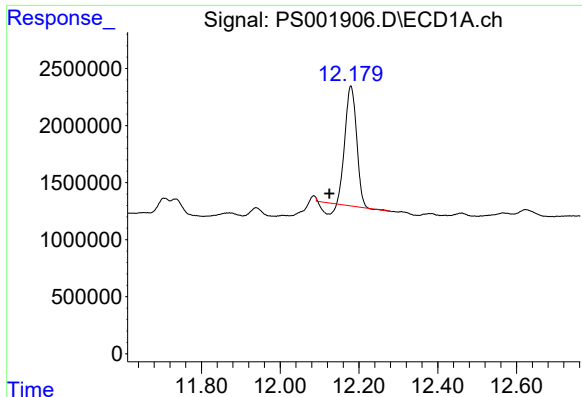

#6 MCP


R.T.: 12.179 min
Delta R.T.: 0.054 min
Response: 20263634
Conc: 31.80 ug/ml

Instrument :
ECD_S
ClientSampleId :

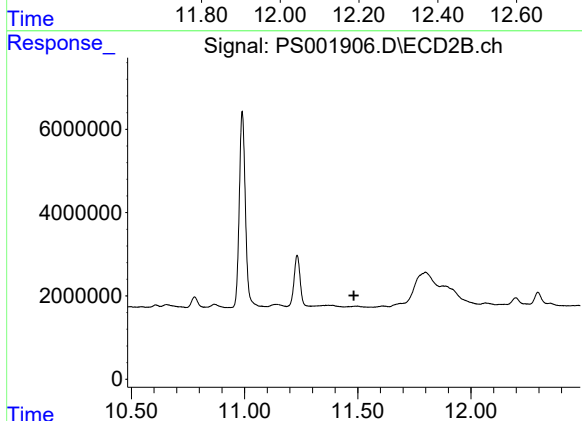


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

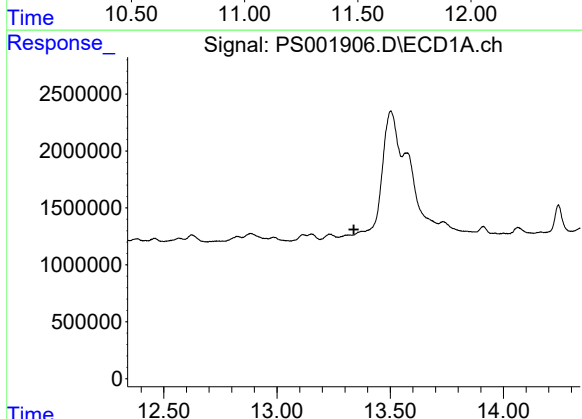


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.340 min
Response: 0
Conc: N.D.

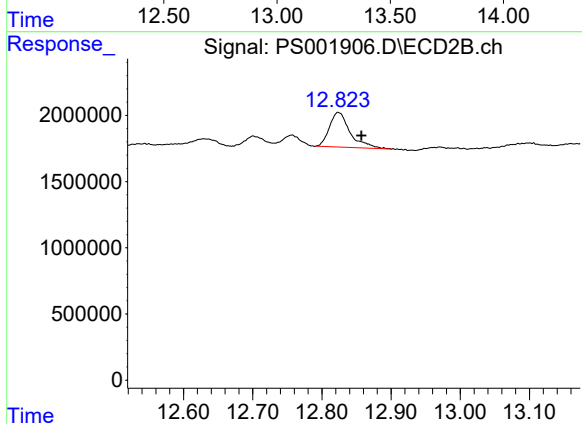

#9 2,4-D


R.T.: 12.824 min
Delta R.T.: -0.033 min
Response: 5420300
Conc: 17.42 ng/ml

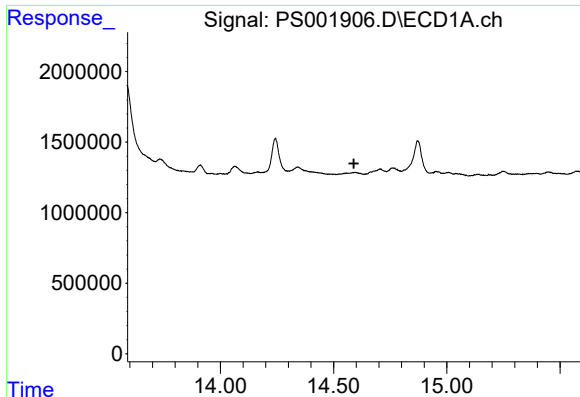

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.590 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

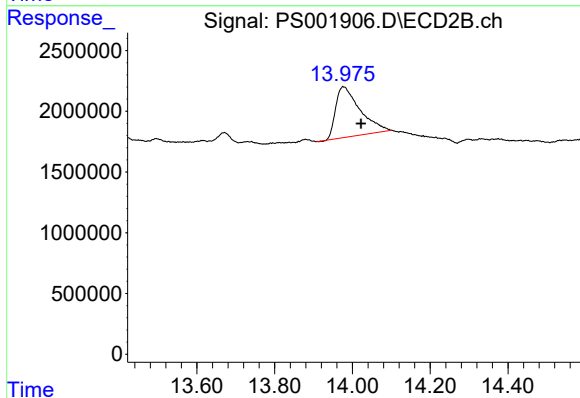


#11 2,4,5-TP (SILVEX)

R.T.: 13.977 min
Delta R.T.: -0.046 min
Response: 18141624
Conc: 13.23 ng/ml

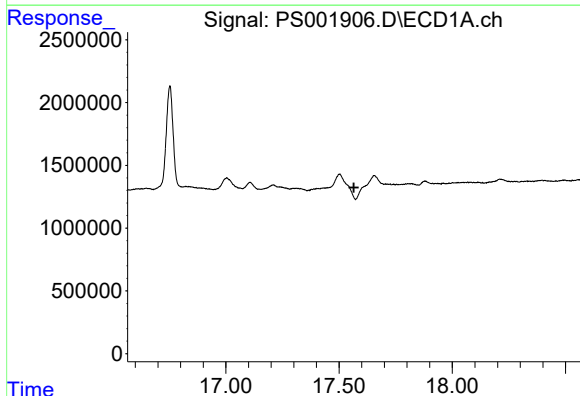

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

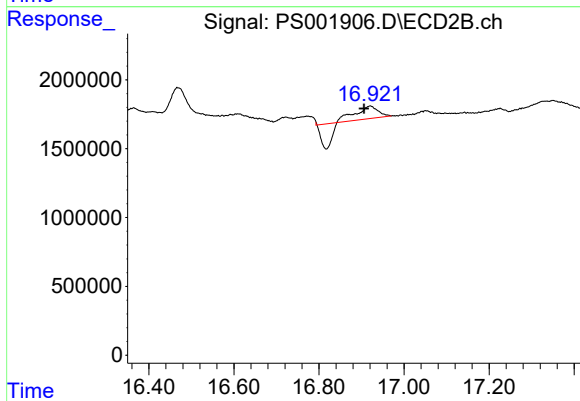

#16 DCPA

R.T.: 16.920 min
Delta R.T.: 0.014 min
Response: 1009699
Conc: 0.55 ng/ml