

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
 Data File : PS001923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2018 22:15
 Operator : EI\SJ
 Sample : J5255-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:19:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.448	10.943	61041373	59595751	272.123	234.614
Target Compounds							
2) T	3,5-DICHL...	0.000	9.185	0	8565789	N.D.	27.138 #
5) T	DICAMBA	11.821	0.000	2415806	0	2.787	N.D. #
6) T	MCP	12.134	0.000	16850074	0	26.442	N.D. #
10) T	Pentachlo...	13.688	13.374	13223130	12143838	4.303	3.543
13) T	2,4-DB	0.000	15.201	0	2734861	N.D.	16.523 #
14) T	DINOSEB	17.202	15.689	4377913	3049282	5.252	3.217 #
15) T	Picloram	0.000	16.876	0	11180445	N.D.	6.574 #
16) T	DCPA	17.594	16.925	-4620489	6730623	N.D.	3.649



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
Data File : PS001923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2018 22:15
Operator : EI\SJ
Sample : J5255-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:19:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

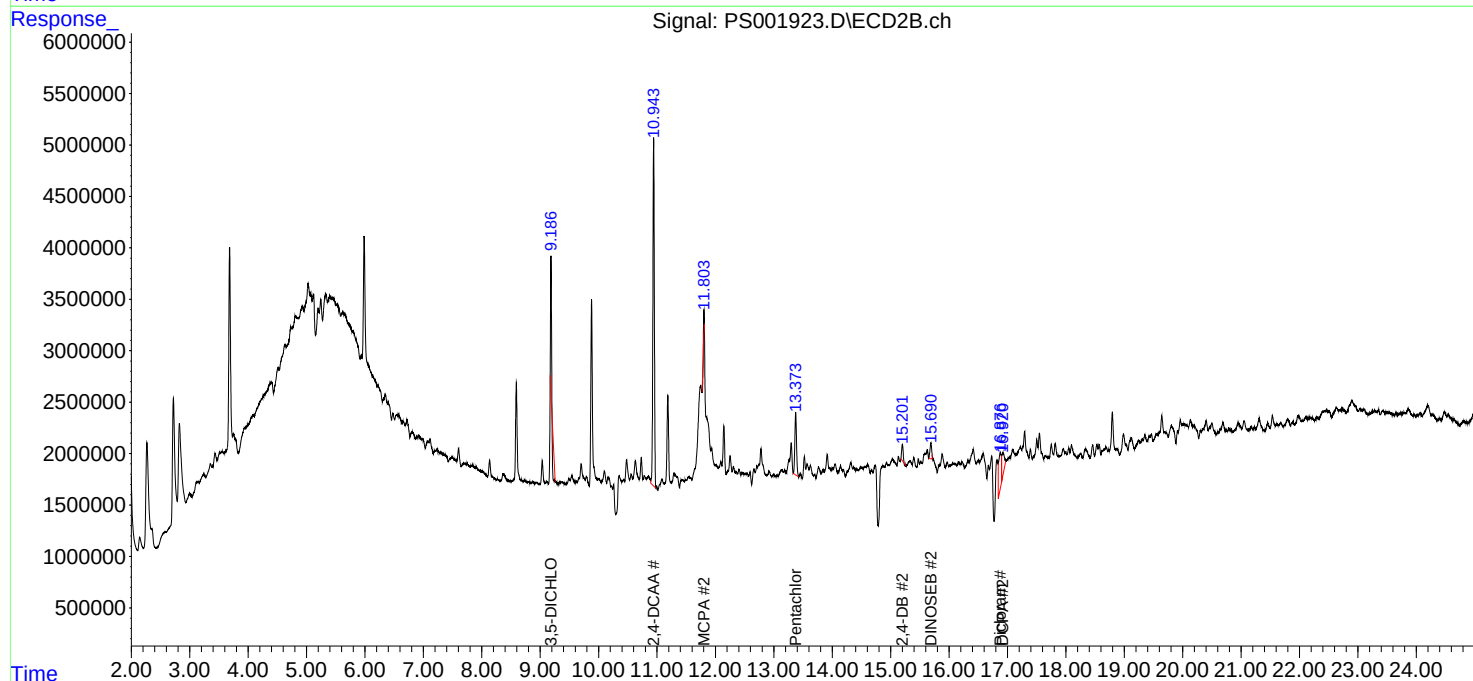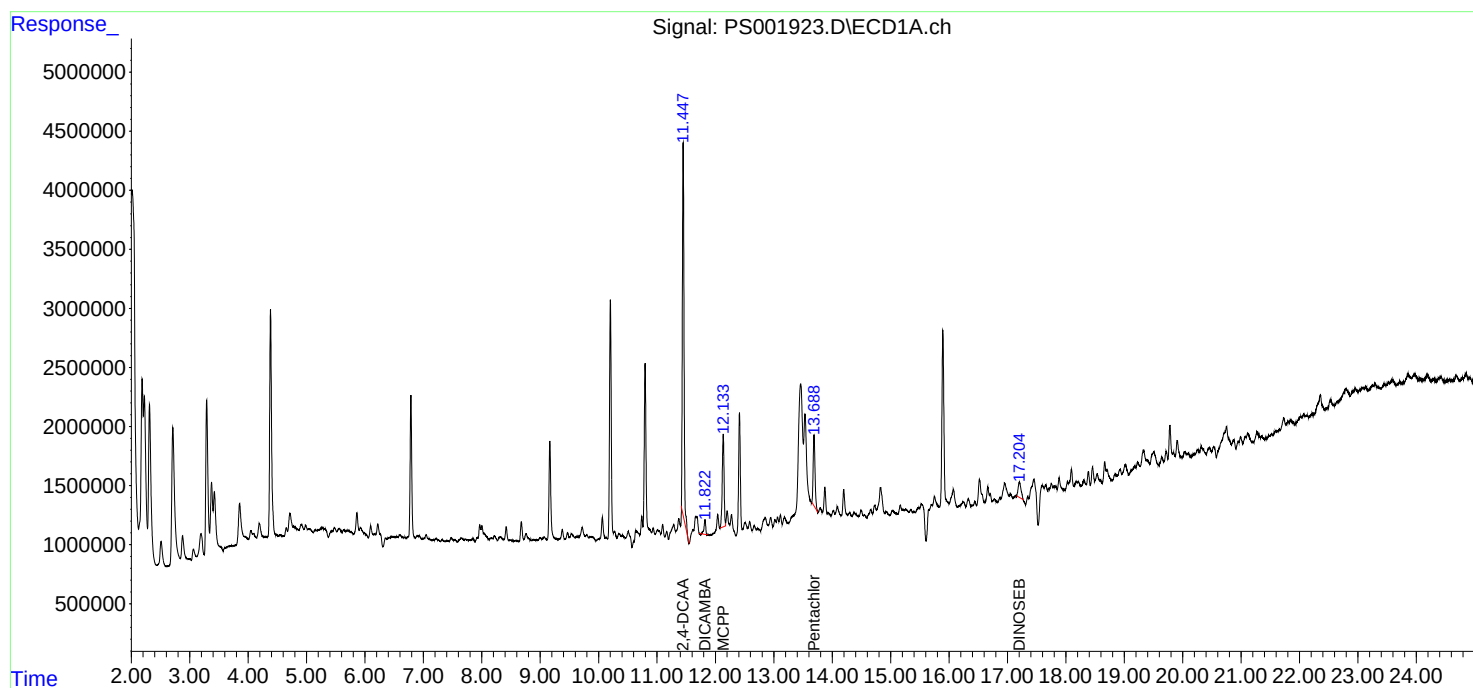


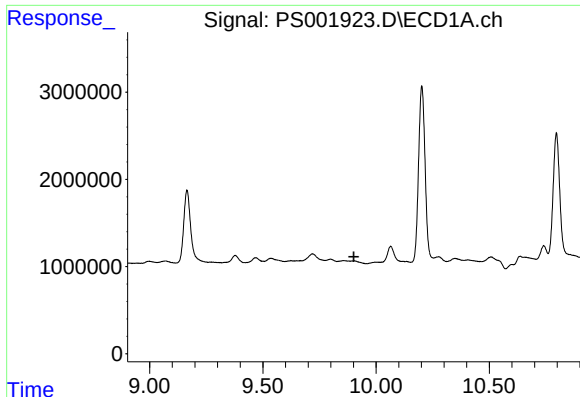

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.902 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

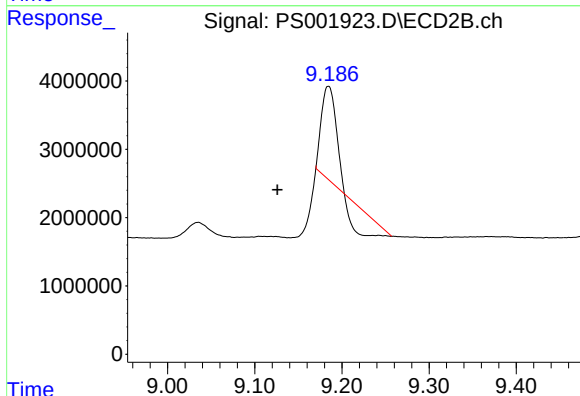


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.185 min
Delta R.T.: 0.059 min
Response: 8565789
Conc: 27.14 ng/ml

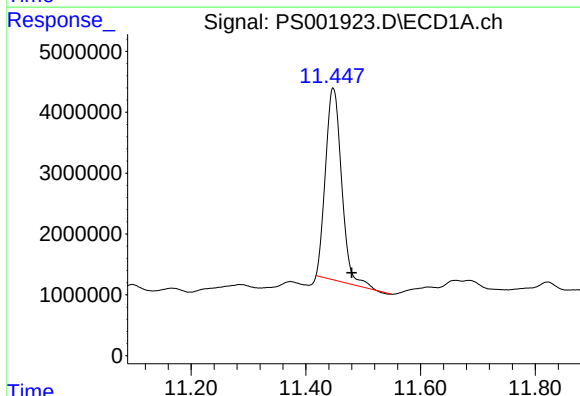


#4 2,4-DCAA

R.T.: 11.448 min
Delta R.T.: -0.032 min
Response: 61041373
Conc: 272.12 ng/ml

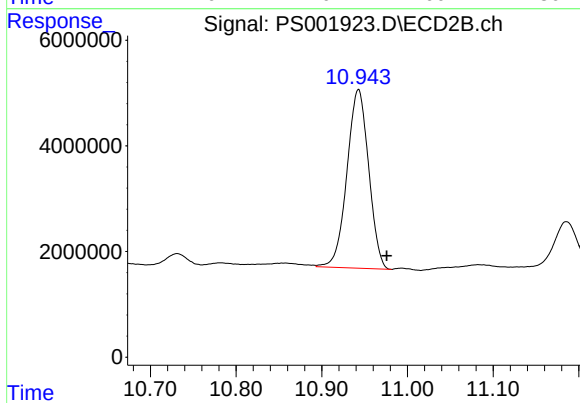

#4 2,4-DCAA


R.T.: 10.943 min
Delta R.T.: -0.033 min
Response: 59595751
Conc: 234.61 ng/ml

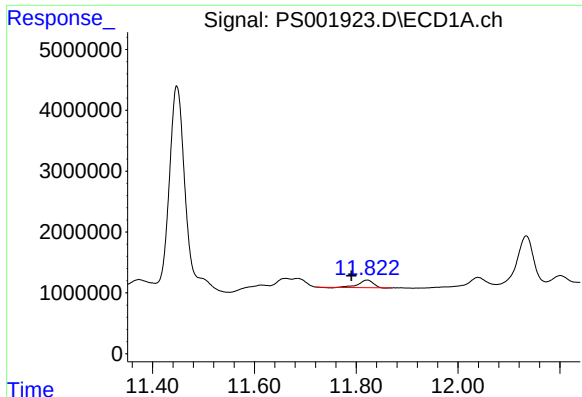

#5 DICAMBA


R.T.: 11.821 min
Delta R.T.: 0.031 min
Response: 2415806
Conc: 2.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

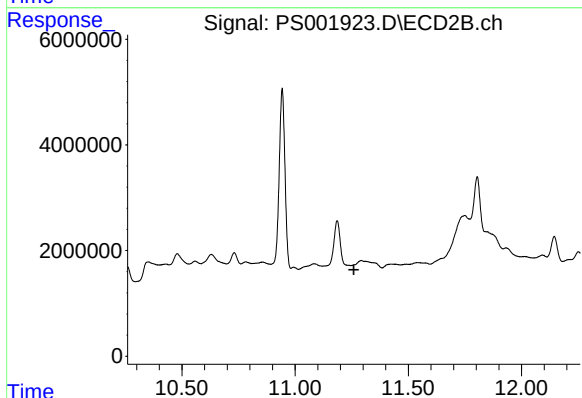


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.260 min
Response: 0
Conc: N.D.

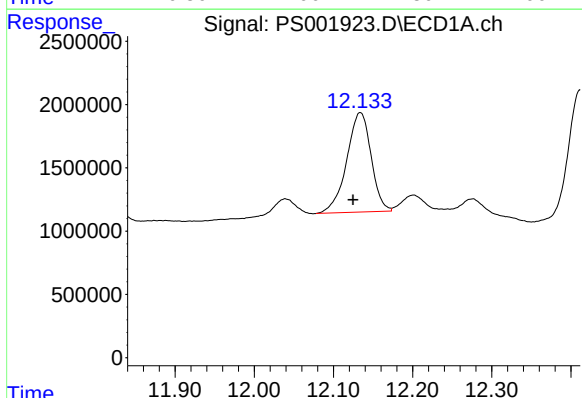


#6 MCP

R.T.: 12.134 min
Delta R.T.: 0.009 min
Response: 16850074
Conc: 26.44 ug/ml

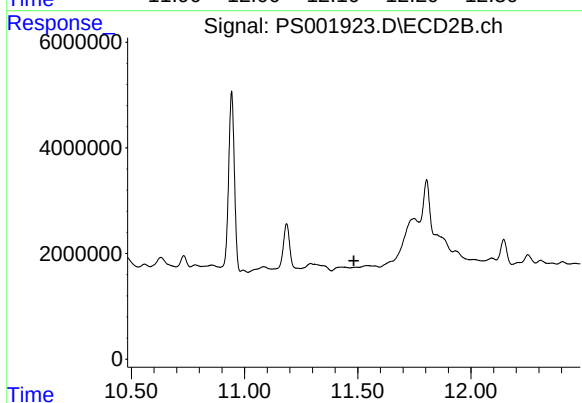

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

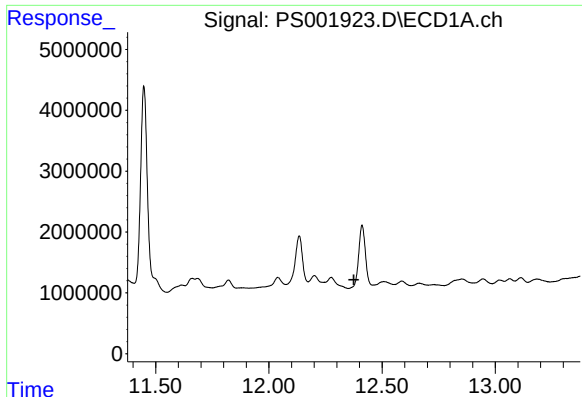

#7 MCPA


R.T.: 12.411 min
Delta R.T.: 0.036 min
Response: -7037996
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

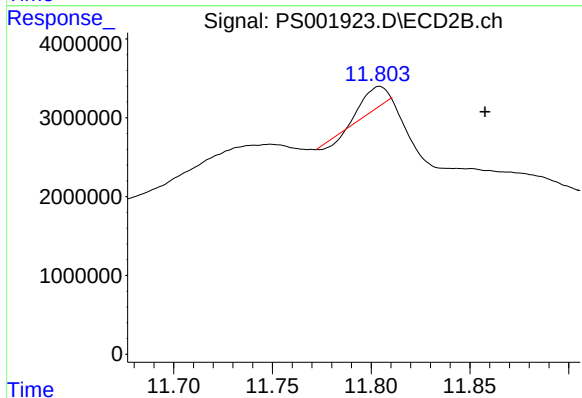


#7 MCPA

R.T.: 11.804 min
Delta R.T.: -0.053 min
Response: 2477069
Conc: 2.86 ug/ml

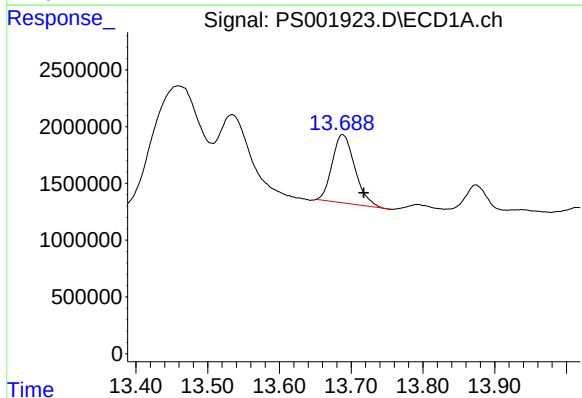


#10 Pentachlorophenol

R.T.: 13.688 min
Delta R.T.: -0.030 min
Response: 13223130
Conc: 4.30 ng/ml

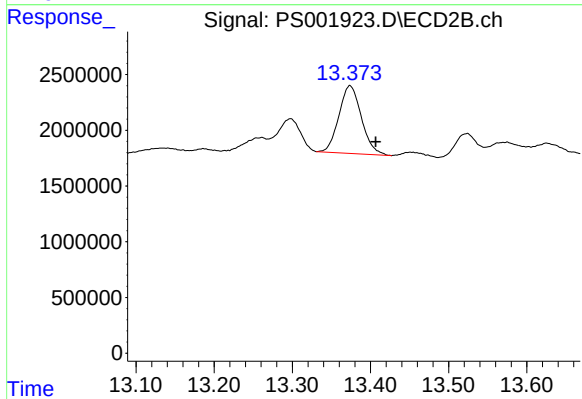

#10 Pentachlorophenol


R.T.: 13.374 min
Delta R.T.: -0.033 min
Response: 12143838
Conc: 3.54 ng/ml

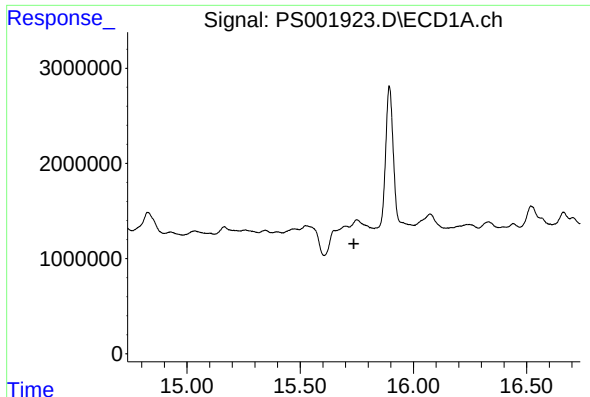

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.737 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

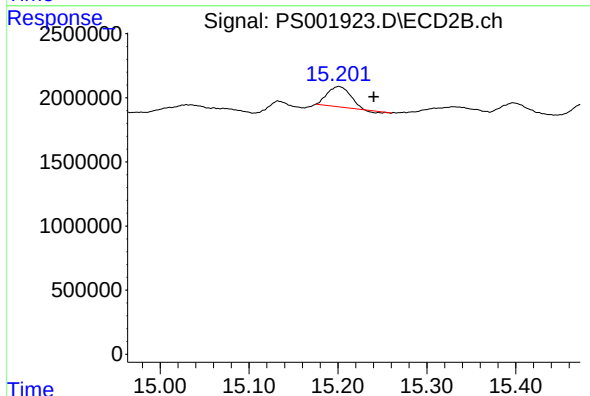


#13 2,4-DB

R.T.: 15.201 min
Delta R.T.: -0.039 min
Response: 2734861
Conc: 16.52 ng/ml

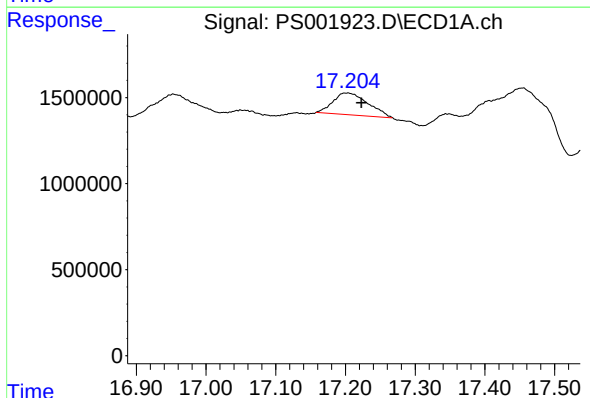


#14 DINOSEB

R.T.: 17.202 min
Delta R.T.: -0.021 min
Response: 4377913
Conc: 5.25 ng/ml

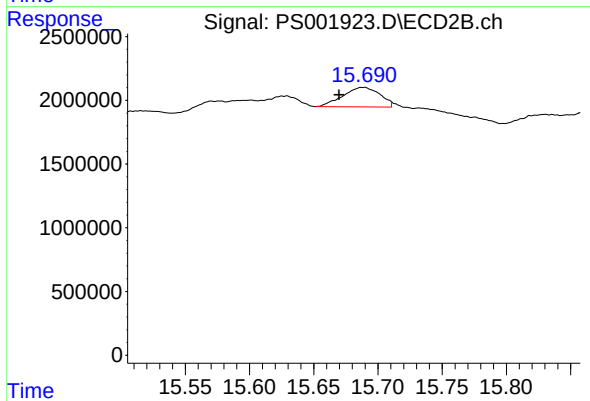

#14 DINOSEB


R.T.: 15.689 min
Delta R.T.: 0.019 min
Response: 3049282
Conc: 3.22 ng/ml

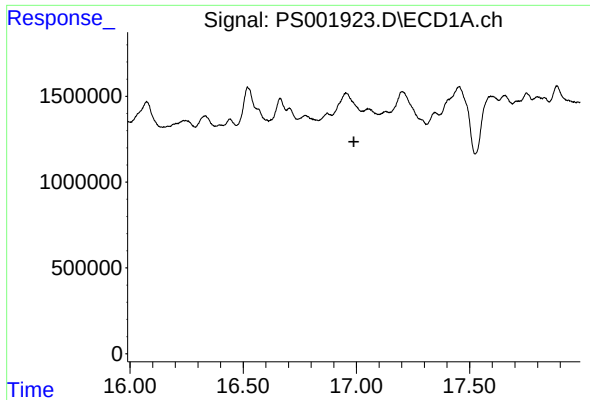

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

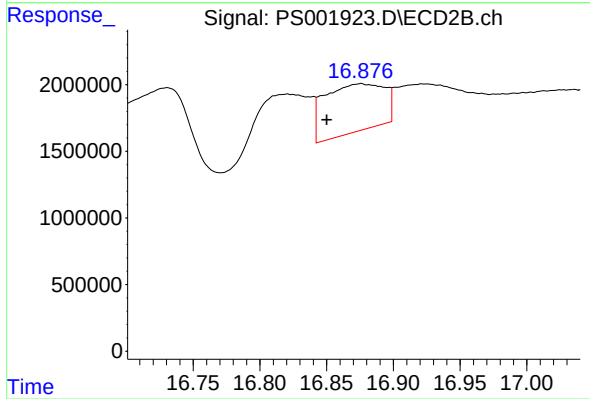


#15 Picloram

R.T.: 16.876 min
Delta R.T.: 0.025 min
Response: 11180445
Conc: 6.57 ng/ml

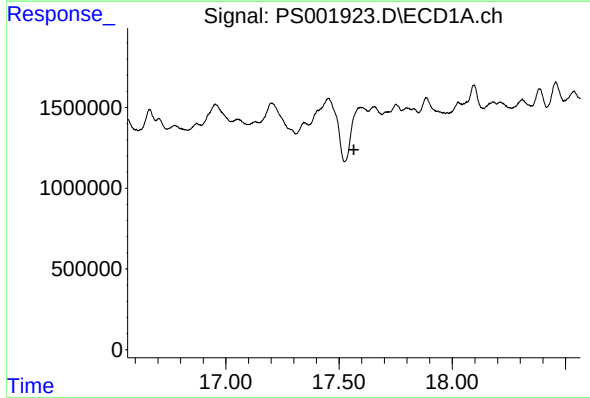

#16 DCPA

R.T.: 17.594 min
Delta R.T.: 0.029 min
Response: -4620489
Conc: N.D.

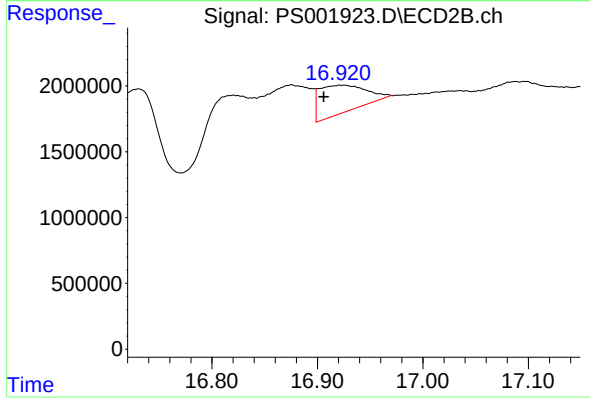

#16 DCPA

R.T.: 16.925 min
Delta R.T.: 0.019 min
Response: 6730623
Conc: 3.65 ng/ml