

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
 Data File : PS001927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2018 00:19
 Operator : EI\SJ
 Sample : J5287-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:20:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.473	10.969	56182794	56143845	250.463	221.024
Target Compounds							
1) T	Dalapon	2.905	0.000	7383753	0	22.708	N.D. #
5) T	DICAMBA	0.000	11.211	0	8958275	N.D.	10.044 #
6) T	MCPD	12.159	0.000	14656741	0	23.001	N.D. #
7) T	MCPA	12.437	11.829	9529154	12306930	9.080	14.198 #
10) T	Pentachlo...	13.714	13.400	12140126	6234265	3.950	1.819 #
11) T	2,4,5-TP ...	0.000	14.075	0	2154880	N.D.	1.572 #
13) T	2,4-DB	15.773	15.229	3084178	3960742	18.938	23.929 #
15) T	Picloram	16.979	16.842	4485883	3021186	2.576	1.776 #
16) T	DCPA	0.000	16.899	0	6390358	N.D.	3.465 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
Data File : PS001927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2018 00:19
Operator : EI\SJ
Sample : J5287-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:20:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

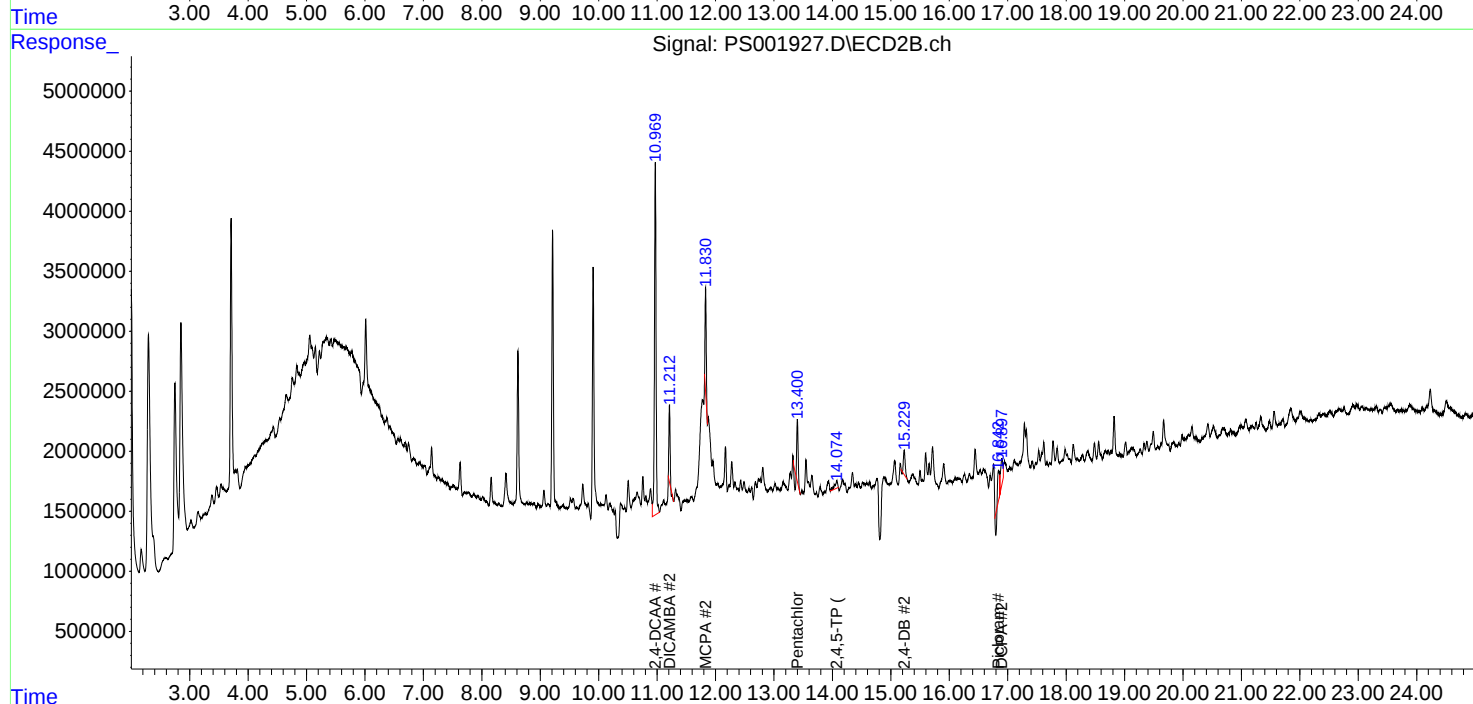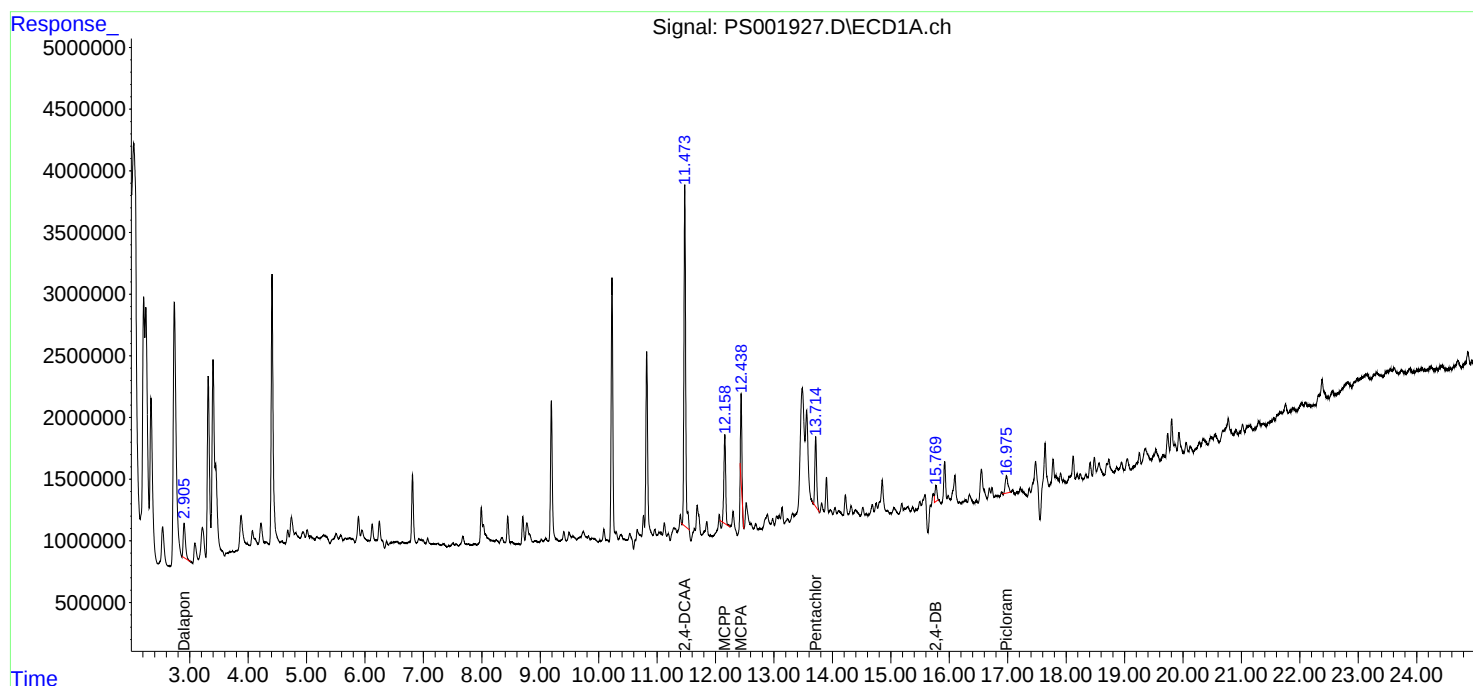


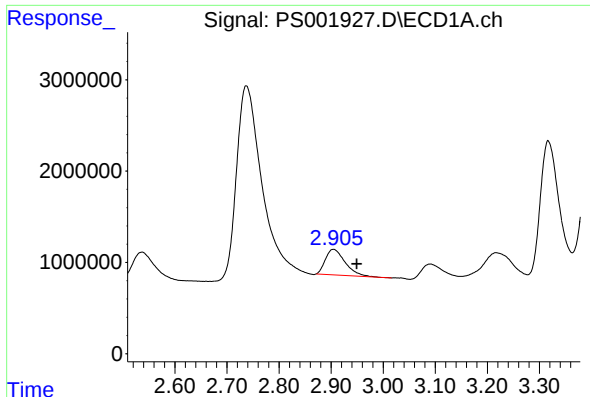

#1 Dalapon


R.T.: 2.905 min
Delta R.T.: -0.044 min
Response: 7383753
Conc: 22.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

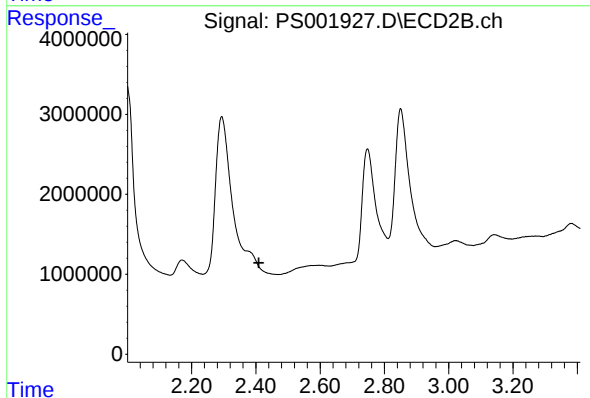


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.410 min
Response: 0
Conc: N.D.

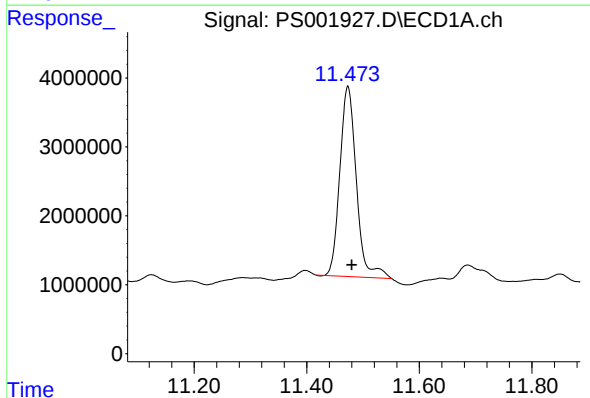


#4 2,4-DCAA

R.T.: 11.473 min
Delta R.T.: -0.007 min
Response: 56182794
Conc: 250.46 ng/ml

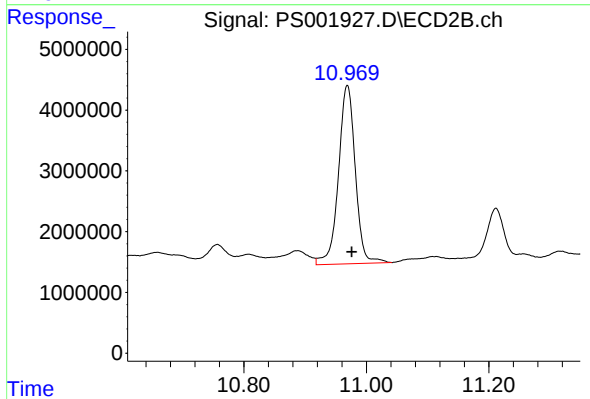

#4 2,4-DCAA


R.T.: 10.969 min
Delta R.T.: -0.007 min
Response: 56143845
Conc: 221.02 ng/ml

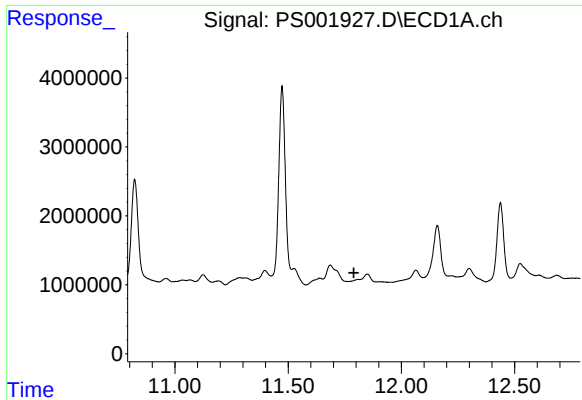

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

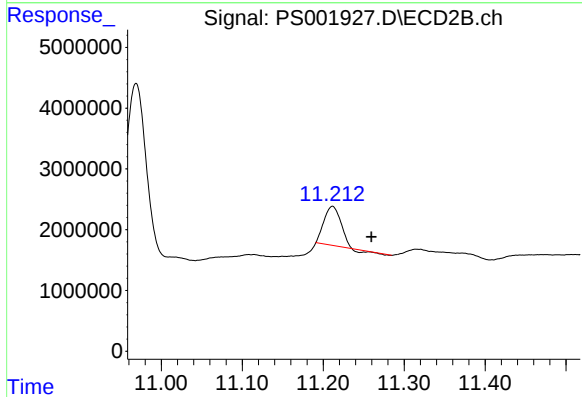


#5 DICAMBA

R.T.: 11.211 min
Delta R.T.: -0.048 min
Response: 8958275
Conc: 10.04 ng/ml

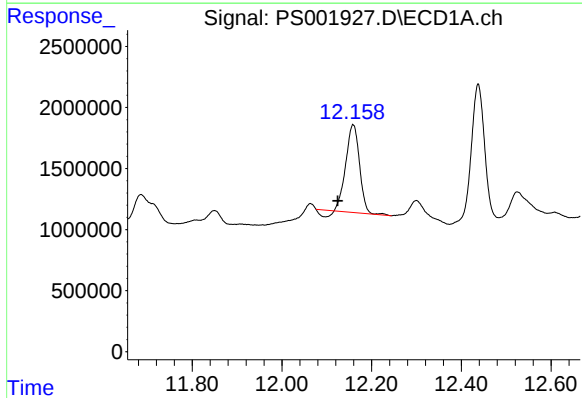


#6 MCP

R.T.: 12.159 min
Delta R.T.: 0.034 min
Response: 14656741
Conc: 23.00 ug/ml

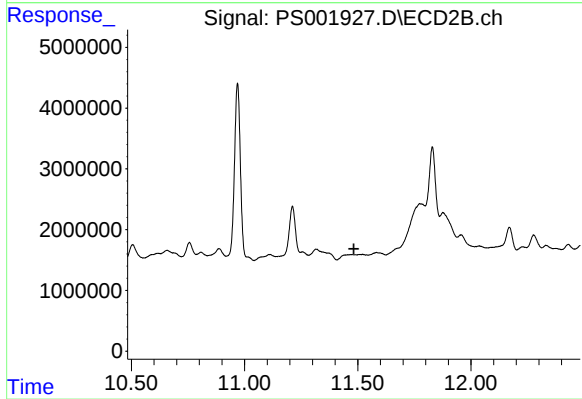

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.483 min
Response: 0
Conc: N.D.

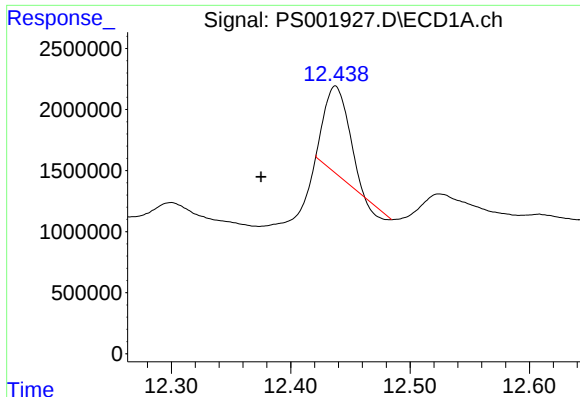

#7 MCPA


R.T.: 12.437 min
Delta R.T.: 0.062 min
Response: 9529154
Conc: 9.08 ug/ml

Instrument :
ECD_S
ClientSampleId :

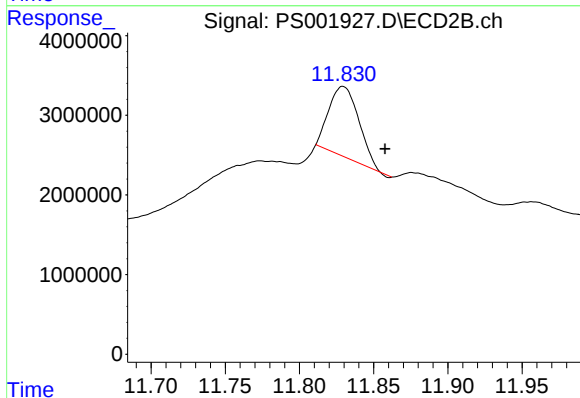


#7 MCPA

R.T.: 11.829 min
Delta R.T.: -0.028 min
Response: 12306930
Conc: 14.20 ug/ml

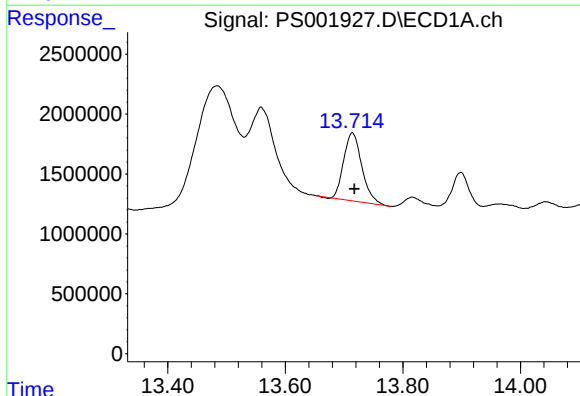


#10 Pentachlorophenol

R.T.: 13.714 min
Delta R.T.: -0.004 min
Response: 12140126
Conc: 3.95 ng/ml

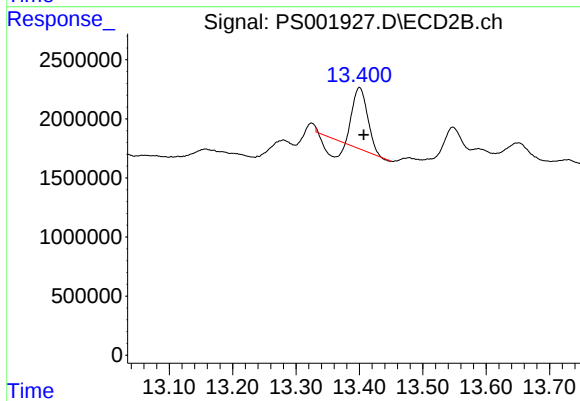

#10 Pentachlorophenol


R.T.: 13.400 min
Delta R.T.: -0.006 min
Response: 6234265
Conc: 1.82 ng/ml

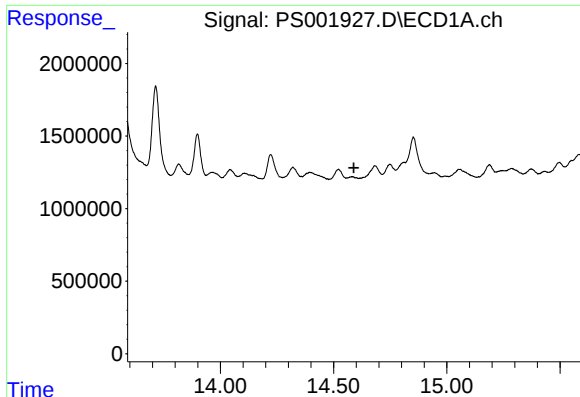

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.590 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

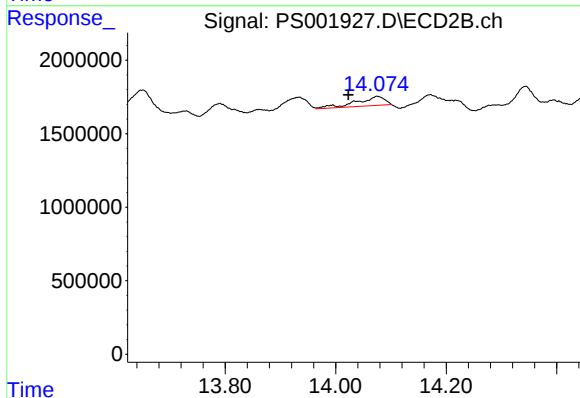


#11 2,4,5-TP (SILVEX)

R.T.: 14.075 min
Delta R.T.: 0.053 min
Response: 2154880
Conc: 1.57 ng/ml

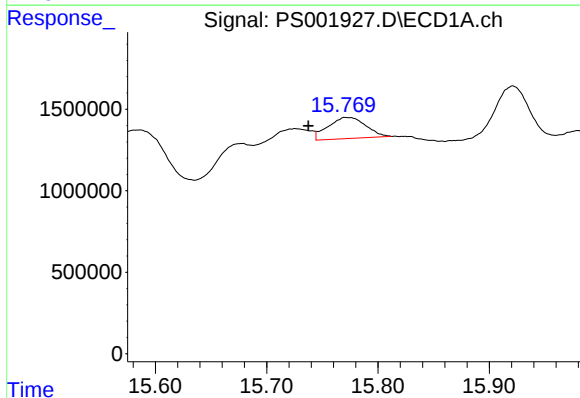


#13 2,4-DB

R.T.: 15.773 min
Delta R.T.: 0.036 min
Response: 3084178
Conc: 18.94 ng/ml

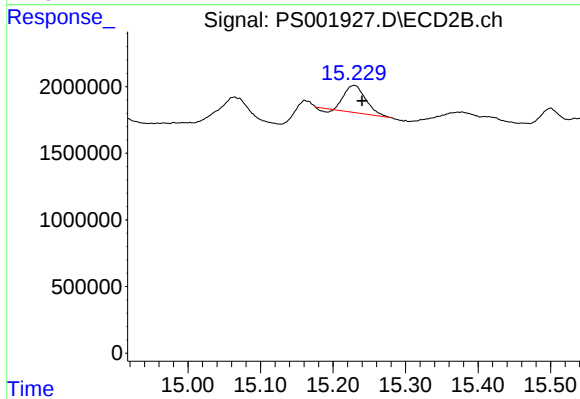

#13 2,4-DB


R.T.: 15.229 min
Delta R.T.: -0.011 min
Response: 3960742
Conc: 23.93 ng/ml

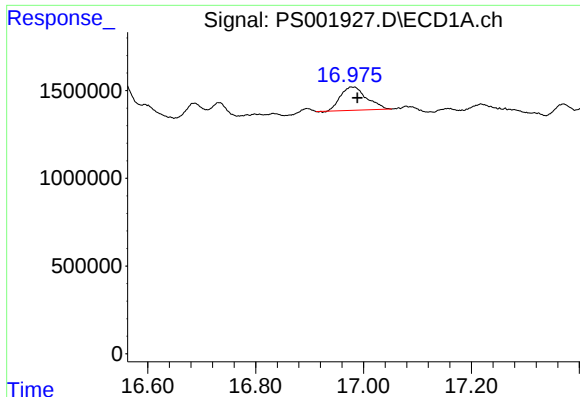

#15 Picloram


R.T.: 16.979 min
Delta R.T.: -0.009 min
Response: 4485883
Conc: 2.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

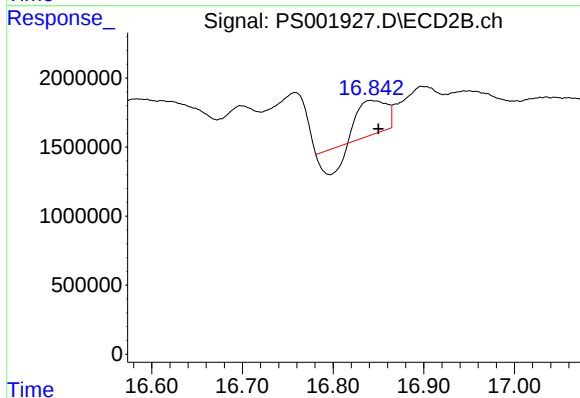


#15 Picloram

R.T.: 16.842 min
Delta R.T.: -0.008 min
Response: 3021186
Conc: 1.78 ng/ml

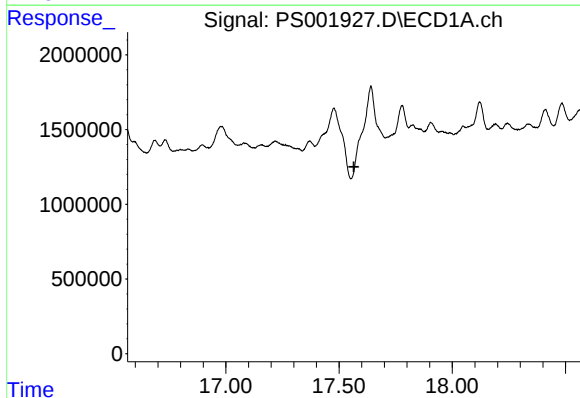

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.565 min
Response: 0
Conc: N.D.

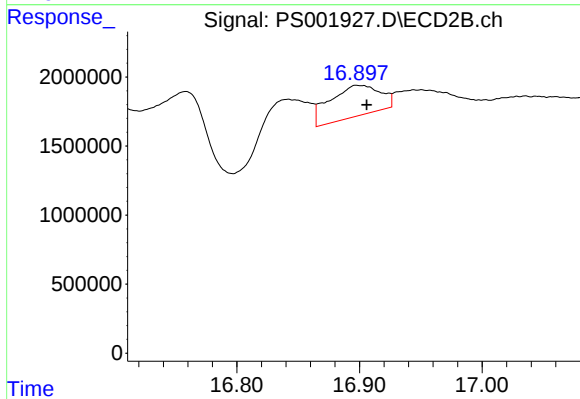

#16 DCPA

R.T.: 16.899 min
Delta R.T.: -0.006 min
Response: 6390358
Conc: 3.46 ng/ml