

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
 Data File : PS001928.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2018 00:50
 Operator : EI\SJ
 Sample : J5287-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:21:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.448	10.942	40310557	37206361	179.705	146.472
Target Compounds							
2) T	3,5-DICHL...	0.000	9.184	0	13600651	N.D.	43.090 #
3) T	4-Nitroph...	11.104	0.000	2642991	0	18.778	N.D. #
6) T	MCP	12.133	0.000	13922570	0	21.848	N.D. #
8) T	DICHLORPROP	12.962	12.403	1685461	2167214	7.263	9.330 #
10) T	Pentachlo...	13.682	0.000	17739293	0	5.772	N.D. #
11) T	2,4,5-TP ...	0.000	14.012	0	3082057	N.D.	2.248 #
13) T	2,4-DB	15.704	0.000	2034489	0	12.493	N.D. #
14) T	DINOSEB	0.000	15.690	0	5058618	N.D.	5.337 #
15) T	Picloram	0.000	16.876	0	7857689	N.D.	4.620 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
Data File : PS001928.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2018 00:50
Operator : EI\SJ
Sample : J5287-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:21:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

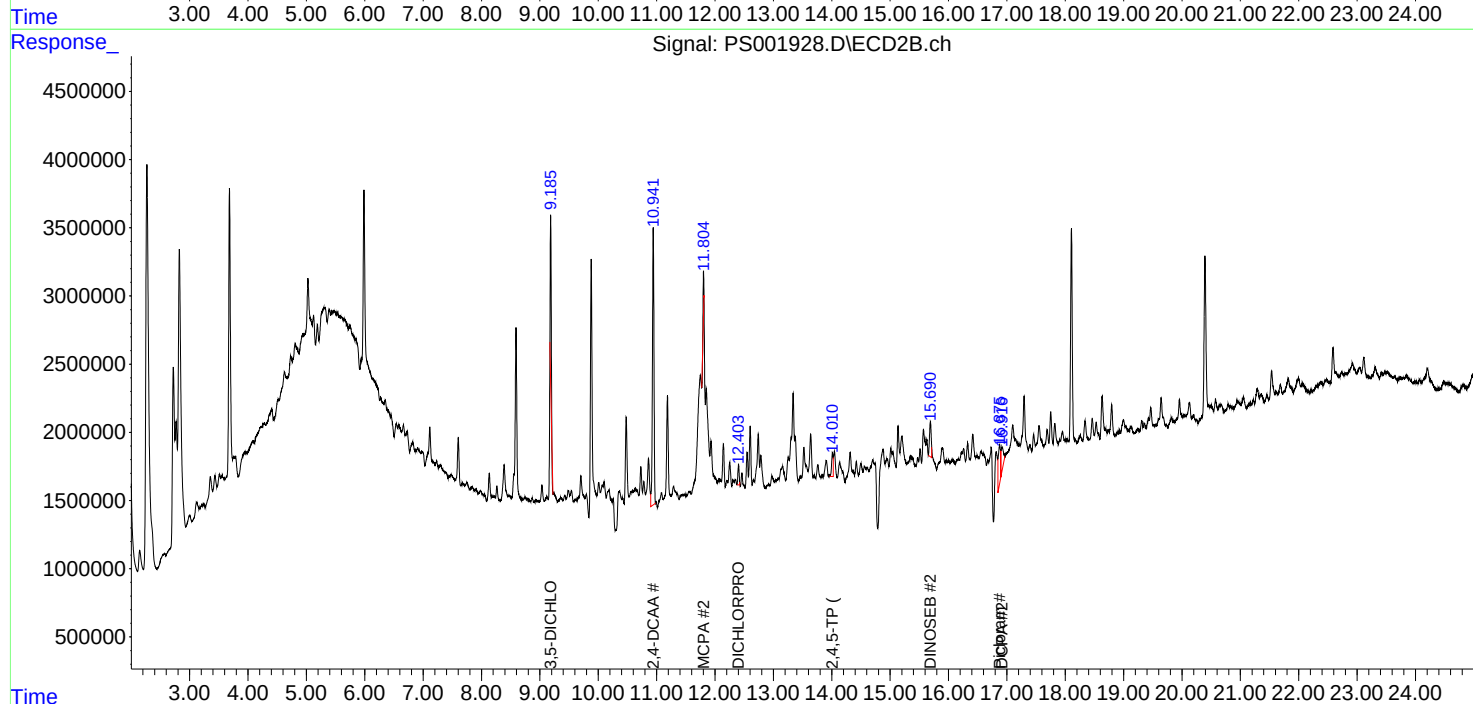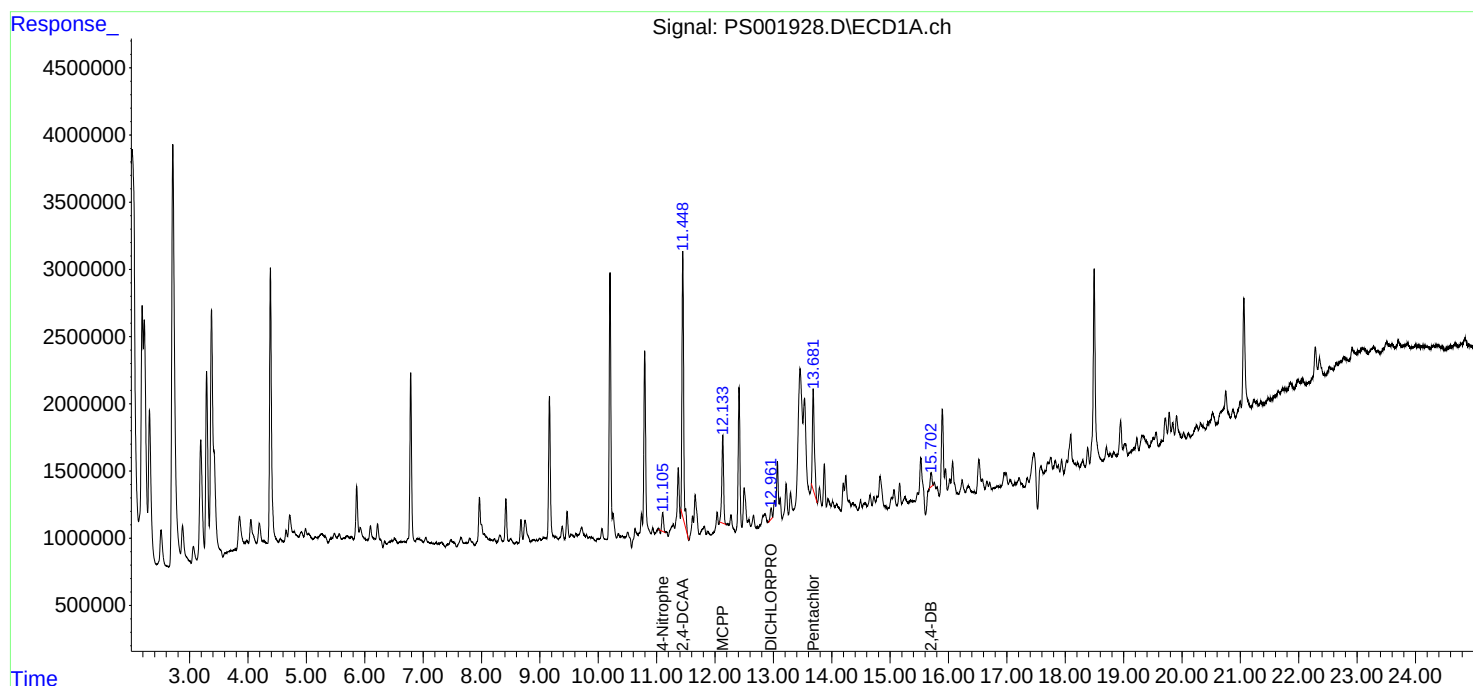


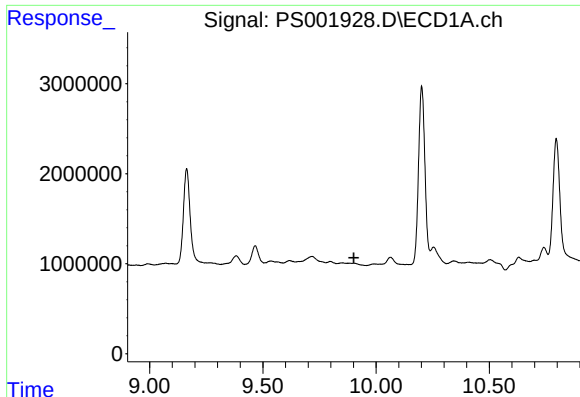

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.902 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

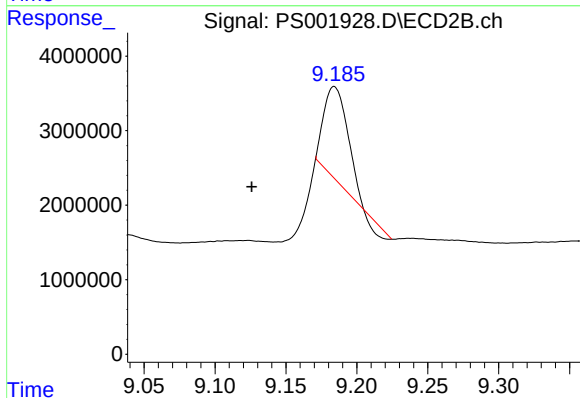


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.184 min
Delta R.T.: 0.058 min
Response: 13600651
Conc: 43.09 ng/ml

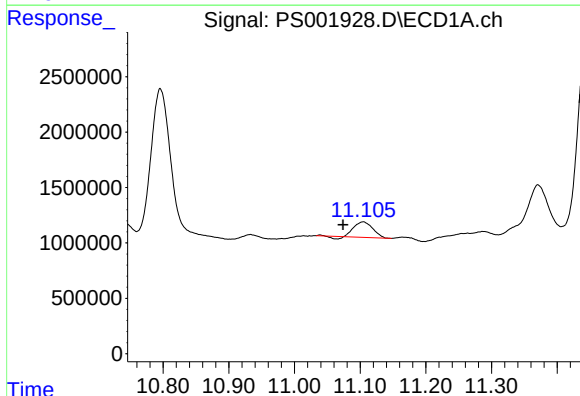


#3 4-Nitrophenol

R.T.: 11.104 min
Delta R.T.: 0.031 min
Response: 2642991
Conc: 18.78 ng/ml

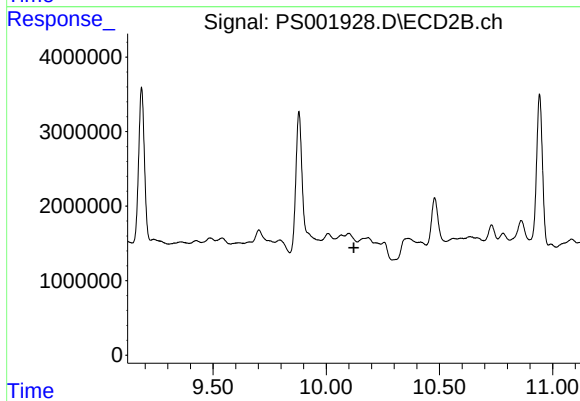

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.122 min
Response: 0
Conc: N.D.

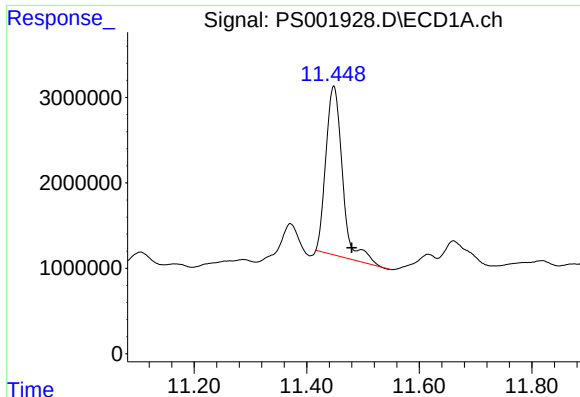

#4 2,4-DCAA


R.T.: 11.448 min
Delta R.T.: -0.032 min
Response: 40310557
Conc: 179.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

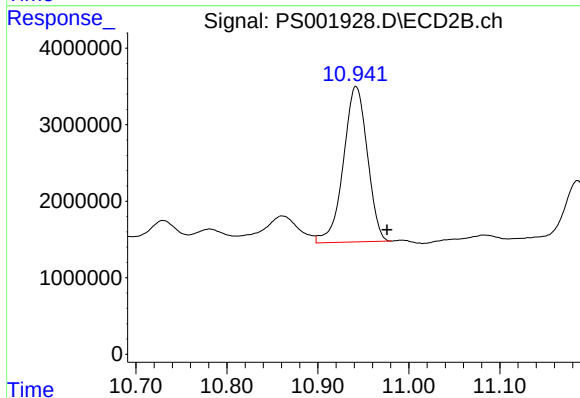


#4 2,4-DCAA

R.T.: 10.942 min
Delta R.T.: -0.034 min
Response: 37206361
Conc: 146.47 ng/ml

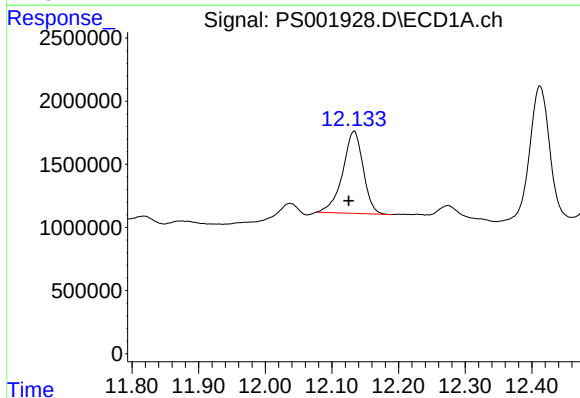


#6 MCP

R.T.: 12.133 min
Delta R.T.: 0.008 min
Response: 13922570
Conc: 21.85 ug/ml

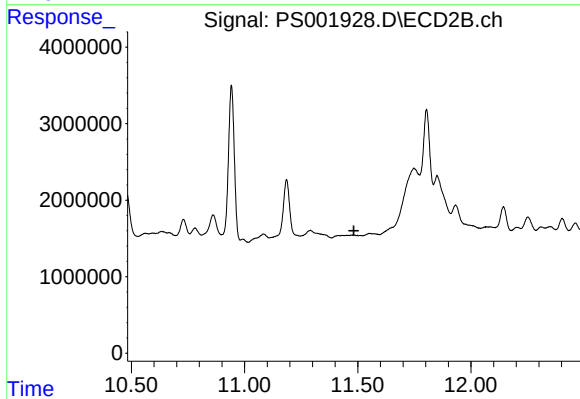

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.483 min
Response: 0
Conc: N.D.

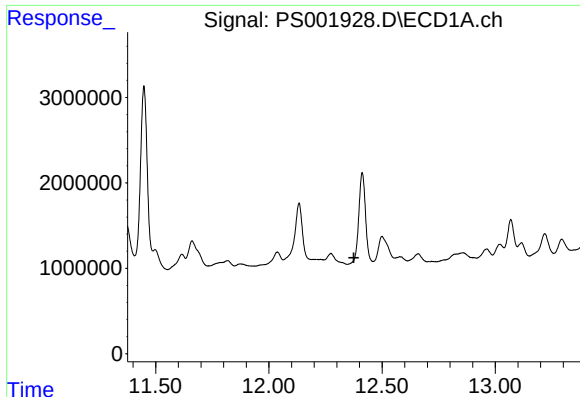

#7 MCPA


R.T.: 12.412 min
Delta R.T.: 0.037 min
Response: -8734011
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

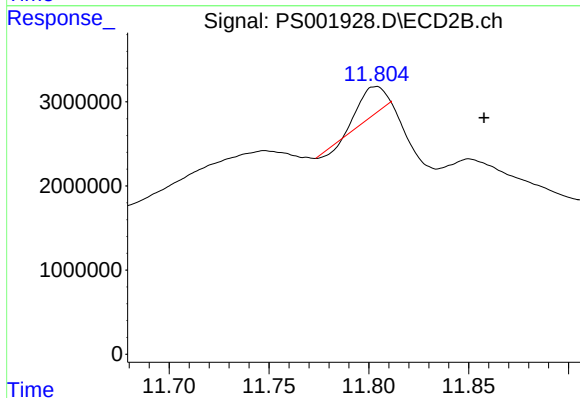


#7 MCPA

R.T.: 11.804 min
Delta R.T.: -0.054 min
Response: 3245320
Conc: 3.74 ug/ml

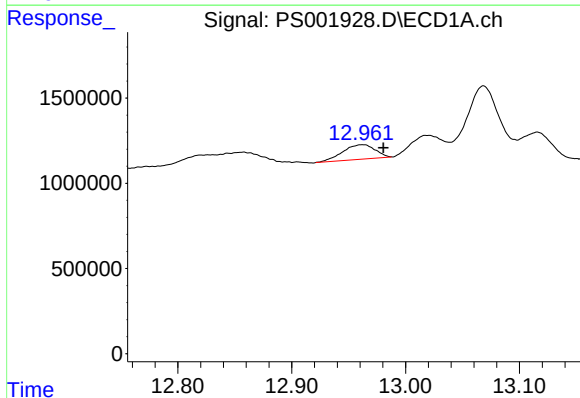


#8 DICHLORPROP

R.T.: 12.962 min
Delta R.T.: -0.019 min
Response: 1685461
Conc: 7.26 ng/ml

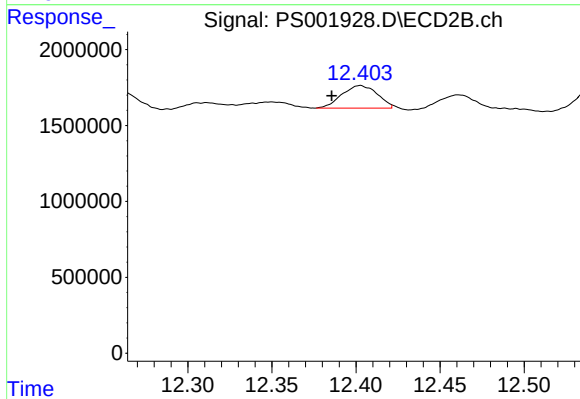

#8 DICHLORPROP


R.T.: 12.403 min
Delta R.T.: 0.017 min
Response: 2167214
Conc: 9.33 ng/ml

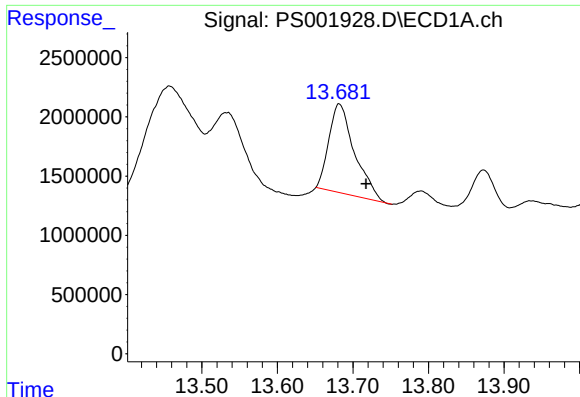

#10 Pentachlorophenol


R.T.: 13.682 min
Delta R.T.: -0.036 min
Response: 17739293
Conc: 5.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

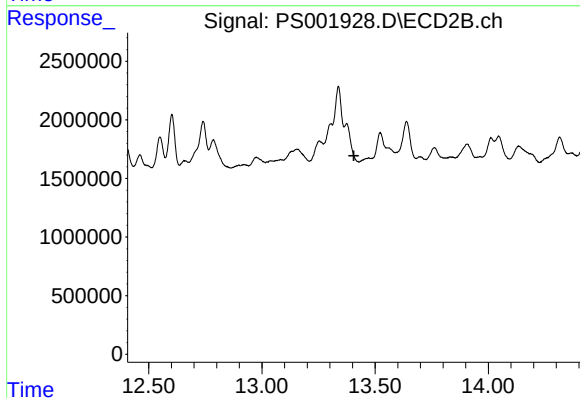


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.407 min
Response: 0
Conc: N.D.

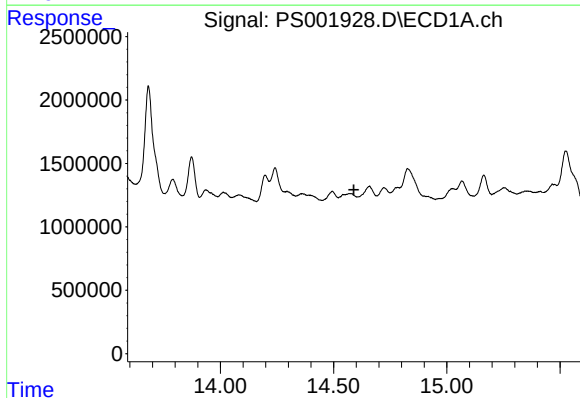


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.590 min
Response: 0
Conc: N.D.

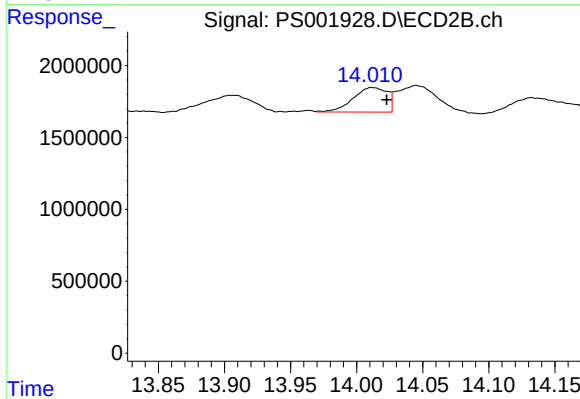

#11 2,4,5-TP (SILVEX)


R.T.: 14.012 min
Delta R.T.: -0.011 min
Response: 3082057
Conc: 2.25 ng/ml

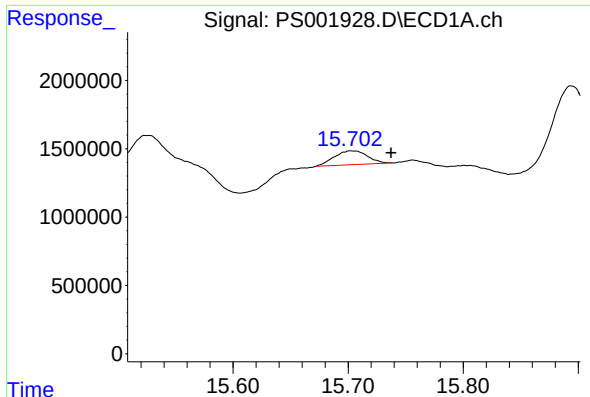

#13 2,4-DB


R.T.: 15.704 min
Delta R.T.: -0.034 min
Response: 2034489
Conc: 12.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

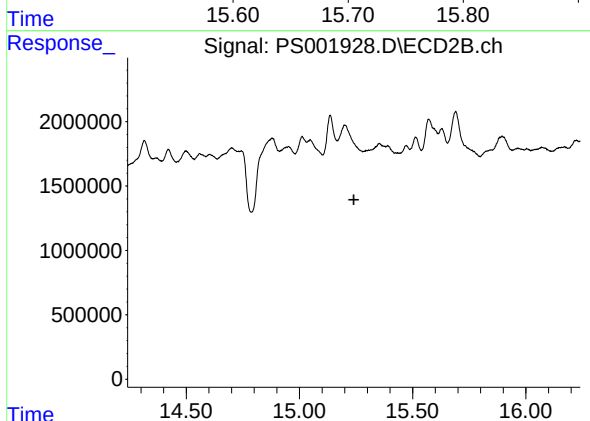


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.240 min
Response: 0
Conc: N.D.

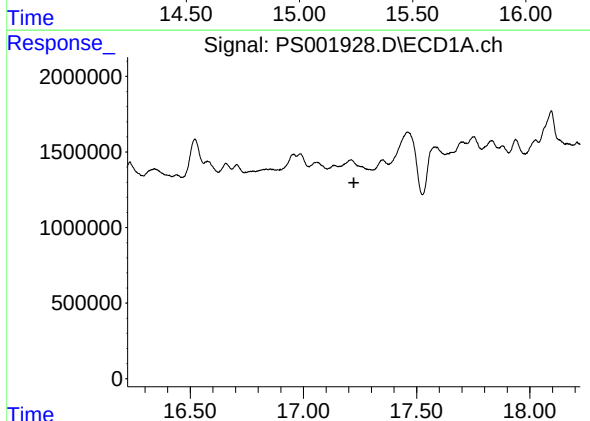


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.223 min
Response: 0
Conc: N.D.

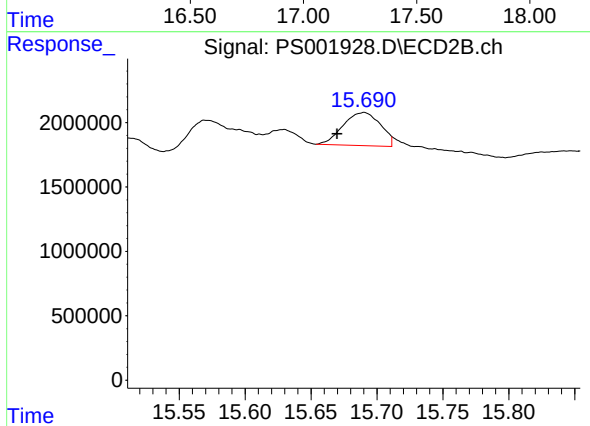

#14 DINOSEB


R.T.: 15.690 min
Delta R.T.: 0.020 min
Response: 5058618
Conc: 5.34 ng/ml

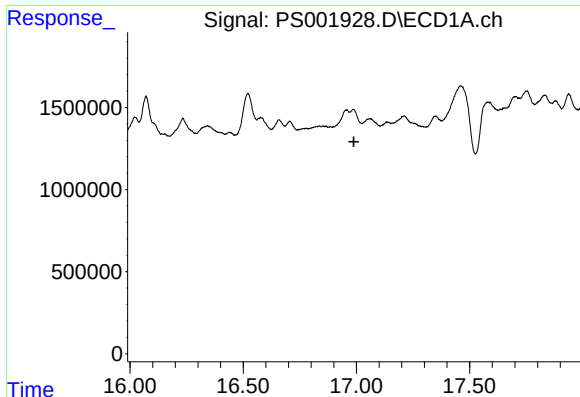

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

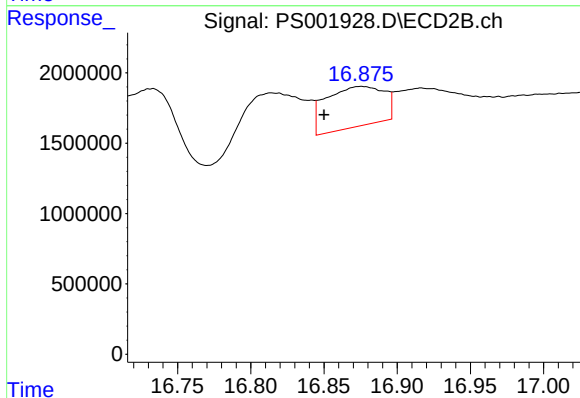


#15 Picloram

R.T.: 16.876 min
Delta R.T.: 0.026 min
Response: 7857689
Conc: 4.62 ng/ml

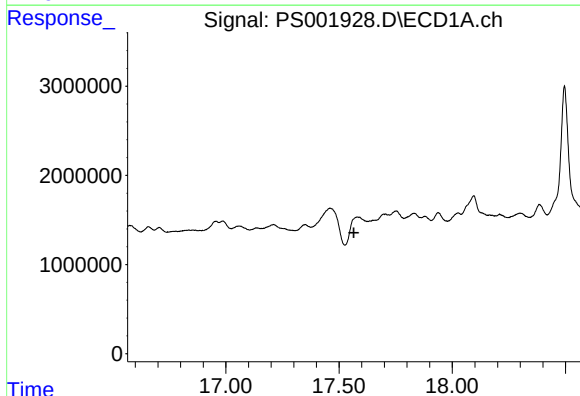

#16 DCPA

R.T.: 17.581 min
Delta R.T.: 0.016 min
Response: -4130478
Conc: N.D.

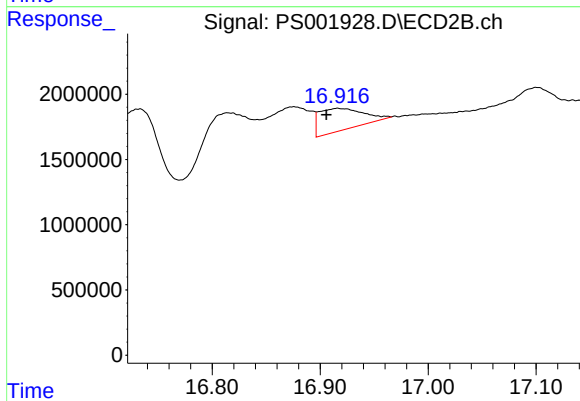

#16 DCPA

R.T.: 16.917 min
Delta R.T.: 0.011 min
Response: 4764976
Conc: 2.58 ng/ml