

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
 Data File : PS001931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2018 02:23
 Operator : EI\SJ
 Sample : J5287-14
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:21:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.451	10.947	57551471	53470564	256.565	210.500
Target Compounds							
2) T	3,5-DICHL...	0.000	9.188	0	28145590	N.D.	89.172 #
3) T	4-Nitroph...	11.108	0.000	4164324	0	29.587	N.D. #
5) T	DICAMBA	11.825	0.000	2778696	0	3.206	N.D. #
6) T	MCP	12.138	0.000	18713660	0	29.367	N.D. #
10) T	Pentachlo...	13.714	0.000	4323993	0	1.407	N.D. #
11) T	2,4,5-TP ...	0.000	14.015	0	4444403	N.D.	3.241 #
13) T	2,4-DB	15.712	0.000	5059577	0	31.068	N.D. #
14) T	DINOSEB	0.000	15.692	0	4445394	N.D.	4.690 #
15) T	Picloram	0.000	16.879	0	10338574	N.D.	6.079 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
Data File : PS001931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2018 02:23
Operator : EI\SJ
Sample : J5287-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:21:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

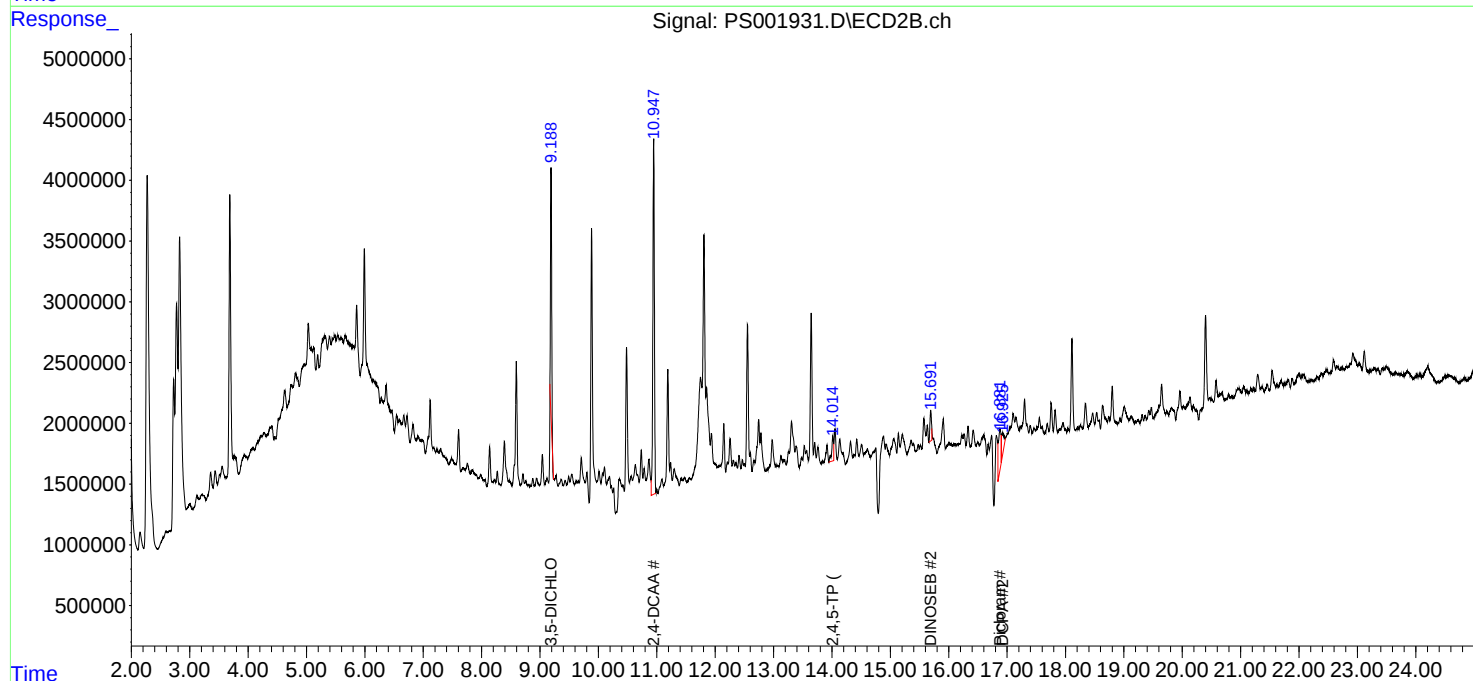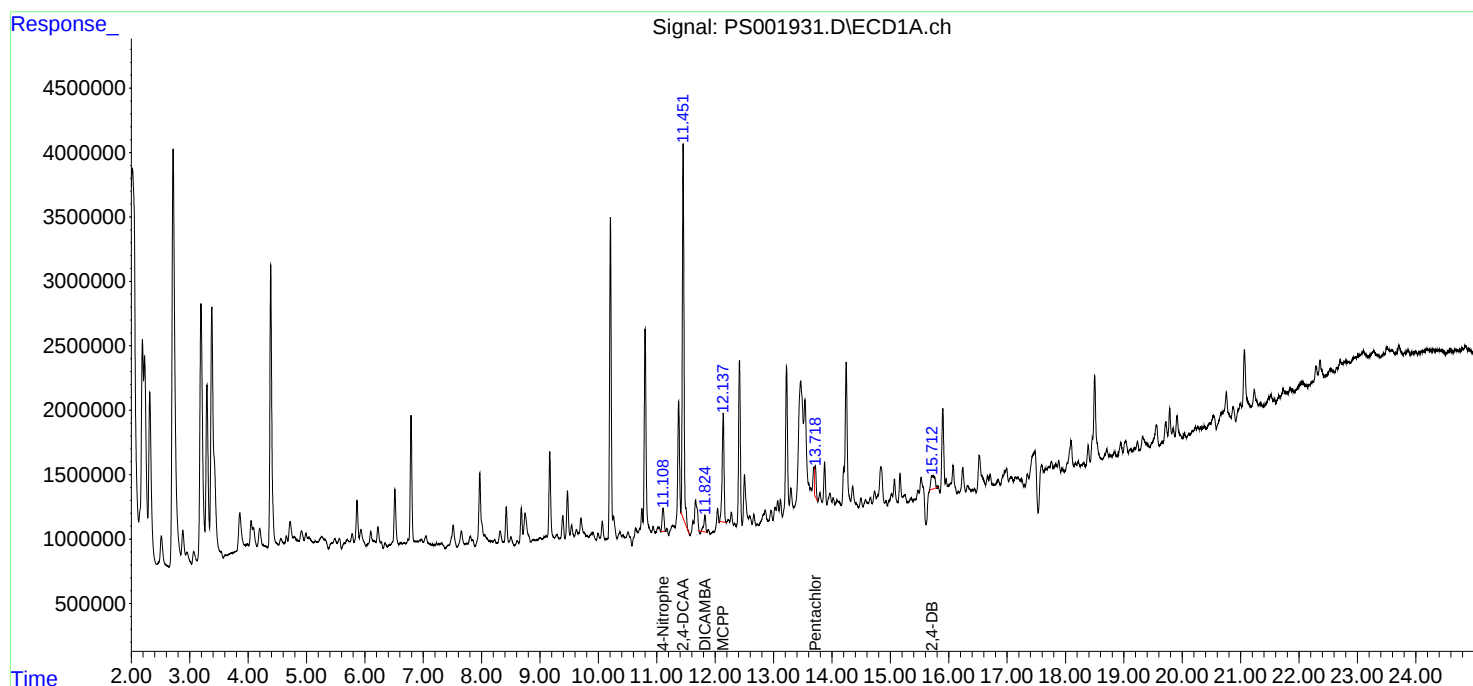


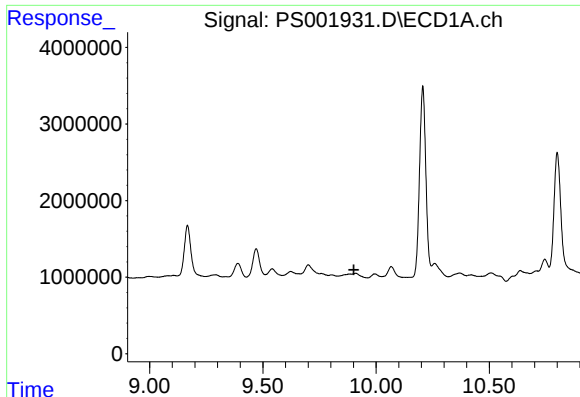

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.902 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

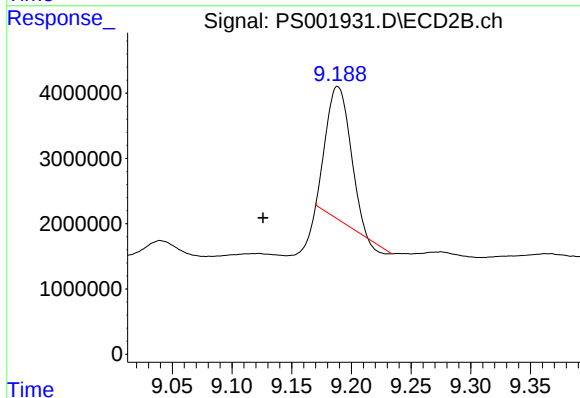


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.188 min
Delta R.T.: 0.063 min
Response: 28145590
Conc: 89.17 ng/ml

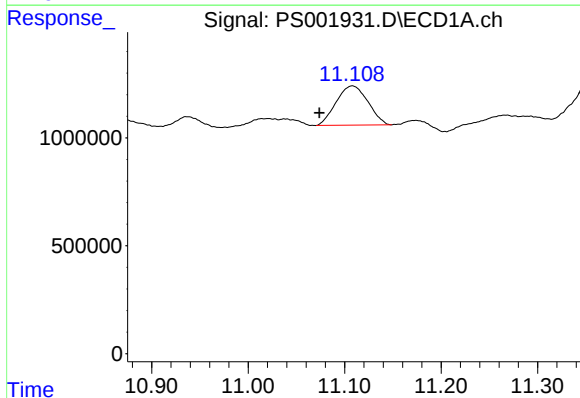


#3 4-Nitrophenol

R.T.: 11.108 min
Delta R.T.: 0.034 min
Response: 4164324
Conc: 29.59 ng/ml

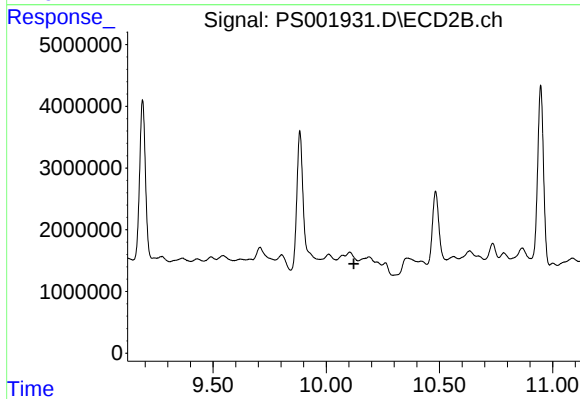

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.122 min
Response: 0
Conc: N.D.

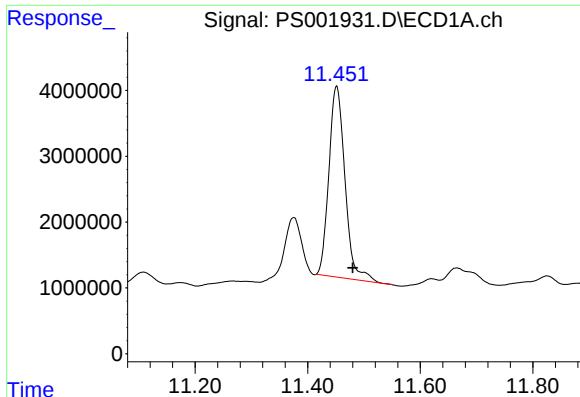

#4 2,4-DCAA


R.T.: 11.451 min
Delta R.T.: -0.028 min
Response: 57551471
Conc: 256.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

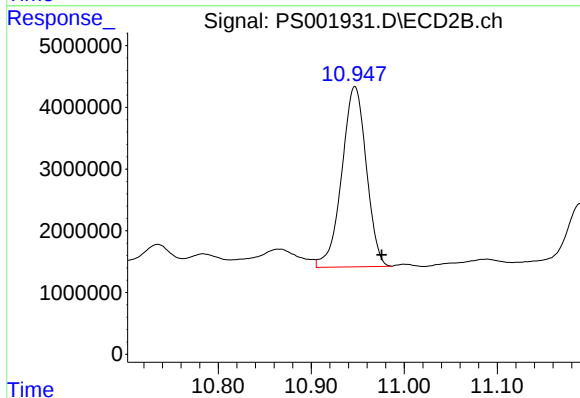


#4 2,4-DCAA

R.T.: 10.947 min
Delta R.T.: -0.029 min
Response: 53470564
Conc: 210.50 ng/ml

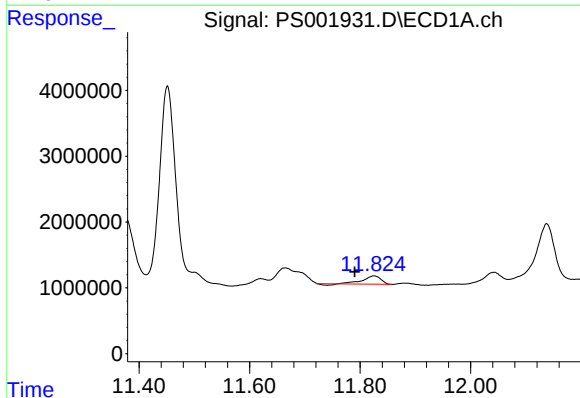


#5 DICAMBA

R.T.: 11.825 min
Delta R.T.: 0.035 min
Response: 2778696
Conc: 3.21 ng/ml

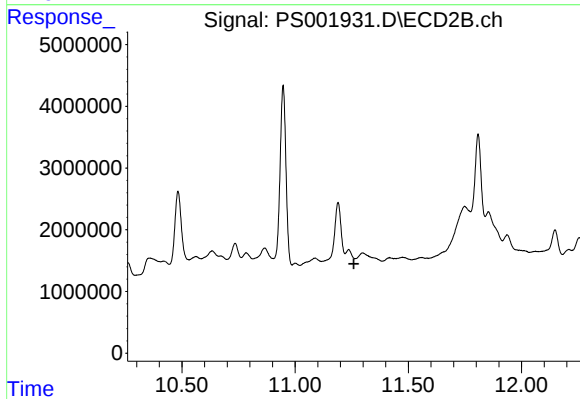

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.260 min
Response: 0
Conc: N.D.

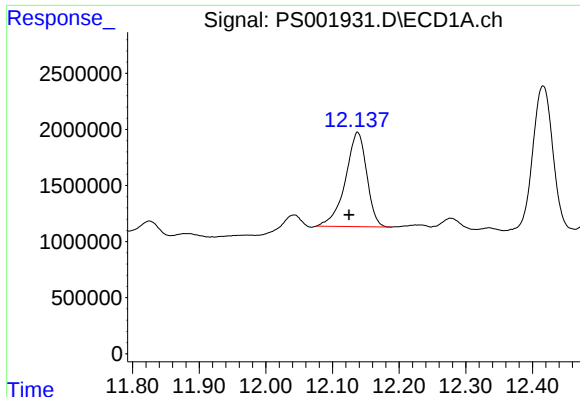

#6 MCP


R.T.: 12.138 min
Delta R.T.: 0.013 min
Response: 18713660
Conc: 29.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

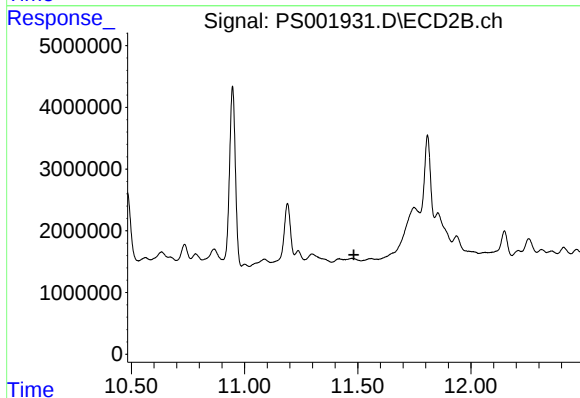


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.483 min
Response: 0
Conc: N.D.

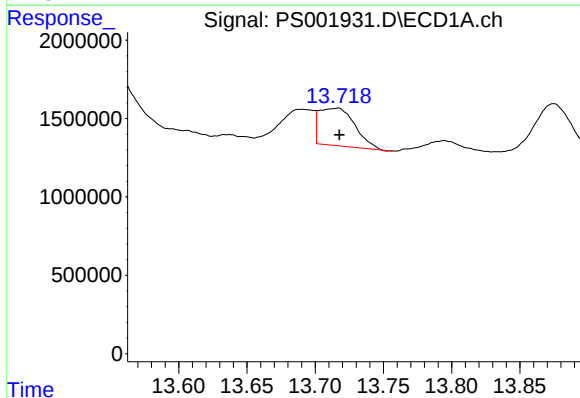


#10 Pentachlorophenol

R.T.: 13.714 min
Delta R.T.: -0.003 min
Response: 4323993
Conc: 1.41 ng/ml

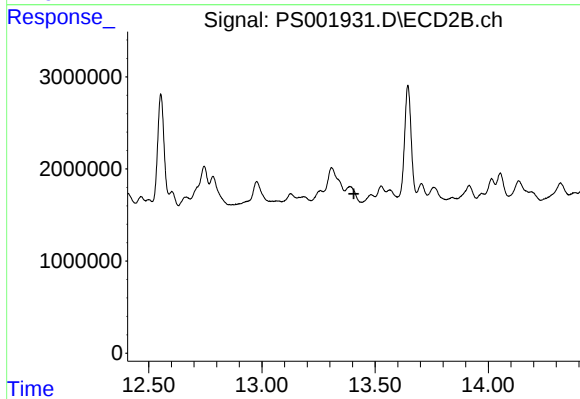

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.407 min
Response: 0
Conc: N.D.

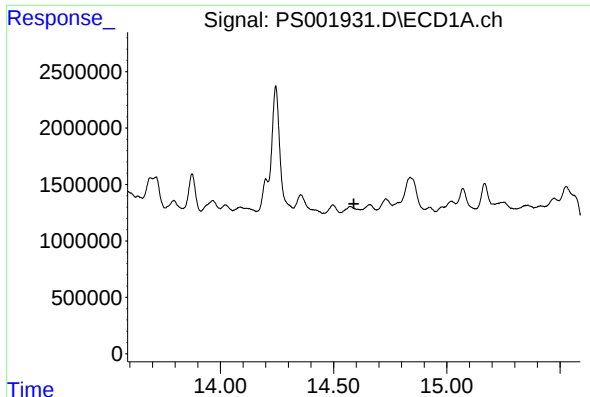

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.590 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

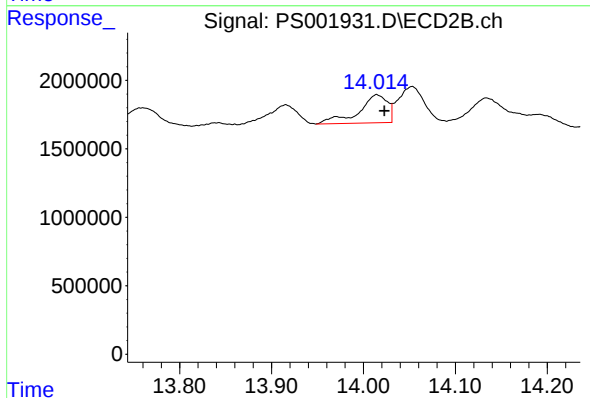


#11 2,4,5-TP (SILVEX)

R.T.: 14.015 min
Delta R.T.: -0.008 min
Response: 4444403
Conc: 3.24 ng/ml

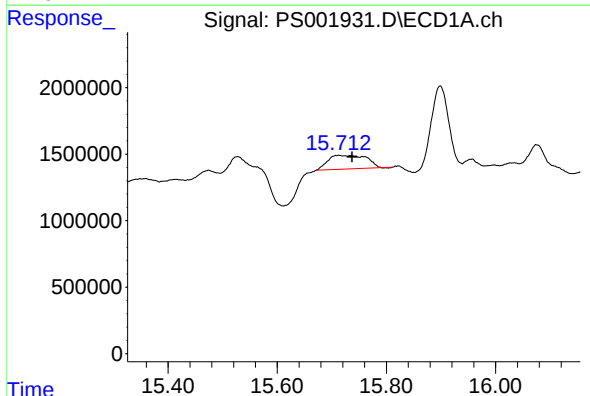


#13 2,4-DB

R.T.: 15.712 min
Delta R.T.: -0.025 min
Response: 5059577
Conc: 31.07 ng/ml

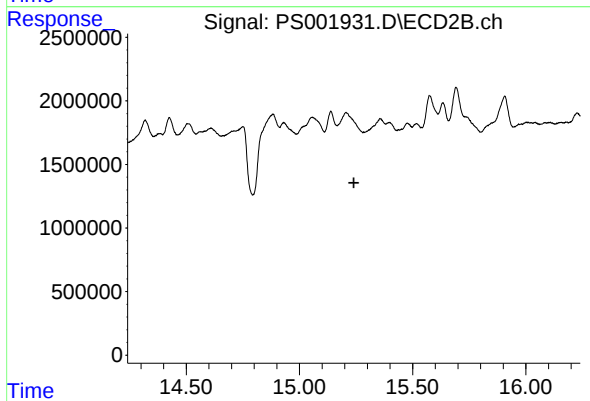

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.240 min
Response: 0
Conc: N.D.

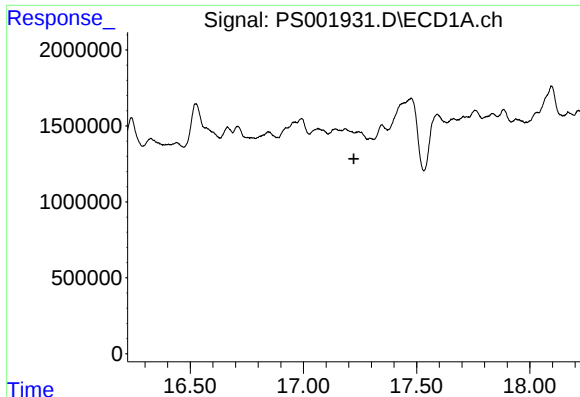

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.223 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

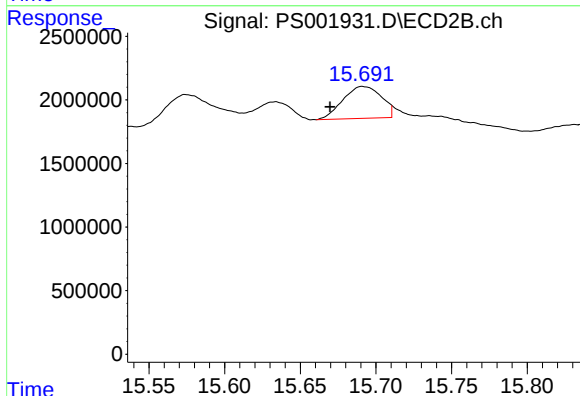


#14 DINOSEB

R.T.: 15.692 min
Delta R.T.: 0.022 min
Response: 4445394
Conc: 4.69 ng/ml

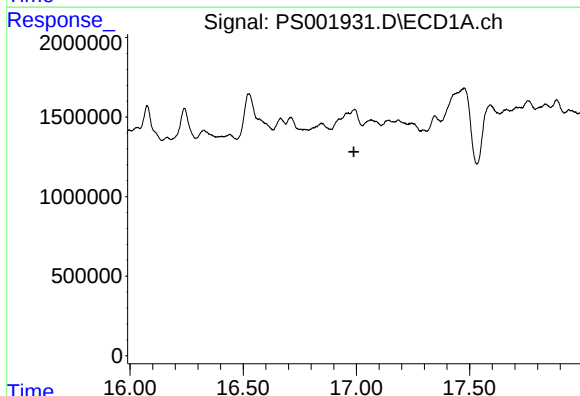


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.988 min
Response: 0
Conc: N.D.

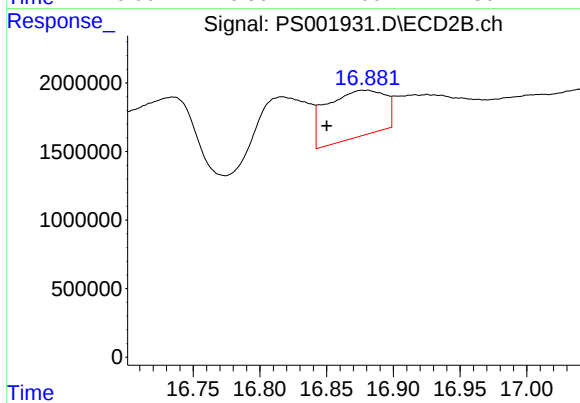

#15 Picloram


R.T.: 16.879 min
Delta R.T.: 0.029 min
Response: 10338574
Conc: 6.08 ng/ml

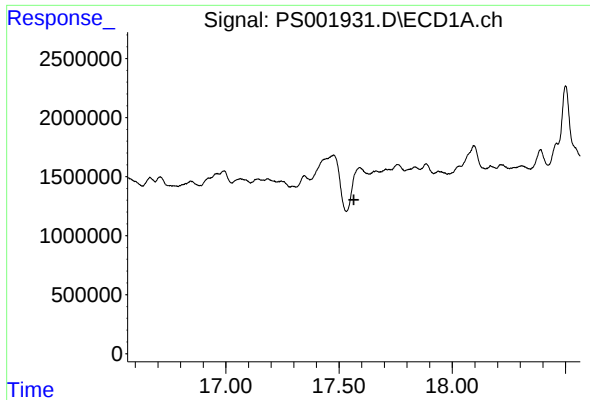

#16 DCPA

R.T.: 17.591 min
Delta R.T.: 0.026 min
Response: -8259902
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

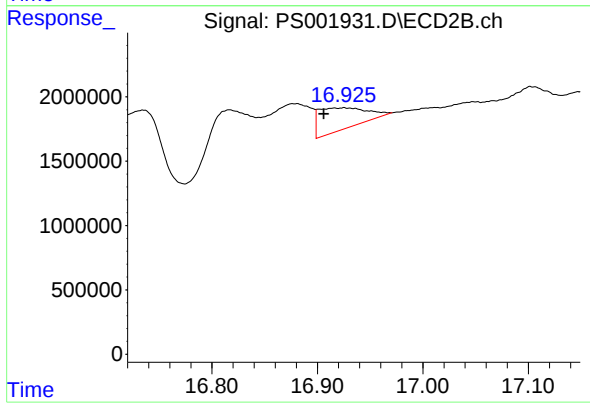

#16 DCPA

R.T.: 16.926 min
Delta R.T.: 0.020 min
Response: 5520884
Conc: 2.99 ng/ml