

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
 Data File : PS001933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2018 03:25
 Operator : EI\SJ
 Sample : J5294-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:22:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.480	10.976	64084084	58341193	285.687	229.675
Target Compounds							
1) T	Dalapon	2.911	0.000	5591199	0	17.195	N.D. #
5) T	DICAMBA	0.000	11.219	0	13293250	N.D.	14.905 #
6) T	MCPD	12.164	0.000	14431938	0	22.648	N.D. #
7) T	MCPA	12.444	11.837	14020825	-633024	13.360	N.D. #
9) T	2,4-D	0.000	12.816	0	9705860	N.D.	31.198 #
10) T	Pentachlo...	13.724	13.406	3273106	-514374	1.065	N.D. #
13) T	2,4-DB	15.763	0.000	4169958	0	25.606	N.D. #
14) T	DINOSEB	0.000	15.662	0	1284777	N.D.	1.356 #
15) T	Picloram	0.000	16.848	0	95569	N.D.	0.056 #
16) T	DCPA	0.000	16.908	0	5199030	N.D.	2.819 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
Data File : PS001933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2018 03:25
Operator : EI\SJ
Sample : J5294-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:22:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

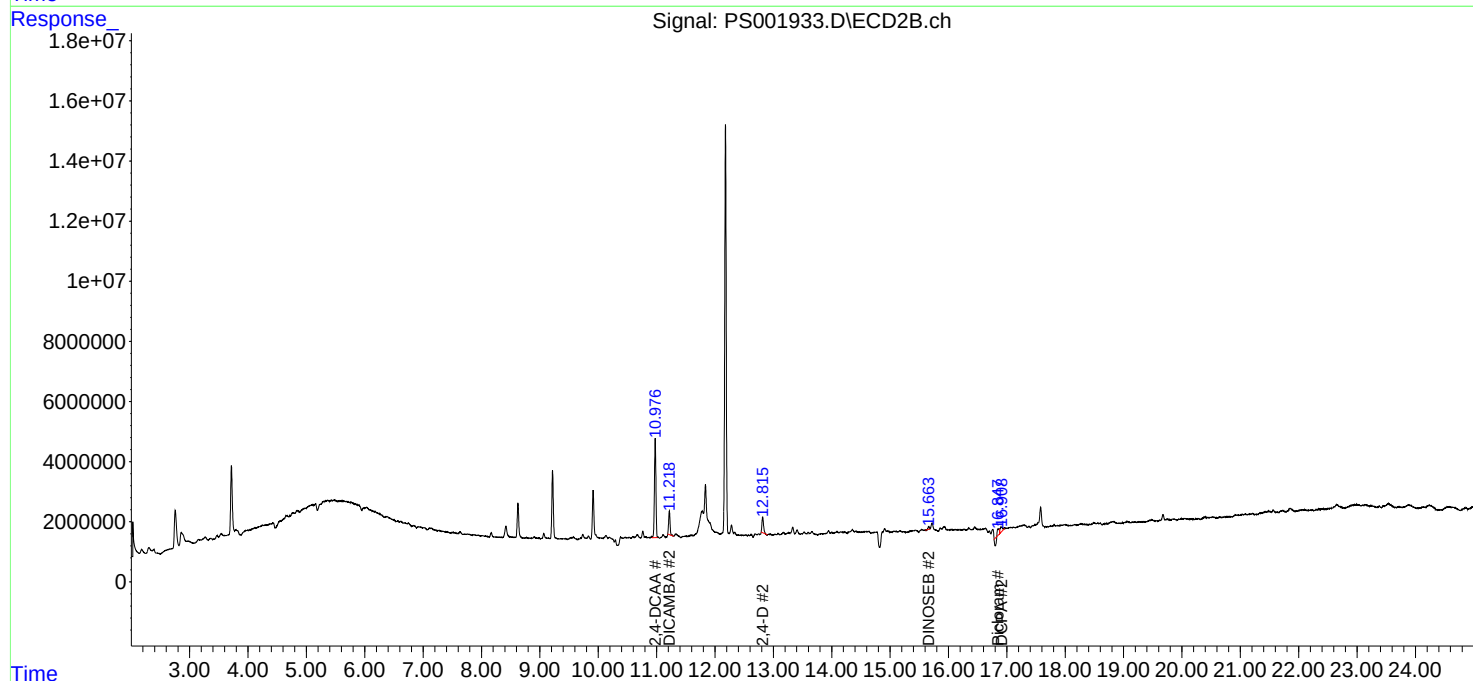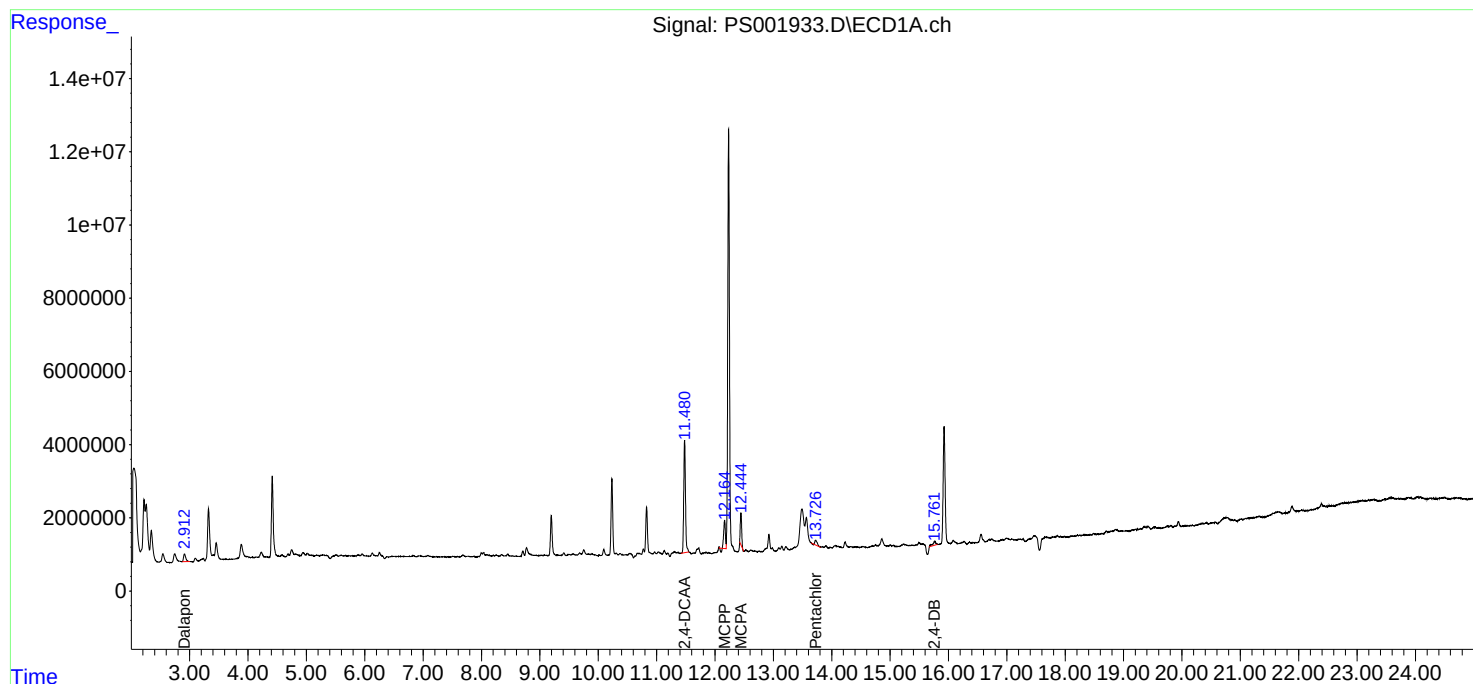


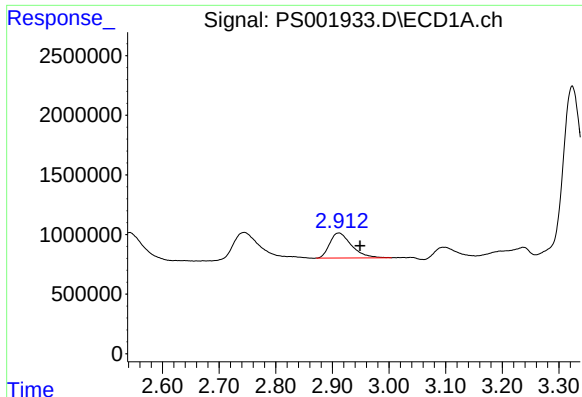

#1 Dalapon


R.T.: 2.911 min
Delta R.T.: -0.038 min
Response: 5591199
Conc: 17.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

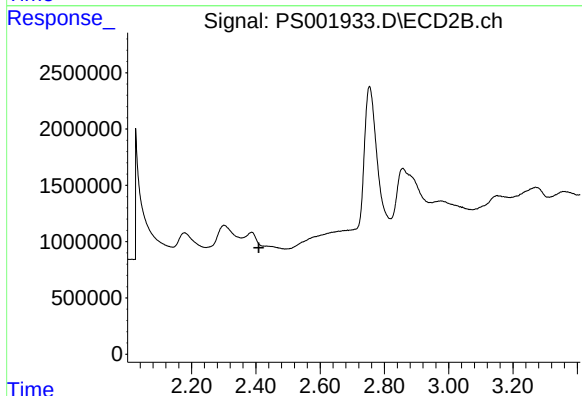


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.410 min
Response: 0
Conc: N.D.

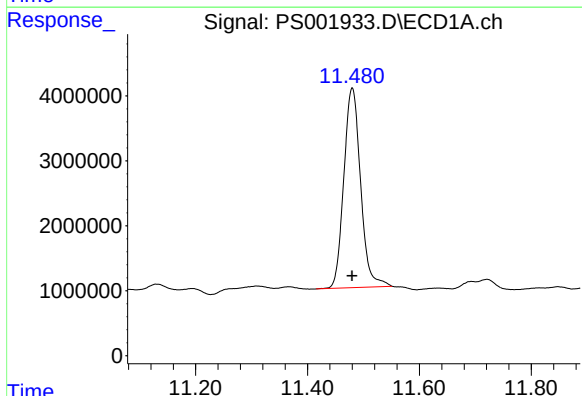


#4 2,4-DCAA

R.T.: 11.480 min
Delta R.T.: 0.000 min
Response: 64084084
Conc: 285.69 ng/ml

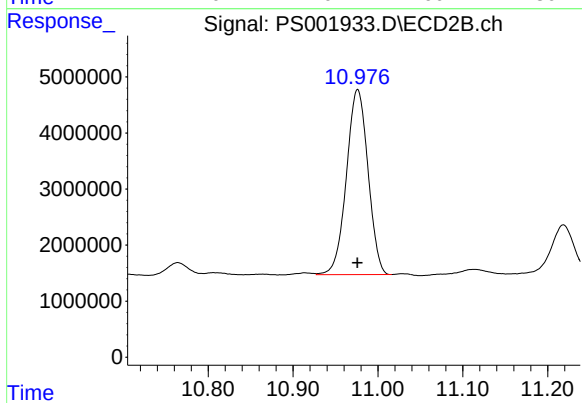

#4 2,4-DCAA


R.T.: 10.976 min
Delta R.T.: 0.000 min
Response: 58341193
Conc: 229.67 ng/ml

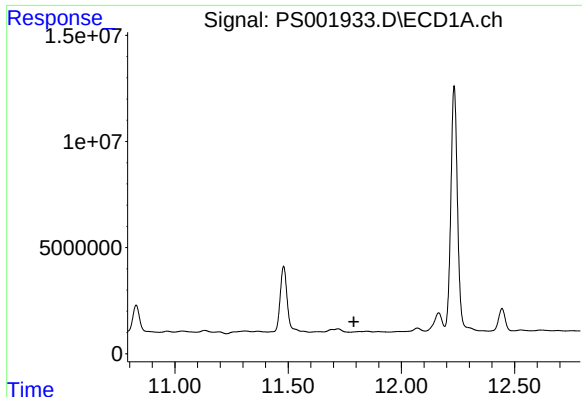

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

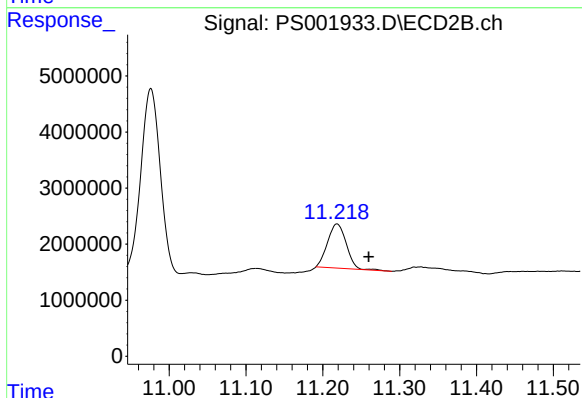


#5 DICAMBA

R.T.: 11.219 min
Delta R.T.: -0.041 min
Response: 13293250
Conc: 14.90 ng/ml

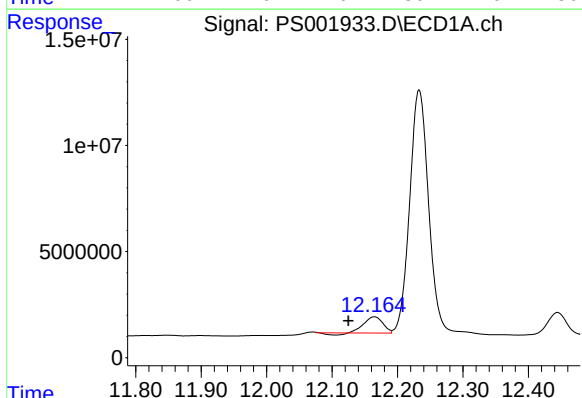


#6 MCPP

R.T.: 12.164 min
Delta R.T.: 0.040 min
Response: 14431938
Conc: 22.65 ug/ml

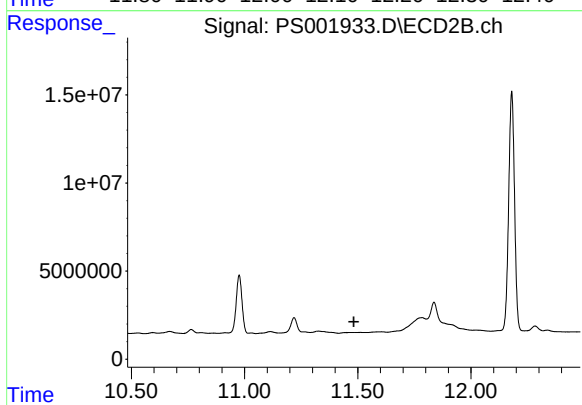

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.483 min
Response: 0
Conc: N.D.

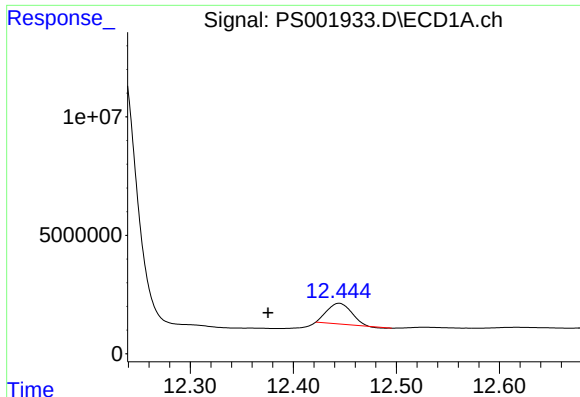

#7 MCPA


R.T.: 12.444 min
Delta R.T.: 0.069 min
Response: 14020825
Conc: 13.36 ug/ml

Instrument :
ECD_S
ClientSampleId :

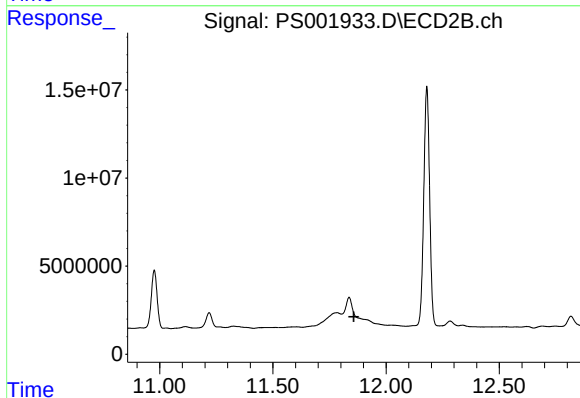


#7 MCPA

R.T.: 11.837 min
Delta R.T.: -0.021 min
Response: -633024
Conc: N.D.

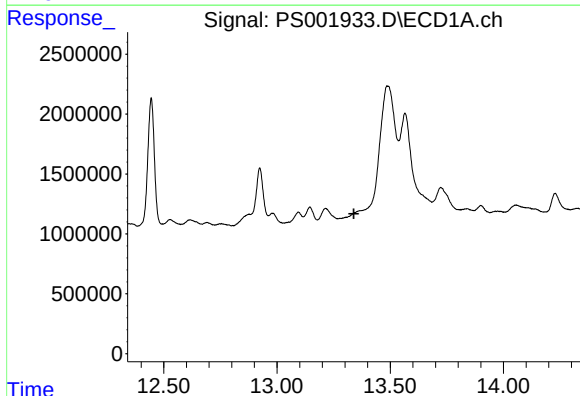


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.340 min
Response: 0
Conc: N.D.

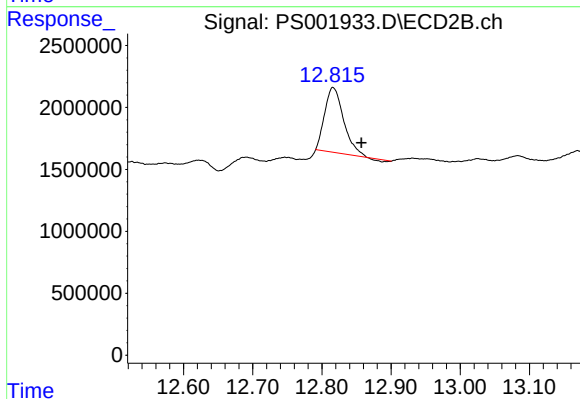

#9 2,4-D


R.T.: 12.816 min
Delta R.T.: -0.041 min
Response: 9705860
Conc: 31.20 ng/ml

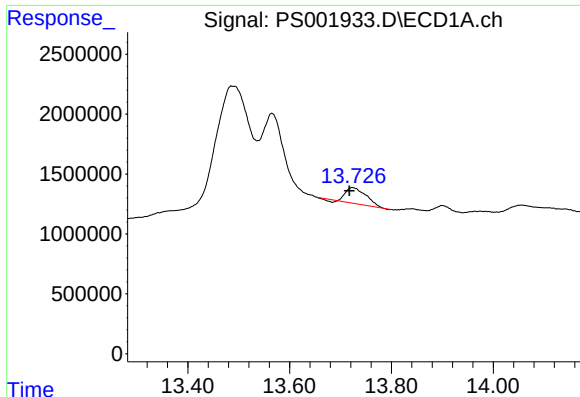

#10 Pentachlorophenol


R.T.: 13.724 min
Delta R.T.: 0.006 min
Response: 3273106
Conc: 1.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

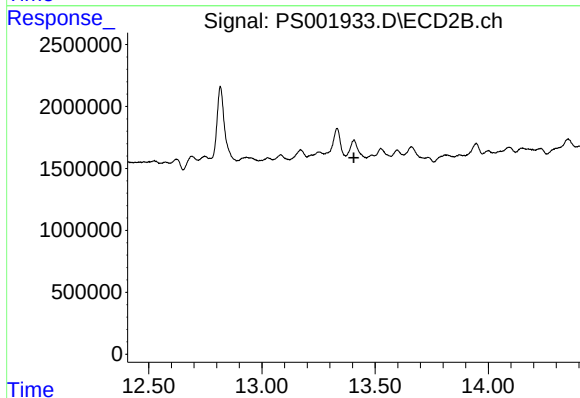


#10 Pentachlorophenol

R.T.: 13.406 min
Delta R.T.: 0.000 min
Response: -514374
Conc: N.D.

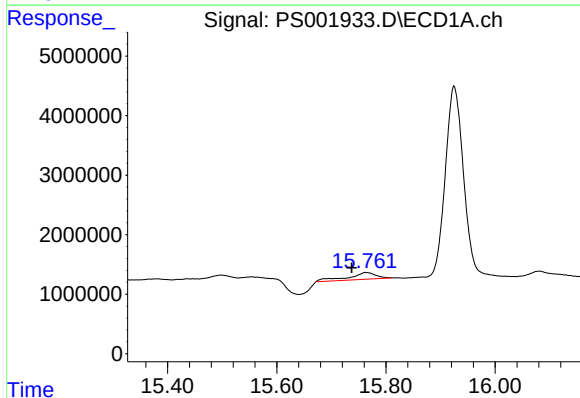


#13 2,4-DB

R.T.: 15.763 min
Delta R.T.: 0.026 min
Response: 4169958
Conc: 25.61 ng/ml

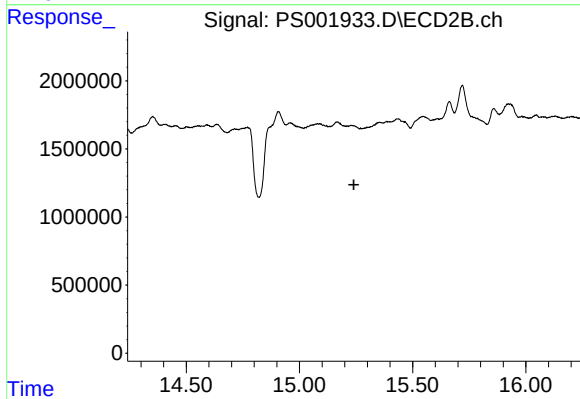

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.240 min
Response: 0
Conc: N.D.

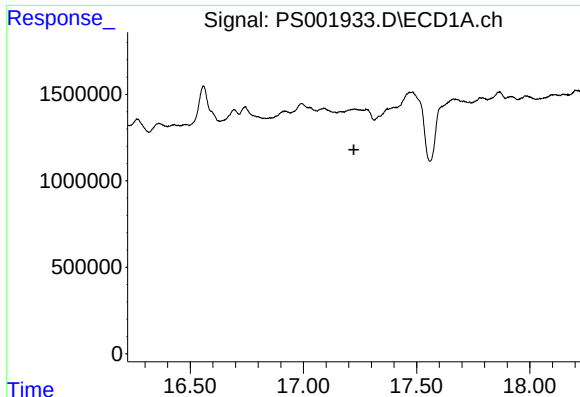

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.223 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

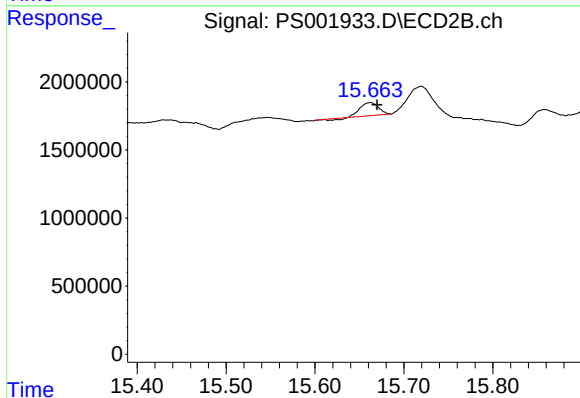


#14 DINOSEB

R.T.: 15.662 min
Delta R.T.: -0.008 min
Response: 1284777
Conc: 1.36 ng/ml

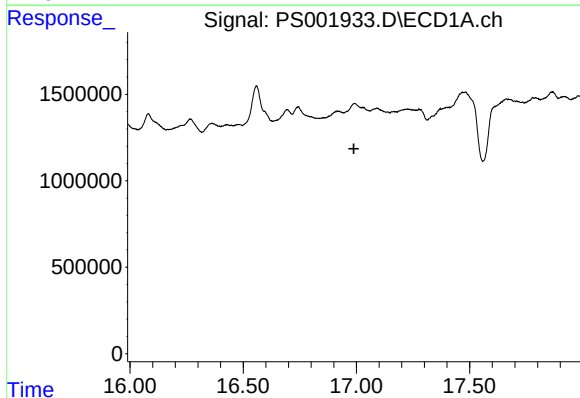


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.988 min
Response: 0
Conc: N.D.

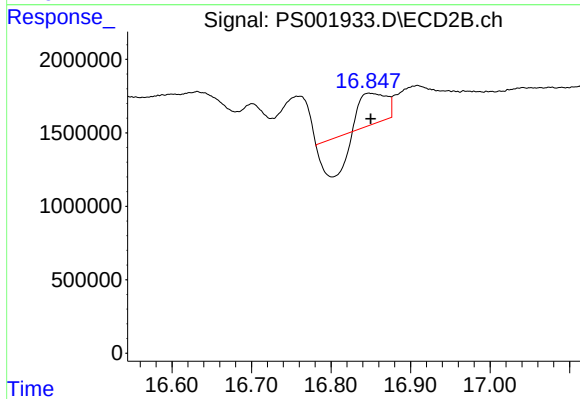

#15 Picloram


R.T.: 16.848 min
Delta R.T.: -0.002 min
Response: 95569
Conc: 0.06 ng/ml

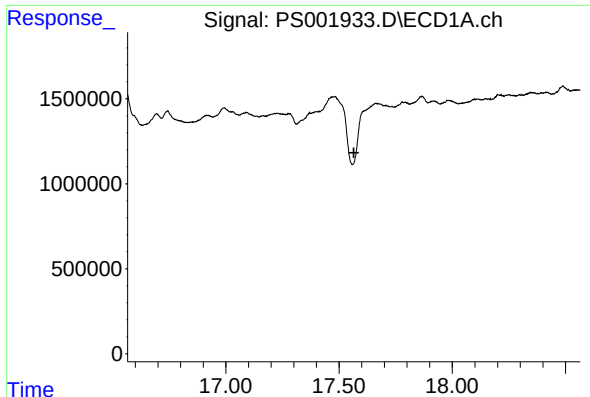

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

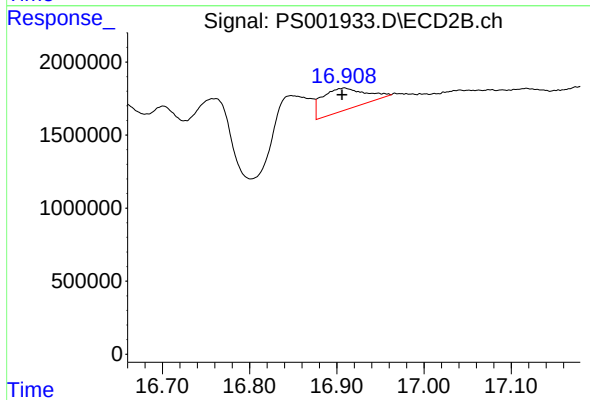

#16 DCPA

R.T.: 16.908 min
Delta R.T.: 0.002 min
Response: 5199030
Conc: 2.82 ng/ml