

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
 Data File : PS001920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2018 20:42
 Operator : EI\SJ
 Sample : J5242-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-01-E9-F9-E9A-F9A

Manual Integrations
 APPROVED

Sohil
 10/9/2018 3:36:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 05:18:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 18 03:01:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	11.475	10.971	53647911	54112462	239.163m	213.027m
------	----------	--------	--------	----------	----------	----------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100818\
Data File : PS001920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2018 20:42
Operator : EI\SJ
Sample : J5242-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-E9-F9-E9A-F9A


Manual Integrations
APPROVED

Sohil
10/9/2018 3:36:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 05:18:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Tue Sep 18 03:01:16 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

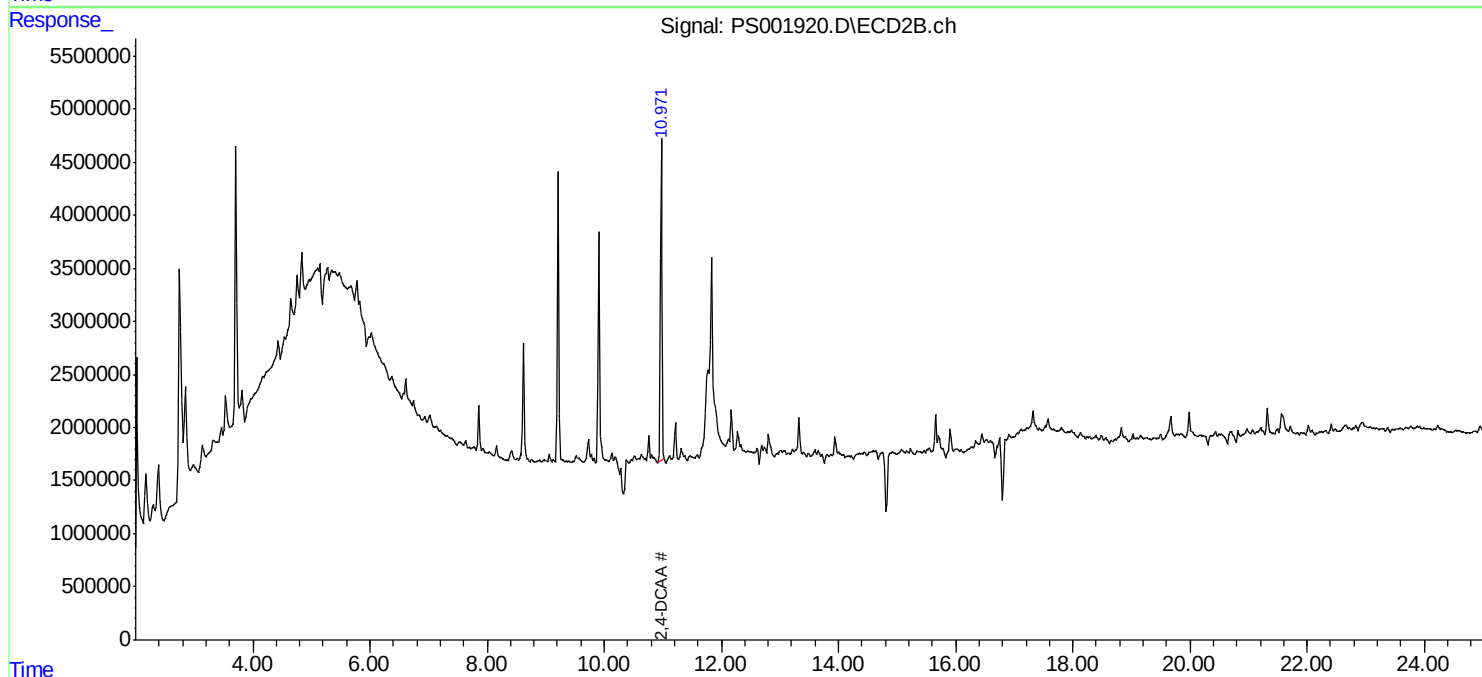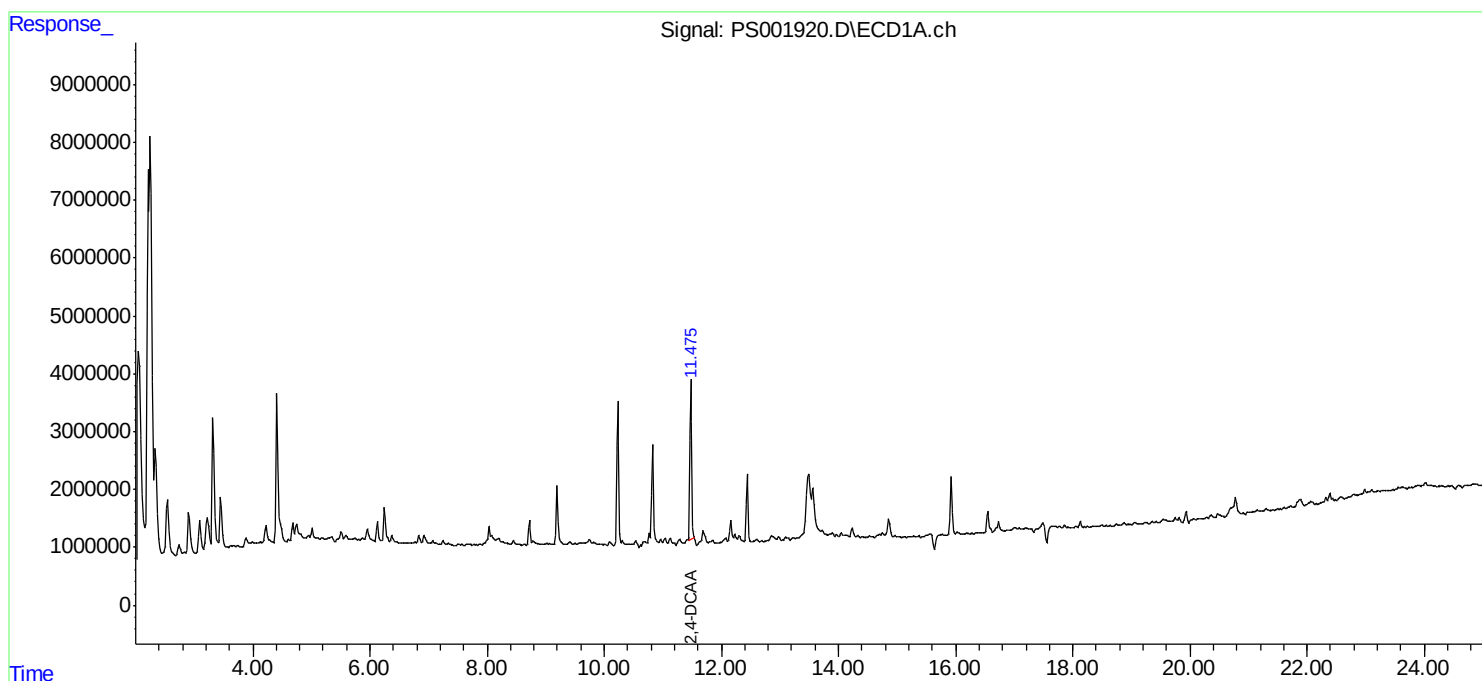

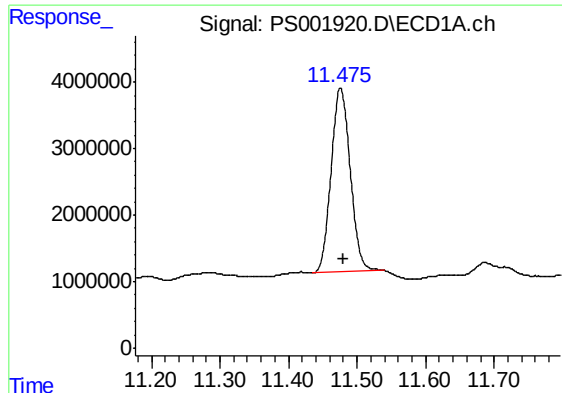


#4 2,4-DCAA

R.T.: 11.475 min
Delta R.T.: -0.004 min
Response: 53647911
Conc: 239.16 ng/ml m

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-E9-F9-E9A-F9A

Manual Integrations
APPROVED

Sohil
10/9/2018 3:36:46 PM

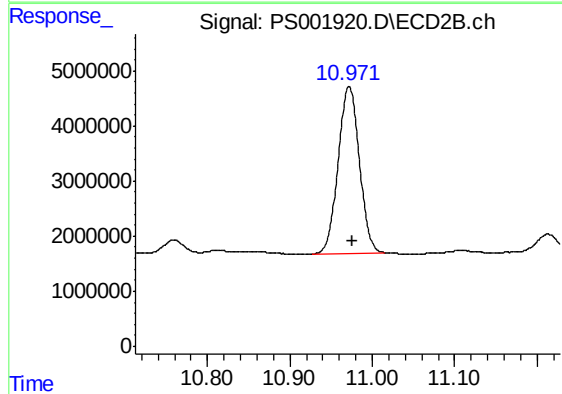

#4 2,4-DCAA

R.T.: 10.971 min
Delta R.T.: -0.005 min
Response: 54112462
Conc: 213.03 ng/ml m