

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100819\
 Data File : PS007093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2019 18:53
 Operator : SM\AJ
 Sample : K5146-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 00:53:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
 Quant Title : 8080.M
 QLast Update : Fri Sep 20 11:14:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.513	5.243	180.0E6	101.5E6	196.961	220.836
Target Compounds							
1) T	Dalapon	2.058	1.772	93187203	88101119	87.221	165.271 #
2) T	3,5-DICHL...	0.000	4.525	0	12837265	N.D.	22.331
5) T	DICAMBA	5.690	0.000	7402313	0	2.291	N.D. #
6) T	MCP	5.803	0.000	9621774	0	4.523	N.D. #
7) T	MCPA	0.000	5.560	0	60973850	N.D.	33.127
8) T	DICHLORPROP	6.229	0.000	8422710	0	10.970	N.D. #
9) T	2,4-D	0.000	6.163	0	18968014	N.D.	37.187
10) T	Pentachlo...	6.733	6.473	28892985	15795566	2.424	2.511
11) T	2,4,5-TP ...	0.000	6.896	0	25474036	N.D.	10.635
12) T	2,4,5-T	7.582	0.000	21861636	0	4.296	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100819\
Data File : PS007093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2019 18:53
Operator : SM\AJ
Sample : K5146-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 00:53:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092019.M
Quant Title : 8080.M
QLast Update : Fri Sep 20 11:14:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

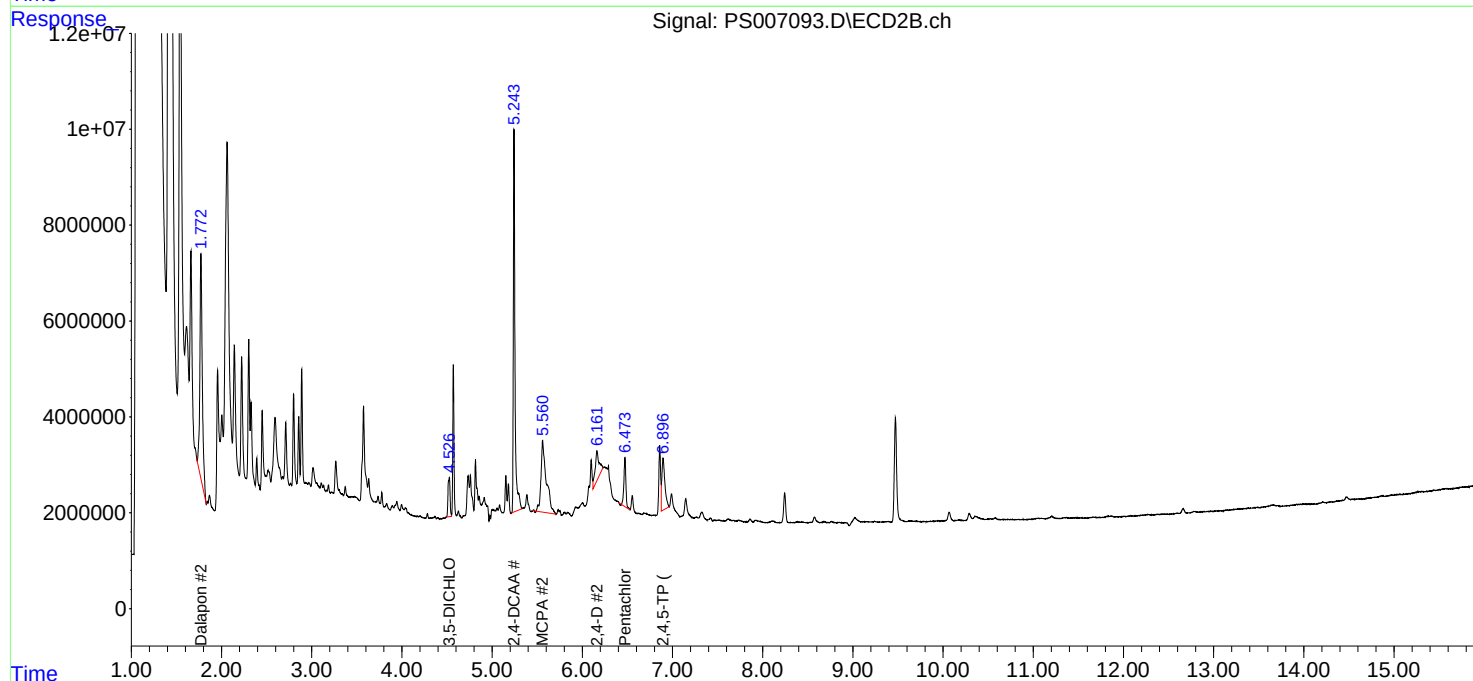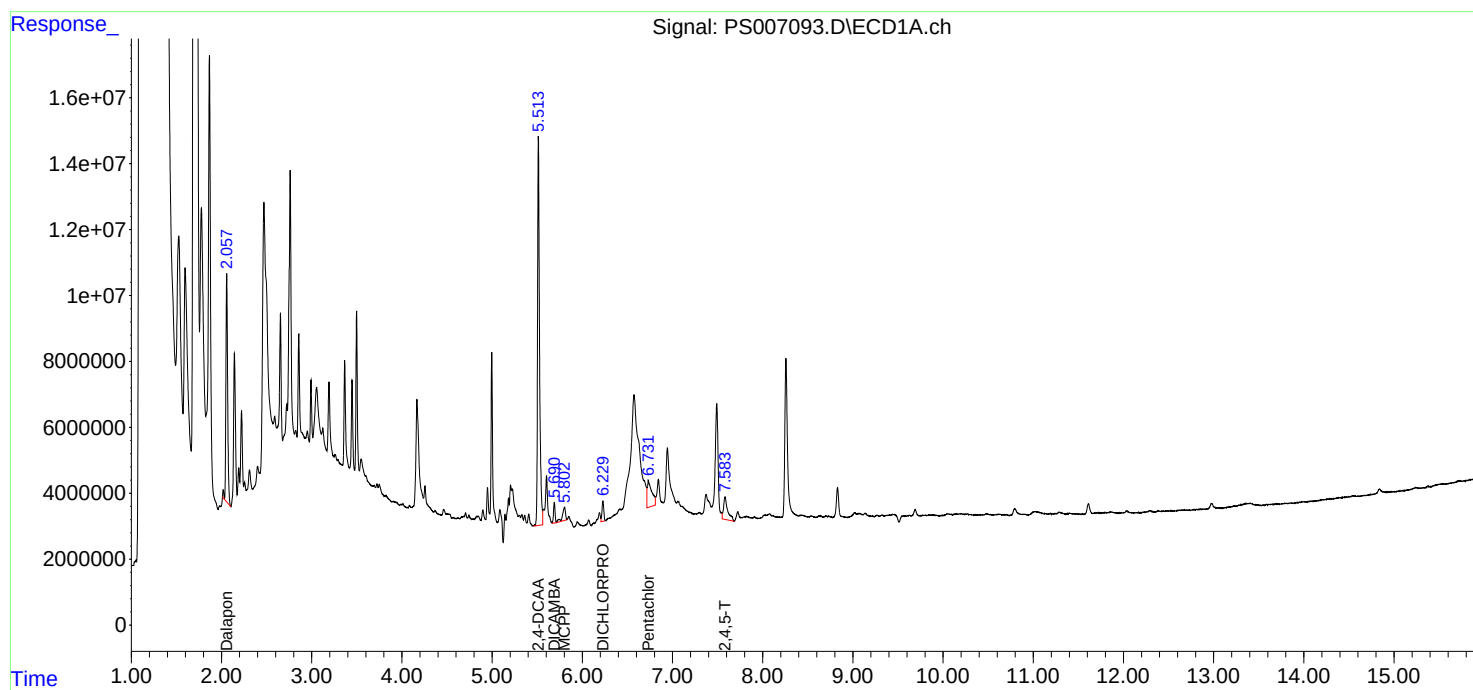


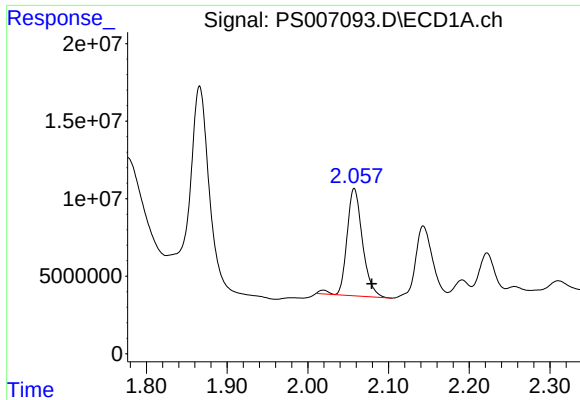

#1 Dalapon


R.T.: 2.058 min
Delta R.T.: -0.021 min
Response: 93187203
Conc: 87.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

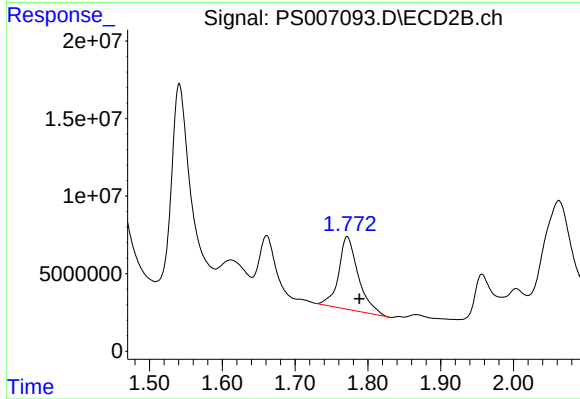


#1 Dalapon

R.T.: 1.772 min
Delta R.T.: -0.016 min
Response: 88101119
Conc: 165.27 ng/ml

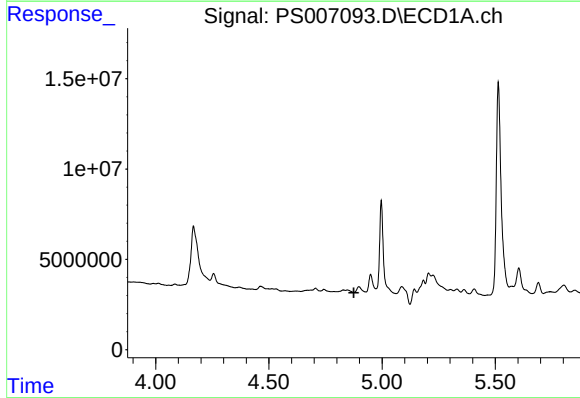


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.876 min
Response: 0
Conc: N.D.

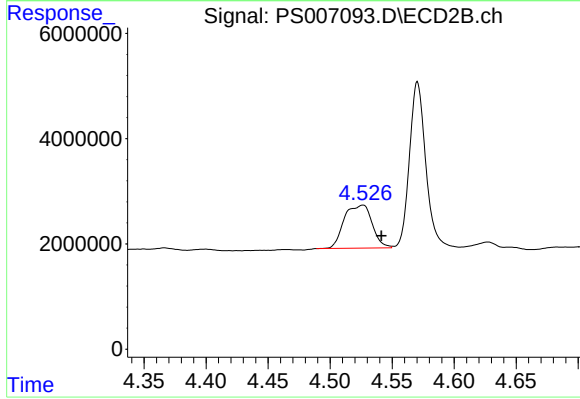

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.525 min
Delta R.T.: -0.016 min
Response: 12837265
Conc: 22.33 ng/ml

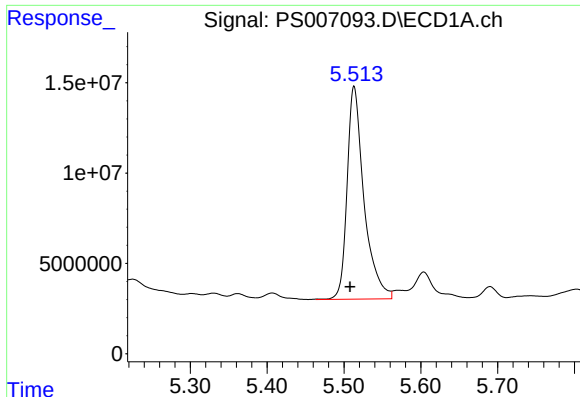

#4 2,4-DCAA


R.T.: 5.513 min
Delta R.T.: 0.005 min
Response: 179985313
Conc: 196.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

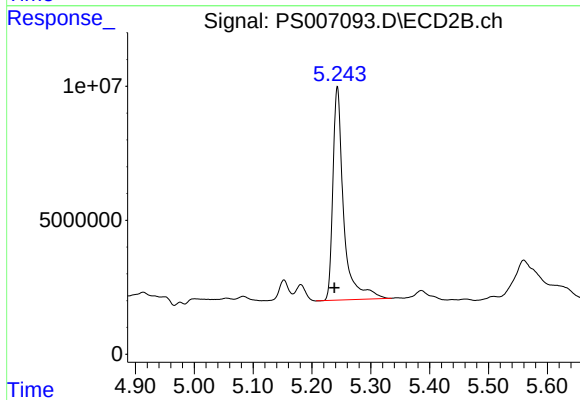


#4 2,4-DCAA

R.T.: 5.243 min
Delta R.T.: 0.005 min
Response: 101549496
Conc: 220.84 ng/ml

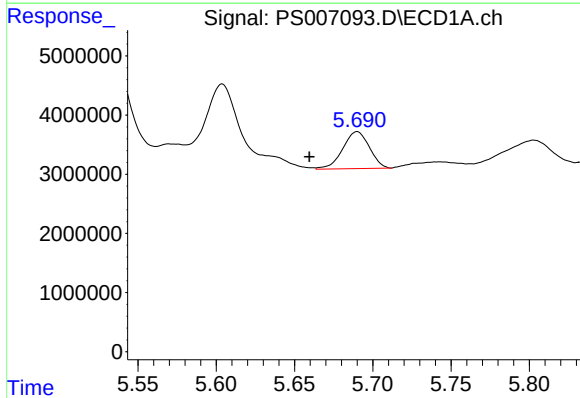


#5 DICAMBA

R.T.: 5.690 min
Delta R.T.: 0.030 min
Response: 7402313
Conc: 2.29 ng/ml

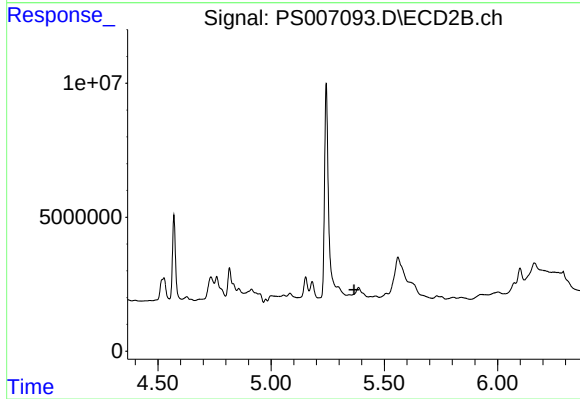

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.366 min
Response: 0
Conc: N.D.

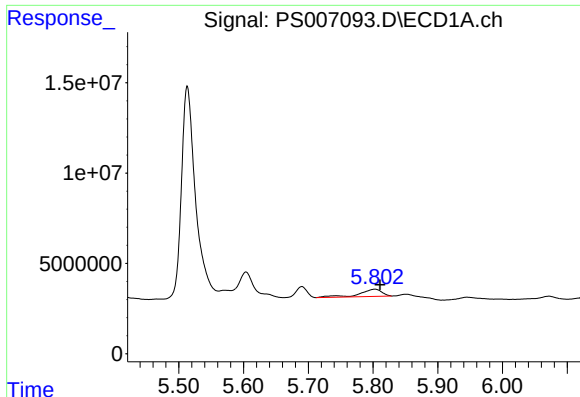

#6 MCP


R.T.: 5.803 min
Delta R.T.: -0.008 min
Response: 9621774
Conc: 4.52 ug/ml

Instrument :
ECD_S
ClientSampleId :

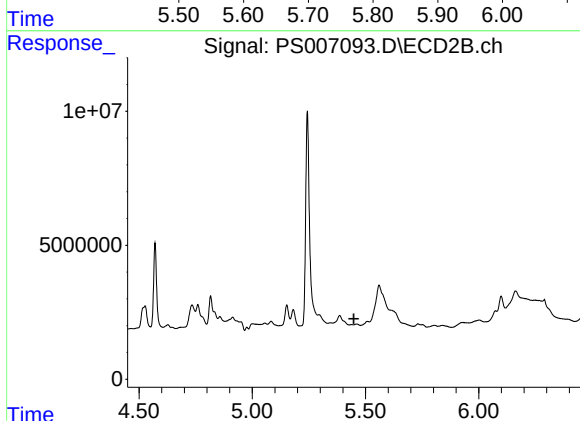


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.449 min
Response: 0
Conc: N.D.

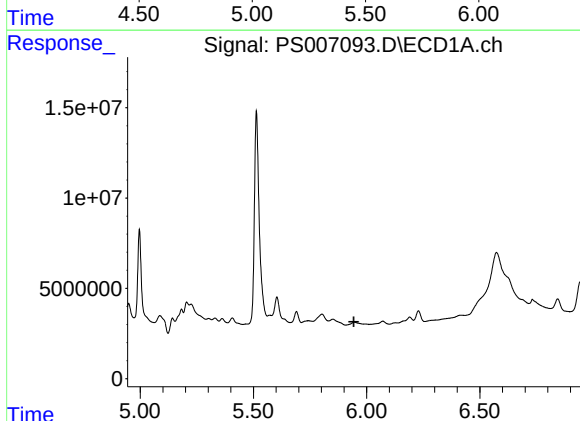


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.944 min
Response: 0
Conc: N.D.

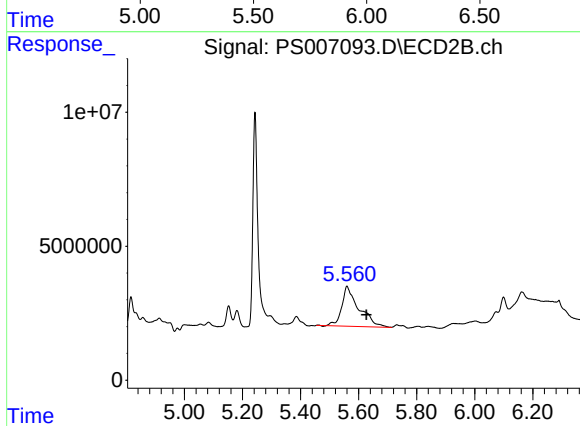

#7 MCPA


R.T.: 5.560 min
Delta R.T.: -0.067 min
Response: 60973850
Conc: 33.13 ug/ml

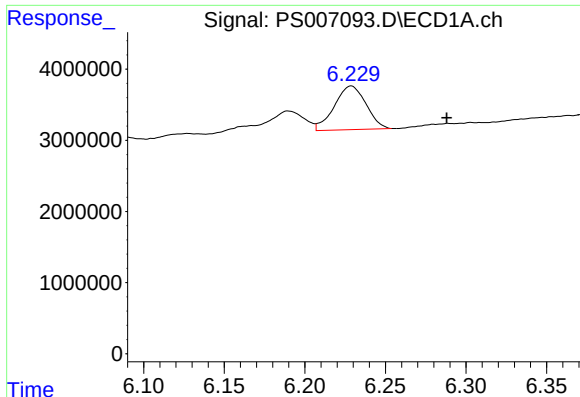

#8 DICHLORPROP


R.T.: 6.229 min
Delta R.T.: -0.059 min
Response: 8422710
Conc: 10.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

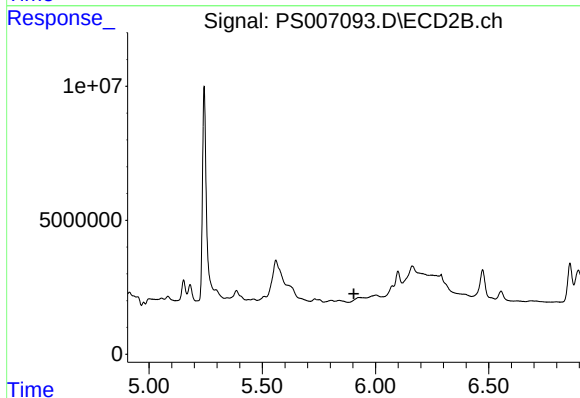


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.905 min
Response: 0
Conc: N.D.

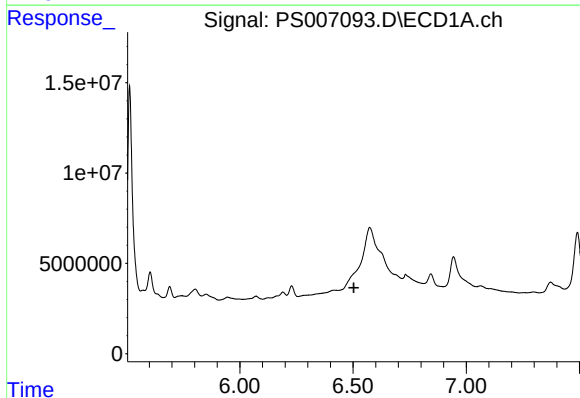


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.504 min
Response: 0
Conc: N.D.

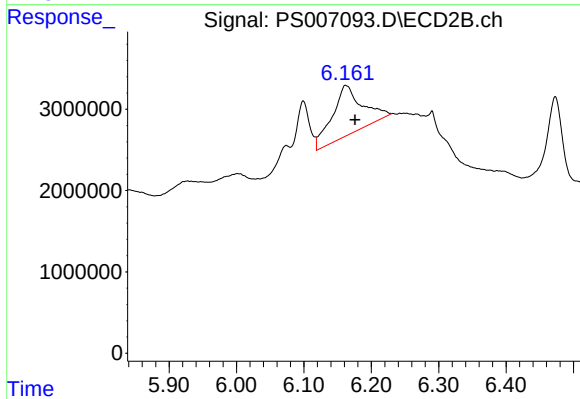

#9 2,4-D


R.T.: 6.163 min
Delta R.T.: -0.013 min
Response: 18968014
Conc: 37.19 ng/ml

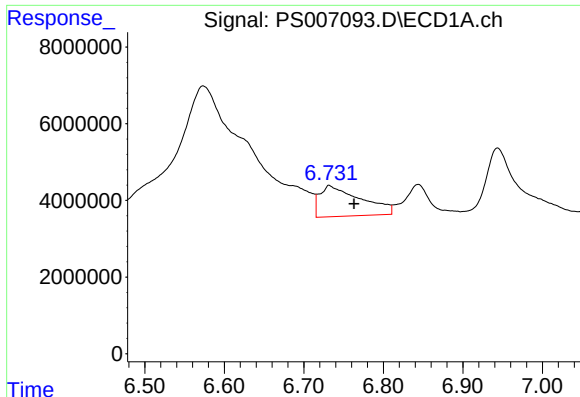

#10 Pentachlorophenol


R.T.: 6.733 min
Delta R.T.: -0.031 min
Response: 28892985
Conc: 2.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

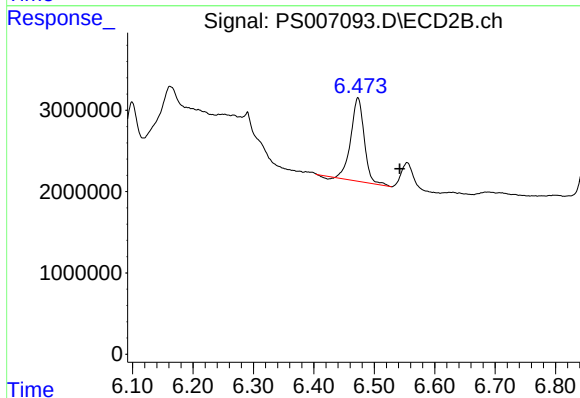


#10 Pentachlorophenol

R.T.: 6.473 min
Delta R.T.: -0.069 min
Response: 15795566
Conc: 2.51 ng/ml

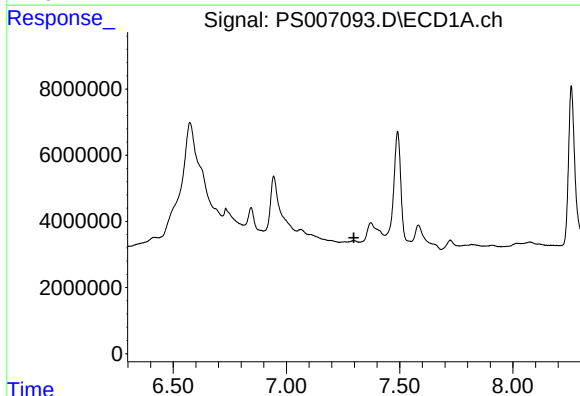


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.298 min
Response: 0
Conc: N.D.

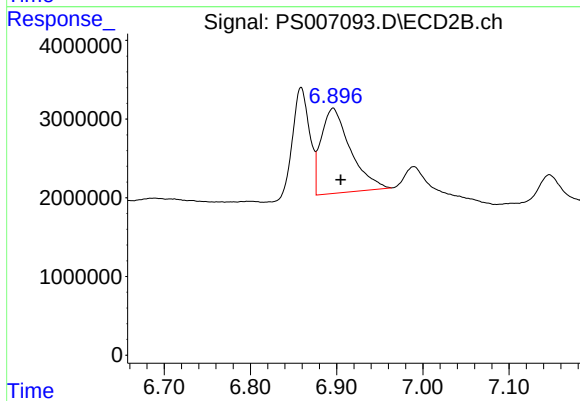

#11 2,4,5-TP (SILVEX)


R.T.: 6.896 min
Delta R.T.: -0.009 min
Response: 25474036
Conc: 10.63 ng/ml

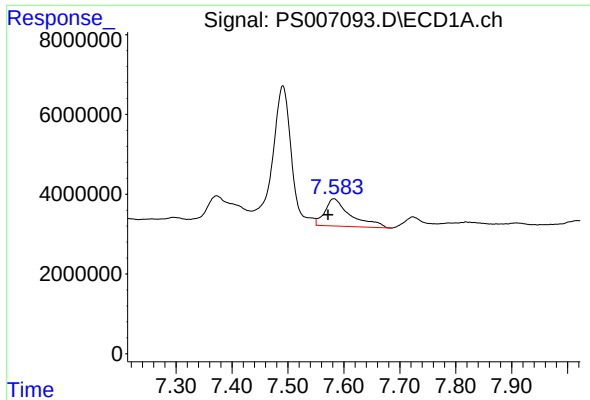

#12 2,4,5-T

R.T.: 7.582 min
Delta R.T.: 0.011 min
Response: 21861636
Conc: 4.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

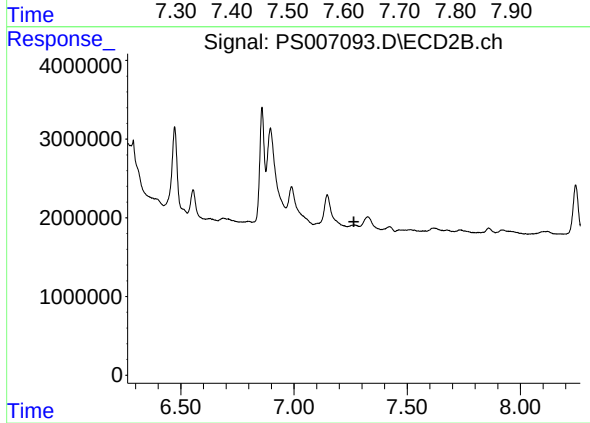

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.265 min
Response: 0
Conc: N.D.