

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100820\
 Data File : PS012760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2020 10:14
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 11:24:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.475	0.000	290.3E6	0	215.295	N.D. #
3) T	4-Nitroph...	7.011	0.000	3015205	0	6.201	N.D. #
7) T	MCPA	7.695	0.000	11931515	0	2.861	N.D. #
8) T	DICHLORPROP	8.140	7.756	27861802	9305247	28.792	18.022 #
15) T	Picloram	10.977	11.027	199.8E6	17361269	27.753	4.405 #
16) T	DCPA	0.000	10.935	0	3427887	N.D.	1.031



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100820\
Data File : PS012760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2020 10:14
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 11:24:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

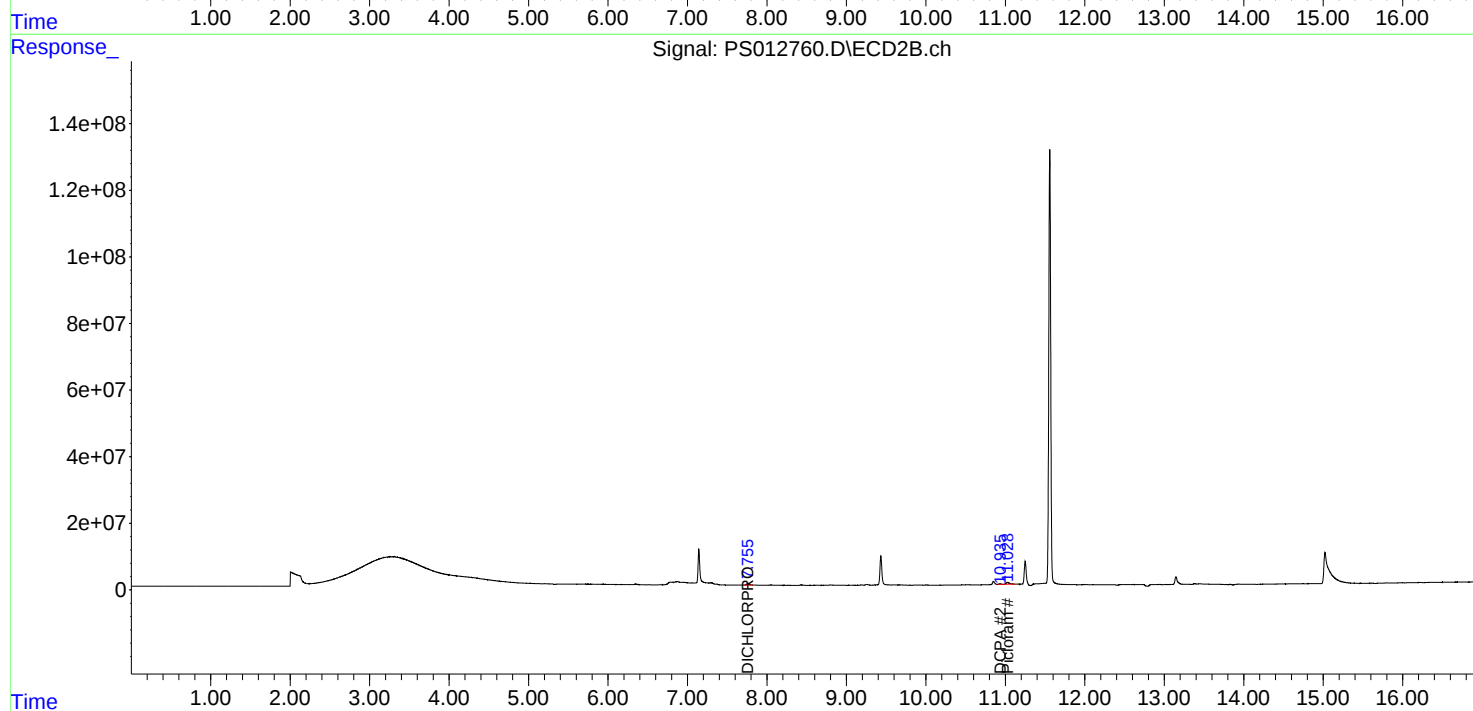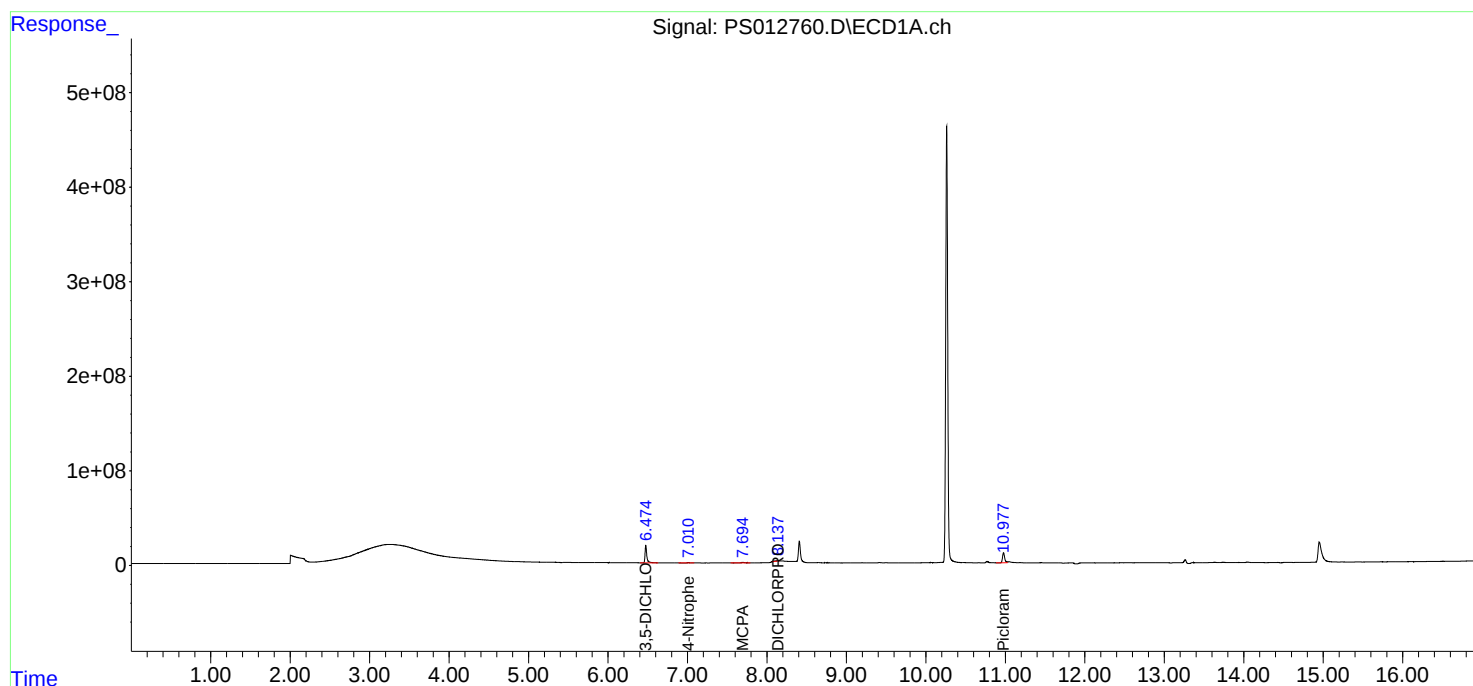


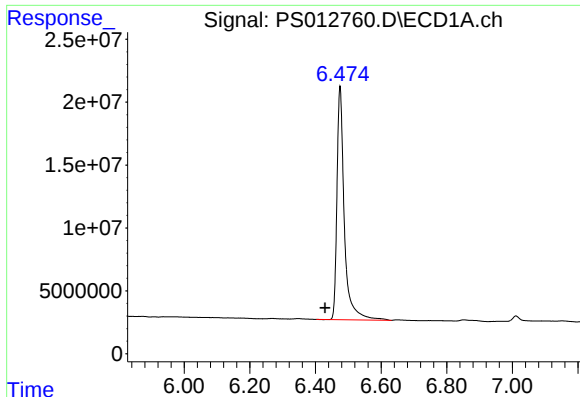

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.475 min
Delta R.T.: 0.045 min
Response: 290312976
Conc: 215.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

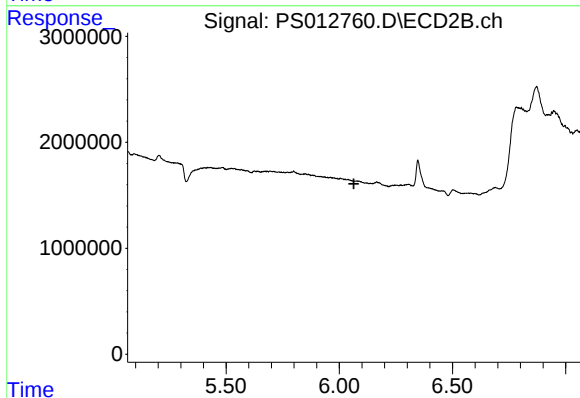


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.064 min
Response: 0
Conc: N.D.

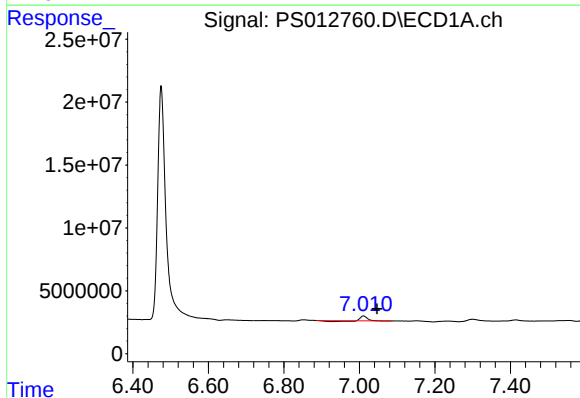


#3 4-Nitrophenol

R.T.: 7.011 min
Delta R.T.: -0.036 min
Response: 3015205
Conc: 6.20 ng/ml

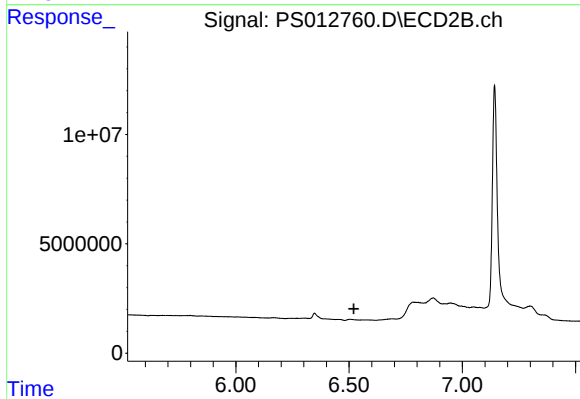

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

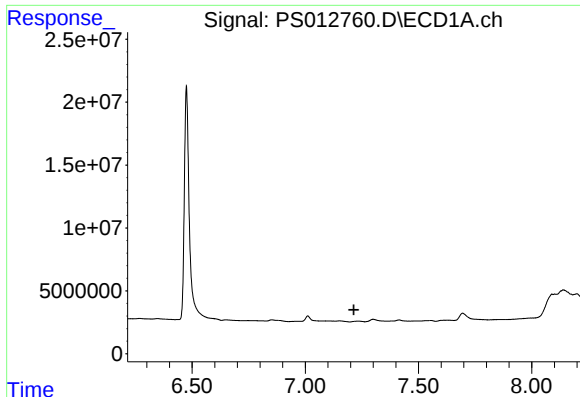

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.215 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

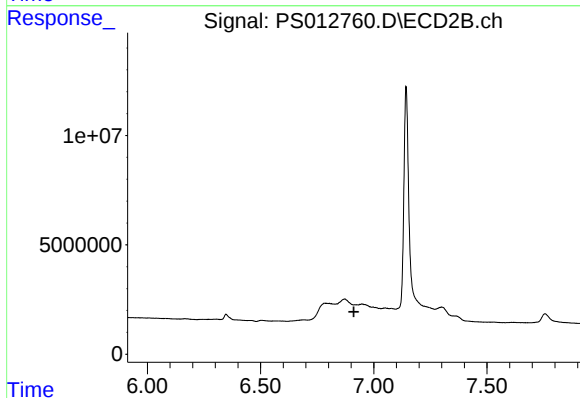


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.912 min
Response: 0
Conc: N.D.

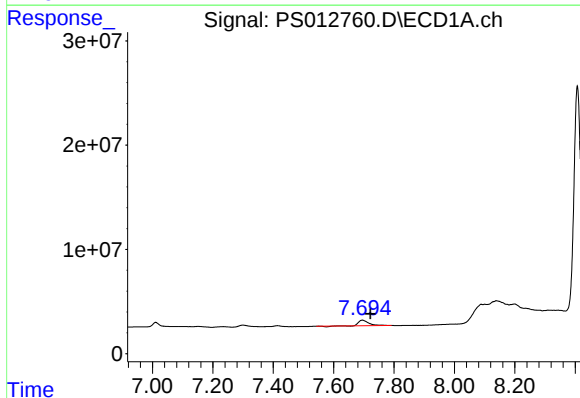


#7 MCPA

R.T.: 7.695 min
Delta R.T.: -0.027 min
Response: 11931515
Conc: 2.86 ug/ml

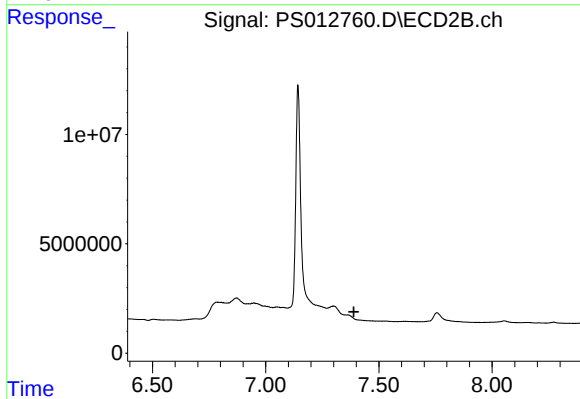

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

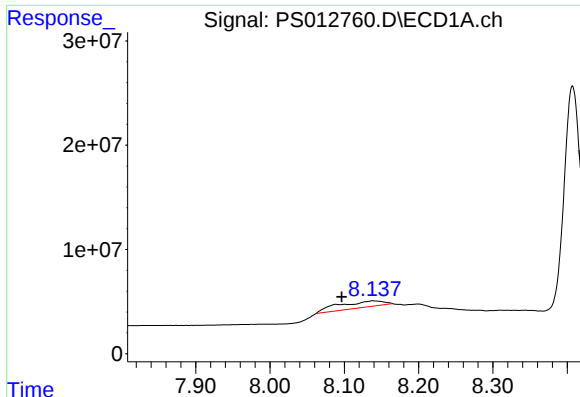

#8 DICHLORPROP


R.T.: 8.140 min
Delta R.T.: 0.043 min
Response: 27861802
Conc: 28.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

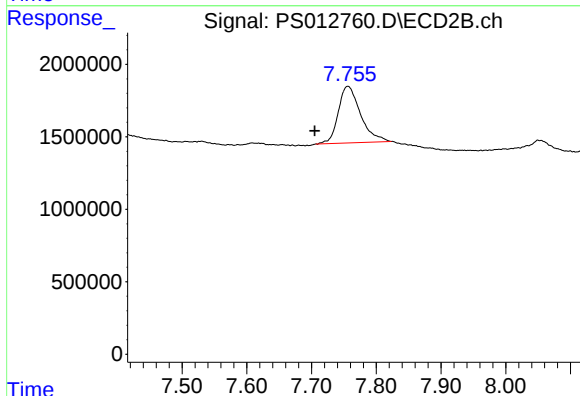


#8 DICHLORPROP

R.T.: 7.756 min
Delta R.T.: 0.051 min
Response: 9305247
Conc: 18.02 ng/ml

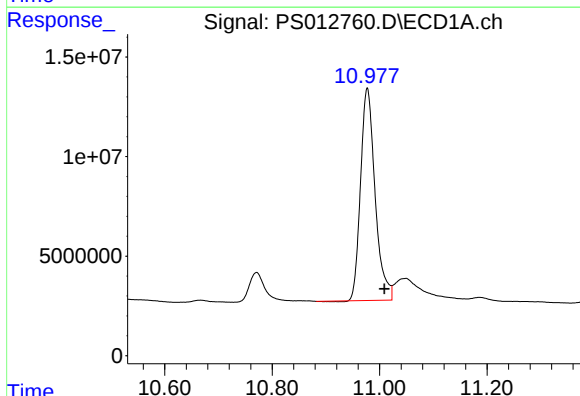


#15 Picloram

R.T.: 10.977 min
Delta R.T.: -0.032 min
Response: 199827836
Conc: 27.75 ng/ml

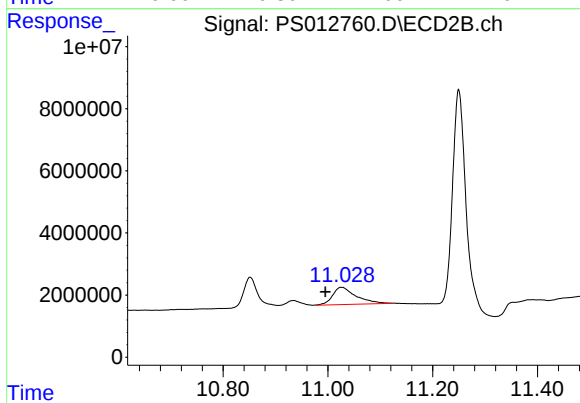

#15 Picloram


R.T.: 11.027 min
Delta R.T.: 0.032 min
Response: 17361269
Conc: 4.40 ng/ml

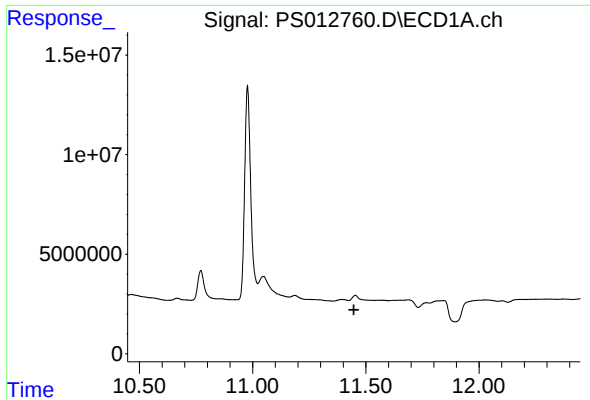

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.447 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

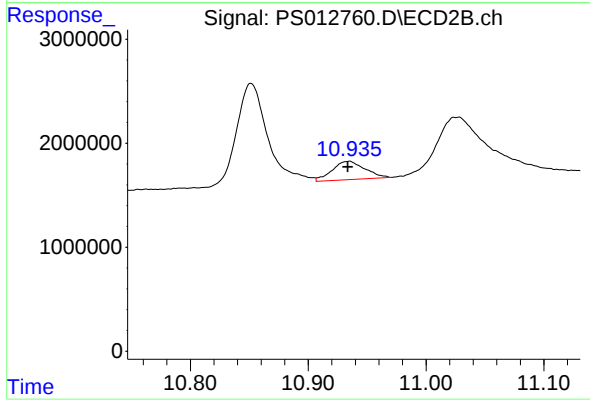

#16 DCPA

R.T.: 10.935 min
Delta R.T.: 0.001 min
Response: 3427887
Conc: 1.03 ng/ml