

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100821\
 Data File : PS017035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2021 14:45
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 00:37:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.746	683.9E6	297.2E6	448.912	506.797
Target Compounds							
2) T	3,5-DICHL...	6.421	0.000	5092617	0	2.393	N.D. #
5) T	DICAMBA	7.350	0.000	3340030	0	<MDL	N.D. #
7) T	MCPA	7.615f	0.000	12565415	0	2.032	N.D. #
9) T	2,4-D	8.338f	0.000	113.9E6	0	64.758	N.D. #
10) T	Pentachlo...	8.574	0.000	10662342	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.122	0.000	4365623	0	<MDL	N.D. #
12) T	2,4,5-T	9.416	0.000	4524249	0	<MDL	N.D. #
14) T	DINOSEB	11.105	0.000	10240783	0	1.681	N.D. #
15) T	Picloram	10.948	0.000	7316688	0	<MDL	N.D. #
16) T	DCPA	11.372	0.000	5816898	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100821\
Data File : PS017035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2021 14:45
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 00:37:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

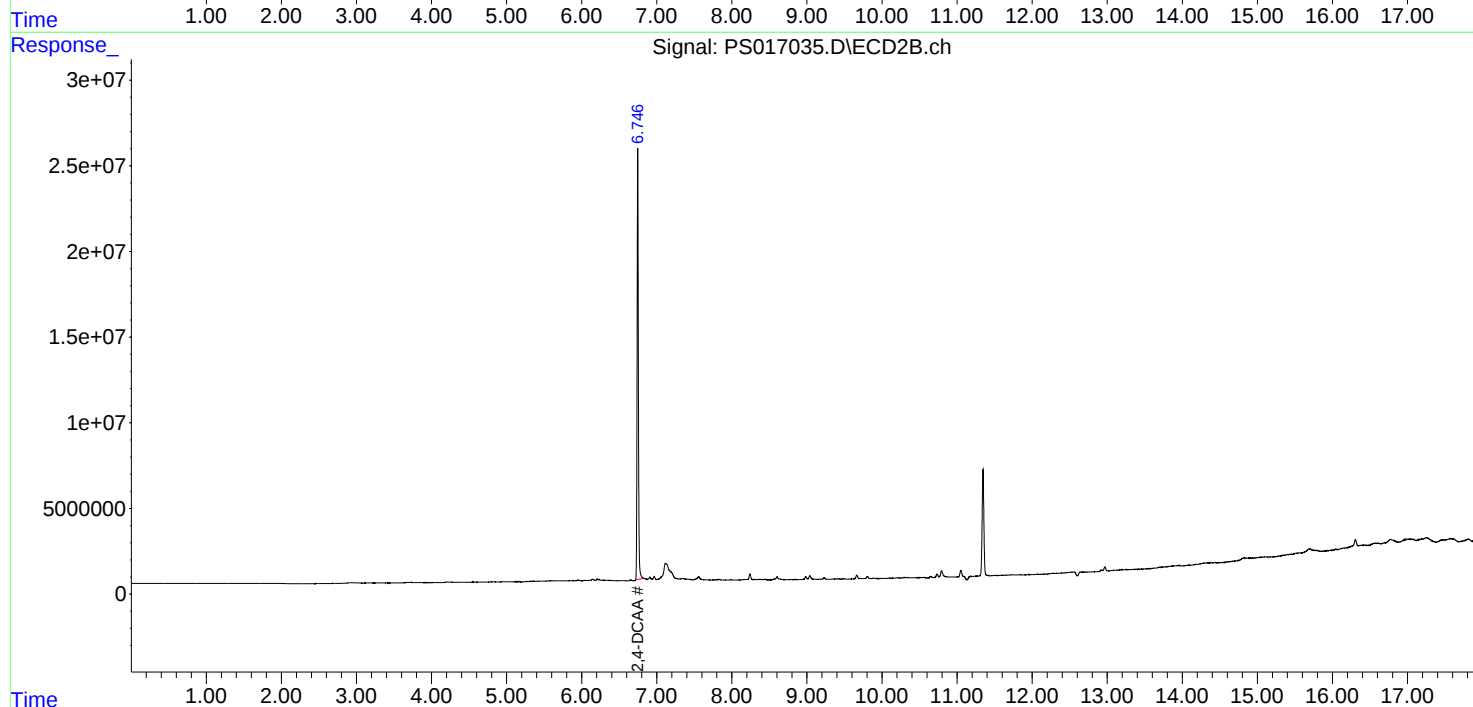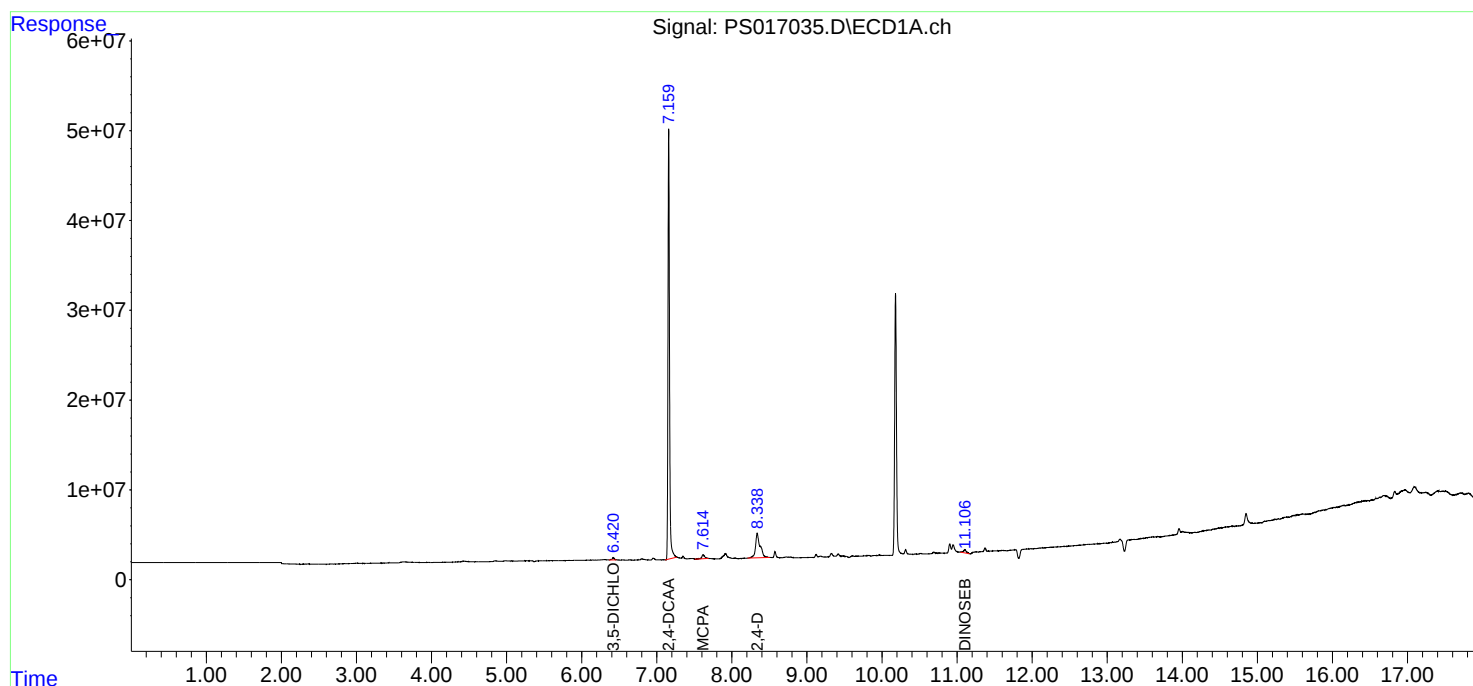


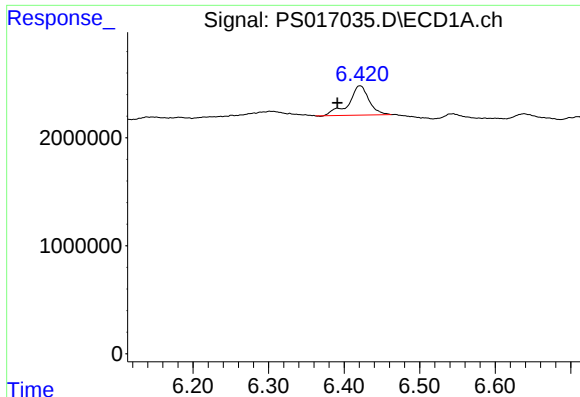

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.421 min
Delta R.T.: 0.030 min
Response: 5092617
Conc: 2.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

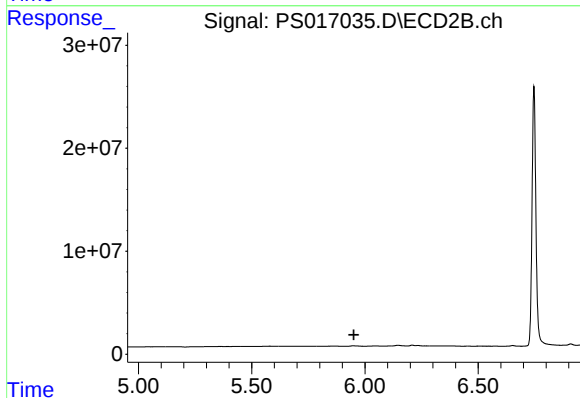


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.951 min
Response: 0
Conc: N.D.

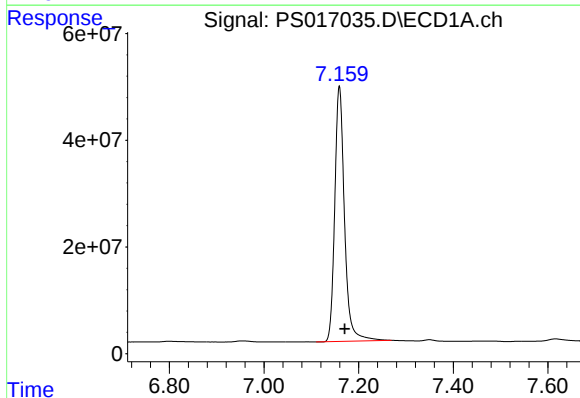


#4 2,4-DCAA

R.T.: 7.159 min
Delta R.T.: -0.011 min
Response: 683939907
Conc: 448.91 ng/ml

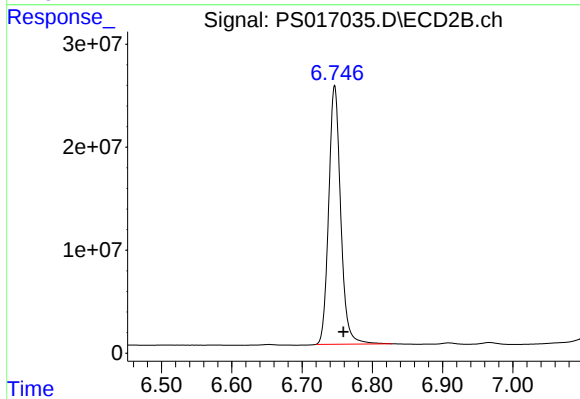

#4 2,4-DCAA


R.T.: 6.746 min
Delta R.T.: -0.013 min
Response: 297167297
Conc: 506.80 ng/ml

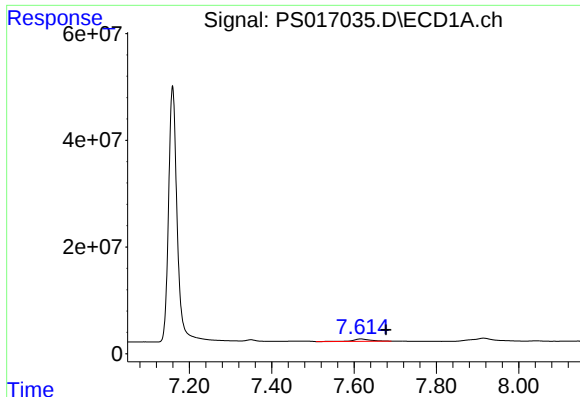

#7 MCPA


R.T.: 7.615 min
Delta R.T.: -0.062 min
Response: 12565415
Conc: 2.03 ug/ml

Instrument :
ECD_S
ClientSampleId :

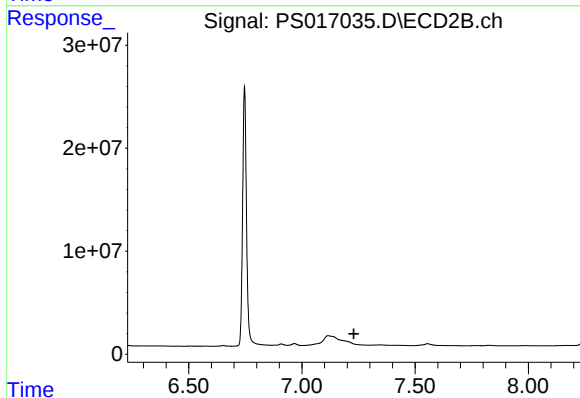


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.229 min
Response: 0
Conc: N.D.

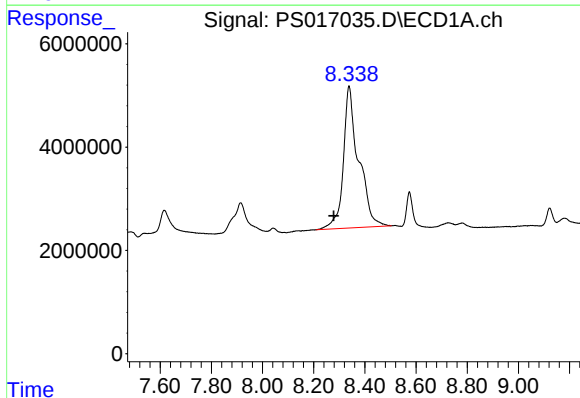


#9 2,4-D

R.T.: 8.338 min
Delta R.T.: 0.060 min
Response: 113861830
Conc: 64.76 ng/ml

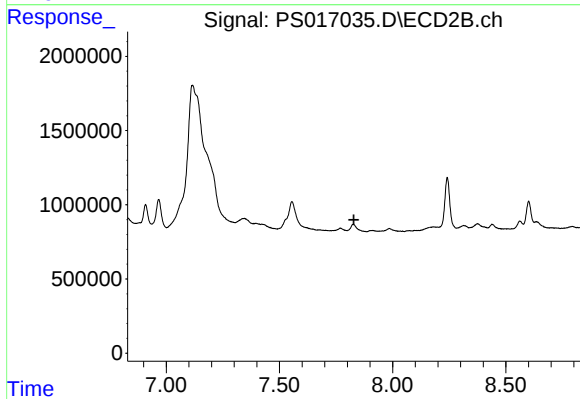

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.829 min
Response: 0
Conc: N.D.

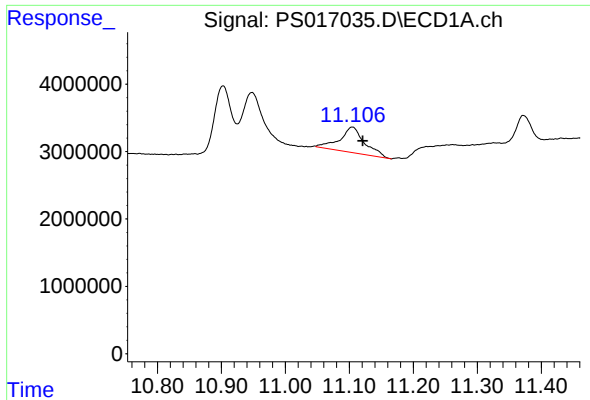

#14 DINOSEB

R.T.: 11.105 min
Delta R.T.: -0.017 min
Response: 10240783
Conc: 1.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

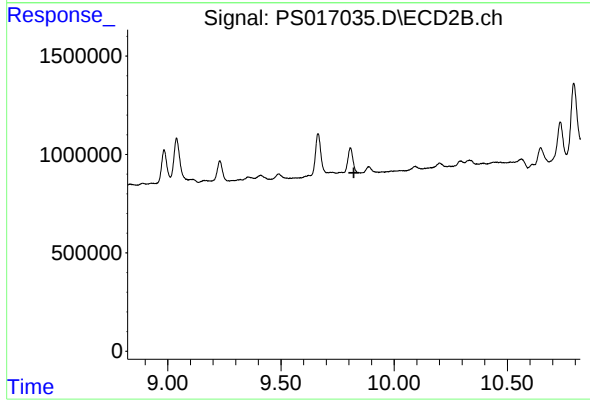

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.822 min
Response: 0
Conc: N.D.