

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100821\
 Data File : PS017046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Oct 2021 19:11
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 00:46:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.160	6.747	702.6E6	305.2E6	461.167	520.495
Target Compounds							
2) T	3,5-DICHL...	6.422	0.000	4211223	0	1.979	N.D. #
3) T	4-Nitroph...	6.954f	0.000	4924146	0	5.684	N.D. #
7) T	MCPA	7.618f	0.000	13848063	0	2.239	N.D. #
9) T	2,4-D	8.337f	0.000	123.3E6	0	70.117	N.D. #
12) T	2,4,5-T	9.474f	0.000	13281723	0	1.609	N.D. #
14) T	DINOSEB	11.068f	0.000	11660472	0	1.914	N.D. #
15) T	Picloram	10.903	0.000	13968445	0	1.174	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100821\
Data File : PS017046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Oct 2021 19:11
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 00:46:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

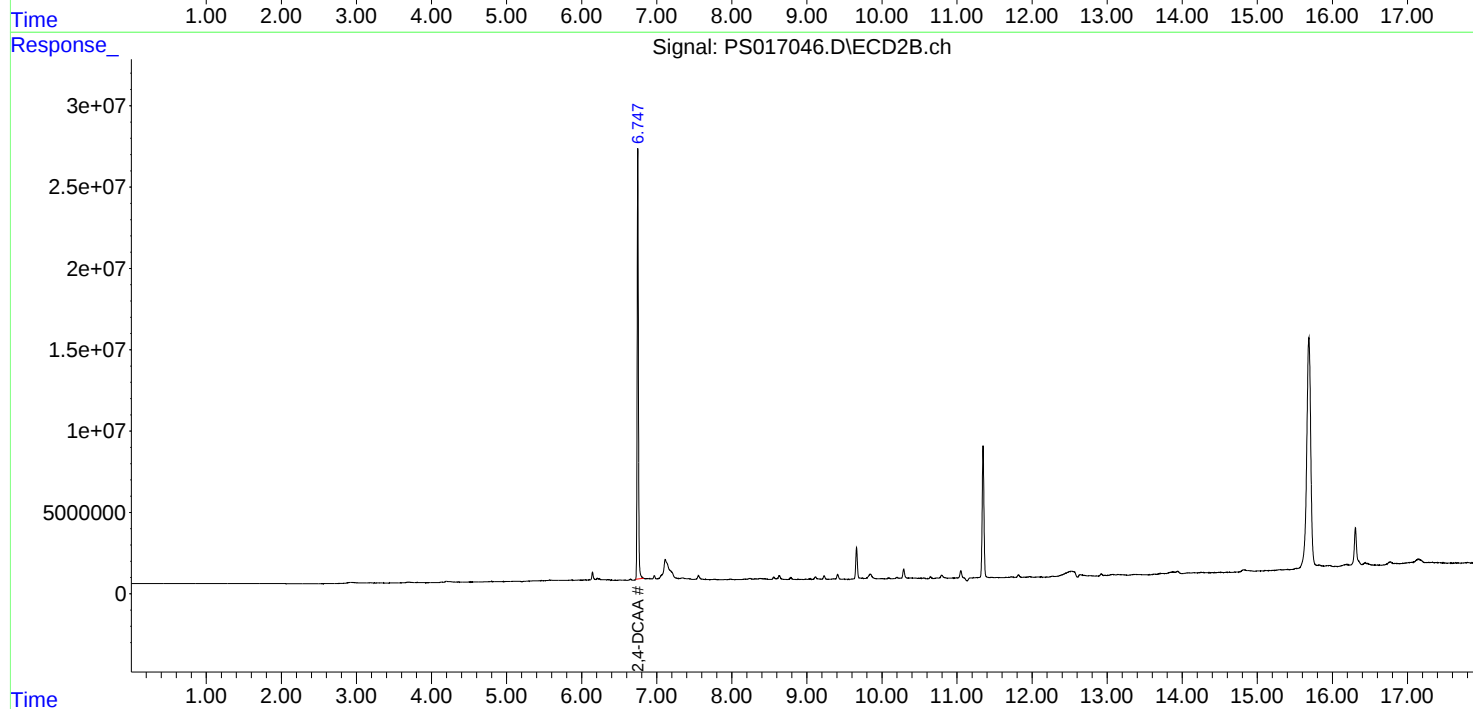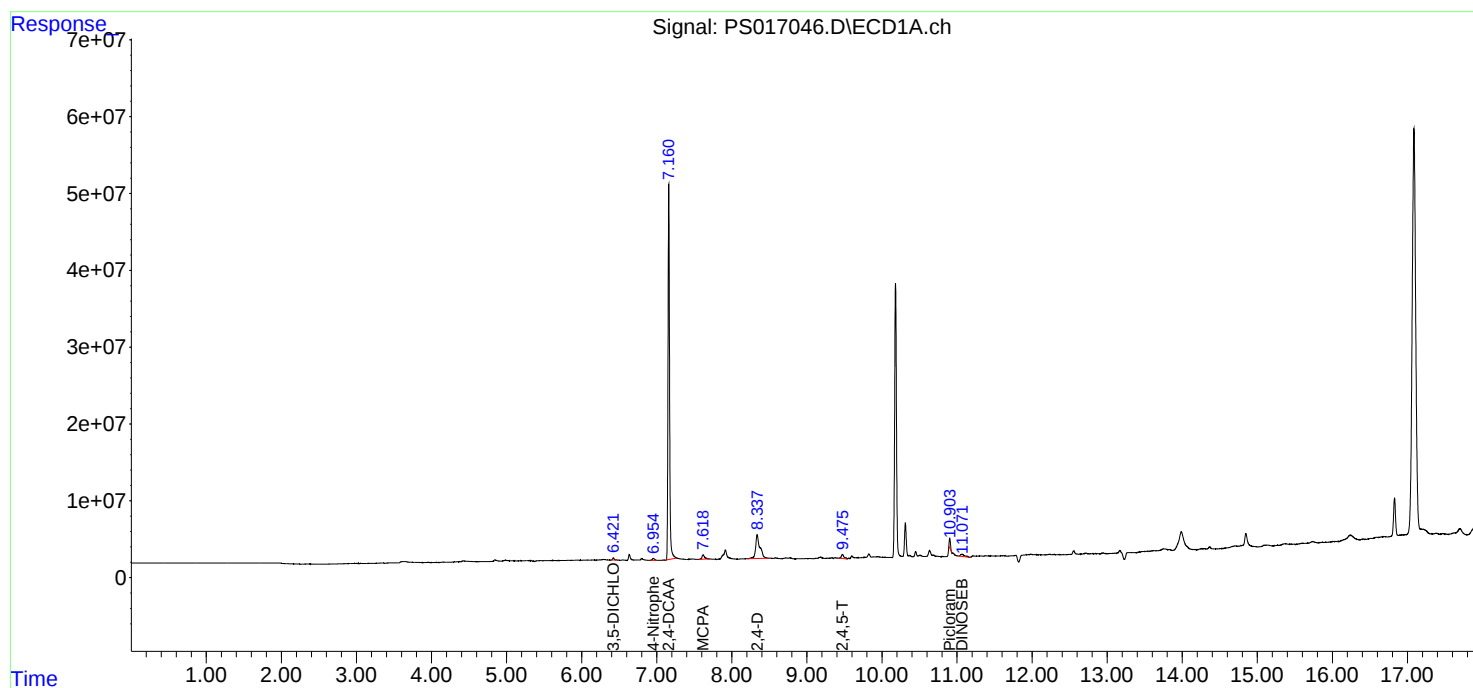


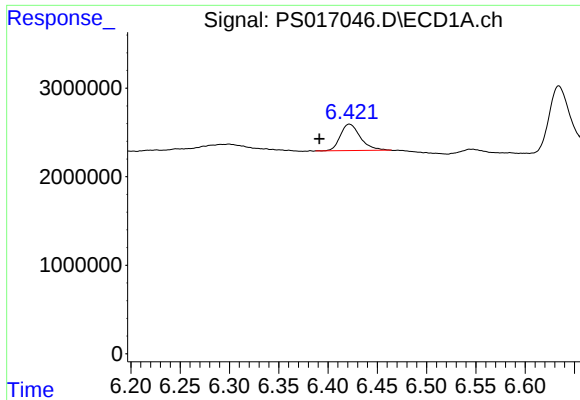

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.422 min
Delta R.T.: 0.031 min
Response: 4211223
Conc: 1.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

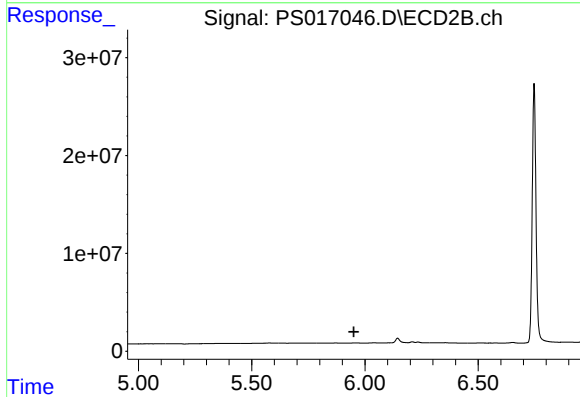


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.951 min
Response: 0
Conc: N.D.

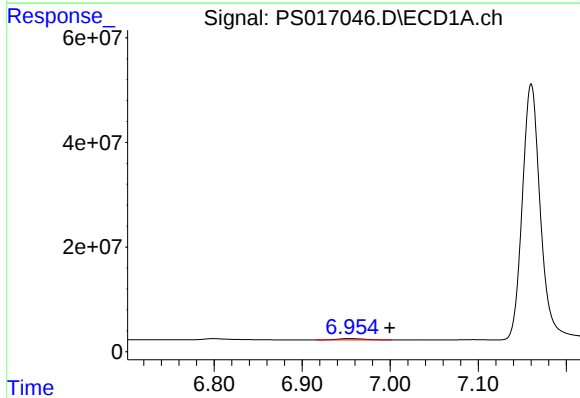


#3 4-Nitrophenol

R.T.: 6.954 min
Delta R.T.: -0.045 min
Response: 4924146
Conc: 5.68 ng/ml

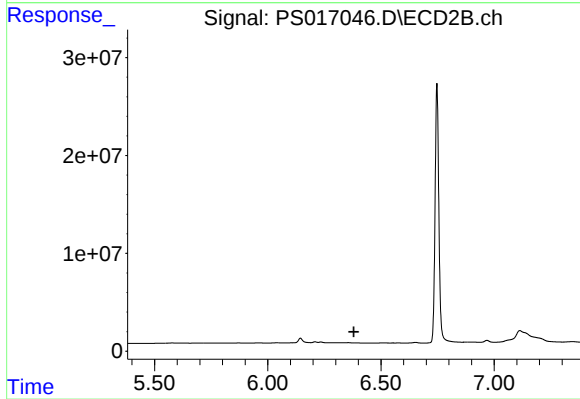

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.381 min
Response: 0
Conc: N.D.

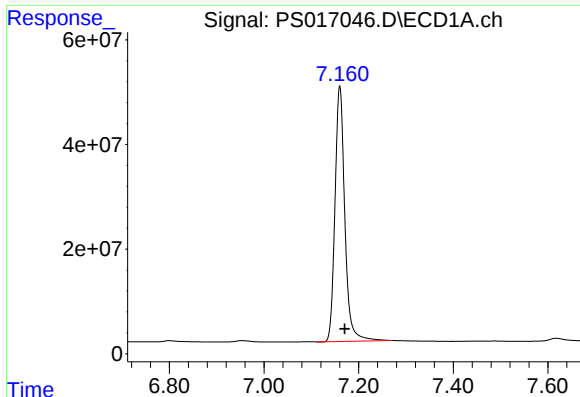

#4 2,4-DCAA


R.T.: 7.160 min
Delta R.T.: -0.010 min
Response: 702610383
Conc: 461.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

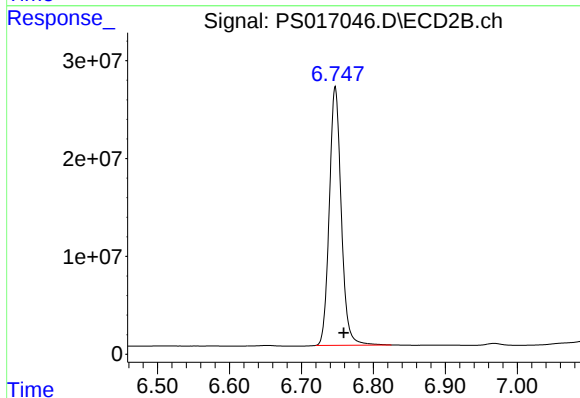


#4 2,4-DCAA

R.T.: 6.747 min
Delta R.T.: -0.012 min
Response: 305199287
Conc: 520.50 ng/ml

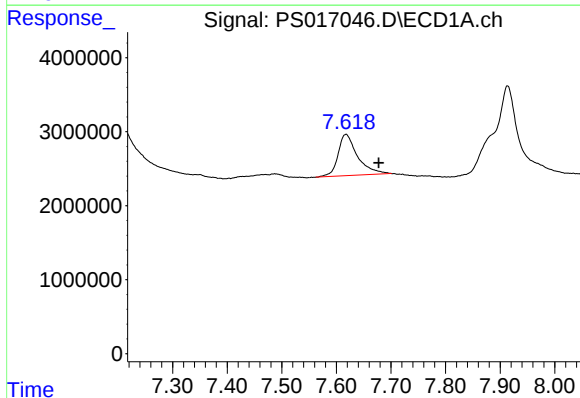


#7 MCPA

R.T.: 7.618 min
Delta R.T.: -0.060 min
Response: 13848063
Conc: 2.24 ug/ml

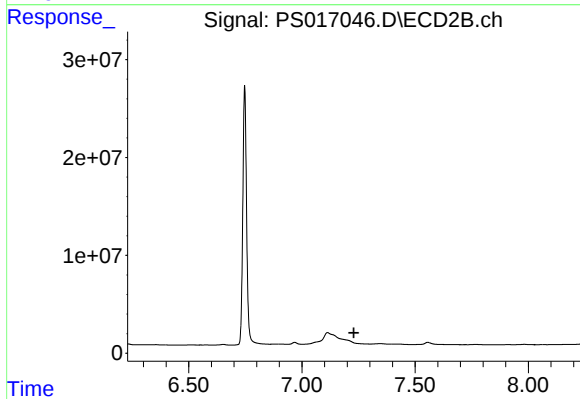

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.229 min
Response: 0
Conc: N.D.

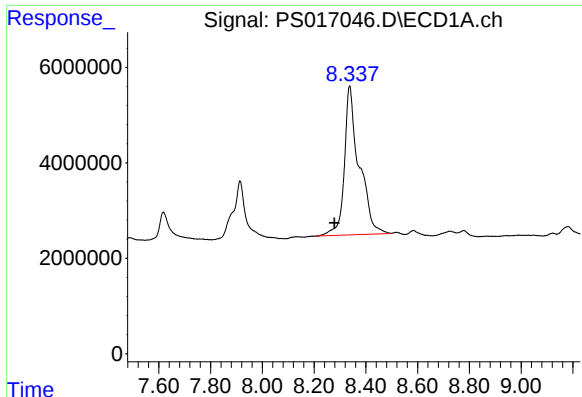

#9 2,4-D


R.T.: 8.337 min
Delta R.T.: 0.059 min
Response: 123283982
Conc: 70.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

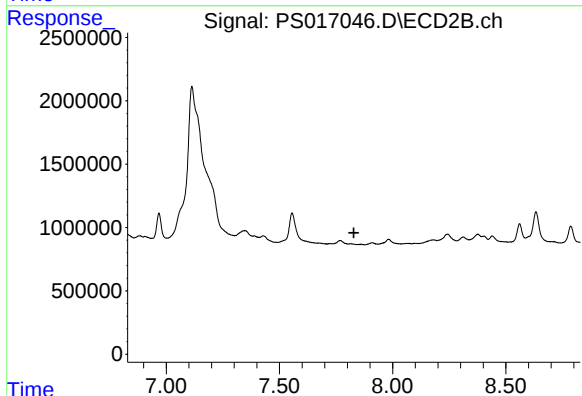


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.829 min
Response: 0
Conc: N.D.

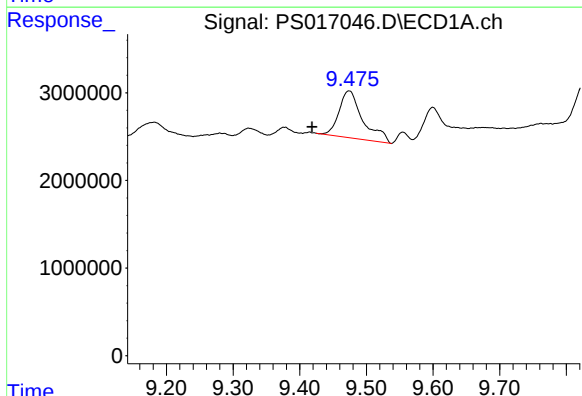


#12 2,4,5-T

R.T.: 9.474 min
Delta R.T.: 0.056 min
Response: 13281723
Conc: 1.61 ng/ml

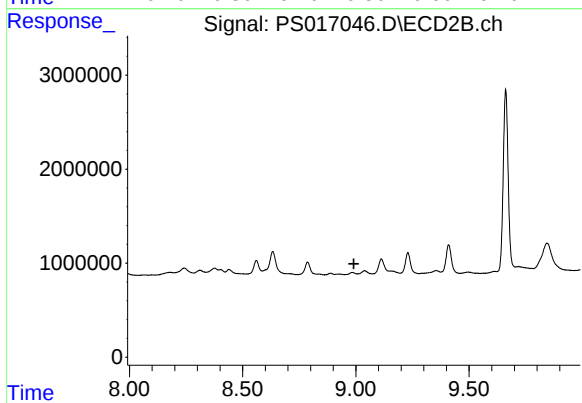

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.

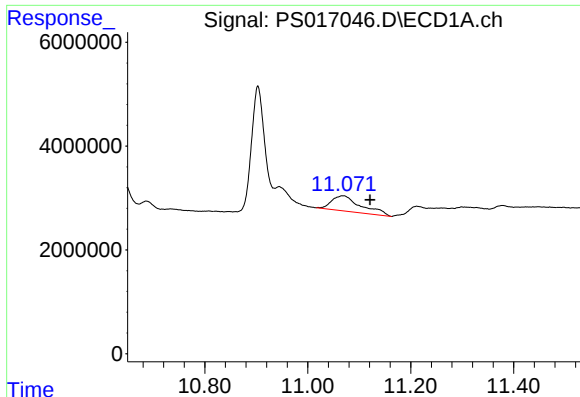

#14 DINOSEB


R.T.: 11.068 min
Delta R.T.: -0.053 min
Response: 11660472
Conc: 1.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

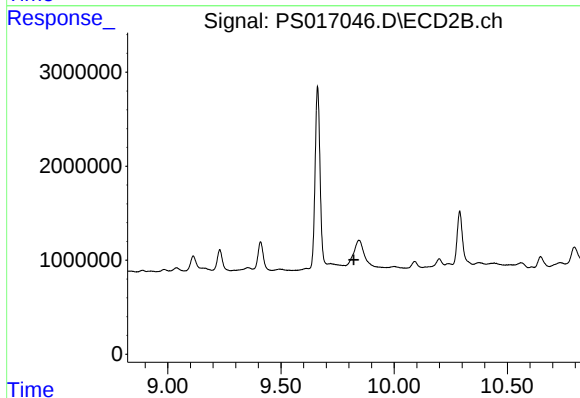


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.822 min
Response: 0
Conc: N.D.

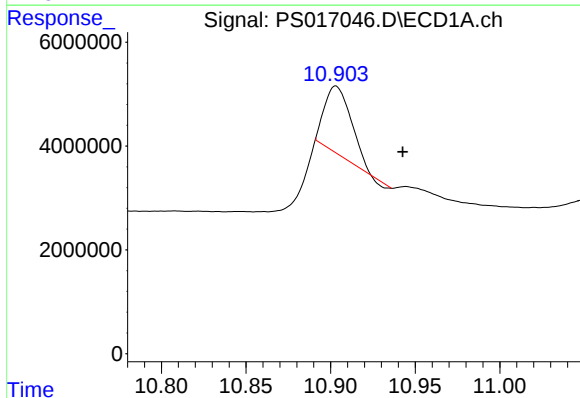

#15 Picloram

R.T.: 10.903 min
Delta R.T.: -0.040 min
Response: 13968445
Conc: 1.17 ng/ml

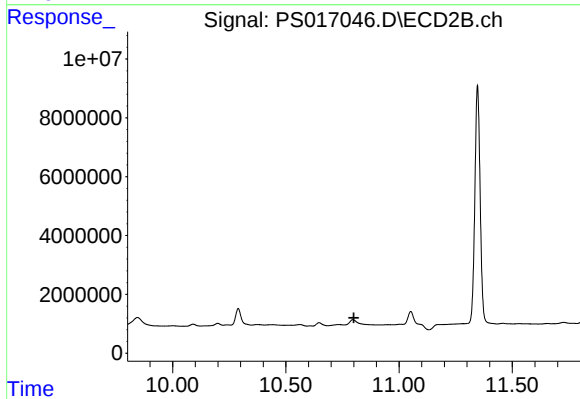

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.801 min
Response: 0
Conc: N.D.