

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100920\
 Data File : PS012773.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2020 12:28
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 13:32:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.473	0.000	370.7E6	0	274.918	N.D. #
3) T	4-Nitroph...	7.008	0.000	7699258	0	15.833	N.D. #
7) T	MCPA	7.675	0.000	29006814	0	6.955	N.D. #
8) T	DICHLORPROP	0.000	7.740	0	11283301	N.D.	21.853
12) T	2,4,5-T	0.000	9.237	0	8047744	N.D.	3.130
15) T	Picloram	11.023	11.005	43140195	23619839	5.992	5.993
16) T	DCPA	11.451	10.932	8634846	7588637	1.223	2.282 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100920\
Data File : PS012773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2020 12:28
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 13:32:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

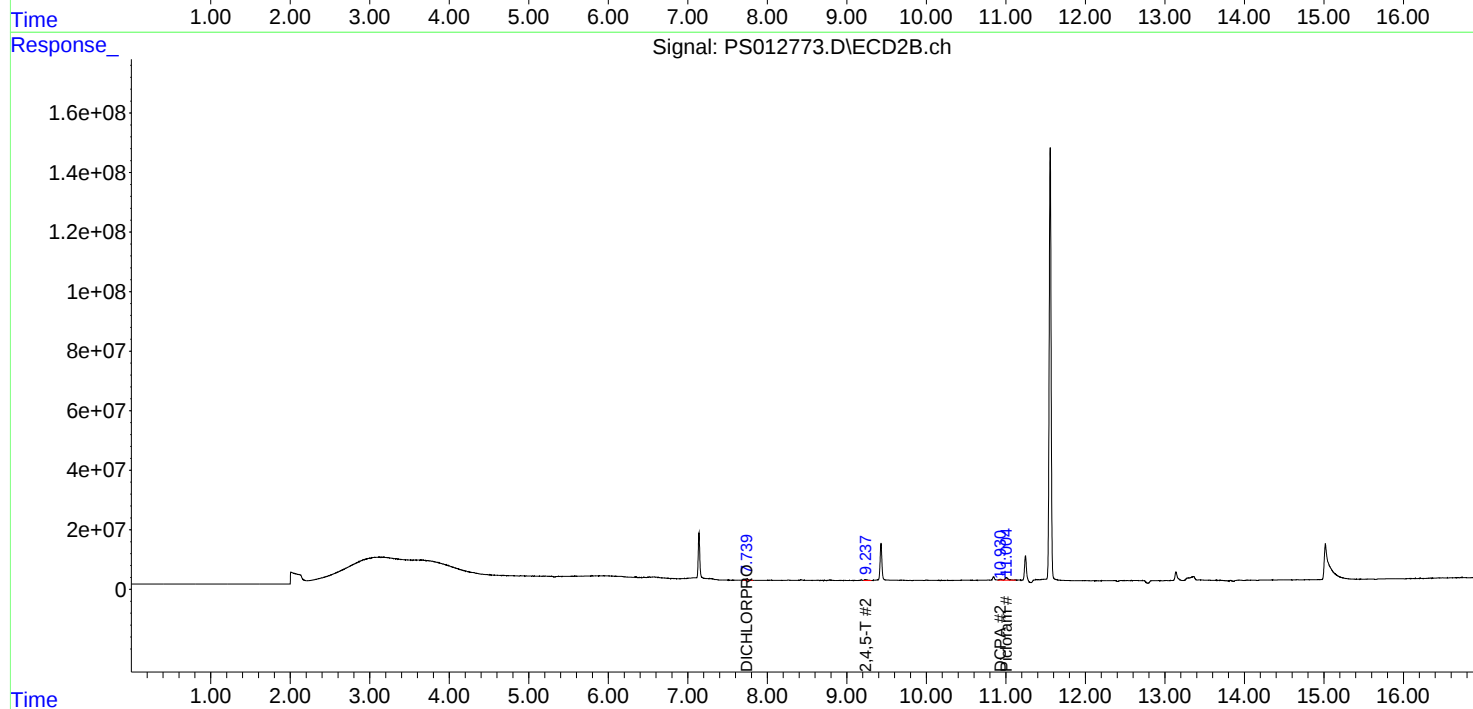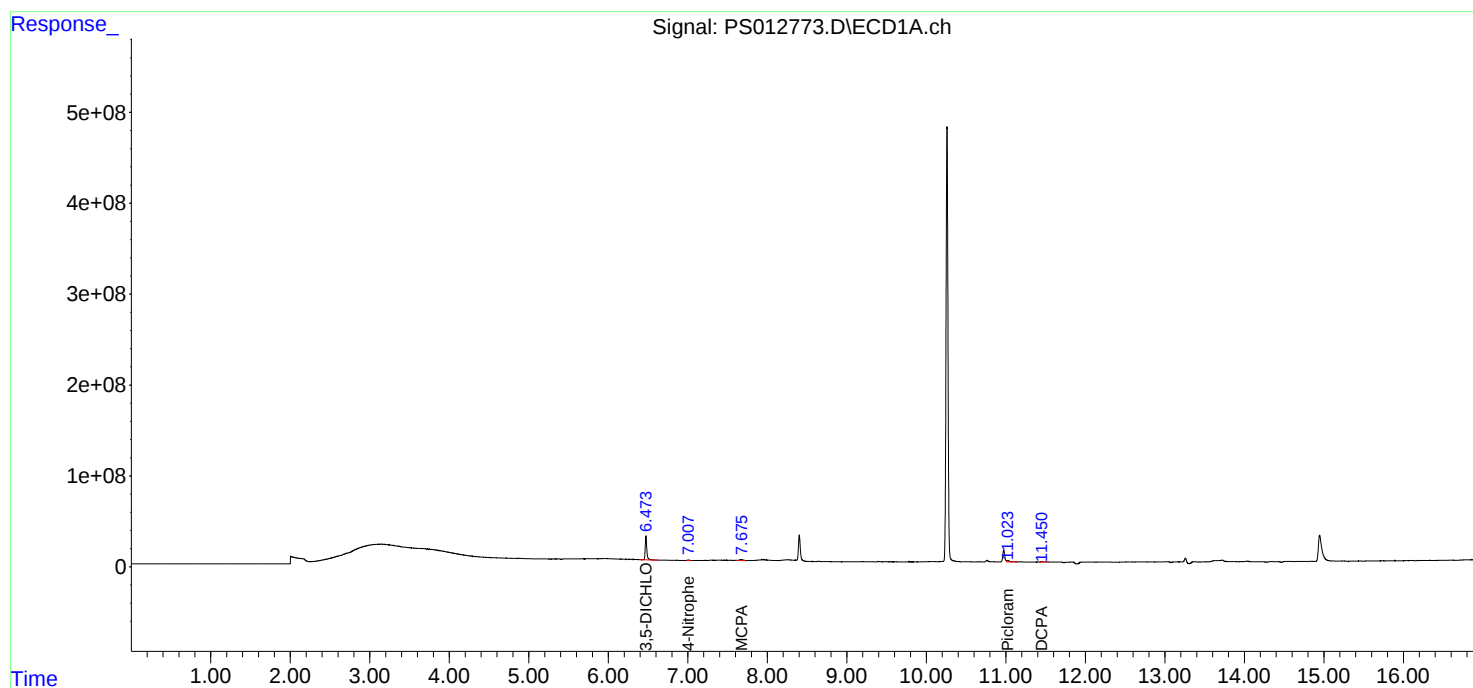


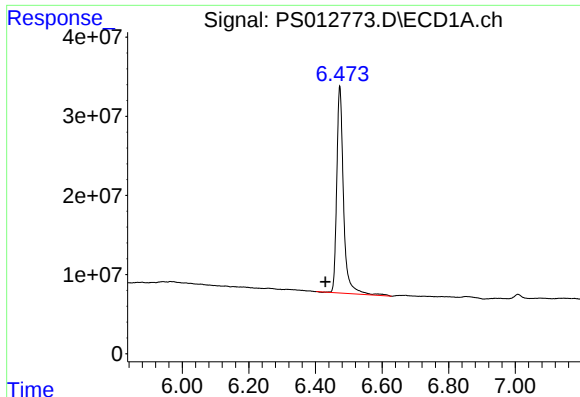

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.473 min
Delta R.T.: 0.043 min
Response: 370711802
Conc: 274.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

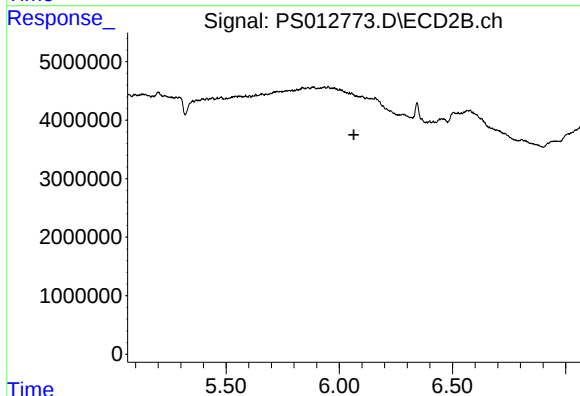


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.064 min
Response: 0
Conc: N.D.

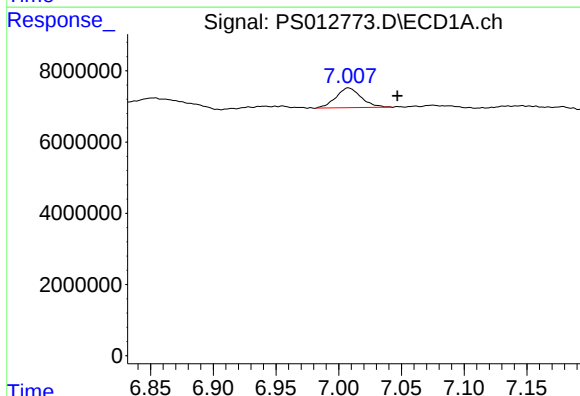


#3 4-Nitrophenol

R.T.: 7.008 min
Delta R.T.: -0.039 min
Response: 7699258
Conc: 15.83 ng/ml

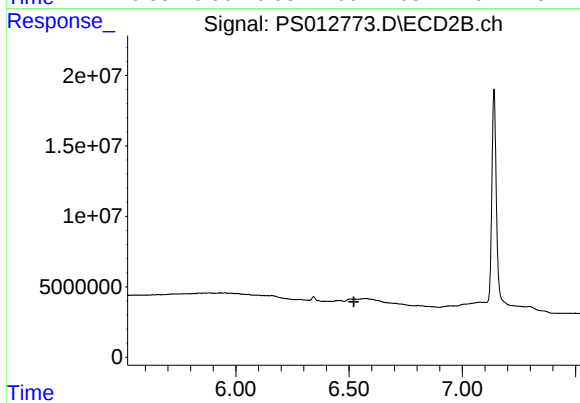

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

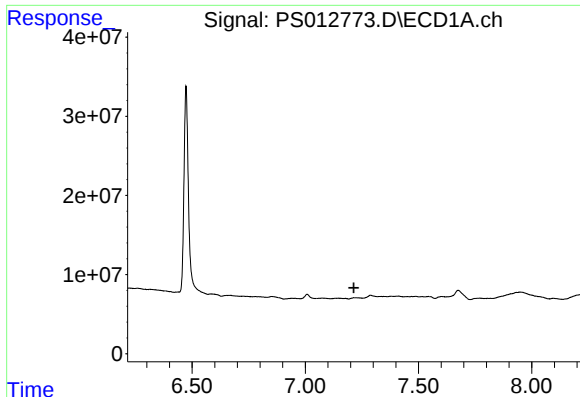

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.215 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

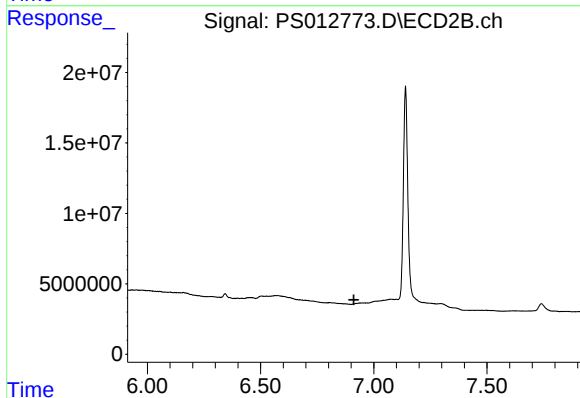


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.912 min
Response: 0
Conc: N.D.

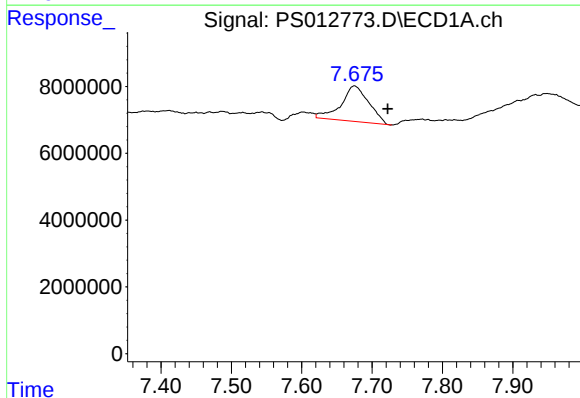


#7 MCPA

R.T.: 7.675 min
Delta R.T.: -0.047 min
Response: 29006814
Conc: 6.95 ug/ml

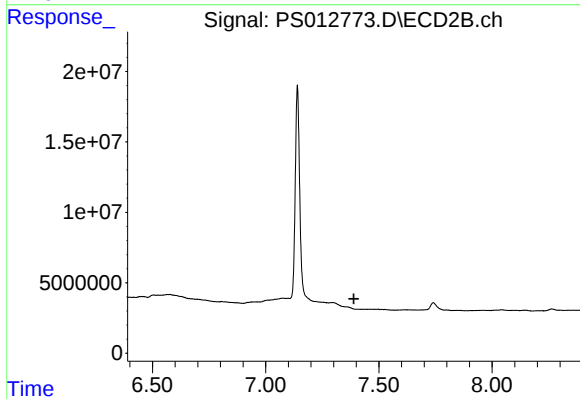

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.390 min
Response: 0
Conc: N.D.

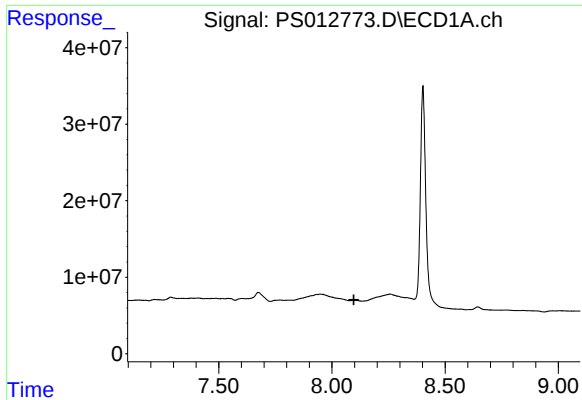

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.097 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

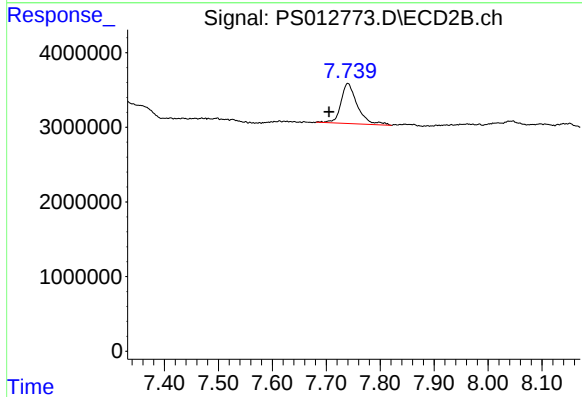


#8 DICHLORPROP

R.T.: 7.740 min
Delta R.T.: 0.035 min
Response: 11283301
Conc: 21.85 ng/ml

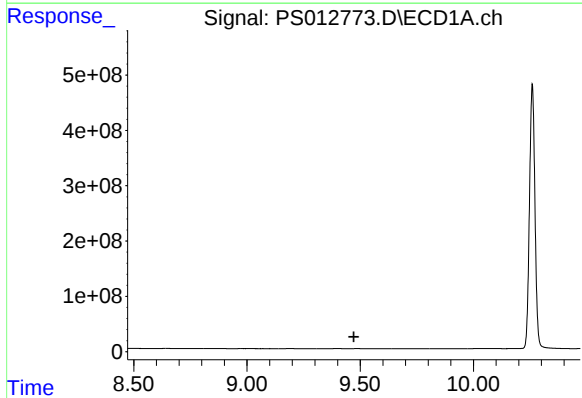


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.472 min
Response: 0
Conc: N.D.

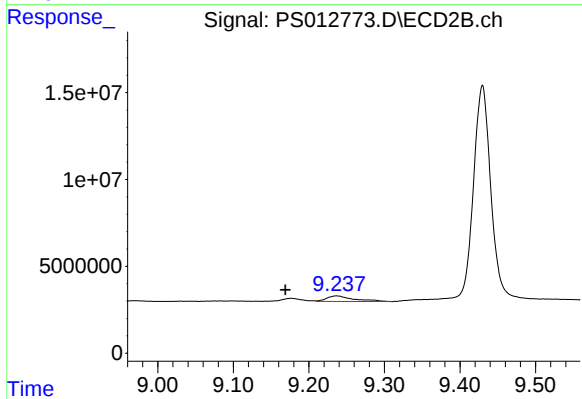

#12 2,4,5-T


R.T.: 9.237 min
Delta R.T.: 0.068 min
Response: 8047744
Conc: 3.13 ng/ml

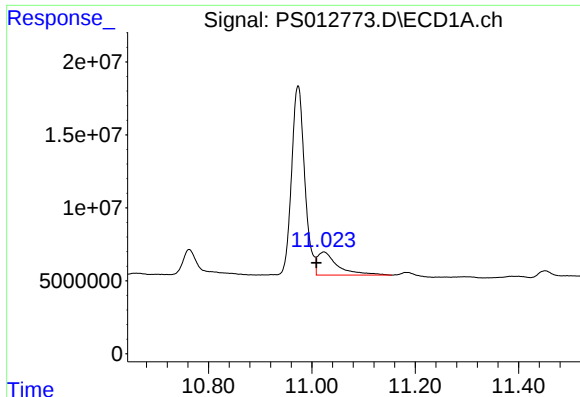

#15 Picloram


R.T.: 11.023 min
Delta R.T.: 0.014 min
Response: 43140195
Conc: 5.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

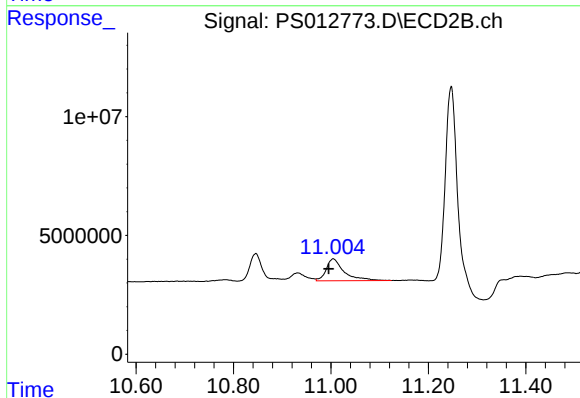


#15 Picloram

R.T.: 11.005 min
Delta R.T.: 0.010 min
Response: 23619839
Conc: 5.99 ng/ml

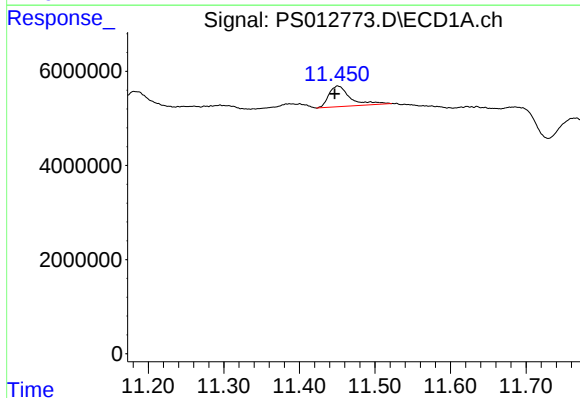

#16 DCPA

R.T.: 11.451 min
Delta R.T.: 0.004 min
Response: 8634846
Conc: 1.22 ng/ml

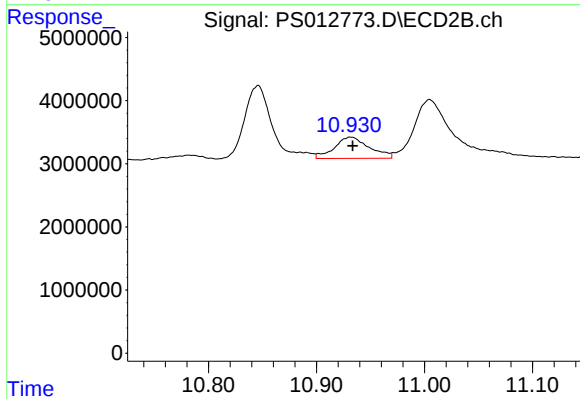

#16 DCPA

R.T.: 10.932 min
Delta R.T.: -0.002 min
Response: 7588637
Conc: 2.28 ng/ml