

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100920\
 Data File : PS012815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2020 07:40
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 08:57:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.912	435.6E6	231.6E6	444.742	503.443
Target Compounds							
7) T	MCPA	0.000	7.343	0	11238402	N.D.	4.688
9) T	2,4-D	8.395	0.000	88365627	0	77.826	N.D. #
15) T	Picloram	11.071	0.000	20300417	0	2.819	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100920\
Data File : PS012815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2020 07:40
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 08:57:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

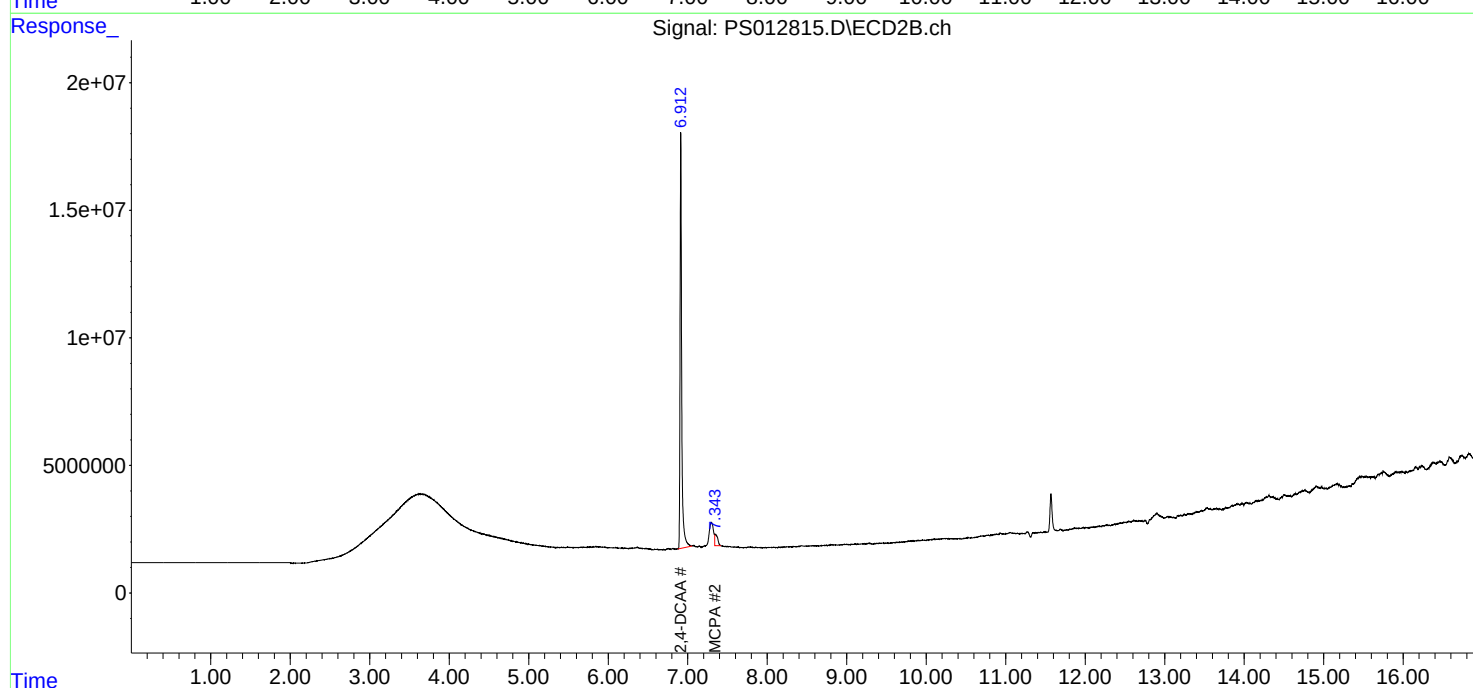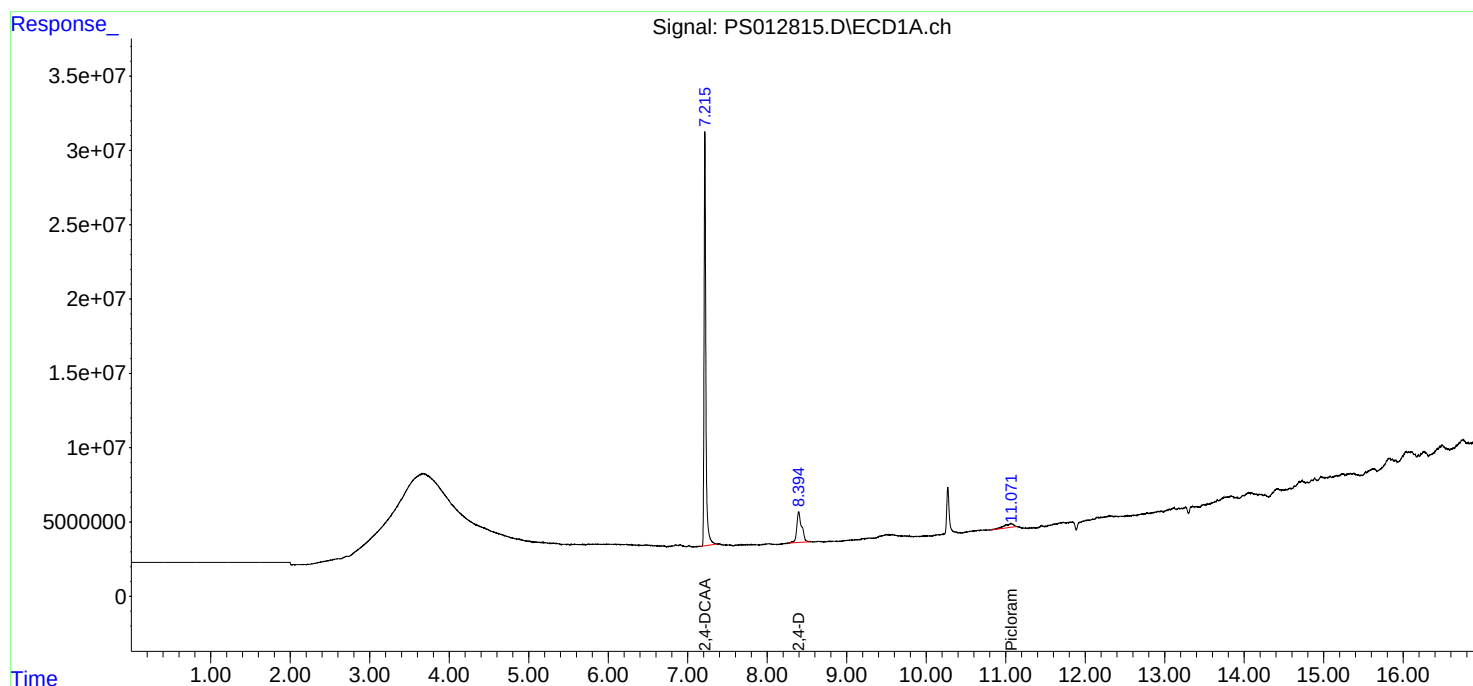


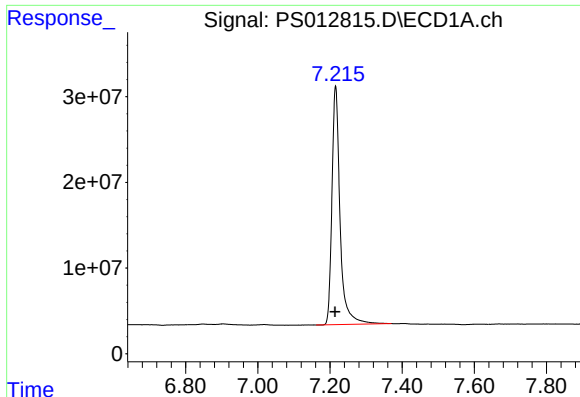

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: 0.001 min
Response: 435601792
Conc: 444.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

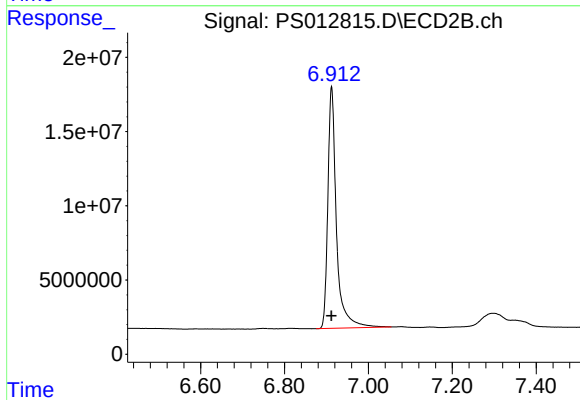


#4 2,4-DCAA

R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 231591951
Conc: 503.44 ng/ml

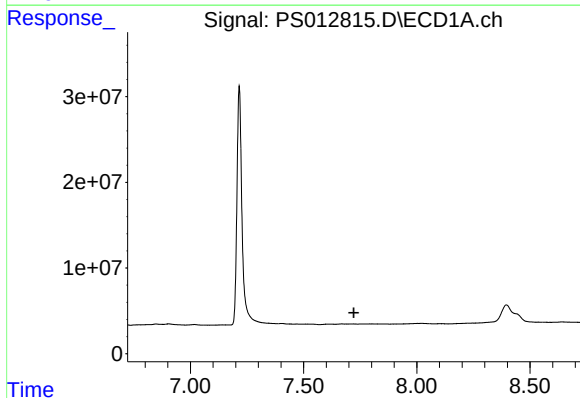


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.722 min
Response: 0
Conc: N.D.

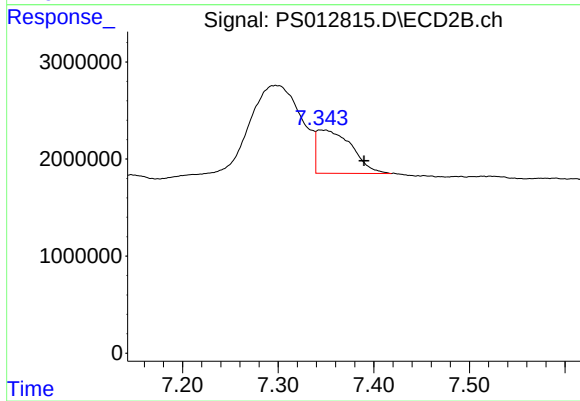

#7 MCPA


R.T.: 7.343 min
Delta R.T.: -0.046 min
Response: 11238402
Conc: 4.69 ug/ml

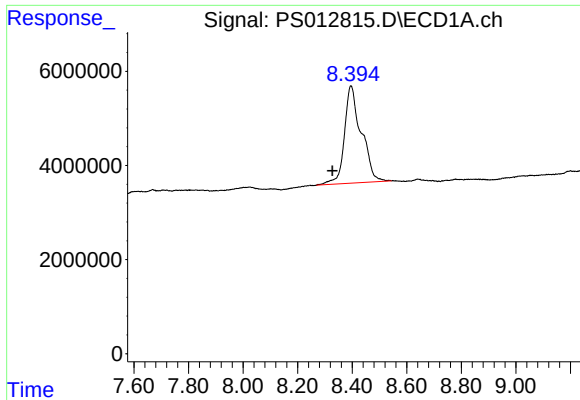

#9 2,4-D


R.T.: 8.395 min
Delta R.T.: 0.067 min
Response: 88365627
Conc: 77.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

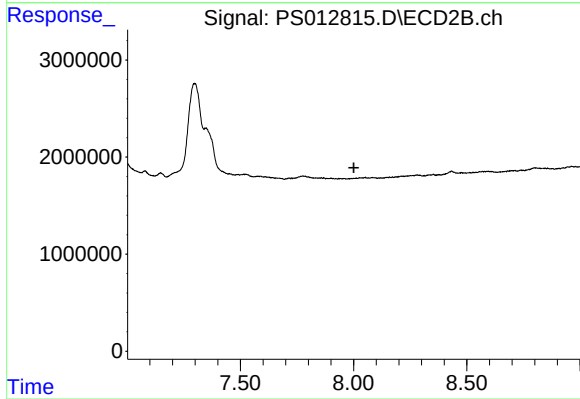


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.001 min
Response: 0
Conc: N.D.

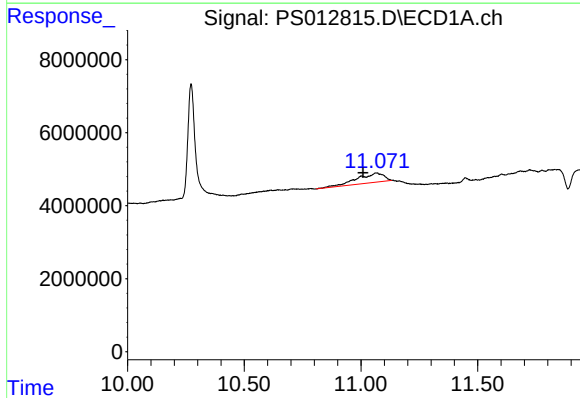

#15 Picloram

R.T.: 11.071 min
Delta R.T.: 0.062 min
Response: 20300417
Conc: 2.82 ng/ml

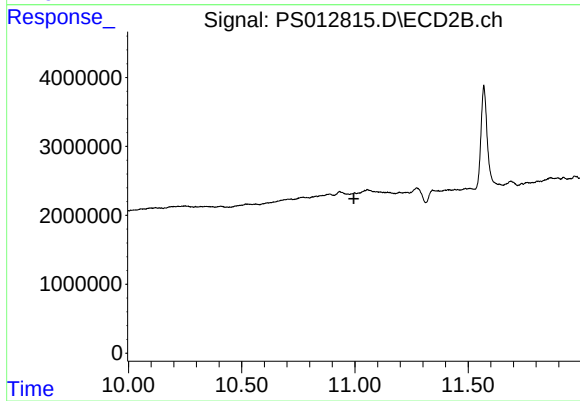

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.