

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100925\
 Data File : PS031970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2025 11:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 02:47:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.283	7.746	1724.0E6	448.6E6	478.696	493.556
Target Compounds							
1) T	Dalapon	0.000	2.654f	0	71315033	N.D.	25.310
2) T	3,5-DICHL...	6.449	0.000	997784	0	<MDL	N.D. #
3) T	4-Nitroph...	7.074	0.000	1564848	0	1.418	N.D. #
7) T	MCPA	7.752f	8.240f	2800156	17869080	<MDL	6.379 #
10) T	Pentachlo...	8.706	9.512	9831895	4725708	<MDL	<MDL #
11) T	2,4,5-TP ...	9.300	9.921f	5180239	2280281	<MDL	<MDL #
12) T	2,4,5-T	9.600	0.000	2946080	0	<MDL	N.D. #
13) T	2,4-DB	10.151	0.000	894918	0	<MDL	N.D. #
14) T	DINOSEB	11.359	0.000	1385834	0	<MDL	N.D. #
15) T	Picloram	11.201	0.000	682143	0	<MDL	N.D. #
16) T	DCPA	11.647	12.312	7010457	570737	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100925\
Data File : PS031970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2025 11:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 02:47:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

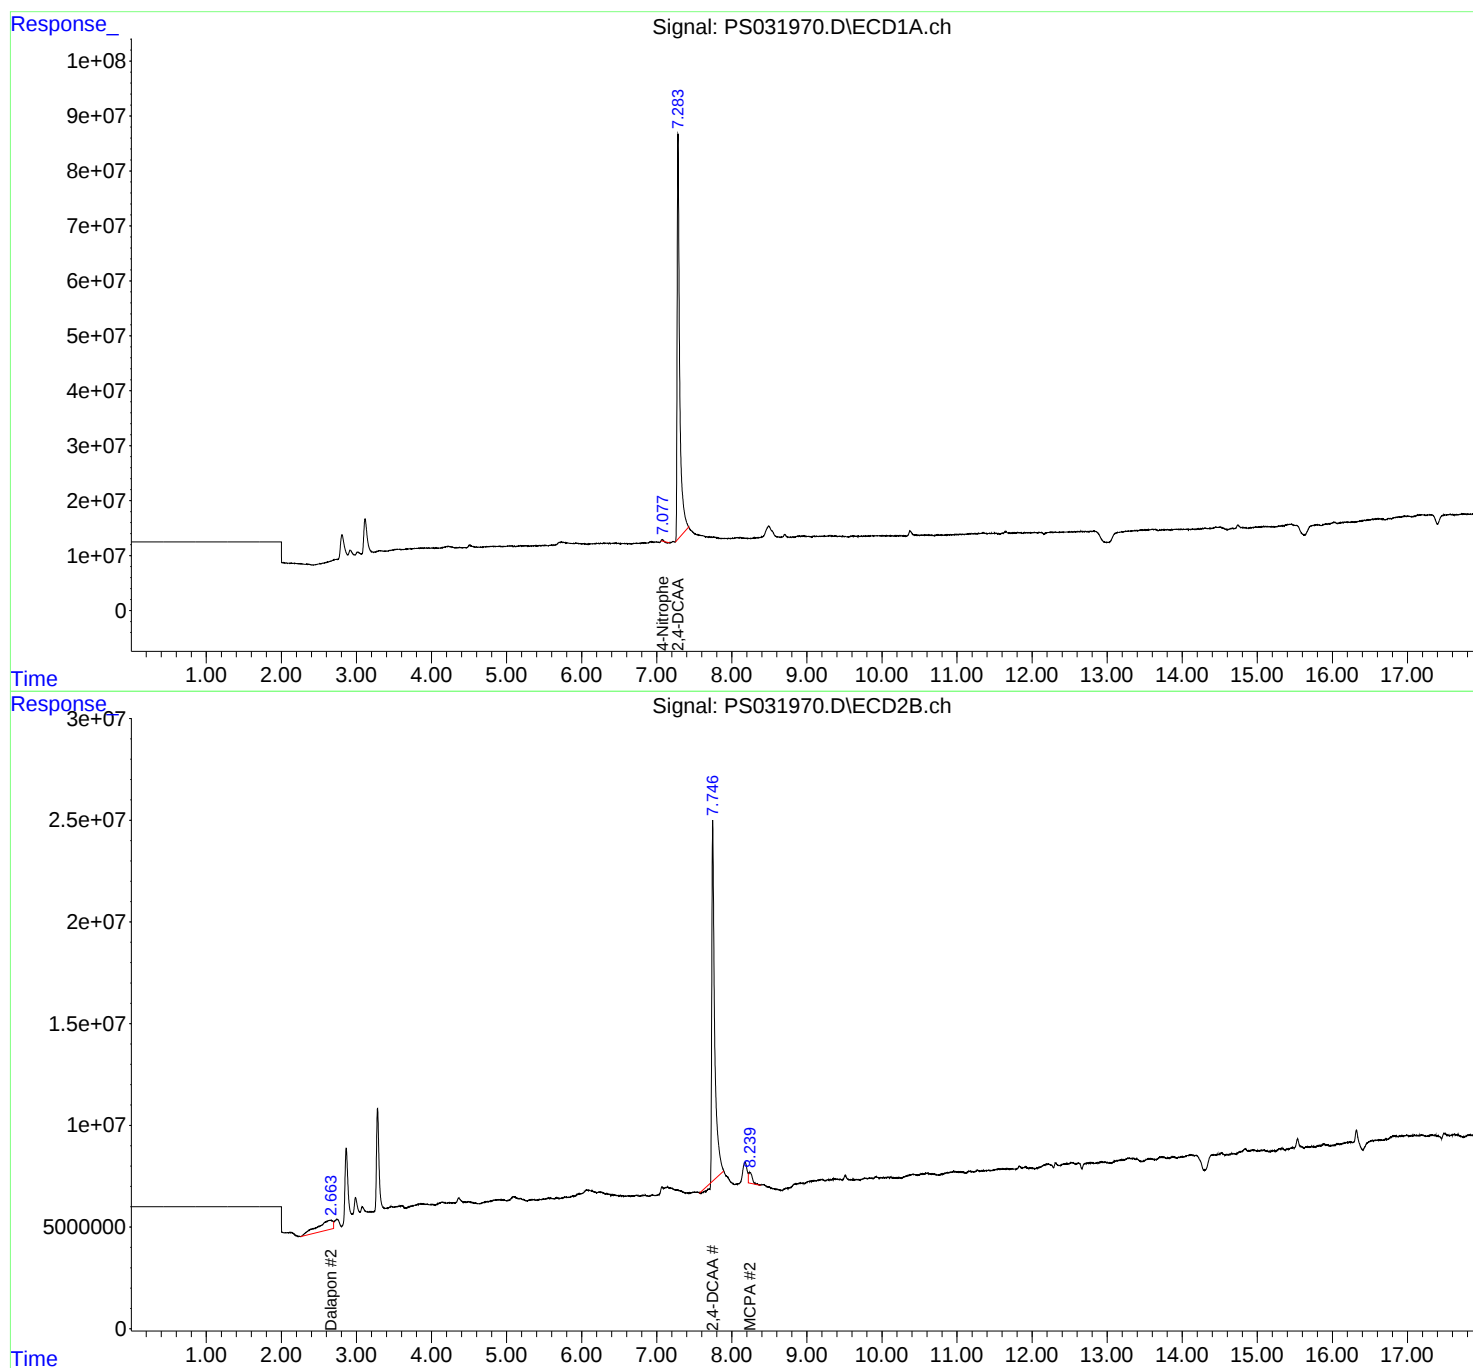


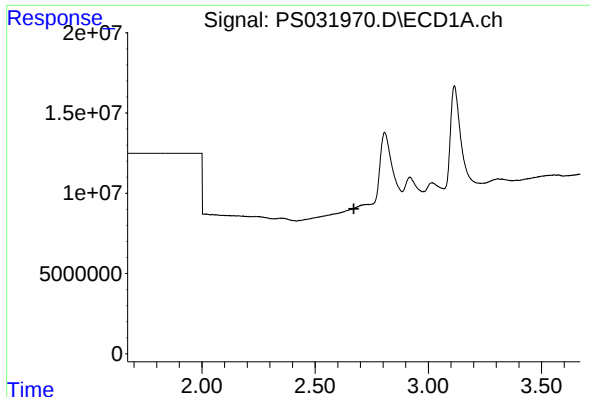

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

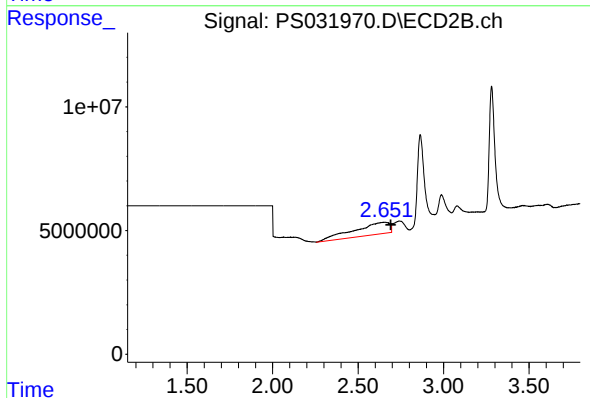


#1 Dalapon

R.T.: 2.654 min
Delta R.T.: -0.038 min
Response: 71315033
Conc: 25.31 ng/ml

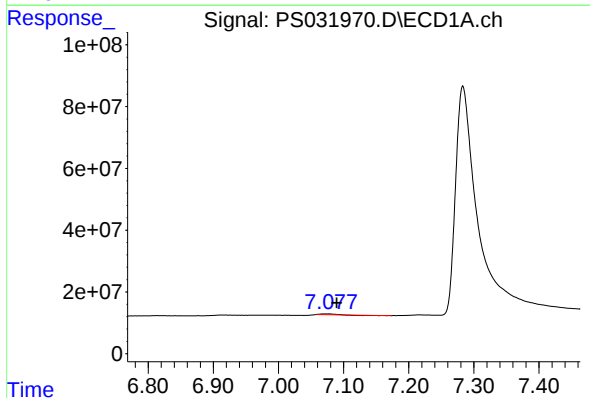


#3 4-Nitrophenol

R.T.: 7.074 min
Delta R.T.: -0.015 min
Response: 1564848
Conc: 1.42 ng/ml

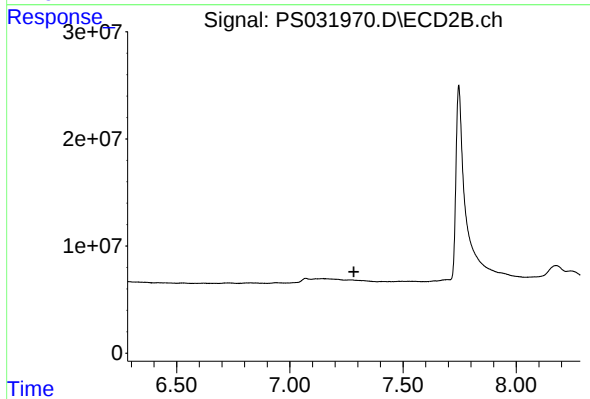

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.283 min
Response: 0
Conc: N.D.

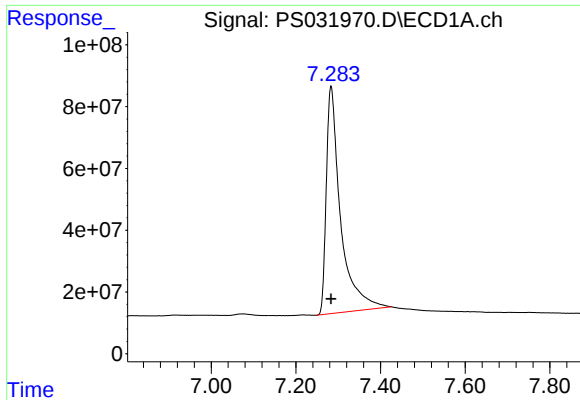

#4 2,4-DCAA


R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 1724035109
Conc: 478.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

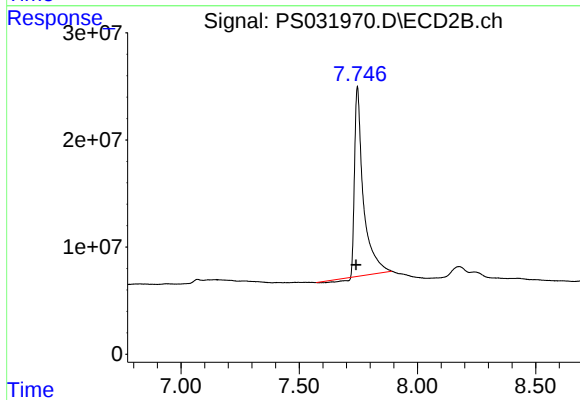


#4 2,4-DCAA

R.T.: 7.746 min
Delta R.T.: 0.006 min
Response: 448592784
Conc: 493.56 ng/ml

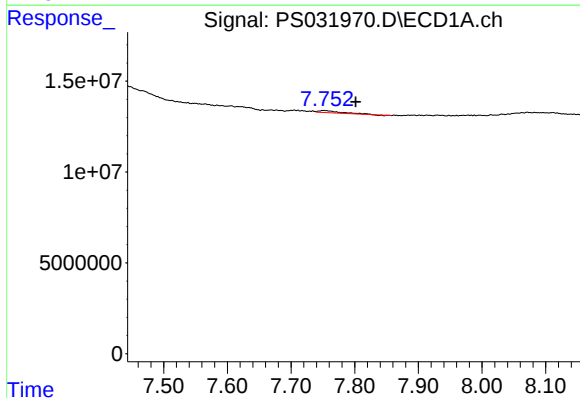

#7 MCPA

R.T.: 7.752 min
Delta R.T.: -0.050 min
Response: 2800156
Conc: N.D.

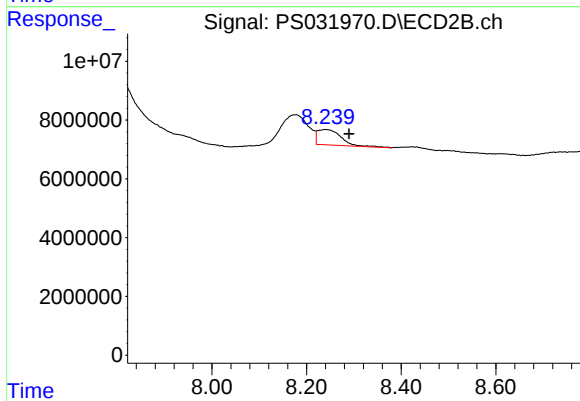

#7 MCPA

R.T.: 8.240 min
Delta R.T.: -0.050 min
Response: 17869080
Conc: 6.38 ug/ml