

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100925\
 Data File : PS031975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2025 18:25
 Operator : AR\AJ
 Sample : PB170010TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB170010TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 02:50:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.280	7.741	1501.3E6	437.7E6	416.864	481.592
Target Compounds							
1) T	Dalapon	0.000	2.663f	0	1317.4E6	N.D.	467.556
2) T	3,5-DICHL...	6.455	0.000	5675716	0	1.064	N.D. #
8) T	DICHLORPROP	8.184	8.666	7741797	5977060	2.174	4.108 #
10) T	Pentachlo...	8.701	9.504	10856087	59575886	<MDL	1.501 #
11) T	2,4,5-TP ...	9.328f	9.881	192.2E6	242.4E6	9.162	16.101 #
12) T	2,4,5-T	9.598	10.346f	125.6E6	65127042	6.862	4.840 #
13) T	2,4-DB	10.184f	0.000	223.6E6	0	95.838	N.D. #
14) T	DINOSEB	0.000	11.284	0	106.4E6	N.D.	10.943
15) T	Picloram	0.000	12.330f	0	99521089	N.D.	4.202
16) T	DCPA	0.000	12.330	0	99521089	N.D.	4.129



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100925\
Data File : PS031975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2025 18:25
Operator : AR\AJ
Sample : PB170010TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB170010TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 02:50:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

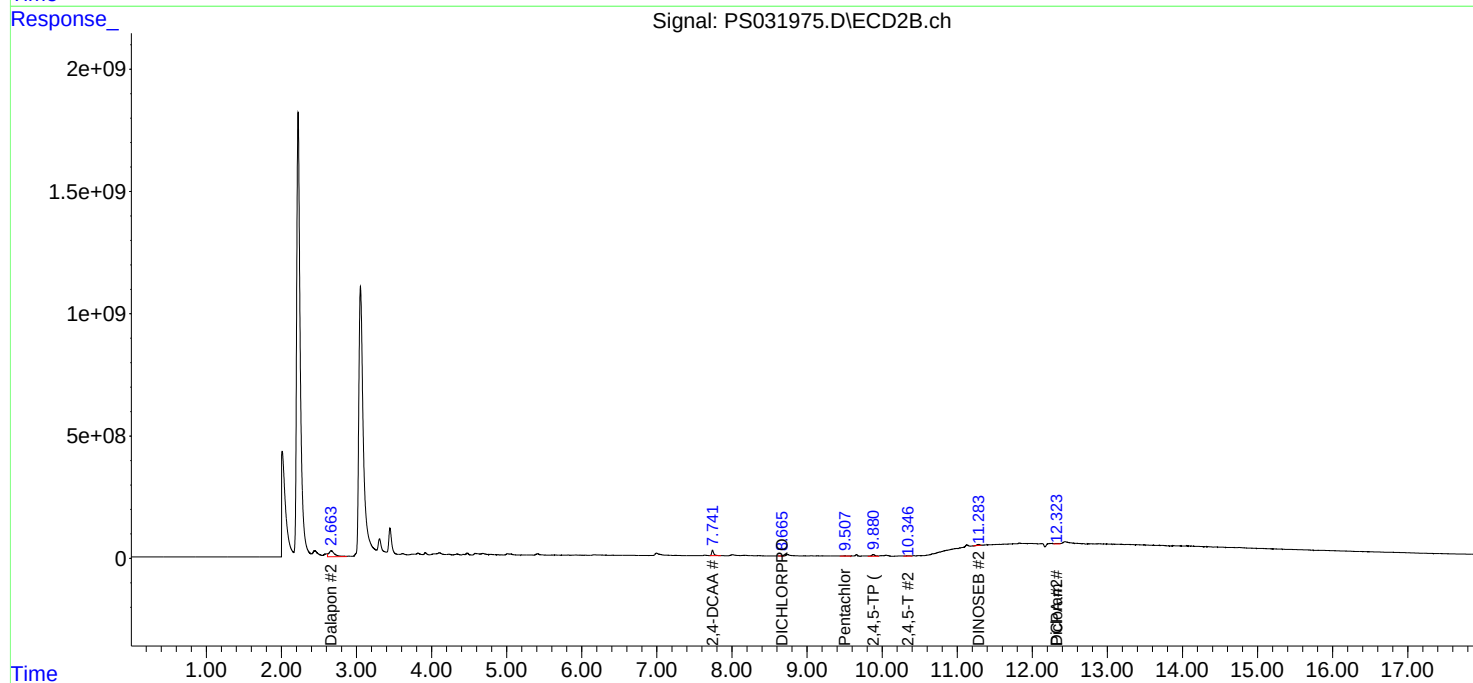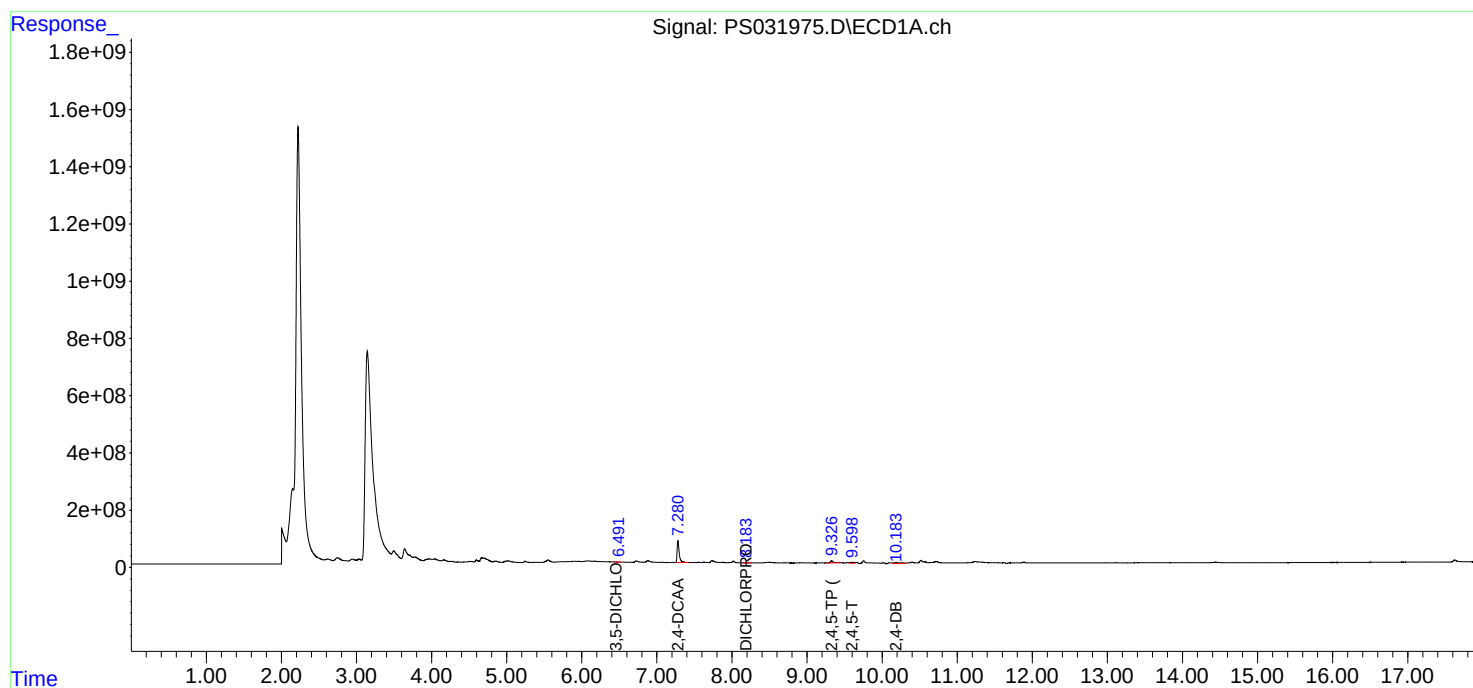


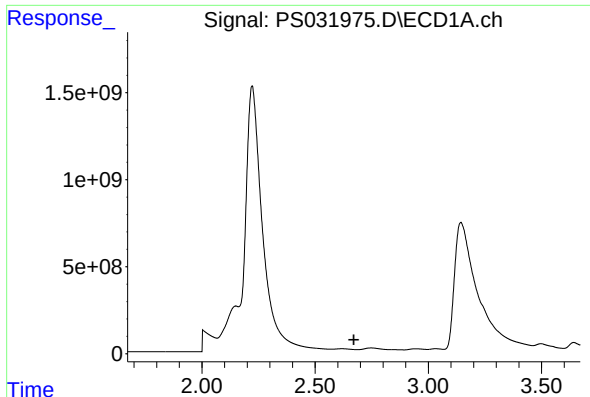

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB170010TB

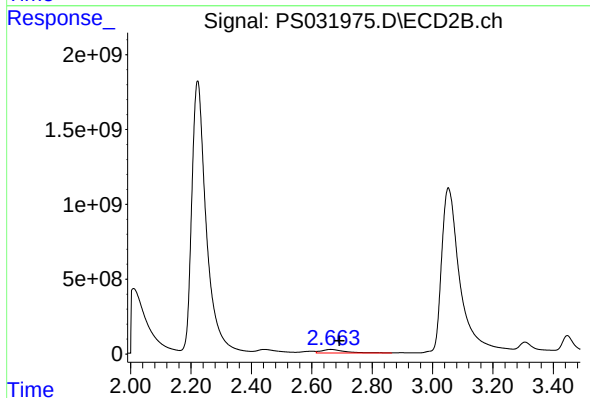


#1 Dalapon

R.T.: 2.663 min
Delta R.T.: -0.029 min
Response: 1317397317
Conc: 467.56 ng/ml

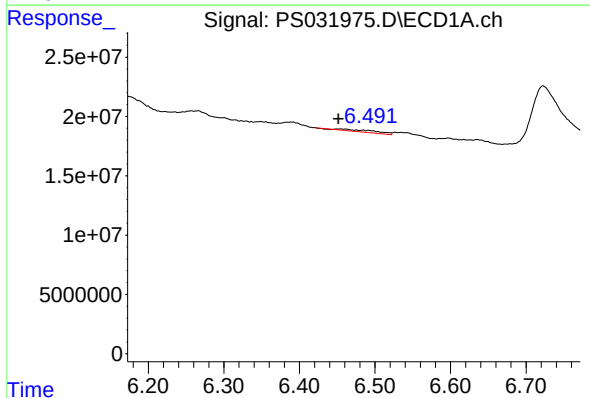


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.455 min
Delta R.T.: 0.003 min
Response: 5675716
Conc: 1.06 ng/ml

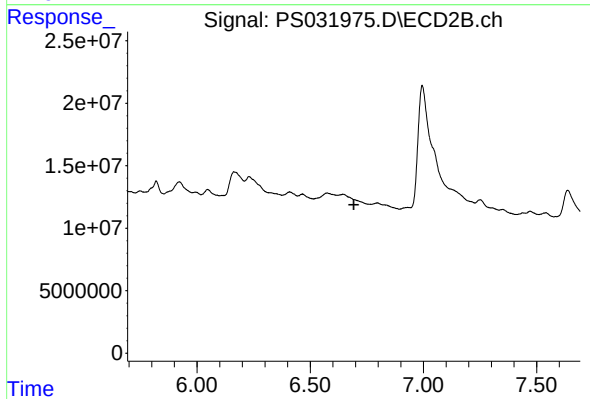

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.693 min
Response: 0
Conc: N.D.

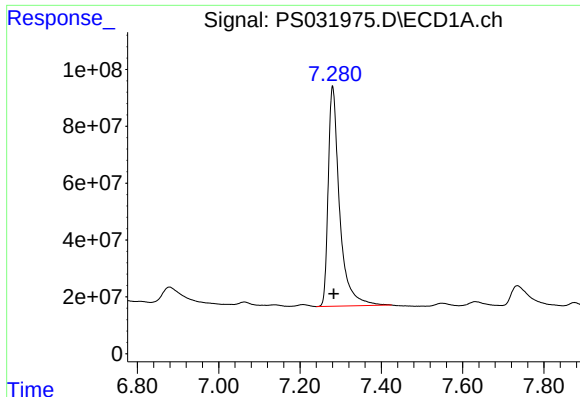

#4 2,4-DCAA


R.T.: 7.280 min
Delta R.T.: -0.003 min
Response: 1501347196
Conc: 416.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB170010TB

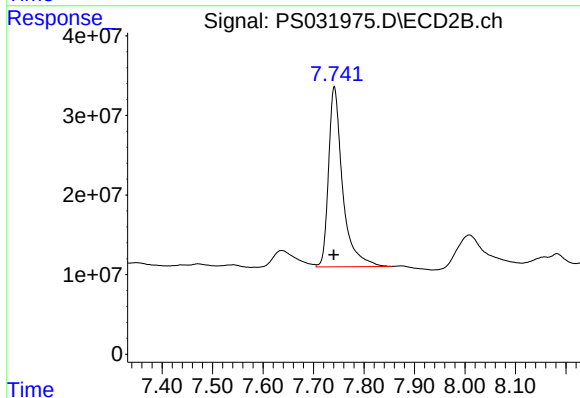


#4 2,4-DCAA

R.T.: 7.741 min
Delta R.T.: 0.000 min
Response: 437718862
Conc: 481.59 ng/ml

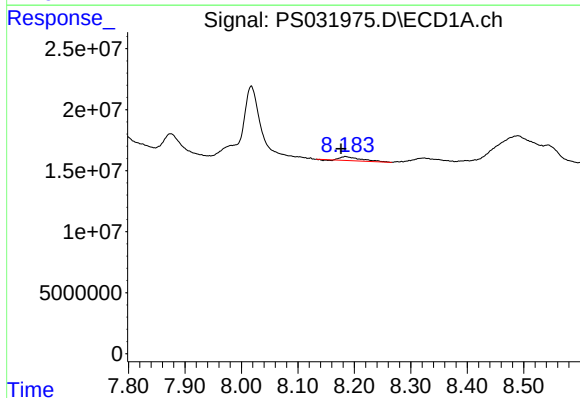


#8 DICHLORPROP

R.T.: 8.184 min
Delta R.T.: 0.008 min
Response: 7741797
Conc: 2.17 ng/ml

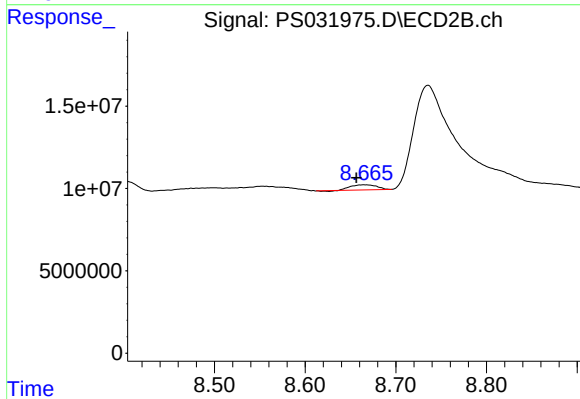

#8 DICHLORPROP


R.T.: 8.666 min
Delta R.T.: 0.009 min
Response: 5977060
Conc: 4.11 ng/ml

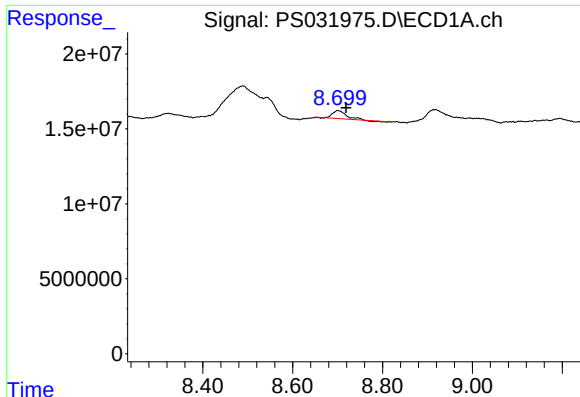

#10 Pentachlorophenol


R.T.: 8.701 min
Delta R.T.: -0.018 min
Response: 10856087
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB170010TB

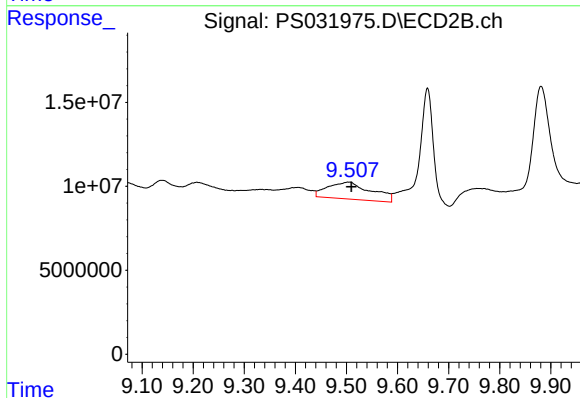


#10 Pentachlorophenol

R.T.: 9.504 min
Delta R.T.: -0.005 min
Response: 59575886
Conc: 1.50 ng/ml

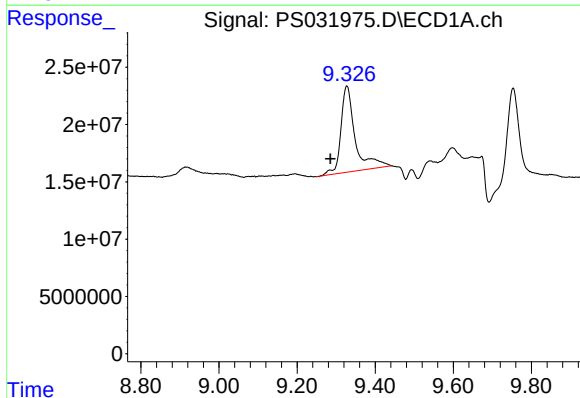


#11 2,4,5-TP (SILVEX)

R.T.: 9.328 min
Delta R.T.: 0.042 min
Response: 192156463
Conc: 9.16 ng/ml

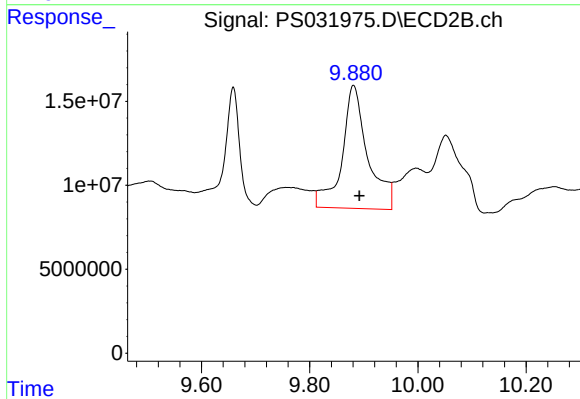

#11 2,4,5-TP (SILVEX)


R.T.: 9.881 min
Delta R.T.: -0.011 min
Response: 242388973
Conc: 16.10 ng/ml

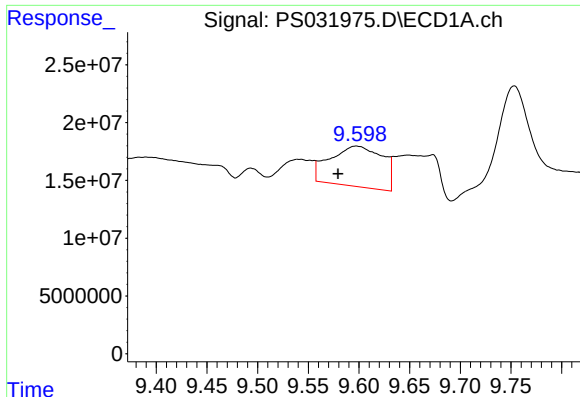

#12 2,4,5-T


R.T.: 9.598 min
Delta R.T.: 0.018 min
Response: 125566248
Conc: 6.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB170010TB

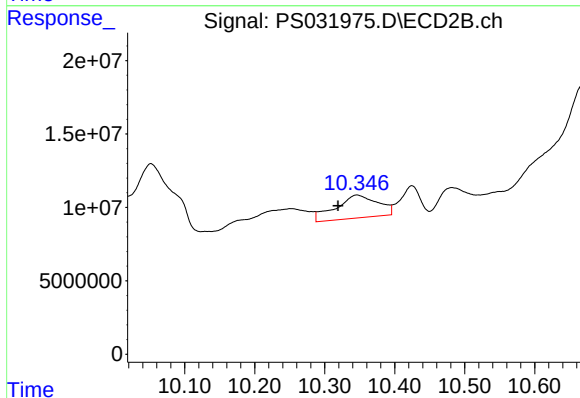


#12 2,4,5-T

R.T.: 10.346 min
Delta R.T.: 0.027 min
Response: 65127042
Conc: 4.84 ng/ml

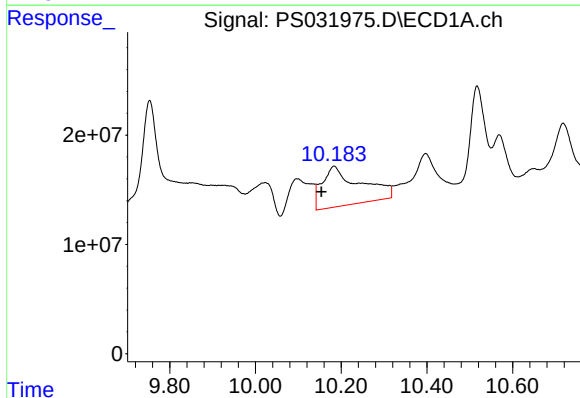


#13 2,4-DB

R.T.: 10.184 min
Delta R.T.: 0.029 min
Response: 223568787
Conc: 95.84 ng/ml

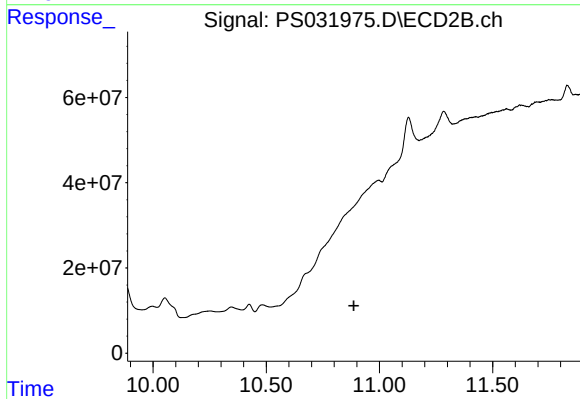

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.887 min
Response: 0
Conc: N.D.

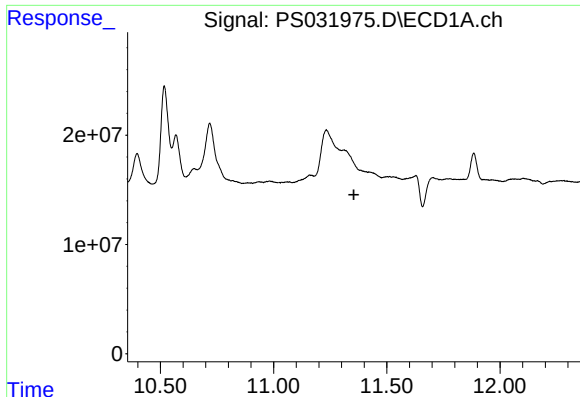

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB170010TB

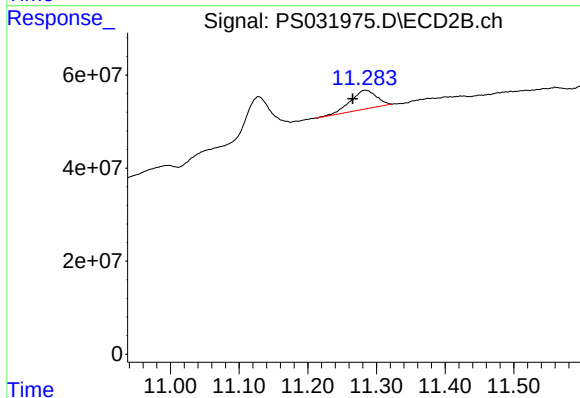


#14 DINOSEB

R.T.: 11.284 min
Delta R.T.: 0.018 min
Response: 106375585
Conc: 10.94 ng/ml

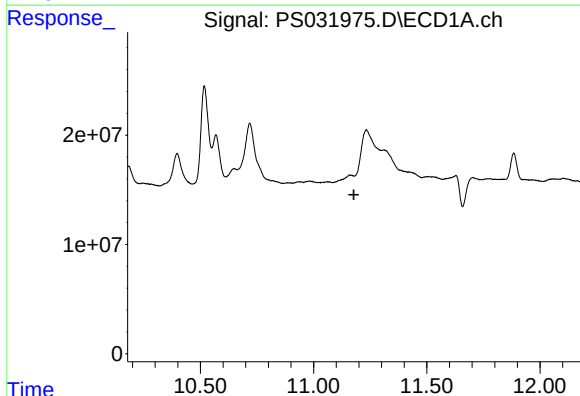


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.178 min
Response: 0
Conc: N.D.

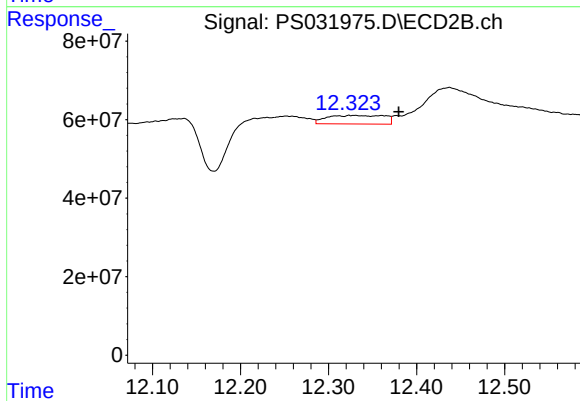

#15 Picloram


R.T.: 12.330 min
Delta R.T.: -0.050 min
Response: 99521089
Conc: 4.20 ng/ml

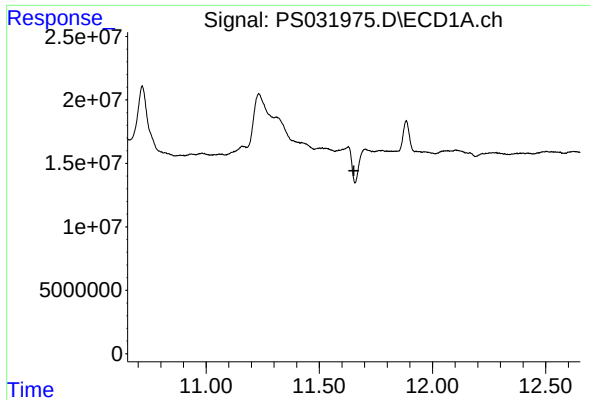

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.653 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB170010TB

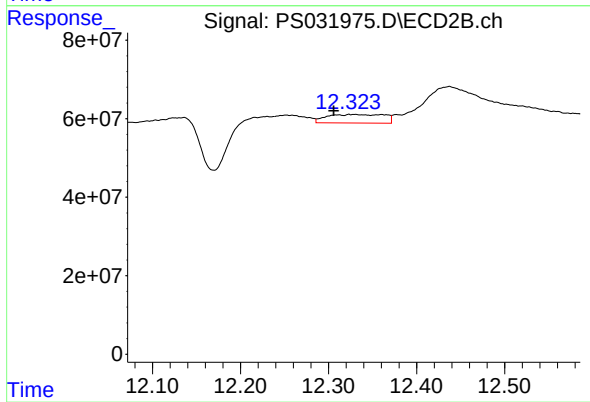

#16 DCPA

R.T.: 12.330 min
Delta R.T.: 0.024 min
Response: 99521089
Conc: 4.13 ng/ml