

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100925\
 Data File : PS031979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2025 20:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 02:51:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 09 13:56:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.284	7.747	1724.9E6	478.1E6	478.922	526.052
Target Compounds							
1) T	Dalapon	2.718f	2.657f	14002690	44627766	2.422	15.839 #
2) T	3,5-DICHL...	6.445	0.000	2003918	0	<MDL	N.D. #
3) T	4-Nitroph...	7.076	0.000	4856746	0	4.402	N.D. #
7) T	MCPA	7.800	0.000	2388780	0	<MDL	N.D. #
10) T	Pentachlo...	8.707	9.514	10627140	7325120	<MDL	<MDL #
11) T	2,4,5-TP ...	9.306	9.925f	9372926	5287363	<MDL	<MDL #
12) T	2,4,5-T	9.628f	0.000	8967268	0	<MDL	N.D. #
13) T	2,4-DB	10.150	0.000	5785799	0	2.480	N.D. #
14) T	DINOSEB	11.353	0.000	10005735	0	<MDL	N.D. #
15) T	Picloram	11.164	0.000	1337355	0	<MDL	N.D. #
16) T	DCPA	11.647	0.000	8826814	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS100925\
Data File : PS031979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2025 20:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 02:51:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090925.M
Quant Title : 8080.M
QLast Update : Tue Sep 09 13:56:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

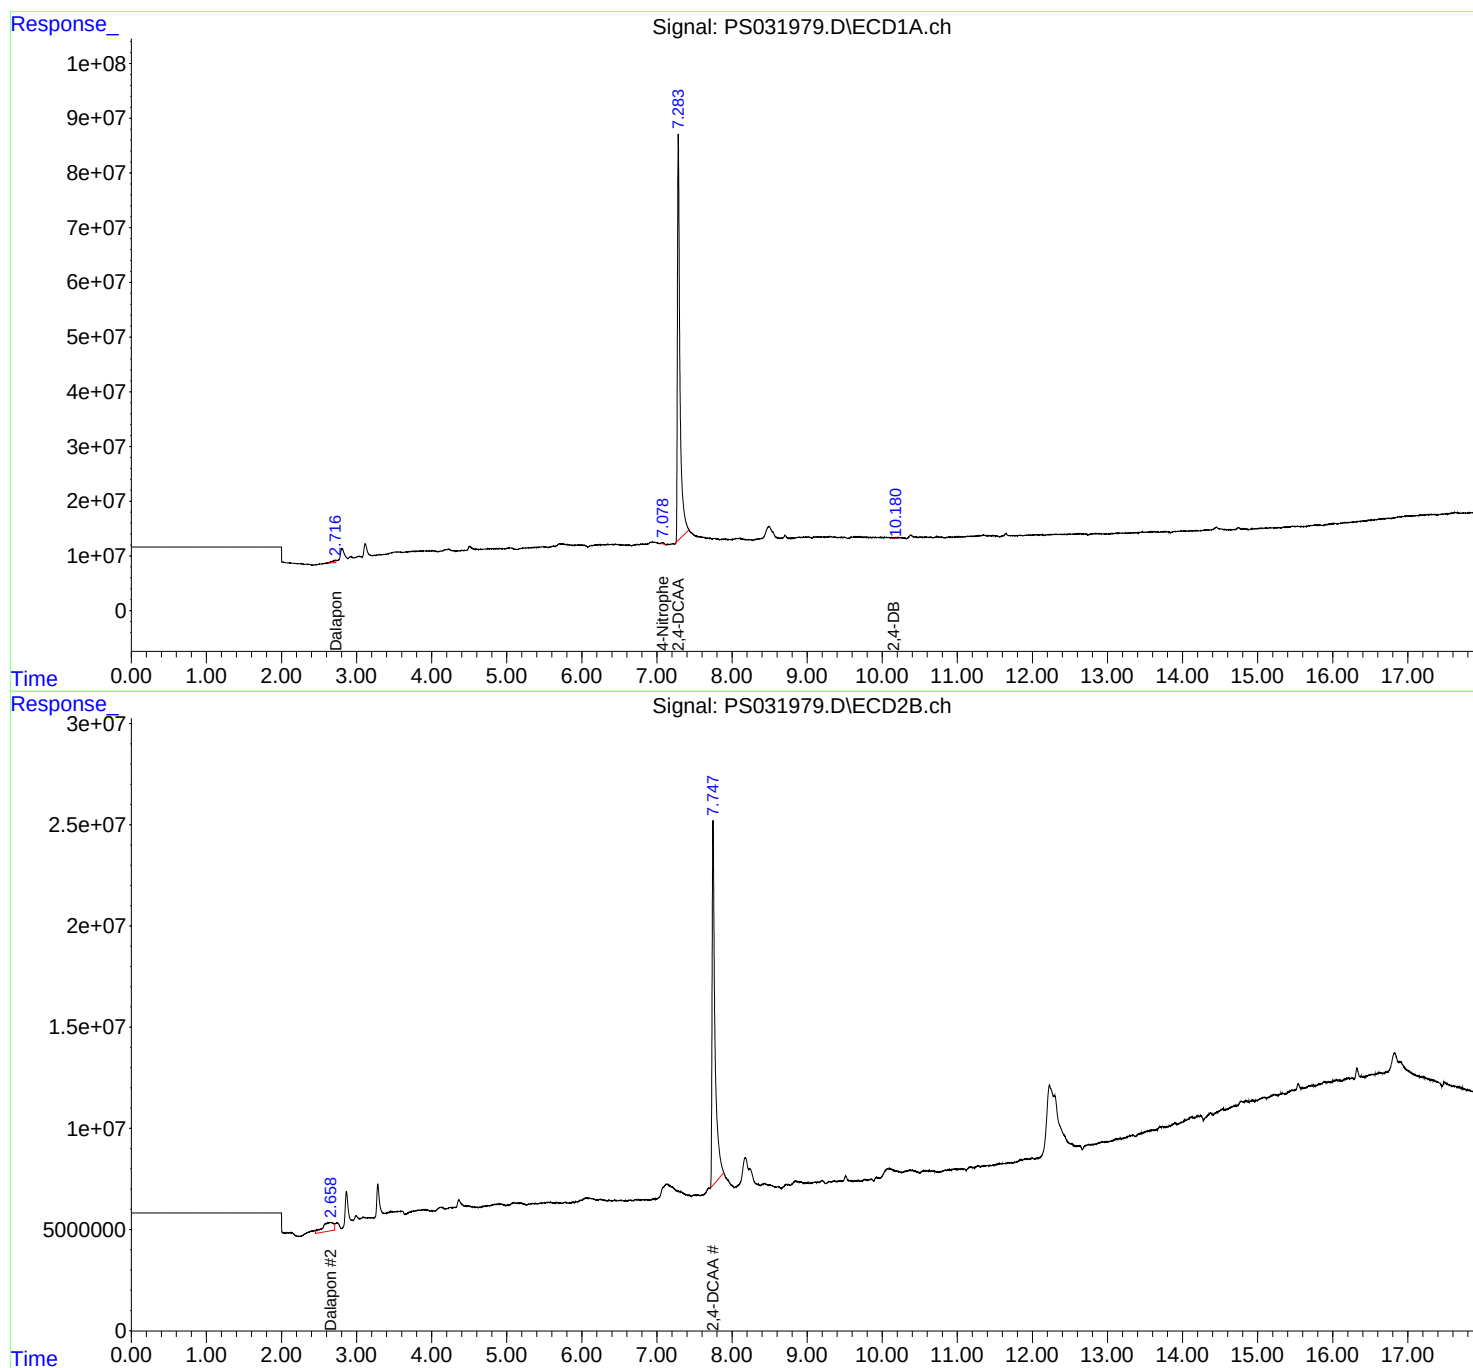


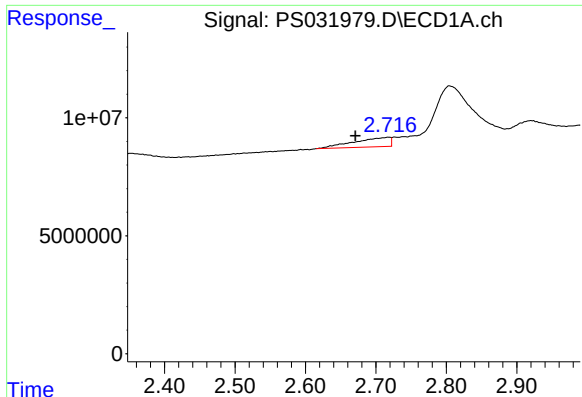

#1 Dalapon


R.T.: 2.718 min
Delta R.T.: 0.047 min
Response: 14002690
Conc: 2.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

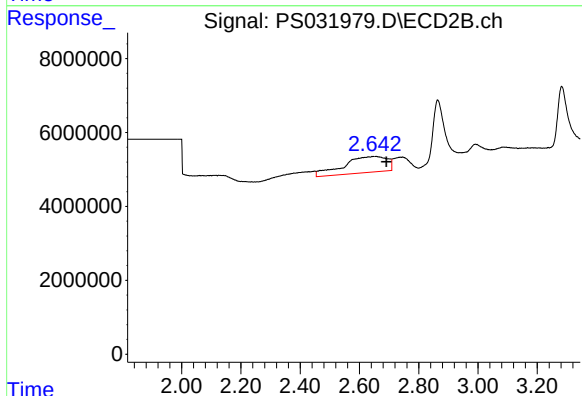


#1 Dalapon

R.T.: 2.657 min
Delta R.T.: -0.035 min
Response: 44627766
Conc: 15.84 ng/ml

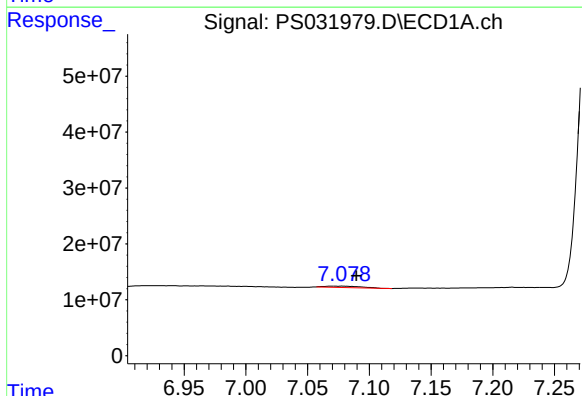


#3 4-Nitrophenol

R.T.: 7.076 min
Delta R.T.: -0.013 min
Response: 4856746
Conc: 4.40 ng/ml

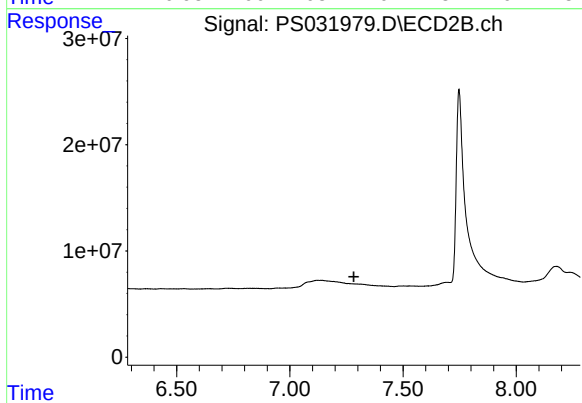

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.283 min
Response: 0
Conc: N.D.

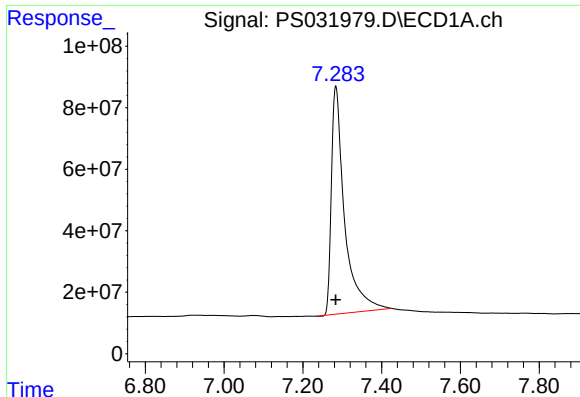

#4 2,4-DCAA


R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 1724851597
Conc: 478.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

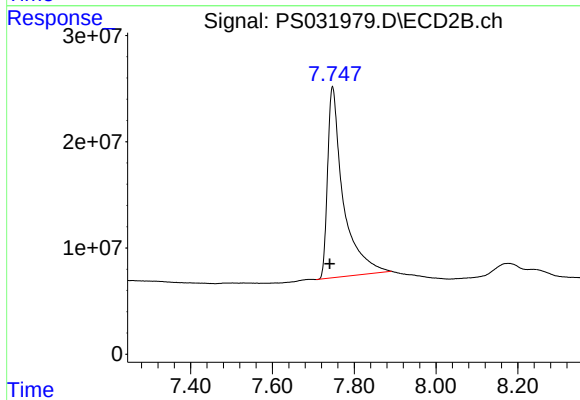


#4 2,4-DCAA

R.T.: 7.747 min
Delta R.T.: 0.007 min
Response: 478128705
Conc: 526.05 ng/ml

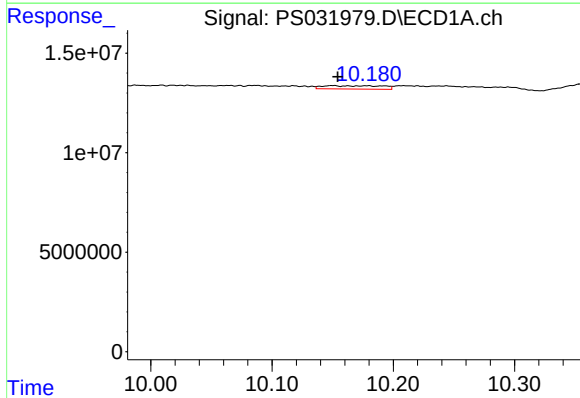

#13 2,4-DB

R.T.: 10.150 min
Delta R.T.: -0.005 min
Response: 5785799
Conc: 2.48 ng/ml

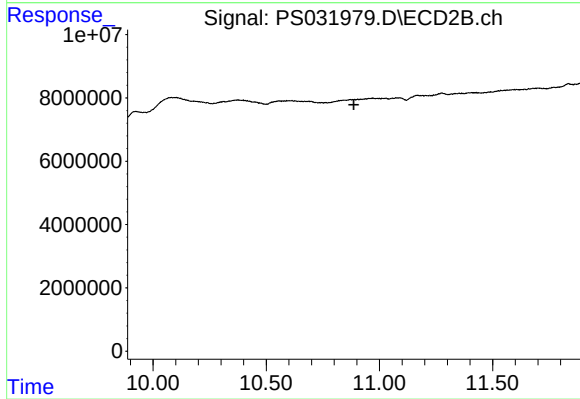

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.887 min
Response: 0
Conc: N.D.