

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 08:45
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 14:33:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	11.001	0	2080087	N.D.	8.189 #
Target Compounds							
2) T	3,5-DICHL...	9.821	0.000	1803381	0	5.479	N.D. #
5) T	DICAMBA	0.000	11.251	0	232725	N.D.	0.261 #
8) T	DICHLORPROP	13.016	0.000	2082248	0	8.973	N.D. #
15) T	Picloram	16.987	16.883	4701049	4221741	2.700	2.482
16) T	DCPA	0.000	16.883	0	4221741	N.D.	2.289 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 08:45
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 14:33:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

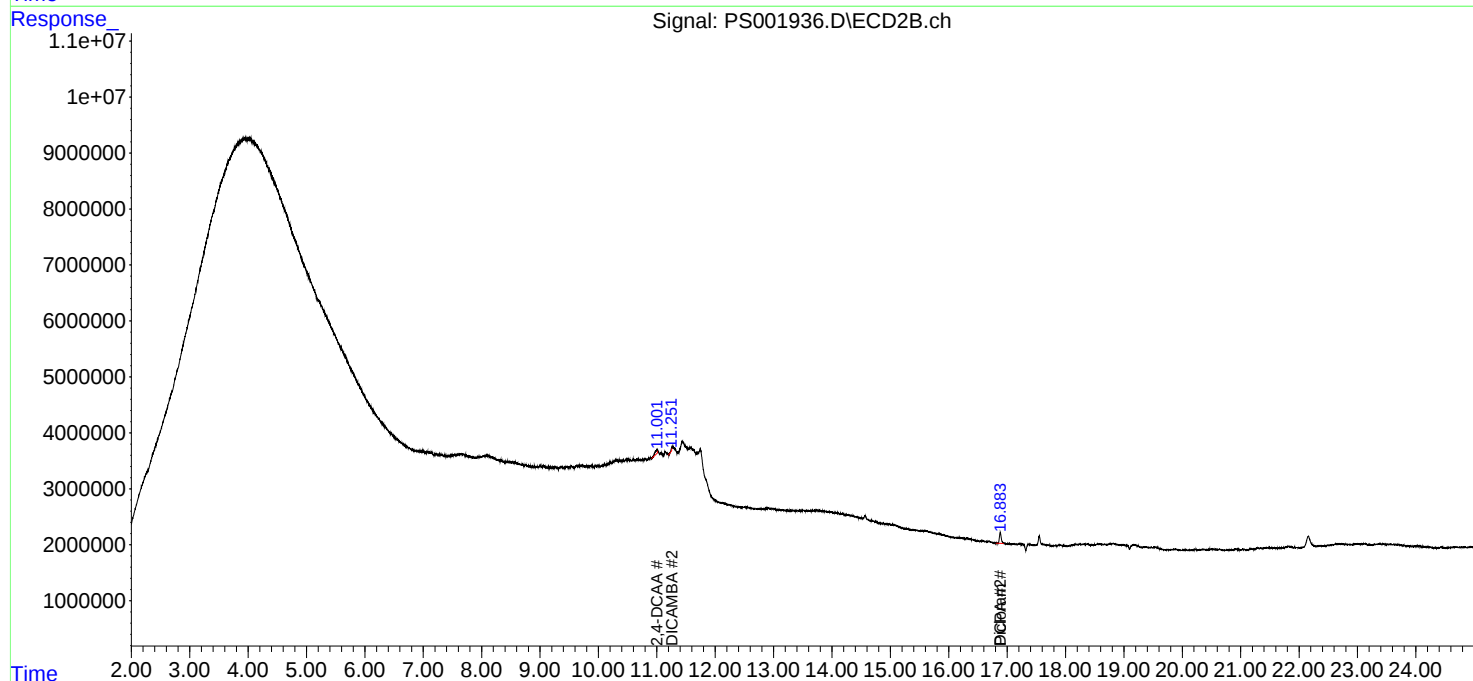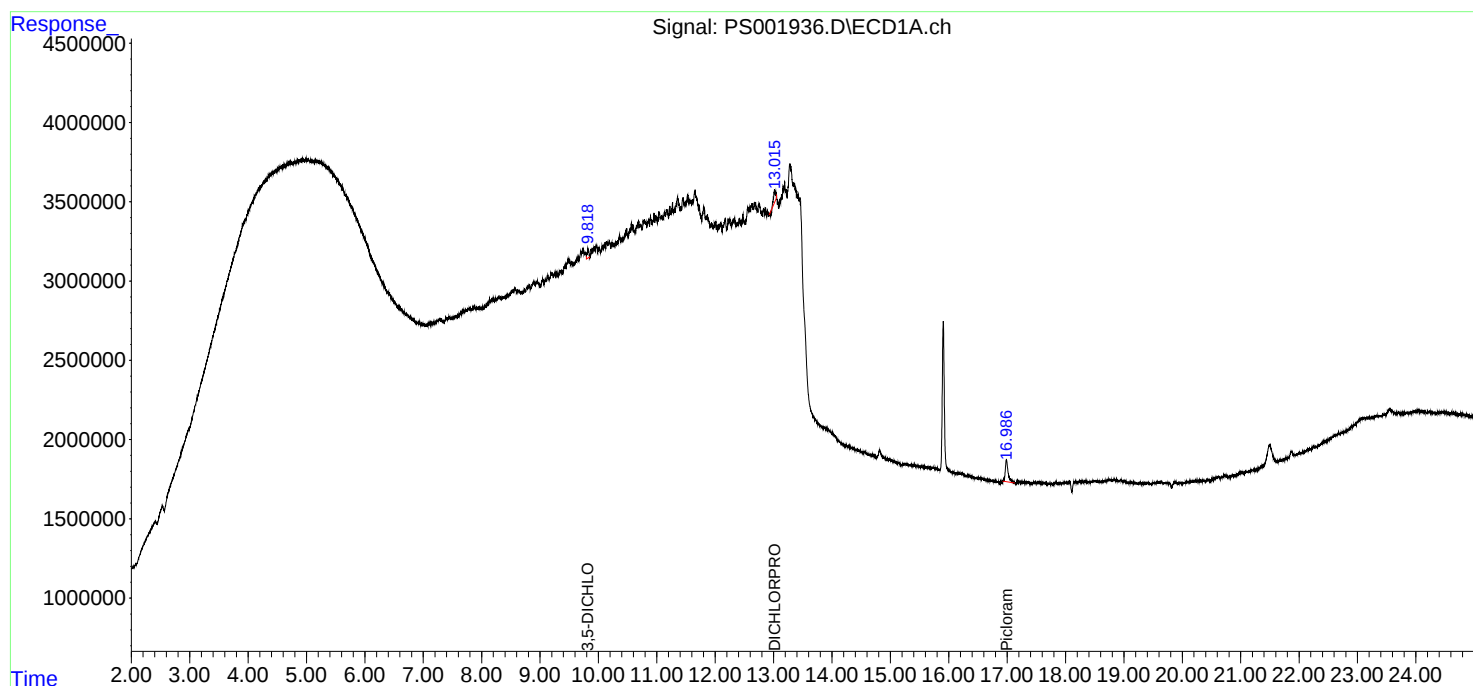


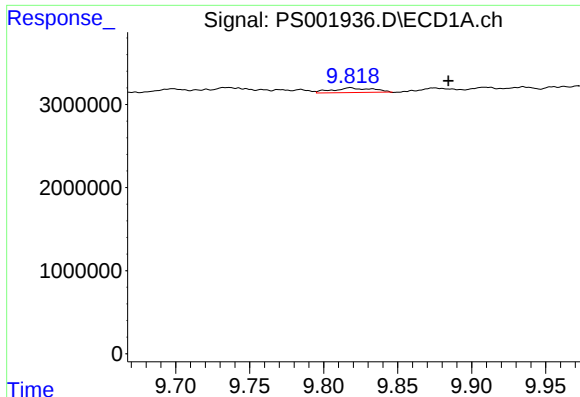

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.821 min
Delta R.T.: -0.063 min
Response: 1803381
Conc: 5.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

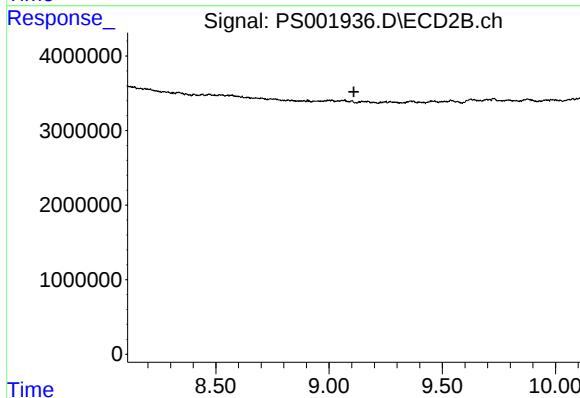


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.109 min
Response: 0
Conc: N.D.

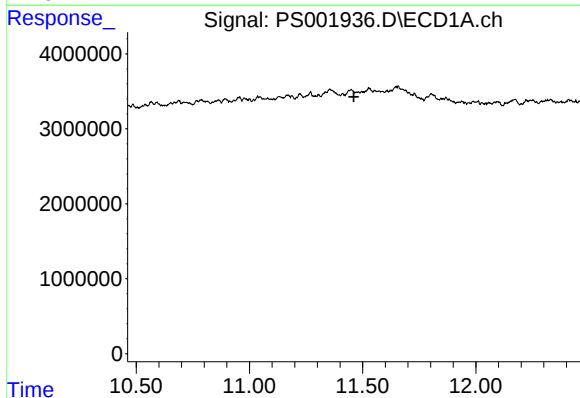


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.461 min
Response: 0
Conc: N.D.

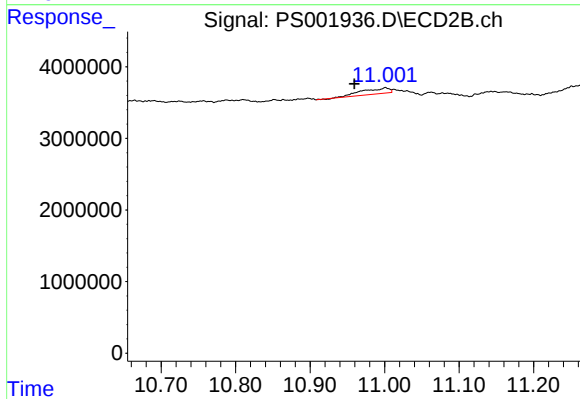

#4 2,4-DCAA


R.T.: 11.001 min
Delta R.T.: 0.042 min
Response: 2080087
Conc: 8.19 ng/ml

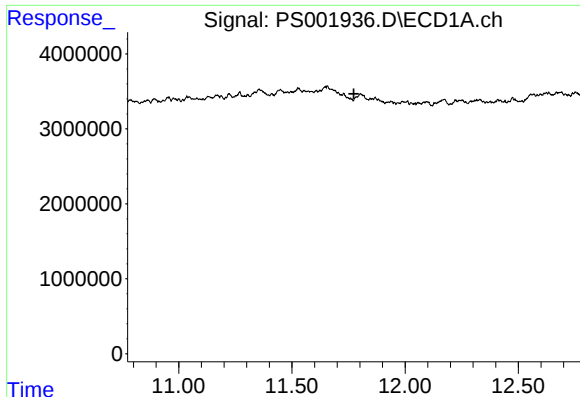

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.774 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

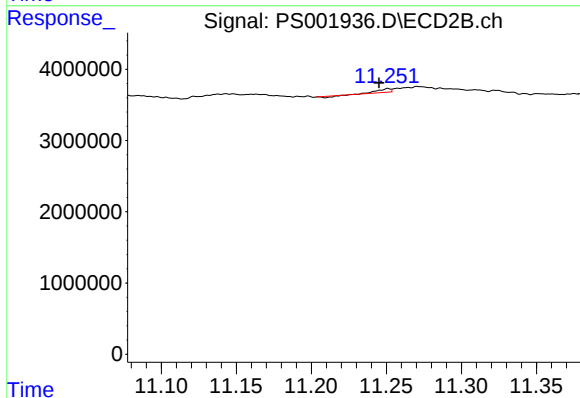


#5 DICAMBA

R.T.: 11.251 min
Delta R.T.: 0.006 min
Response: 232725
Conc: 0.26 ng/ml

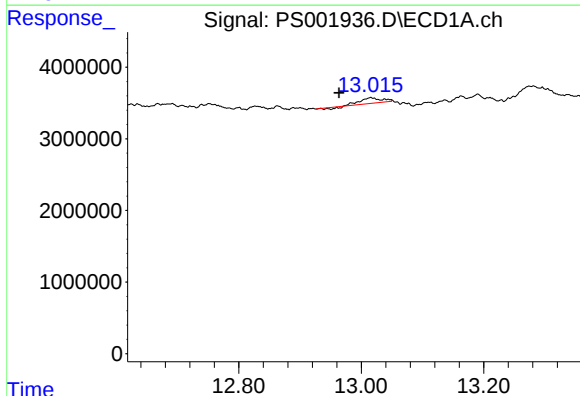


#8 DICHLORPROP

R.T.: 13.016 min
Delta R.T.: 0.052 min
Response: 2082248
Conc: 8.97 ng/ml

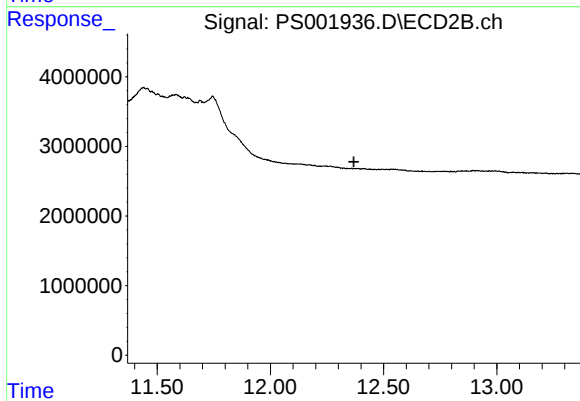

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.369 min
Response: 0
Conc: N.D.

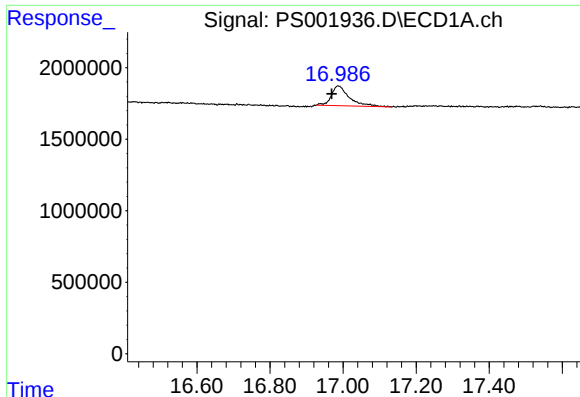

#15 Picloram


R.T.: 16.987 min
Delta R.T.: 0.019 min
Response: 4701049
Conc: 2.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

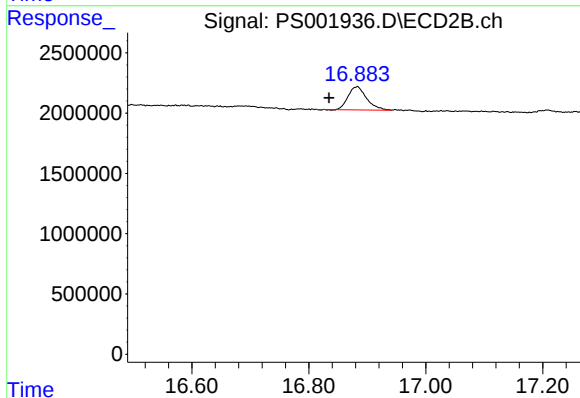


#15 Picloram

R.T.: 16.883 min
Delta R.T.: 0.049 min
Response: 4221741
Conc: 2.48 ng/ml

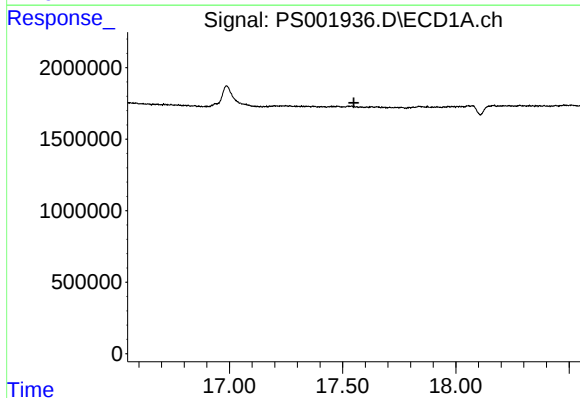

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.549 min
Response: 0
Conc: N.D.

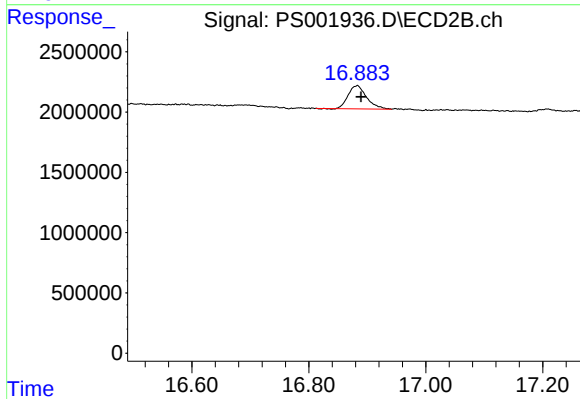

#16 DCPA

R.T.: 16.883 min
Delta R.T.: -0.006 min
Response: 4221741
Conc: 2.29 ng/ml