

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 12:58
 Operator : EI\SJ
 Sample : J5270-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 14:33:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.491	10.963	91983473	95747673	410.063	376.935
Target Compounds							
1) T	Dalapon	2.921	2.380	16315675	9246868	50.176	31.301 #
2) T	3,5-DICHL...	0.000	9.119	0	1854779	N.D.	5.876 #
6) T	MCP	12.175	0.000	13853317	0	21.740	N.D. #
9) T	2,4-D	0.000	12.796	0	2324238	N.D.	7.471 #
15) T	Picloram	0.000	16.901	0	7290128	N.D.	4.286 #
16) T	DCPA	0.000	16.901	0	7290128	N.D.	3.953 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 12:58
Operator : EI\SJ
Sample : J5270-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 14:33:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

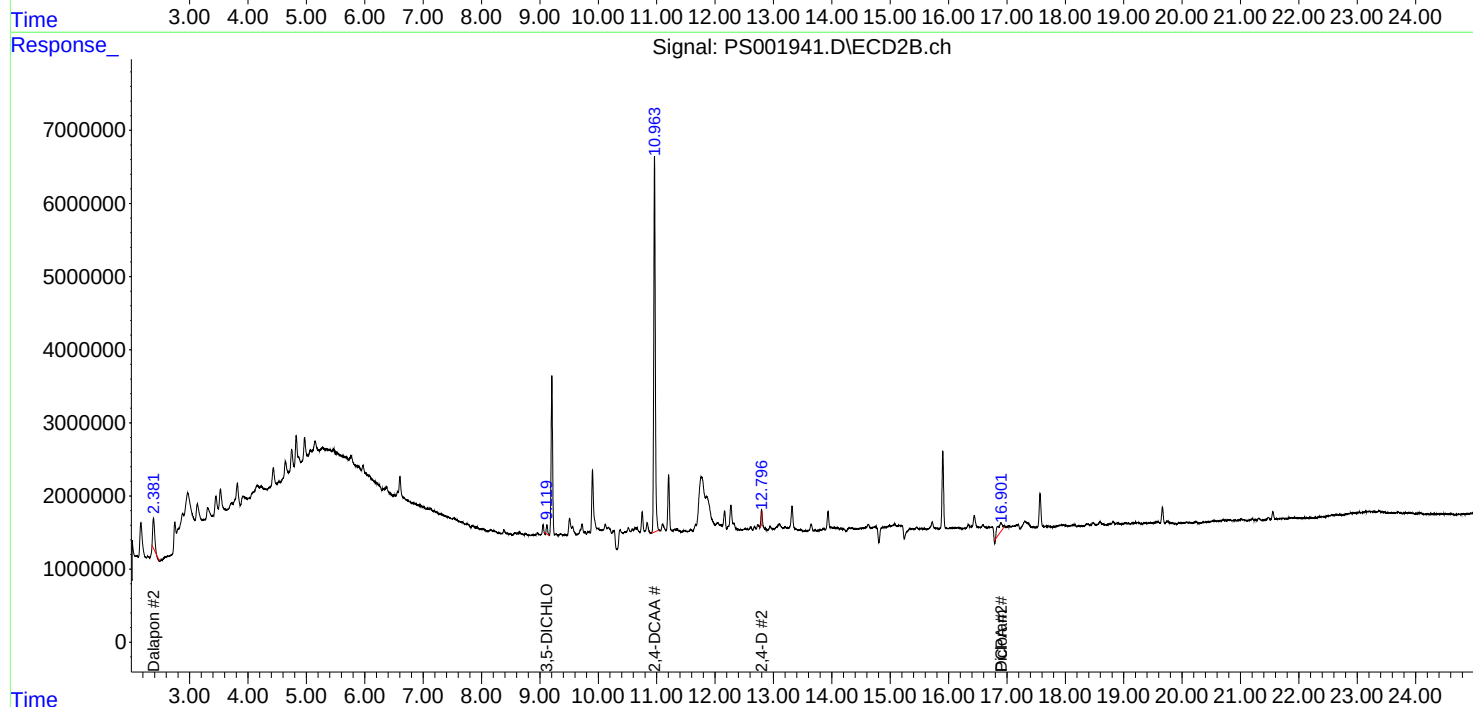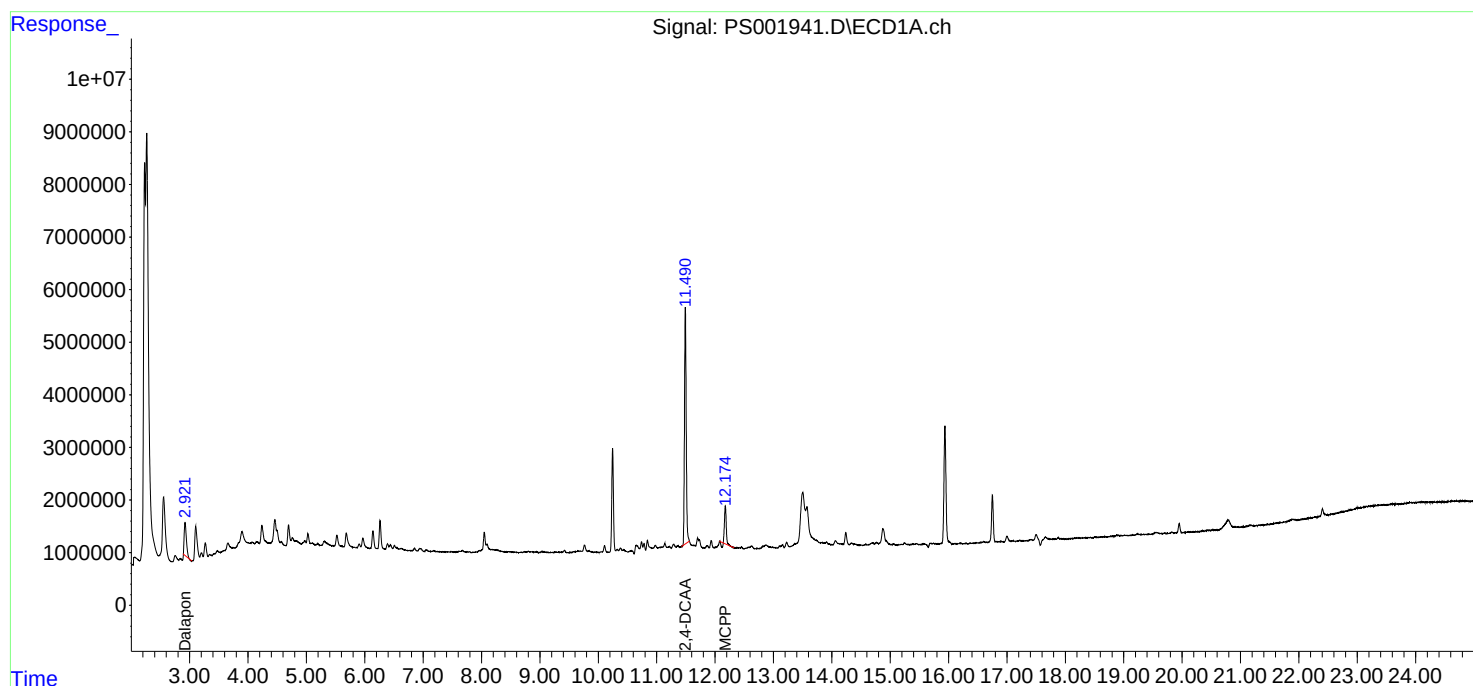


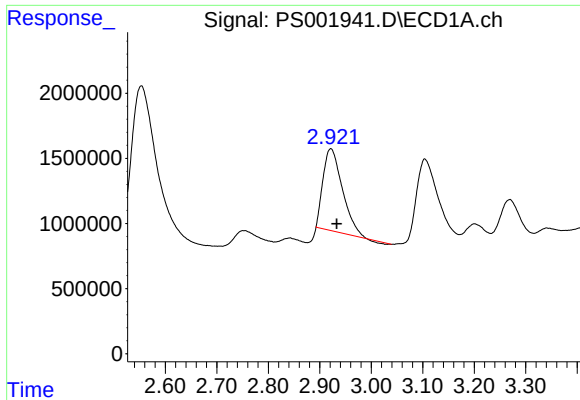

#1 Dalapon


R.T.: 2.921 min
Delta R.T.: -0.012 min
Response: 16315675
Conc: 50.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

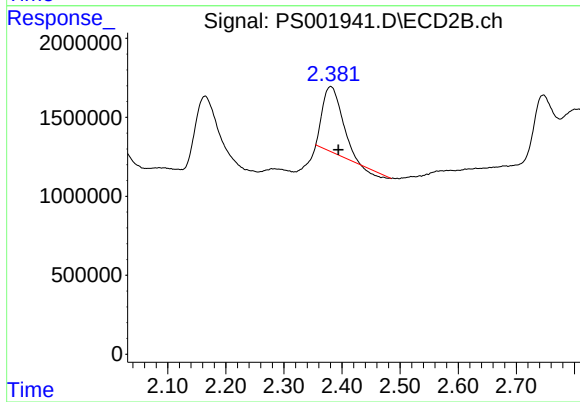


#1 Dalapon

R.T.: 2.380 min
Delta R.T.: -0.014 min
Response: 9246868
Conc: 31.30 ng/ml

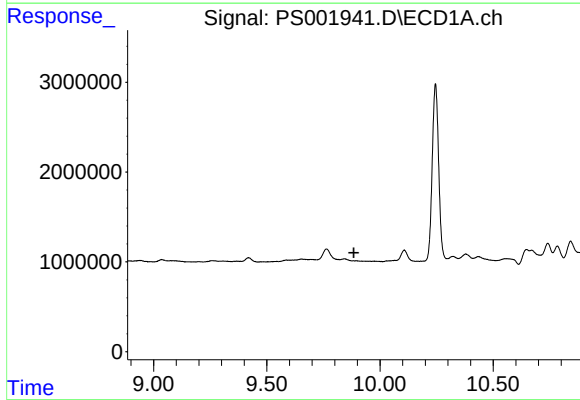


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.884 min
Response: 0
Conc: N.D.

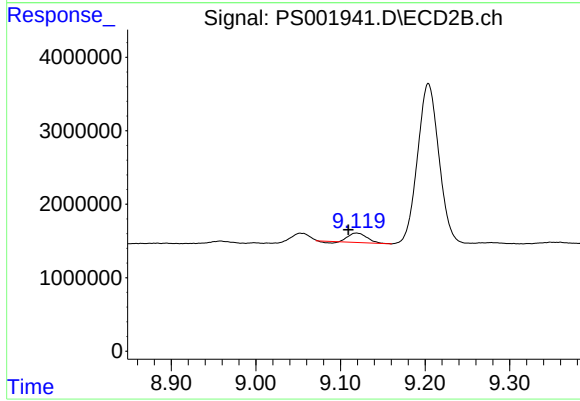

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.119 min
Delta R.T.: 0.009 min
Response: 1854779
Conc: 5.88 ng/ml

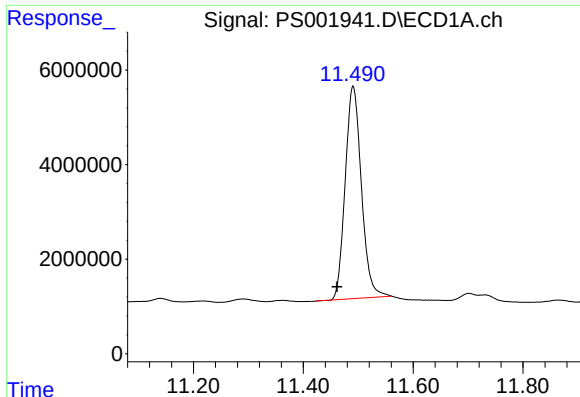

#4 2,4-DCAA


R.T.: 11.491 min
Delta R.T.: 0.029 min
Response: 91983473
Conc: 410.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

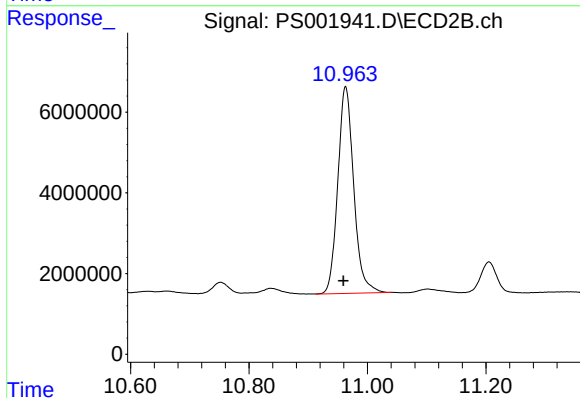


#4 2,4-DCAA

R.T.: 10.963 min
Delta R.T.: 0.003 min
Response: 95747673
Conc: 376.93 ng/ml

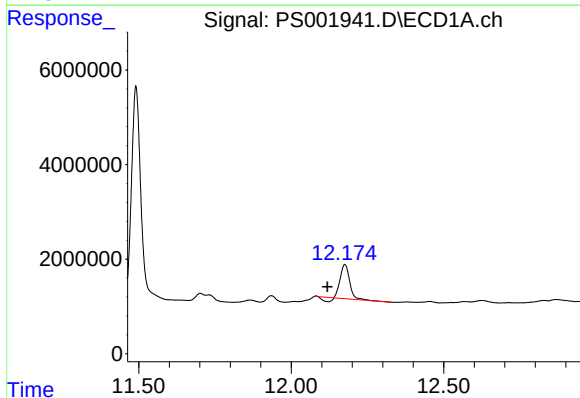


#6 MCPP

R.T.: 12.175 min
Delta R.T.: 0.057 min
Response: 13853317
Conc: 21.74 ug/ml

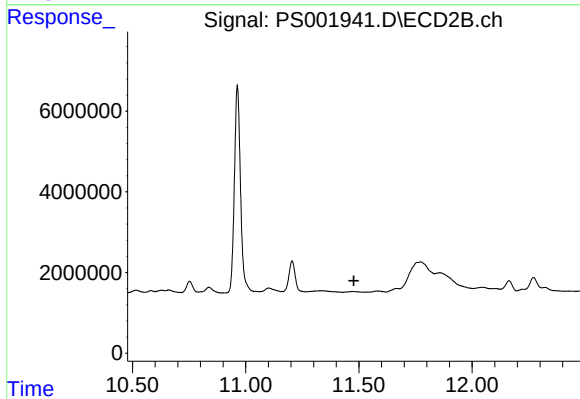

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

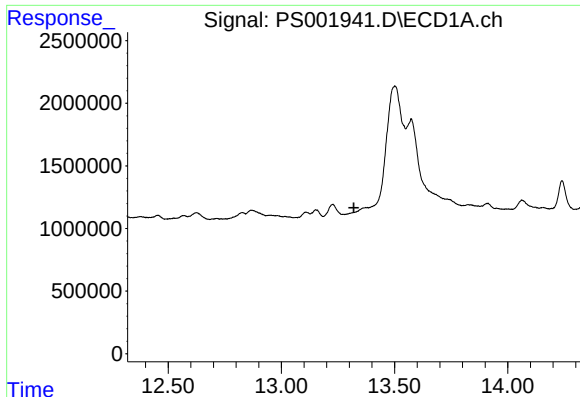

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

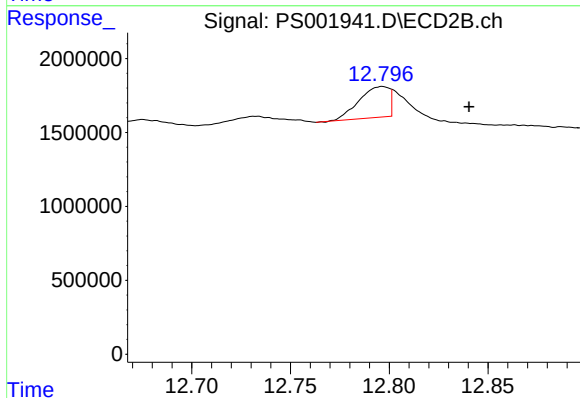


#9 2,4-D

R.T.: 12.796 min
Delta R.T.: -0.044 min
Response: 2324238
Conc: 7.47 ng/ml

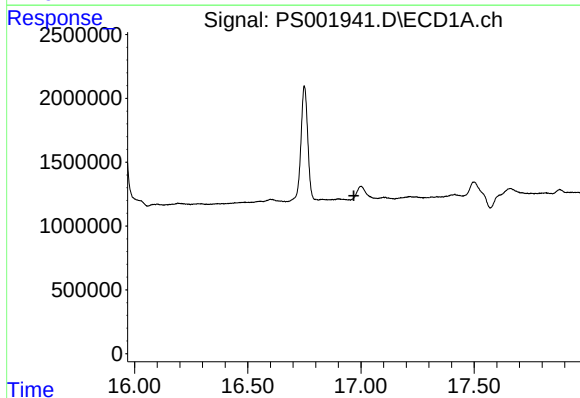


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.969 min
Response: 0
Conc: N.D.

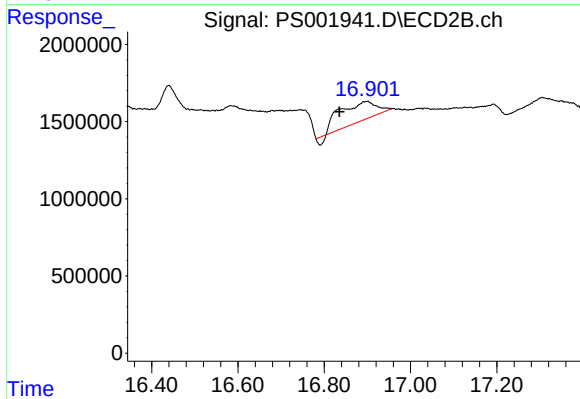

#15 Picloram


R.T.: 16.901 min
Delta R.T.: 0.066 min
Response: 7290128
Conc: 4.29 ng/ml

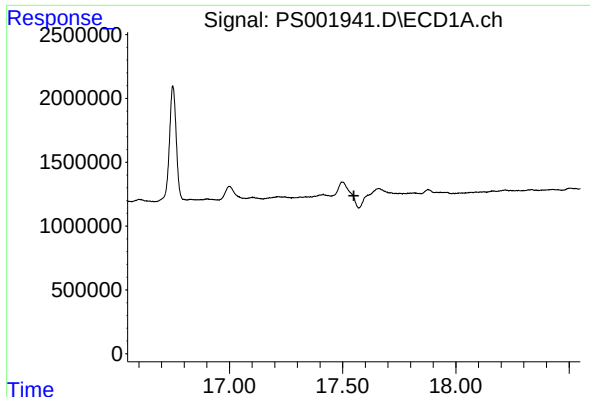

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

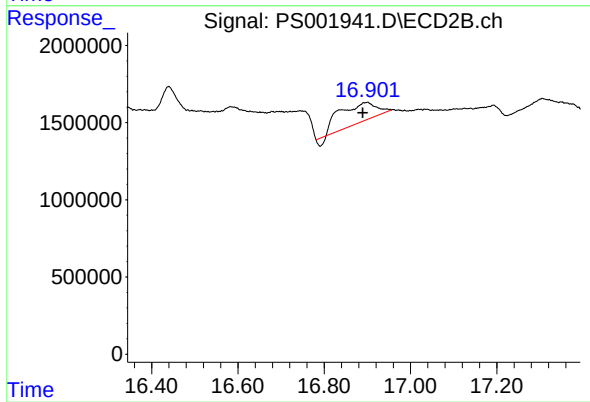

#16 DCPA

R.T.: 16.901 min
Delta R.T.: 0.011 min
Response: 7290128
Conc: 3.95 ng/ml