

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 14:33
 Operator : EI\SJ
 Sample : J5331-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 03:46:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.448	10.942	62338365	88801931	277.905	349.591 #
Target Compounds							
1) T	Dalapon	2.880	0.000	5774051	0	17.757	N.D. #
2) T	3,5-DICHL...	0.000	9.098	0	2568215	N.D.	8.137 #
5) T	DICAMBA	0.000	11.226	0	1539768	N.D.	1.726 #
6) T	MCP	12.133	0.000	11133071	0	17.471	N.D. #
9) T	2,4-D	0.000	12.775	0	5588549	N.D.	17.963 #
15) T	Picloram	0.000	16.819	0	3810227	N.D.	2.240 #
16) T	DCPA	17.613	16.878	-509574	4443701	N.D.	2.409



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 14:33
Operator : EI\SJ
Sample : J5331-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 03:46:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

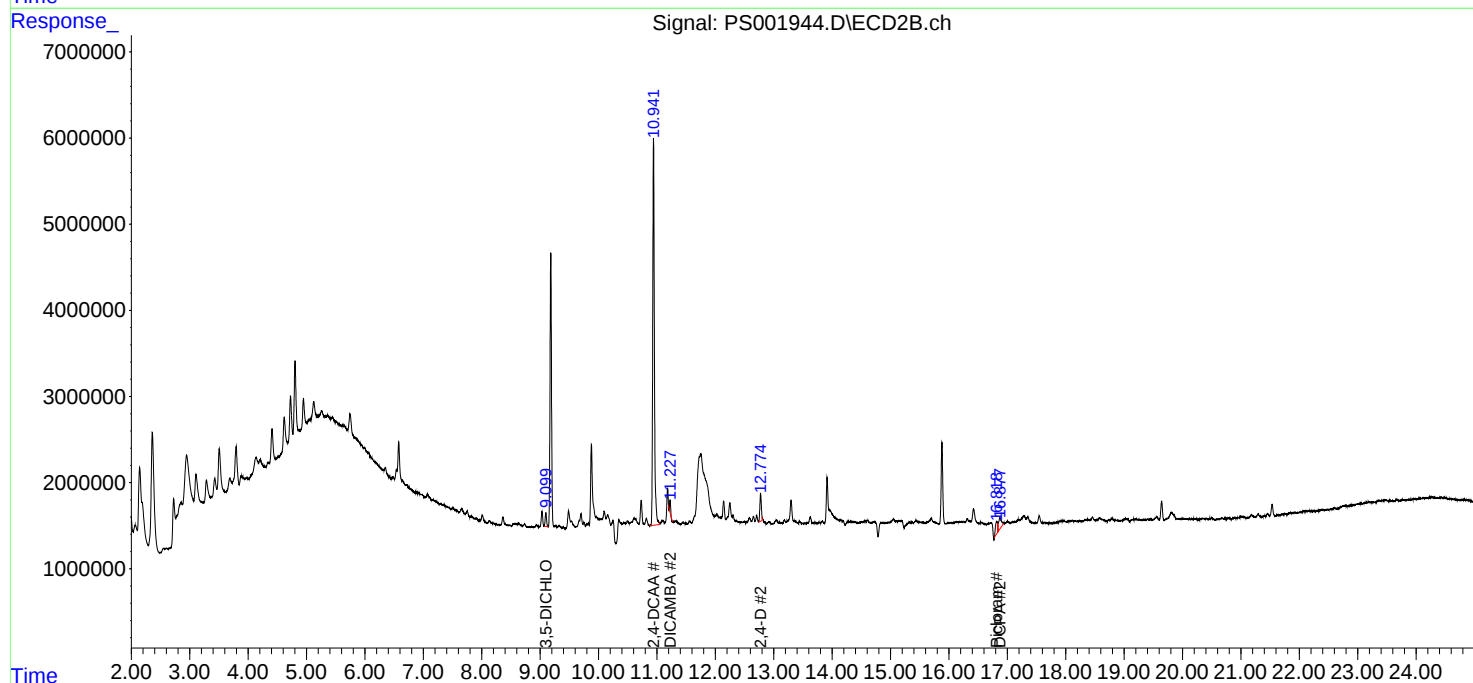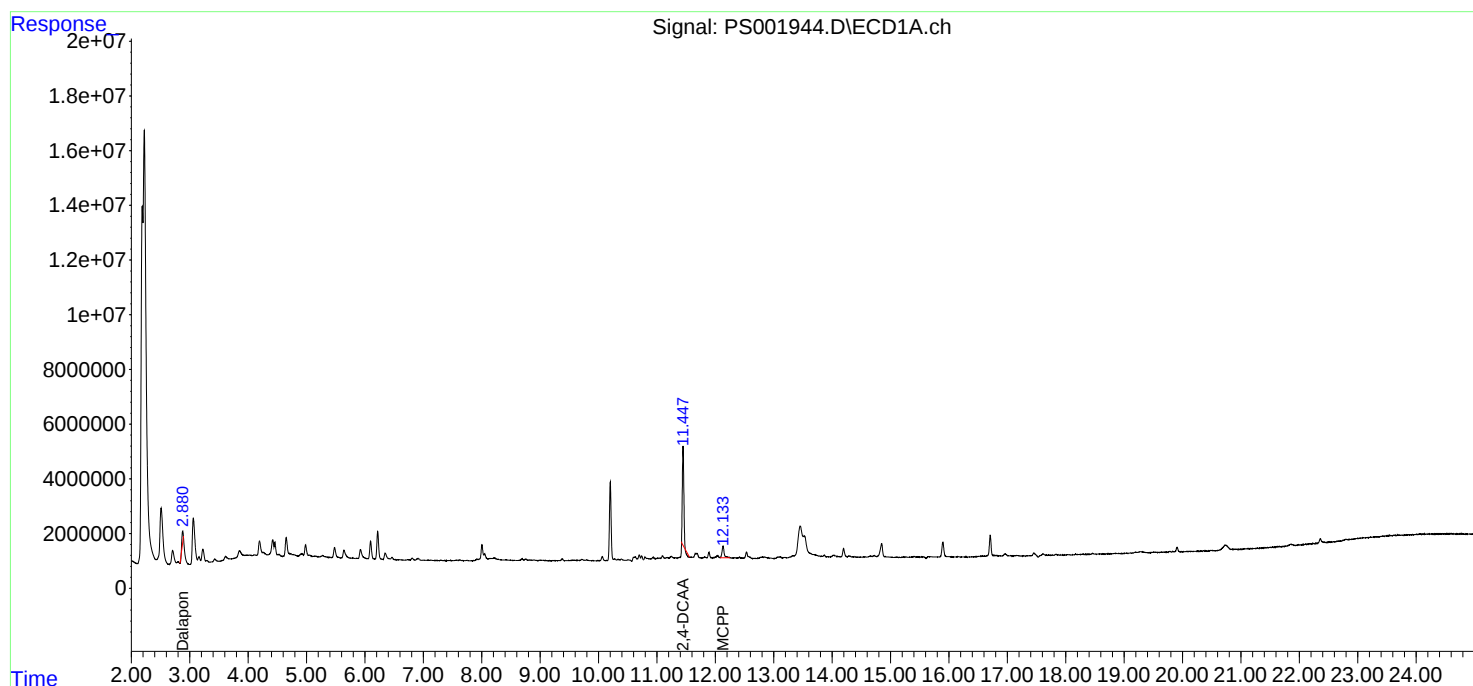


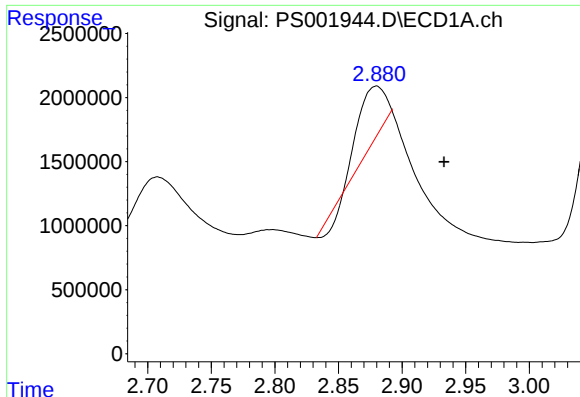

#1 Dalapon


R.T.: 2.880 min
Delta R.T.: -0.053 min
Response: 5774051
Conc: 17.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

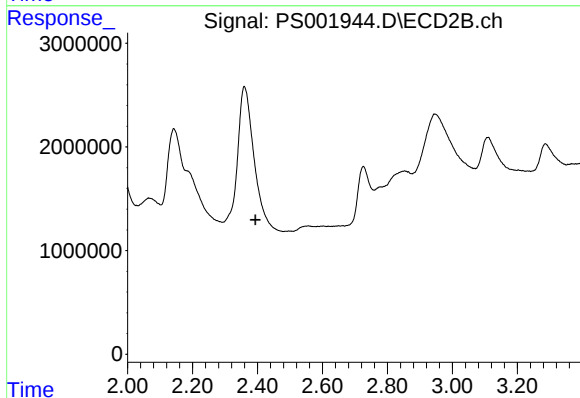


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.394 min
Response: 0
Conc: N.D.

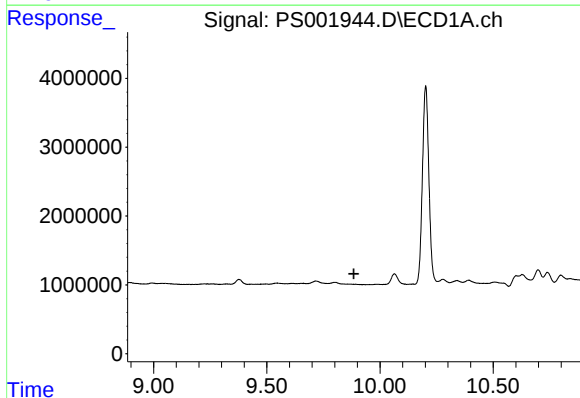


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.884 min
Response: 0
Conc: N.D.

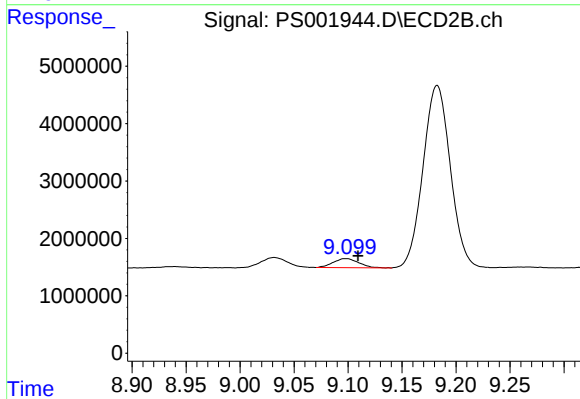

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.098 min
Delta R.T.: -0.011 min
Response: 2568215
Conc: 8.14 ng/ml

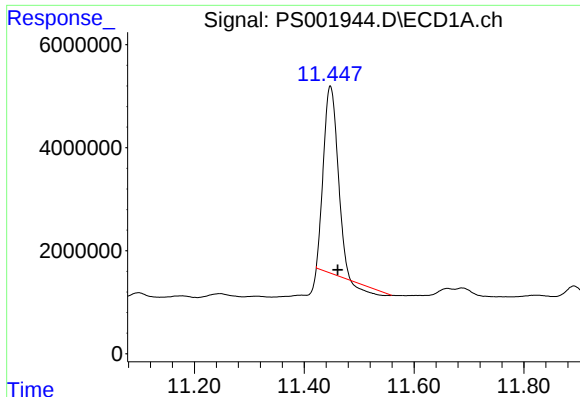

#4 2,4-DCAA


R.T.: 11.448 min
Delta R.T.: -0.014 min
Response: 62338365
Conc: 277.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

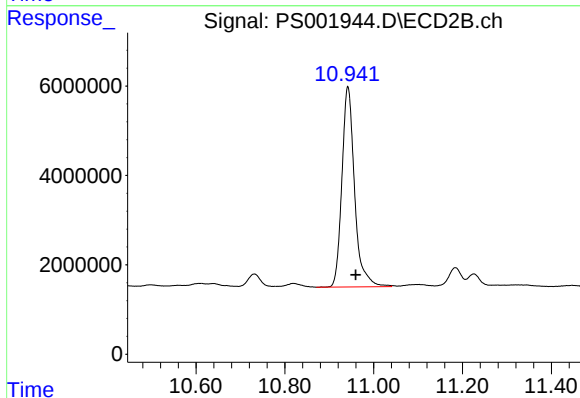


#4 2,4-DCAA

R.T.: 10.942 min
Delta R.T.: -0.018 min
Response: 88801931
Conc: 349.59 ng/ml

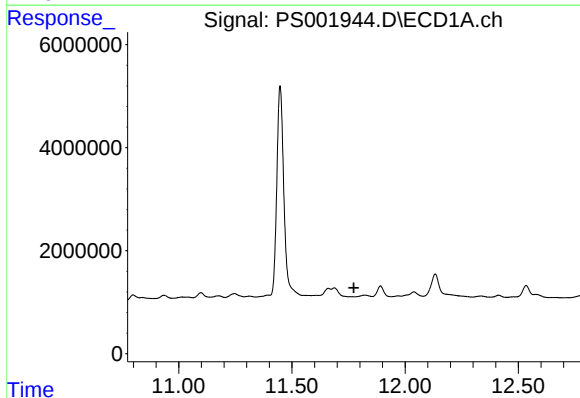


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.774 min
Response: 0
Conc: N.D.

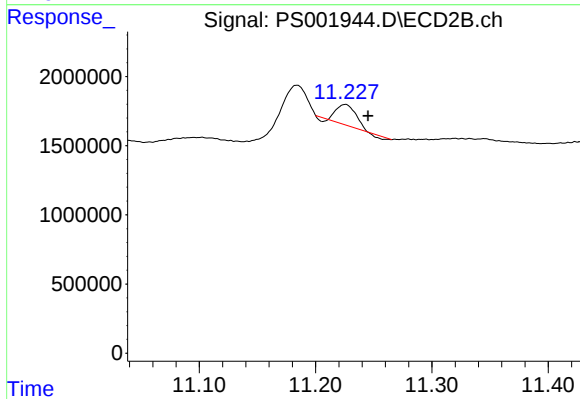

#5 DICAMBA


R.T.: 11.226 min
Delta R.T.: -0.019 min
Response: 1539768
Conc: 1.73 ng/ml

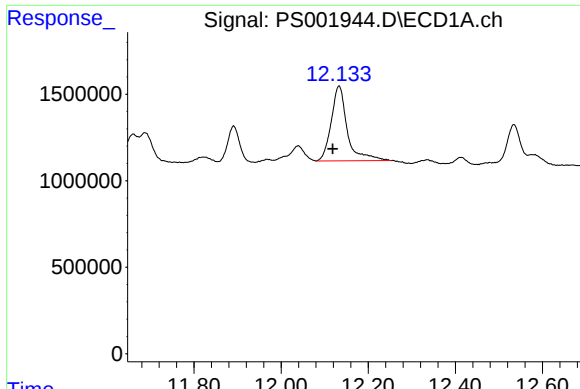

#6 MCP


R.T.: 12.133 min
Delta R.T.: 0.014 min
Response: 11133071
Conc: 17.47 ug/ml

Instrument :
ECD_S
ClientSampleId :

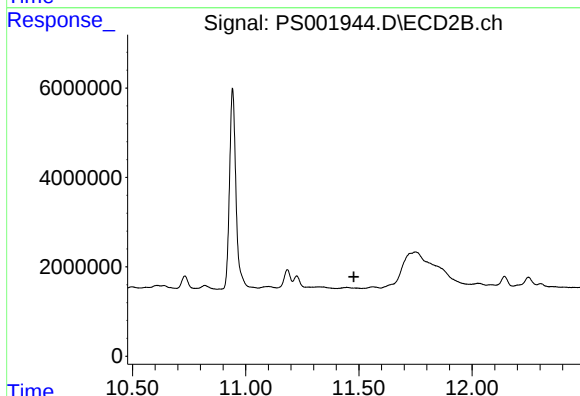


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

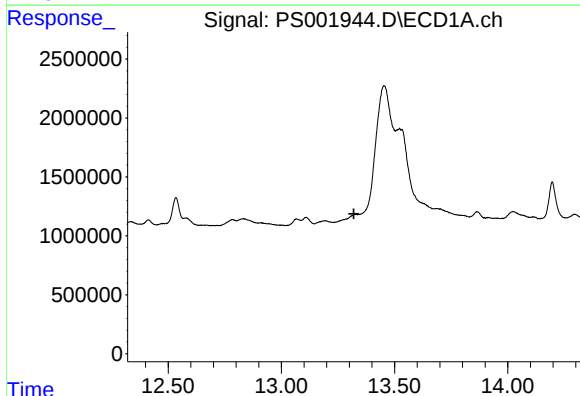


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.320 min
Response: 0
Conc: N.D.

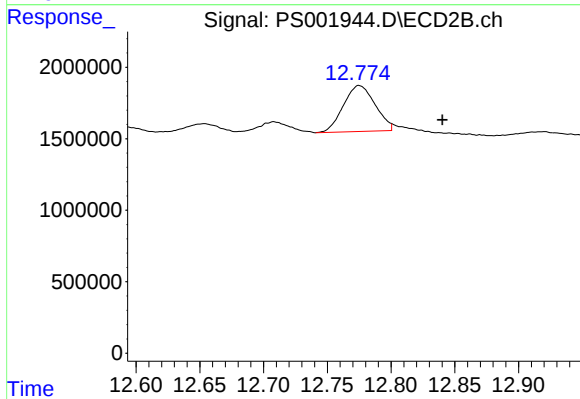

#9 2,4-D


R.T.: 12.775 min
Delta R.T.: -0.065 min
Response: 5588549
Conc: 17.96 ng/ml

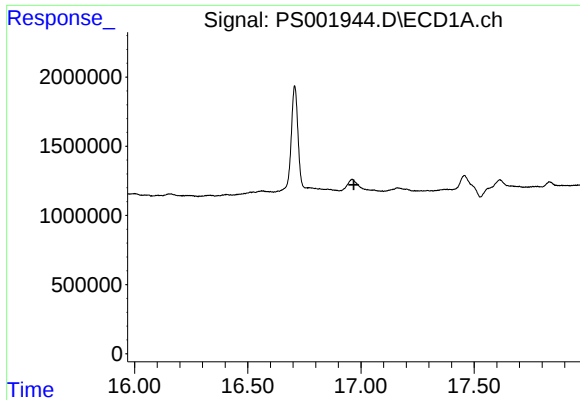

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

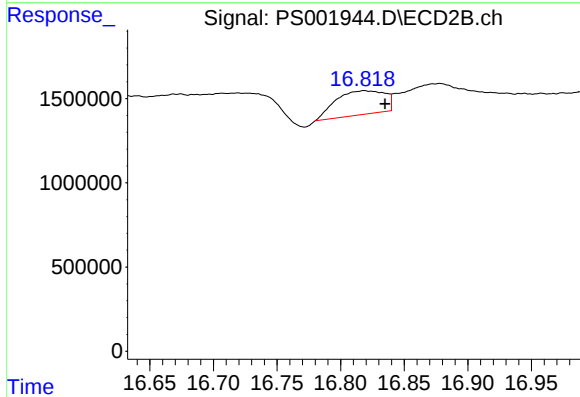


#15 Picloram

R.T.: 16.819 min
Delta R.T.: -0.016 min
Response: 3810227
Conc: 2.24 ng/ml

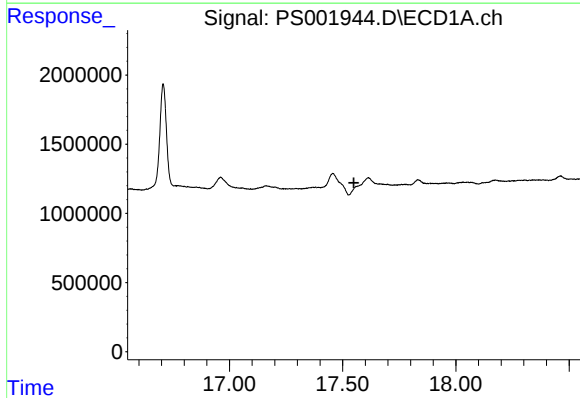

#16 DCPA

R.T.: 17.613 min
Delta R.T.: 0.064 min
Response: -509574
Conc: N.D.

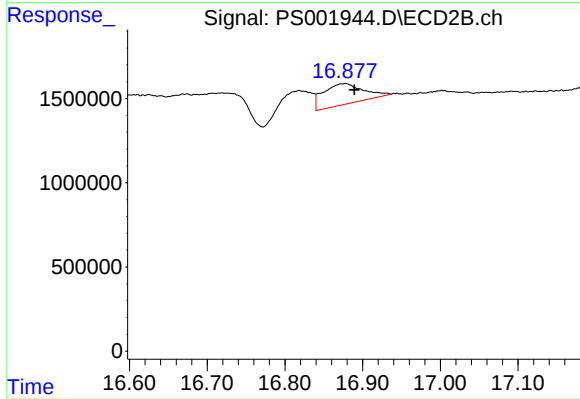

#16 DCPA

R.T.: 16.878 min
Delta R.T.: -0.011 min
Response: 4443701
Conc: 2.41 ng/ml