

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001945.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 15:04
 Operator : EI\SJ
 Sample : J5329-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 03:46:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.466	10.961	71620142	71915961	319.283	283.115
Target Compounds							
1) T	Dalapon	0.000	2.379	0	12492602	N.D.	42.288 #
2) T	3,5-DICHL...	0.000	9.118	0	1561006	N.D.	4.946 #
5) T	DICAMBA	11.705	0.000	2179711	0	2.515	N.D. #
6) T	MCP	12.151	0.000	11079314	0	17.387	N.D. #
15) T	Picloram	16.973	16.833	3150220	2979985	1.809	1.752
16) T	DCPA	0.000	16.895	0	2820167	N.D.	1.529 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 15:04
Operator : EI\SJ
Sample : J5329-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 03:46:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

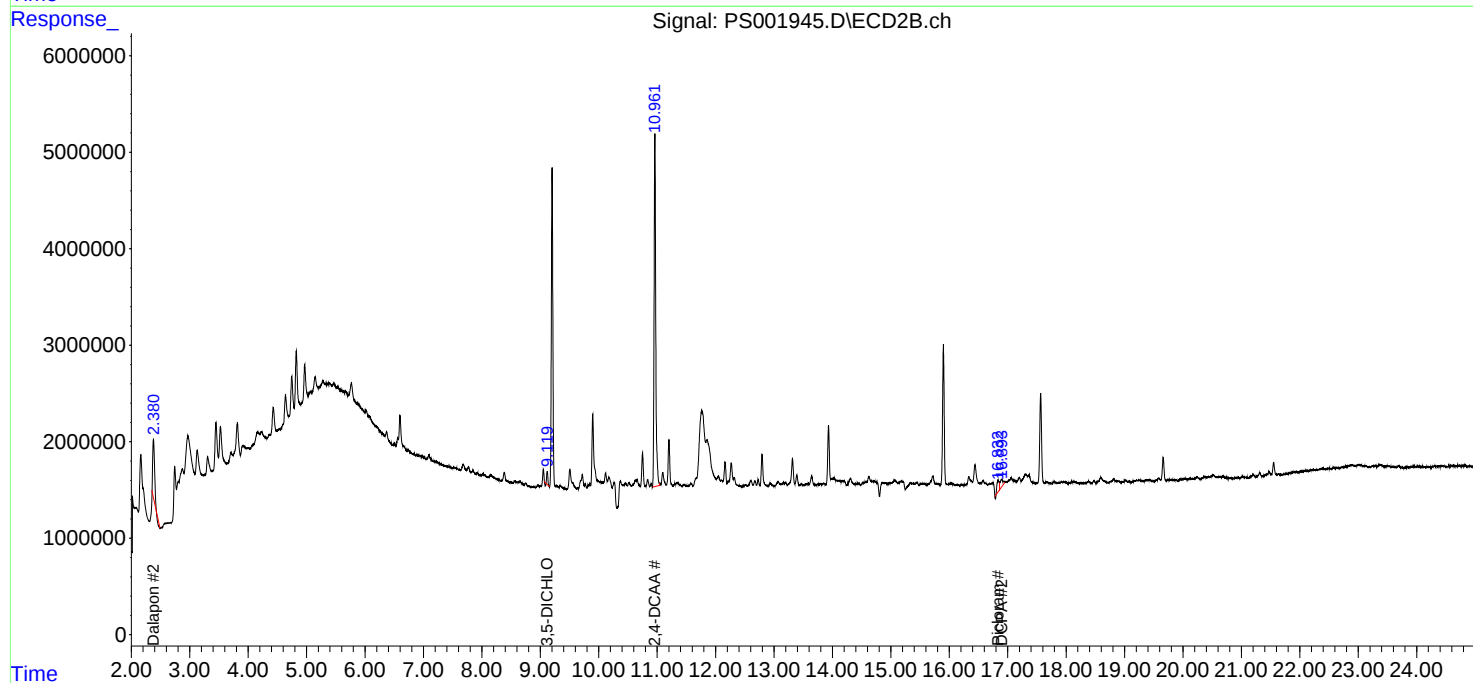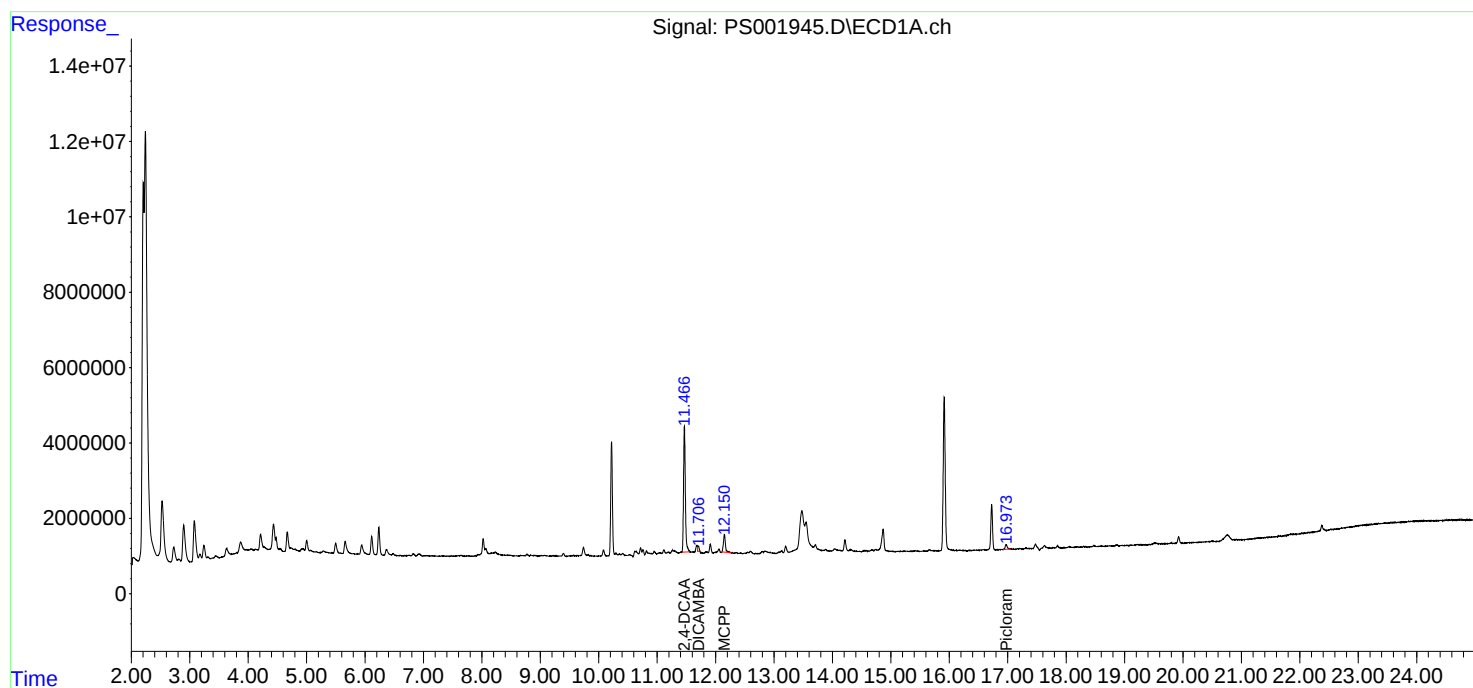


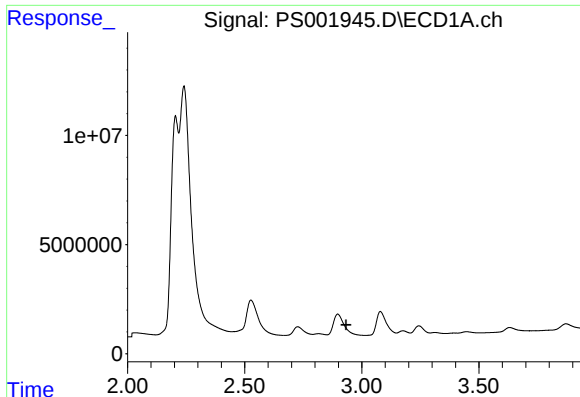

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.933 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

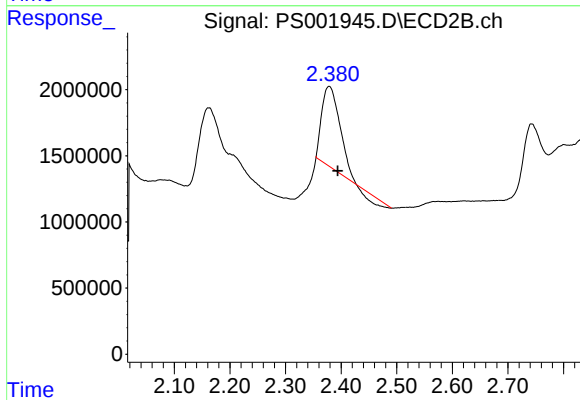


#1 Dalapon

R.T.: 2.379 min
Delta R.T.: -0.015 min
Response: 12492602
Conc: 42.29 ng/ml

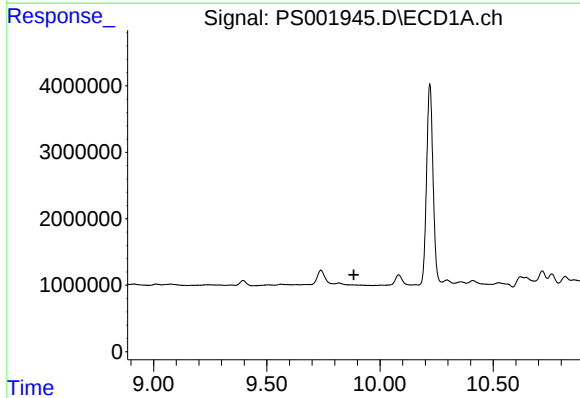


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.884 min
Response: 0
Conc: N.D.

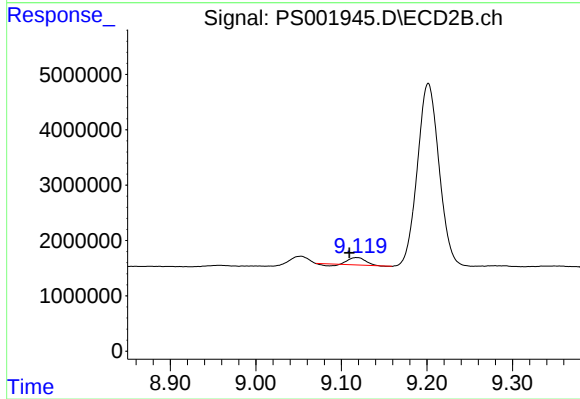

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.118 min
Delta R.T.: 0.009 min
Response: 1561006
Conc: 4.95 ng/ml

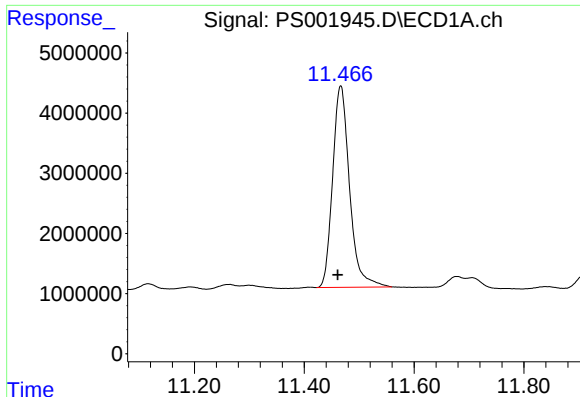

#4 2,4-DCAA


R.T.: 11.466 min
Delta R.T.: 0.005 min
Response: 71620142
Conc: 319.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

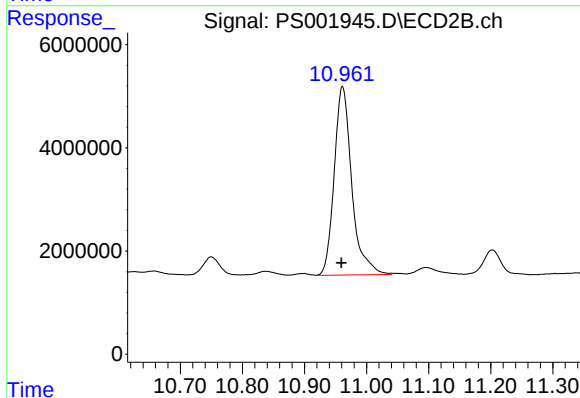


#4 2,4-DCAA

R.T.: 10.961 min
Delta R.T.: 0.002 min
Response: 71915961
Conc: 283.12 ng/ml

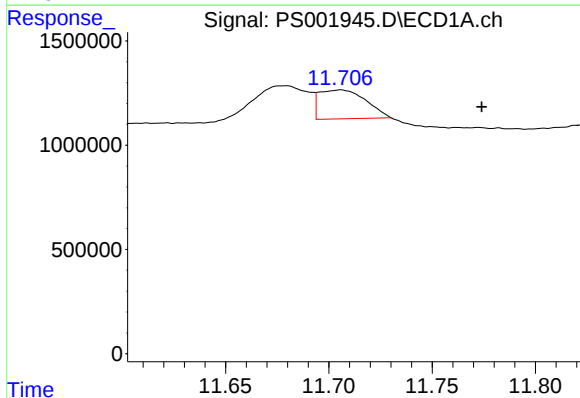


#5 DICAMBA

R.T.: 11.705 min
Delta R.T.: -0.069 min
Response: 2179711
Conc: 2.51 ng/ml

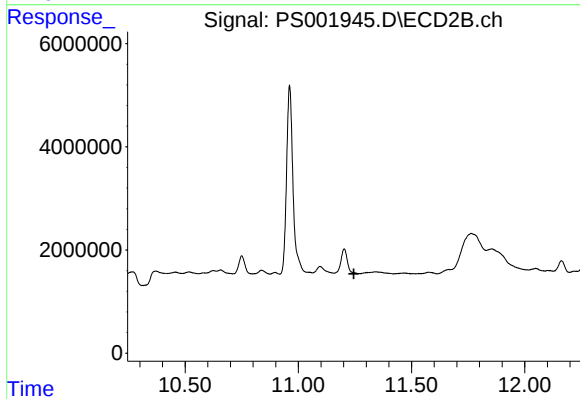

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.245 min
Response: 0
Conc: N.D.

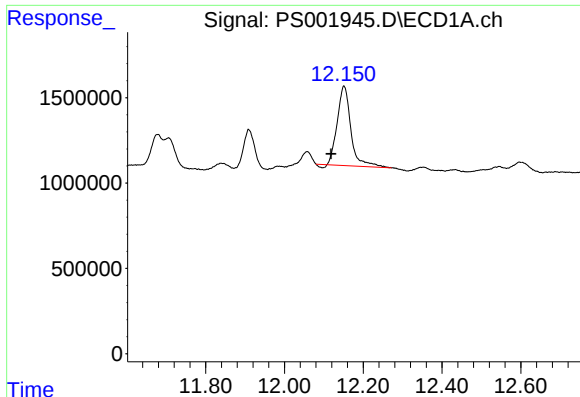

#6 MCPP


R.T.: 12.151 min
Delta R.T.: 0.033 min
Response: 11079314
Conc: 17.39 ug/ml

Instrument :
ECD_S
ClientSampleId :

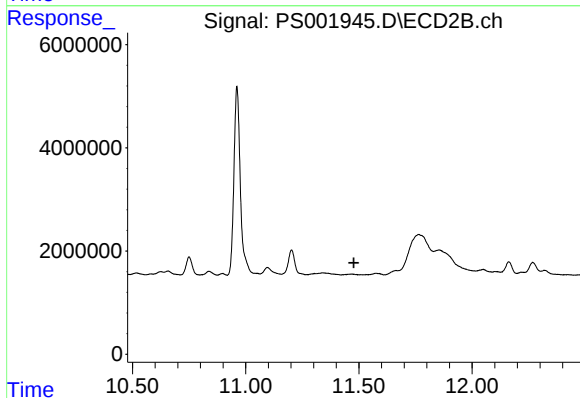


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

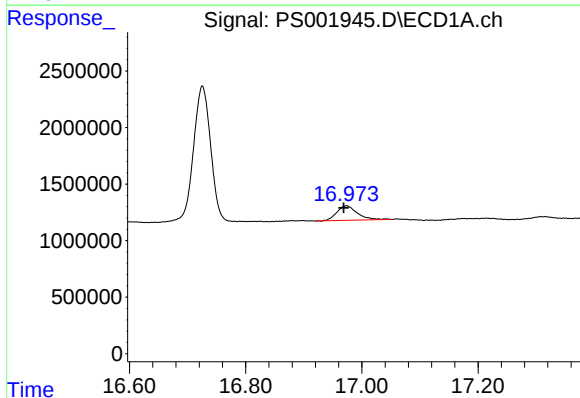


#15 Picloram

R.T.: 16.973 min
Delta R.T.: 0.005 min
Response: 3150220
Conc: 1.81 ng/ml

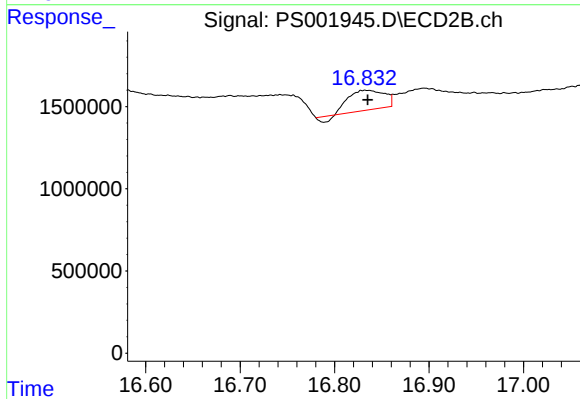

#15 Picloram


R.T.: 16.833 min
Delta R.T.: -0.002 min
Response: 2979985
Conc: 1.75 ng/ml

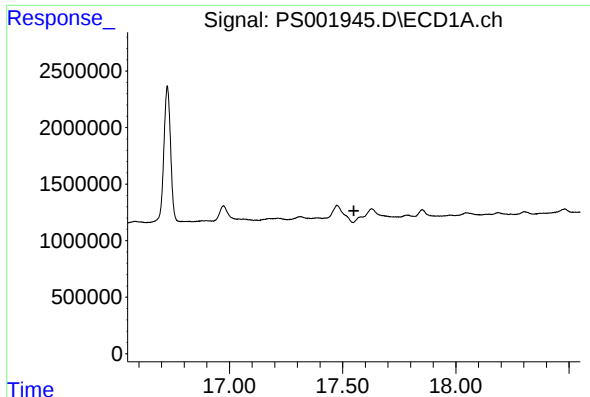

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

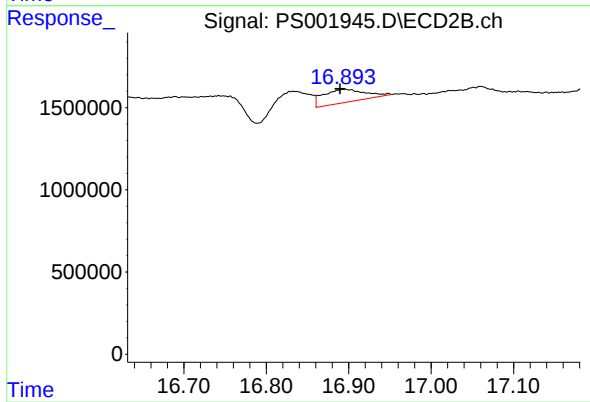

#16 DCPA

R.T.: 16.895 min
Delta R.T.: 0.006 min
Response: 2820167
Conc: 1.53 ng/ml