

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 15:35
 Operator : EI\SJ
 Sample : J5201-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-02-100818-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 03:46:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.464	10.960	111.9E6	110.1E6	499.006	433.271
Target Compounds							
1) T	Dalapon	0.000	2.378	0	21309574	N.D.	72.134 #
2) T	3,5-DICHL...	0.000	9.117	0	1885209	N.D.	5.973 #
3) T	4-Nitroph...	11.114	0.000	1648582	0	11.713	N.D. #
5) T	DICAMBA	11.704	0.000	2429123	0	2.803	N.D. #
6) T	MCP	12.151	0.000	19521908	0	30.635	N.D. #
9) T	2,4-D	0.000	12.794	0	4203226	N.D.	13.511 #
15) T	Picloram	0.000	16.835	0	4679971	N.D.	2.752 #
16) T	DCPA	0.000	16.893	0	3616037	N.D.	1.961 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 15:35
Operator : EI\SJ
Sample : J5201-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 03:46:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

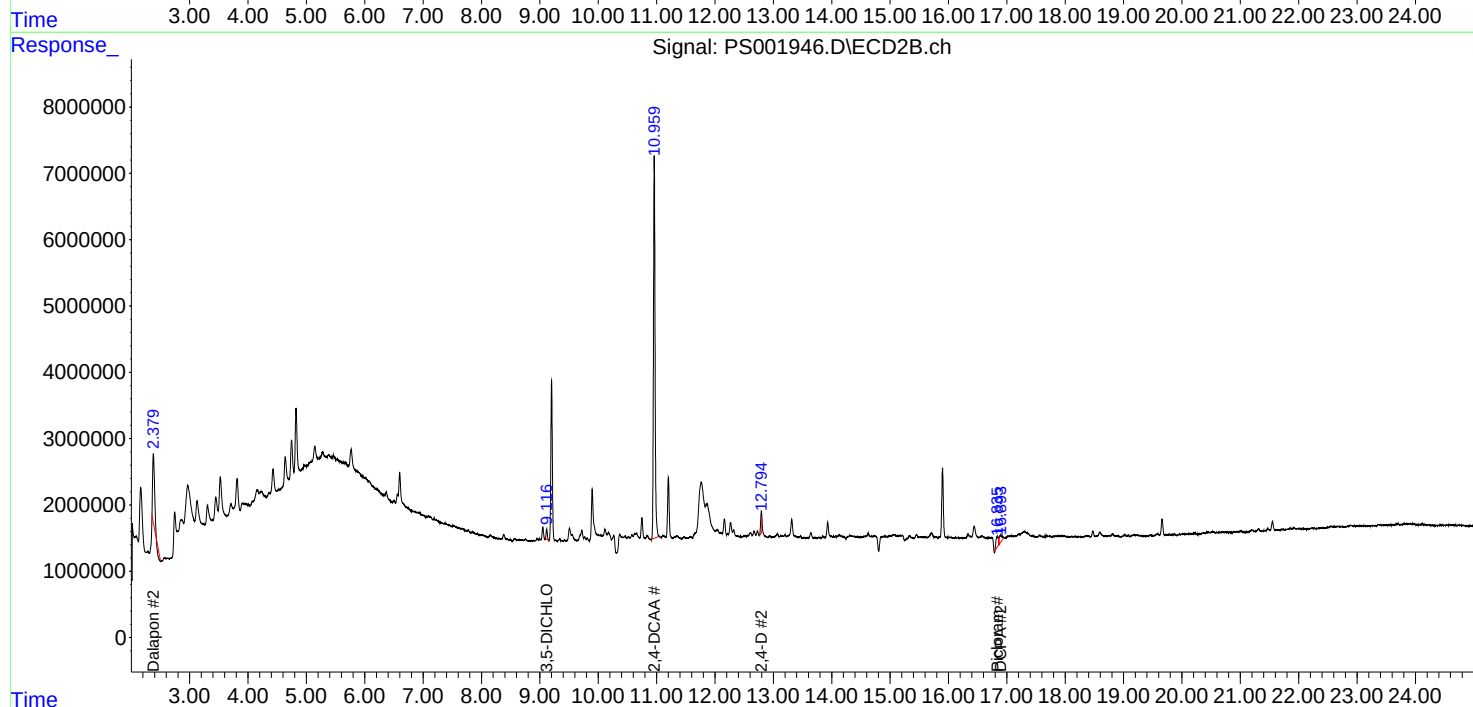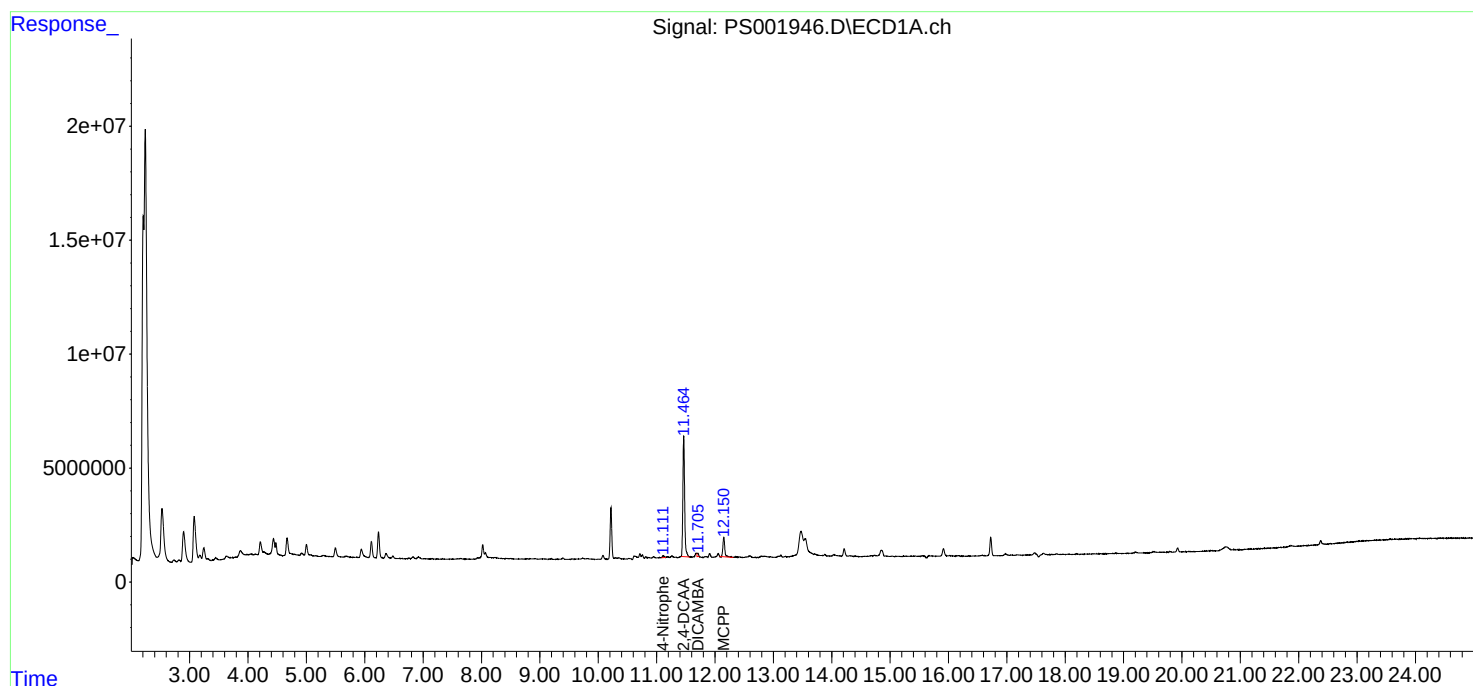


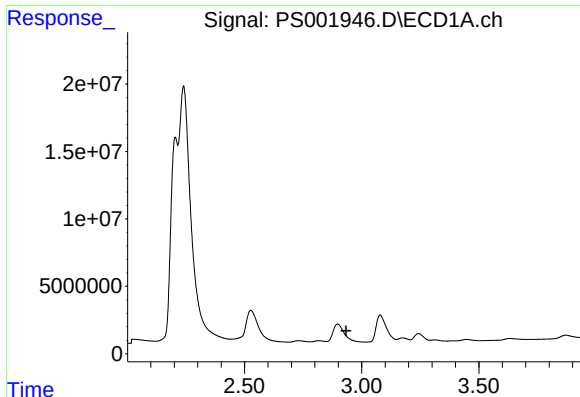

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.933 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-A

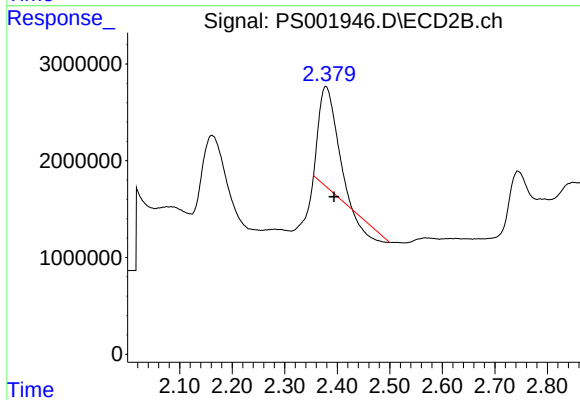


#1 Dalapon

R.T.: 2.378 min
Delta R.T.: -0.016 min
Response: 21309574
Conc: 72.13 ng/ml

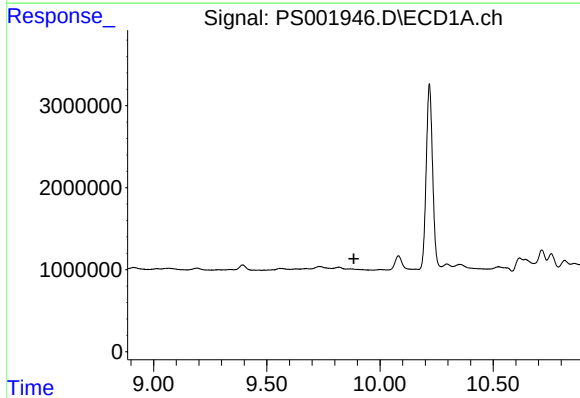


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.884 min
Response: 0
Conc: N.D.

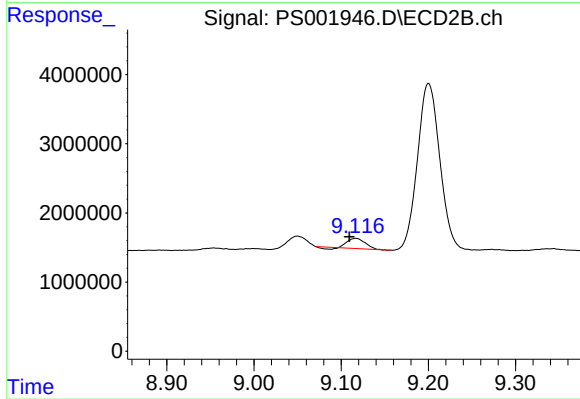

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.117 min
Delta R.T.: 0.007 min
Response: 1885209
Conc: 5.97 ng/ml

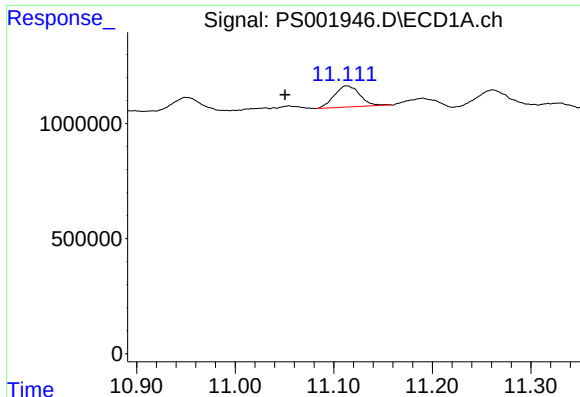

#3 4-Nitrophenol


R.T.: 11.114 min
Delta R.T.: 0.063 min
Response: 1648582
Conc: 11.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-A

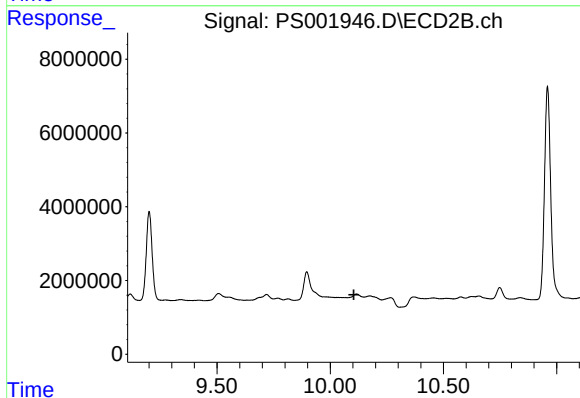


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.105 min
Response: 0
Conc: N.D.

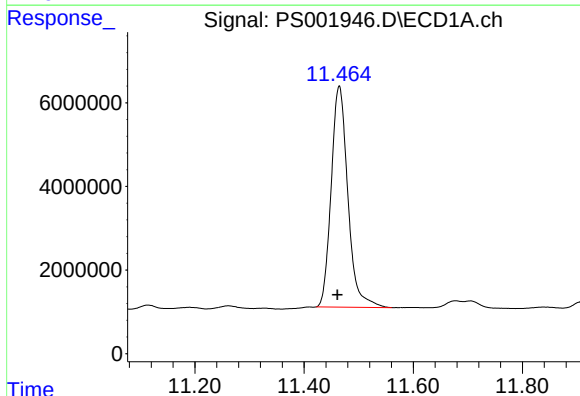


#4 2,4-DCAA

R.T.: 11.464 min
Delta R.T.: 0.003 min
Response: 111934783
Conc: 499.01 ng/ml

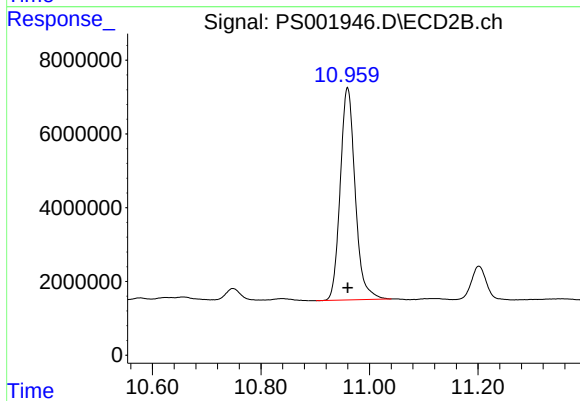

#4 2,4-DCAA


R.T.: 10.960 min
Delta R.T.: 0.000 min
Response: 110058164
Conc: 433.27 ng/ml

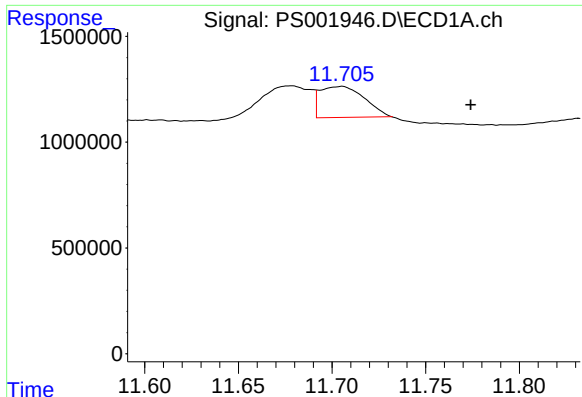

#5 DICAMBA


R.T.: 11.704 min
Delta R.T.: -0.070 min
Response: 2429123
Conc: 2.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-A

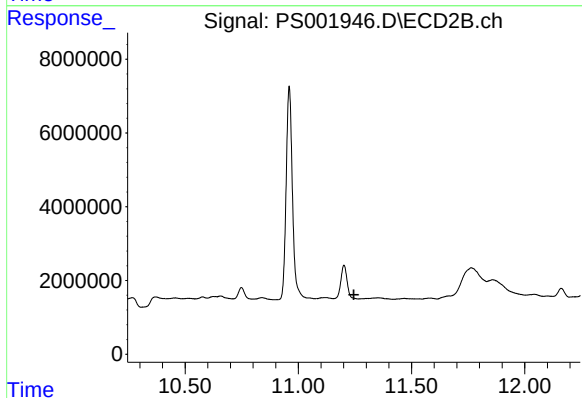


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.245 min
Response: 0
Conc: N.D.

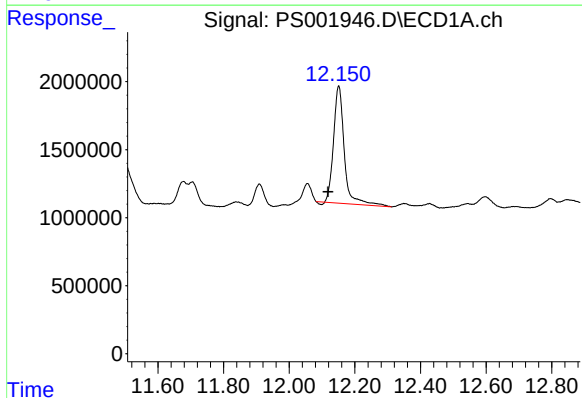


#6 MCP

R.T.: 12.151 min
Delta R.T.: 0.032 min
Response: 19521908
Conc: 30.64 ug/ml

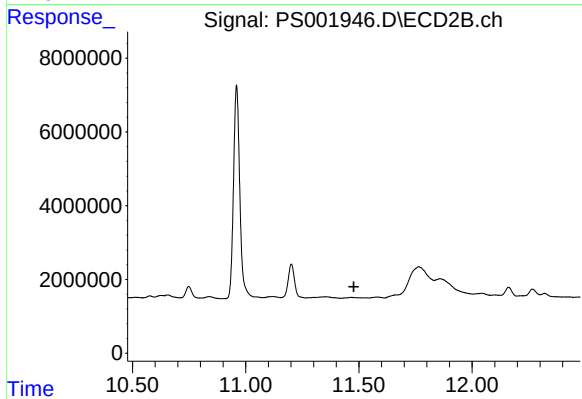

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

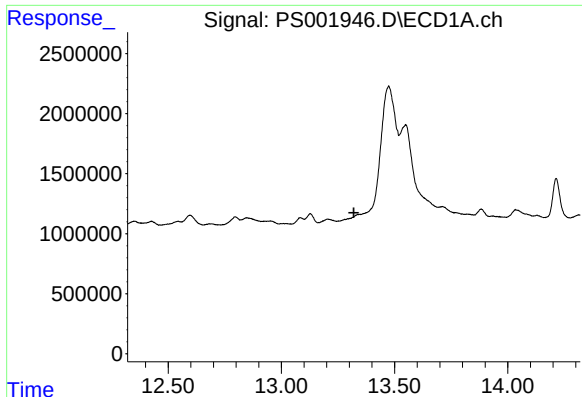

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-A

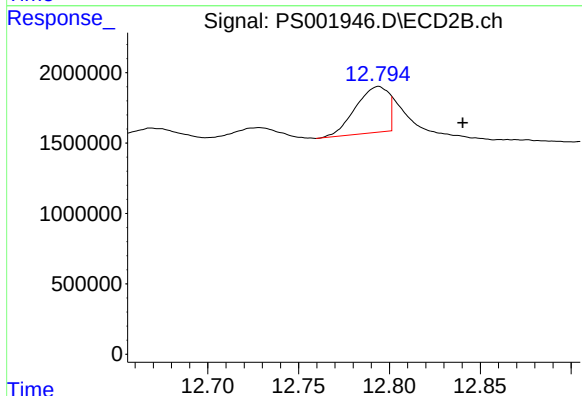


#9 2,4-D

R.T.: 12.794 min
Delta R.T.: -0.046 min
Response: 4203226
Conc: 13.51 ng/ml

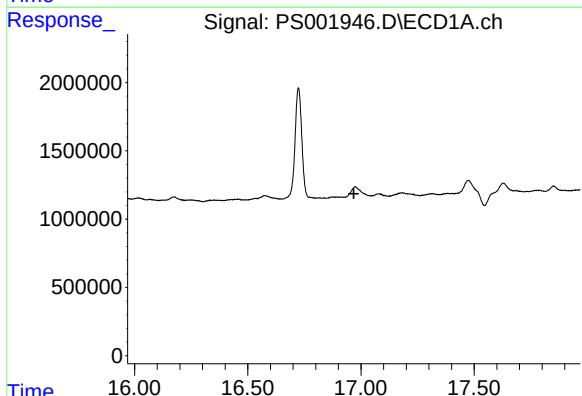


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.969 min
Response: 0
Conc: N.D.

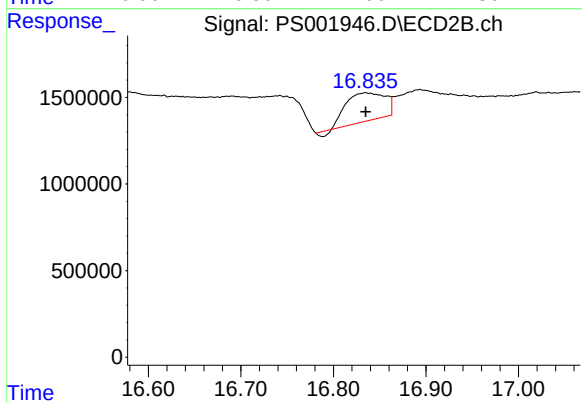

#15 Picloram


R.T.: 16.835 min
Delta R.T.: 0.000 min
Response: 4679971
Conc: 2.75 ng/ml

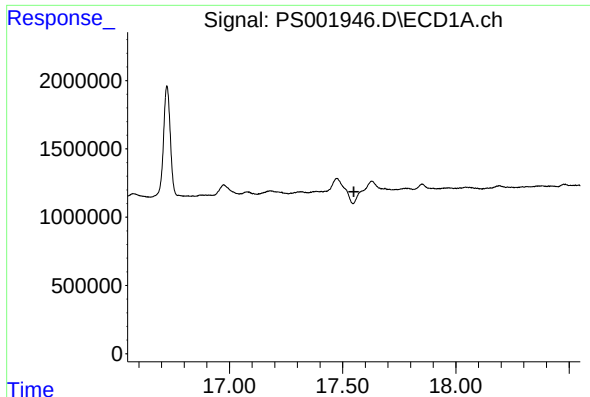

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-A

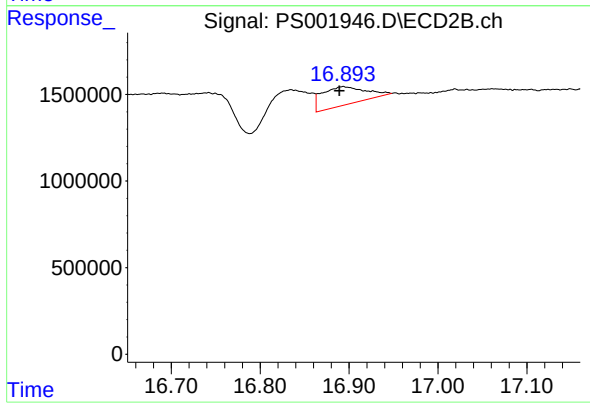

#16 DCPA

R.T.: 16.893 min
Delta R.T.: 0.004 min
Response: 3616037
Conc: 1.96 ng/ml