

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 16:36
 Operator : EI\SJ
 Sample : J5201-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-02-100818-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 03:47:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.449	10.944	63794014	83851690	284.394	330.103
Target Compounds							
1) T	Dalapon	2.881	0.000	5523903	0	16.988	N.D. #
2) T	3,5-DICHL...	0.000	9.101	0	2822999	N.D.	8.944 #
5) T	DICAMBA	0.000	11.186	0	3472122	N.D.	3.893 #
6) T	MCP	12.133	0.000	10240678	0	16.070	N.D. #
9) T	2,4-D	0.000	12.777	0	5637770	N.D.	18.122 #
15) T	Picloram	0.000	16.817	0	3989944	N.D.	2.346 #
16) T	DCPA	0.000	16.876	0	2188139	N.D.	1.186 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 16:36
Operator : EI\SJ
Sample : J5201-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 03:47:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

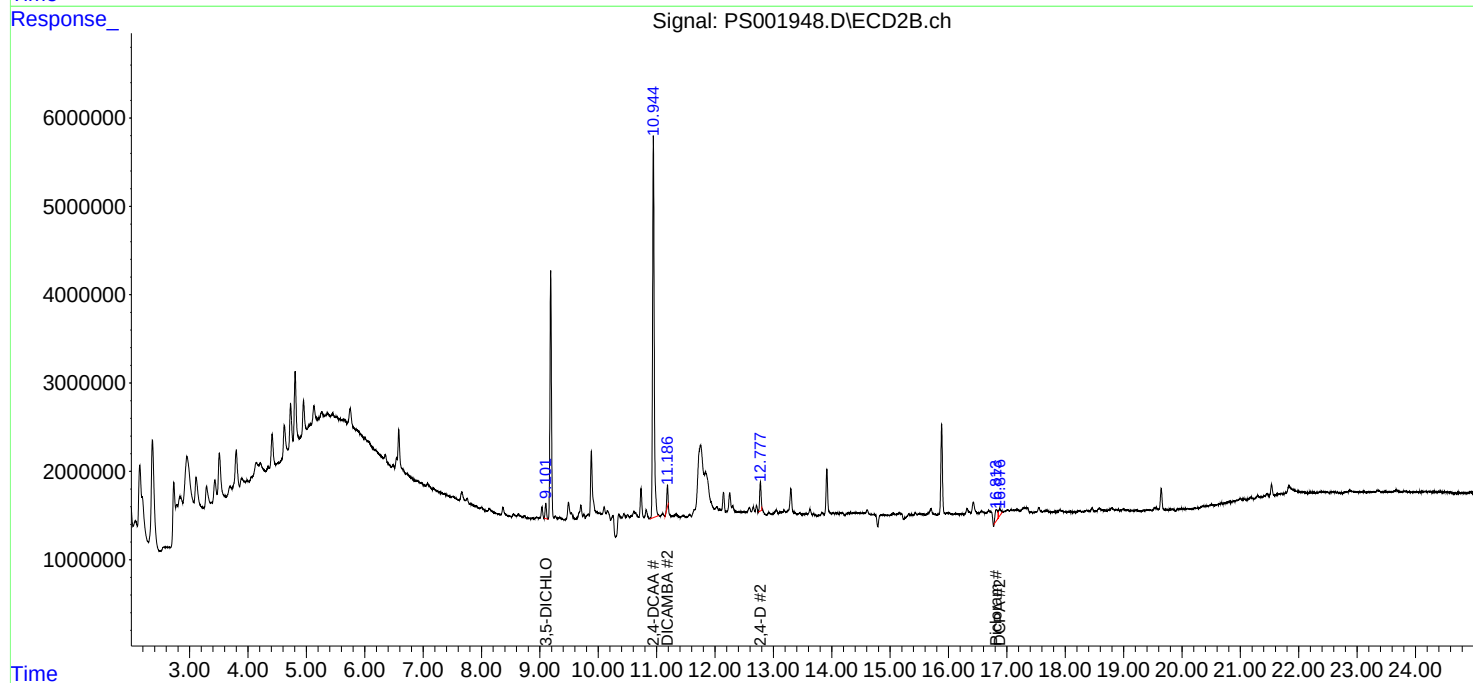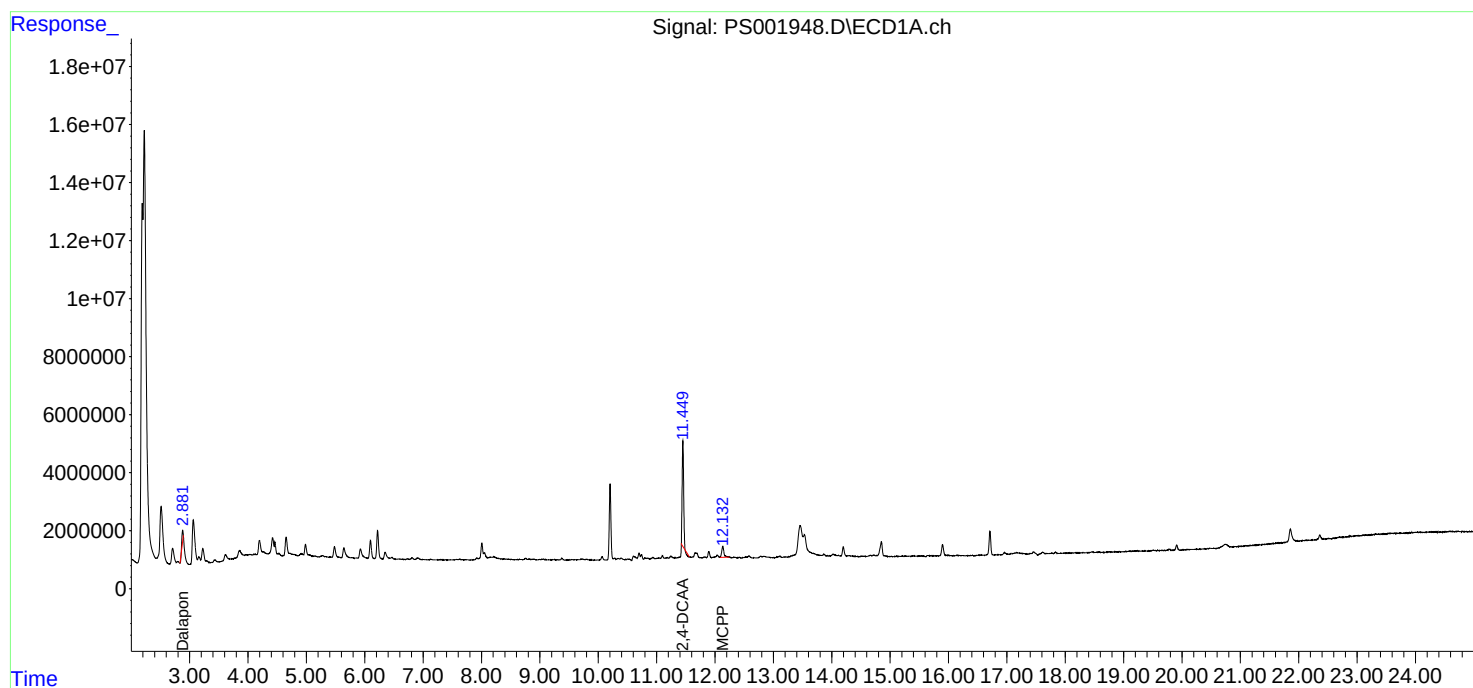


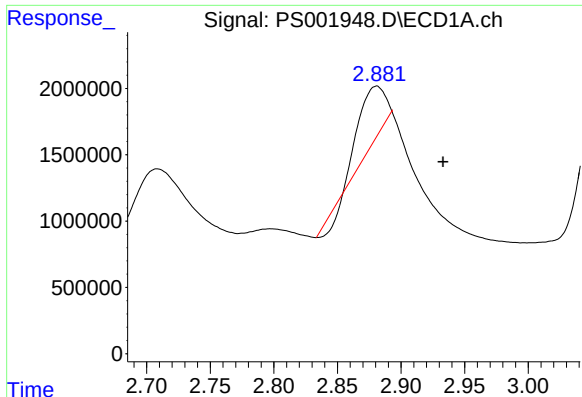

#1 Dalapon


R.T.: 2.881 min
Delta R.T.: -0.052 min
Response: 5523903
Conc: 16.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-B

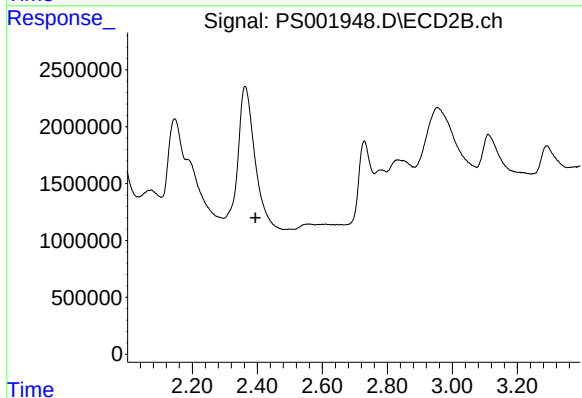


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.394 min
Response: 0
Conc: N.D.

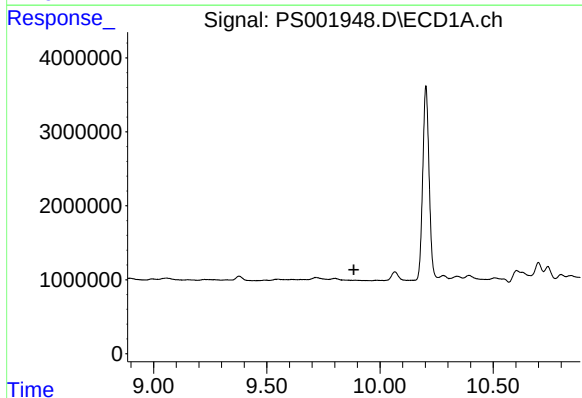


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.884 min
Response: 0
Conc: N.D.

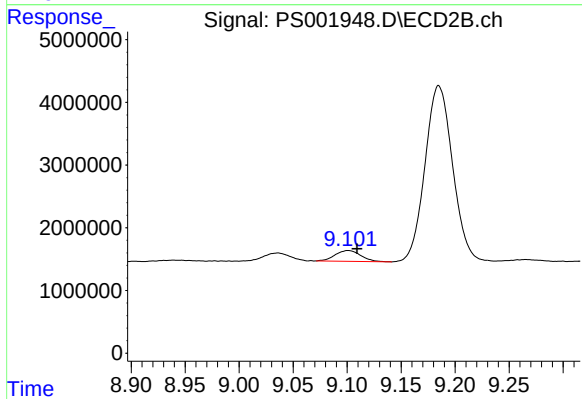

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.101 min
Delta R.T.: -0.008 min
Response: 2822999
Conc: 8.94 ng/ml

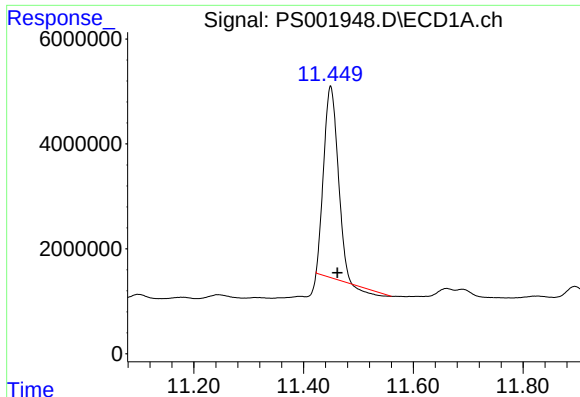

#4 2,4-DCAA


R.T.: 11.449 min
Delta R.T.: -0.012 min
Response: 63794014
Conc: 284.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-B

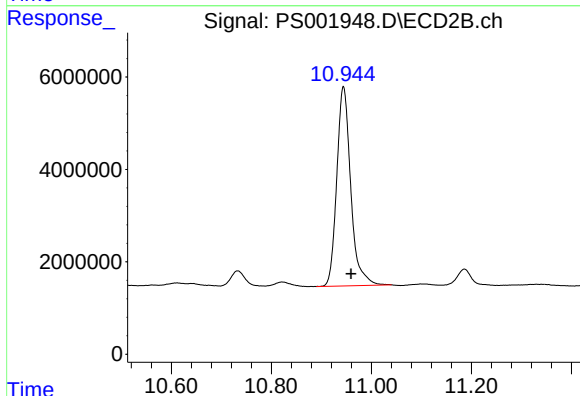


#4 2,4-DCAA

R.T.: 10.944 min
Delta R.T.: -0.015 min
Response: 83851690
Conc: 330.10 ng/ml

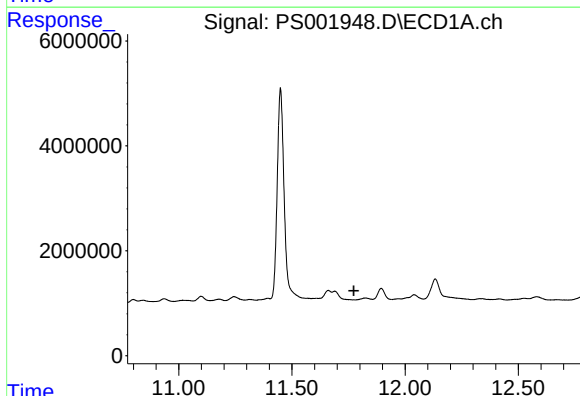


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.774 min
Response: 0
Conc: N.D.

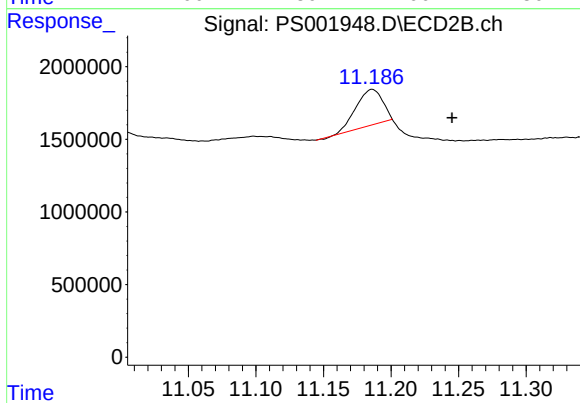

#5 DICAMBA


R.T.: 11.186 min
Delta R.T.: -0.059 min
Response: 3472122
Conc: 3.89 ng/ml

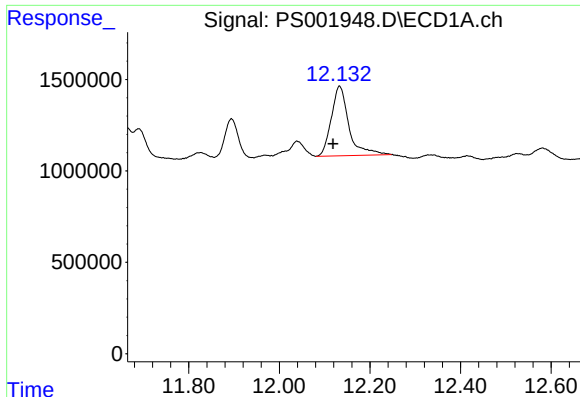

#6 MCP


R.T.: 12.133 min
Delta R.T.: 0.014 min
Response: 10240678
Conc: 16.07 ug/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-B

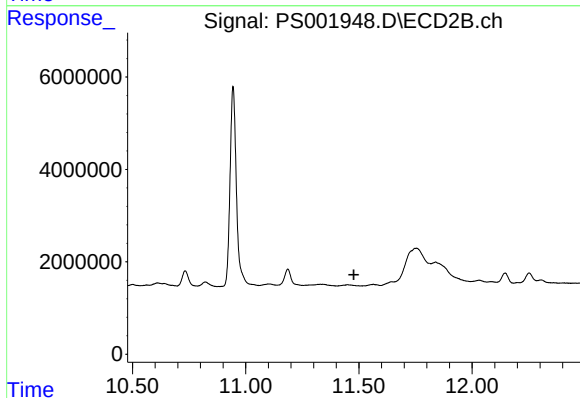


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

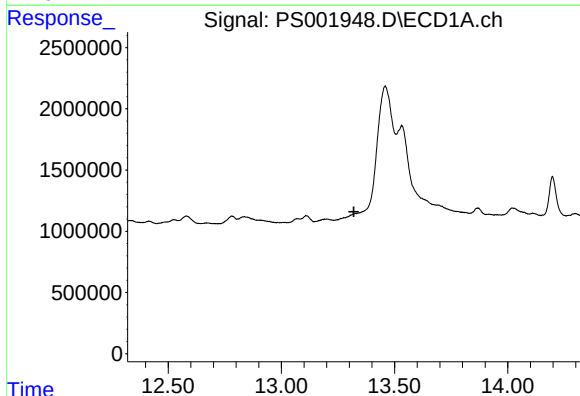


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.320 min
Response: 0
Conc: N.D.

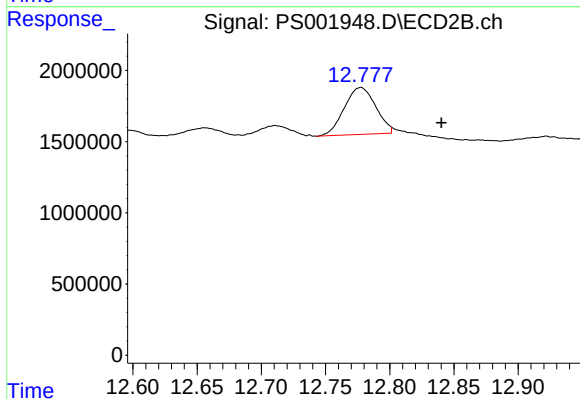

#9 2,4-D


R.T.: 12.777 min
Delta R.T.: -0.063 min
Response: 5637770
Conc: 18.12 ng/ml

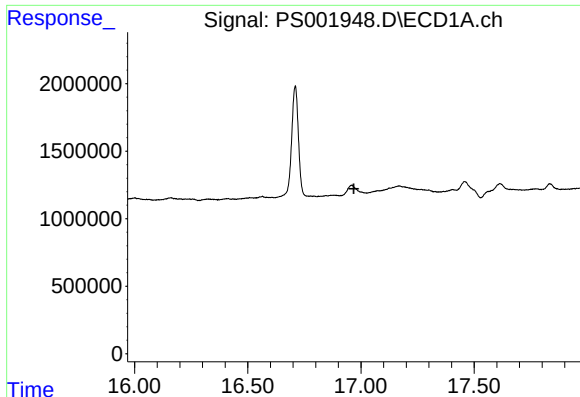

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-B

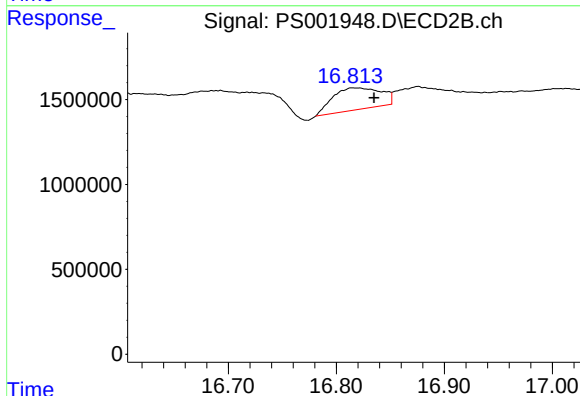


#15 Picloram

R.T.: 16.817 min
Delta R.T.: -0.018 min
Response: 3989944
Conc: 2.35 ng/ml

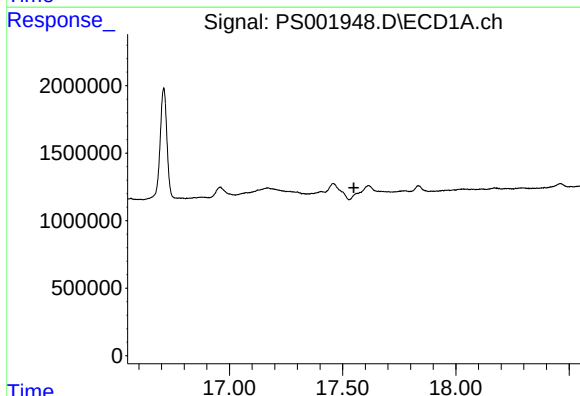

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.549 min
Response: 0
Conc: N.D.

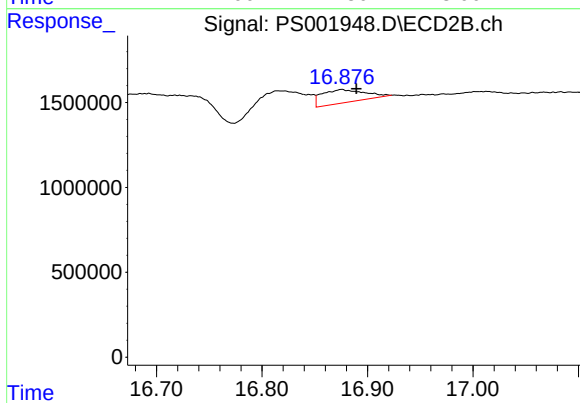

#16 DCPA

R.T.: 16.876 min
Delta R.T.: -0.014 min
Response: 2188139
Conc: 1.19 ng/ml