

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 18:40
 Operator : EI\SJ
 Sample : J5200-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 03:47:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.476	10.970	64168515	65335086	286.064	257.208
Target Compounds							
1) T	Dalapon	2.908	2.389	-973154	32115129	N.D.	108.711
2) T	3,5-DICHL...	0.000	9.127	0	1452797	N.D.	4.603 #
6) T	MCP	12.161	0.000	7538609	0	11.830	N.D. #
10) T	Pentachlo...	0.000	13.324	0	1203451	N.D.	0.351 #
11) T	2,4,5-TP ...	0.000	13.941	0	7035861	N.D.	5.131 #
15) T	Picloram	0.000	16.844	0	523492	N.D.	0.308 #
16) T	DCPA	0.000	16.906	0	2270398	N.D.	1.231 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 18:40
Operator : EI\SJ
Sample : J5200-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 03:47:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

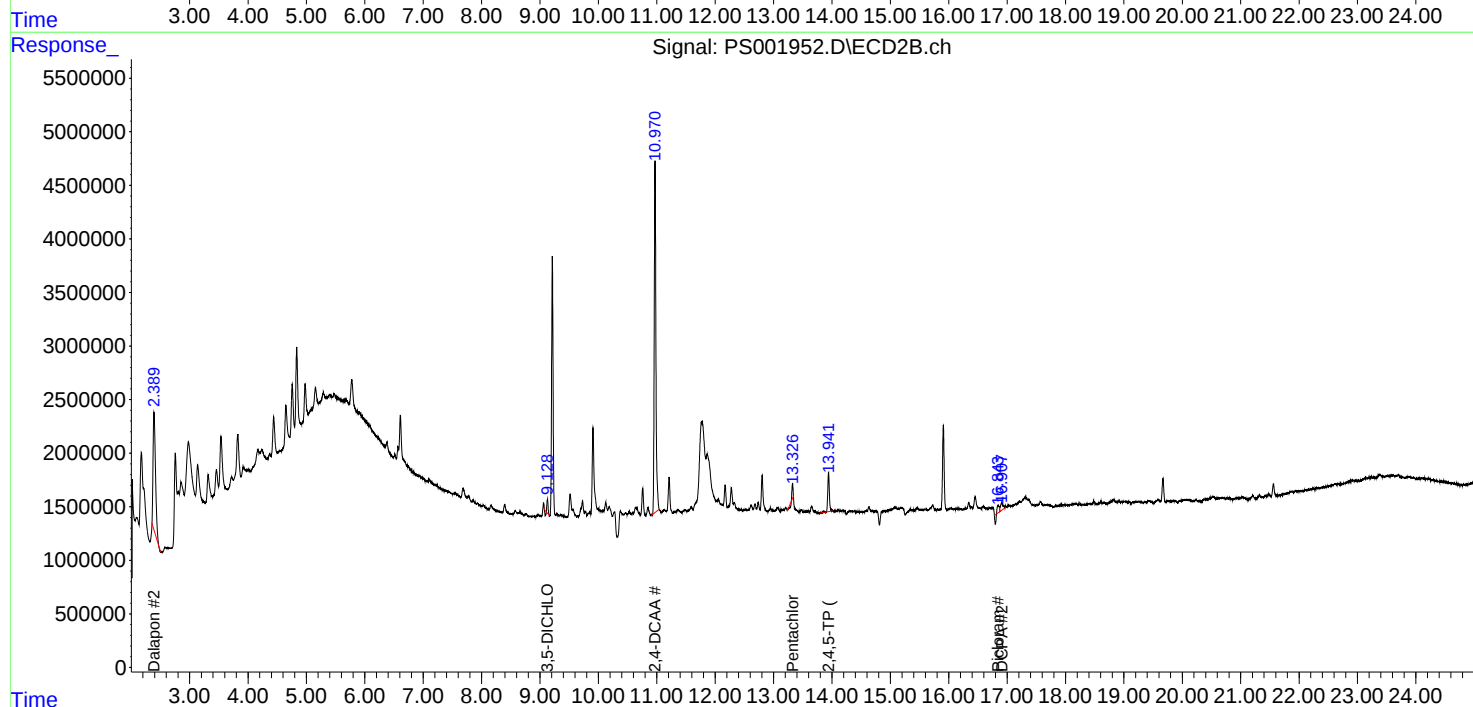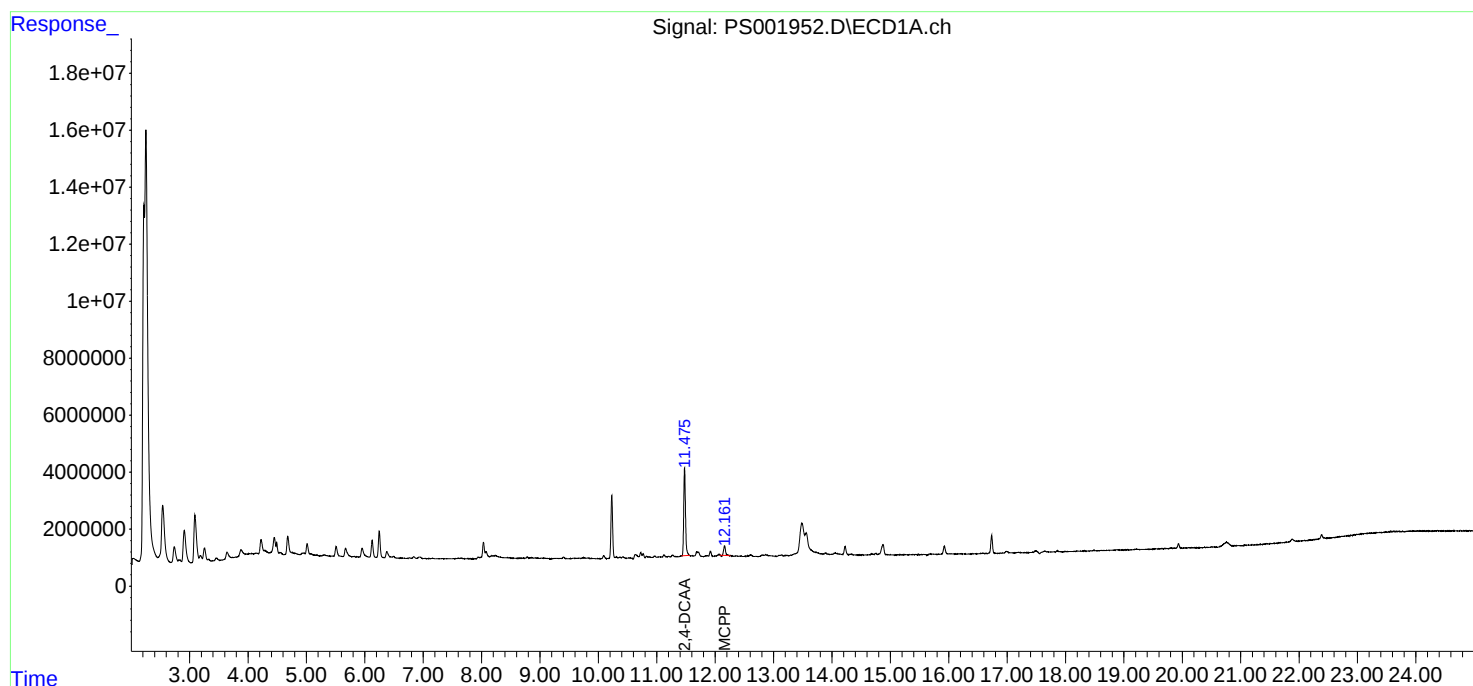


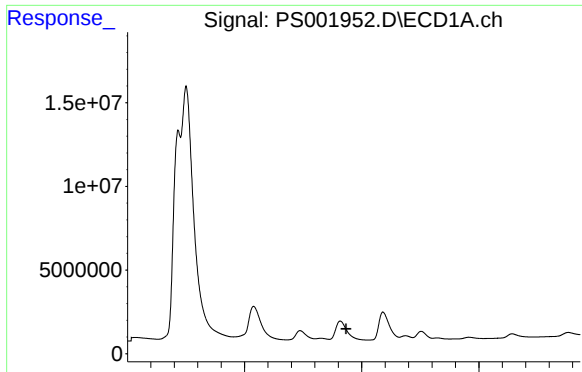

#1 Dalapon


R.T.: 2.908 min
Delta R.T.: -0.025 min
Response: -973154
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

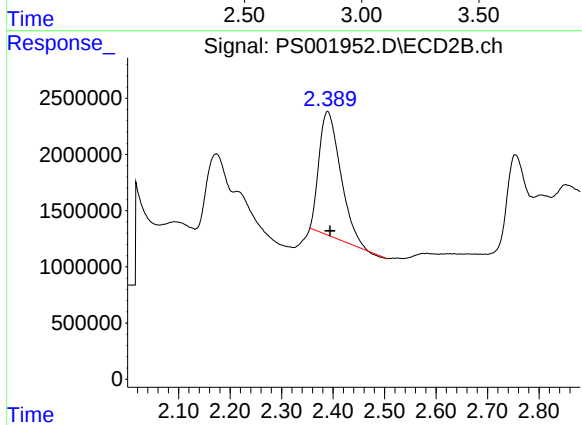


#1 Dalapon

R.T.: 2.389 min
Delta R.T.: -0.005 min
Response: 32115129
Conc: 108.71 ng/ml

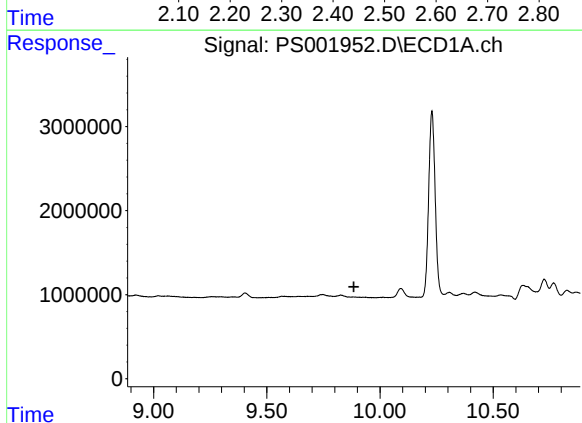


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.884 min
Response: 0
Conc: N.D.

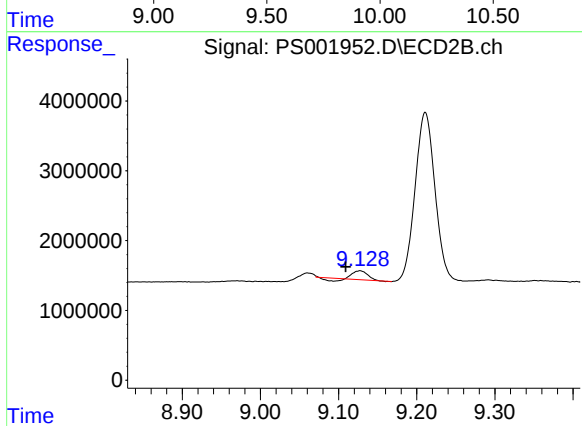

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.127 min
Delta R.T.: 0.018 min
Response: 1452797
Conc: 4.60 ng/ml

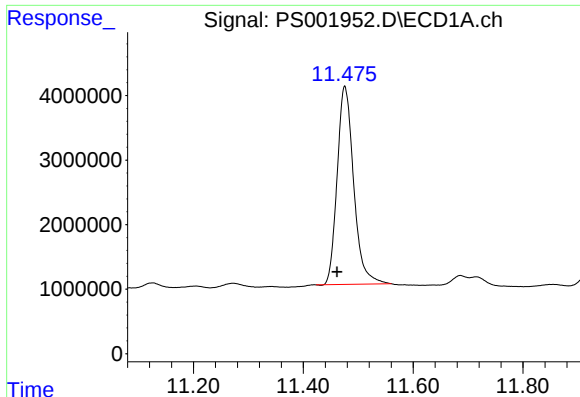

#4 2,4-DCAA


R.T.: 11.476 min
Delta R.T.: 0.014 min
Response: 64168515
Conc: 286.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

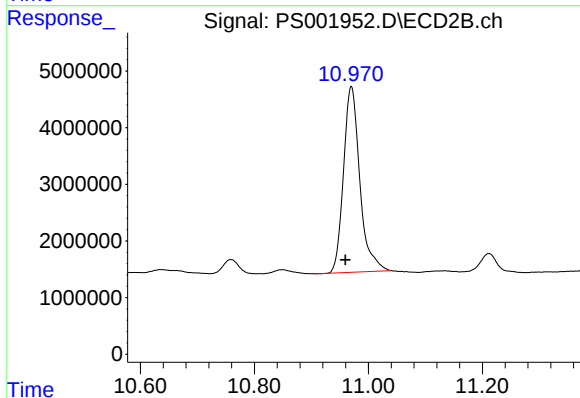


#4 2,4-DCAA

R.T.: 10.970 min
Delta R.T.: 0.010 min
Response: 65335086
Conc: 257.21 ng/ml

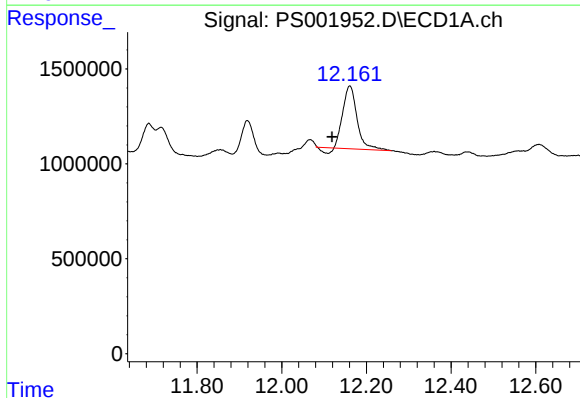


#6 MCP

R.T.: 12.161 min
Delta R.T.: 0.042 min
Response: 7538609
Conc: 11.83 ug/ml

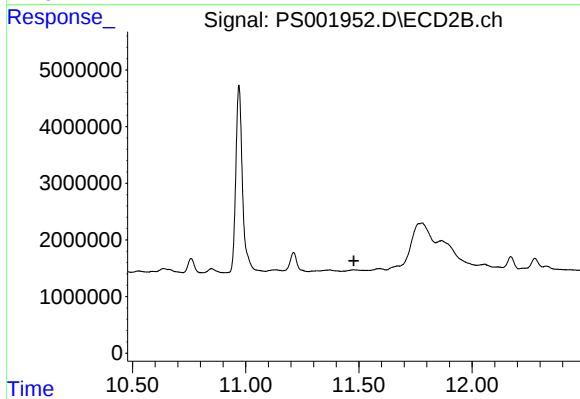

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.478 min
Response: 0
Conc: N.D.

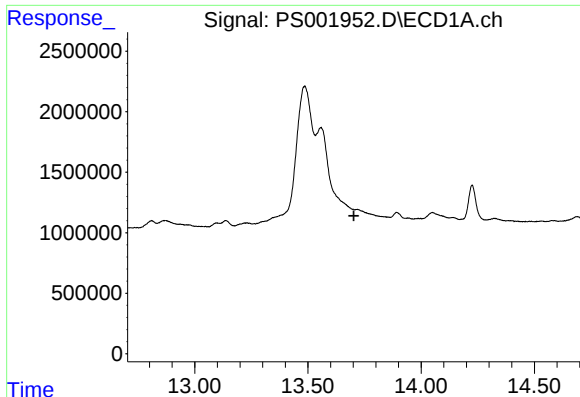

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.703 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

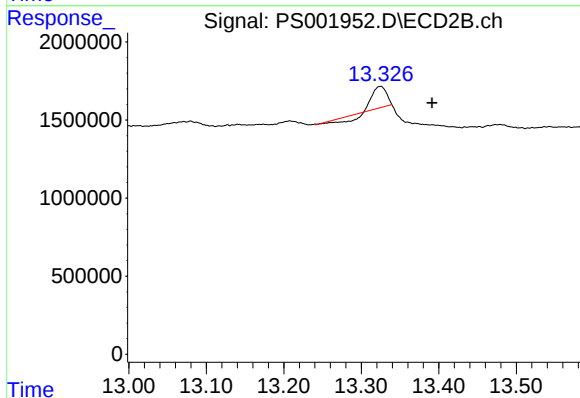


#10 Pentachlorophenol

R.T.: 13.324 min
Delta R.T.: -0.067 min
Response: 1203451
Conc: 0.35 ng/ml

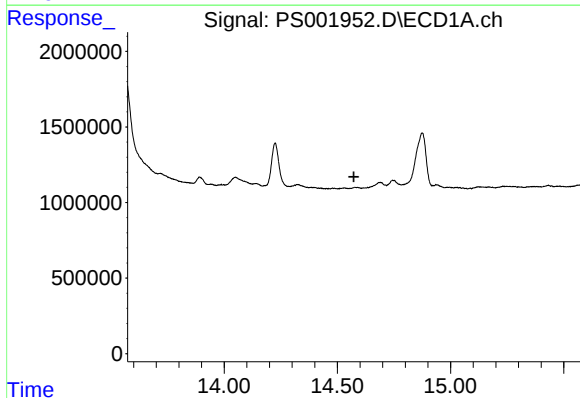


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.573 min
Response: 0
Conc: N.D.

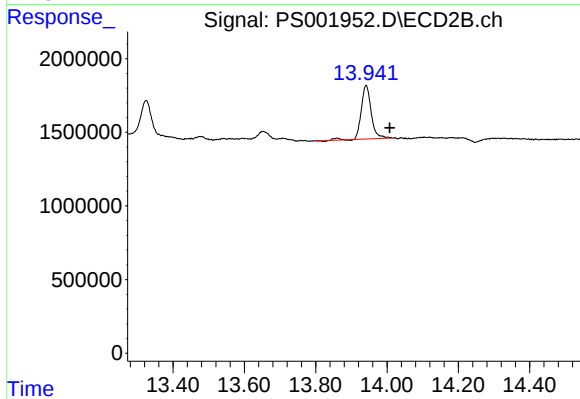

#11 2,4,5-TP (SILVEX)


R.T.: 13.941 min
Delta R.T.: -0.067 min
Response: 7035861
Conc: 5.13 ng/ml

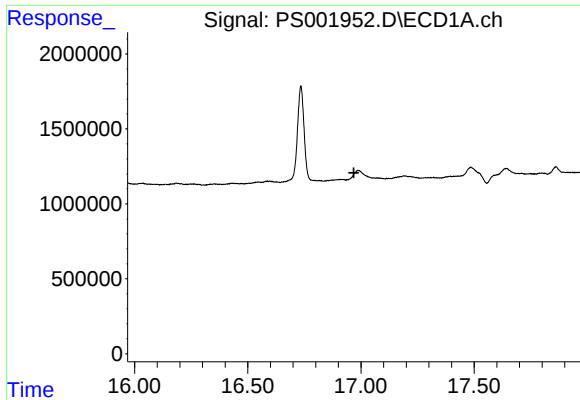

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

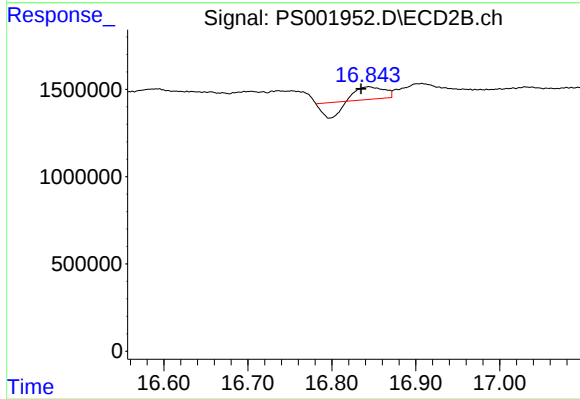


#15 Picloram

R.T.: 16.844 min
Delta R.T.: 0.009 min
Response: 523492
Conc: 0.31 ng/ml

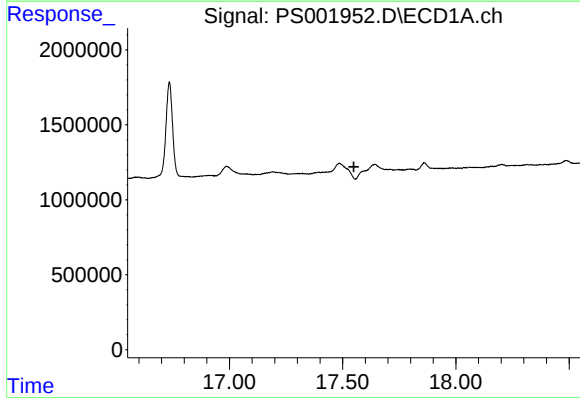

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.549 min
Response: 0
Conc: N.D.

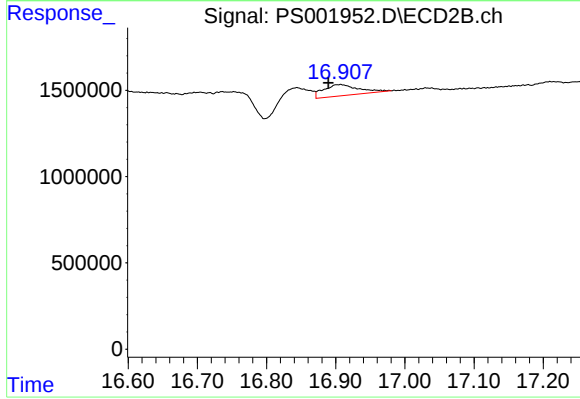

#16 DCPA

R.T.: 16.906 min
Delta R.T.: 0.017 min
Response: 2270398
Conc: 1.23 ng/ml