

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 19:42
 Operator : EI\SJ
 Sample : J5200-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 03:48:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.467	10.945	81252186	81899032	362.223	322.416
Target Compounds							
2) T	3,5-DICHL...	0.000	9.101	0	2661966	N.D.	8.434 #
3) T	4-Nitroph...	11.116	0.000	2171453	0	15.428	N.D. #
5) T	DICAMBA	0.000	11.186	0	3792490	N.D.	4.252 #
6) T	MCP	12.151	0.000	10712827	0	16.811	N.D. #
9) T	2,4-D	0.000	12.778	0	5849258	N.D.	18.801 #
15) T	Picloram	16.973	16.818	2501086	3685419	1.436	2.167 #
16) T	DCPA	0.000	16.876	0	1710336	N.D.	0.927 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 19:42
Operator : EI\SJ
Sample : J5200-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 03:48:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

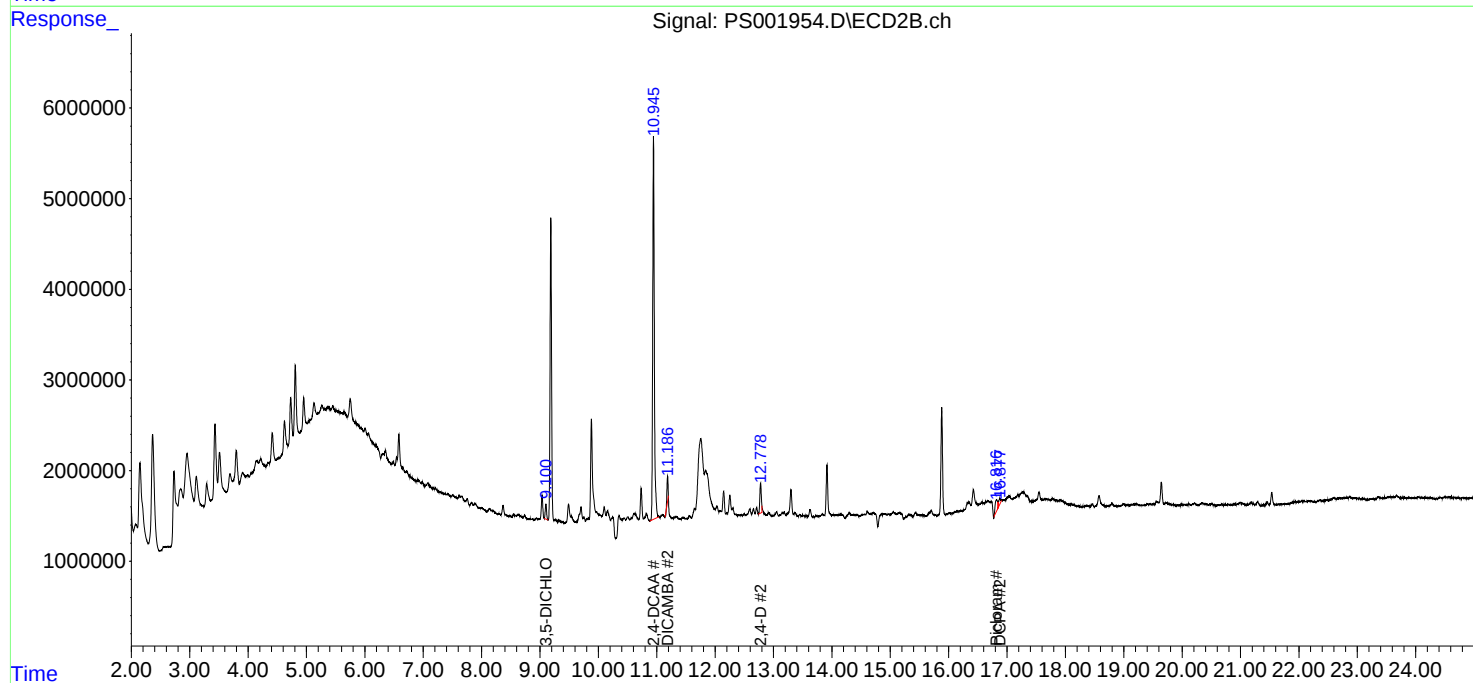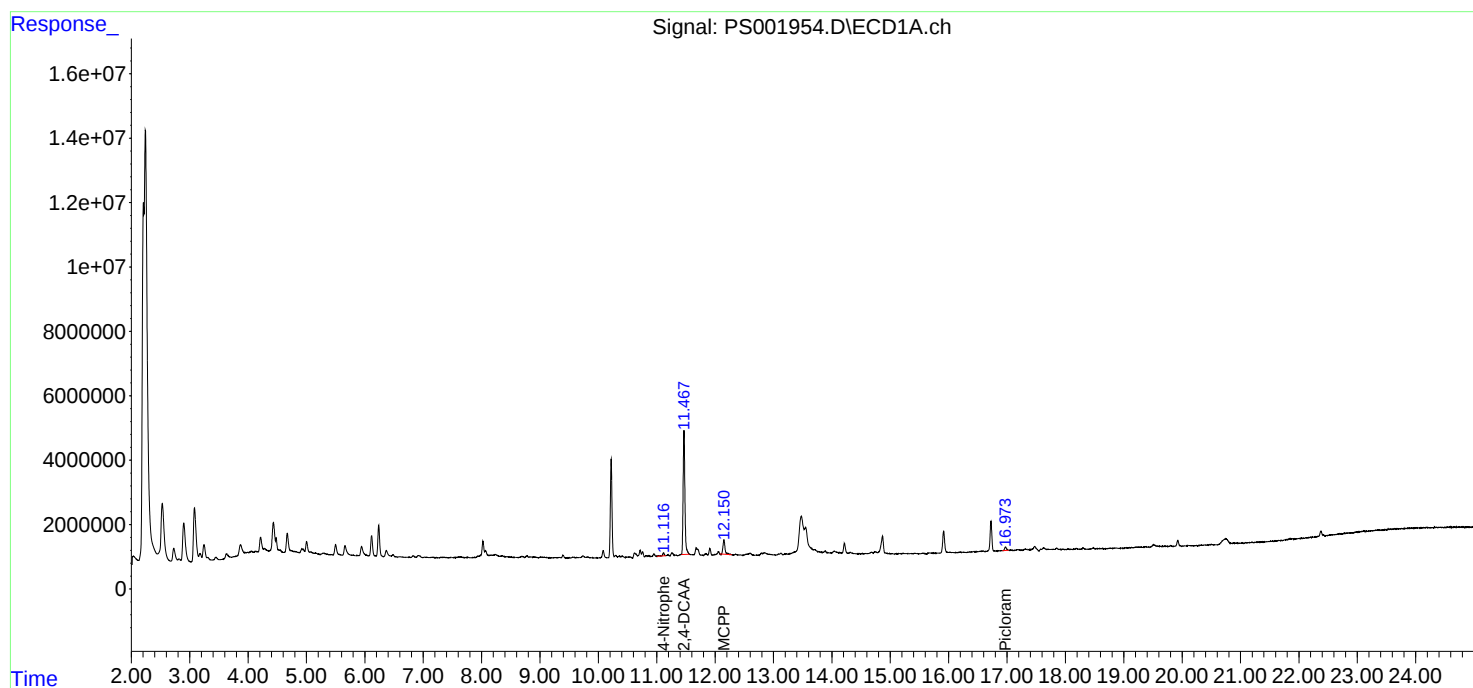


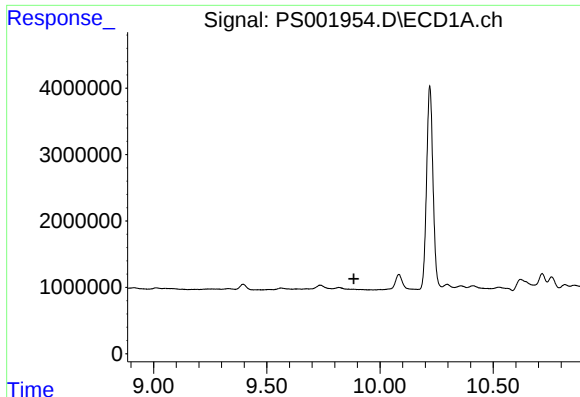

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.884 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

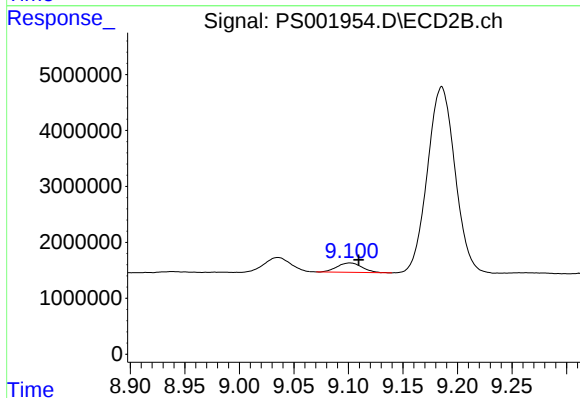


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.101 min
Delta R.T.: -0.008 min
Response: 2661966
Conc: 8.43 ng/ml

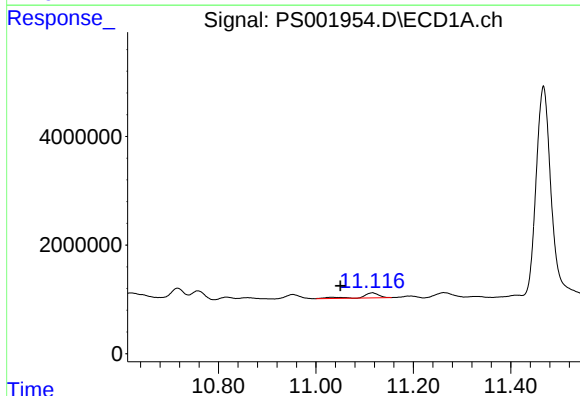


#3 4-Nitrophenol

R.T.: 11.116 min
Delta R.T.: 0.065 min
Response: 2171453
Conc: 15.43 ng/ml

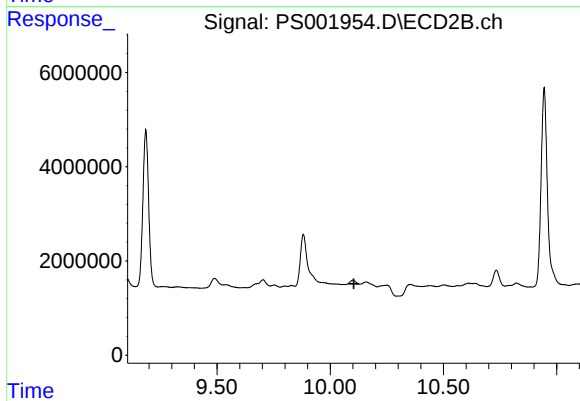

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.105 min
Response: 0
Conc: N.D.

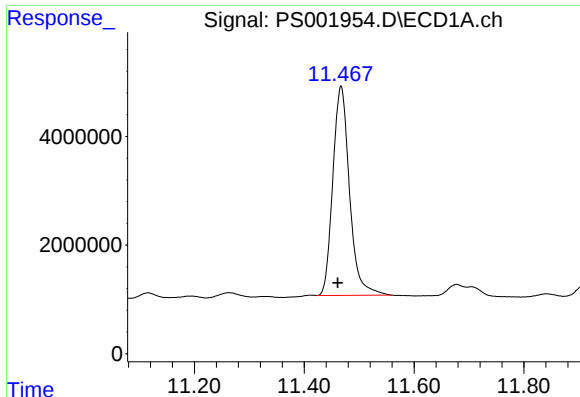

#4 2,4-DCAA


R.T.: 11.467 min
Delta R.T.: 0.006 min
Response: 81252186
Conc: 362.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

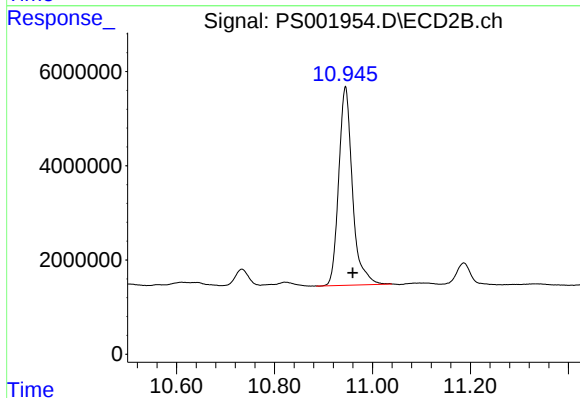


#4 2,4-DCAA

R.T.: 10.945 min
Delta R.T.: -0.015 min
Response: 81899032
Conc: 322.42 ng/ml

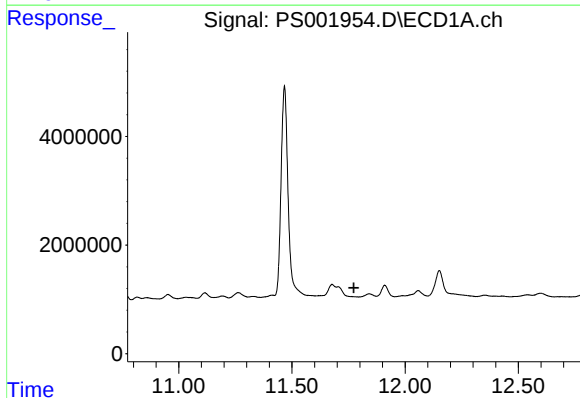


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.774 min
Response: 0
Conc: N.D.

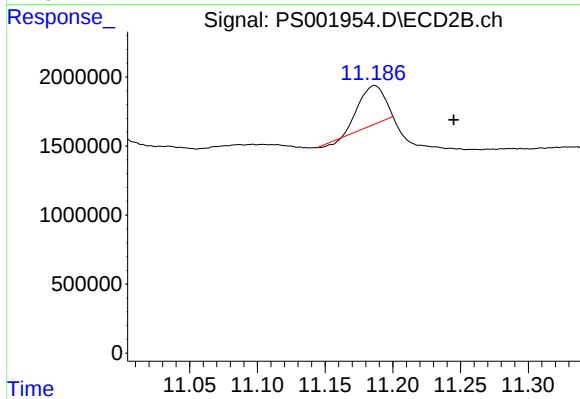

#5 DICAMBA


R.T.: 11.186 min
Delta R.T.: -0.059 min
Response: 3792490
Conc: 4.25 ng/ml

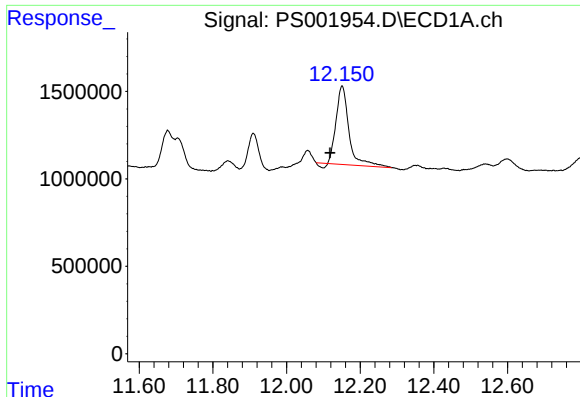

#6 MCP


R.T.: 12.151 min
Delta R.T.: 0.032 min
Response: 10712827
Conc: 16.81 ug/ml

Instrument :
ECD_S
ClientSampleId :

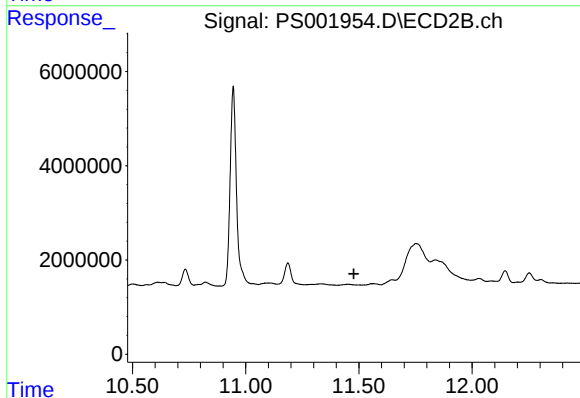


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

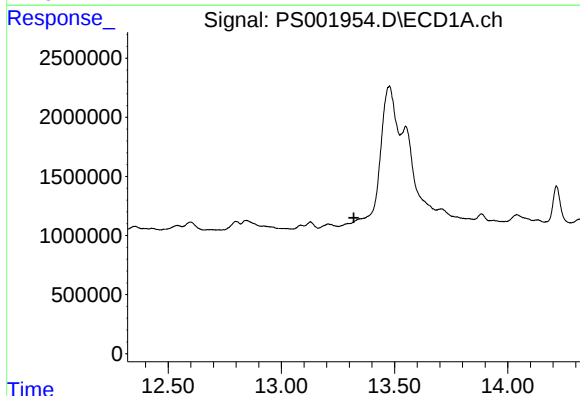


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.320 min
Response: 0
Conc: N.D.

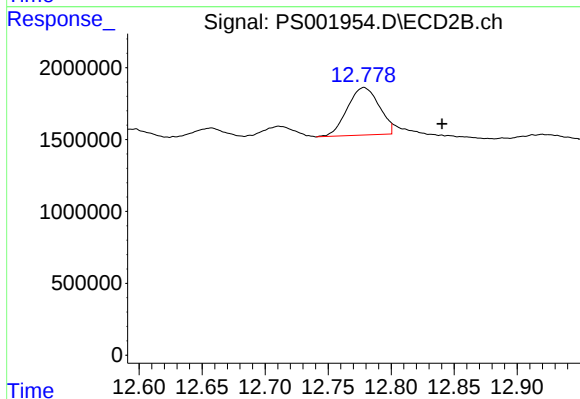

#9 2,4-D


R.T.: 12.778 min
Delta R.T.: -0.062 min
Response: 5849258
Conc: 18.80 ng/ml

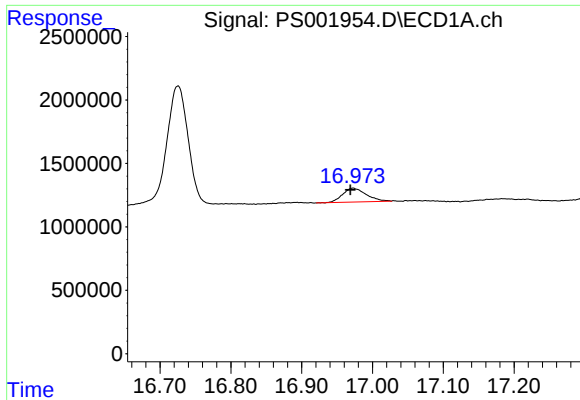

#15 Picloram


R.T.: 16.973 min
Delta R.T.: 0.004 min
Response: 2501086
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

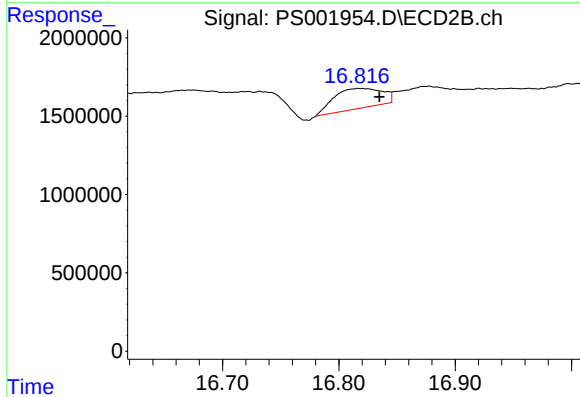


#15 Picloram

R.T.: 16.818 min
Delta R.T.: -0.017 min
Response: 3685419
Conc: 2.17 ng/ml

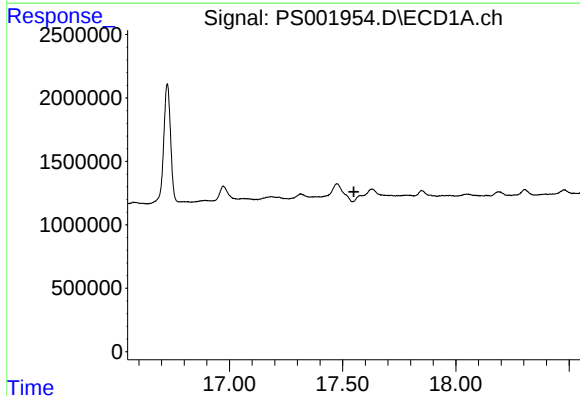

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.549 min
Response: 0
Conc: N.D.

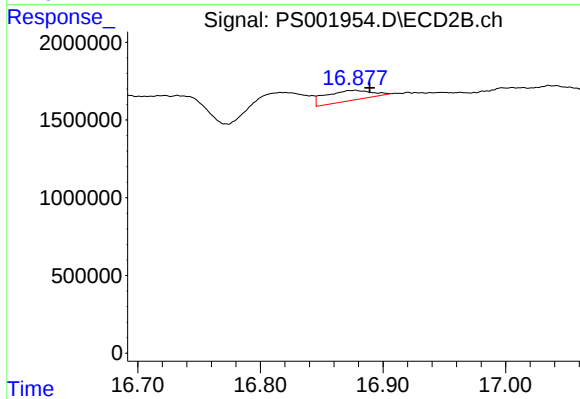

#16 DCPA

R.T.: 16.876 min
Delta R.T.: -0.013 min
Response: 1710336
Conc: 0.93 ng/ml