

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 20:13
 Operator : EI\SJ
 Sample : J5201-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-02-100818-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 03:48:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.489	10.984	83203101	79618521	370.920	313.438
Target Compounds							
1) T	Dalapon	2.921	2.403	21633596	28013458	66.531	94.827 #
2) T	3,5-DICHL...	0.000	9.140	0	844821	N.D.	2.677 #
5) T	DICAMBA	0.000	11.226	0	3702055	N.D.	4.151 #
6) T	MCP	12.173	0.000	6480230	0	10.169	N.D. #
7) T	MCPA	0.000	11.790	0	15625473	N.D.	18.026 #
9) T	2,4-D	0.000	12.818	0	2240275	N.D.	7.201 #
11) T	2,4,5-TP ...	0.000	13.956	0	6452162	N.D.	4.706 #
15) T	Picloram	16.995	16.856	2676867	-1833091	1.537	N.D. #
16) T	DCPA	0.000	16.918	0	1020982	N.D.	0.554 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 20:13
Operator : EI\SJ
Sample : J5201-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 03:48:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

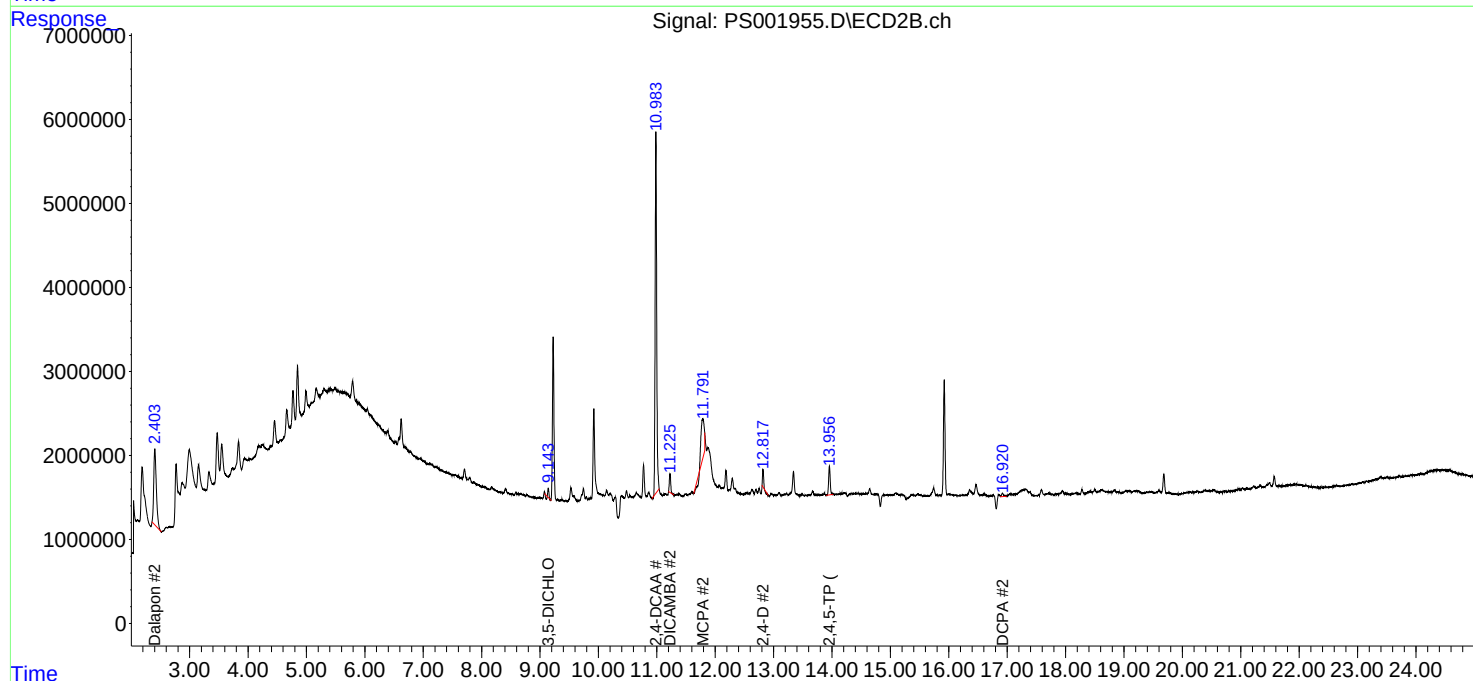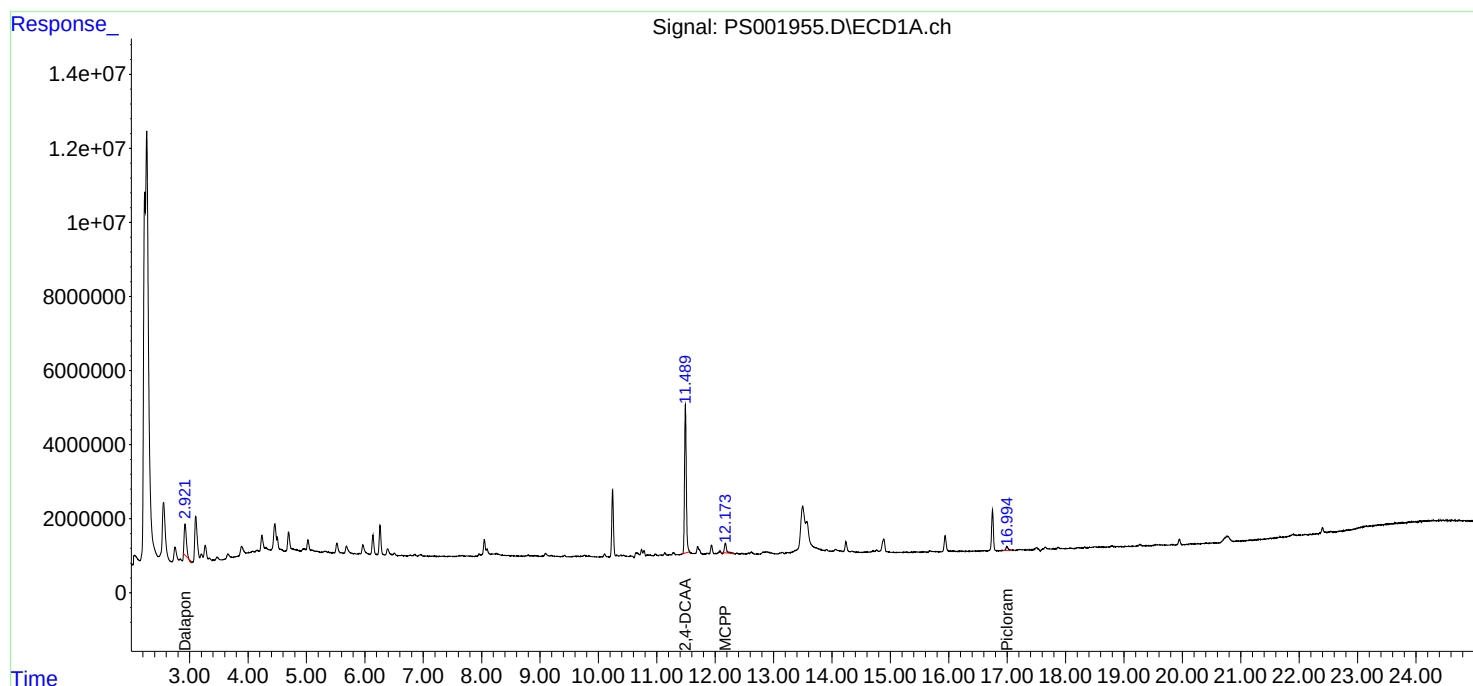


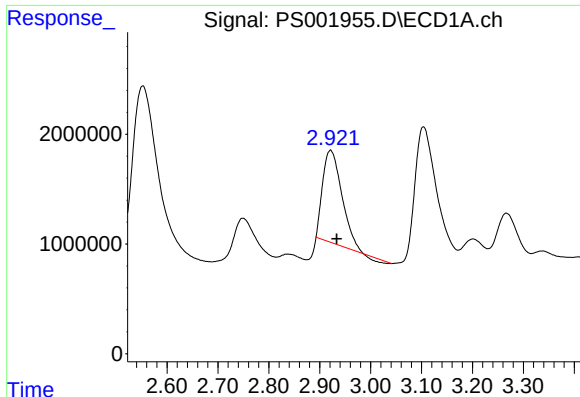

#1 Dalapon


R.T.: 2.921 min
Delta R.T.: -0.012 min
Response: 21633596
Conc: 66.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-C

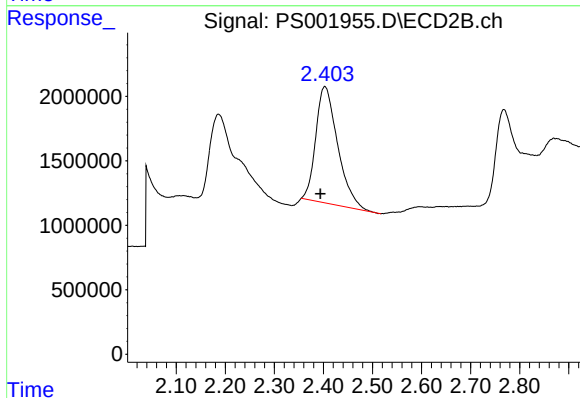


#1 Dalapon

R.T.: 2.403 min
Delta R.T.: 0.009 min
Response: 28013458
Conc: 94.83 ng/ml

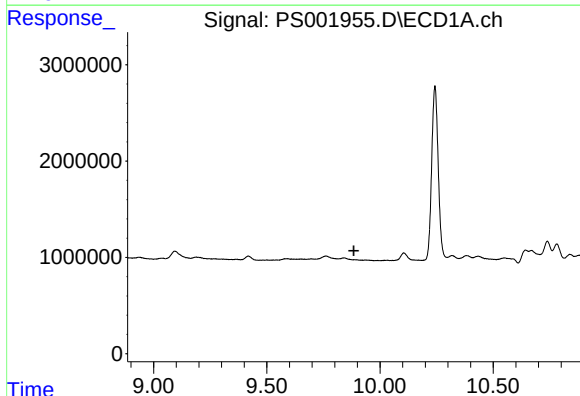


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.884 min
Response: 0
Conc: N.D.

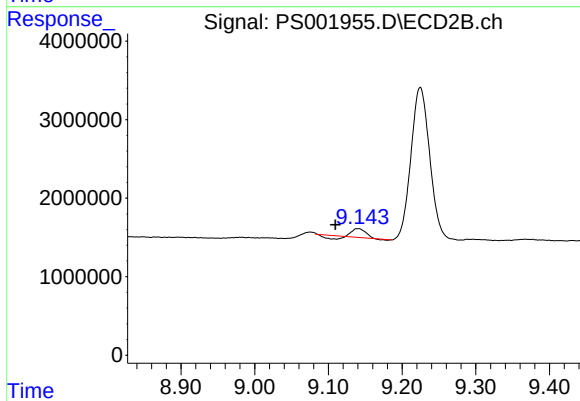

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.140 min
Delta R.T.: 0.031 min
Response: 844821
Conc: 2.68 ng/ml

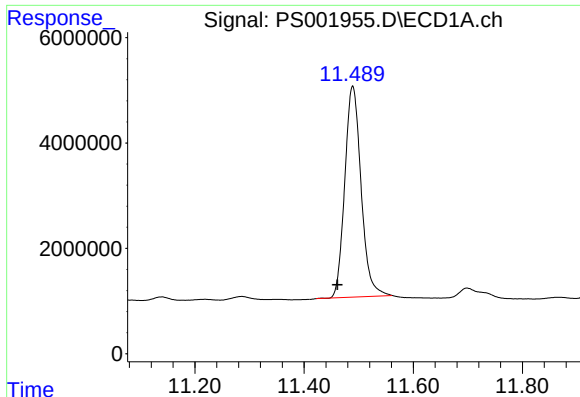

#4 2,4-DCAA


R.T.: 11.489 min
Delta R.T.: 0.028 min
Response: 83203101
Conc: 370.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-C

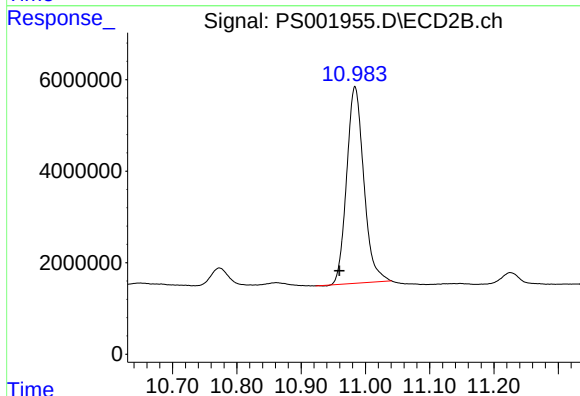


#4 2,4-DCAA

R.T.: 10.984 min
Delta R.T.: 0.024 min
Response: 79618521
Conc: 313.44 ng/ml

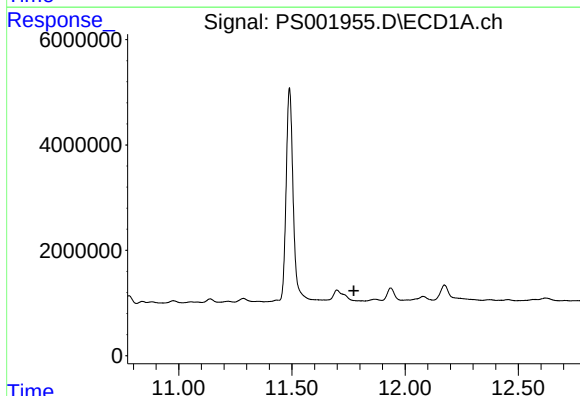


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.774 min
Response: 0
Conc: N.D.

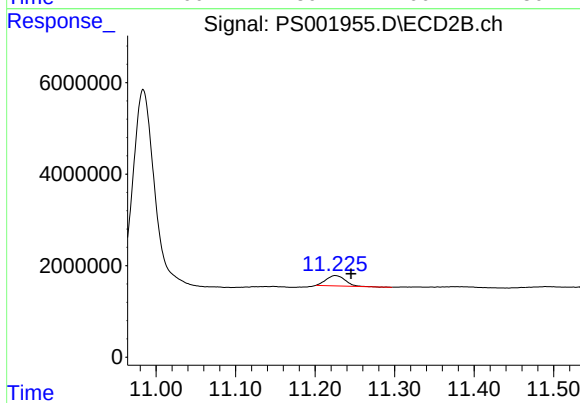

#5 DICAMBA


R.T.: 11.226 min
Delta R.T.: -0.019 min
Response: 3702055
Conc: 4.15 ng/ml

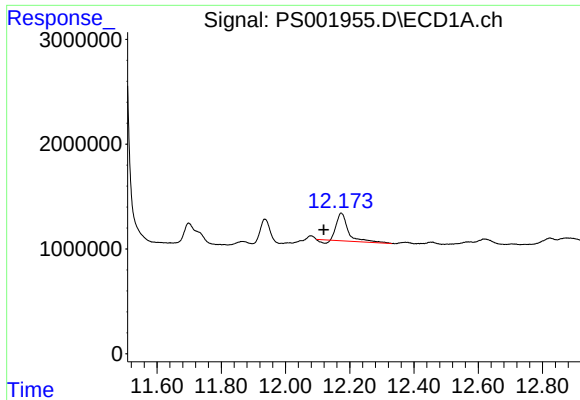

#6 MCPP


R.T.: 12.173 min
Delta R.T.: 0.055 min
Response: 6480230
Conc: 10.17 ug/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-C

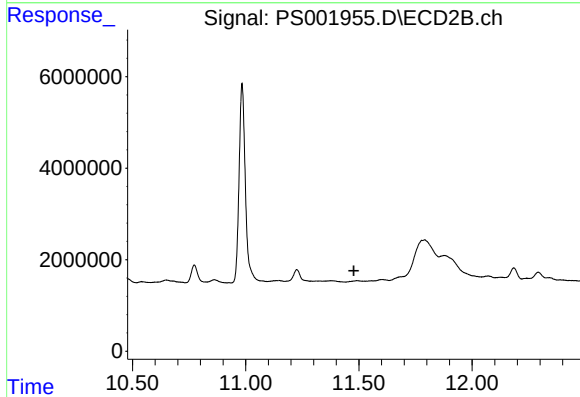


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

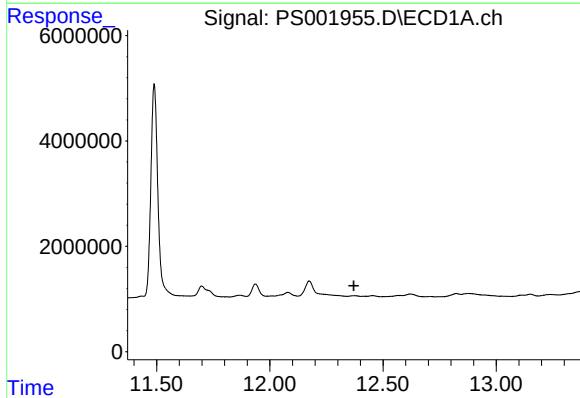


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.371 min
Response: 0
Conc: N.D.

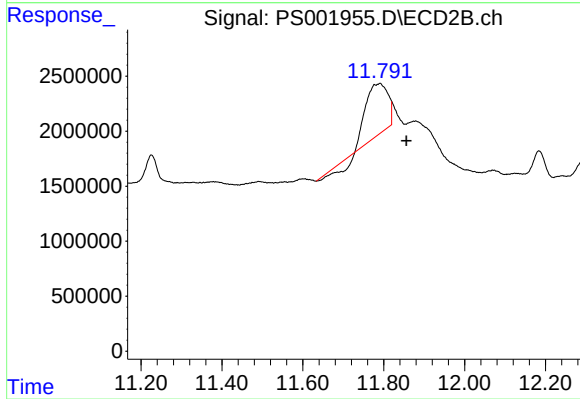

#7 MCPA


R.T.: 11.790 min
Delta R.T.: -0.066 min
Response: 15625473
Conc: 18.03 ug/ml

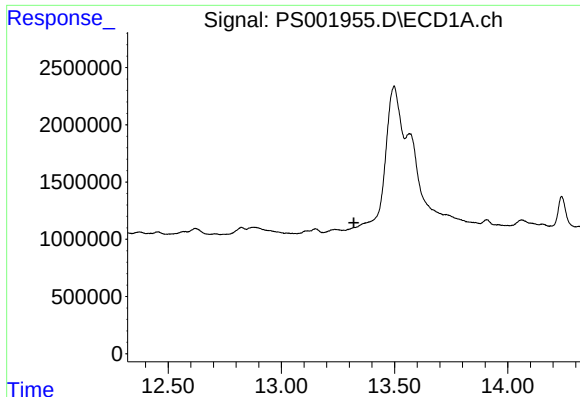

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-C

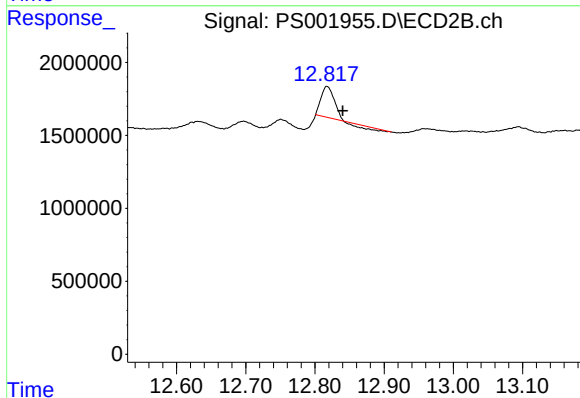


#9 2,4-D

R.T.: 12.818 min
Delta R.T.: -0.023 min
Response: 2240275
Conc: 7.20 ng/ml

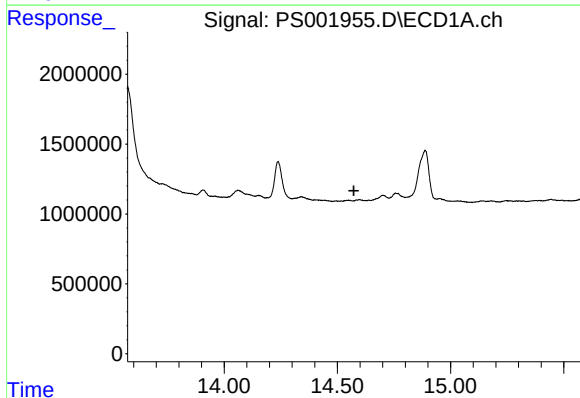


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.573 min
Response: 0
Conc: N.D.

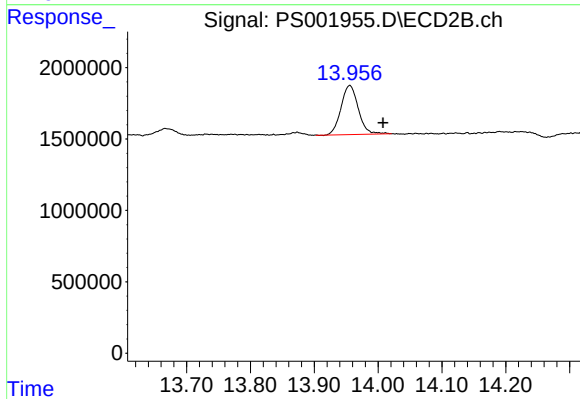

#11 2,4,5-TP (SILVEX)


R.T.: 13.956 min
Delta R.T.: -0.052 min
Response: 6452162
Conc: 4.71 ng/ml

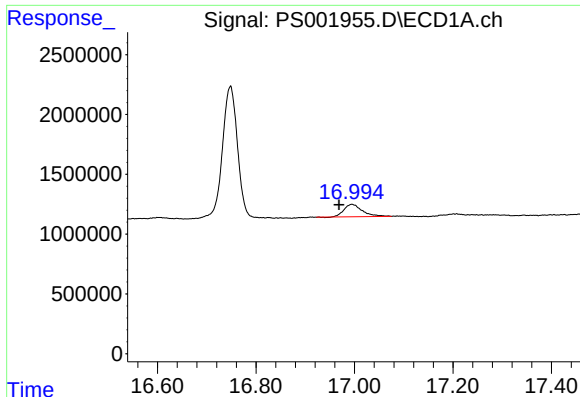

#15 Picloram


R.T.: 16.995 min
Delta R.T.: 0.026 min
Response: 2676867
Conc: 1.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-02-100818-C

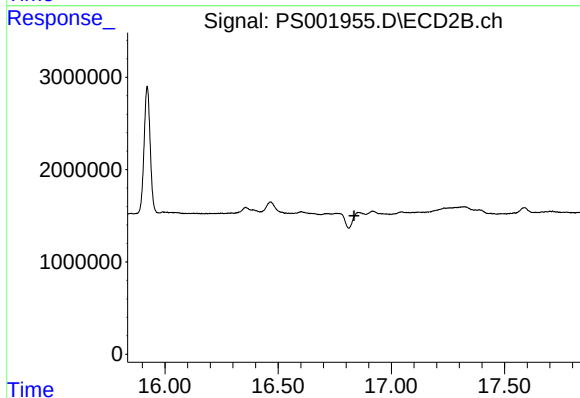


#15 Picloram

R.T.: 16.856 min
Delta R.T.: 0.021 min
Response: -1833091
Conc: N.D.

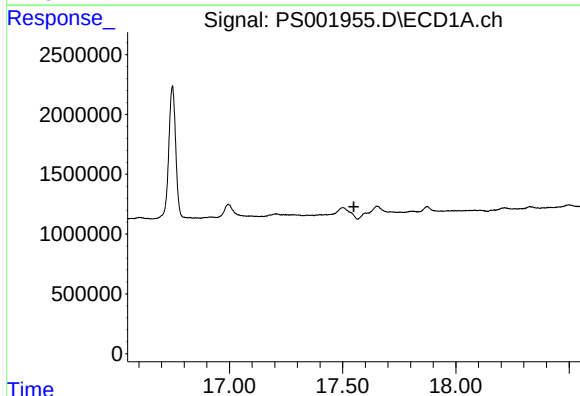

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.549 min
Response: 0
Conc: N.D.

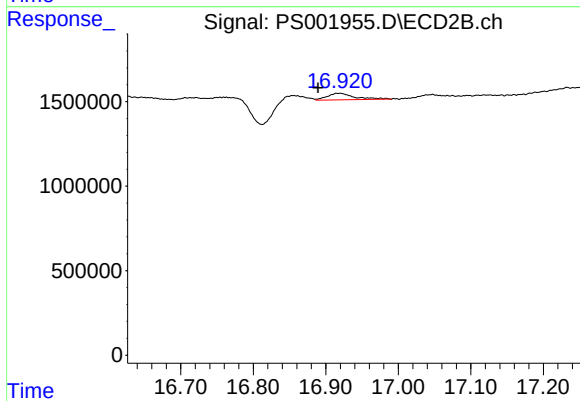

#16 DCPA

R.T.: 16.918 min
Delta R.T.: 0.029 min
Response: 1020982
Conc: 0.55 ng/ml