

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2018 20:44
 Operator : EI\SJ
 Sample : PB113680BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB113680BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 03:48:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	11.467	10.961	117.1E6	113.3E6	521.823	446.196
Target Compounds						
1) T Dalapon	0.000	2.378	0	10644317	N.D.	36.031 #
6) T MCPP	12.153	0.000	12944426	0	20.313	N.D. #
15) T Picloram	0.000	16.836	0	7999252	N.D.	4.703 #
16) T DCPA	0.000	16.902	0	4888523	N.D.	2.650 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2018 20:44
Operator : EI\SJ
Sample : PB113680BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB113680BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 03:48:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

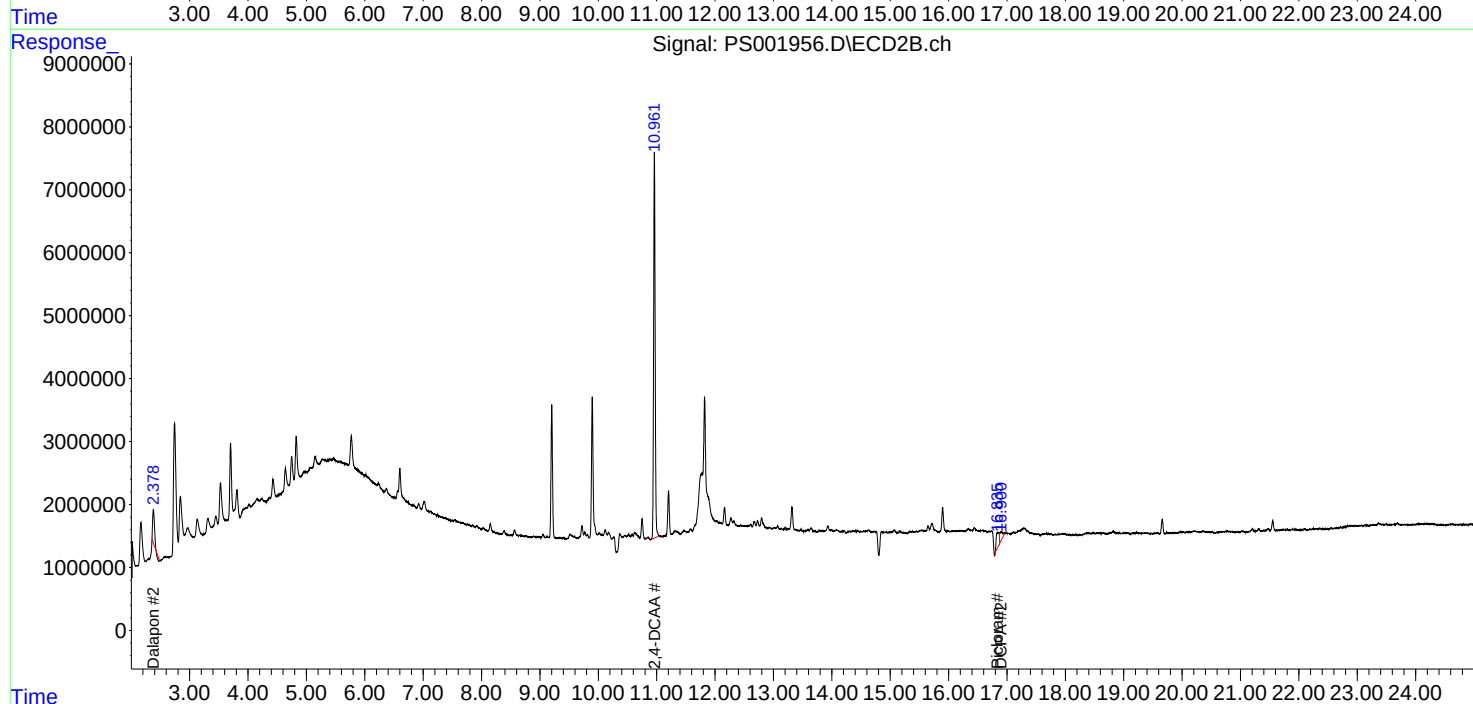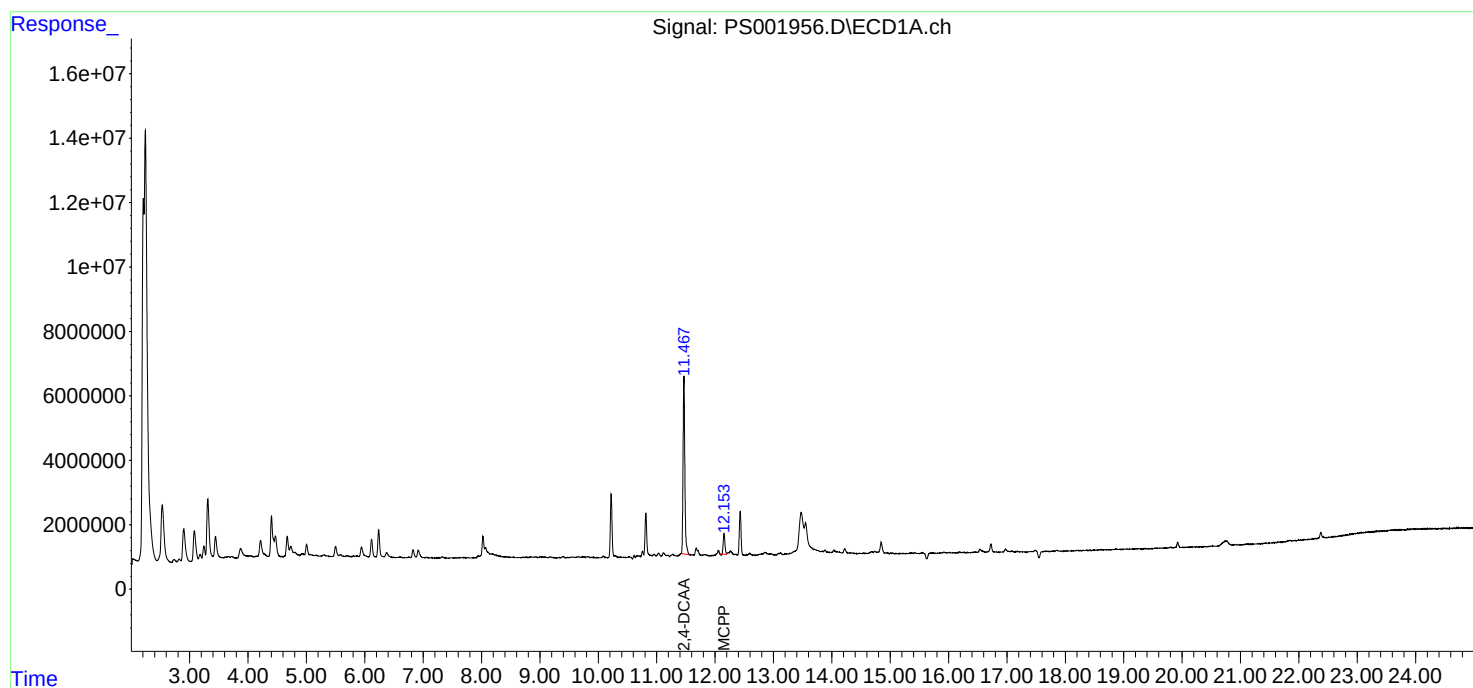


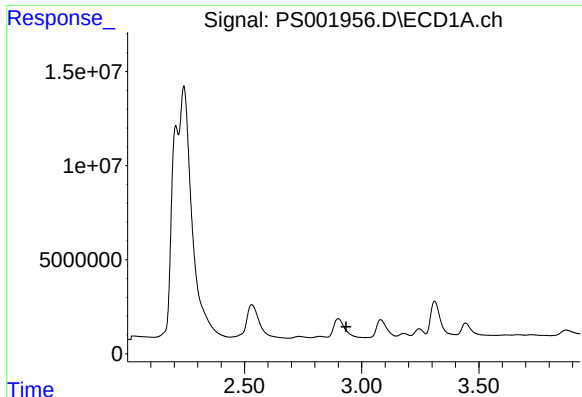

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.933 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB113680BL

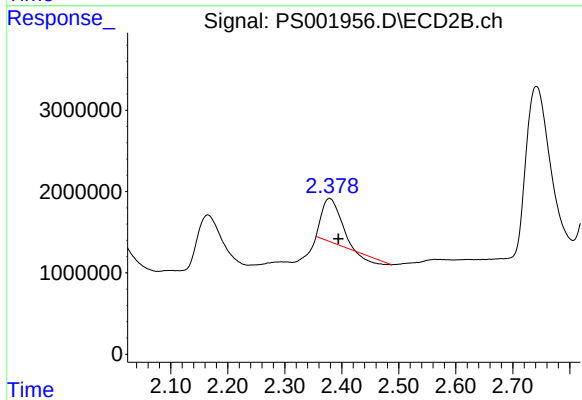


#1 Dalapon

R.T.: 2.378 min
Delta R.T.: -0.016 min
Response: 10644317
Conc: 36.03 ng/ml

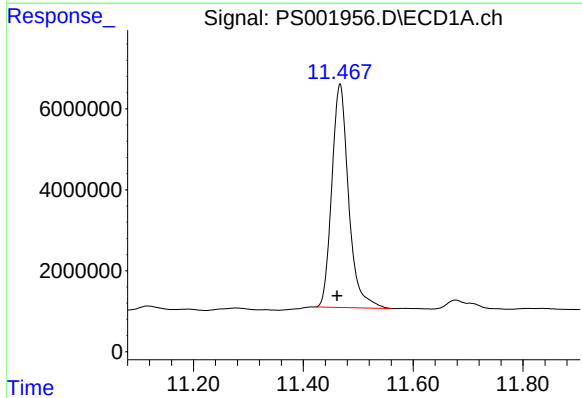


#4 2,4-DCAA

R.T.: 11.467 min
Delta R.T.: 0.005 min
Response: 117053126
Conc: 521.82 ng/ml

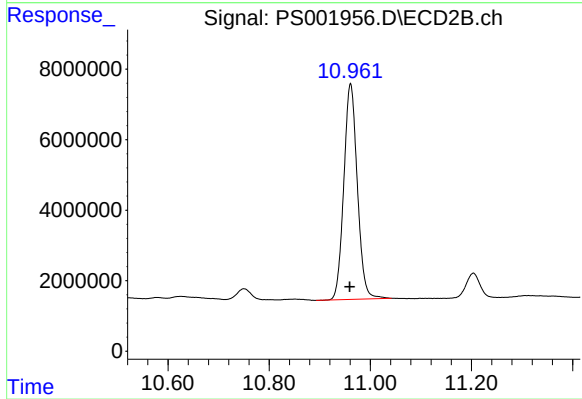

#4 2,4-DCAA


R.T.: 10.961 min
Delta R.T.: 0.001 min
Response: 113341176
Conc: 446.20 ng/ml

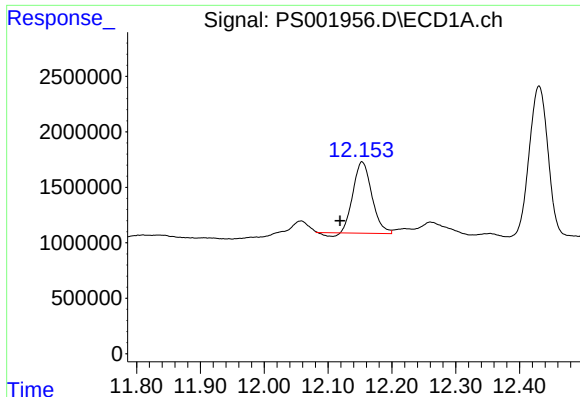

#6 MCP


R.T.: 12.153 min
Delta R.T.: 0.035 min
Response: 12944426
Conc: 20.31 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB113680BL

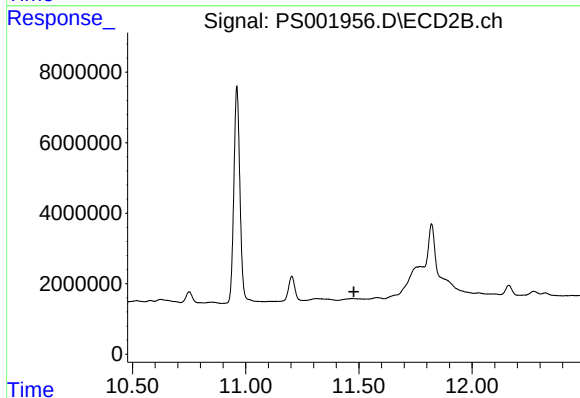


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

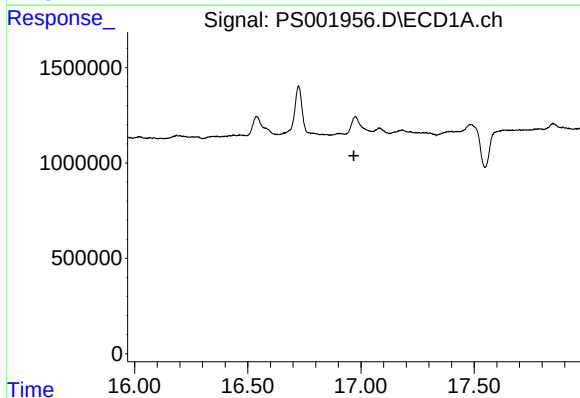


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.969 min
Response: 0
Conc: N.D.

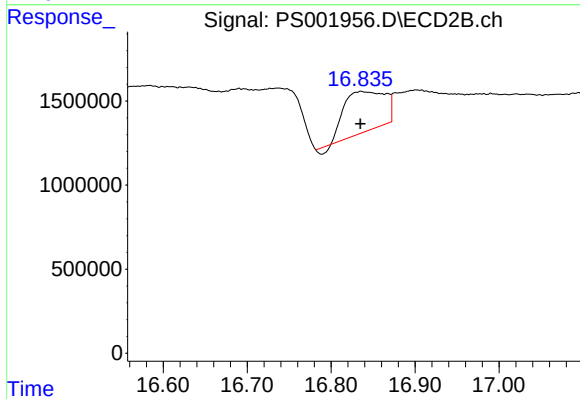

#15 Picloram


R.T.: 16.836 min
Delta R.T.: 0.000 min
Response: 7999252
Conc: 4.70 ng/ml

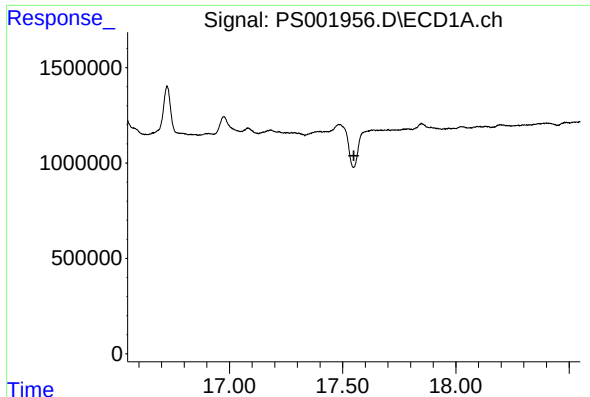

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB113680BL

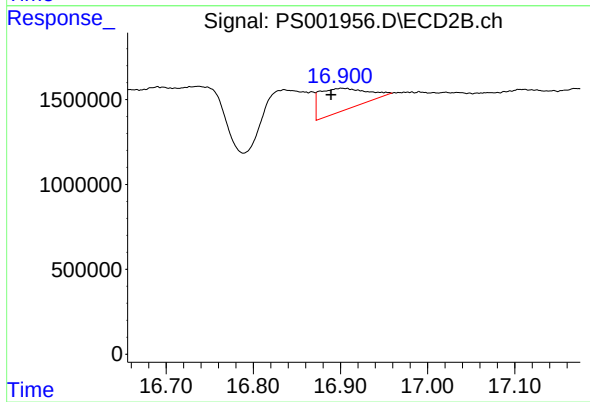

#16 DCPA

R.T.: 16.902 min
Delta R.T.: 0.013 min
Response: 4888523
Conc: 2.65 ng/ml