

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2018 05:32
 Operator : EI\SJ
 Sample : J5366-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RBR200035

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 08:08:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.463	10.957	110.5E6	109.2E6	492.535	429.903
Target Compounds							
1) T	Dalapon	0.000	2.377	0	11488829	N.D.	38.890 #
2) T	3,5-DICHL...	0.000	9.049	0	2848875	N.D.	9.026 #
6) T	MCP	12.149	0.000	10748889	0	16.868	N.D. #
9) T	2,4-D	0.000	12.792	0	3748357	N.D.	12.048 #
10) T	Pentachlo...	13.704	13.387	2124570	3144243	0.691	0.917 #
12) T	2,4,5-T	0.000	14.577	0	2146293	N.D.	1.944 #
14) T	DINOSEB	0.000	15.711	0	521170	N.D.	0.550 #
15) T	Picloram	16.983	16.889	13360131	23229579	7.673	13.659 #
16) T	DCPA	0.000	16.889	0	23229579	N.D.	12.594 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2018 05:32
Operator : EI\SJ
Sample : J5366-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RBR200035

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 08:08:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

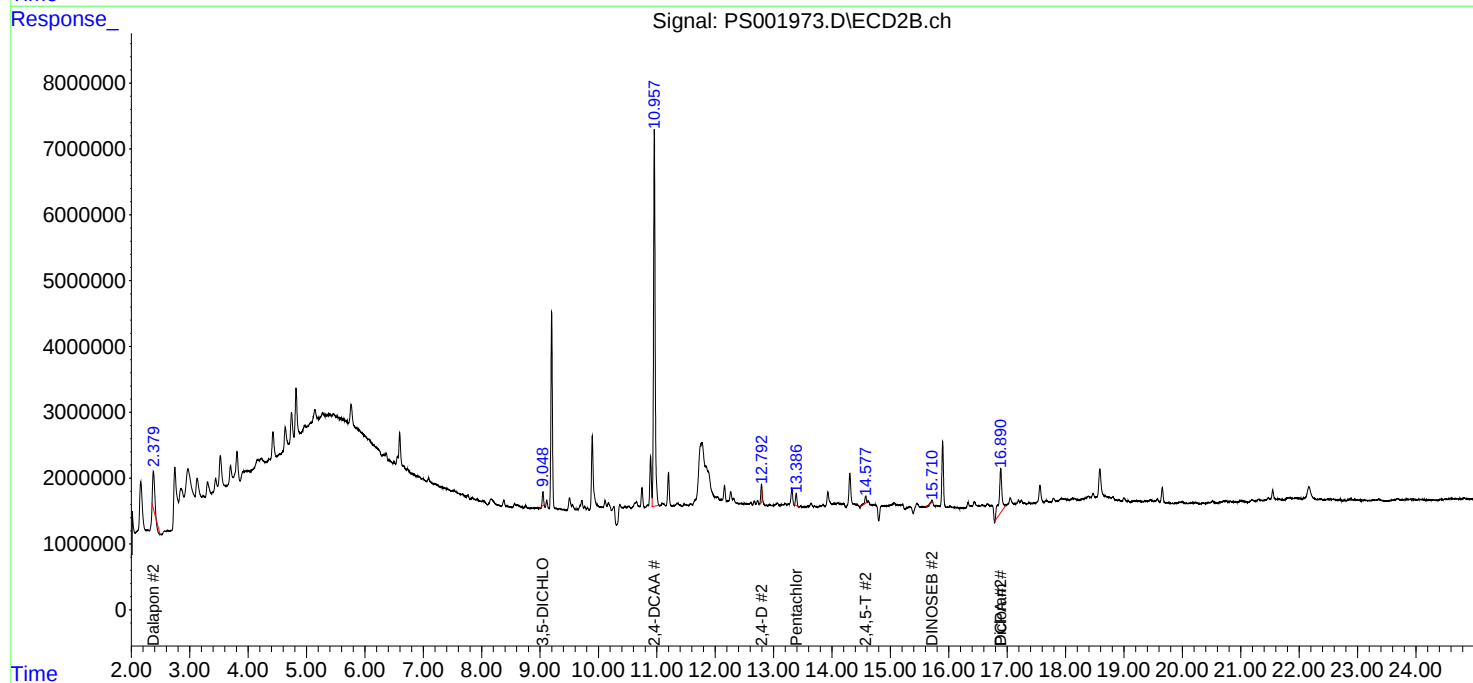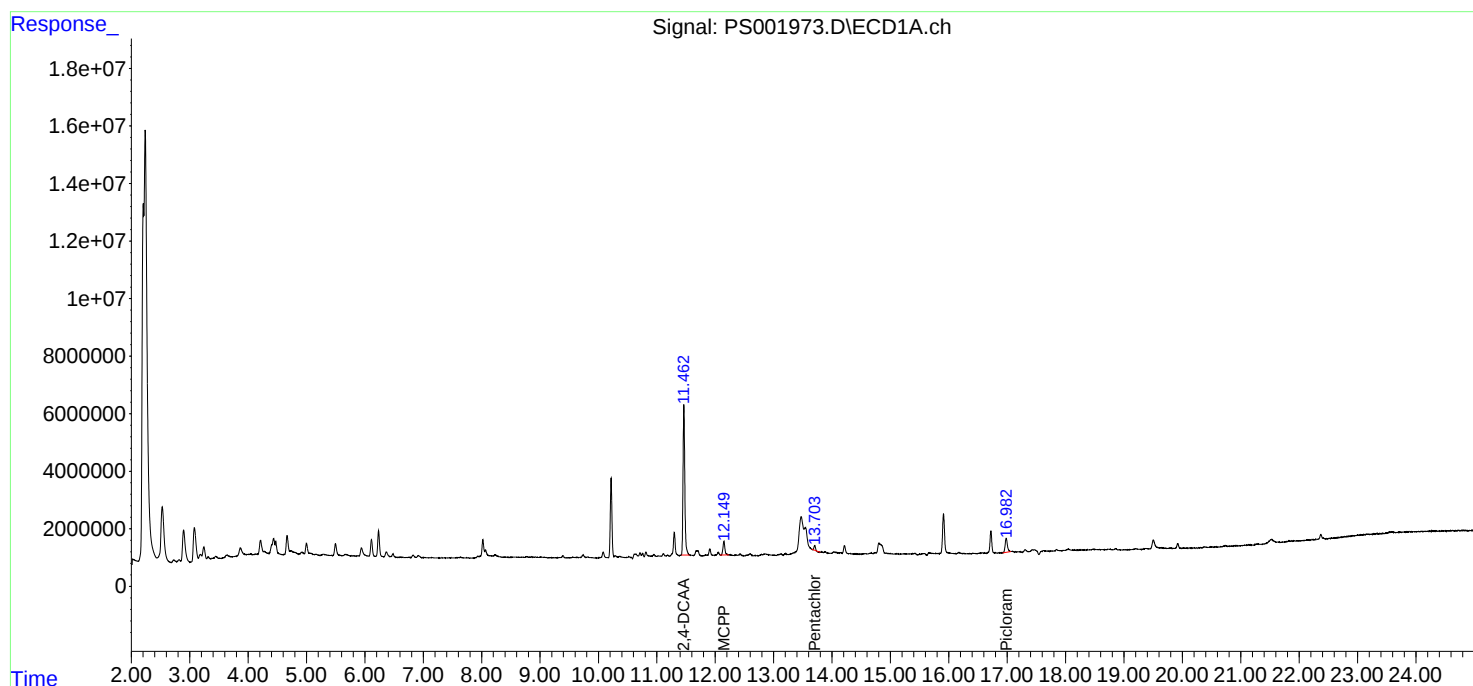


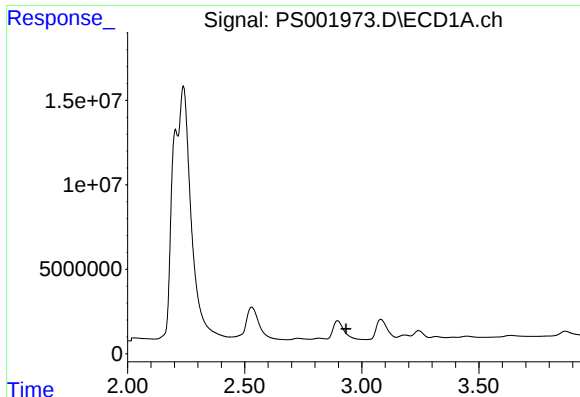

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.933 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR200035

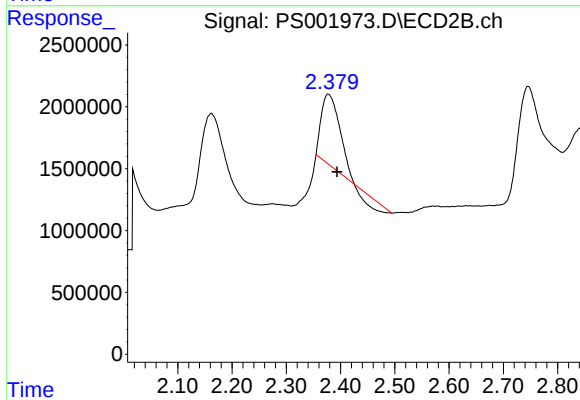


#1 Dalapon

R.T.: 2.377 min
Delta R.T.: -0.017 min
Response: 11488829
Conc: 38.89 ng/ml

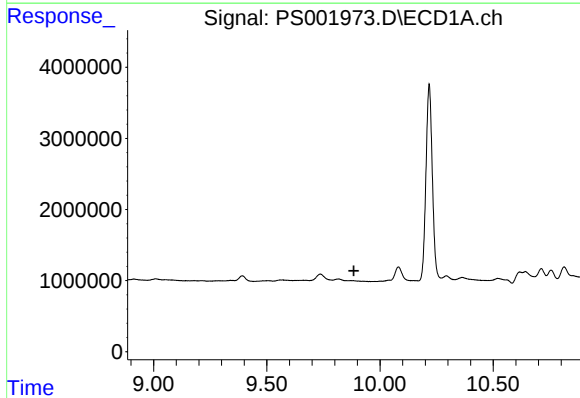


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.884 min
Response: 0
Conc: N.D.

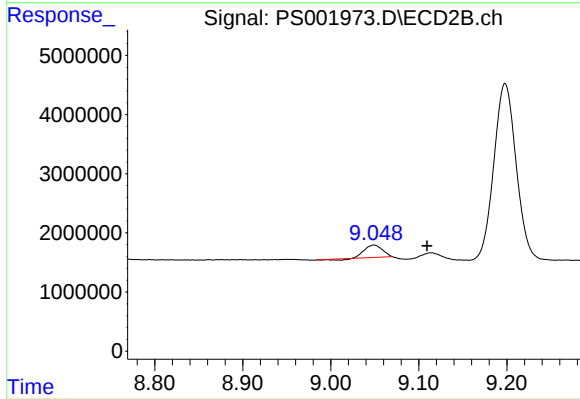

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.049 min
Delta R.T.: -0.061 min
Response: 2848875
Conc: 9.03 ng/ml

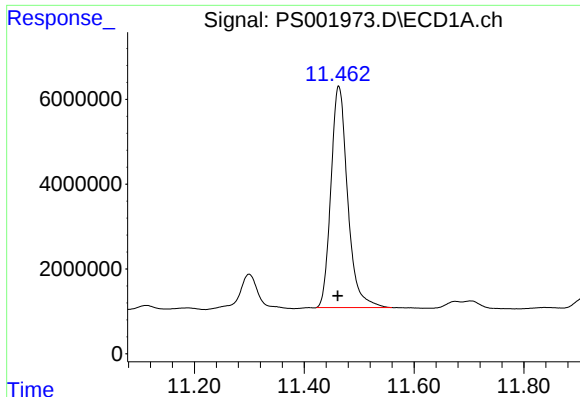

#4 2,4-DCAA


R.T.: 11.463 min
Delta R.T.: 0.002 min
Response: 110483247
Conc: 492.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
RBR200035

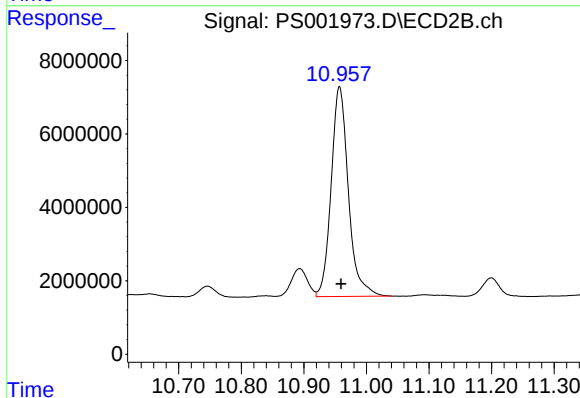


#4 2,4-DCAA

R.T.: 10.957 min
Delta R.T.: -0.003 min
Response: 109202625
Conc: 429.90 ng/ml

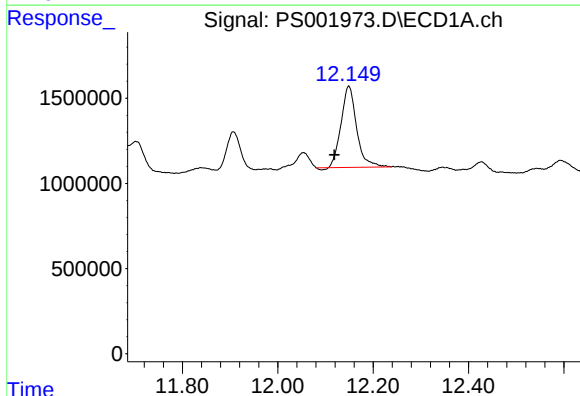


#6 MCP

R.T.: 12.149 min
Delta R.T.: 0.030 min
Response: 10748889
Conc: 16.87 ug/ml

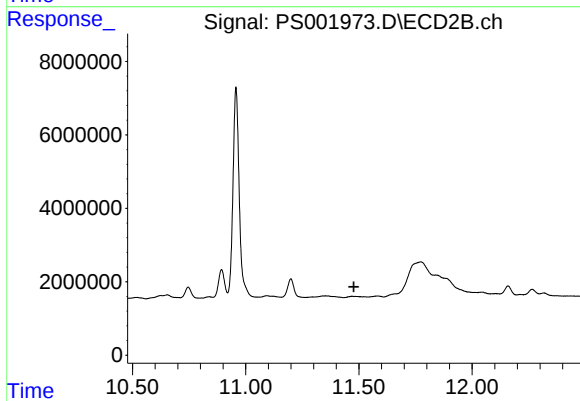

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.478 min
Response: 0
Conc: N.D.

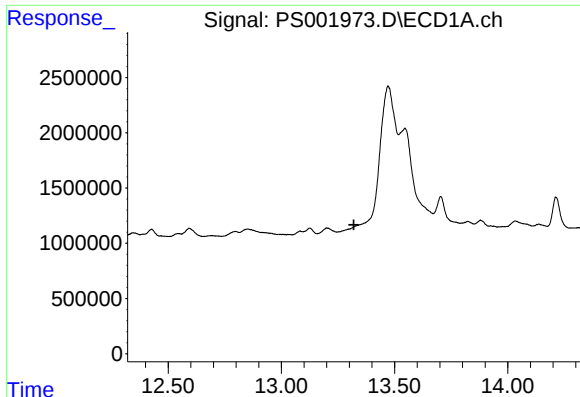

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR200035

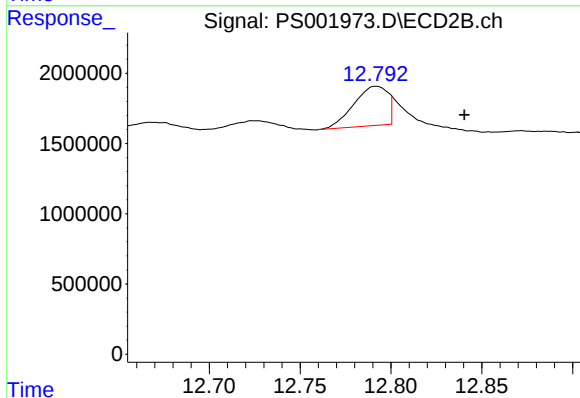


#9 2,4-D

R.T.: 12.792 min
Delta R.T.: -0.048 min
Response: 3748357
Conc: 12.05 ng/ml

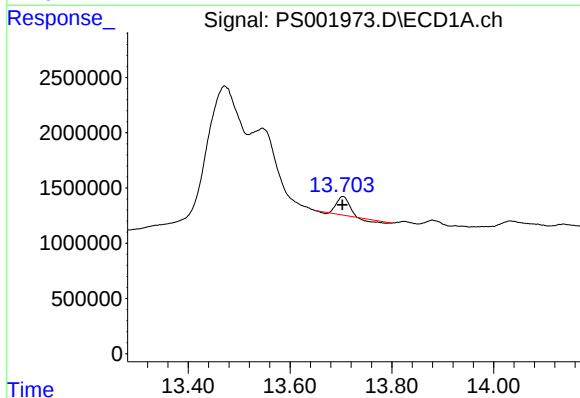


#10 Pentachlorophenol

R.T.: 13.704 min
Delta R.T.: 0.000 min
Response: 2124570
Conc: 0.69 ng/ml

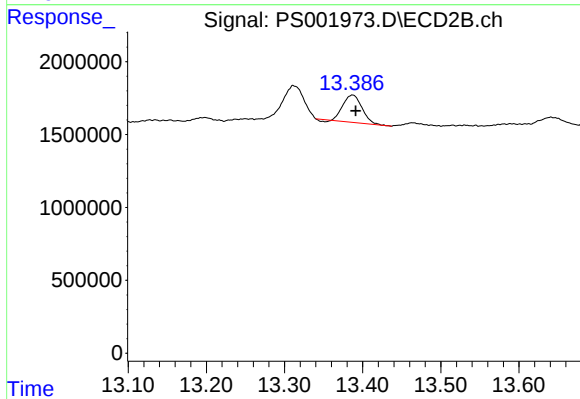

#10 Pentachlorophenol


R.T.: 13.387 min
Delta R.T.: -0.004 min
Response: 3144243
Conc: 0.92 ng/ml

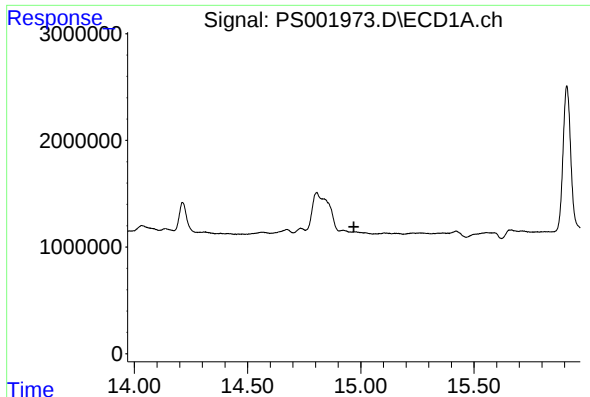

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR200035

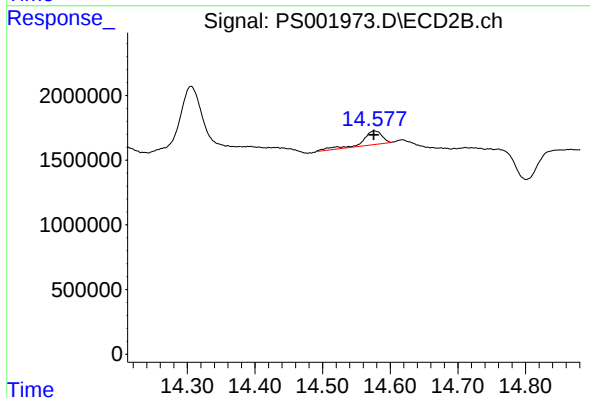


#12 2,4,5-T

R.T.: 14.577 min
Delta R.T.: 0.002 min
Response: 2146293
Conc: 1.94 ng/ml

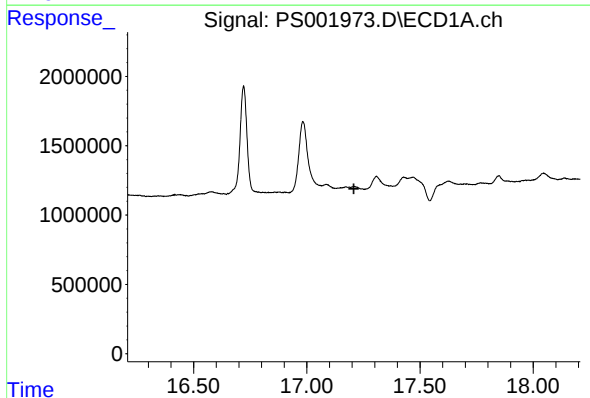


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.208 min
Response: 0
Conc: N.D.

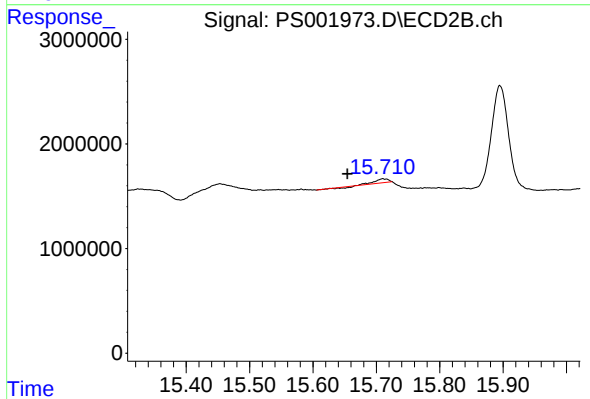

#14 DINOSEB


R.T.: 15.711 min
Delta R.T.: 0.057 min
Response: 521170
Conc: 0.55 ng/ml

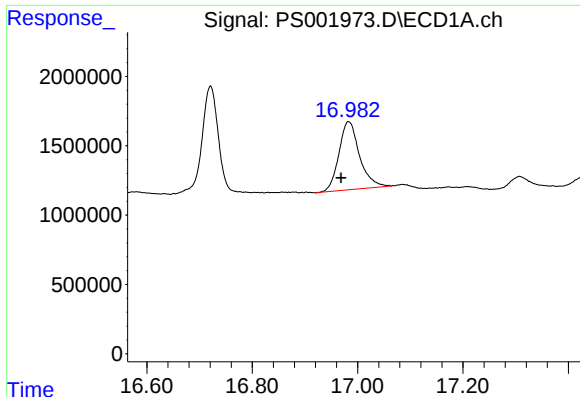

#15 Picloram


R.T.: 16.983 min
Delta R.T.: 0.014 min
Response: 13360131
Conc: 7.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
RBR200035

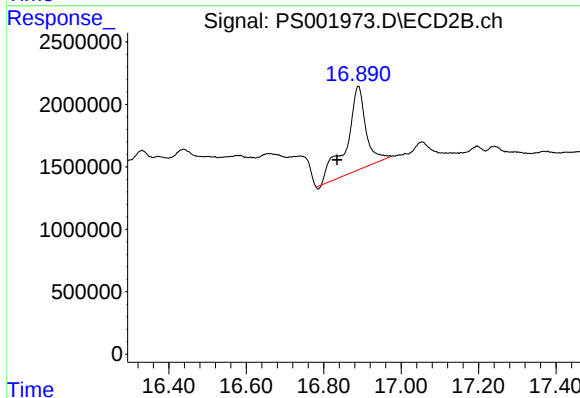


#15 Picloram

R.T.: 16.889 min
Delta R.T.: 0.054 min
Response: 23229579
Conc: 13.66 ng/ml

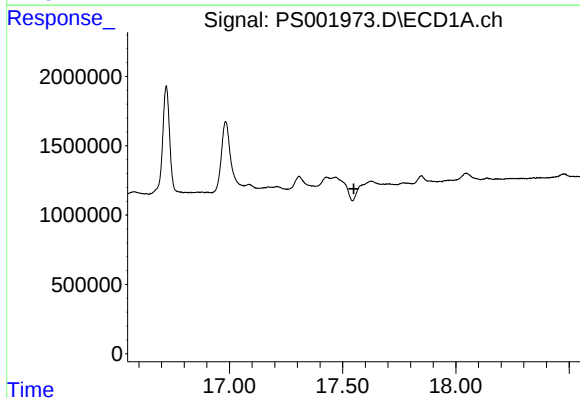

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.549 min
Response: 0
Conc: N.D.

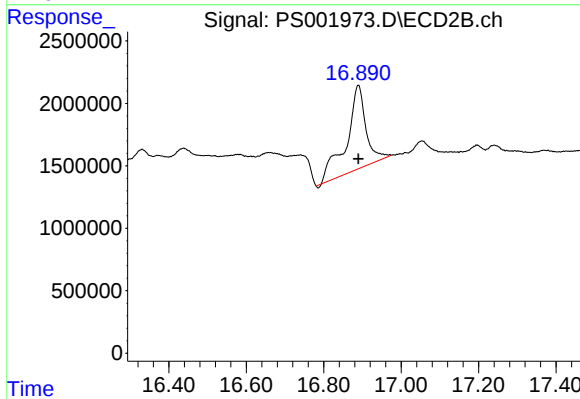

#16 DCPA

R.T.: 16.889 min
Delta R.T.: 0.000 min
Response: 23229579
Conc: 12.59 ng/ml