

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2018 06:03
 Operator : EI\SJ
 Sample : J5369-10
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CONCRETE-PILE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 08:09:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.462	10.957	108.3E6	106.2E6	482.968	417.954
Target Compounds							
1) T	Dalapon	0.000	2.376	0	6828548	N.D.	23.115 #
2) T	3,5-DICHL...	0.000	9.048	0	2225742	N.D.	7.052 #
3) T	4-Nitroph...	11.112	0.000	1870055	0	13.286	N.D. #
6) T	MCP	12.149	0.000	10070647	0	15.804	N.D. #
9) T	2,4-D	0.000	12.791	0	4029559	N.D.	12.952 #
10) T	Pentachlo...	13.703	13.387	2528163	2913888	0.823	0.850
15) T	Picloram	0.000	16.891	0	11180077	N.D.	6.574 #
16) T	DCPA	0.000	16.891	0	11180077	N.D.	6.062 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2018 06:03
Operator : EI\SJ
Sample : J5369-10
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CONCRETE-PILE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 08:09:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

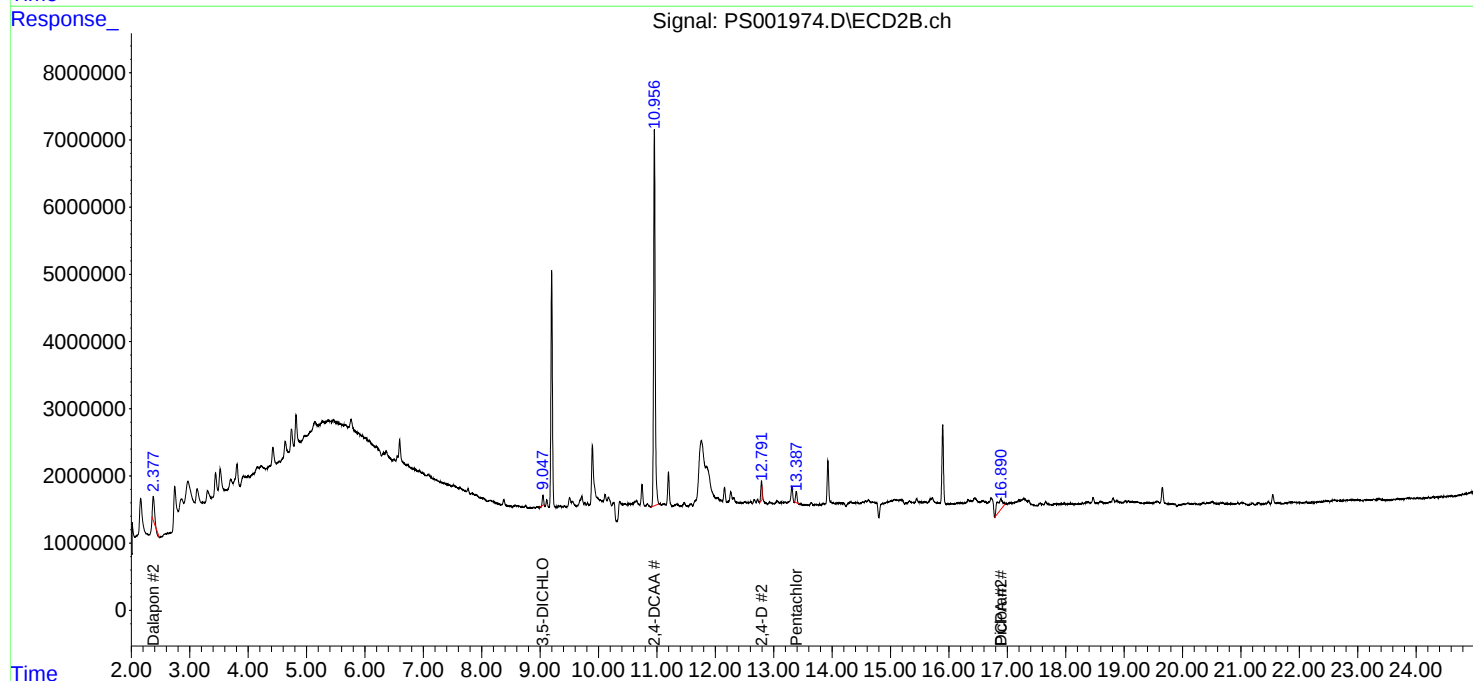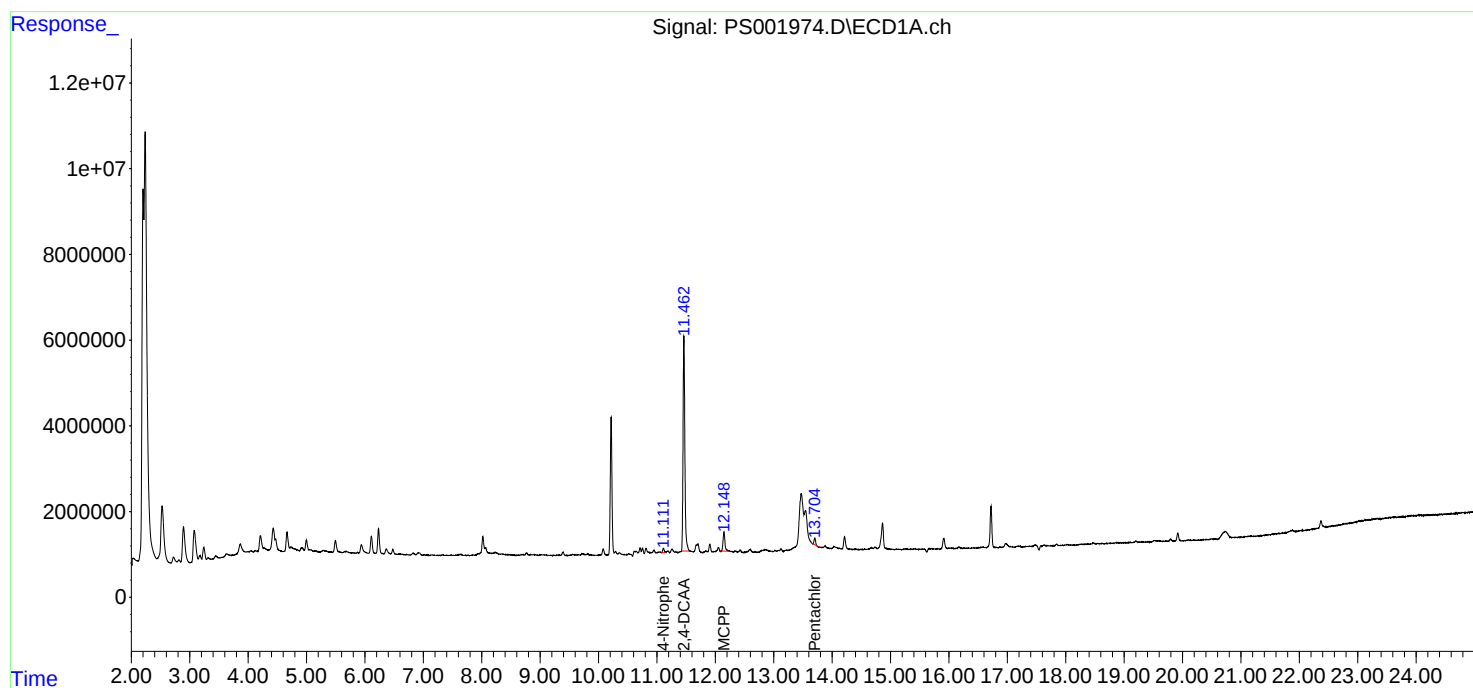


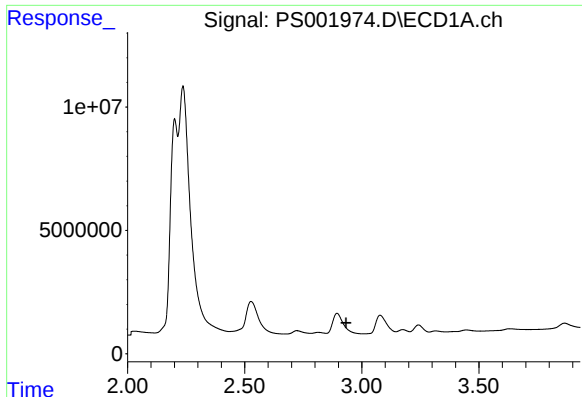

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.933 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CONCRETE-PILE

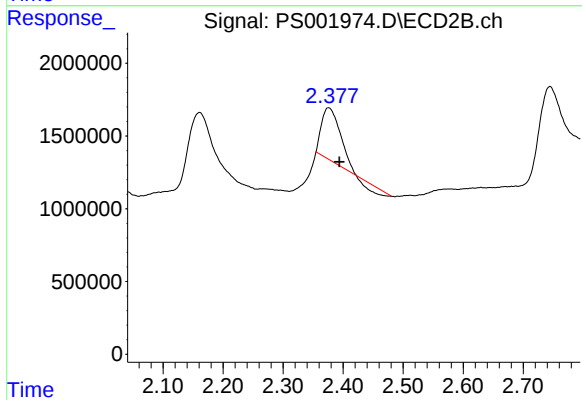


#1 Dalapon

R.T.: 2.376 min
Delta R.T.: -0.018 min
Response: 6828548
Conc: 23.11 ng/ml

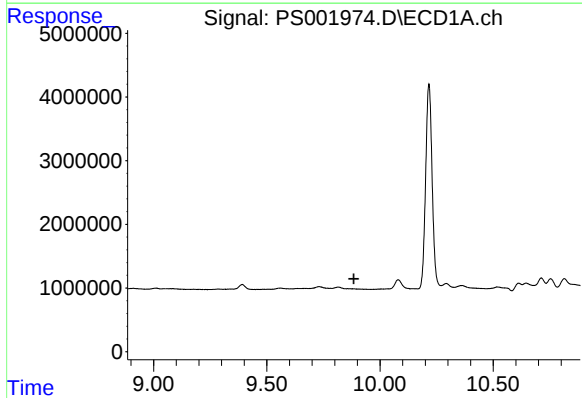


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.884 min
Response: 0
Conc: N.D.

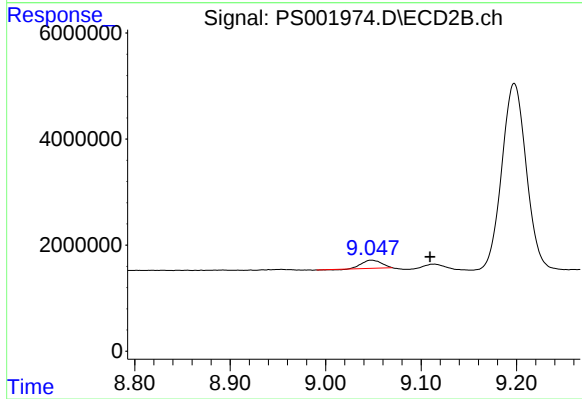

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.048 min
Delta R.T.: -0.062 min
Response: 2225742
Conc: 7.05 ng/ml

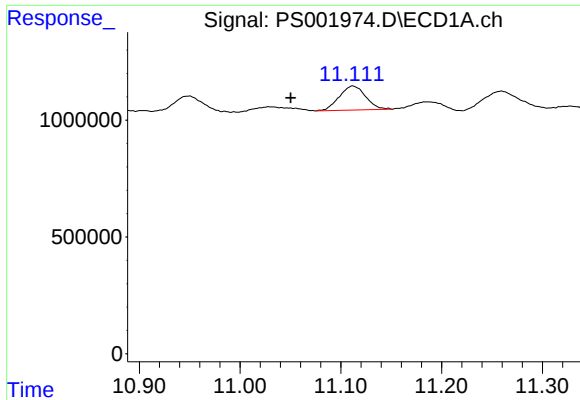

#3 4-Nitrophenol


R.T.: 11.112 min
Delta R.T.: 0.062 min
Response: 1870055
Conc: 13.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
CONCRETE-PILE

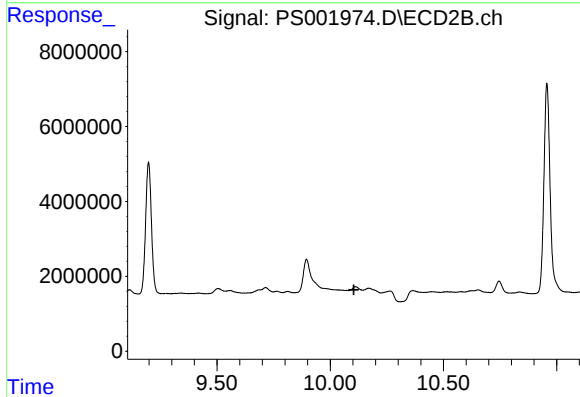


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.105 min
Response: 0
Conc: N.D.

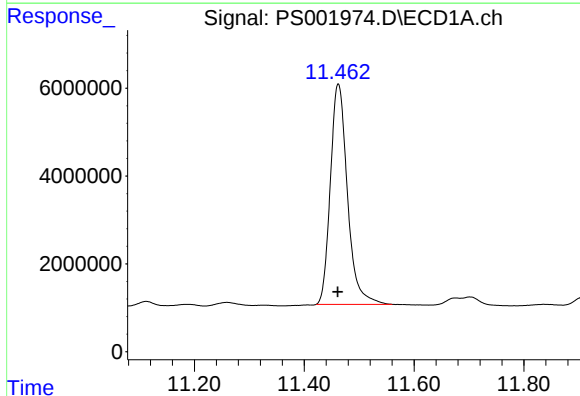


#4 2,4-DCAA

R.T.: 11.462 min
Delta R.T.: 0.000 min
Response: 108337224
Conc: 482.97 ng/ml

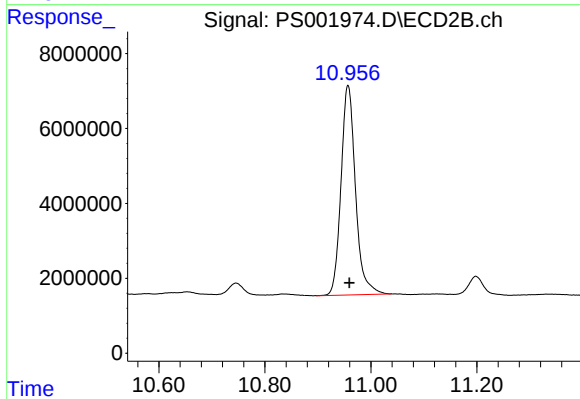

#4 2,4-DCAA


R.T.: 10.957 min
Delta R.T.: -0.003 min
Response: 106167248
Conc: 417.95 ng/ml

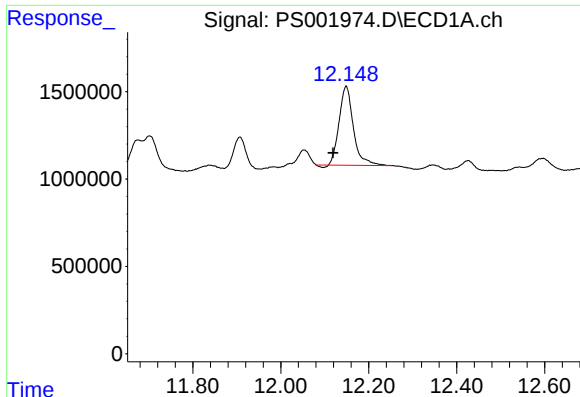

#6 MCP


R.T.: 12.149 min
Delta R.T.: 0.030 min
Response: 10070647
Conc: 15.80 ug/ml

Instrument :
ECD_S
ClientSampleId :
CONCRETE-PILE

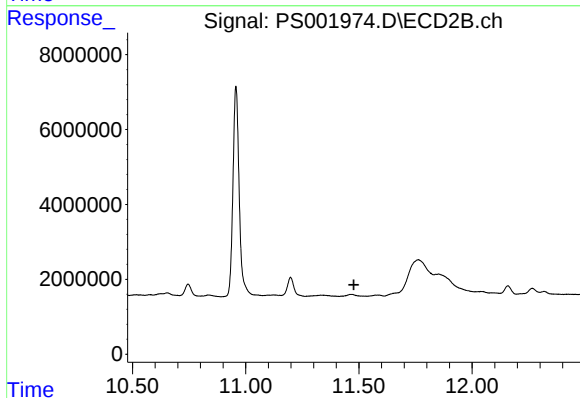


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

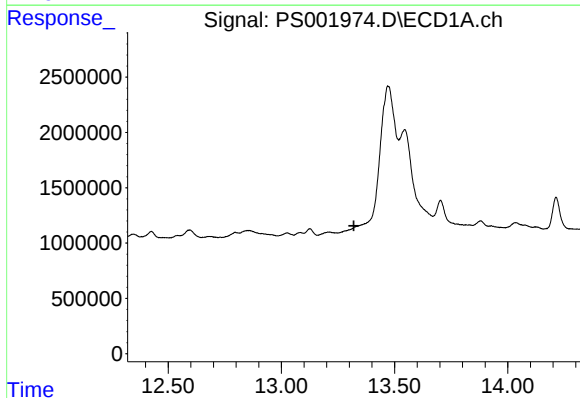


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.320 min
Response: 0
Conc: N.D.

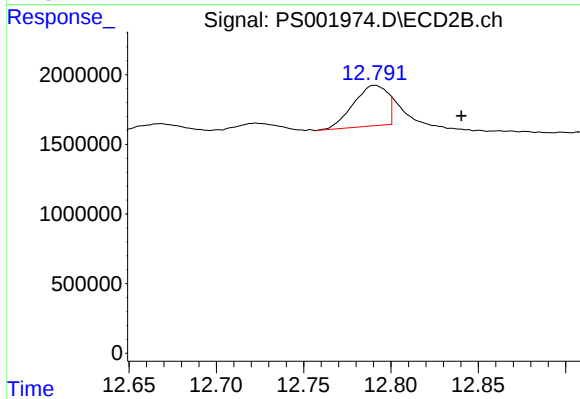

#9 2,4-D

R.T.: 12.791 min
Delta R.T.: -0.049 min
Response: 4029559
Conc: 12.95 ng/ml

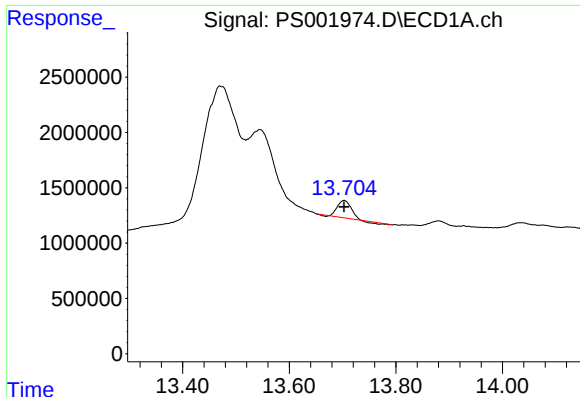

#10 Pentachlorophenol


R.T.: 13.703 min

Delta R.T.: 0.000 min

Response: 2528163

Conc: 0.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
CONCRETE-PILE

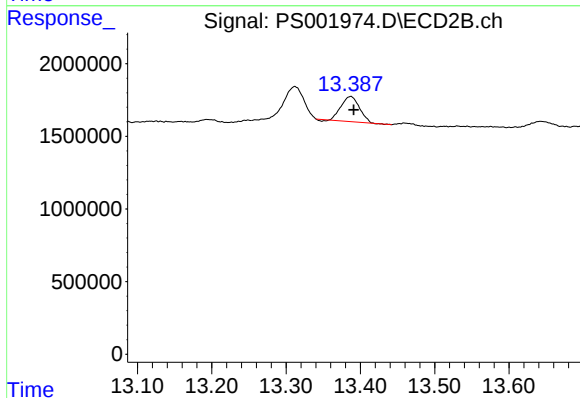


#10 Pentachlorophenol

R.T.: 13.387 min

Delta R.T.: -0.005 min

Response: 2913888

Conc: 0.85 ng/ml

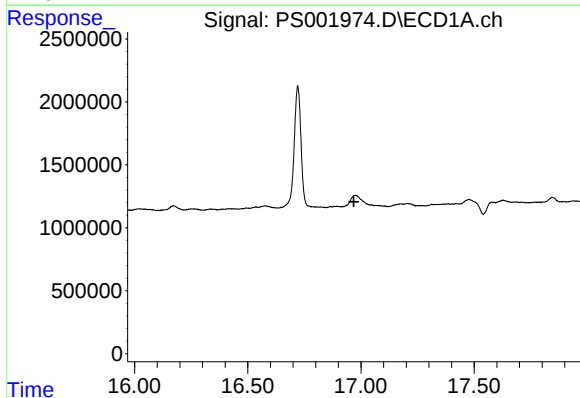


#15 Picloram

R.T.: 0.000 min

Exp R.T. : 16.969 min

Response: 0

Conc: N.D.

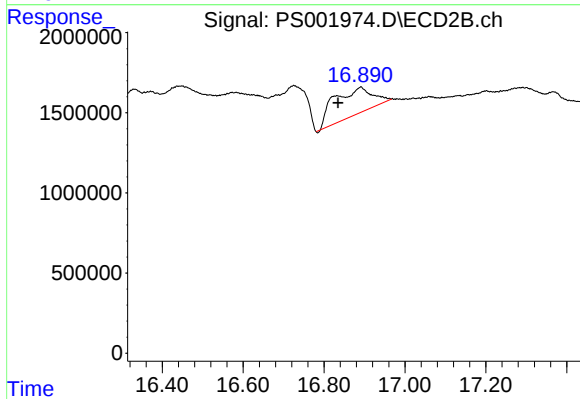


#15 Picloram

R.T.: 16.891 min

Delta R.T.: 0.056 min

Response: 11180077


Conc: 6.57 ng/ml

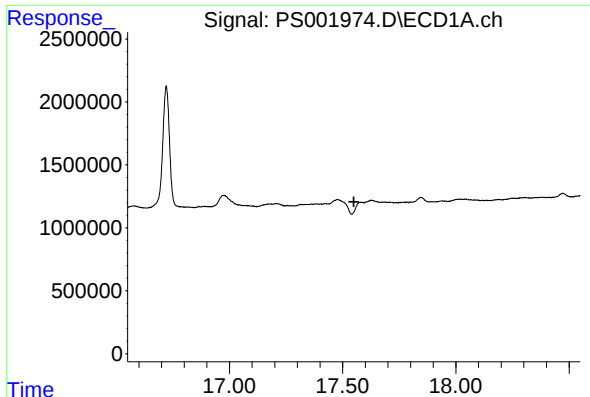

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CONCRETE-PILE

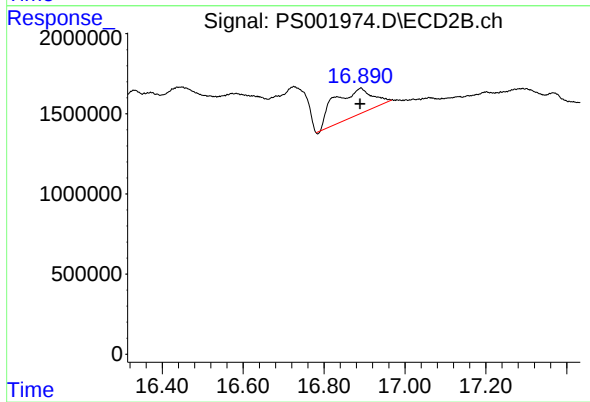

#16 DCPA

R.T.: 16.891 min
Delta R.T.: 0.002 min
Response: 11180077
Conc: 6.06 ng/ml