

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
 Data File : PS001979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2018 08:38
 Operator : EI\SJ
 Sample : PB113714TB
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB113714TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 13:00:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.450	10.944	87704766	106.7E6	390.988	420.215
Target Compounds							
1) T	Dalapon	2.881	0.000	2405194	0	7.397	N.D. #
3) T	4-Nitroph...	11.098	10.098	1663793	1856469	11.821	14.805 #
5) T	DICAMBA	0.000	11.186	0	2706382	N.D.	3.034 #
6) T	MCP	12.136	0.000	12835132	0	20.142	N.D. #
9) T	2,4-D	0.000	12.779	0	4647587	N.D.	14.939 #
15) T	Picloram	0.000	16.821	0	4574512	N.D.	2.690 #
16) T	DCPA	0.000	16.882	0	6358632	N.D.	3.447 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101018\
Data File : PS001979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2018 08:38
Operator : EI\SJ
Sample : PB113714TB
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB113714TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 13:00:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

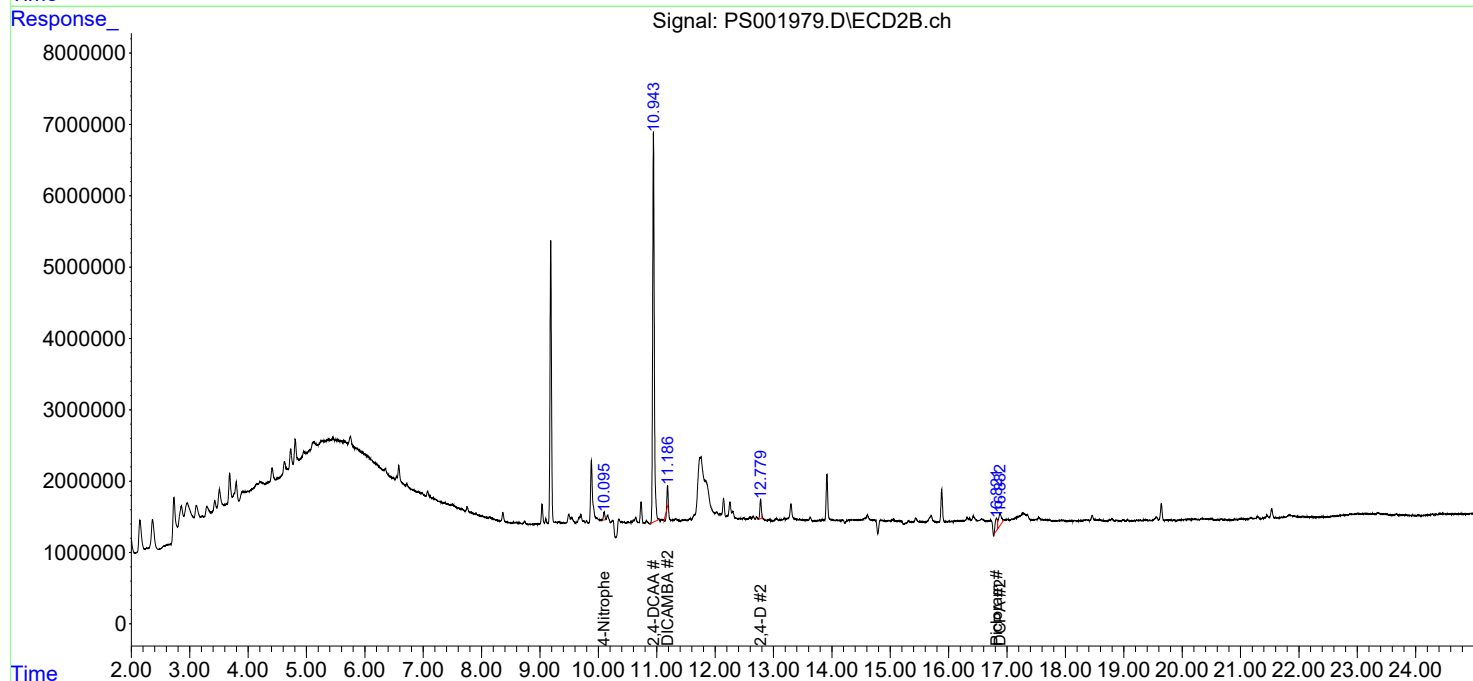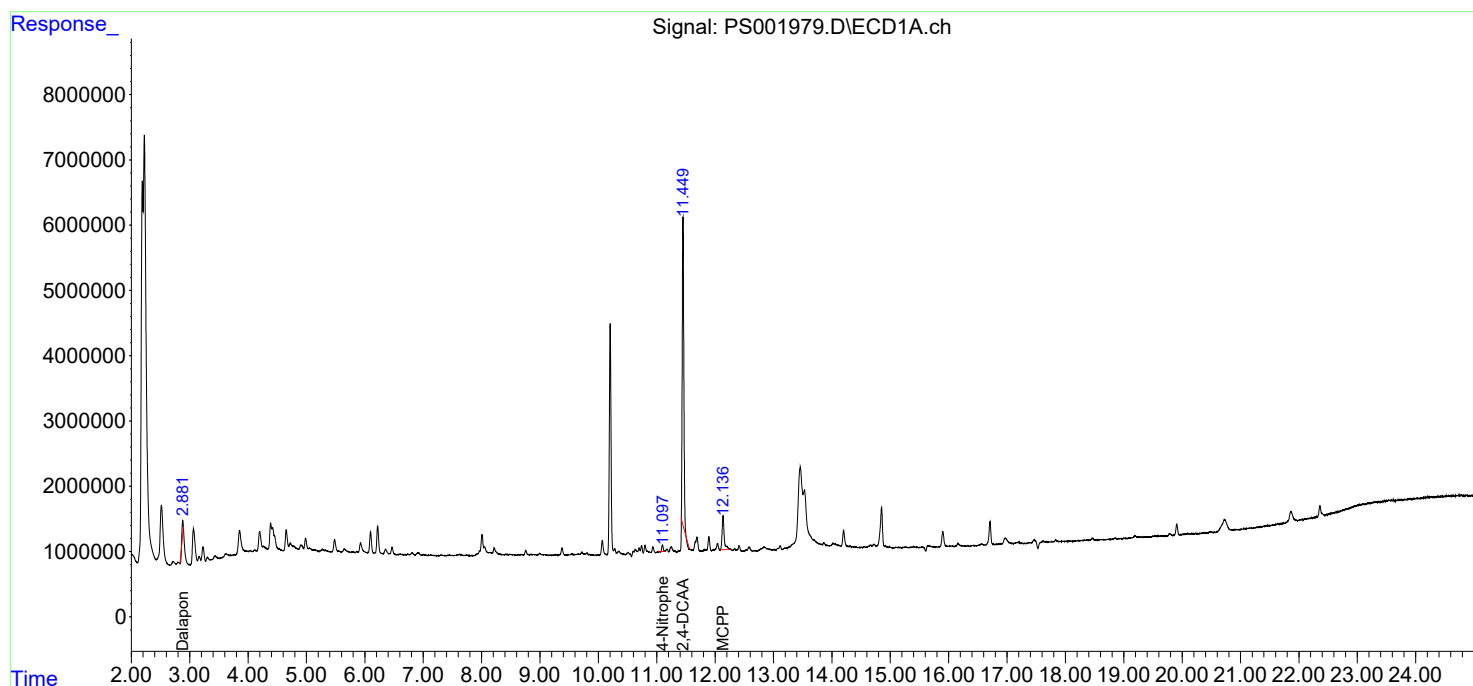


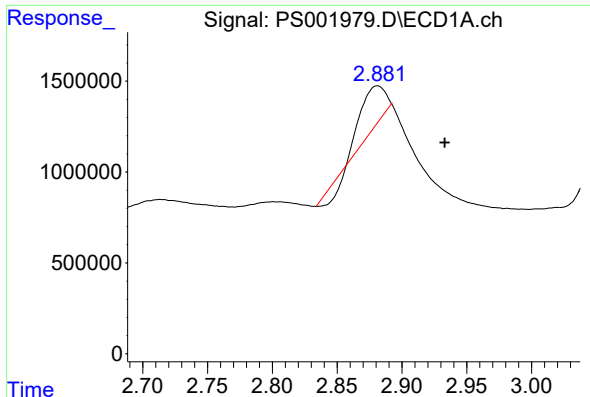

#1 Dalapon


R.T.: 2.881 min
Delta R.T.: -0.052 min
Response: 2405194
Conc: 7.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB113714TB

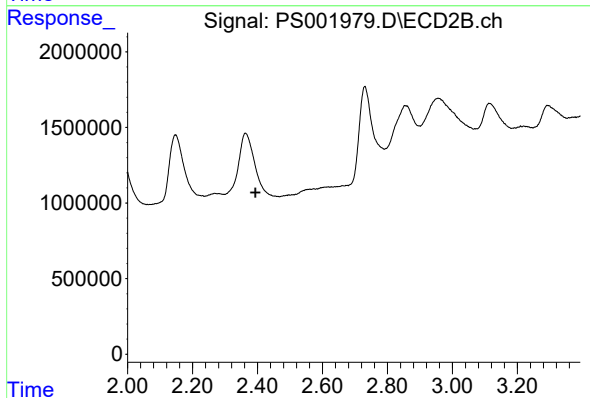


#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.394 min
Response: 0
Conc: N.D.

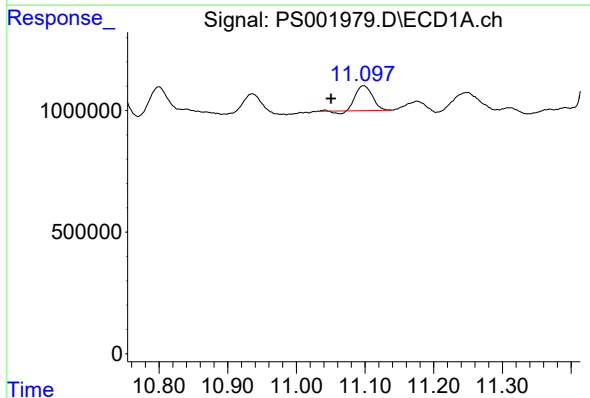


#3 4-Nitrophenol

R.T.: 11.098 min
Delta R.T.: 0.047 min
Response: 1663793
Conc: 11.82 ng/ml

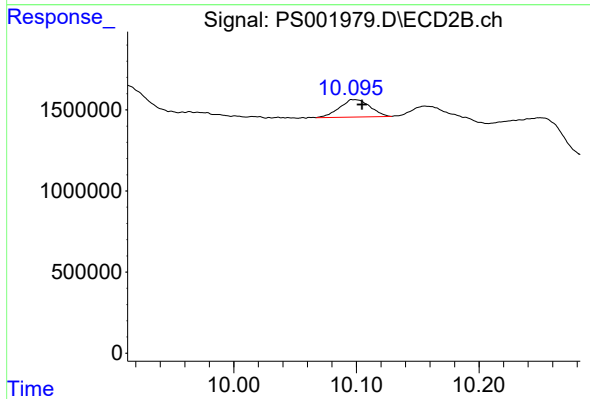

#3 4-Nitrophenol


R.T.: 10.098 min
Delta R.T.: -0.007 min
Response: 1856469
Conc: 14.80 ng/ml

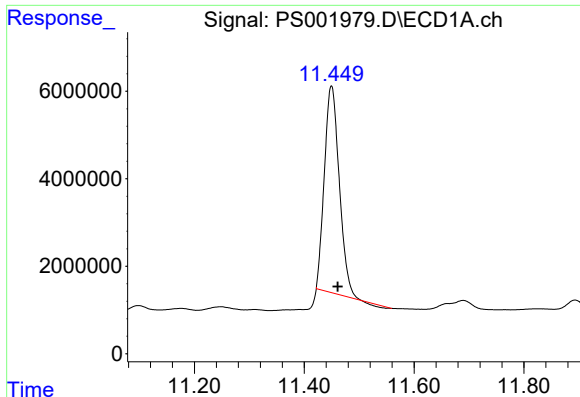

#4 2,4-DCAA


R.T.: 11.450 min
Delta R.T.: -0.012 min
Response: 87704766
Conc: 390.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB113714TB

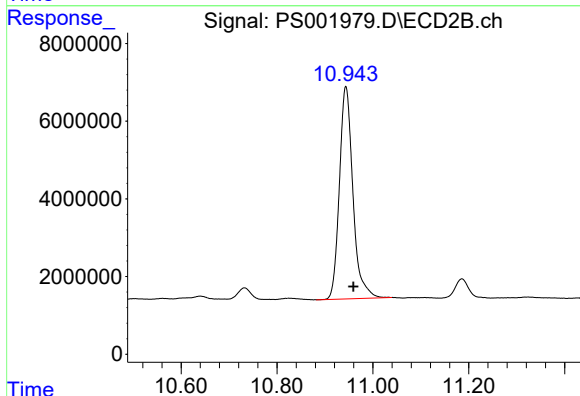


#4 2,4-DCAA

R.T.: 10.944 min
Delta R.T.: -0.016 min
Response: 106741683
Conc: 420.22 ng/ml

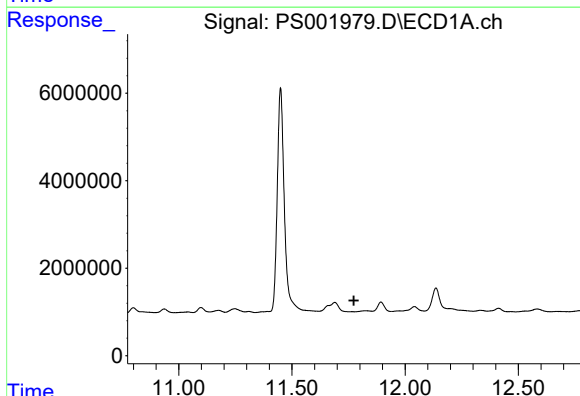


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.774 min
Response: 0
Conc: N.D.

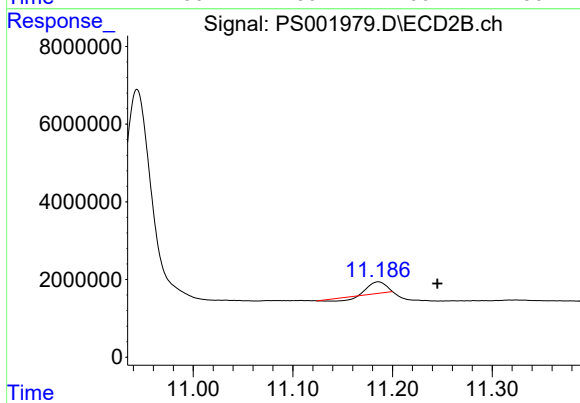

#5 DICAMBA


R.T.: 11.186 min
Delta R.T.: -0.059 min
Response: 2706382
Conc: 3.03 ng/ml

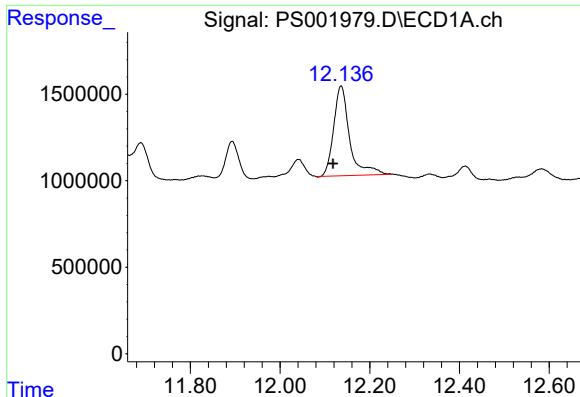

#6 MCP


R.T.: 12.136 min
Delta R.T.: 0.017 min
Response: 12835132
Conc: 20.14 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB113714TB

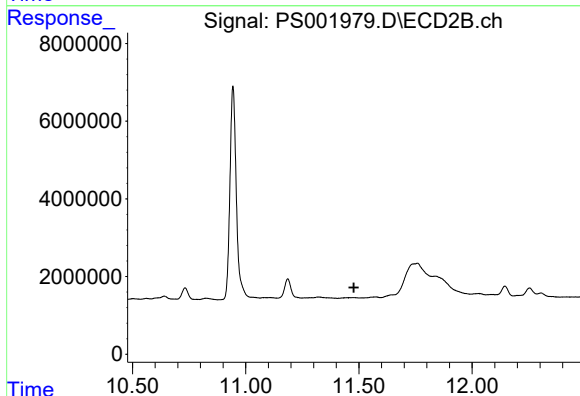


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

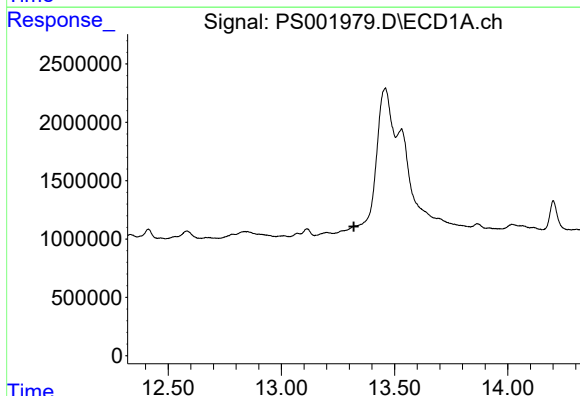


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.320 min
Response: 0
Conc: N.D.

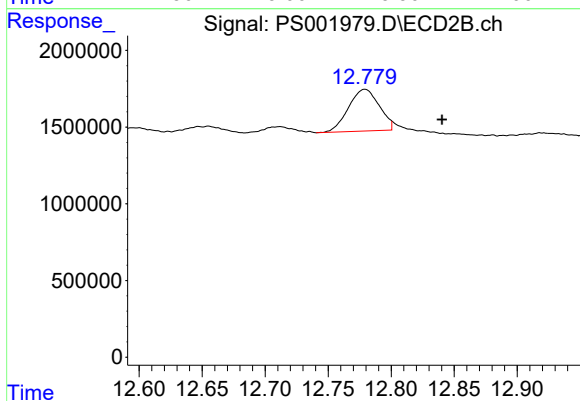

#9 2,4-D


R.T.: 12.779 min
Delta R.T.: -0.061 min
Response: 4647587
Conc: 14.94 ng/ml

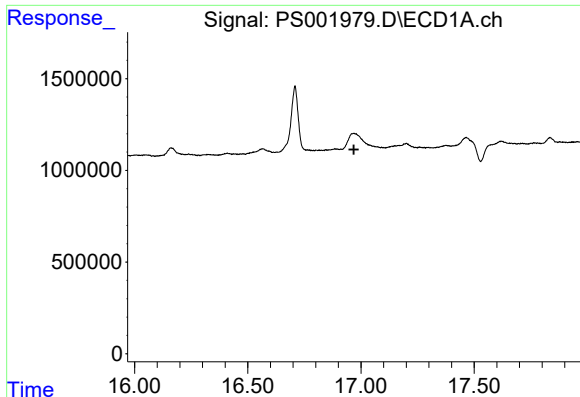

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB113714TB

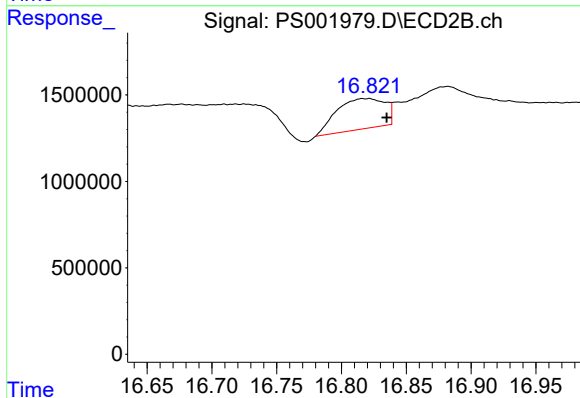


#15 Picloram

R.T.: 16.821 min
Delta R.T.: -0.014 min
Response: 4574512
Conc: 2.69 ng/ml

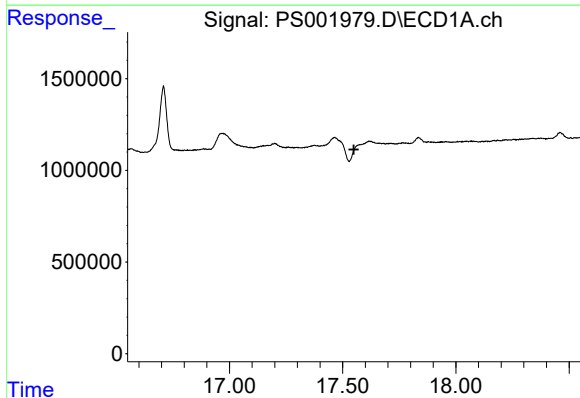

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.549 min
Response: 0
Conc: N.D.

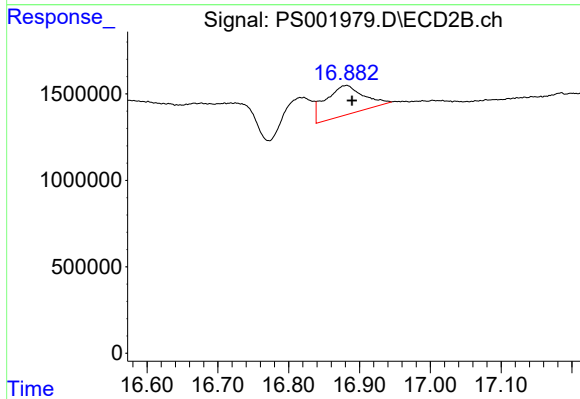

#16 DCPA

R.T.: 16.882 min
Delta R.T.: -0.007 min
Response: 6358632
Conc: 3.45 ng/ml