

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101024\
 Data File : PS027901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2024 10:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 11:49:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 07 13:46:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.095	7.623	1367.9E6	462.0E6	507.711	464.958
Target Compounds							
1) T	Dalapon	2.548	2.608	39056595	545870	8.703	<MDL #
2) T	3,5-DICHL...	6.280	0.000	215912	0	<MDL	N.D. #
3) T	4-Nitroph...	6.893	0.000	11900235	0	6.518	N.D. #
5) T	DICAMBA	0.000	7.809	0	4968937	N.D.	1.429
6) T	MCPD	0.000	7.917	0	1198416	N.D.	<MDL
7) T	MCPA	7.584	8.144	695989	8392663	<MDL	1.678 #
8) T	DICHLORPROP	7.946	8.567f	463804	2328921	<MDL	2.360 #
11) T	2,4,5-TP ...	9.002f	9.750	6310374	1456897	<MDL	<MDL #
12) T	2,4,5-T	9.326	10.139	301898	2675863	<MDL	<MDL #
14) T	DINOSEB	11.054	0.000	2294787	0	<MDL	N.D. #
15) T	Picloram	10.879	12.179	21606724	2279248	1.004	<MDL #
16) T	DCPA	11.355	12.105	1342769	2224452	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101024\
Data File : PS027901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2024 10:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 11:49:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

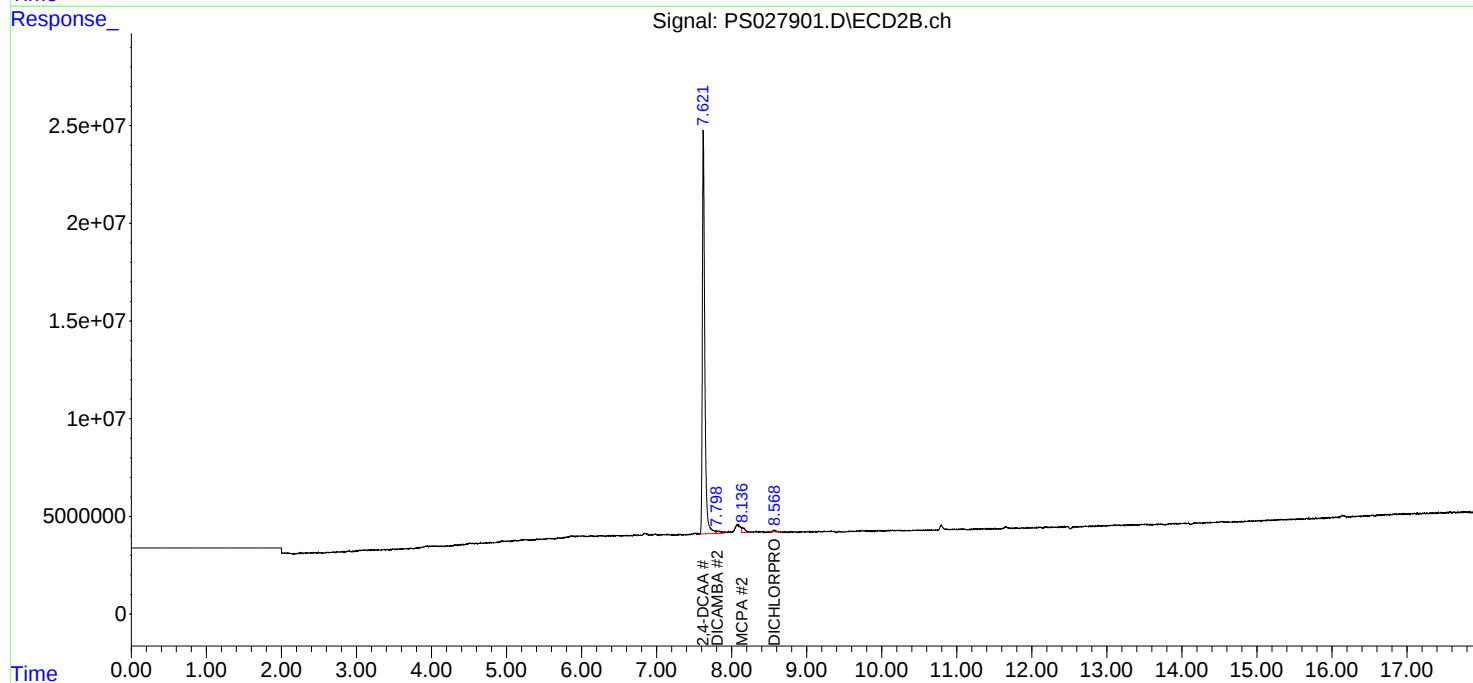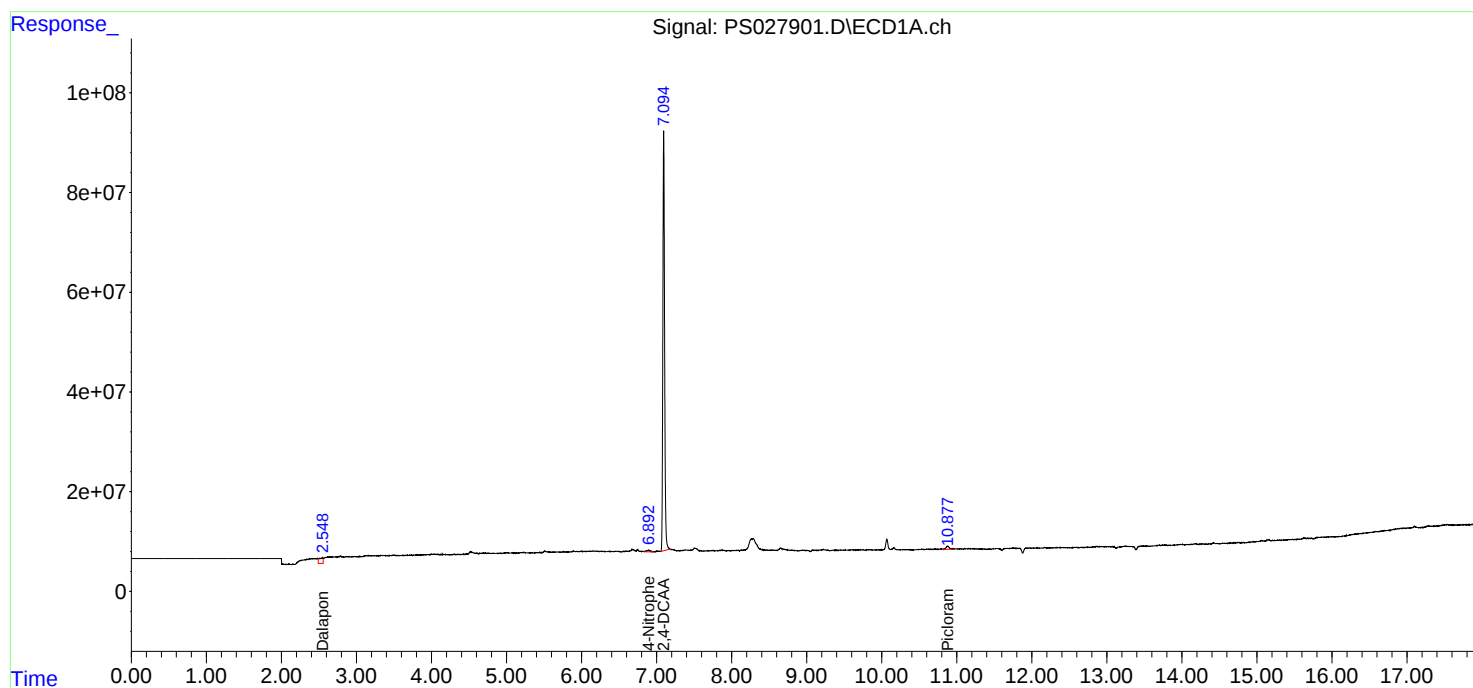


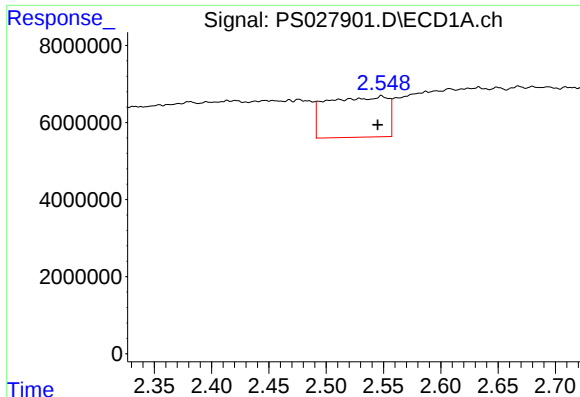

#1 Dalapon


R.T.: 2.548 min
Delta R.T.: 0.003 min
Response: 39056595
Conc: 8.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

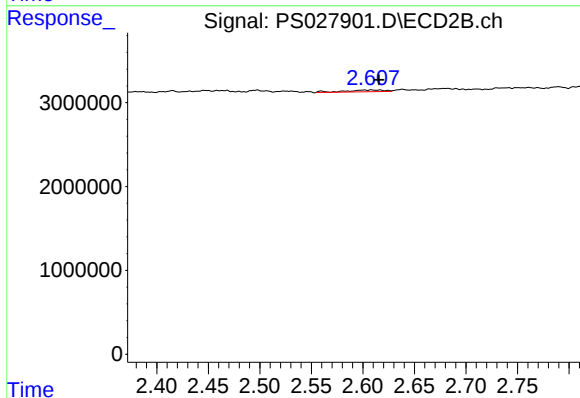


#1 Dalapon

R.T.: 2.608 min
Delta R.T.: -0.007 min
Response: 545870
Conc: N.D.

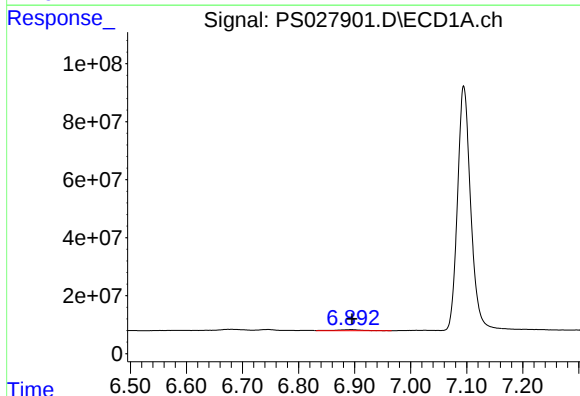


#3 4-Nitrophenol

R.T.: 6.893 min
Delta R.T.: -0.003 min
Response: 11900235
Conc: 6.52 ng/ml

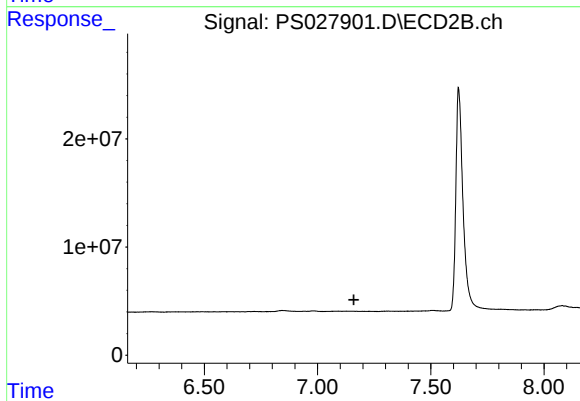

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.160 min
Response: 0
Conc: N.D.

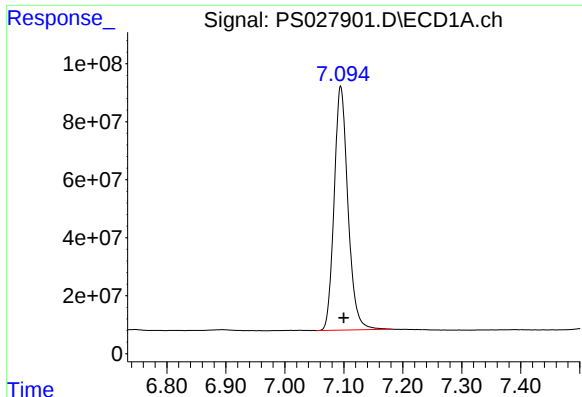

#4 2,4-DCAA


R.T.: 7.095 min
Delta R.T.: -0.005 min
Response: 1367921576
Conc: 507.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

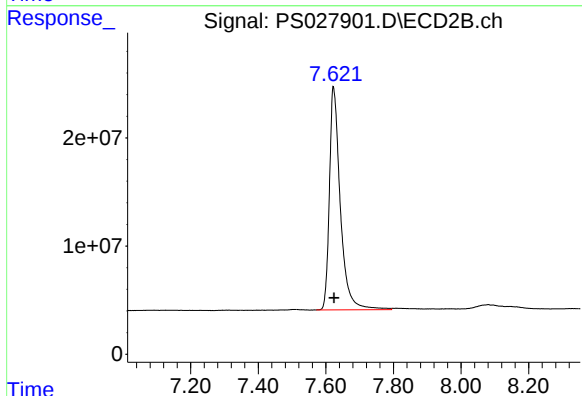


#4 2,4-DCAA

R.T.: 7.623 min
Delta R.T.: -0.002 min
Response: 462022212
Conc: 464.96 ng/ml

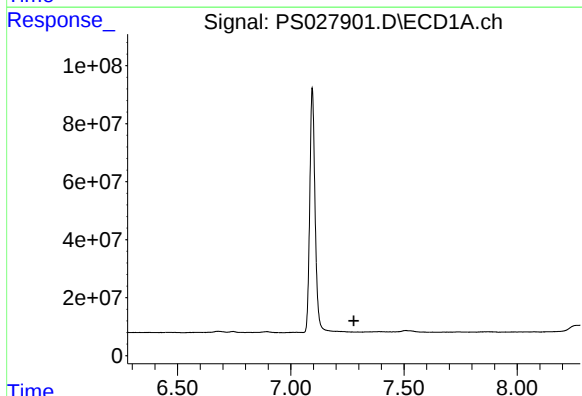


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.279 min
Response: 0
Conc: N.D.

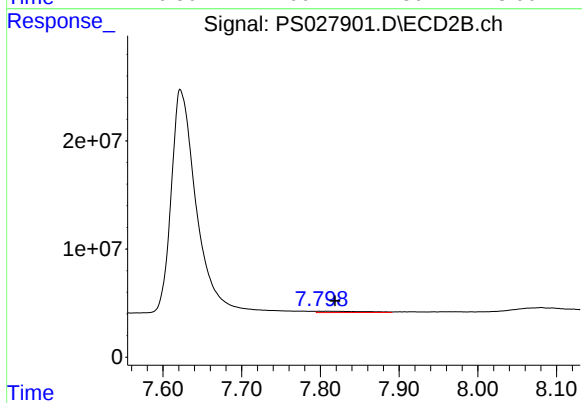

#5 DICAMBA


R.T.: 7.809 min
Delta R.T.: -0.010 min
Response: 4968937
Conc: 1.43 ng/ml

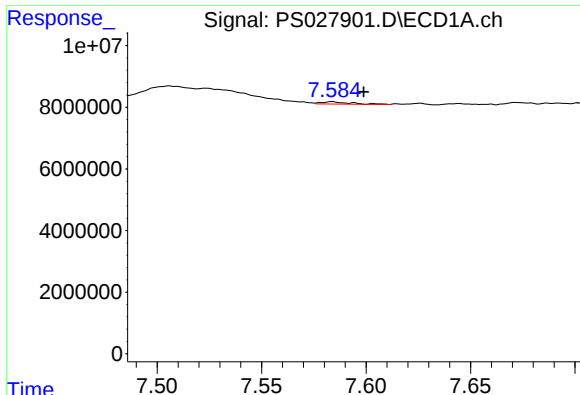

#7 MCPA


R.T.: 7.584 min
Delta R.T.: -0.015 min
Response: 695989
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

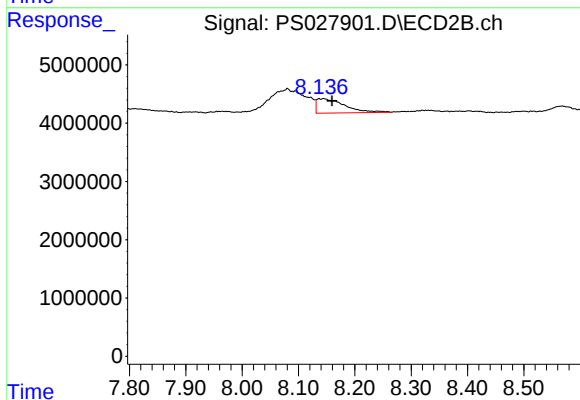


#7 MCPA

R.T.: 8.144 min
Delta R.T.: -0.016 min
Response: 8392663
Conc: 1.68 ug/ml

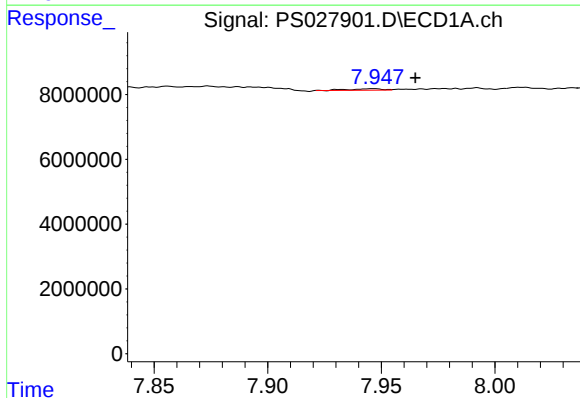


#8 DICHLORPROP

R.T.: 7.946 min
Delta R.T.: -0.019 min
Response: 463804
Conc: N.D.

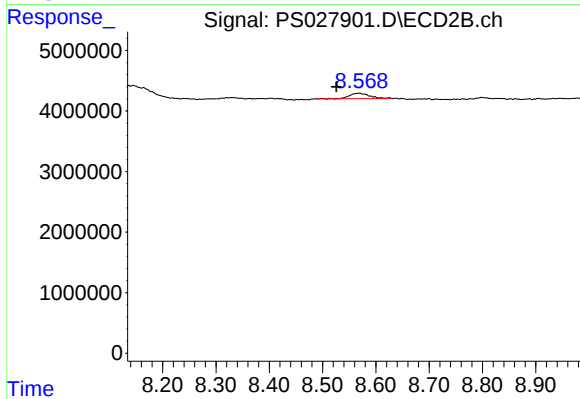

#8 DICHLORPROP


R.T.: 8.567 min
Delta R.T.: 0.042 min
Response: 2328921
Conc: 2.36 ng/ml

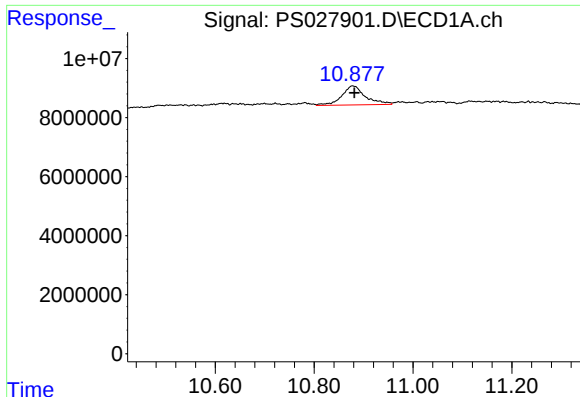

#15 Picloram

R.T.: 10.879 min
Delta R.T.: -0.003 min
Response: 21606724
Conc: 1.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

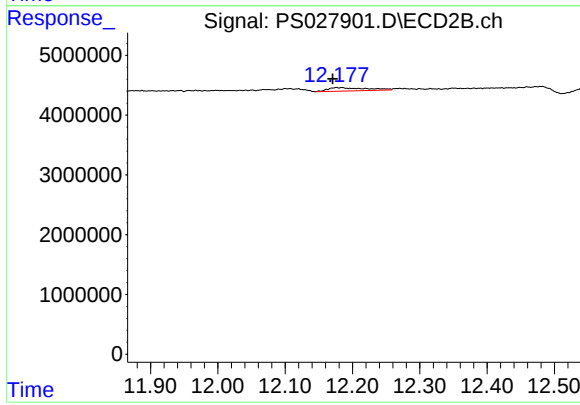

#15 Picloram

R.T.: 12.179 min
Delta R.T.: 0.009 min
Response: 2279248
Conc: N.D.