

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101121\
 Data File : PS017048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2021 11:53
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 04:14:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.160	0.000	14053370	0	9.224	N.D.	#
Target Compounds								
5) T	DICAMBA	7.346	0.000	4239522	0	<MDL	N.D.	#
6) T	MCPD	7.537	0.000	1560689	0	<MDL	N.D.	#
7) T	MCPA	7.691	0.000	1337300	0	<MDL	N.D.	#
9) T	2,4-D	8.268	0.000	4397586	0	2.501	N.D.	#
10) T	Pentachlo...	8.571	0.000	10186433	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.120	0.000	7600702	0	<MDL	N.D.	#
12) T	2,4,5-T	9.405	9.023	15386882	20222658	1.864	6.214	#
14) T	DINOSEB	11.104	0.000	8483543	0	1.392	N.D.	#
15) T	Picloram	10.929	10.779	216.2E6	71299104	18.165	16.621	
16) T	DCPA	11.371	10.779	12533565	71299104	1.221	16.357	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101121\
Data File : PS017048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2021 11:53
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 04:14:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

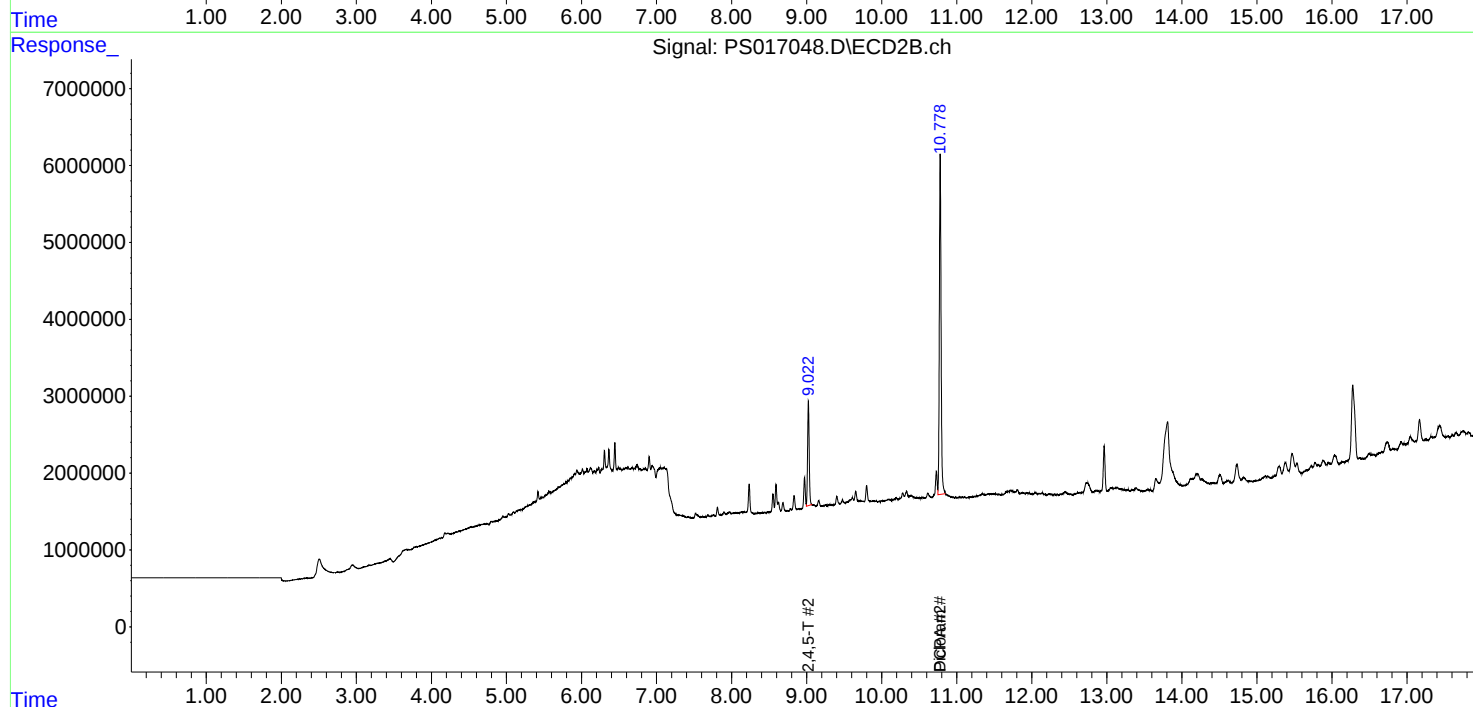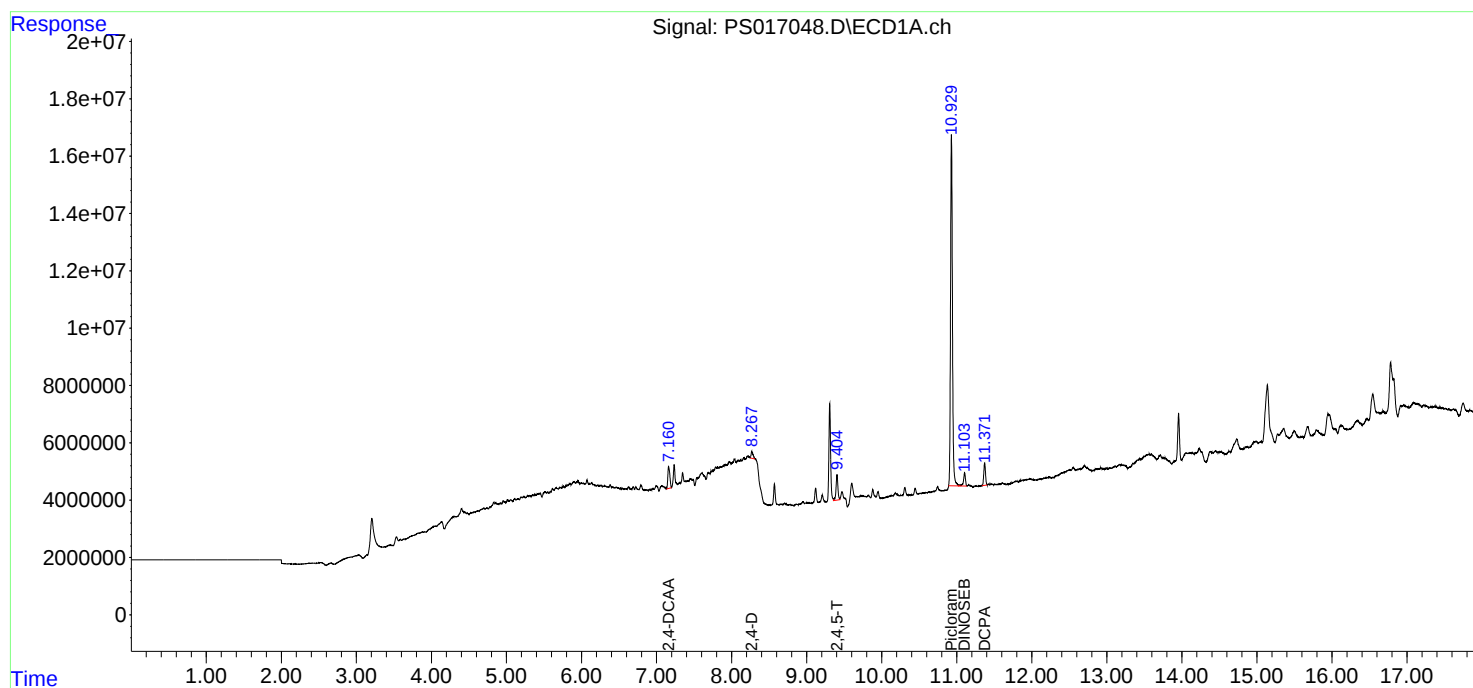


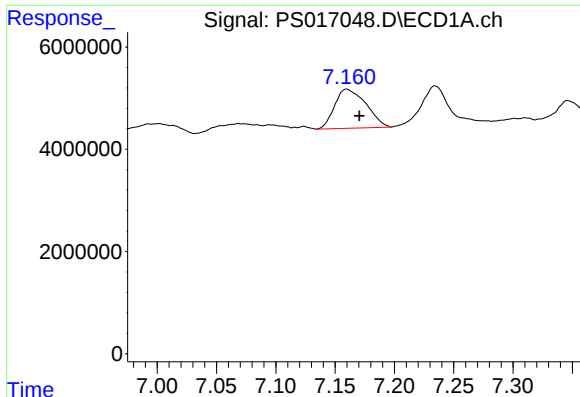

#4 2,4-DCAA


R.T.: 7.160 min
Delta R.T.: -0.011 min
Response: 14053370
Conc: 9.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

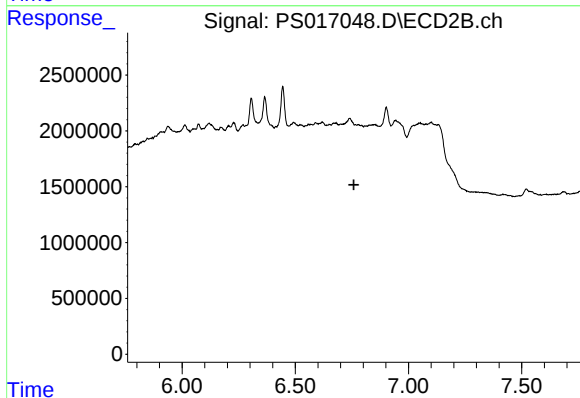


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

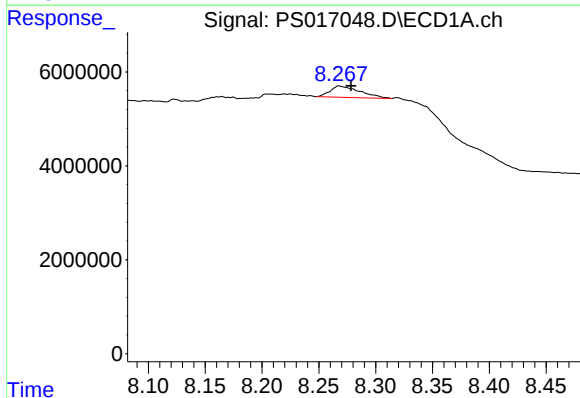


#9 2,4-D

R.T.: 8.268 min
Delta R.T.: -0.011 min
Response: 4397586
Conc: 2.50 ng/ml

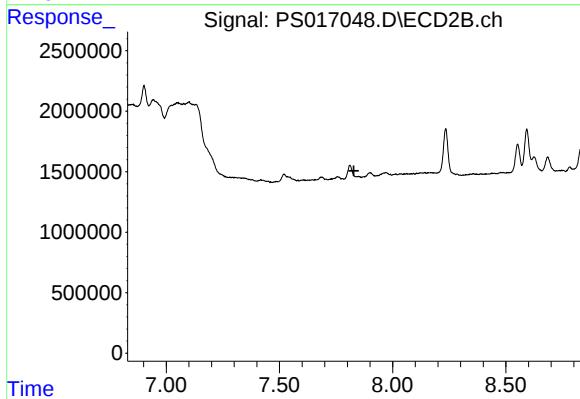

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.829 min
Response: 0
Conc: N.D.

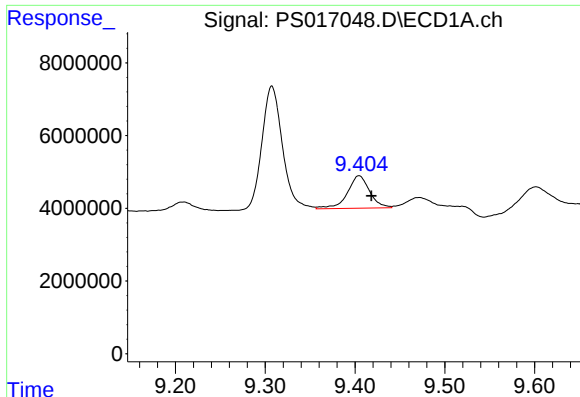

#12 2,4,5-T


R.T.: 9.405 min
Delta R.T.: -0.014 min
Response: 15386882
Conc: 1.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

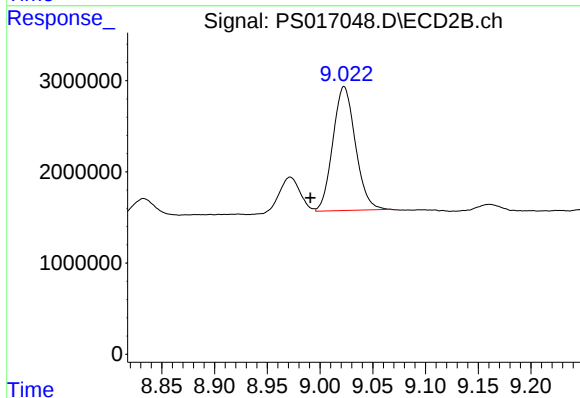


#12 2,4,5-T

R.T.: 9.023 min
Delta R.T.: 0.032 min
Response: 20222658
Conc: 6.21 ng/ml

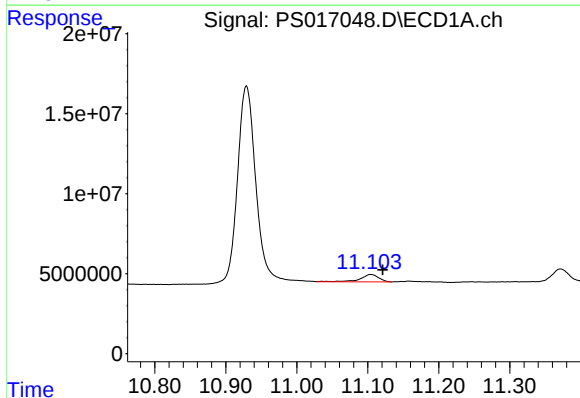


#14 DINOSEB

R.T.: 11.104 min
Delta R.T.: -0.017 min
Response: 8483543
Conc: 1.39 ng/ml

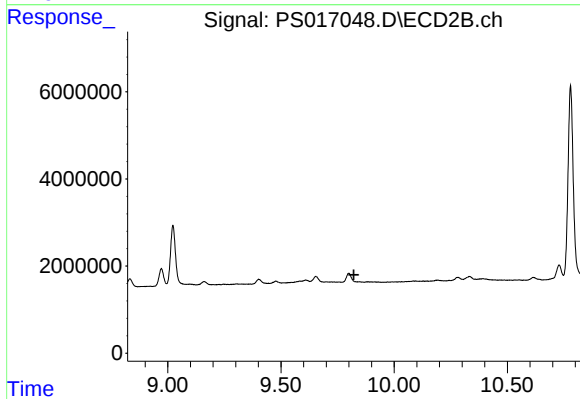

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.822 min
Response: 0
Conc: N.D.

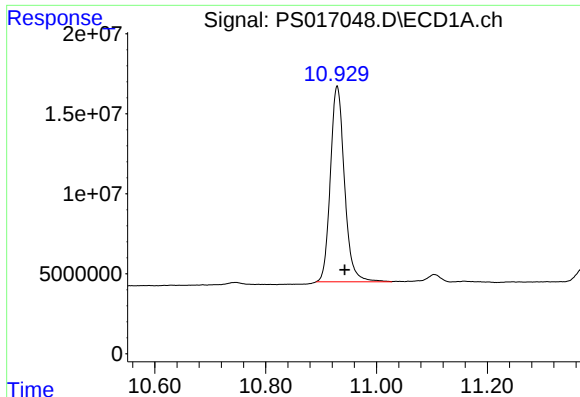

#15 Picloram


R.T.: 10.929 min
Delta R.T.: -0.014 min
Response: 216192865
Conc: 18.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

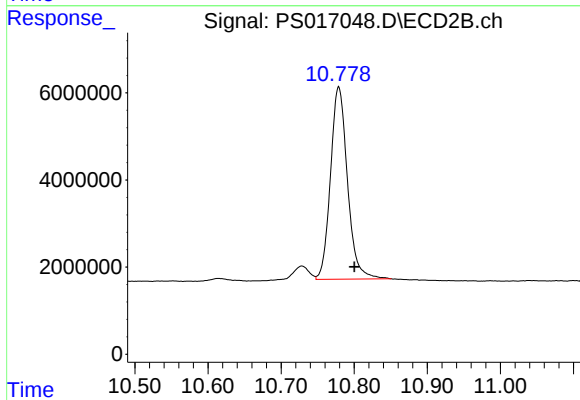


#15 Picloram

R.T.: 10.779 min
Delta R.T.: -0.022 min
Response: 71299104
Conc: 16.62 ng/ml

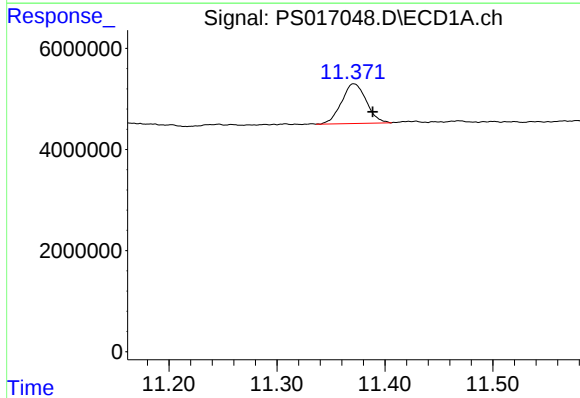

#16 DCPA

R.T.: 11.371 min
Delta R.T.: -0.017 min
Response: 12533565
Conc: 1.22 ng/ml

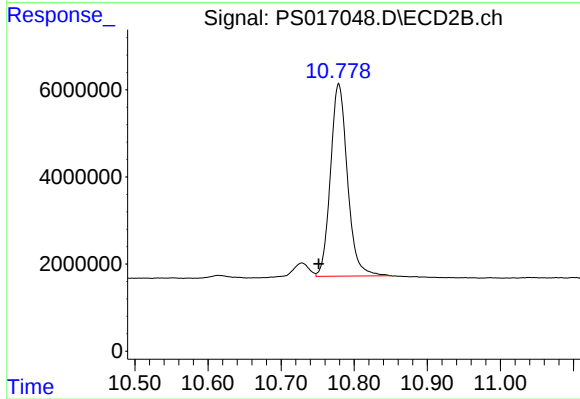

#16 DCPA

R.T.: 10.779 min
Delta R.T.: 0.027 min
Response: 71299104
Conc: 16.36 ng/ml