

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101121\
 Data File : PS017061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2021 18:58
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 04:18:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.746	650.3E6	277.8E6	426.855	473.779
Target Compounds							
7) T	MCPA	7.617f	0.000	5420899	0	<MDL	N.D. #
9) T	2,4-D	8.338f	0.000	110.6E6	0	62.888	N.D. #
11) T	2,4,5-TP ...	9.180f	0.000	34681617	0	4.343	N.D. #
12) T	2,4,5-T	9.473f	0.000	51157577	0	6.198	N.D. #
13) T	2,4-DB	9.950	0.000	2891154	0	1.749	N.D. #
14) T	DINOSEB	11.066f	0.000	9547356	0	1.567	N.D. #
15) T	Picloram	10.949	0.000	3789061	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101121\
Data File : PS017061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2021 18:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 04:18:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

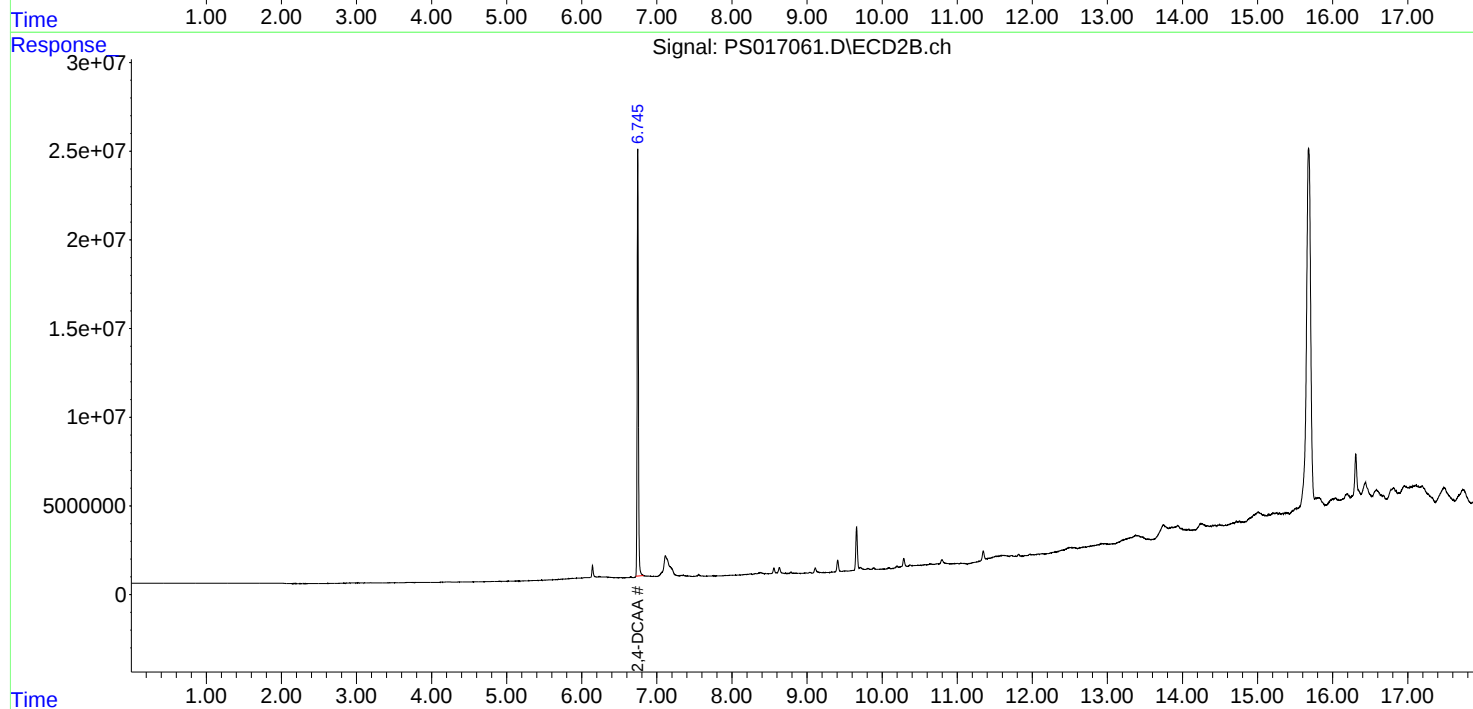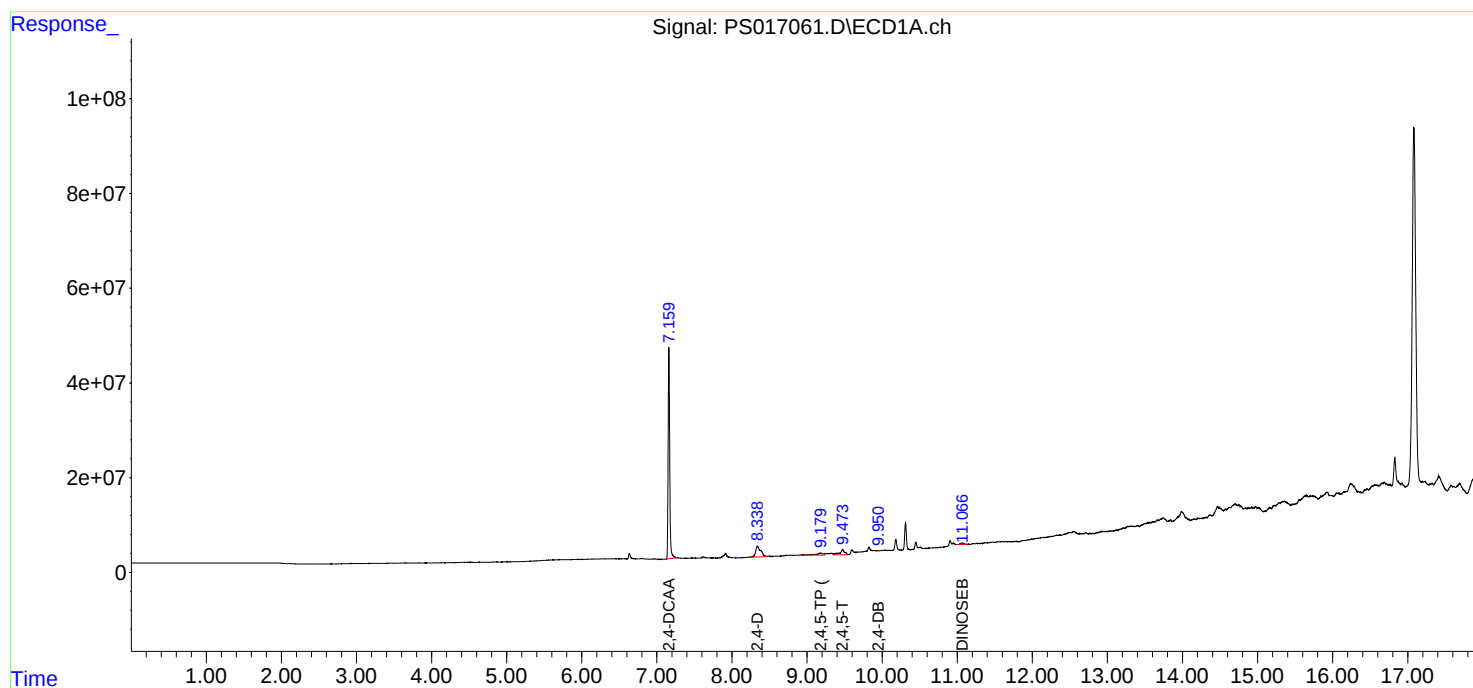


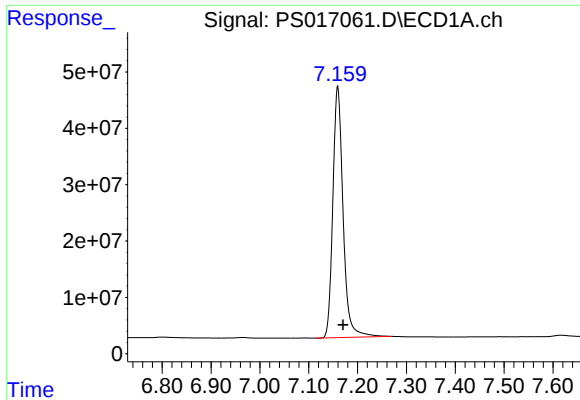

#4 2,4-DCAA


R.T.: 7.159 min
Delta R.T.: -0.011 min
Response: 650335146
Conc: 426.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

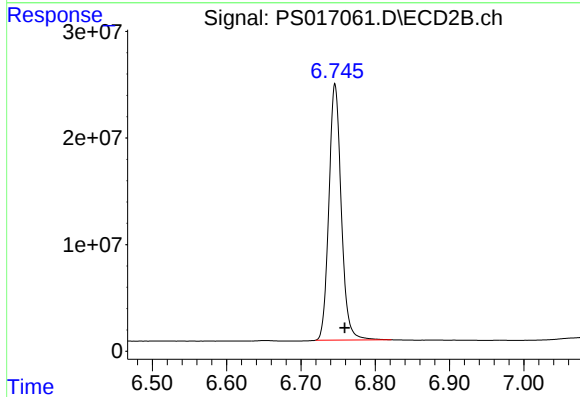


#4 2,4-DCAA

R.T.: 6.746 min
Delta R.T.: -0.013 min
Response: 277806225
Conc: 473.78 ng/ml

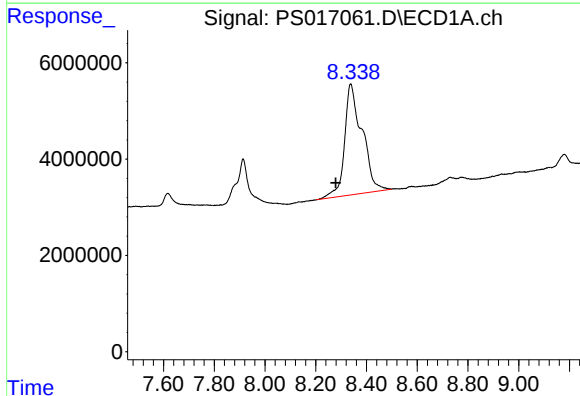


#9 2,4-D

R.T.: 8.338 min
Delta R.T.: 0.060 min
Response: 110573190
Conc: 62.89 ng/ml

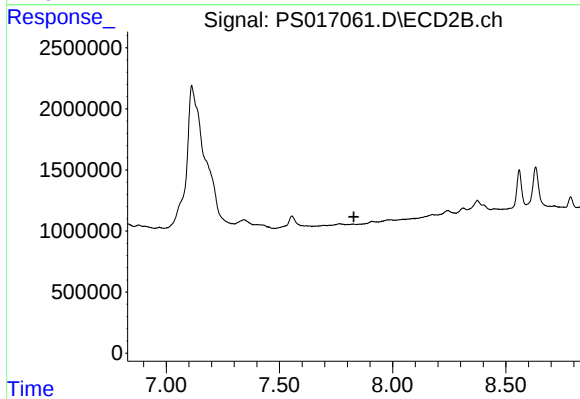

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.829 min
Response: 0
Conc: N.D.

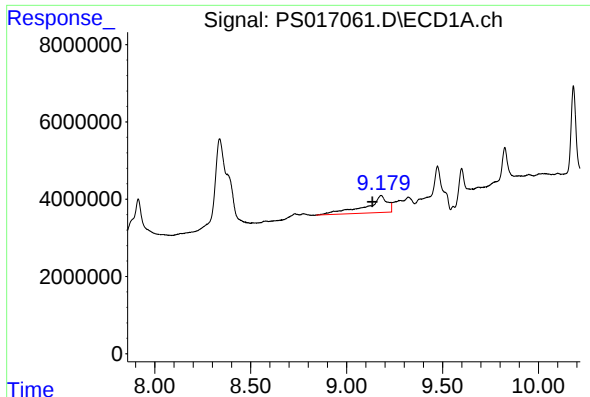

#11 2,4,5-TP (SILVEX)


R.T.: 9.180 min
Delta R.T.: 0.046 min
Response: 34681617
Conc: 4.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

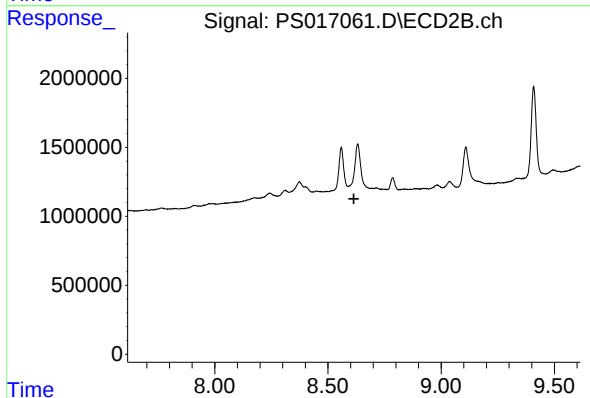


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.614 min
Response: 0
Conc: N.D.

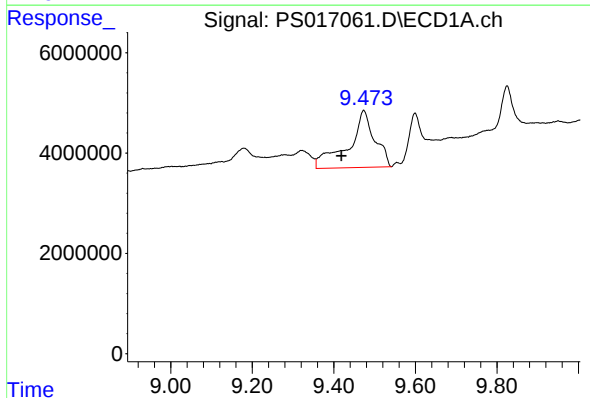


#12 2,4,5-T

R.T.: 9.473 min
Delta R.T.: 0.055 min
Response: 51157577
Conc: 6.20 ng/ml

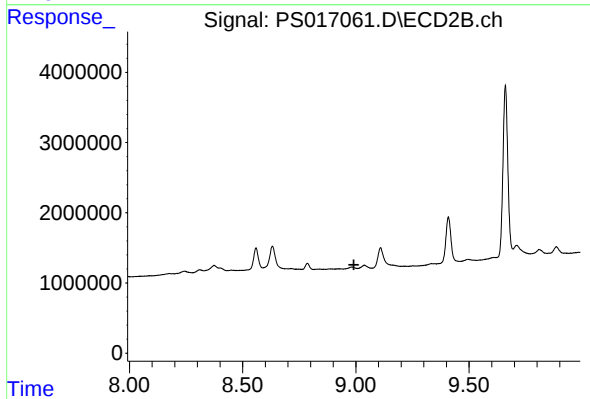

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.

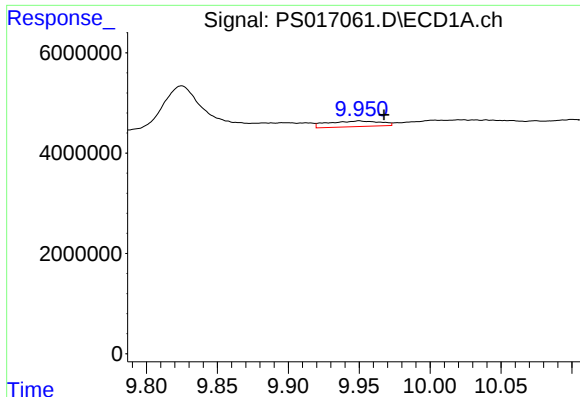

#13 2,4-DB


R.T.: 9.950 min
Delta R.T.: -0.018 min
Response: 2891154
Conc: 1.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

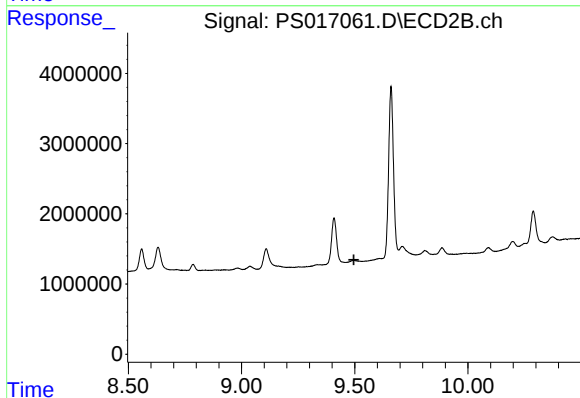


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.496 min
Response: 0
Conc: N.D.

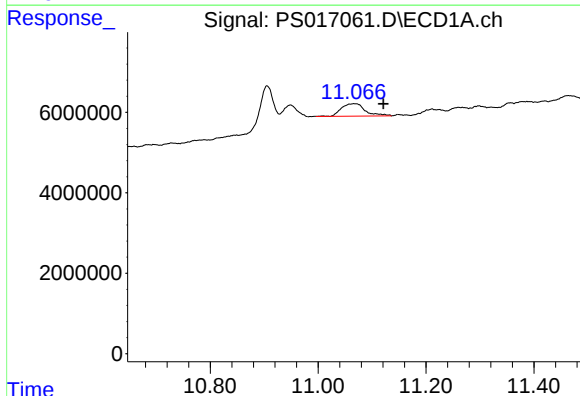

#14 DINOSEB

R.T.: 11.066 min
Delta R.T.: -0.055 min
Response: 9547356
Conc: 1.57 ng/ml

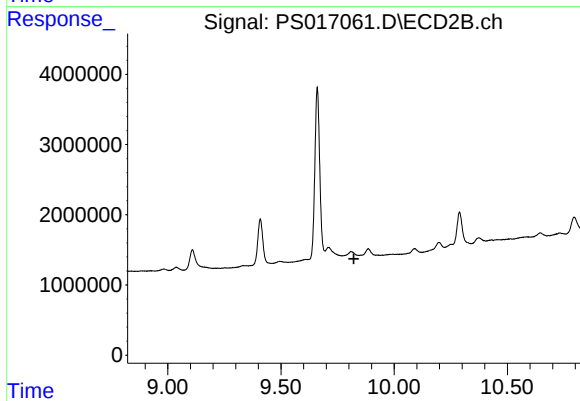

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.822 min
Response: 0
Conc: N.D.