

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101121\
 Data File : PS017070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2021 22:35
 Operator : DD\AJ
 Sample : PB139805BS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 04:21:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.158	6.746	816.0E6	317.3E6	535.590	541.115
Target Compounds							
1) T	Dalapon	2.999	2.502	1157.0E6	349.2E6	485.221	480.450
2) T	3,5-DICHL...	6.381	5.941	1036.5E6	421.5E6	487.072	478.047
3) T	4-Nitroph...	6.988	6.370	436.1E6	148.8E6	503.385	475.803
5) T	DICAMBA	7.348	6.907	2997.0E6	1320.3E6	513.497	518.293
6) T	MCPD	7.516	7.002	185.1E6	102.6E6	42.722	50.079
7) T	MCPA	7.663	7.212	314.7E6	151.5E6	50.877	49.762
8) T	DICHLORPROP	8.037	7.524	754.0E6	314.9E6	510.693	485.535
9) T	2,4-D	8.265	7.814	911.1E6	354.5E6	518.201	465.990
10) T	Pentachlo...	8.571	8.239	10873.6E6	4464.9E6	538.126	542.579
11) T	2,4,5-TP ...	9.119	8.598	4214.5E6	1855.6E6	527.787	530.008
12) T	2,4,5-T	9.402	8.975	4417.0E6	1693.2E6	535.158	520.290
13) T	2,4-DB	9.950	9.479	898.7E6	222.0E6	543.699	532.896
14) T	DINOSEB	11.103	9.804	3112.6E6	1305.5E6	510.894	532.970
15) T	Picloram	10.925	10.781	5604.6E6	2131.0E6	470.907	496.757
16) T	DCPA	11.370	10.733	5382.5E6	2327.7E6	524.215	534.025



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101121\
Data File : PS017070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2021 22:35
Operator : DD\AJ
Sample : PB139805BS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 04:21:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

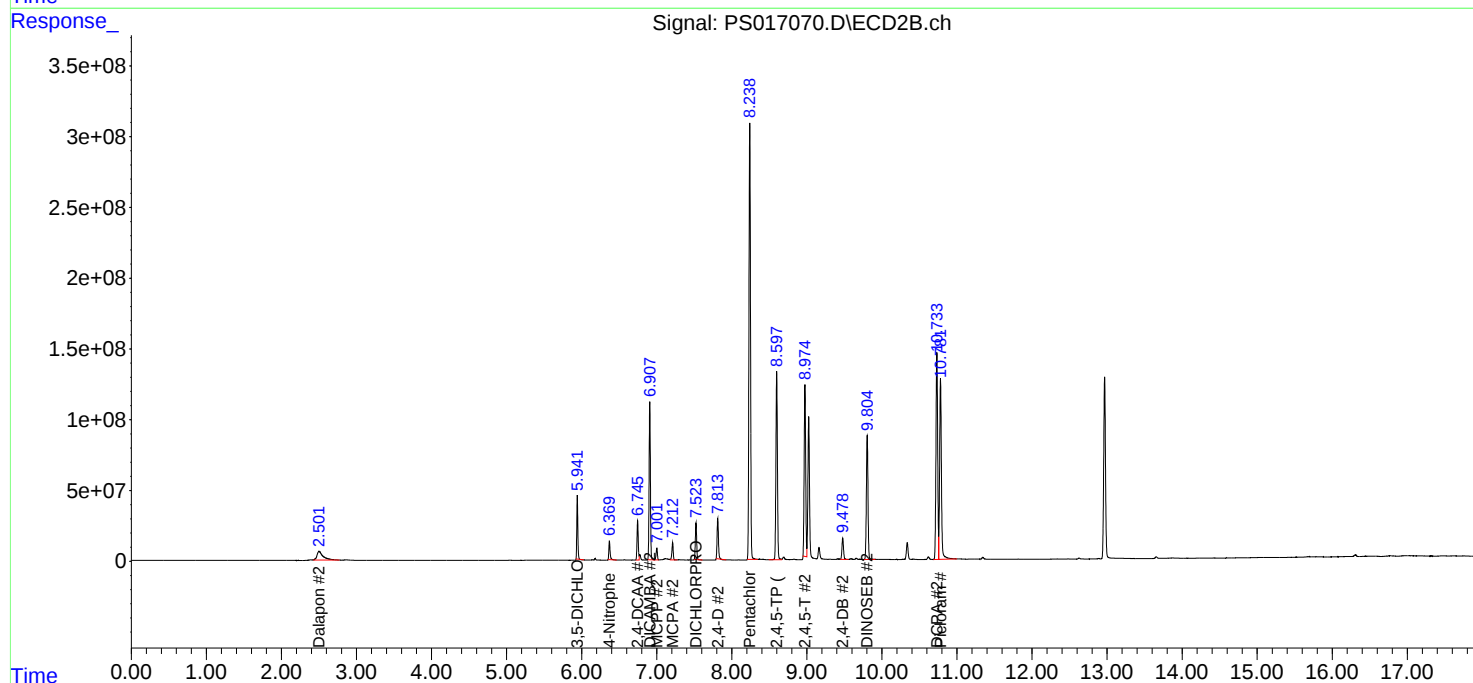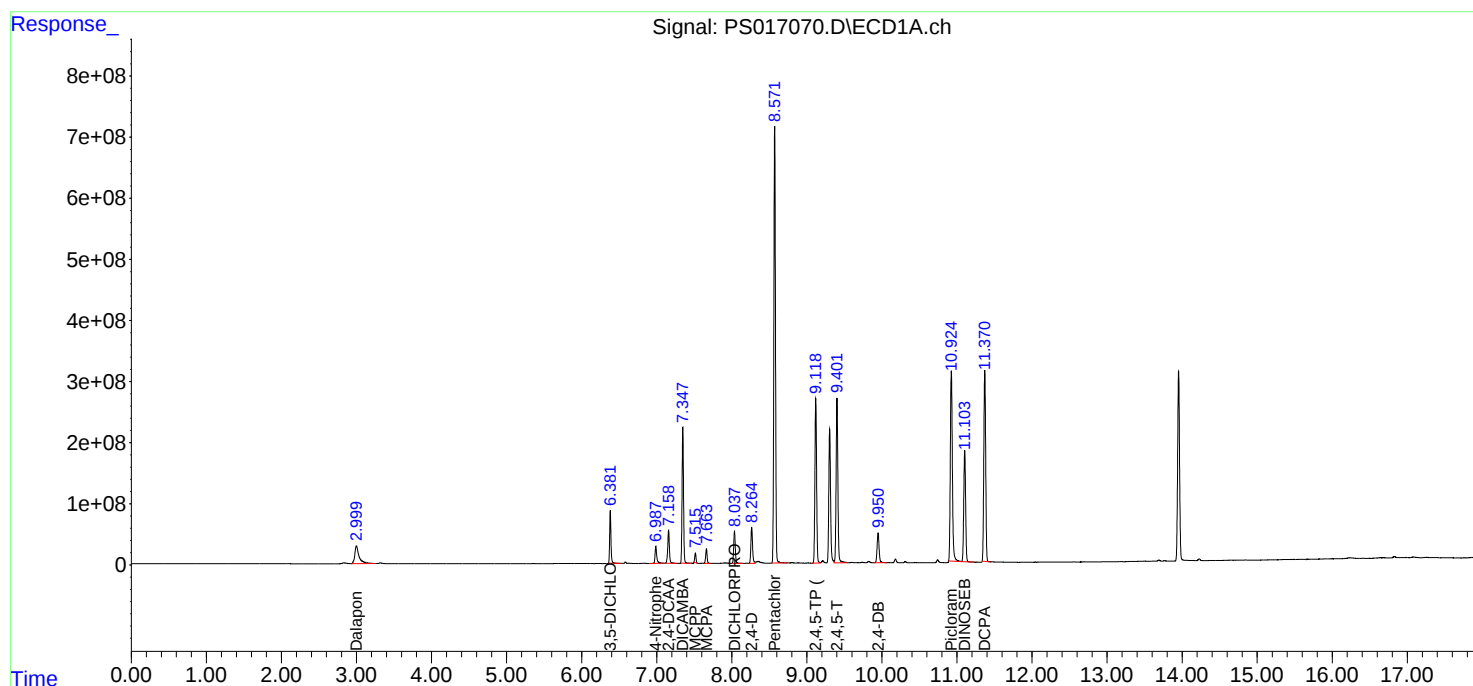


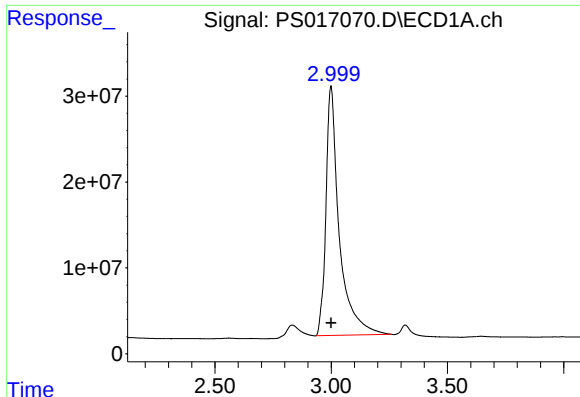

#1 Dalapon


R.T.: 2.999 min
Delta R.T.: 0.000 min
Response: 1156985437
Conc: 485.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

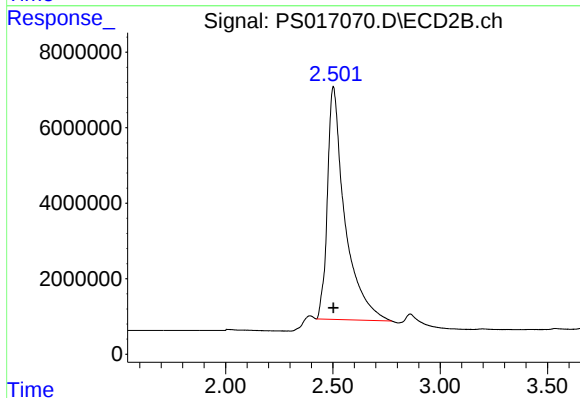


#1 Dalapon

R.T.: 2.502 min
Delta R.T.: 0.000 min
Response: 349204893
Conc: 480.45 ng/ml

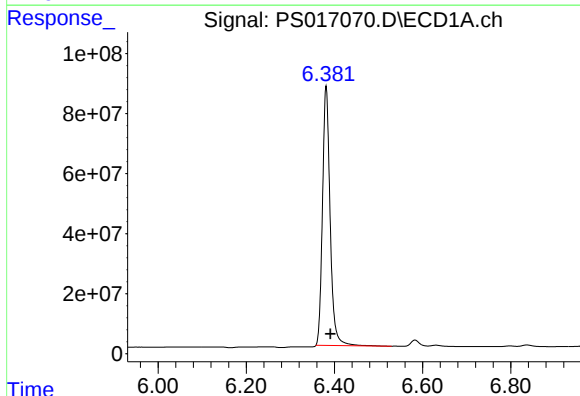


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.381 min
Delta R.T.: -0.010 min
Response: 1036537075
Conc: 487.07 ng/ml

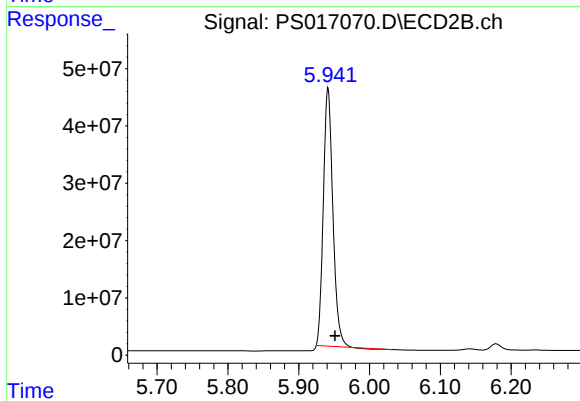

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.941 min
Delta R.T.: -0.010 min
Response: 421463599
Conc: 478.05 ng/ml

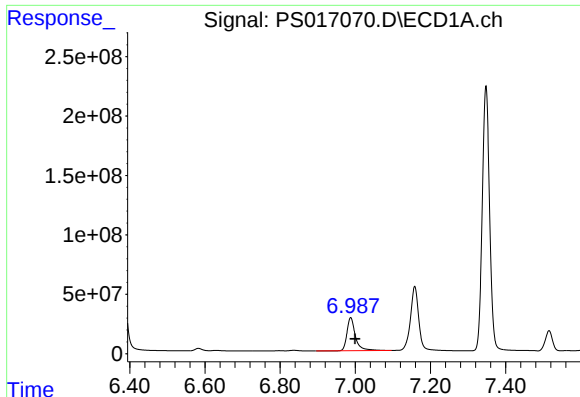

#3 4-Nitrophenol


R.T.: 6.988 min
Delta R.T.: -0.012 min
Response: 436063425
Conc: 503.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

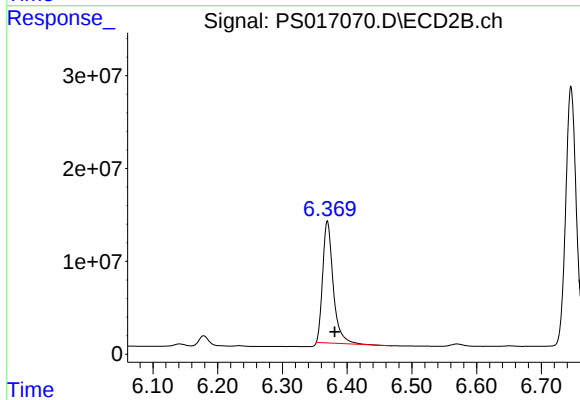


#3 4-Nitrophenol

R.T.: 6.370 min
Delta R.T.: -0.011 min
Response: 148795672
Conc: 475.80 ng/ml

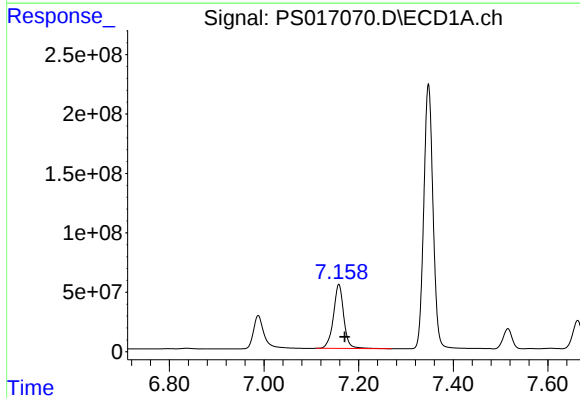


#4 2,4-DCAA

R.T.: 7.158 min
Delta R.T.: -0.012 min
Response: 815997277
Conc: 535.59 ng/ml

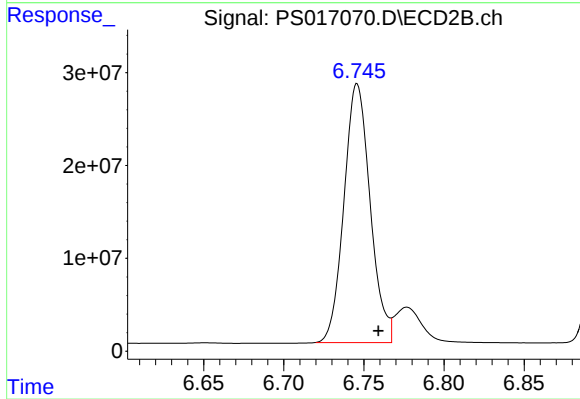

#4 2,4-DCAA


R.T.: 6.746 min
Delta R.T.: -0.013 min
Response: 317289665
Conc: 541.11 ng/ml

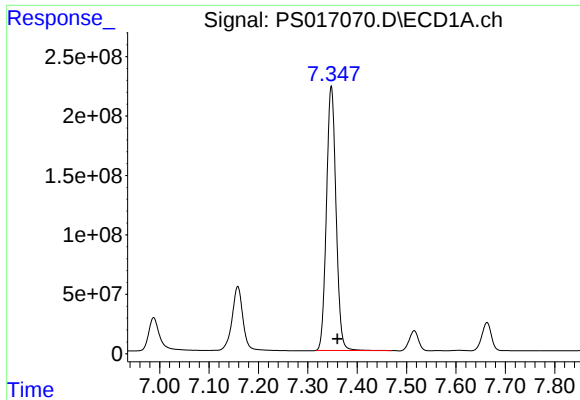

#5 DICAMBA


R.T.: 7.348 min
Delta R.T.: -0.012 min
Response: 2996982607
Conc: 513.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

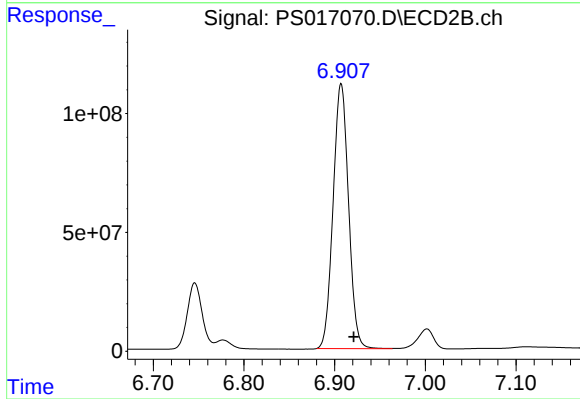


#5 DICAMBA

R.T.: 6.907 min
Delta R.T.: -0.014 min
Response: 1320322269
Conc: 518.29 ng/ml

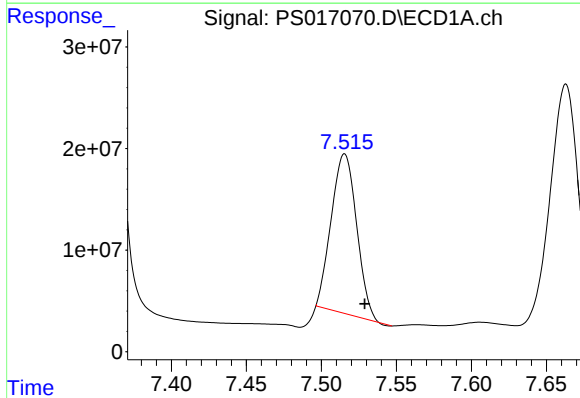


#6 MCP

R.T.: 7.516 min
Delta R.T.: -0.013 min
Response: 185099553
Conc: 42.72 ug/ml

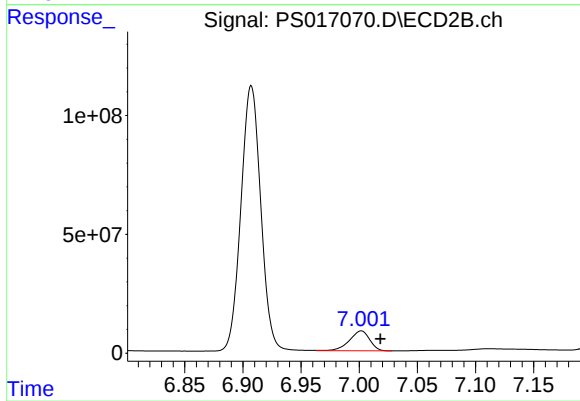

#6 MCP


R.T.: 7.002 min
Delta R.T.: -0.016 min
Response: 102589007
Conc: 50.08 ug/ml

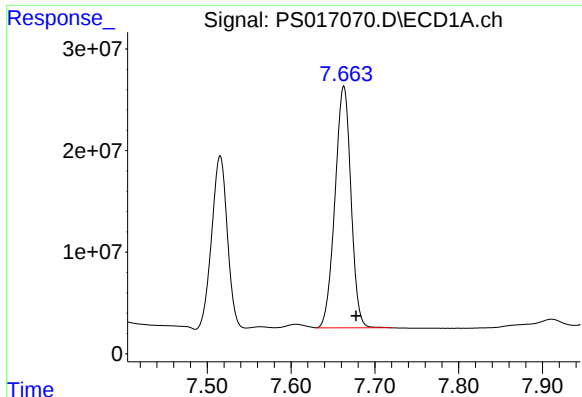

#7 MCPA


R.T.: 7.663 min
Delta R.T.: -0.015 min
Response: 314652313
Conc: 50.88 ug/ml

Instrument :
ECD_S
ClientSampleId :

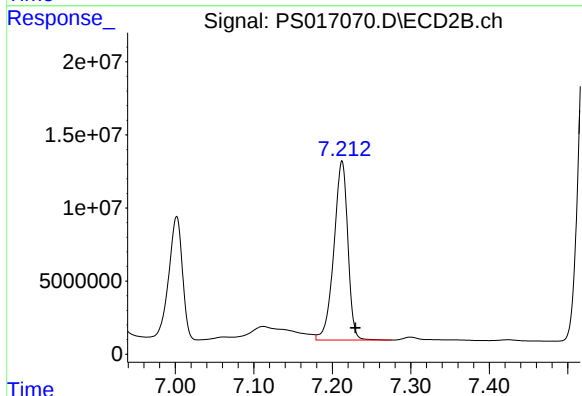


#7 MCPA

R.T.: 7.212 min
Delta R.T.: -0.017 min
Response: 151530138
Conc: 49.76 ug/ml

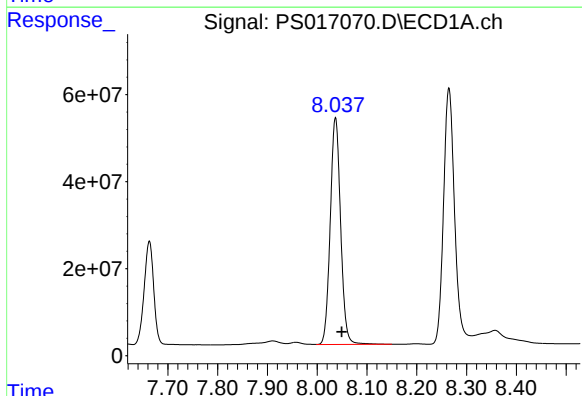


#8 DICHLORPROP

R.T.: 8.037 min
Delta R.T.: -0.013 min
Response: 754007658
Conc: 510.69 ng/ml

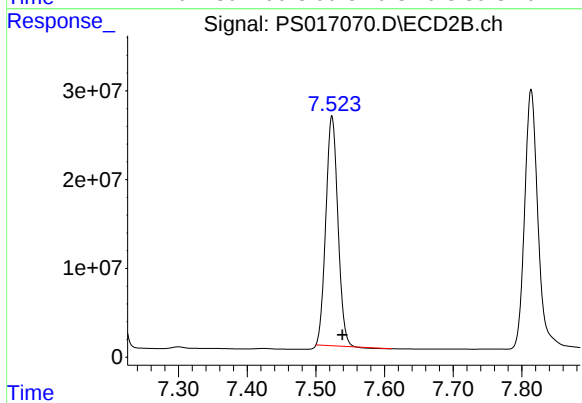

#8 DICHLORPROP


R.T.: 7.524 min
Delta R.T.: -0.015 min
Response: 314881001
Conc: 485.54 ng/ml

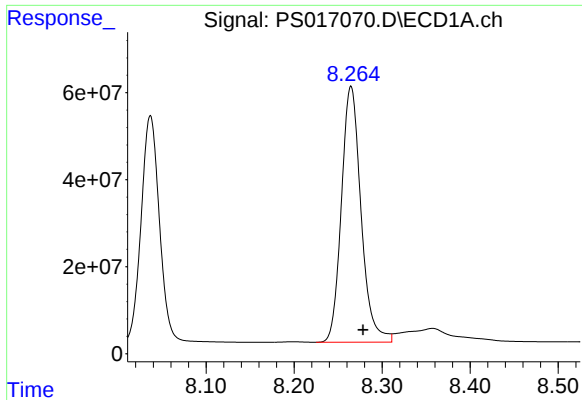

#9 2,4-D


R.T.: 8.265 min
Delta R.T.: -0.014 min
Response: 911128798
Conc: 518.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

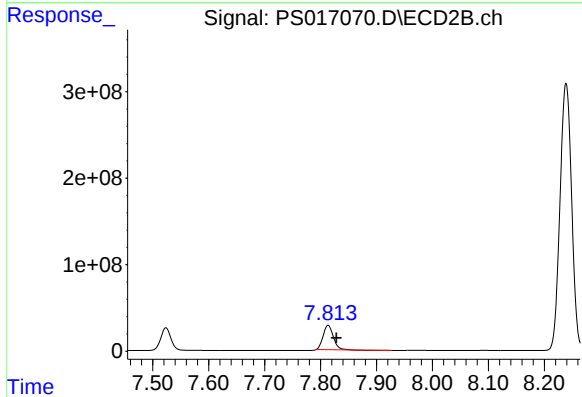


#9 2,4-D

R.T.: 7.814 min
Delta R.T.: -0.015 min
Response: 354541351
Conc: 465.99 ng/ml

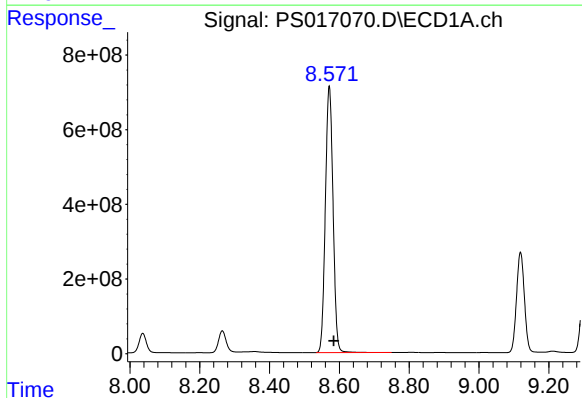


#10 Pentachlorophenol

R.T.: 8.571 min
Delta R.T.: -0.013 min
Response: 10873566512
Conc: 538.13 ng/ml

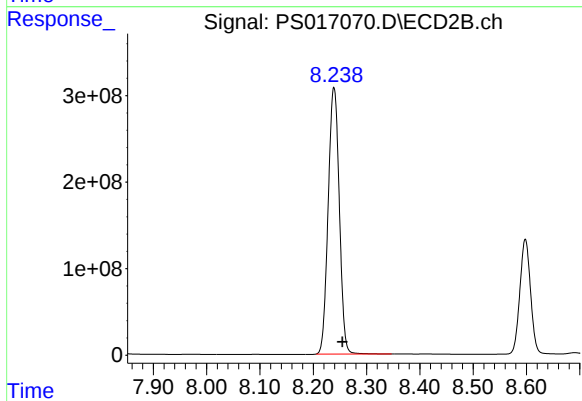

#10 Pentachlorophenol


R.T.: 8.239 min
Delta R.T.: -0.016 min
Response: 4464897337
Conc: 542.58 ng/ml

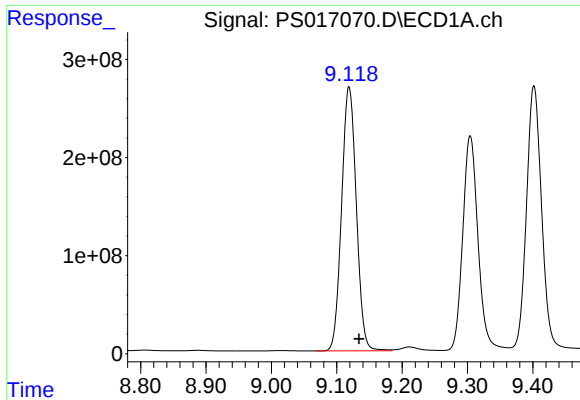

#11 2,4,5-TP (SILVEX)


R.T.: 9.119 min
Delta R.T.: -0.015 min
Response: 4214523879
Conc: 527.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

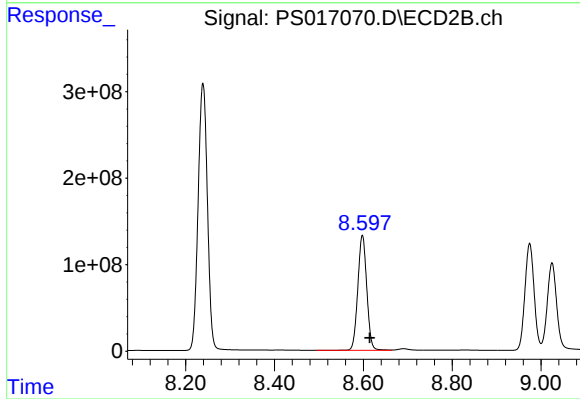


#11 2,4,5-TP (SILVEX)

R.T.: 8.598 min
Delta R.T.: -0.017 min
Response: 1855618824
Conc: 530.01 ng/ml

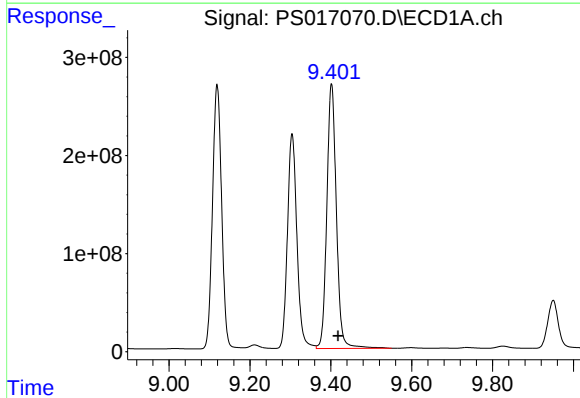


#12 2,4,5-T

R.T.: 9.402 min
Delta R.T.: -0.017 min
Response: 4416951730
Conc: 535.16 ng/ml

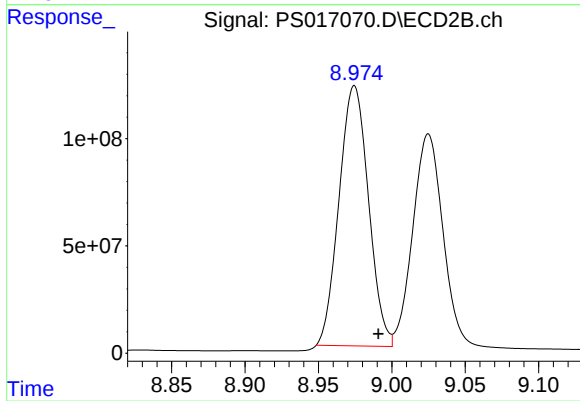

#12 2,4,5-T


R.T.: 8.975 min
Delta R.T.: -0.016 min
Response: 1693159050
Conc: 520.29 ng/ml

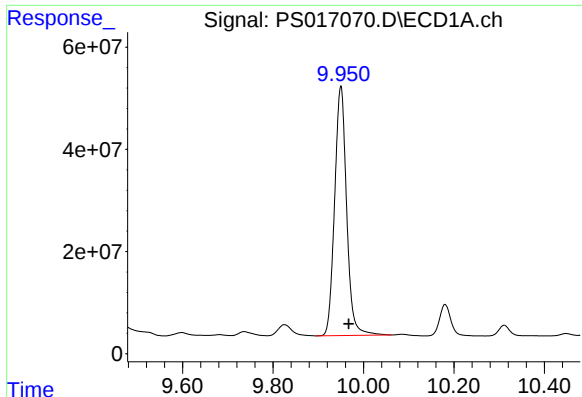

#13 2,4-DB


R.T.: 9.950 min
Delta R.T.: -0.018 min
Response: 898747852
Conc: 543.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

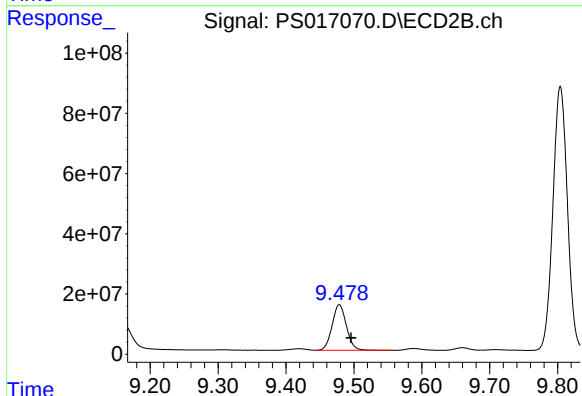


#13 2,4-DB

R.T.: 9.479 min
Delta R.T.: -0.017 min
Response: 222043961
Conc: 532.90 ng/ml

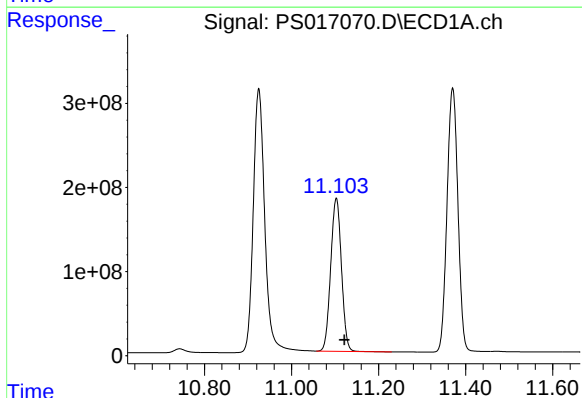


#14 DINOSEB

R.T.: 11.103 min
Delta R.T.: -0.018 min
Response: 3112649889
Conc: 510.89 ng/ml

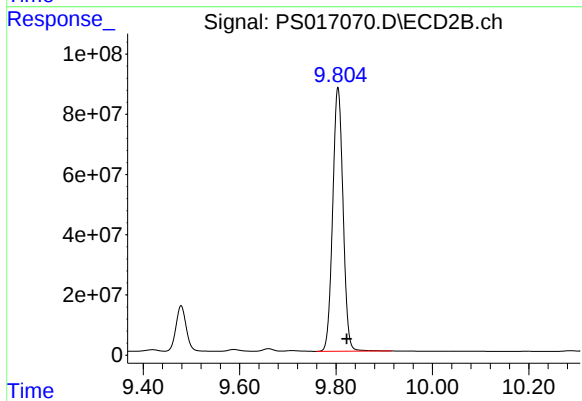

#14 DINOSEB


R.T.: 9.804 min
Delta R.T.: -0.018 min
Response: 1305532968
Conc: 532.97 ng/ml

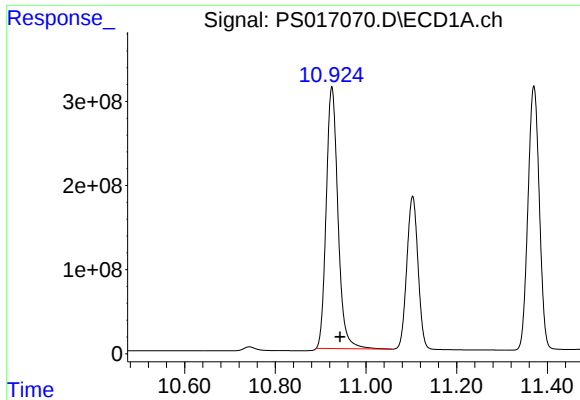

#15 Picloram


R.T.: 10.925 min
Delta R.T.: -0.018 min
Response: 5604645566
Conc: 470.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

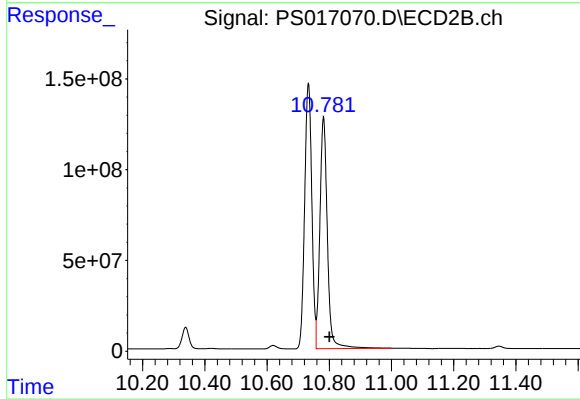


#15 Picloram

R.T.: 10.781 min
Delta R.T.: -0.019 min
Response: 2130953297
Conc: 496.76 ng/ml

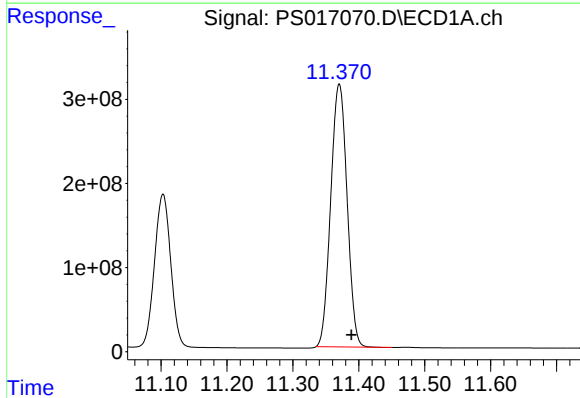

#16 DCPA

R.T.: 11.370 min
Delta R.T.: -0.018 min
Response: 5382519080
Conc: 524.22 ng/ml

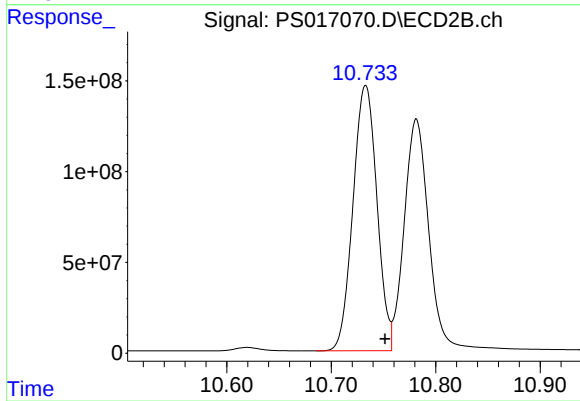

#16 DCPA

R.T.: 10.733 min
Delta R.T.: -0.019 min
Response: 2327735170
Conc: 534.03 ng/ml