

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101123\
 Data File : PS024601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 09:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 01:07:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	6.781	1021.3E6	334.3E6	496.429	483.587
Target Compounds							
1) T	Dalapon	2.515	2.572	8924760	4581735	3.612	4.094
3) T	4-Nitroph...	6.201	0.000	6731434	0	4.973	N.D. #
5) T	DICAMBA	0.000	6.983	0	1335868	N.D.	<MDL
6) T	MCP	0.000	6.983f	0	1335868	N.D.	<MDL
7) T	MCPA	0.000	7.227	0	5069046	N.D.	1.582
8) T	DICHLORPROP	0.000	7.572	0	2077647	N.D.	2.763
9) T	2,4-D	7.251	7.785f	6970331	848931	2.523	<MDL #
11) T	2,4,5-TP ...	0.000	8.622	0	584981	N.D.	<MDL
12) T	2,4,5-T	0.000	9.037f	0	4151027	N.D.	1.007
13) T	2,4-DB	0.000	9.491	0	728776	N.D.	1.430
15) T	Picloram	9.687	10.781	61656790	16818844	3.536	2.706
16) T	DCPA	0.000	10.781	0	16818844	N.D.	3.224



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101123\
Data File : PS024601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 09:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 01:07:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

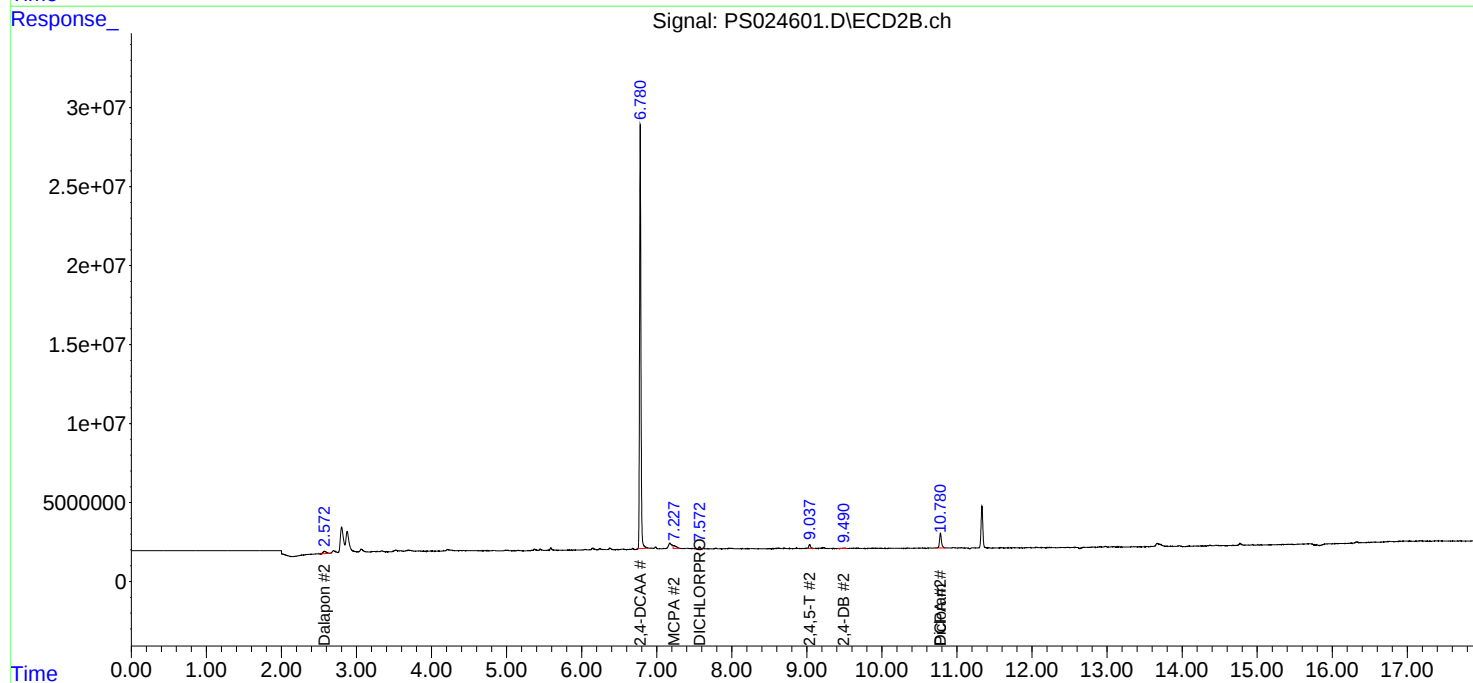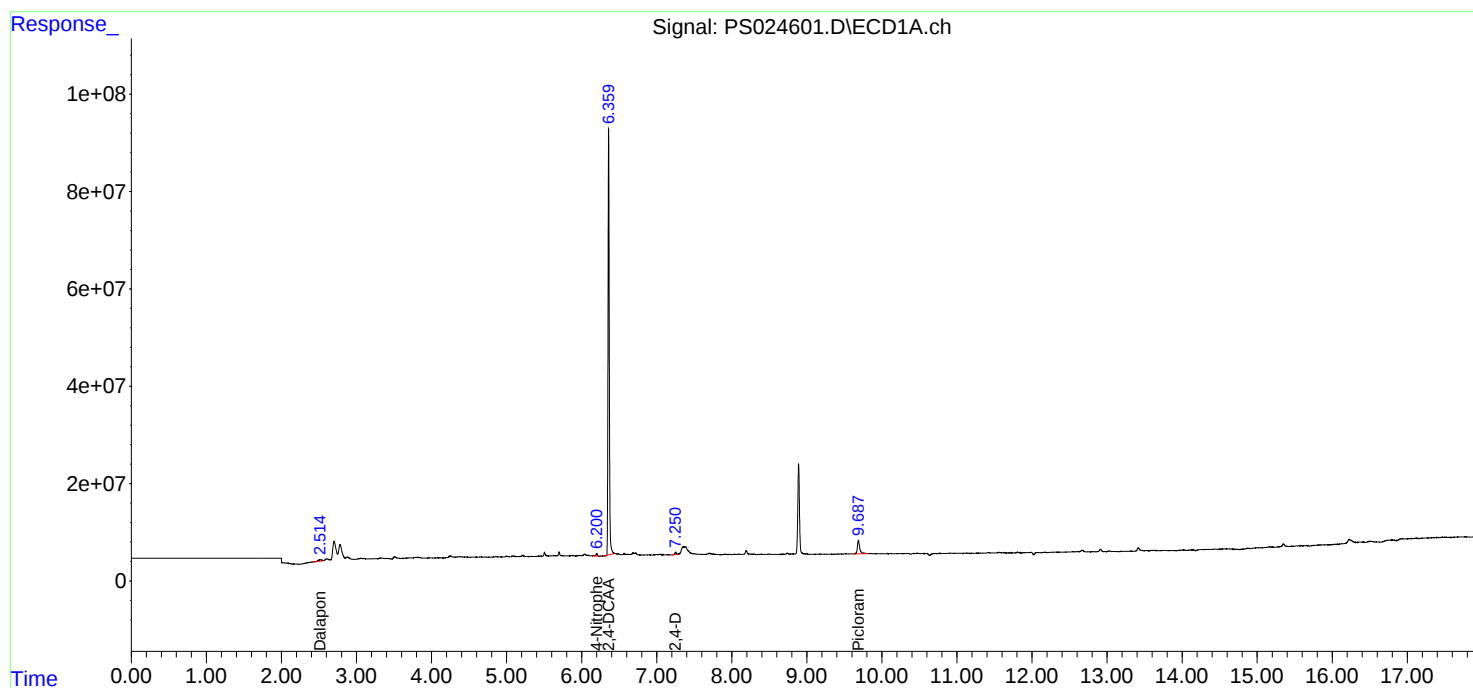


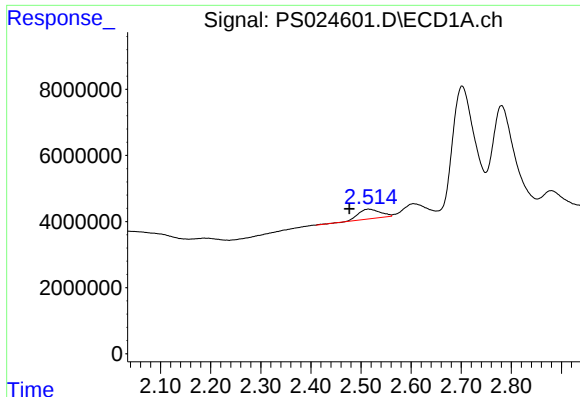

#1 Dalapon


R.T.: 2.515 min
Delta R.T.: 0.038 min
Response: 8924760
Conc: 3.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

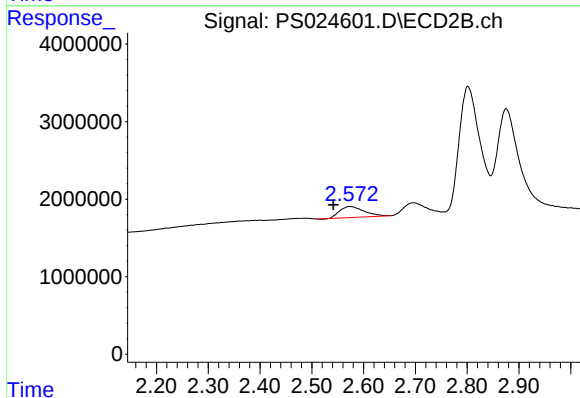


#1 Dalapon

R.T.: 2.572 min
Delta R.T.: 0.030 min
Response: 4581735
Conc: 4.09 ng/ml

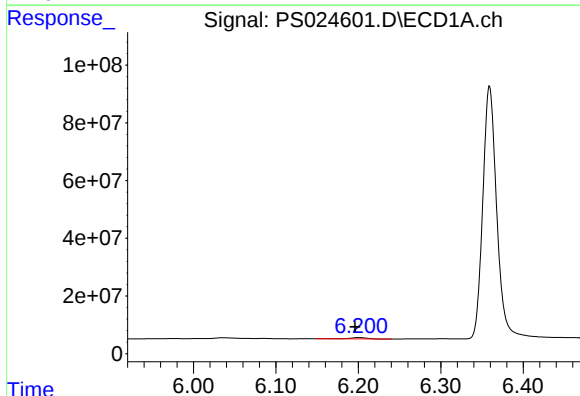


#3 4-Nitrophenol

R.T.: 6.201 min
Delta R.T.: 0.005 min
Response: 6731434
Conc: 4.97 ng/ml

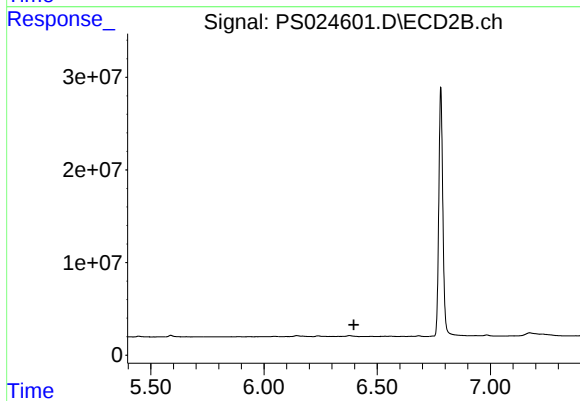

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.397 min
Response: 0
Conc: N.D.

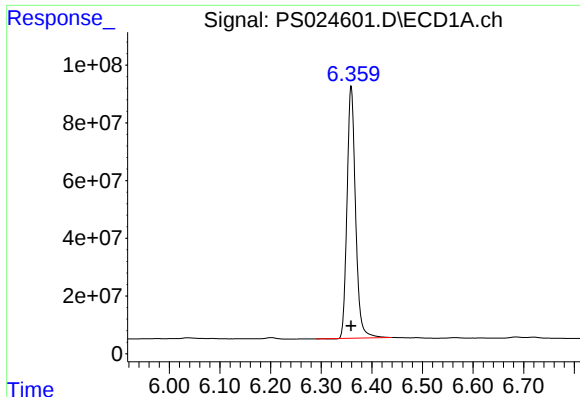

#4 2,4-DCAA


R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 1021317467
Conc: 496.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

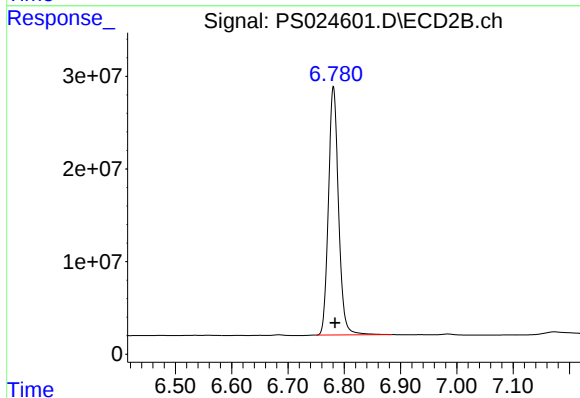


#4 2,4-DCAA

R.T.: 6.781 min
Delta R.T.: -0.003 min
Response: 334298862
Conc: 483.59 ng/ml

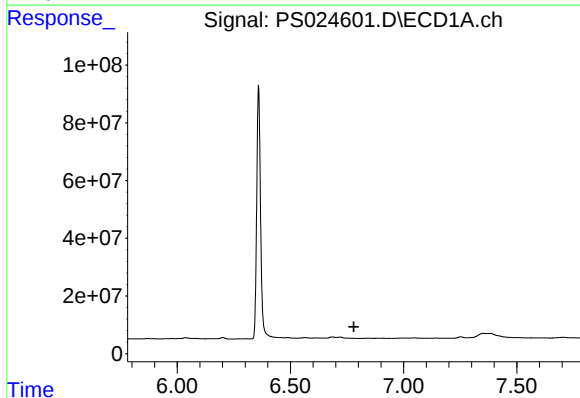


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.780 min
Response: 0
Conc: N.D.

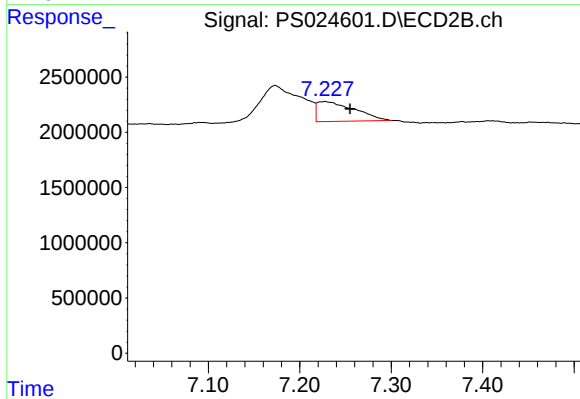

#7 MCPA


R.T.: 7.227 min
Delta R.T.: -0.028 min
Response: 5069046
Conc: 1.58 ug/ml

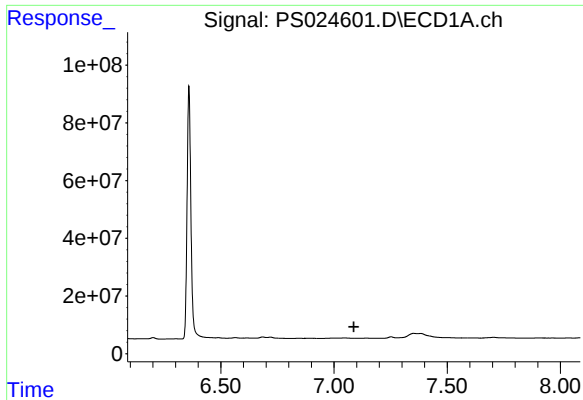

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

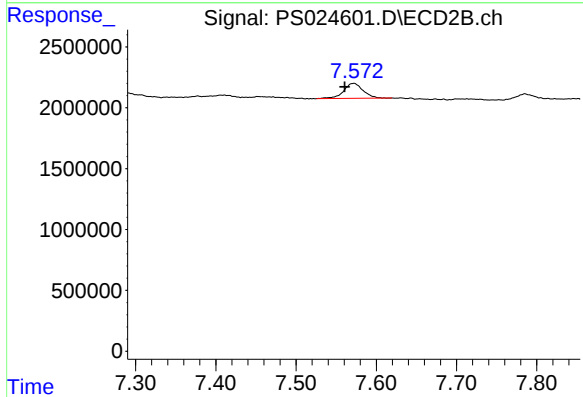


#8 DICHLORPROP

R.T.: 7.572 min
Delta R.T.: 0.011 min
Response: 2077647
Conc: 2.76 ng/ml

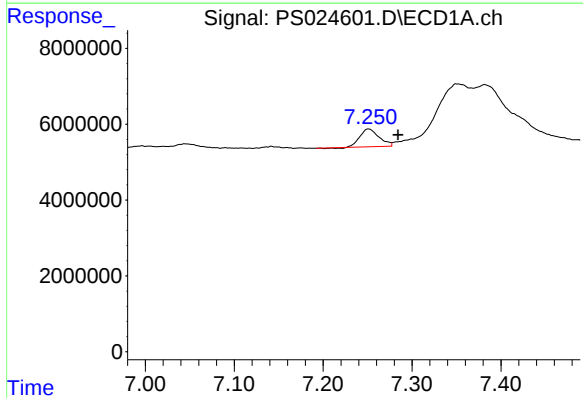


#9 2,4-D

R.T.: 7.251 min
Delta R.T.: -0.033 min
Response: 6970331
Conc: 2.52 ng/ml

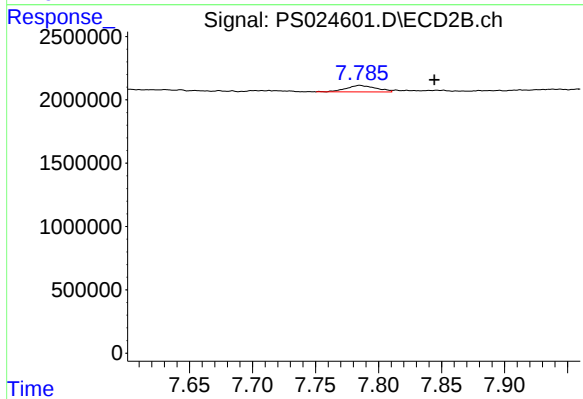

#9 2,4-D


R.T.: 7.785 min
Delta R.T.: -0.059 min
Response: 848931
Conc: N.D.

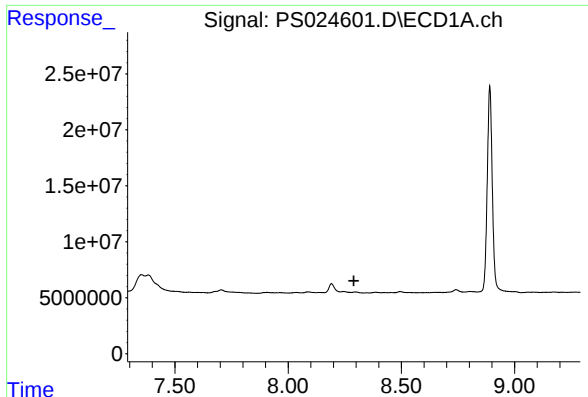

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

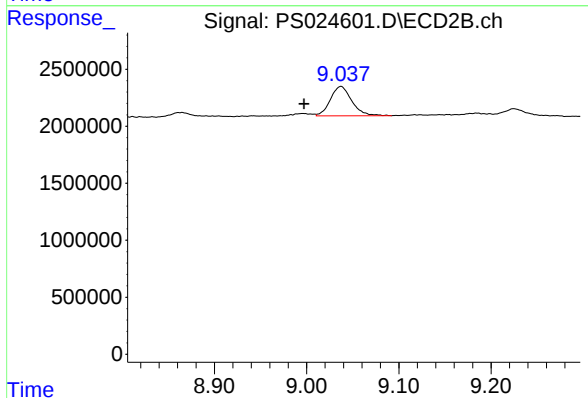


#12 2,4,5-T

R.T.: 9.037 min
Delta R.T.: 0.040 min
Response: 4151027
Conc: 1.01 ng/ml

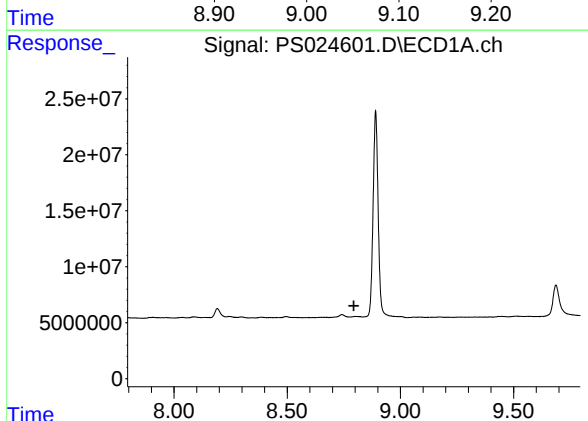


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

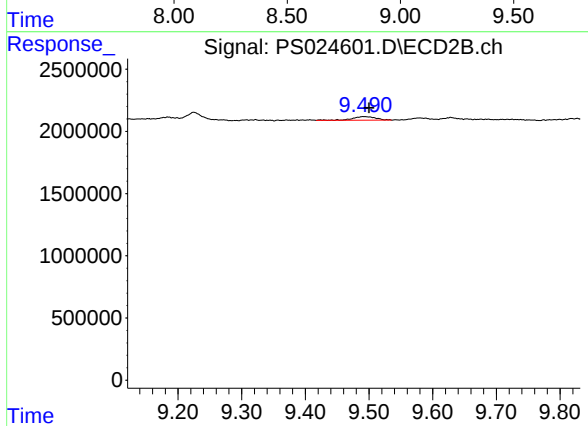

#13 2,4-DB


R.T.: 9.491 min
Delta R.T.: -0.009 min
Response: 728776
Conc: 1.43 ng/ml

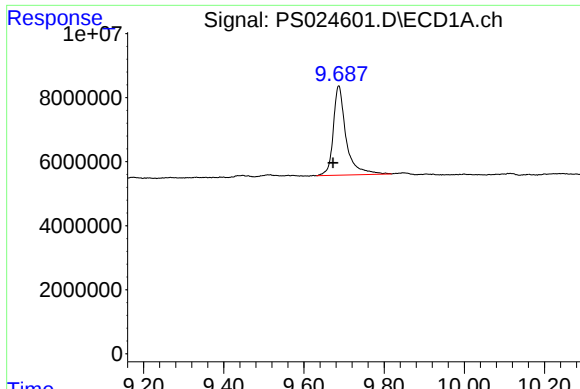

#15 Picloram


R.T.: 9.687 min
Delta R.T.: 0.014 min
Response: 61656790
Conc: 3.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

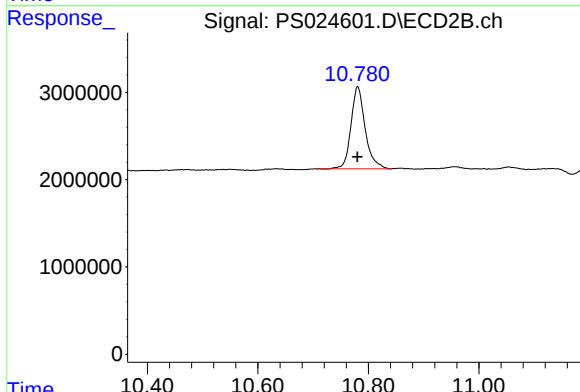


#15 Picloram

R.T.: 10.781 min
Delta R.T.: 0.000 min
Response: 16818844
Conc: 2.71 ng/ml

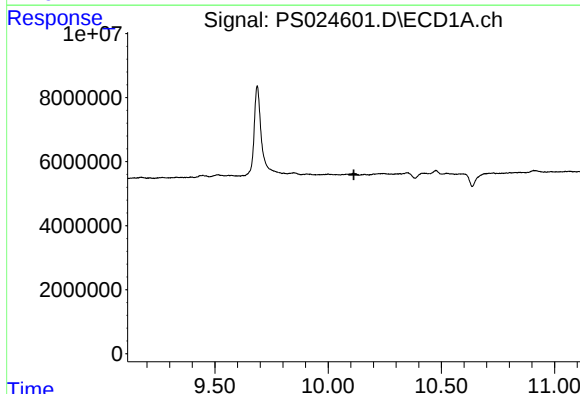

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.114 min
Response: 0
Conc: N.D.

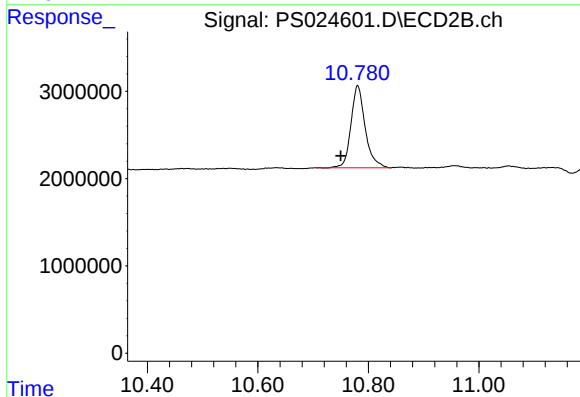

#16 DCPA

R.T.: 10.781 min
Delta R.T.: 0.031 min
Response: 16818844
Conc: 3.22 ng/ml