

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
 Data File : PS001985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2018 17:45
 Operator : EI\SJ
 Sample : PB113785BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 01:26:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.447	10.939	70202127	106.8E6	312.961	420.623 #
Target Compounds							
1) T	Dalapon	2.879	0.000	7002924	0	21.536	N.D. #
5) T	DICAMBA	0.000	11.181	0	4983865	N.D.	5.588 #
6) T	MCPD	12.134	0.000	8690078	0	13.637	N.D. #
7) T	MCPA	12.409	11.798	-3223949	19174122	N.D.	22.120
9) T	2,4-D	0.000	12.775	0	2566056	N.D.	8.248 #
12) T	2,4,5-T	0.000	14.565	0	4084426	N.D.	3.699 #
14) T	DINOSEB	0.000	15.625	0	2042626	N.D.	2.155 #
15) T	Picloram	16.989	16.877	13580852	29535933	7.800	17.367 #
16) T	DCPA	0.000	16.877	0	29535933	N.D.	16.014 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
Data File : PS001985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2018 17:45
Operator : EI\SJ
Sample : PB113785BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 01:26:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

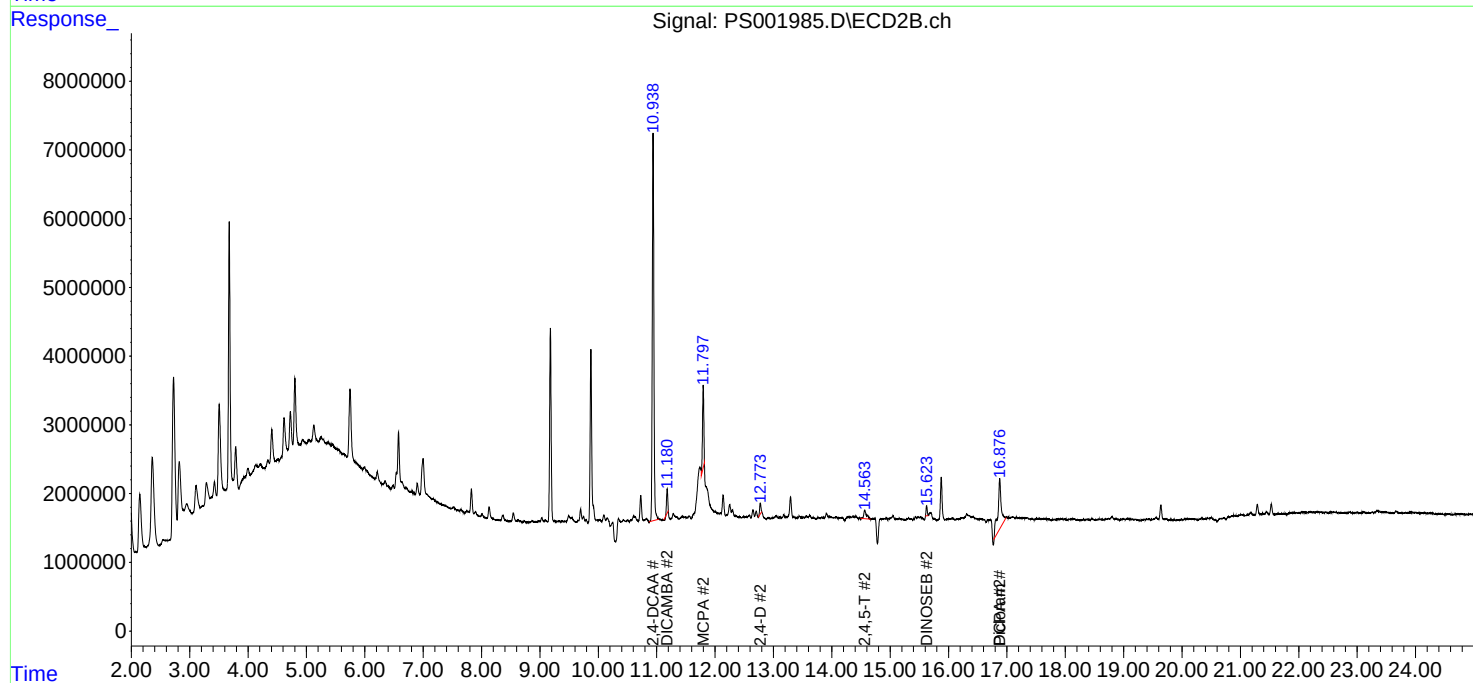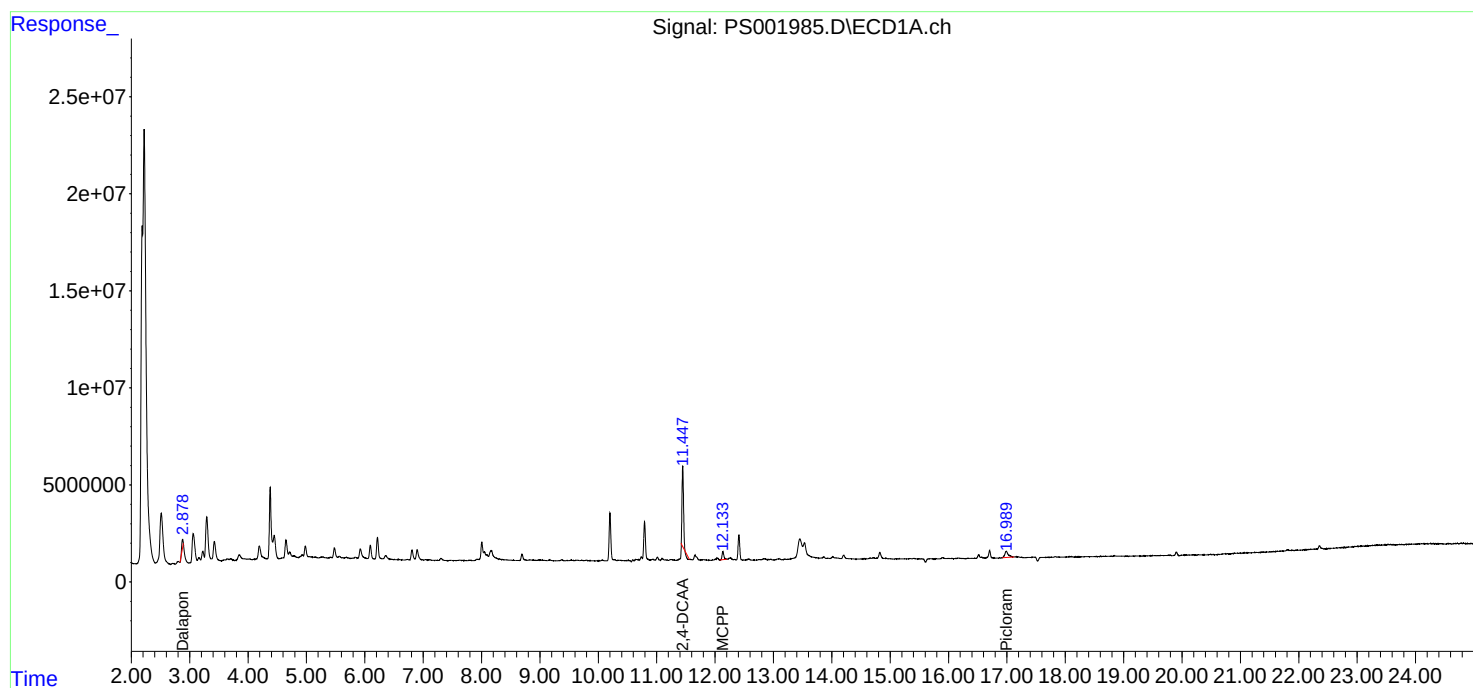


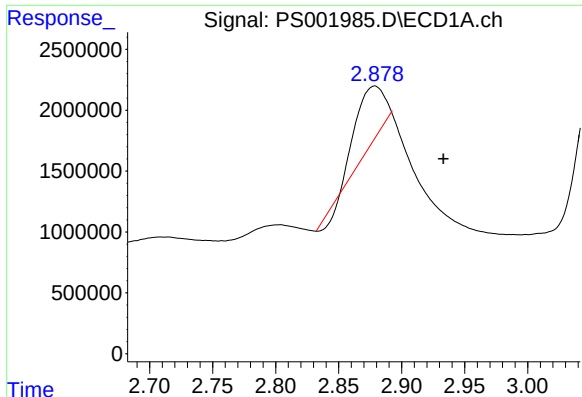

#1 Dalapon


R.T.: 2.879 min
Delta R.T.: -0.054 min
Response: 7002924
Conc: 21.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

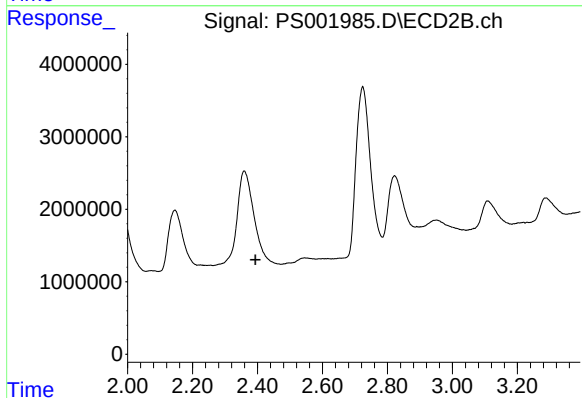


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.394 min
Response: 0
Conc: N.D.

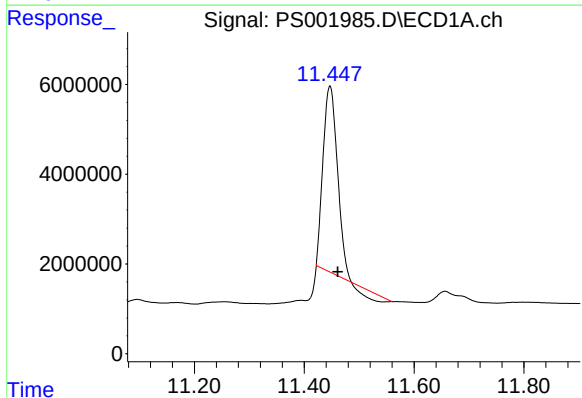


#4 2,4-DCAA

R.T.: 11.447 min
Delta R.T.: -0.015 min
Response: 70202127
Conc: 312.96 ng/ml

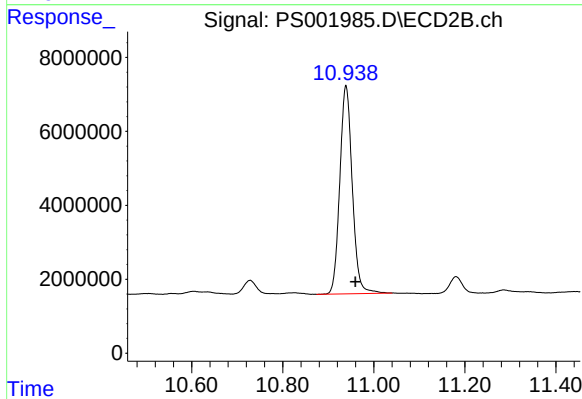

#4 2,4-DCAA


R.T.: 10.939 min
Delta R.T.: -0.021 min
Response: 106845344
Conc: 420.62 ng/ml

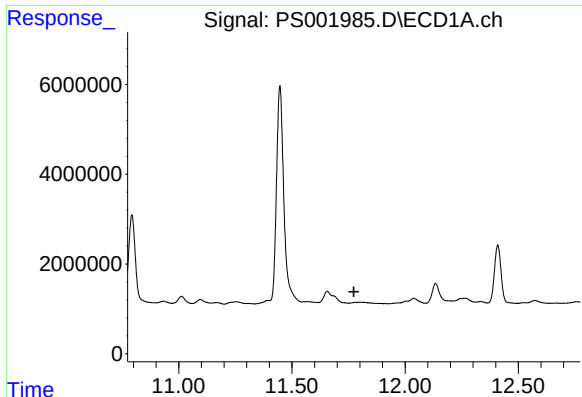

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.774 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

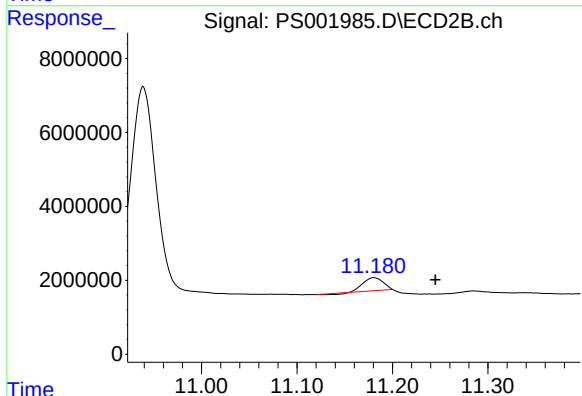


#5 DICAMBA

R.T.: 11.181 min
Delta R.T.: -0.064 min
Response: 4983865
Conc: 5.59 ng/ml

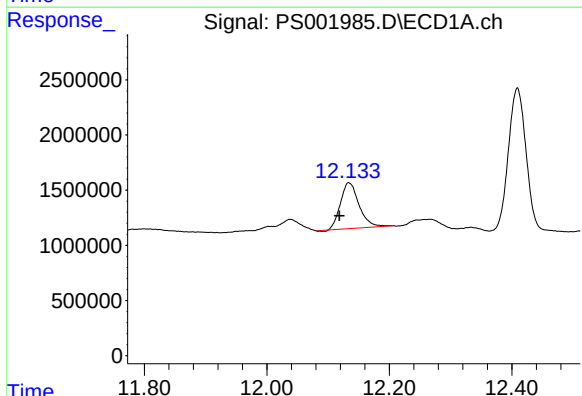


#6 MCP

R.T.: 12.134 min
Delta R.T.: 0.016 min
Response: 8690078
Conc: 13.64 ug/ml

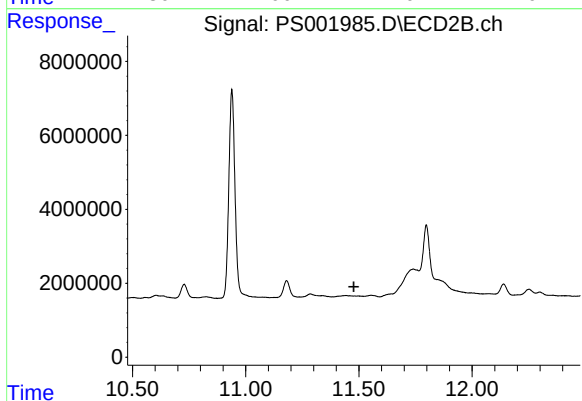

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.478 min
Response: 0
Conc: N.D.

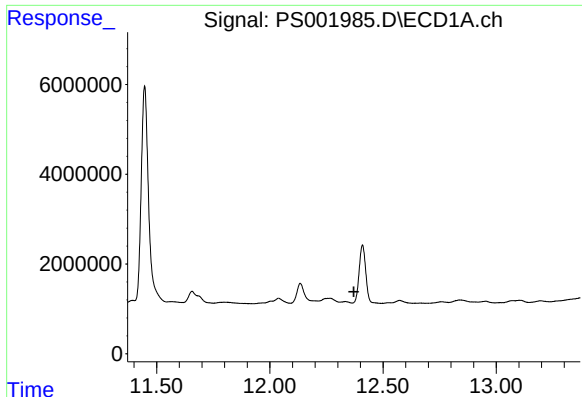

#7 MCPA


R.T.: 12.409 min
Delta R.T.: 0.038 min
Response: -3223949
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

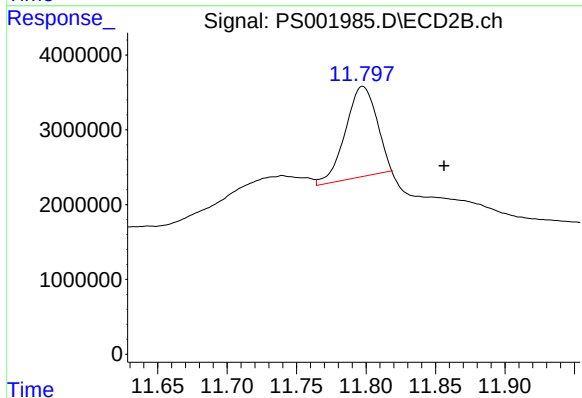


#7 MCPA

R.T.: 11.798 min
Delta R.T.: -0.058 min
Response: 19174122
Conc: 22.12 ug/ml

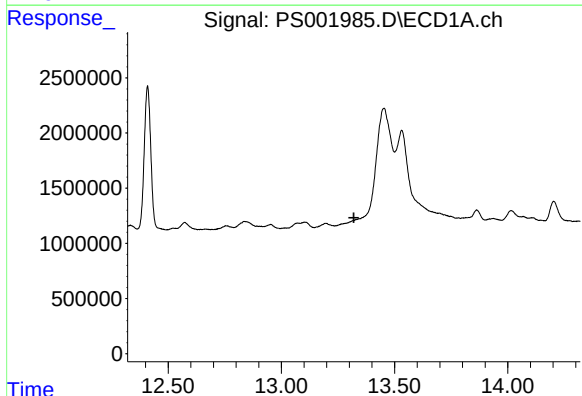


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.320 min
Response: 0
Conc: N.D.

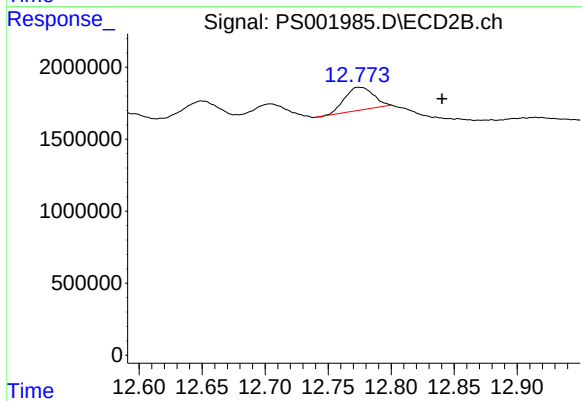

#9 2,4-D


R.T.: 12.775 min
Delta R.T.: -0.065 min
Response: 2566056
Conc: 8.25 ng/ml

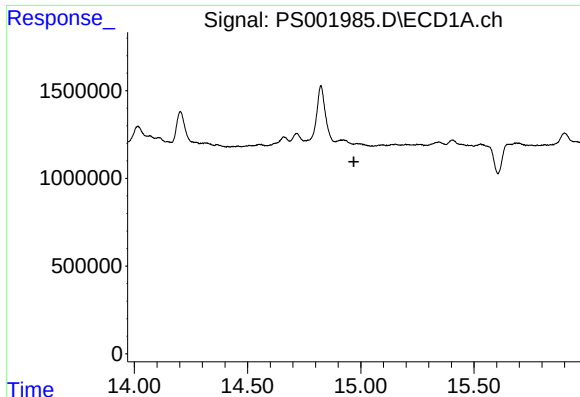

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

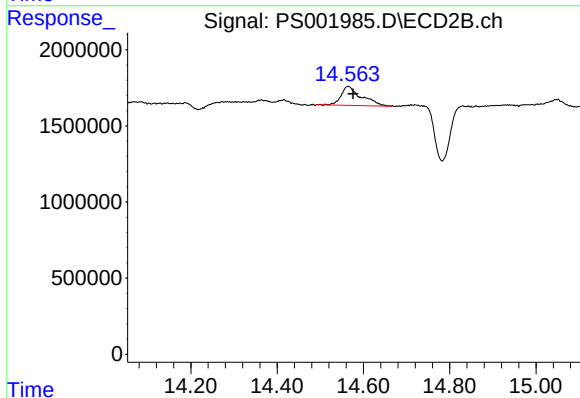


#12 2,4,5-T

R.T.: 14.565 min
Delta R.T.: -0.011 min
Response: 4084426
Conc: 3.70 ng/ml

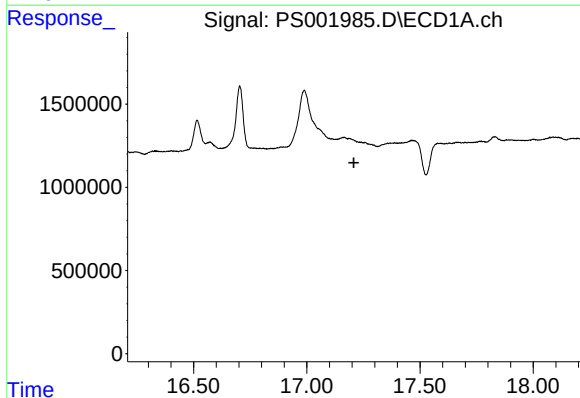


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.208 min
Response: 0
Conc: N.D.

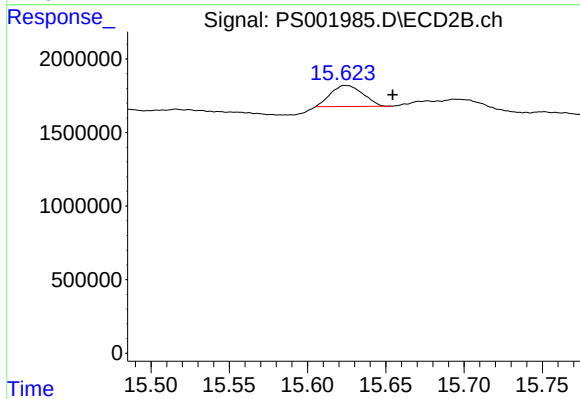

#14 DINOSEB


R.T.: 15.625 min
Delta R.T.: -0.030 min
Response: 2042626
Conc: 2.16 ng/ml

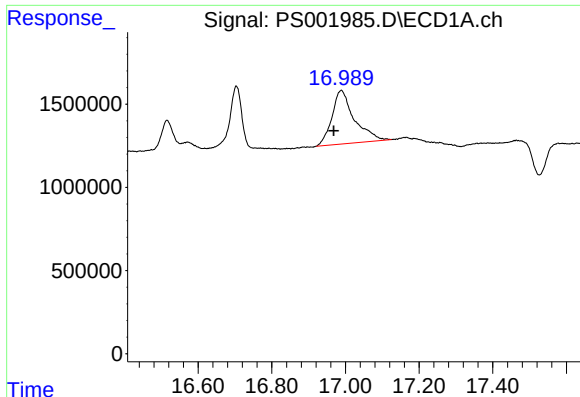

#15 Picloram


R.T.: 16.989 min
Delta R.T.: 0.020 min
Response: 13580852
Conc: 7.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

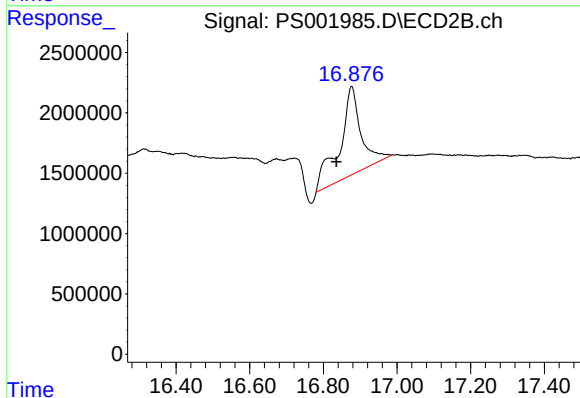


#15 Picloram

R.T.: 16.877 min
Delta R.T.: 0.042 min
Response: 29535933
Conc: 17.37 ng/ml

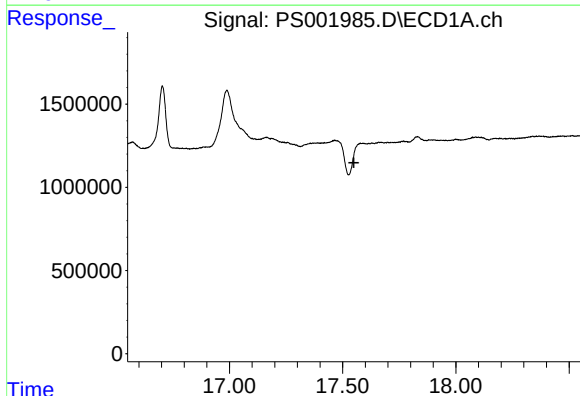

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.549 min
Response: 0
Conc: N.D.

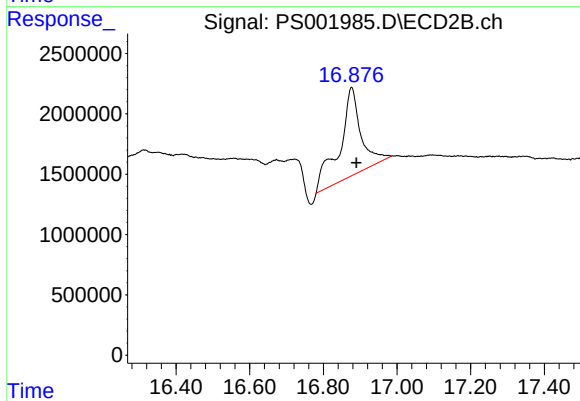

#16 DCPA

R.T.: 16.877 min
Delta R.T.: -0.013 min
Response: 29535933
Conc: 16.01 ng/ml