

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
 Data File : PS001987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2018 18:48
 Operator : EI\SJ
 Sample : J5394-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 01:27:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.504	10.998	51771737	53569389	230.799	210.889
Target Compounds							
1) T	Dalapon	2.935	2.325	3510653	30943975	10.796	104.747 #
2) T	3,5-DICHL...	0.000	9.090	0	1926944	N.D.	6.105 #
5) T	DICAMBA	11.714	11.240	-3165385	13234531	N.D.	14.839
6) T	MCP	12.187	0.000	16068751	0	25.216	N.D. #
8) T	DICHLORPROP	0.000	12.307	0	6314082	N.D.	27.184 #
9) T	2,4-D	0.000	12.846	0	2215083	N.D.	7.120 #
10) T	Pentachlo...	0.000	13.432	0	3458273	N.D.	1.009 #
11) T	2,4,5-TP ...	0.000	13.966	0	2735477	N.D.	1.995 #
13) T	2,4-DB	0.000	15.260	0	1496612	N.D.	9.042 #
14) T	DINOSEB	0.000	15.684	0	2365817	N.D.	2.496 #
15) T	Picloram	0.000	16.876	0	1347415	N.D.	0.792 #
16) T	DCPA	0.000	16.876	0	1347415	N.D.	0.731 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
Data File : PS001987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2018 18:48
Operator : EI\SJ
Sample : J5394-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 01:27:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

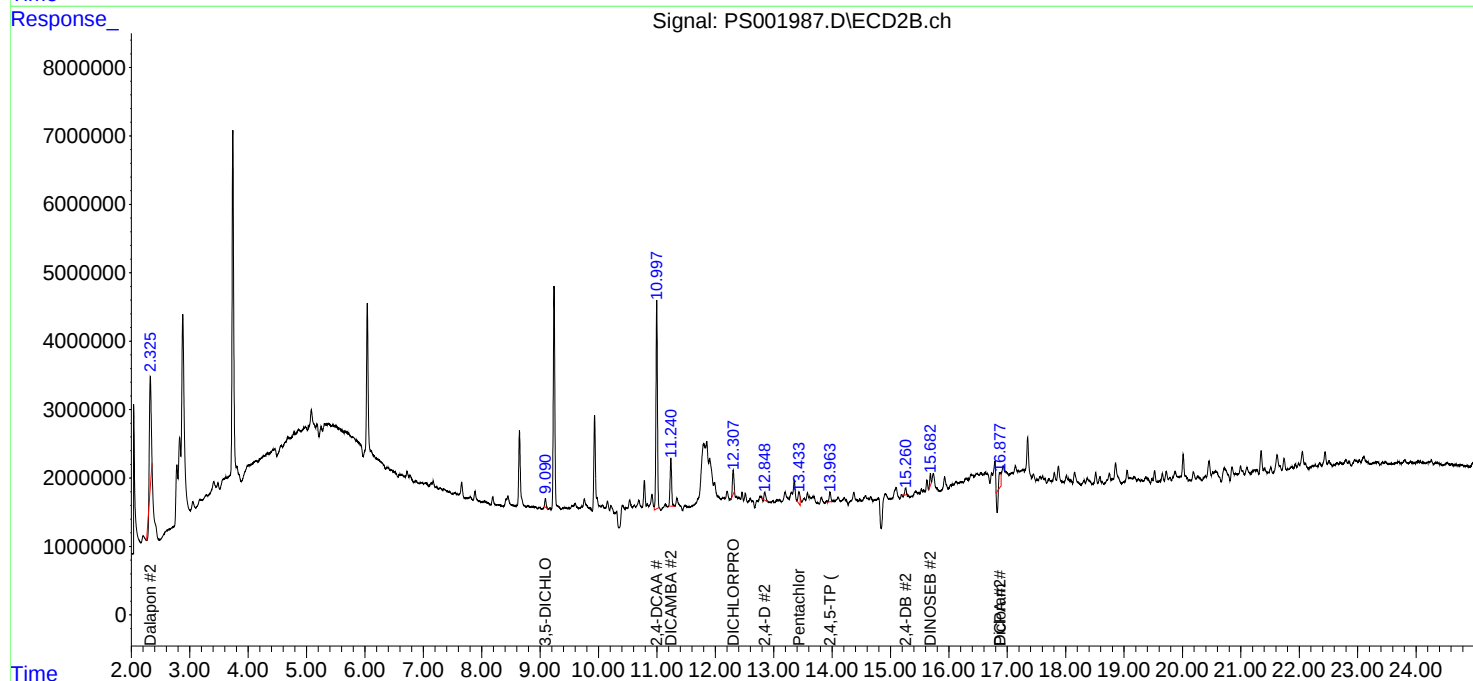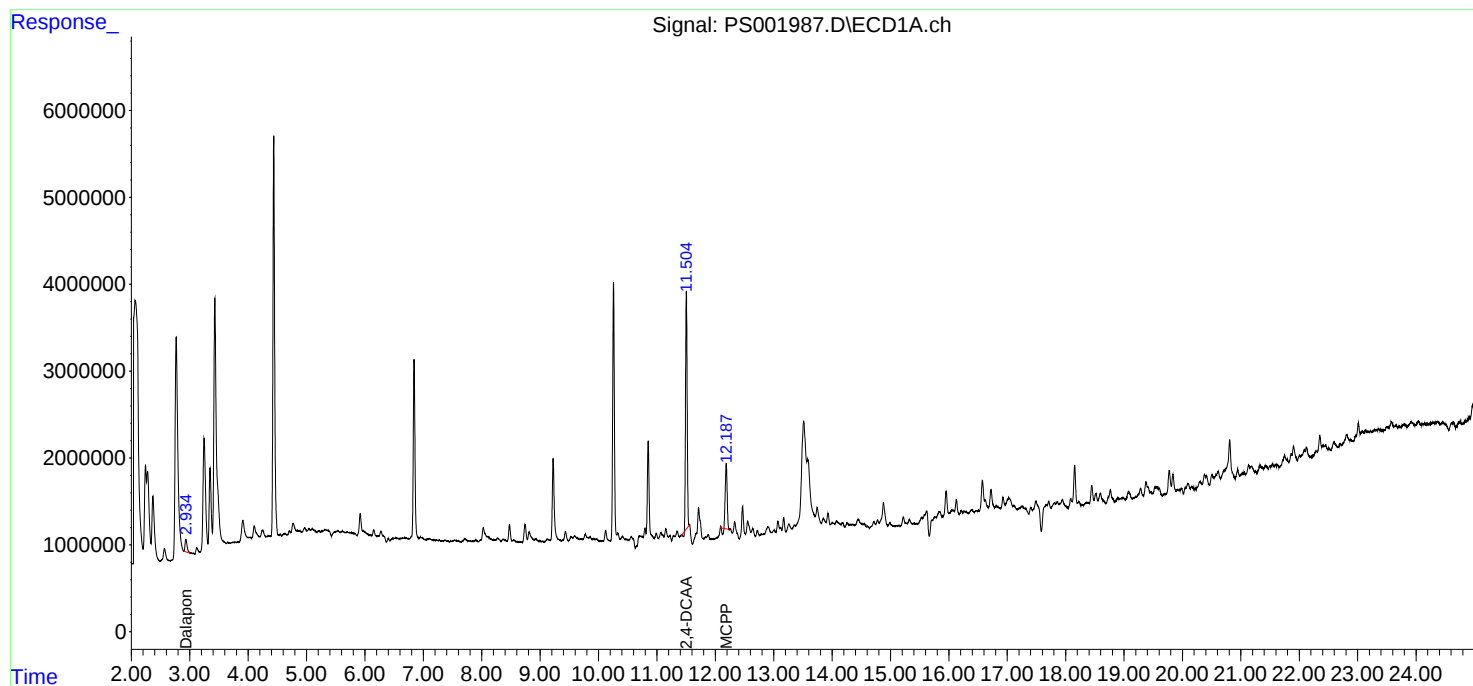


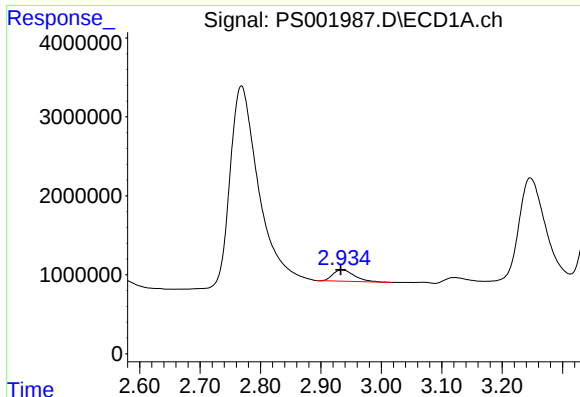

#1 Dalapon


R.T.: 2.935 min
Delta R.T.: 0.002 min
Response: 3510653
Conc: 10.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

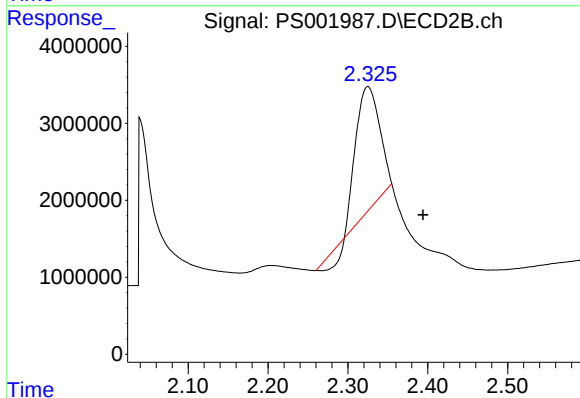


#1 Dalapon

R.T.: 2.325 min
Delta R.T.: -0.069 min
Response: 30943975
Conc: 104.75 ng/ml

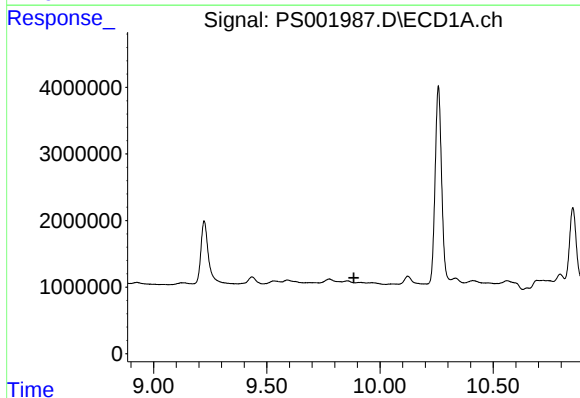


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.884 min
Response: 0
Conc: N.D.

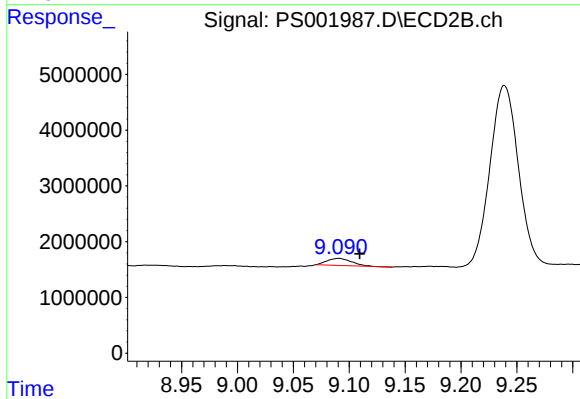

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.090 min
Delta R.T.: -0.019 min
Response: 1926944
Conc: 6.11 ng/ml

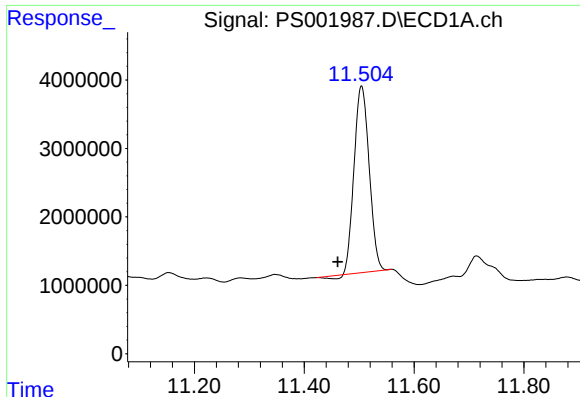

#4 2,4-DCAA


R.T.: 11.504 min
Delta R.T.: 0.043 min
Response: 51771737
Conc: 230.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

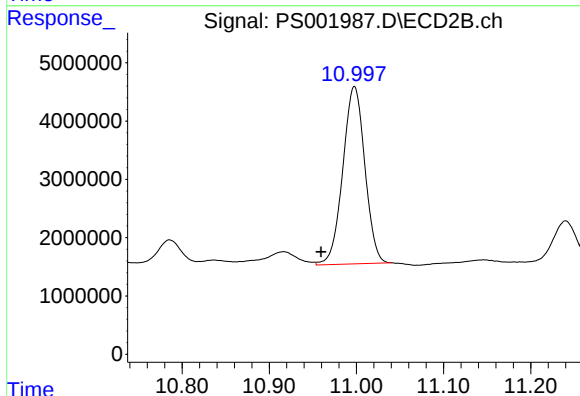


#4 2,4-DCAA

R.T.: 10.998 min
Delta R.T.: 0.038 min
Response: 53569389
Conc: 210.89 ng/ml

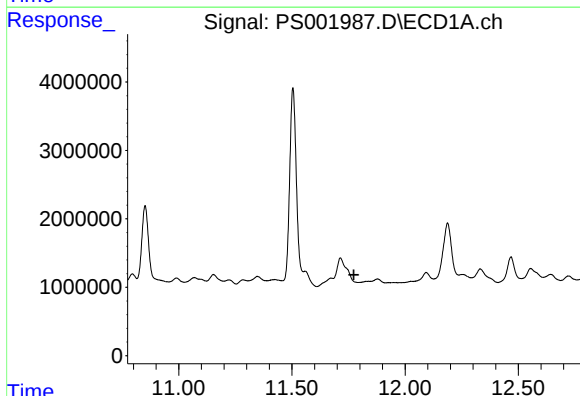


#5 DICAMBA

R.T.: 11.714 min
Delta R.T.: -0.060 min
Response: -3165385
Conc: N.D.

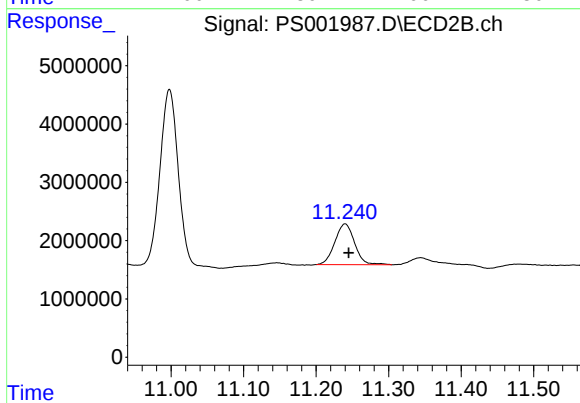

#5 DICAMBA


R.T.: 11.240 min
Delta R.T.: -0.005 min
Response: 13234531
Conc: 14.84 ng/ml

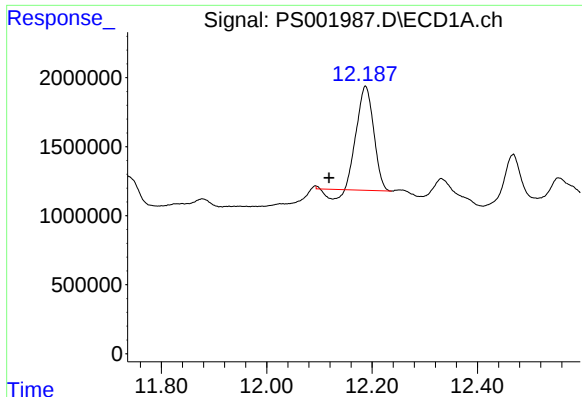

#6 MCP


R.T.: 12.187 min
Delta R.T.: 0.069 min
Response: 16068751
Conc: 25.22 ug/ml

Instrument :
ECD_S
ClientSampleId :

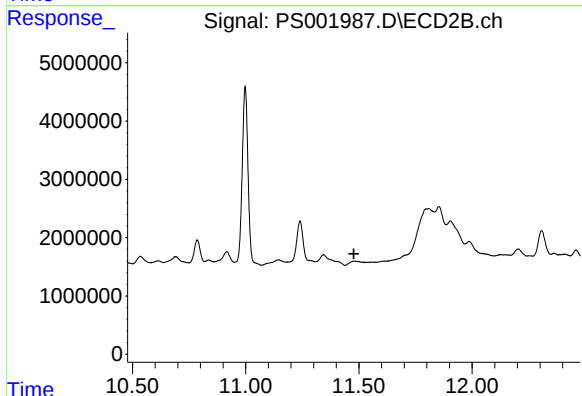


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

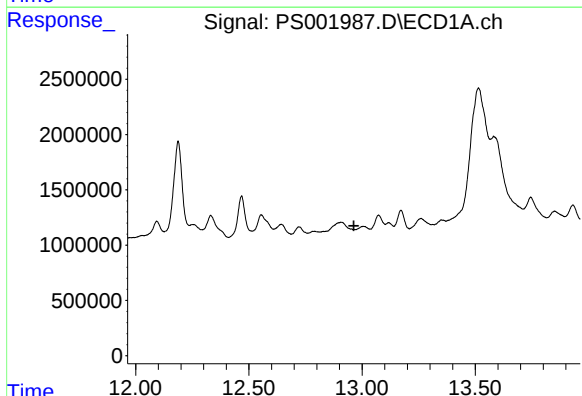


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.964 min
Response: 0
Conc: N.D.

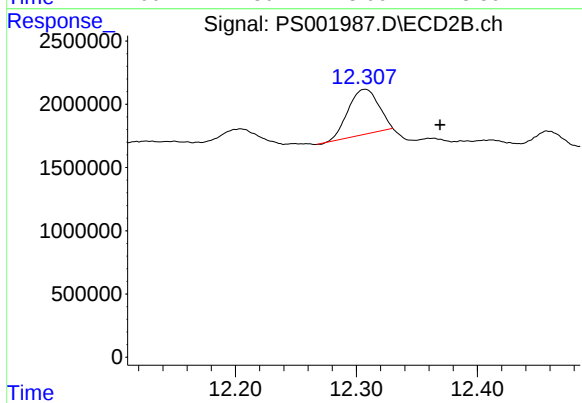

#8 DICHLORPROP


R.T.: 12.307 min
Delta R.T.: -0.062 min
Response: 6314082
Conc: 27.18 ng/ml

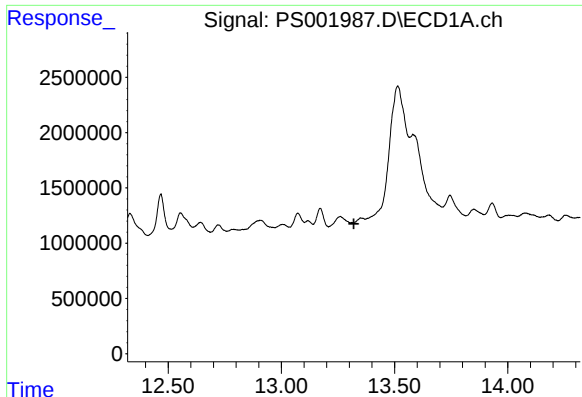

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

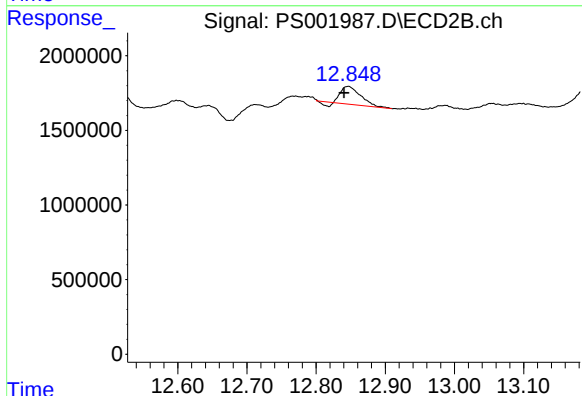


#9 2,4-D

R.T.: 12.846 min
Delta R.T.: 0.006 min
Response: 2215083
Conc: 7.12 ng/ml

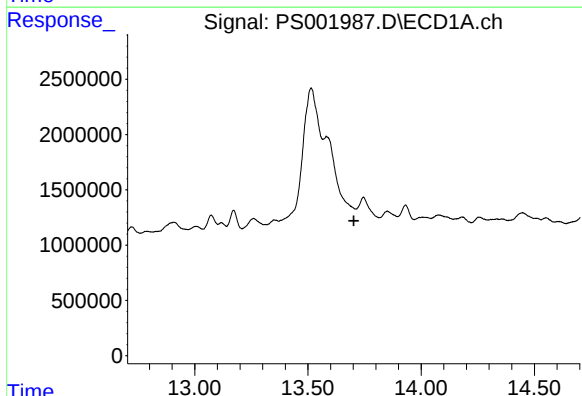


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.703 min
Response: 0
Conc: N.D.

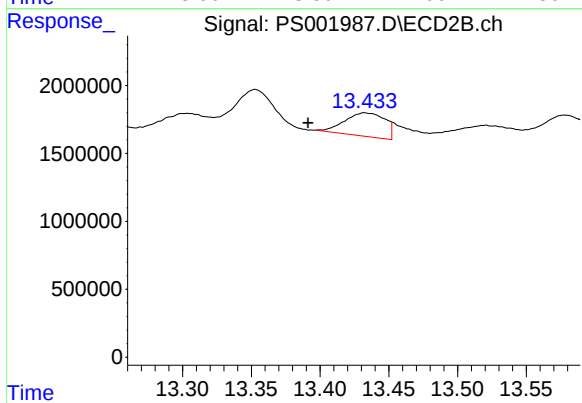

#10 Pentachlorophenol


R.T.: 13.432 min
Delta R.T.: 0.041 min
Response: 3458273
Conc: 1.01 ng/ml

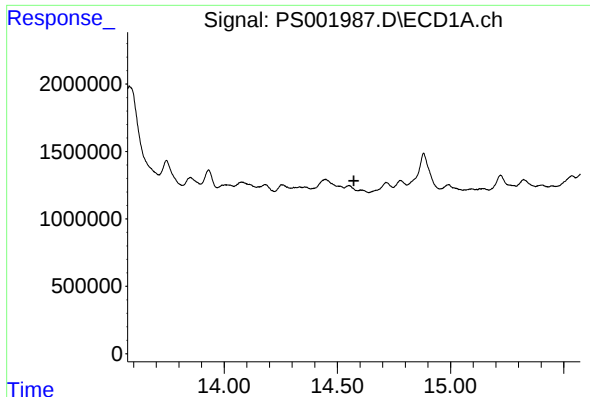

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

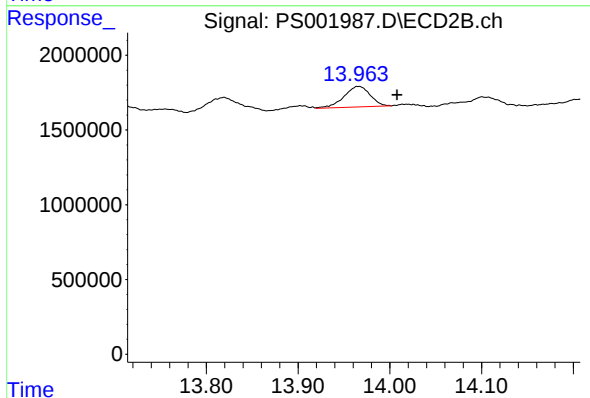


#11 2,4,5-TP (SILVEX)

R.T.: 13.966 min
Delta R.T.: -0.042 min
Response: 2735477
Conc: 2.00 ng/ml

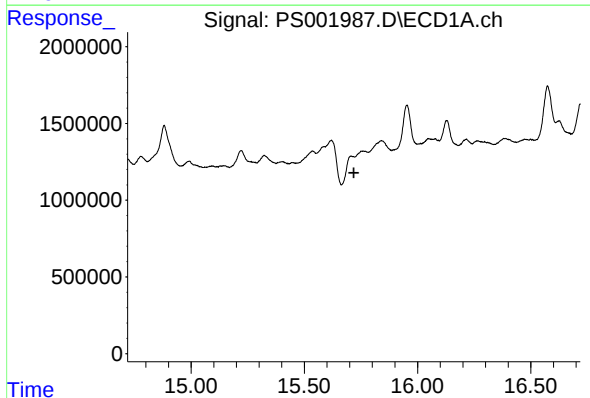


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.718 min
Response: 0
Conc: N.D.

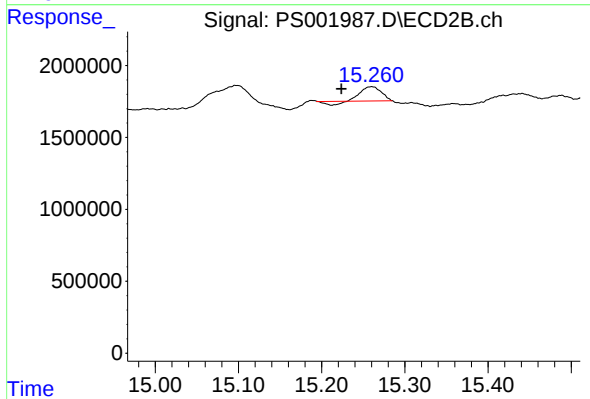

#13 2,4-DB


R.T.: 15.260 min
Delta R.T.: 0.036 min
Response: 1496612
Conc: 9.04 ng/ml

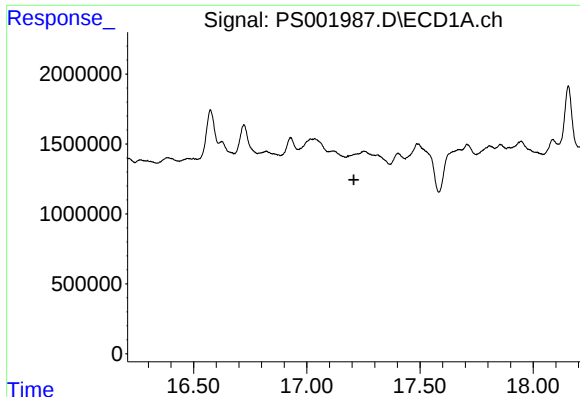

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.208 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

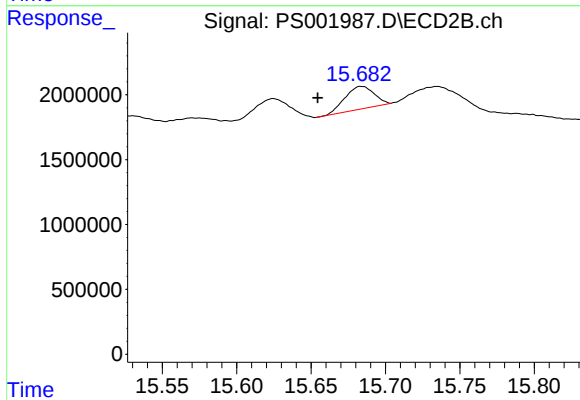


#14 DINOSEB

R.T.: 15.684 min
Delta R.T.: 0.029 min
Response: 2365817
Conc: 2.50 ng/ml

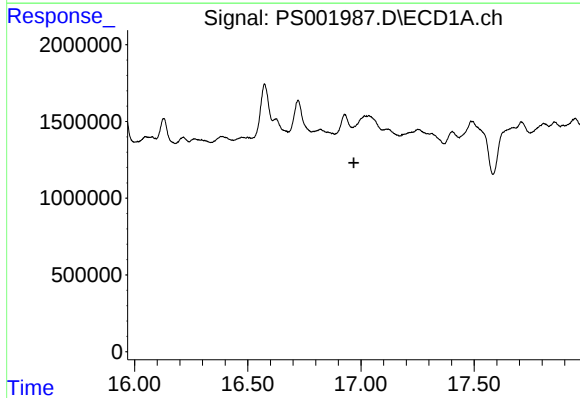


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.969 min
Response: 0
Conc: N.D.

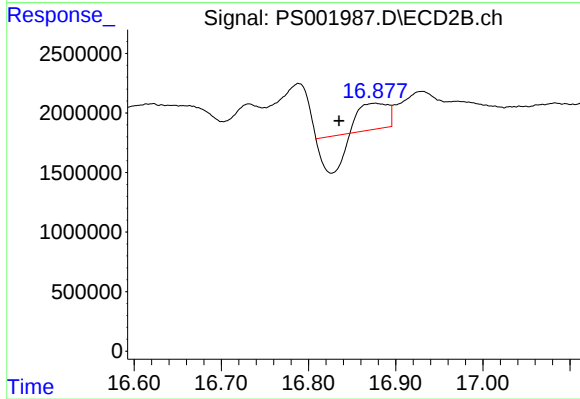

#15 Picloram


R.T.: 16.876 min
Delta R.T.: 0.041 min
Response: 1347415
Conc: 0.79 ng/ml

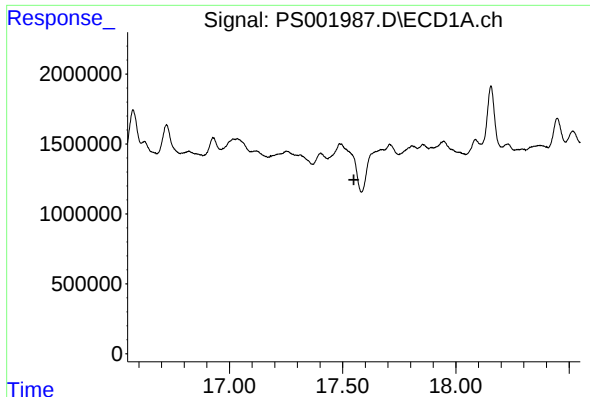

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

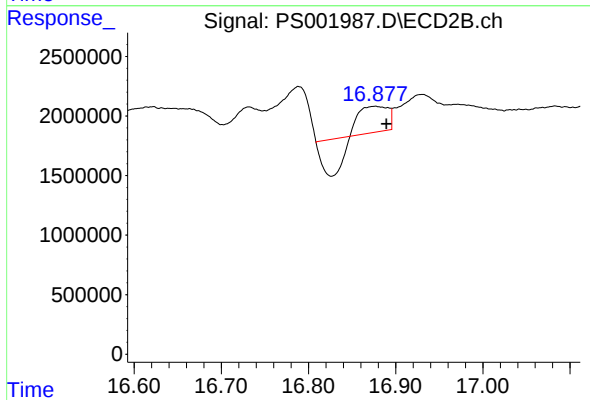

#16 DCPA

R.T.: 16.876 min
Delta R.T.: -0.013 min
Response: 1347415
Conc: 0.73 ng/ml