

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
 Data File : PS001988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2018 19:19
 Operator : EI\SJ
 Sample : J5394-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 01:27:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.450	10.944	56468752	63863737	251.738	251.416
Target Compounds							
1) T	Dalapon	2.881	0.000	772809	0	2.377	N.D. #
3) T	4-Nitroph...	11.099	0.000	2063734	0	14.662	N.D. #
5) T	DICAMBA	0.000	11.291	0	244758	N.D.	0.274 #
6) T	MCP	12.125	11.427	21919117	-148824	34.397	N.D. #
7) T	MCPA	12.414	11.803	-3674708	4190074	N.D.	4.834
9) T	2,4-D	0.000	12.791	0	1015226	N.D.	3.263 #
10) T	Pentachlo...	13.692	13.378	4487394	3331273	1.460	0.972 #
14) T	DINOSEB	17.166	15.631	3353419	4661446	4.023	4.918
15) T	Picloram	0.000	16.826	0	8952456	N.D.	5.264 #
16) T	DCPA	0.000	16.878	0	9047405	N.D.	4.905 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
Data File : PS001988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2018 19:19
Operator : EI\SJ
Sample : J5394-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 01:27:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

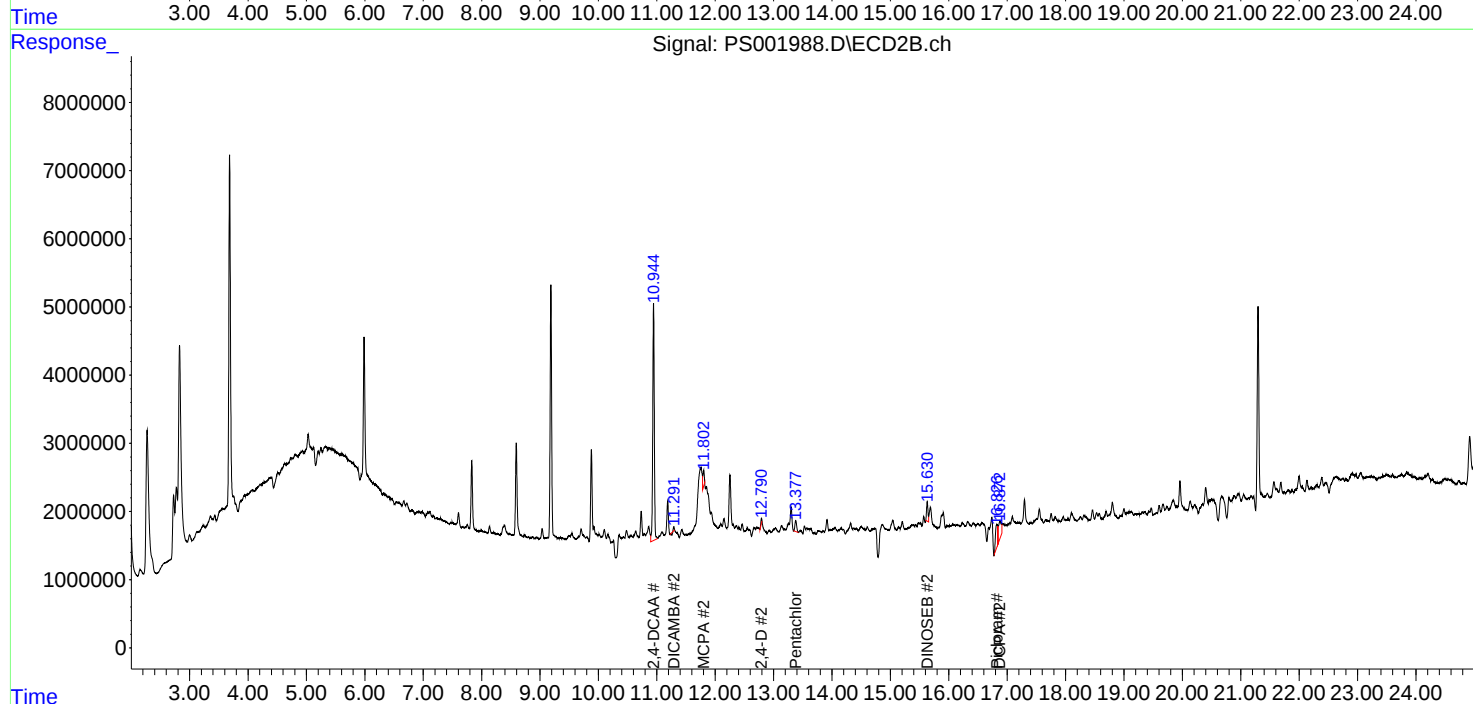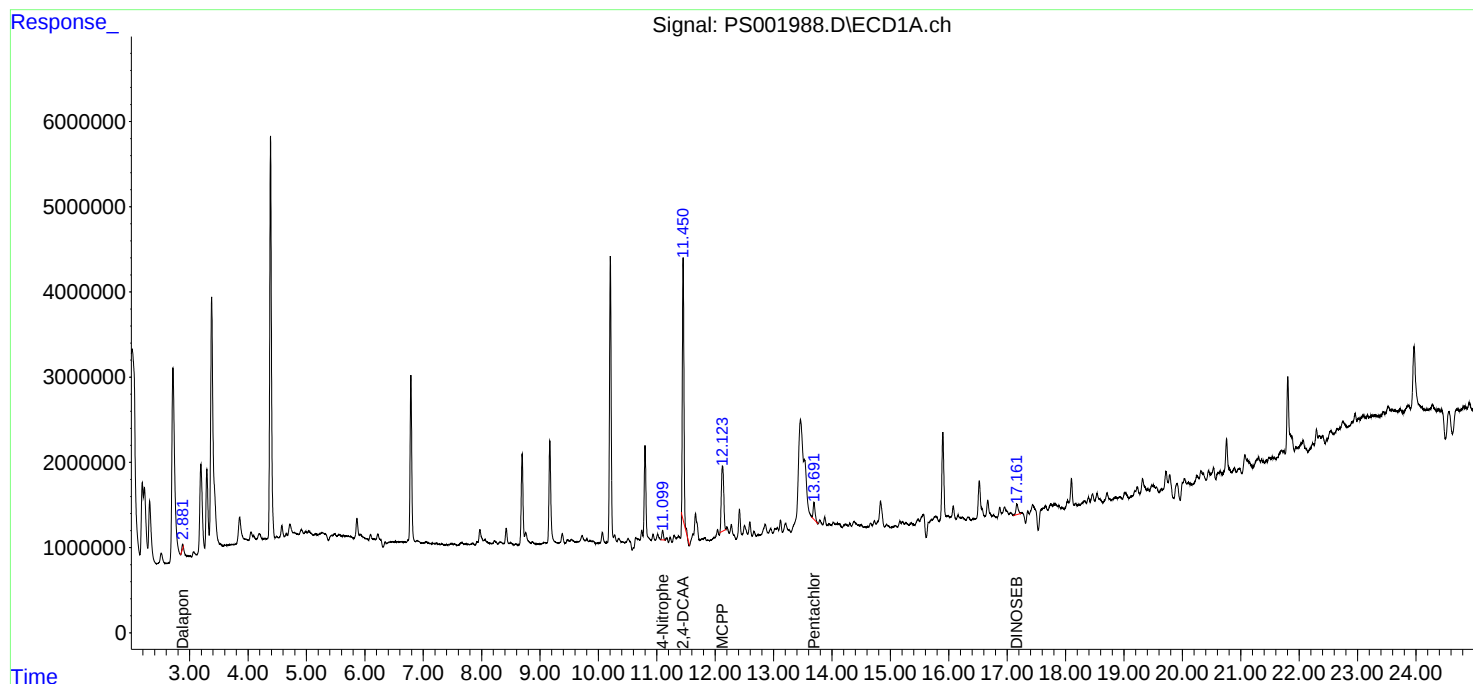


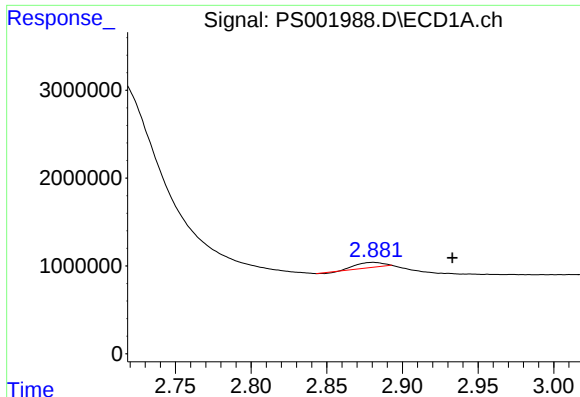

#1 Dalapon


R.T.: 2.881 min
Delta R.T.: -0.052 min
Response: 772809
Conc: 2.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

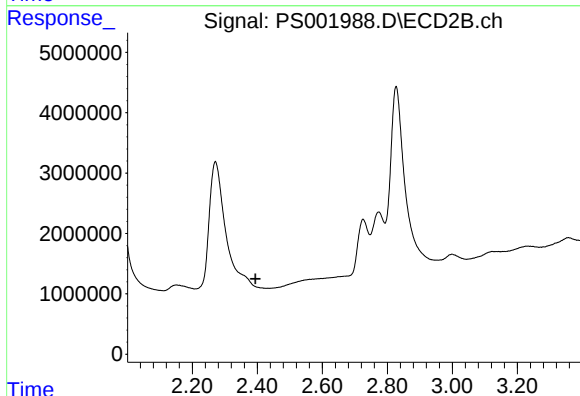


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.394 min
Response: 0
Conc: N.D.

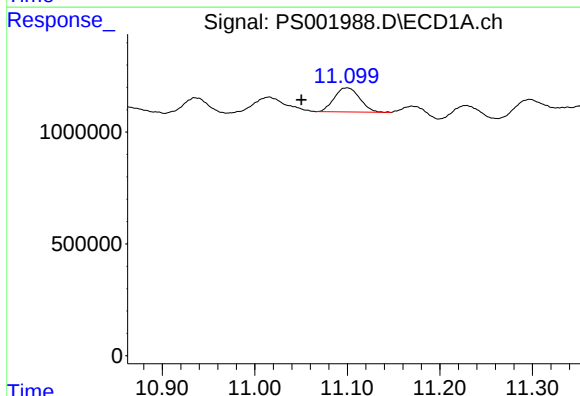


#3 4-Nitrophenol

R.T.: 11.099 min
Delta R.T.: 0.049 min
Response: 2063734
Conc: 14.66 ng/ml

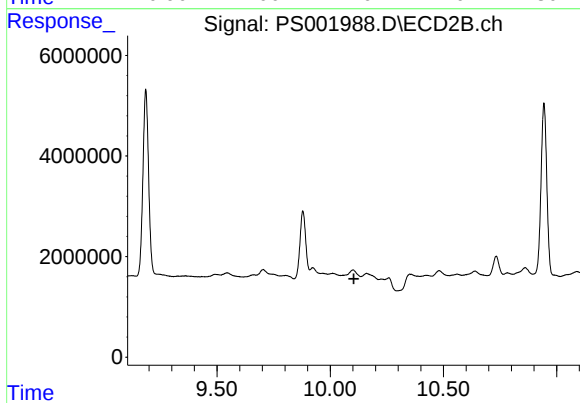

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 10.105 min
Response: 0
Conc: N.D.

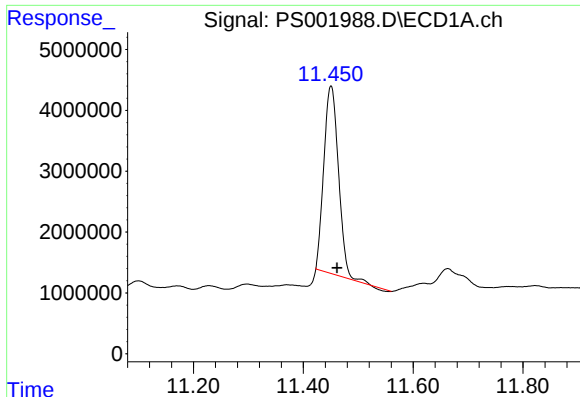

#4 2,4-DCAA


R.T.: 11.450 min
Delta R.T.: -0.011 min
Response: 56468752
Conc: 251.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

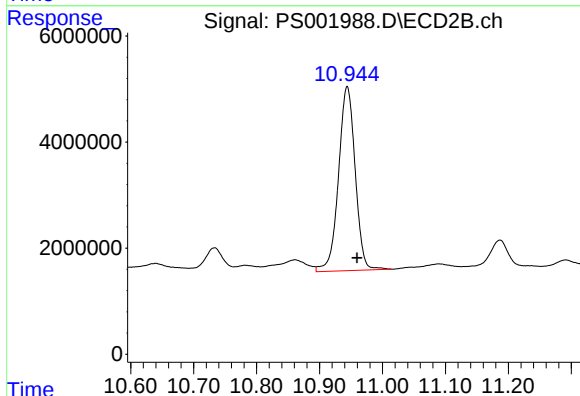


#4 2,4-DCAA

R.T.: 10.944 min
Delta R.T.: -0.016 min
Response: 63863737
Conc: 251.42 ng/ml

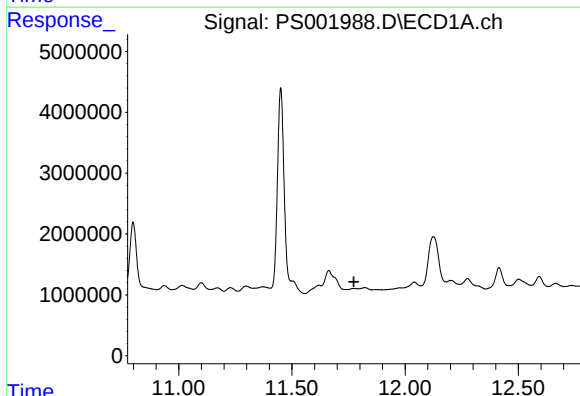


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.774 min
Response: 0
Conc: N.D.

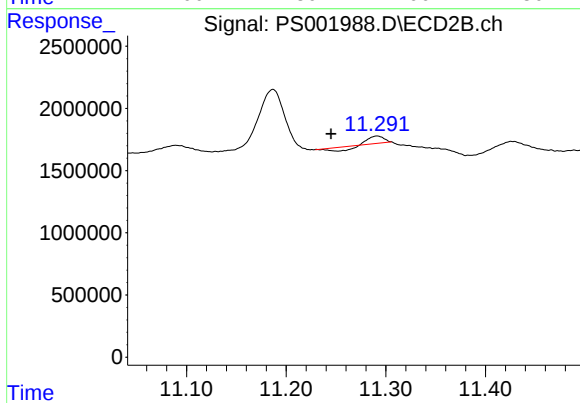

#5 DICAMBA


R.T.: 11.291 min
Delta R.T.: 0.046 min
Response: 244758
Conc: 0.27 ng/ml

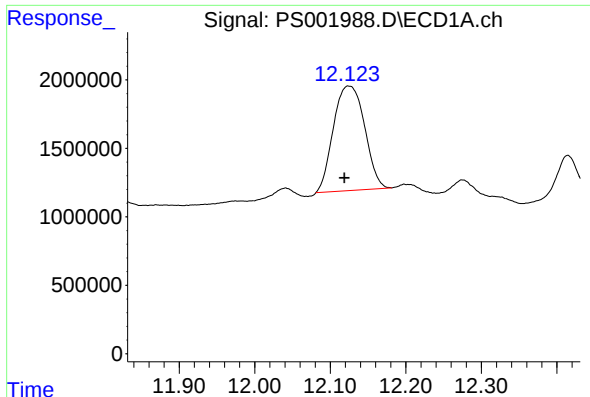

#6 MCPP


R.T.: 12.125 min
Delta R.T.: 0.006 min
Response: 21919117
Conc: 34.40 ug/ml

Instrument :
ECD_S
ClientSampleId :

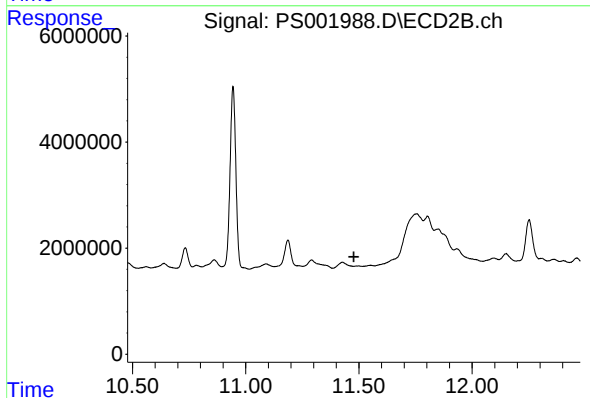


#6 MCPP

R.T.: 11.427 min
Delta R.T.: -0.051 min
Response: -148824
Conc: N.D.

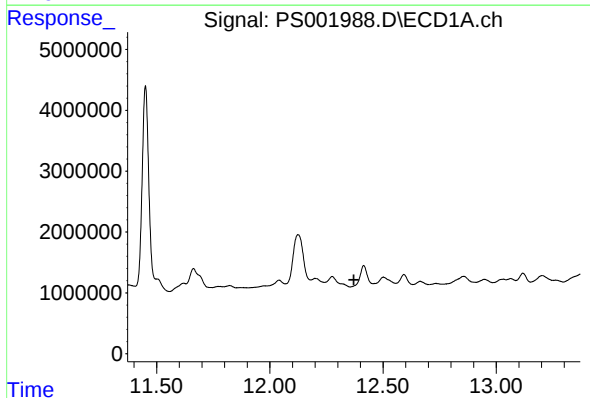


#7 MCPA

R.T.: 12.414 min
Delta R.T.: 0.043 min
Response: -3674708
Conc: N.D.

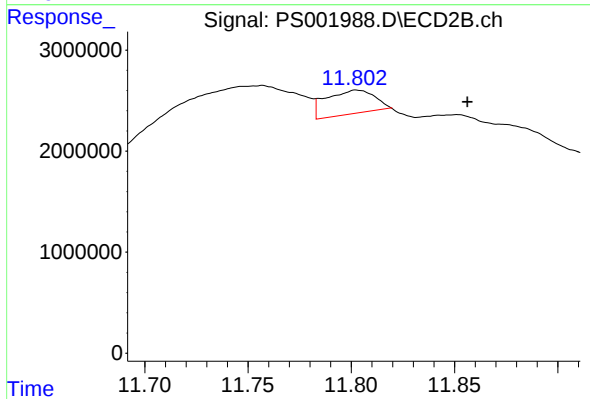

#7 MCPA


R.T.: 11.803 min
Delta R.T.: -0.053 min
Response: 4190074
Conc: 4.83 ug/ml

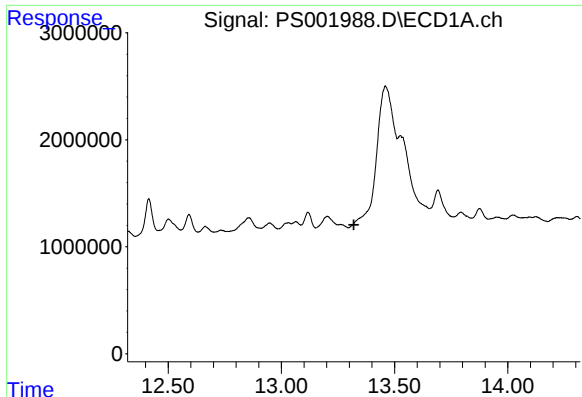

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

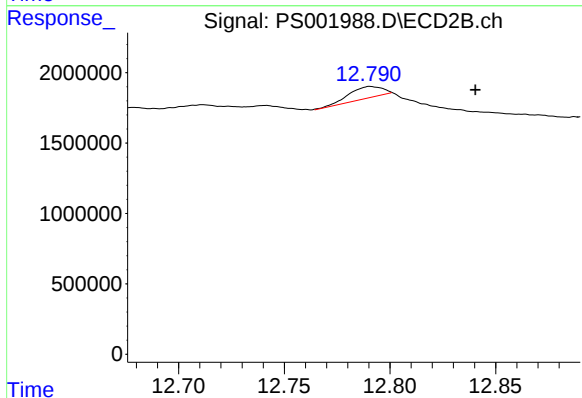


#9 2,4-D

R.T.: 12.791 min
Delta R.T.: -0.049 min
Response: 1015226
Conc: 3.26 ng/ml

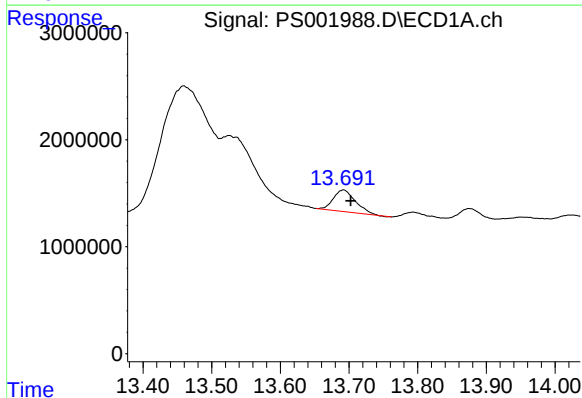


#10 Pentachlorophenol

R.T.: 13.692 min
Delta R.T.: -0.011 min
Response: 4487394
Conc: 1.46 ng/ml

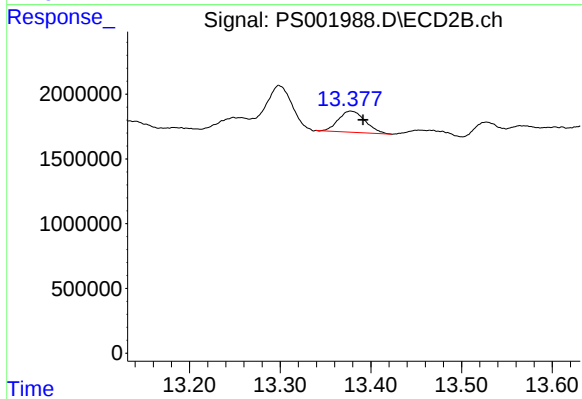

#10 Pentachlorophenol


R.T.: 13.378 min
Delta R.T.: -0.013 min
Response: 3331273
Conc: 0.97 ng/ml

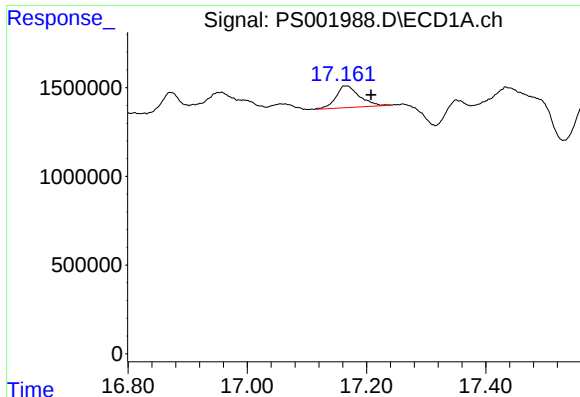

#14 DINOSEB


R.T.: 17.166 min
Delta R.T.: -0.042 min
Response: 3353419
Conc: 4.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

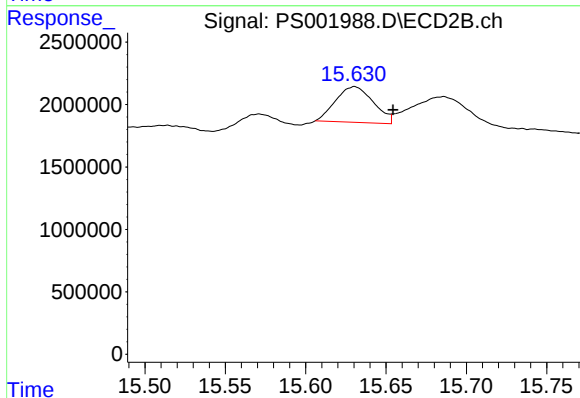


#14 DINOSEB

R.T.: 15.631 min
Delta R.T.: -0.024 min
Response: 4661446
Conc: 4.92 ng/ml

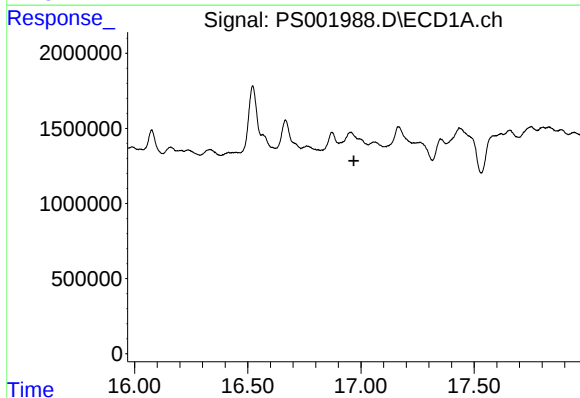


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.969 min
Response: 0
Conc: N.D.

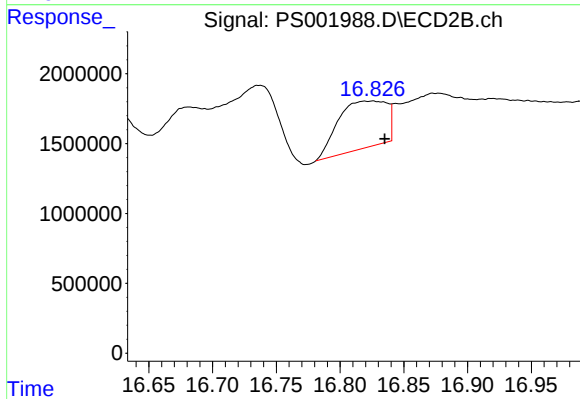

#15 Picloram


R.T.: 16.826 min
Delta R.T.: -0.009 min
Response: 8952456
Conc: 5.26 ng/ml

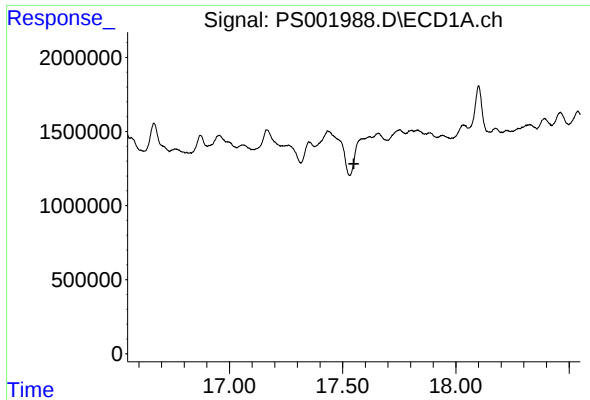

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

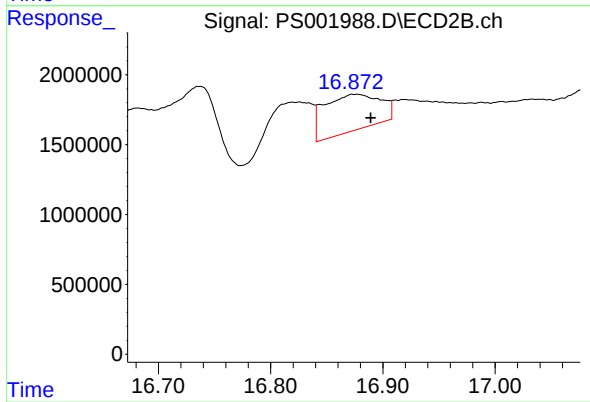

#16 DCPA

R.T.: 16.878 min
Delta R.T.: -0.012 min
Response: 9047405
Conc: 4.91 ng/ml