

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
 Data File : PS001993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2018 21:54
 Operator : EI\SJ
 Sample : PB113795BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 01:30:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.450	10.945	93810817	110.1E6	418.209	433.258
Target Compounds							
1) T	Dalapon	2.886	2.366	2194147	-1608552	6.748	N.D. #
3) T	4-Nitroph...	11.016	0.000	1808737	0	12.851	N.D. #
5) T	DICAMBA	0.000	11.187	0	649275	N.D.	0.728 #
6) T	MCP	12.136	0.000	8986561	0	14.102	N.D. #
7) T	MCPA	12.415	11.805	-8661489	13334735	N.D.	15.384
9) T	2,4-D	0.000	12.779	0	3137162	N.D.	10.084 #
12) T	2,4,5-T	0.000	14.566	0	6122532	N.D.	5.544 #
14) T	DINOSEB	0.000	15.631	0	2443963	N.D.	2.579 #
15) T	Picloram	16.972	16.877	20092279	41681603	11.539	24.508 #
16) T	DCPA	0.000	16.877	0	41681603	N.D.	22.599 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
Data File : PS001993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2018 21:54
Operator : EI\SJ
Sample : PB113795BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 01:30:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

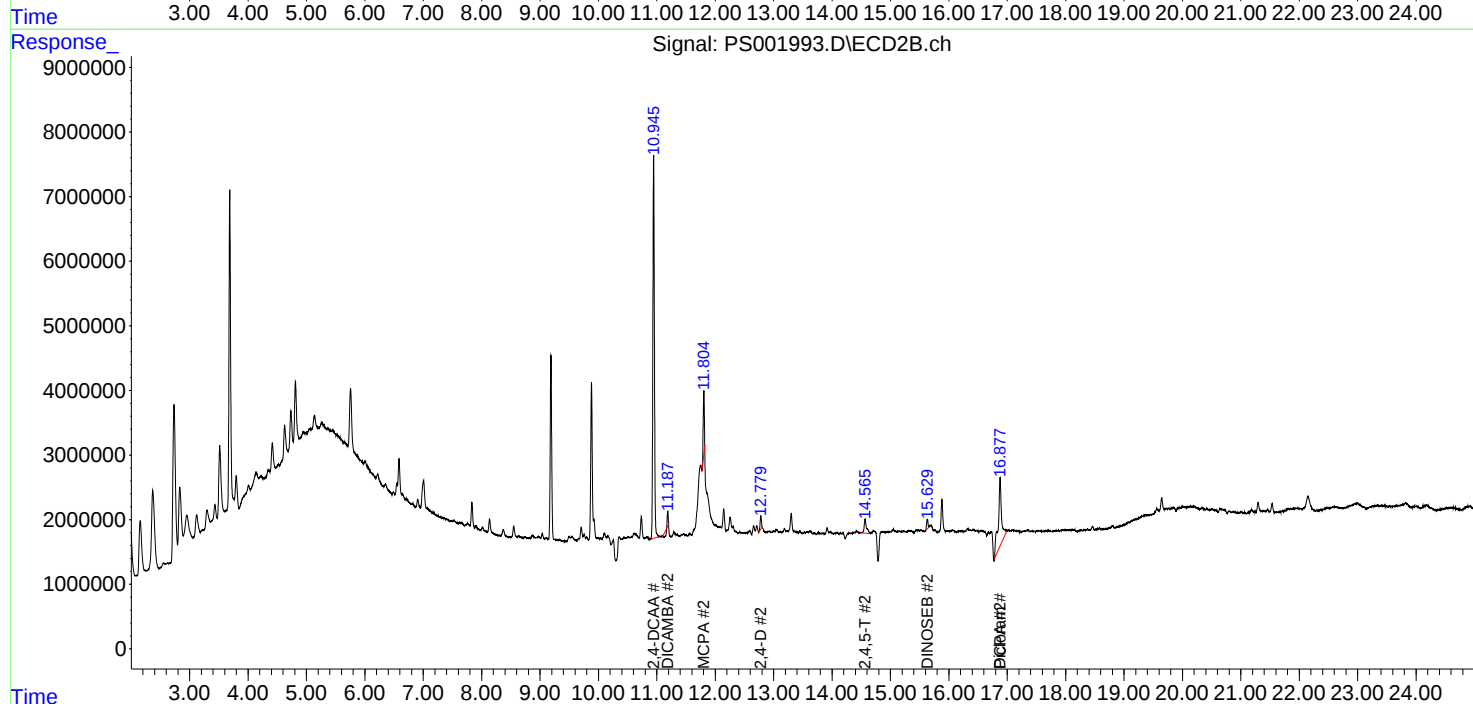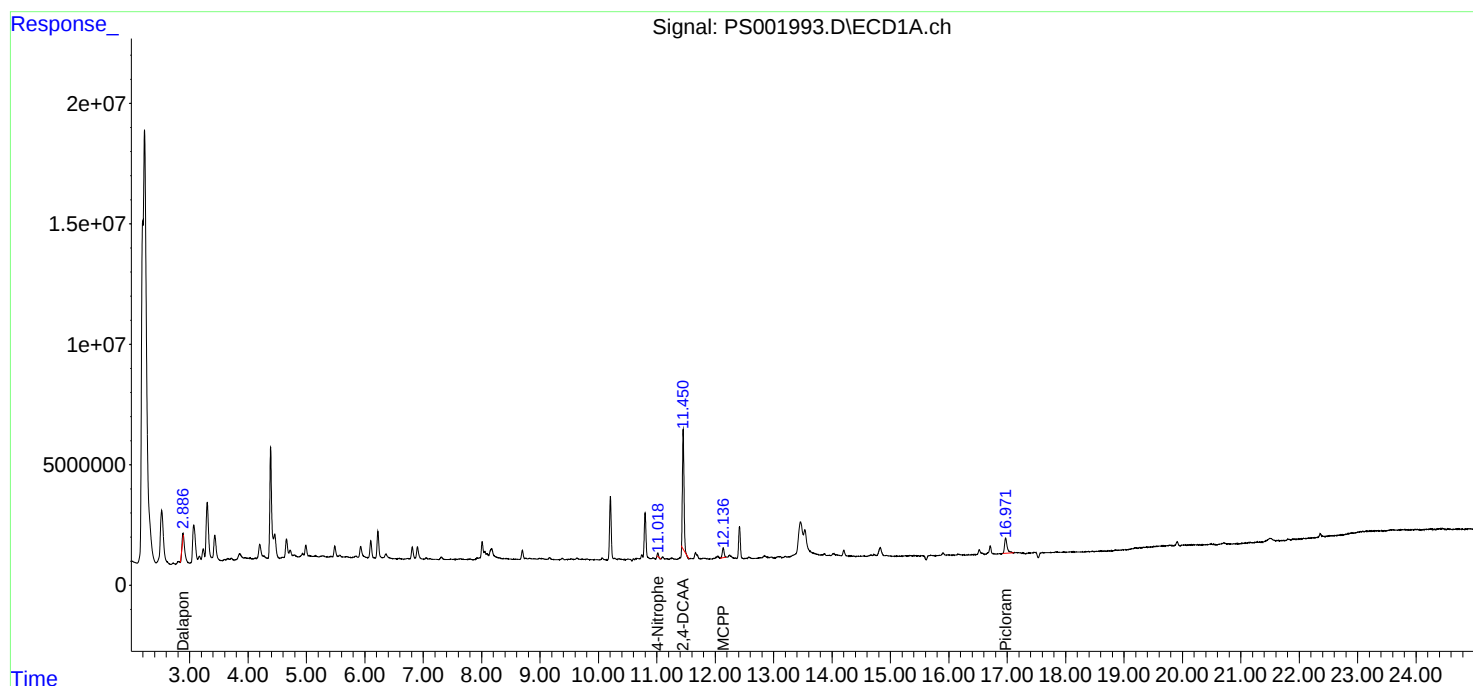


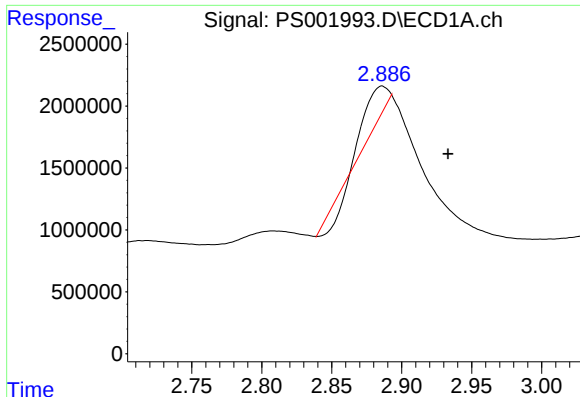

#1 Dalapon


R.T.: 2.886 min
Delta R.T.: -0.047 min
Response: 2194147
Conc: 6.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

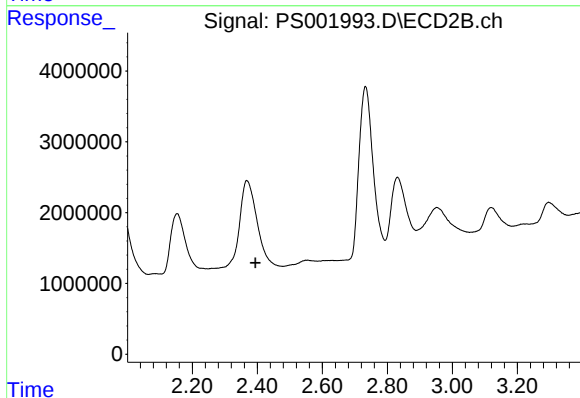


#1 Dalapon

R.T.: 2.366 min
Delta R.T.: -0.028 min
Response: -1608552
Conc: N.D.

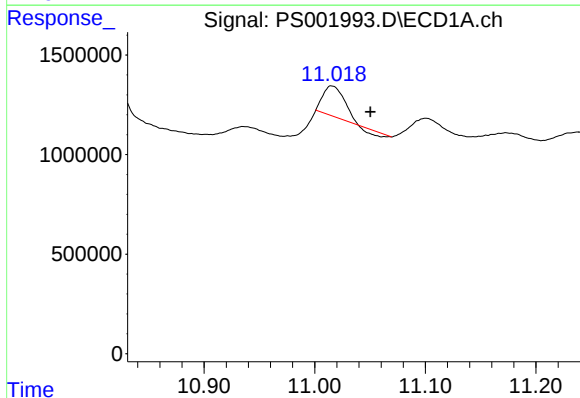


#3 4-Nitrophenol

R.T.: 11.016 min
Delta R.T.: -0.035 min
Response: 1808737
Conc: 12.85 ng/ml

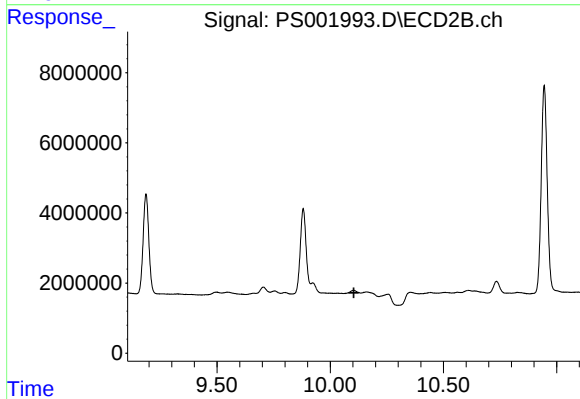

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 10.105 min
Response: 0
Conc: N.D.

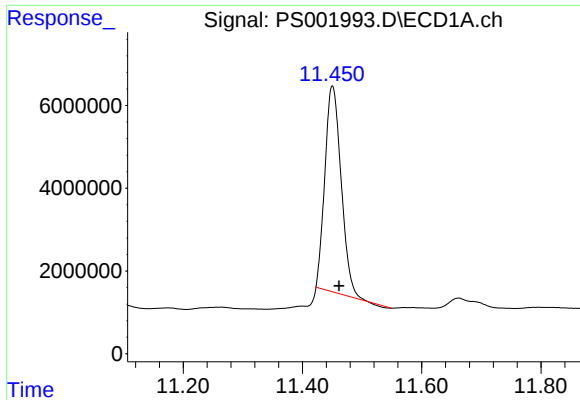

#4 2,4-DCAA


R.T.: 11.450 min
Delta R.T.: -0.011 min
Response: 93810817
Conc: 418.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

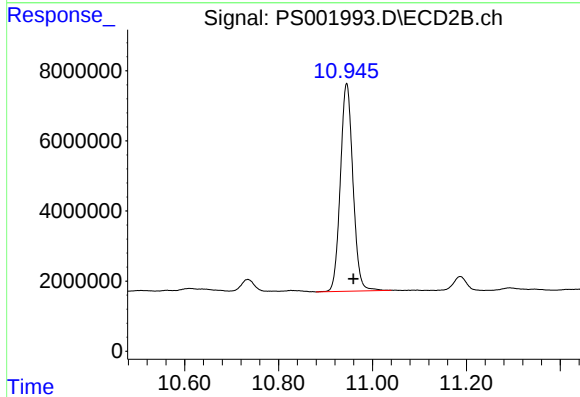


#4 2,4-DCAA

R.T.: 10.945 min
Delta R.T.: -0.015 min
Response: 110054771
Conc: 433.26 ng/ml

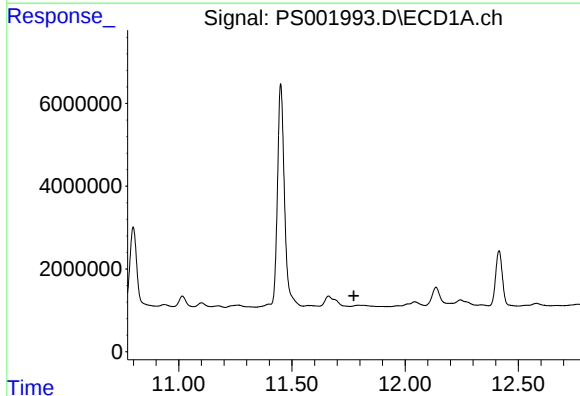


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.774 min
Response: 0
Conc: N.D.

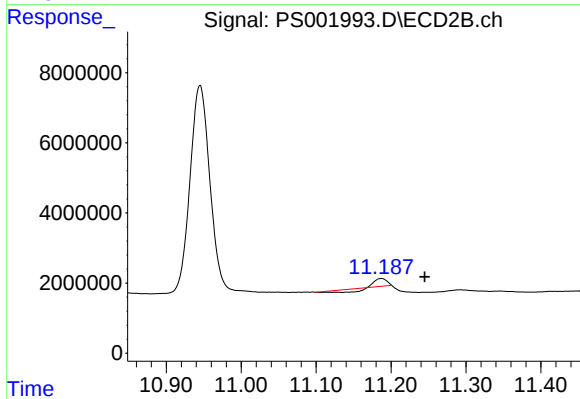

#5 DICAMBA


R.T.: 11.187 min
Delta R.T.: -0.058 min
Response: 649275
Conc: 0.73 ng/ml

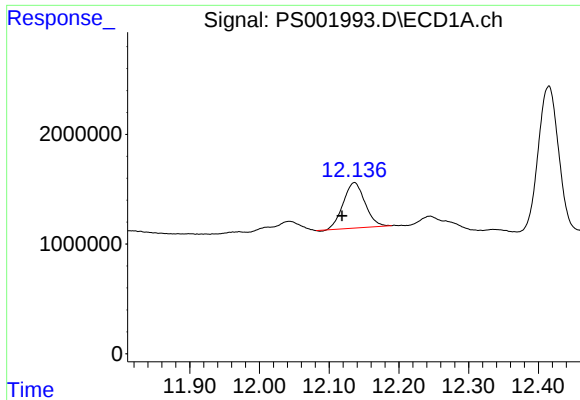

#6 MCPP


R.T.: 12.136 min
Delta R.T.: 0.018 min
Response: 8986561
Conc: 14.10 ug/ml

Instrument :
ECD_S
ClientSampleId :

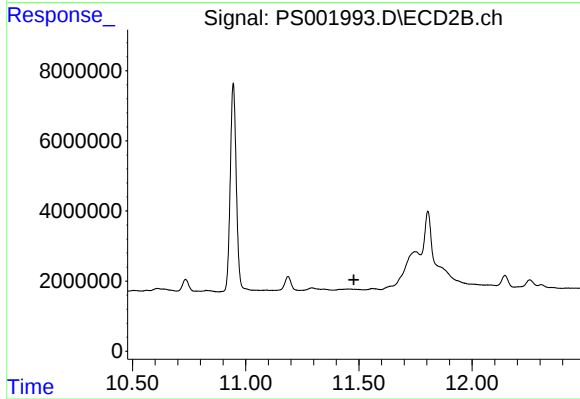


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

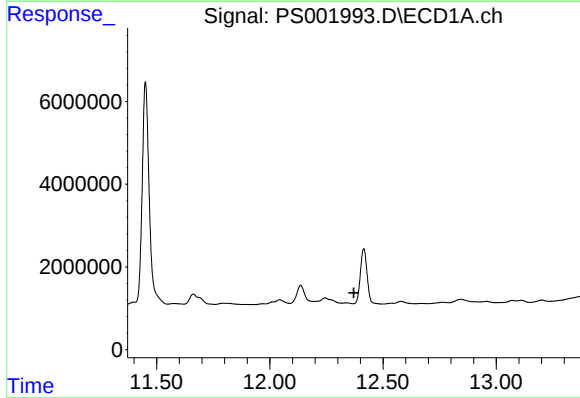


#7 MCPA

R.T.: 12.415 min
Delta R.T.: 0.044 min
Response: -8661489
Conc: N.D.

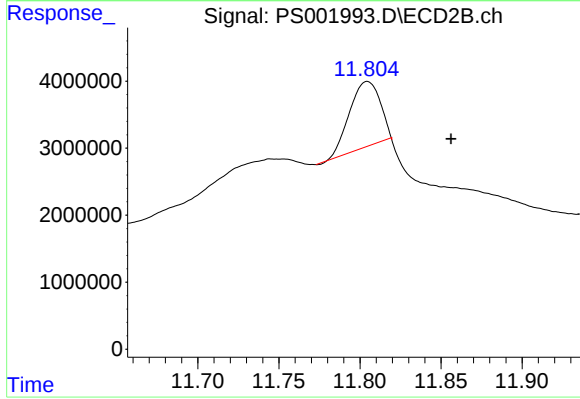

#7 MCPA


R.T.: 11.805 min
Delta R.T.: -0.052 min
Response: 13334735
Conc: 15.38 ug/ml

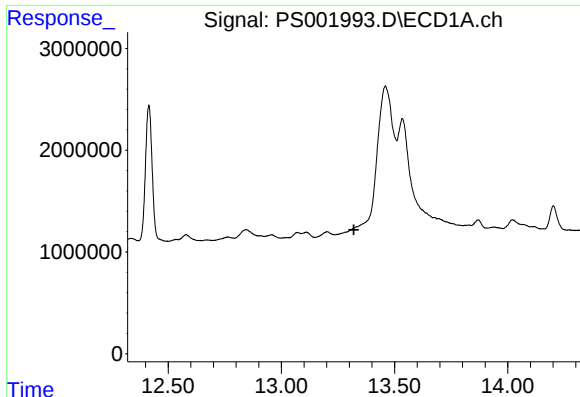

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

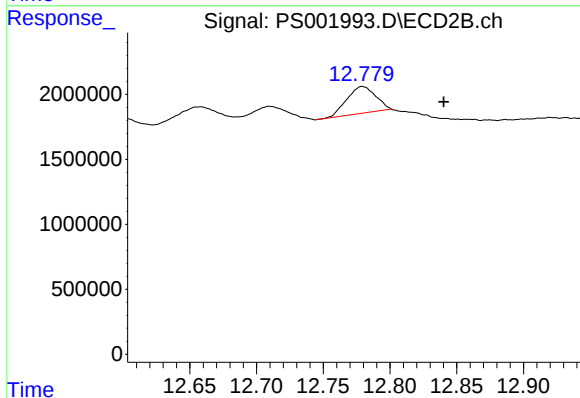


#9 2,4-D

R.T.: 12.779 min
Delta R.T.: -0.061 min
Response: 3137162
Conc: 10.08 ng/ml

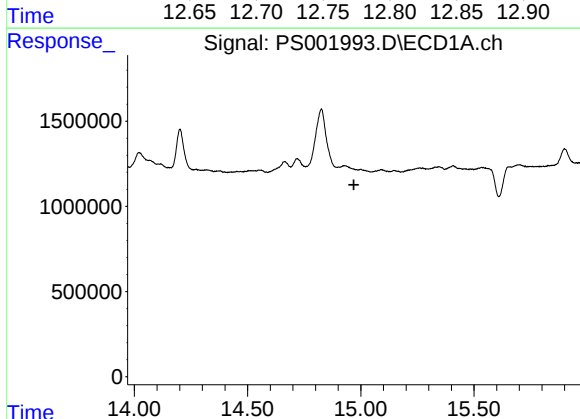


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.969 min
Response: 0
Conc: N.D.

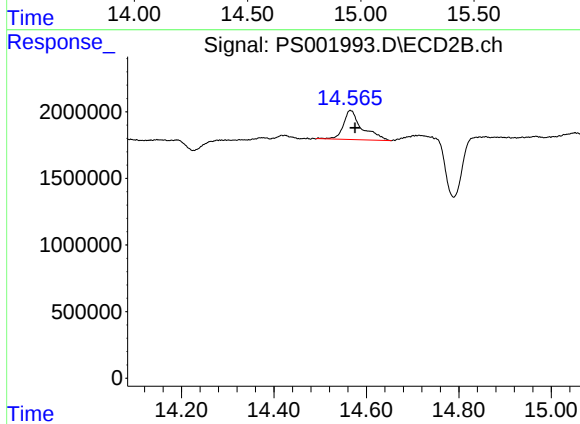

#12 2,4,5-T


R.T.: 14.566 min
Delta R.T.: -0.010 min
Response: 6122532
Conc: 5.54 ng/ml

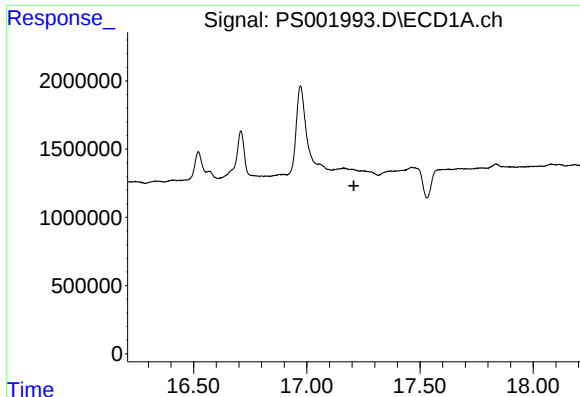

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.208 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

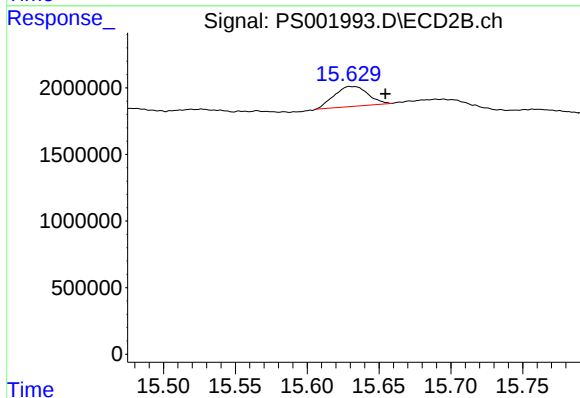


#14 DINOSEB

R.T.: 15.631 min
Delta R.T.: -0.023 min
Response: 2443963
Conc: 2.58 ng/ml

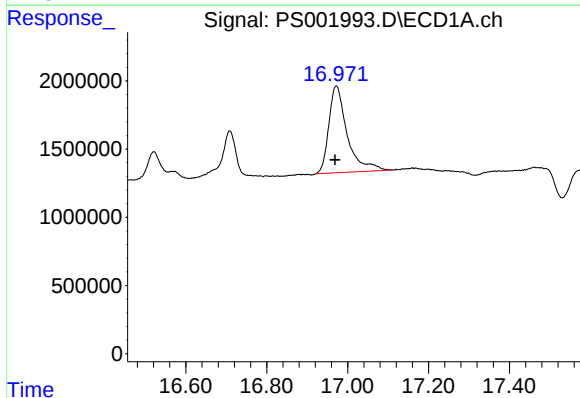


#15 Picloram

R.T.: 16.972 min
Delta R.T.: 0.003 min
Response: 20092279
Conc: 11.54 ng/ml

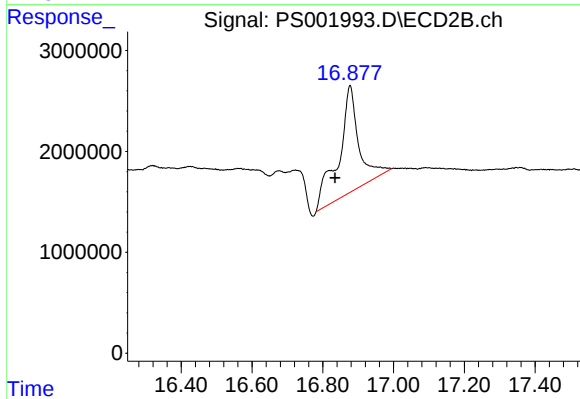

#15 Picloram


R.T.: 16.877 min
Delta R.T.: 0.042 min
Response: 41681603
Conc: 24.51 ng/ml

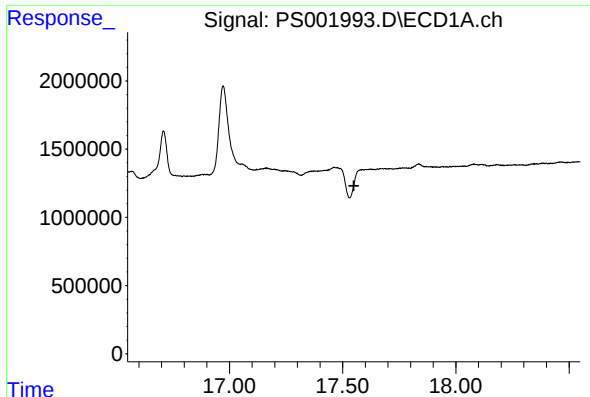

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

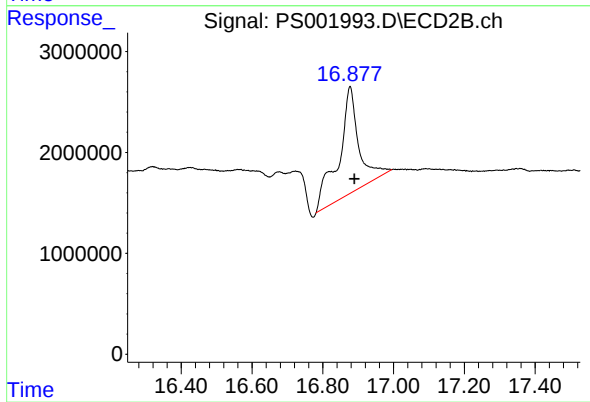

#16 DCPA

R.T.: 16.877 min
Delta R.T.: -0.012 min
Response: 41681603
Conc: 22.60 ng/ml