

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
 Data File : PS001996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2018 23:27
 Operator : EI\SJ
 Sample : J5392-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 01:31:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.462	10.956	99208789	98628166	442.273	388.274
Target Compounds							
1) T	Dalapon	0.000	2.378	0	6397962	N.D.	21.657 #
2) T	3,5-DICHL...	0.000	9.047	0	1850279	N.D.	5.862 #
6) T	MCP	12.145	0.000	13932065	0	21.863	N.D. #
9) T	2,4-D	0.000	12.790	0	3933468	N.D.	12.643 #
15) T	Picloram	0.000	16.890	0	8559607	N.D.	5.033 #
16) T	DCPA	0.000	16.890	0	8559607	N.D.	4.641 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
Data File : PS001996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2018 23:27
Operator : EI\SJ
Sample : J5392-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 01:31:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

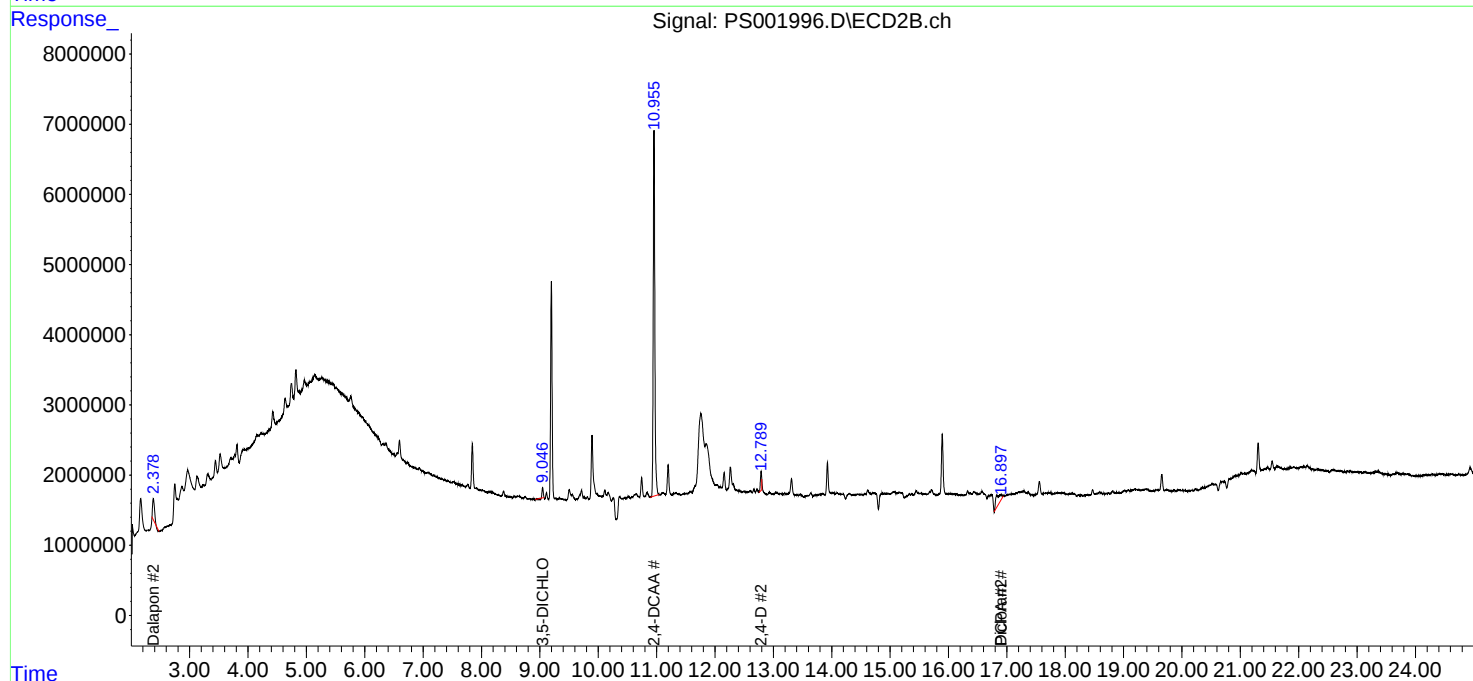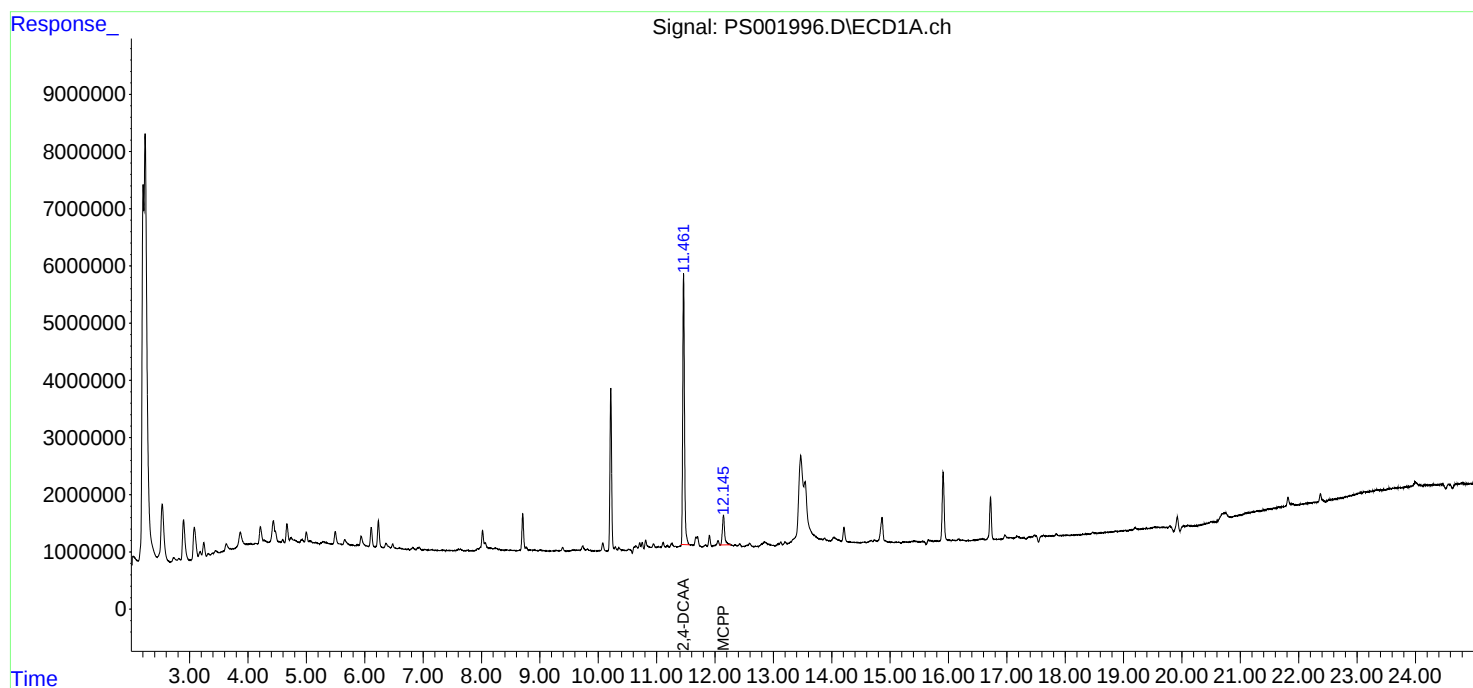


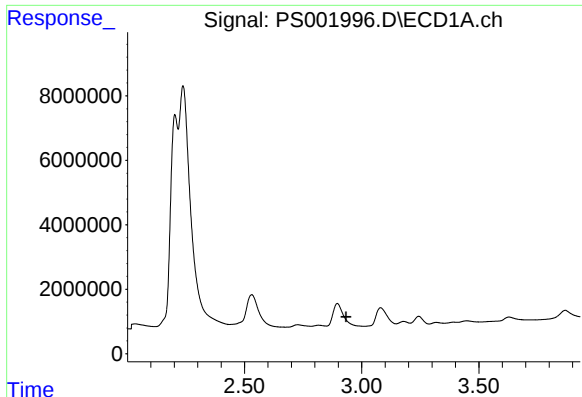

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.933 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

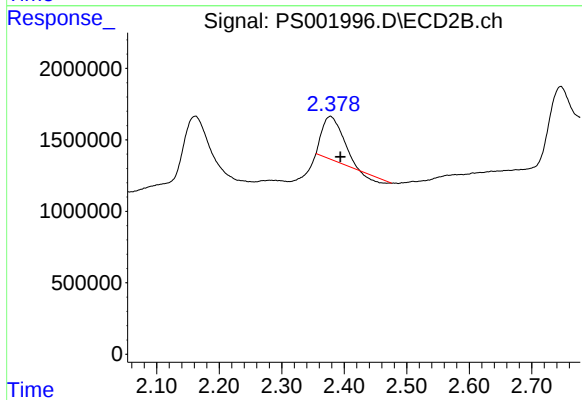


#1 Dalapon

R.T.: 2.378 min
Delta R.T.: -0.016 min
Response: 6397962
Conc: 21.66 ng/ml

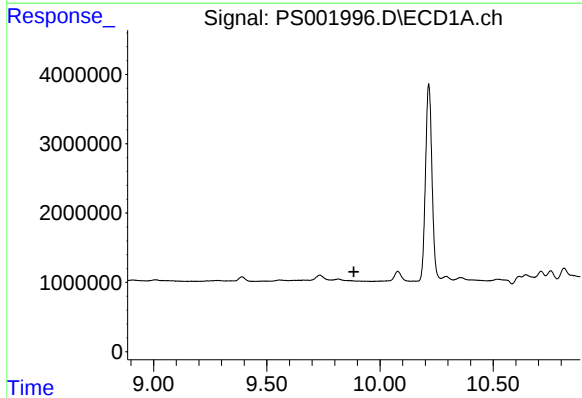


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.884 min
Response: 0
Conc: N.D.

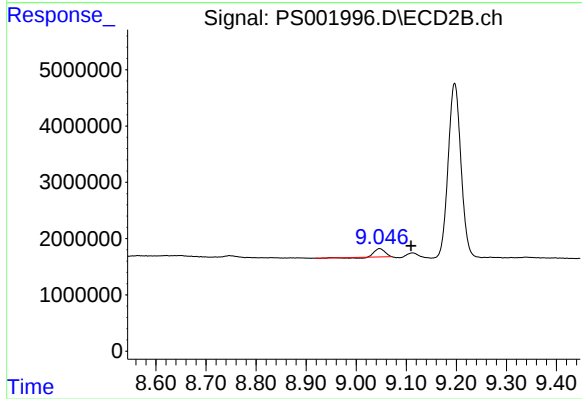

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.047 min
Delta R.T.: -0.063 min
Response: 1850279
Conc: 5.86 ng/ml

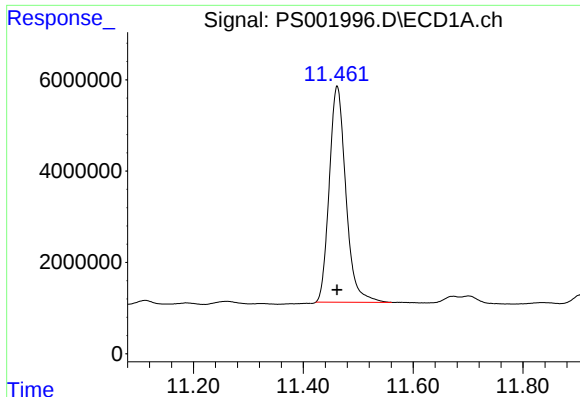

#4 2,4-DCAA


R.T.: 11.462 min
Delta R.T.: 0.000 min
Response: 99208789
Conc: 442.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

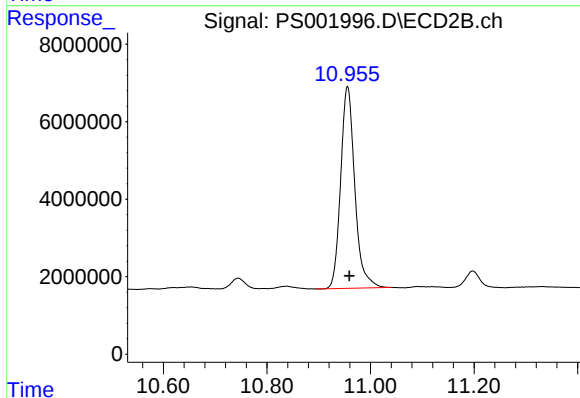


#4 2,4-DCAA

R.T.: 10.956 min
Delta R.T.: -0.004 min
Response: 98628166
Conc: 388.27 ng/ml

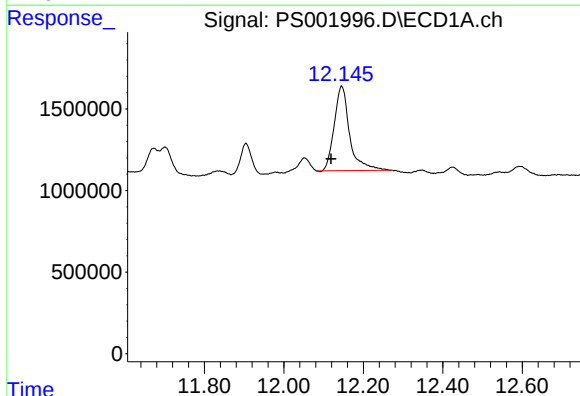


#6 MCP

R.T.: 12.145 min
Delta R.T.: 0.027 min
Response: 13932065
Conc: 21.86 ug/ml

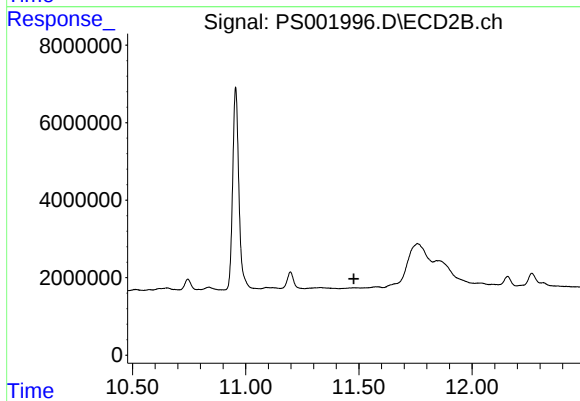

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.478 min
Response: 0
Conc: N.D.

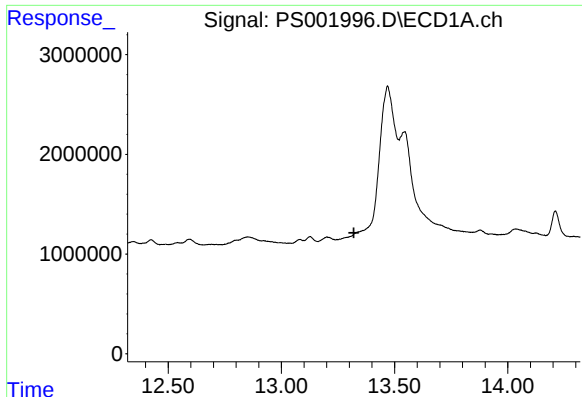

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

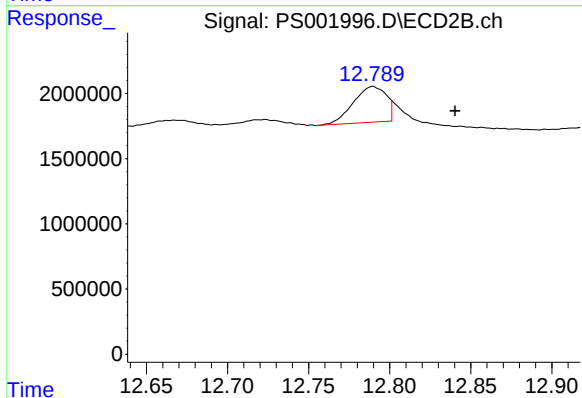


#9 2,4-D

R.T.: 12.790 min
Delta R.T.: -0.050 min
Response: 3933468
Conc: 12.64 ng/ml

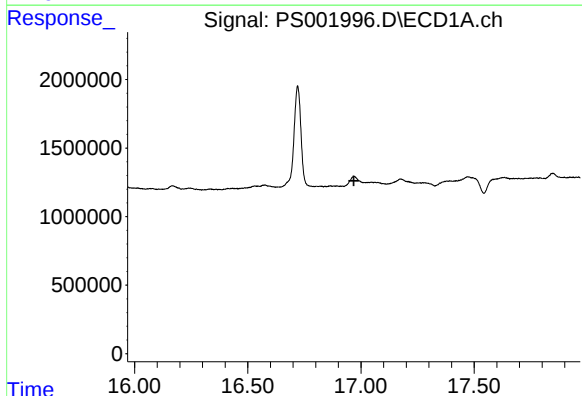


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.969 min
Response: 0
Conc: N.D.

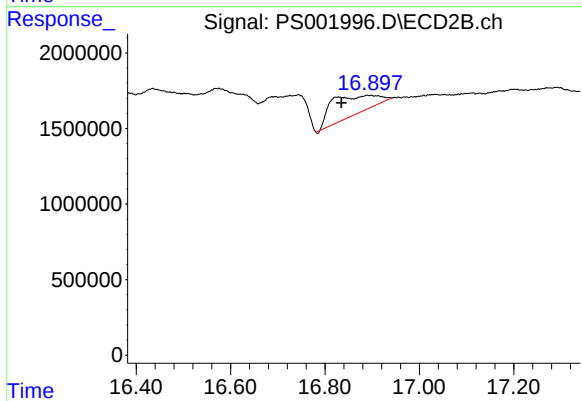

#15 Picloram


R.T.: 16.890 min
Delta R.T.: 0.055 min
Response: 8559607
Conc: 5.03 ng/ml

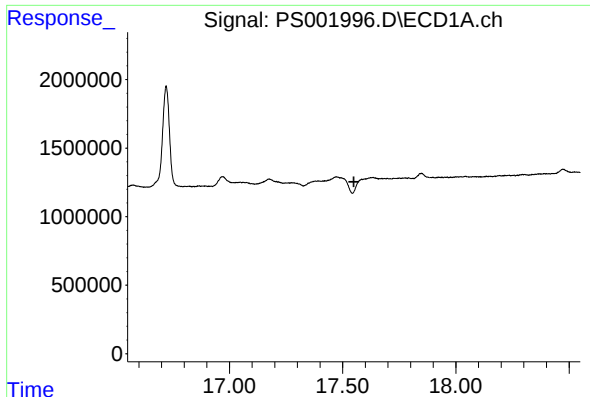

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

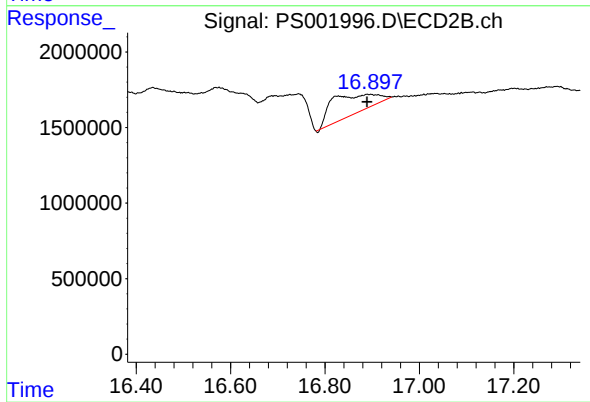

#16 DCPA

R.T.: 16.890 min
Delta R.T.: 0.000 min
Response: 8559607
Conc: 4.64 ng/ml