

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
 Data File : PS002001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2018 02:03
 Operator : EI\SJ
 Sample : J5205-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 03:57:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.448	10.942	54949030	75658096	244.963	297.847
Target Compounds							
1) T	Dalapon	2.882	0.000	2097356	0	6.450	N.D. #
5) T	DICAMBA	0.000	11.184	0	5605052	N.D.	6.285 #
6) T	MCPD	12.128	0.000	14446032	0	22.670	N.D. #
12) T	2,4,5-T	0.000	14.560	0	1669758	N.D.	1.512 #
15) T	Picloram	16.964	16.872	15095125	22909223	8.669	13.470 #
16) T	DCPA	17.608	16.872	-58128	22909223	N.D.	12.421



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
Data File : PS002001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2018 02:03
Operator : EI\SJ
Sample : J5205-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 03:57:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

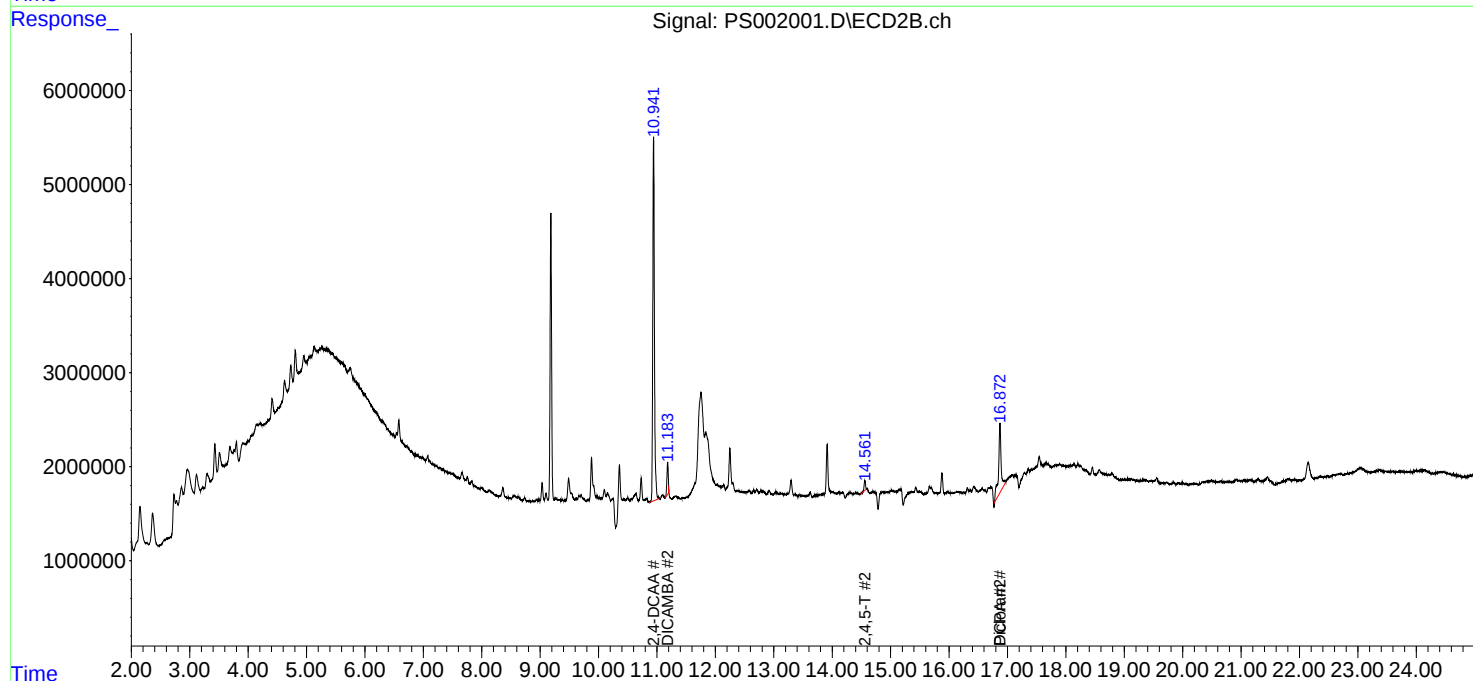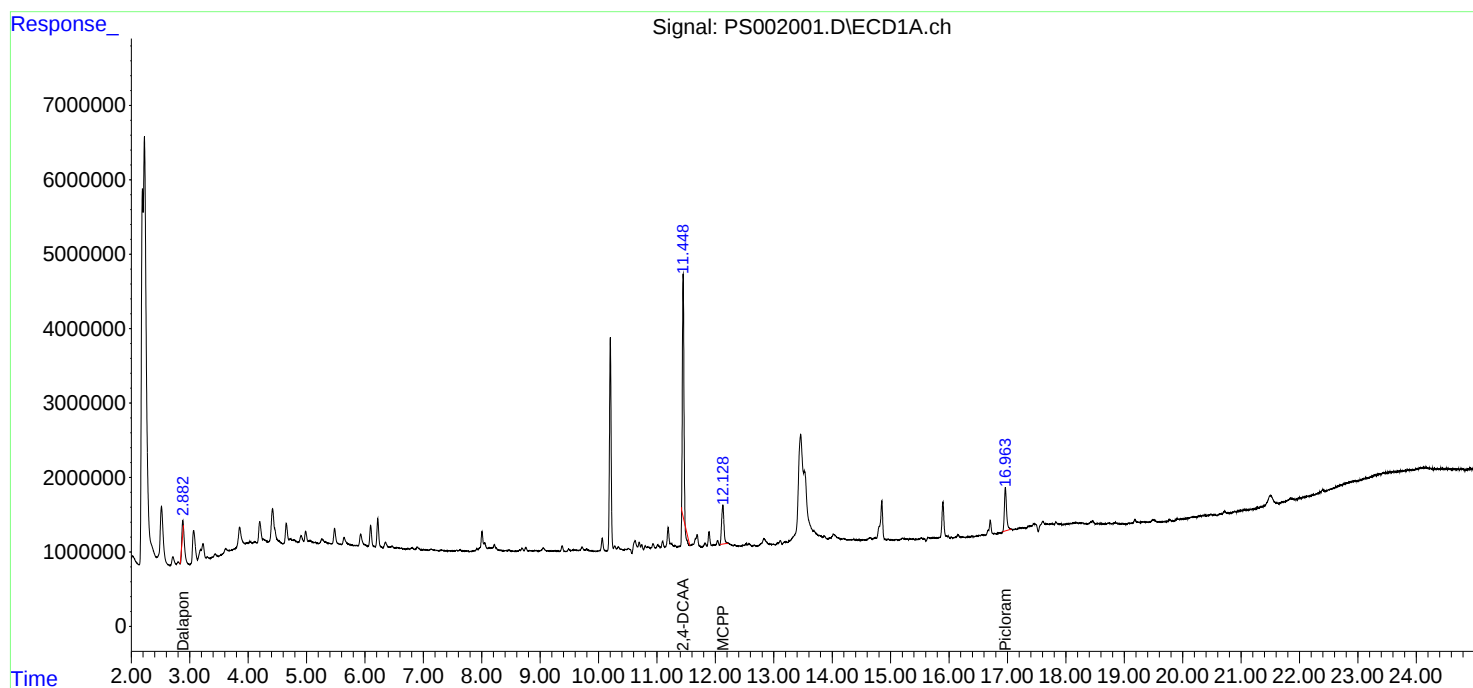


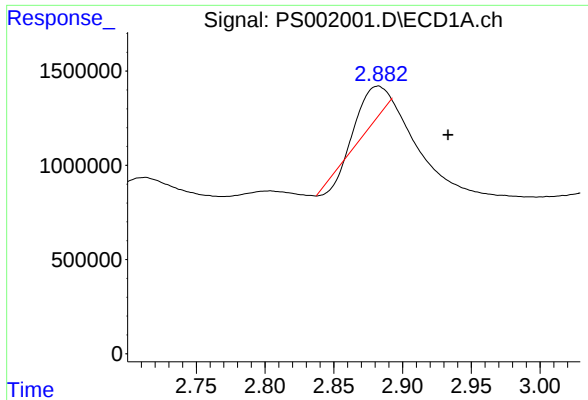

#1 Dalapon


R.T.: 2.882 min
Delta R.T.: -0.051 min
Response: 2097356
Conc: 6.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

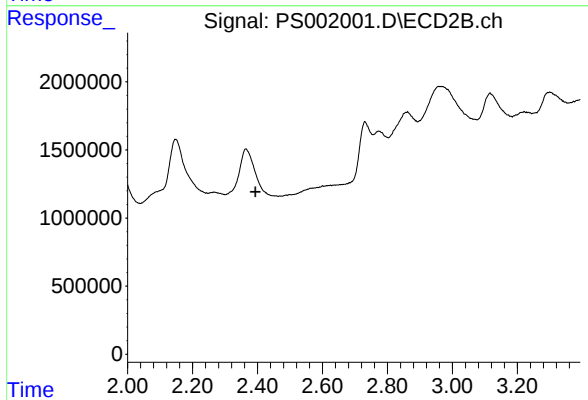


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.394 min
Response: 0
Conc: N.D.

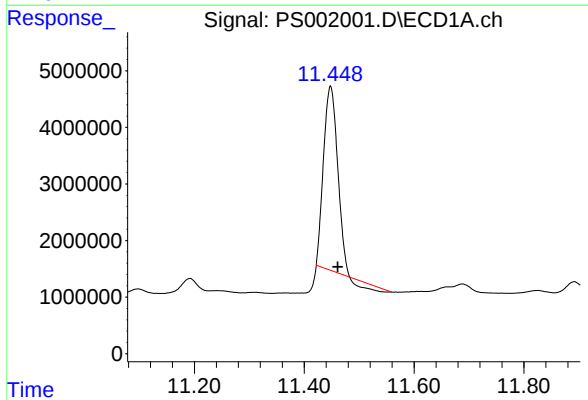


#4 2,4-DCAA

R.T.: 11.448 min
Delta R.T.: -0.013 min
Response: 54949030
Conc: 244.96 ng/ml

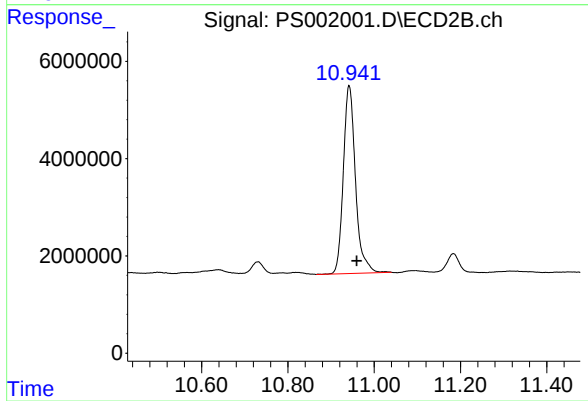

#4 2,4-DCAA


R.T.: 10.942 min
Delta R.T.: -0.018 min
Response: 75658096
Conc: 297.85 ng/ml

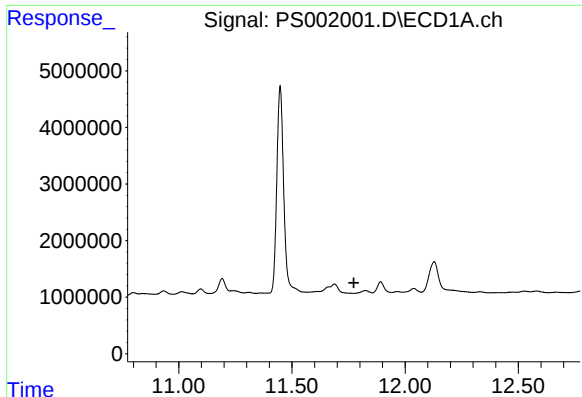

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.774 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

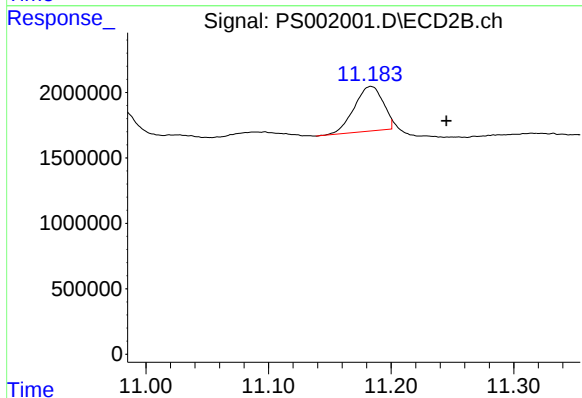


#5 DICAMBA

R.T.: 11.184 min
Delta R.T.: -0.062 min
Response: 5605052
Conc: 6.28 ng/ml

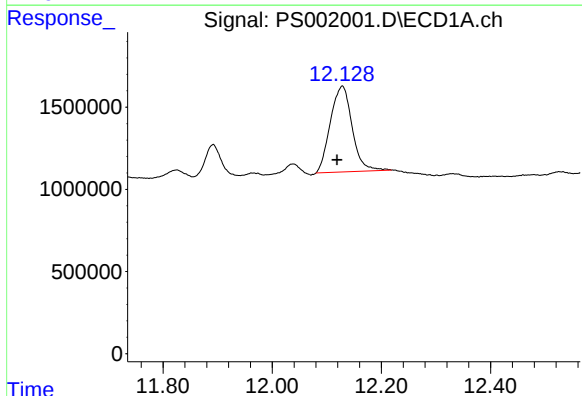


#6 MCP

R.T.: 12.128 min
Delta R.T.: 0.010 min
Response: 14446032
Conc: 22.67 ug/ml

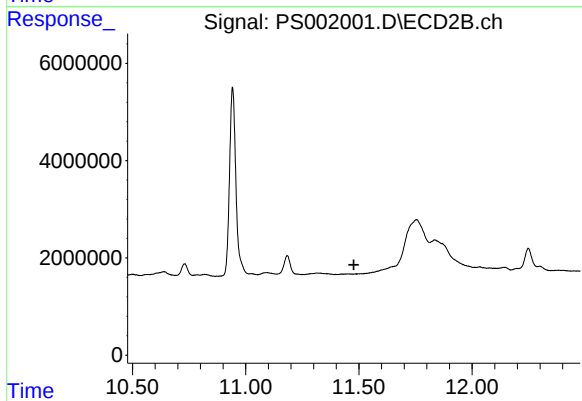

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.478 min
Response: 0
Conc: N.D.

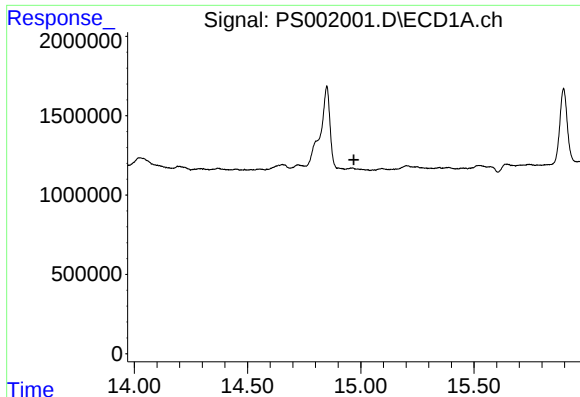

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

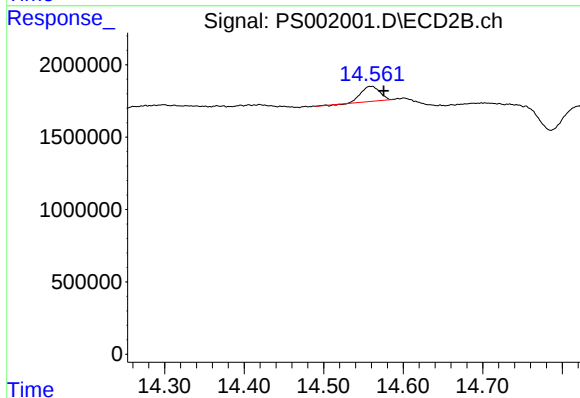


#12 2,4,5-T

R.T.: 14.560 min
Delta R.T.: -0.016 min
Response: 1669758
Conc: 1.51 ng/ml

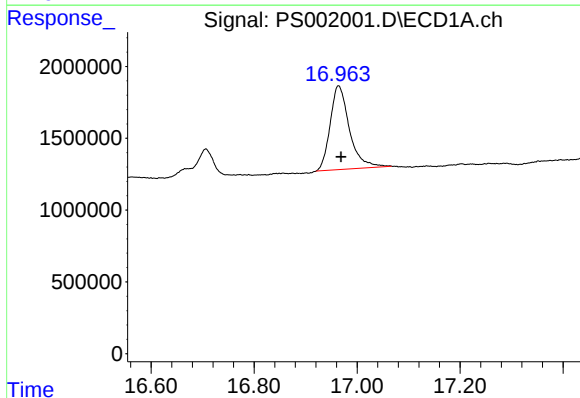


#15 Picloram

R.T.: 16.964 min
Delta R.T.: -0.005 min
Response: 15095125
Conc: 8.67 ng/ml

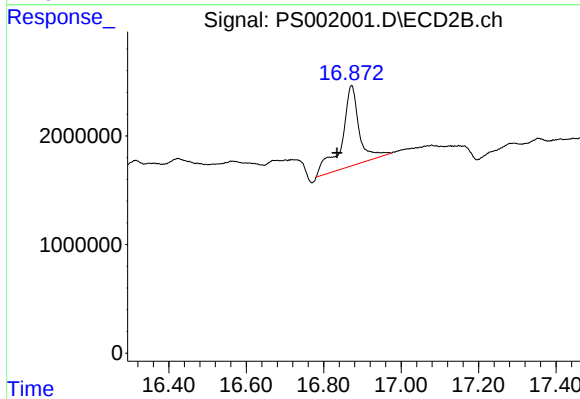

#15 Picloram


R.T.: 16.872 min
Delta R.T.: 0.037 min
Response: 22909223
Conc: 13.47 ng/ml

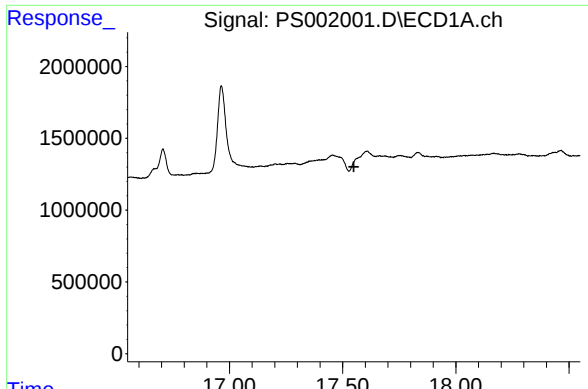

#16 DCPA

R.T.: 17.608 min
Delta R.T.: 0.059 min
Response: -58128
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

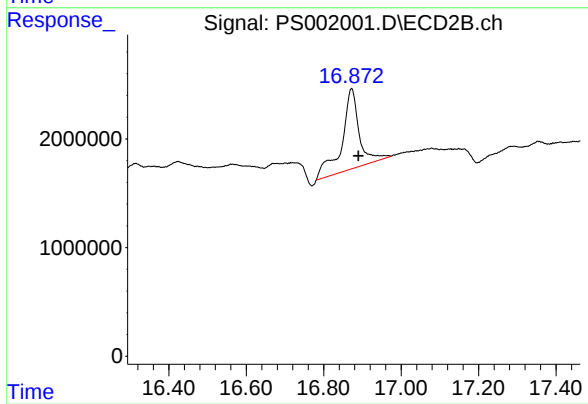

#16 DCPA

R.T.: 16.872 min
Delta R.T.: -0.017 min
Response: 22909223
Conc: 12.42 ng/ml