

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
 Data File : PS002003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2018 03:05
 Operator : EI\SJ
 Sample : J5457-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 03:58:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 10 11:21:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.463	10.943	116.0E6	113.8E6	517.021	447.941
Target Compounds							
2) T	3,5-DICHL...	0.000	9.100	0	2014866	N.D.	6.384 #
5) T	DICAMBA	0.000	11.184	0	100232	N.D.	0.112 #
6) T	MCP	12.147	0.000	12042316	0	18.898	N.D. #
15) T	Picloram	0.000	16.821	0	3806312	N.D.	2.238 #
16) T	DCPA	0.000	16.874	0	5687910	N.D.	3.084 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101218\
Data File : PS002003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2018 03:05
Operator : EI\SJ
Sample : J5457-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 03:58:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091718.M
Quant Title : 8080.M
QLast Update : Wed Oct 10 11:21:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

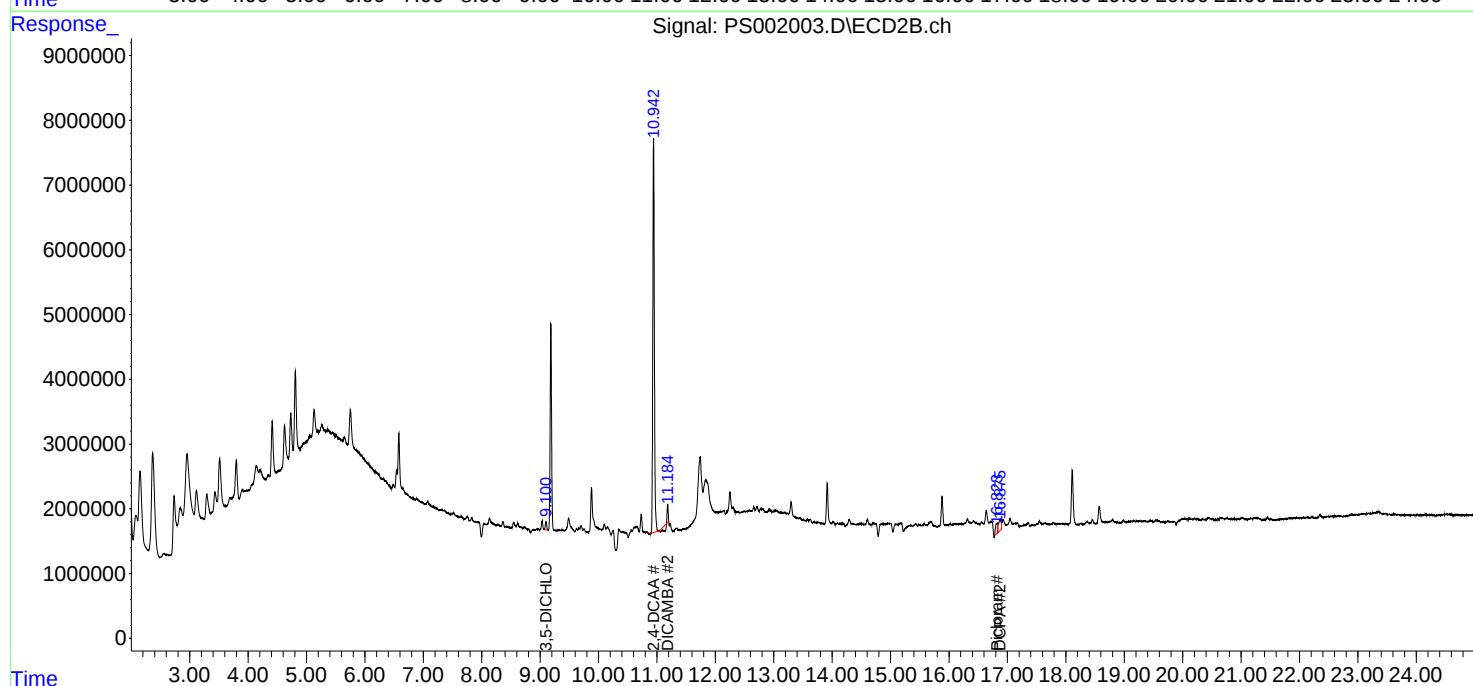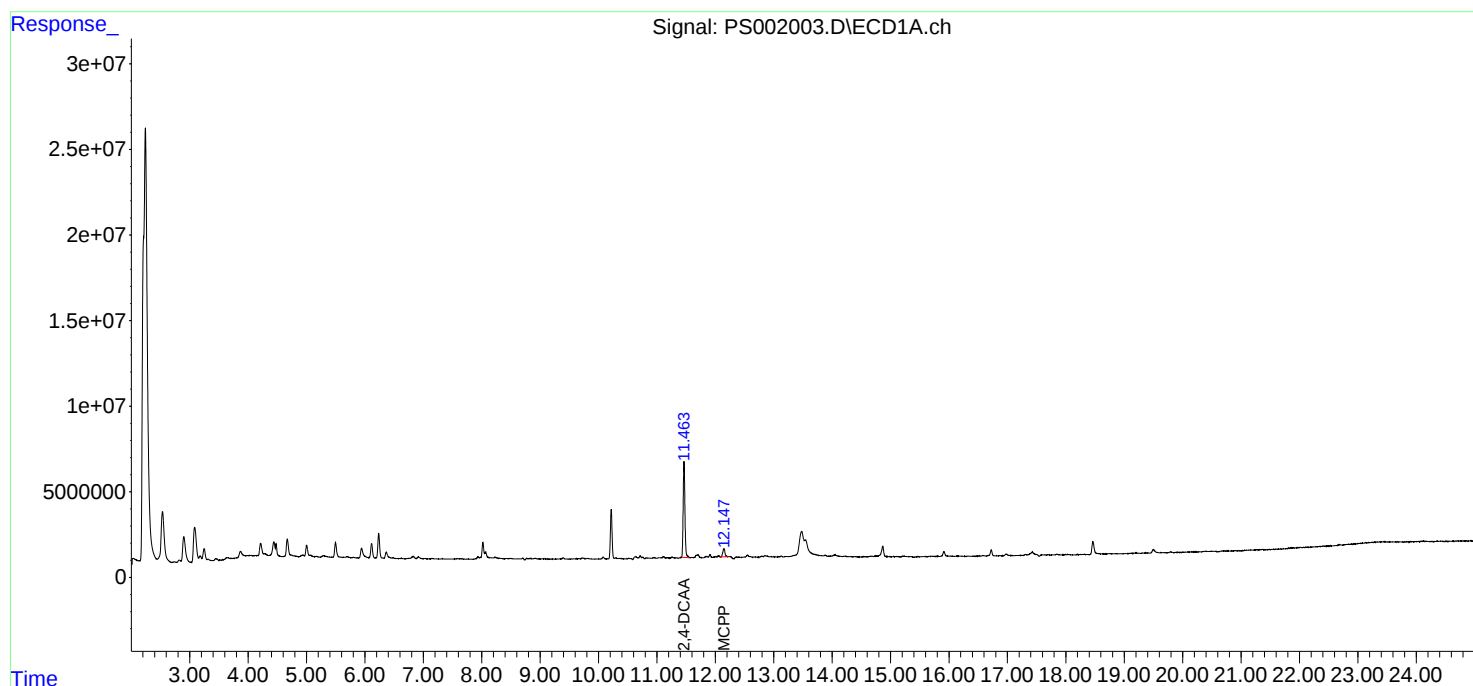


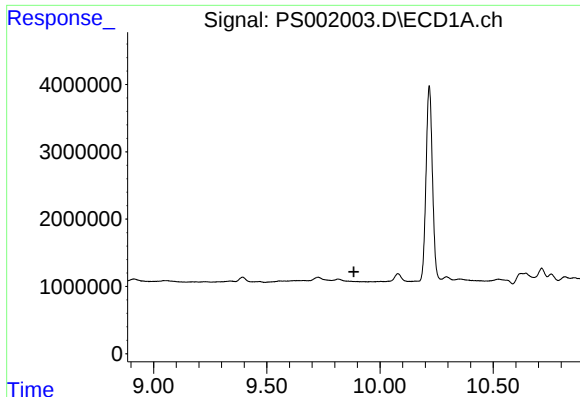

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.884 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

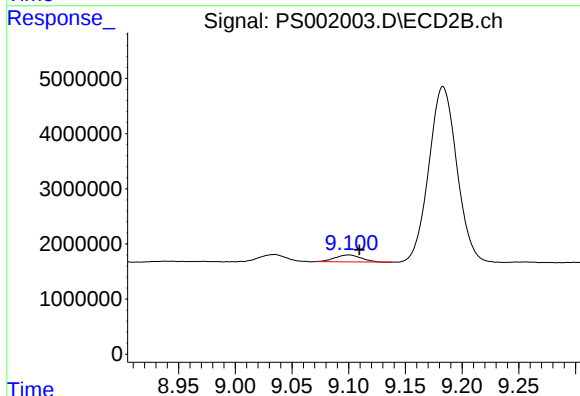


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.100 min
Delta R.T.: -0.009 min
Response: 2014866
Conc: 6.38 ng/ml

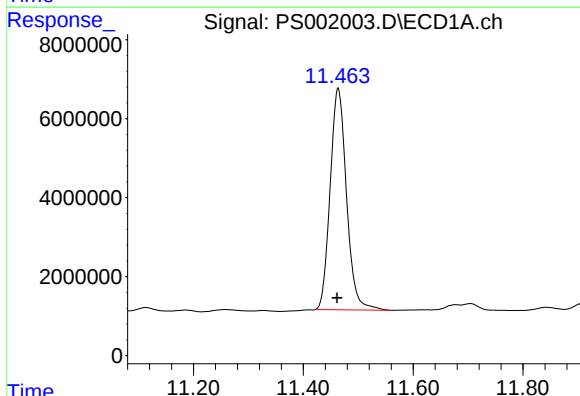


#4 2,4-DCAA

R.T.: 11.463 min
Delta R.T.: 0.002 min
Response: 115975994
Conc: 517.02 ng/ml

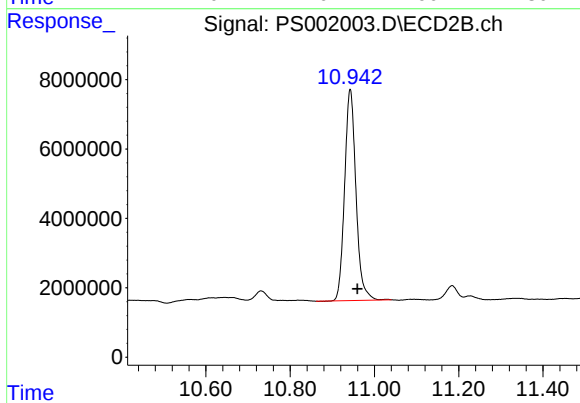

#4 2,4-DCAA


R.T.: 10.943 min
Delta R.T.: -0.017 min
Response: 113784456
Conc: 447.94 ng/ml

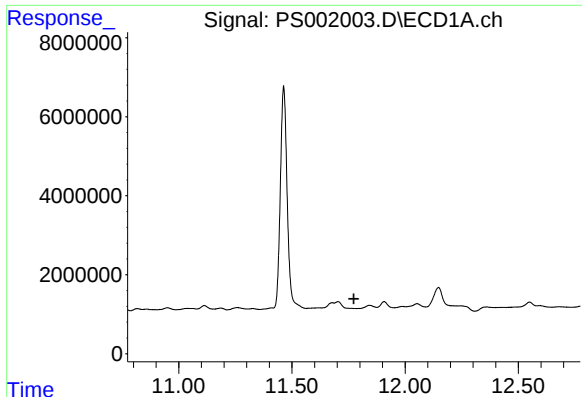

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.774 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

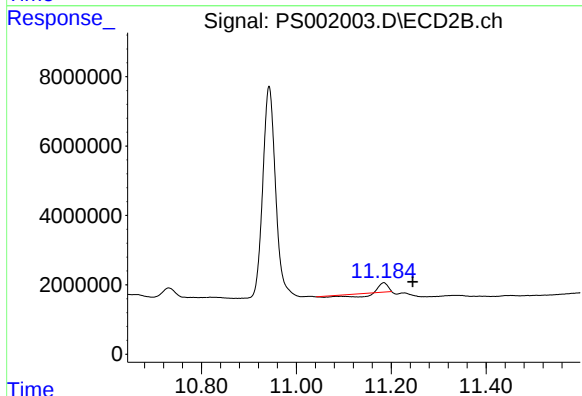


#5 DICAMBA

R.T.: 11.184 min
Delta R.T.: -0.061 min
Response: 100232
Conc: 0.11 ng/ml

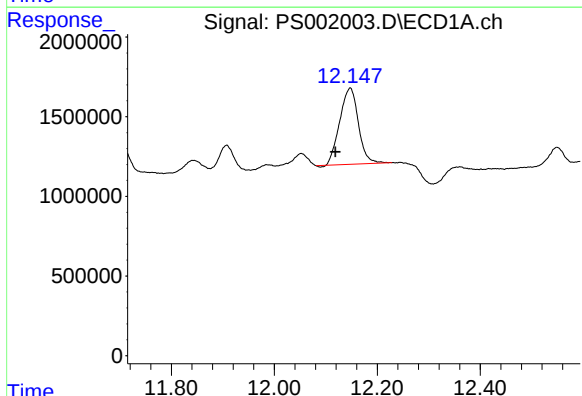


#6 MCP

R.T.: 12.147 min
Delta R.T.: 0.029 min
Response: 12042316
Conc: 18.90 ug/ml

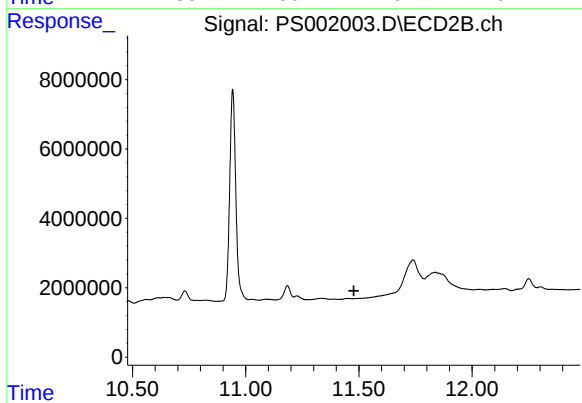

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.478 min
Response: 0
Conc: N.D.

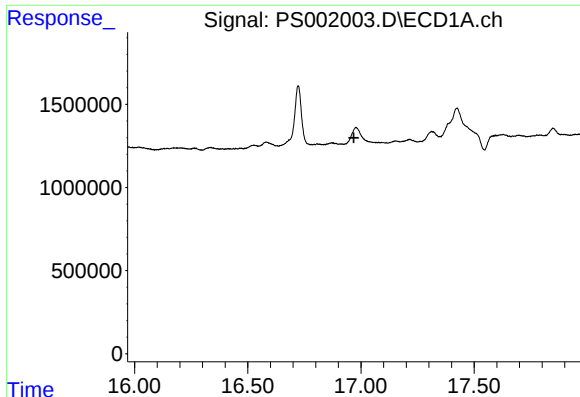

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

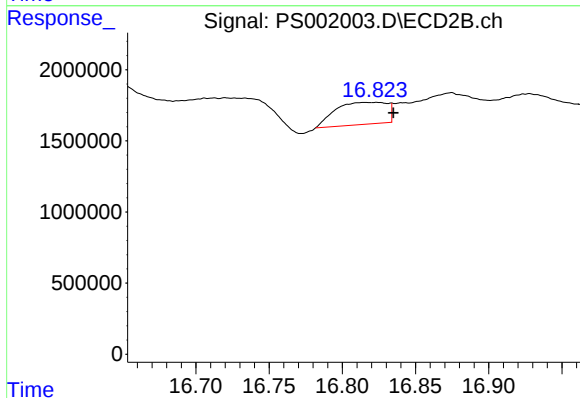


#15 Picloram

R.T.: 16.821 min
Delta R.T.: -0.014 min
Response: 3806312
Conc: 2.24 ng/ml

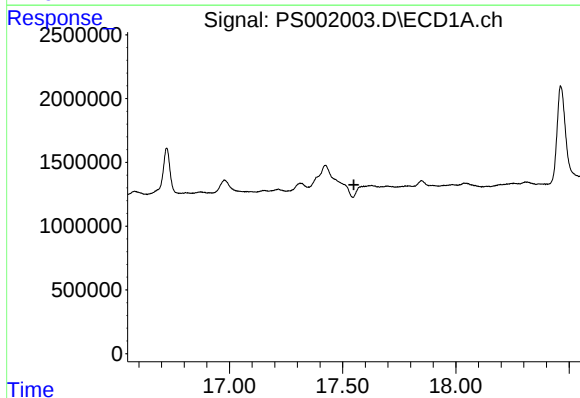

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.549 min
Response: 0
Conc: N.D.

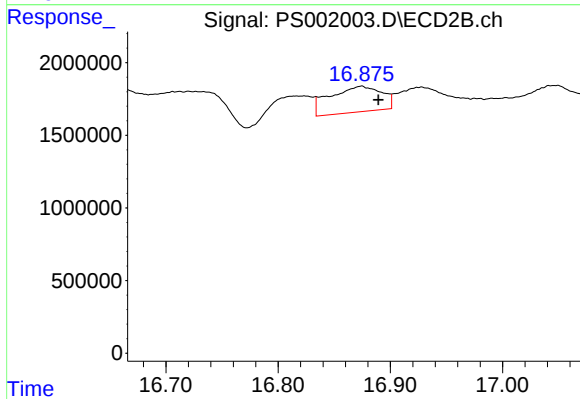

#16 DCPA

R.T.: 16.874 min
Delta R.T.: -0.015 min
Response: 5687910
Conc: 3.08 ng/ml