

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101222\
 Data File : PS020776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 09:20
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 00:32:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.431	0.000	1563730	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.553f	0.000	1117228	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.806	0.000	2876834	0	<MDL	N.D. #
5) T	DICAMBA	6.571	7.026	1013812	1095556	<MDL	<MDL #
6) T	MCP	6.747	7.152	2860193	1195086	<MDL	<MDL #
7) T	MCPA	6.881	0.000	665434	0	<MDL	N.D. #
8) T	DICHLORPROP	7.184	0.000	21639	0	<MDL	N.D. #
9) T	2,4-D	7.369	0.000	3183986	0	1.306	N.D. #
10) T	Pentachlo...	7.606	8.384	834343	1243882	<MDL	<MDL #
11) T	2,4,5-TP ...	8.135	8.749	4821827	1422132	<MDL	<MDL #
12) T	2,4,5-T	8.397	9.170	1855189	5705798	<MDL	<MDL #
13) T	2,4-DB	8.885	0.000	3480938	0	1.524	N.D. #
14) T	DINOSEB	9.972	0.000	2197601	0	<MDL	N.D. #
15) T	Picloram	9.790	10.936	33350524	21925492	2.003	1.860
16) T	DCPA	10.234	10.936	10045458	21925492	<MDL	2.134 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101222\
Data File : PS020776.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 09:20
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 00:32:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

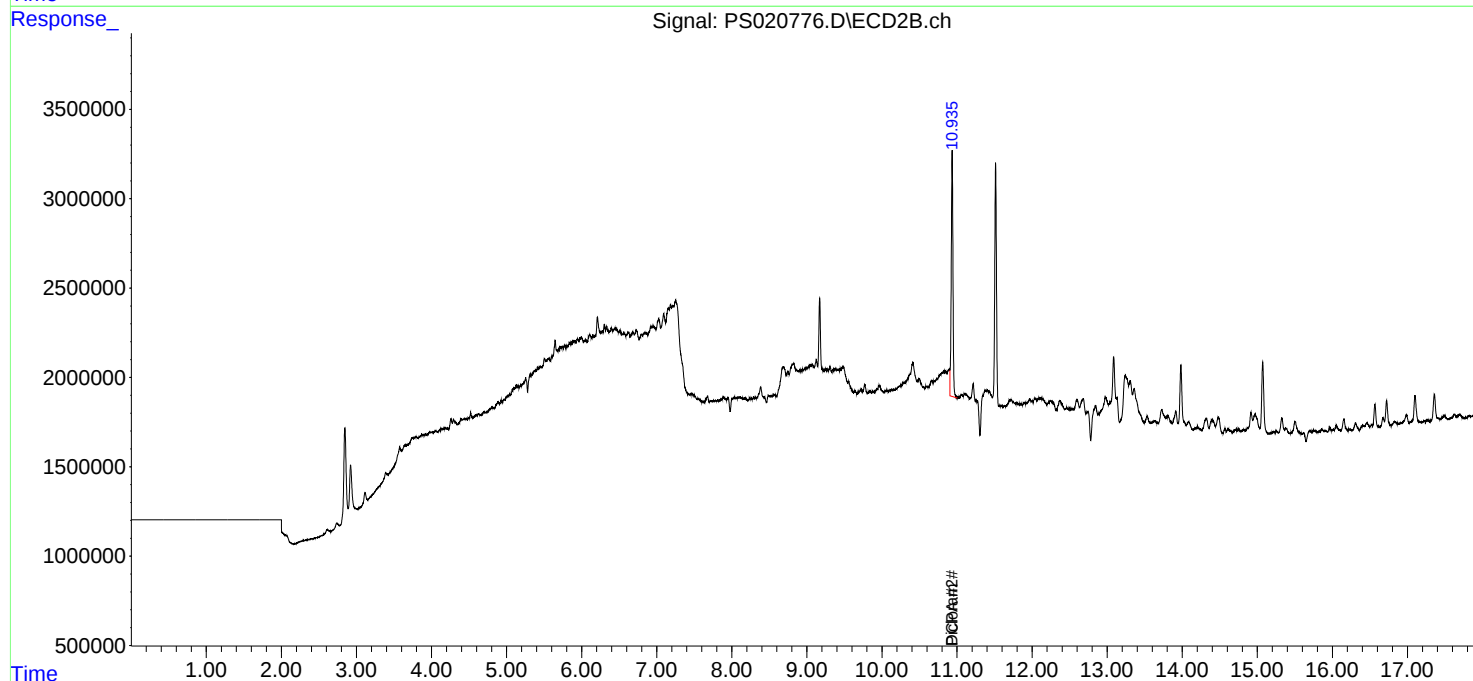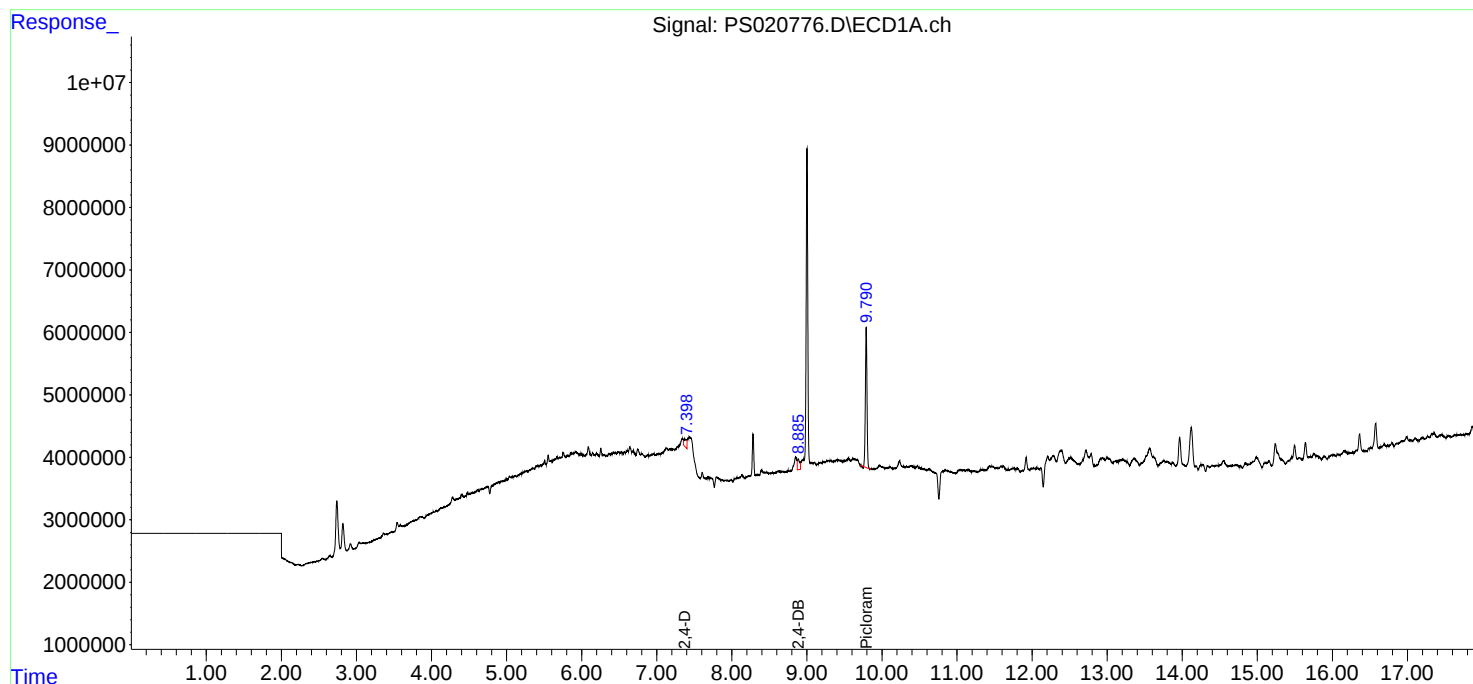


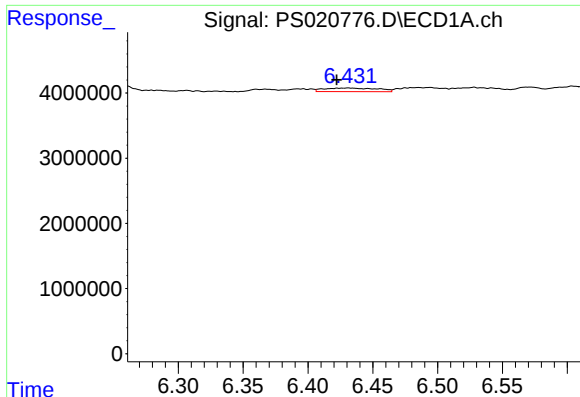

#4 2,4-DCAA


R.T.: 6.431 min
Delta R.T.: 0.009 min
Response: 1563730
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

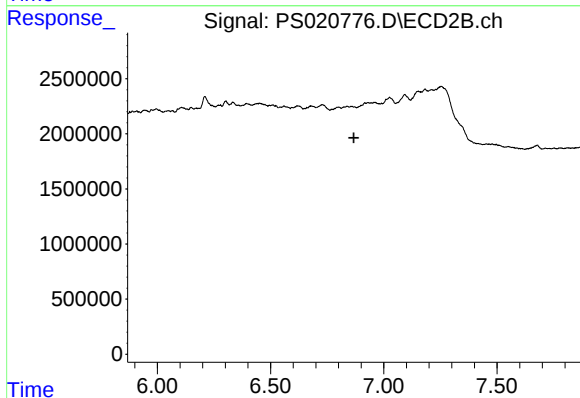


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.868 min
Response: 0
Conc: N.D.

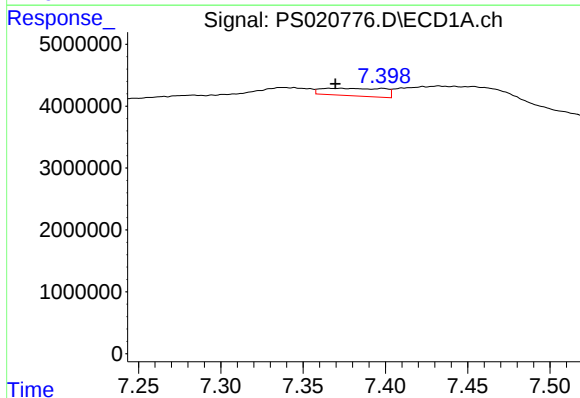


#9 2,4-D

R.T.: 7.369 min
Delta R.T.: 0.000 min
Response: 3183986
Conc: 1.31 ng/ml

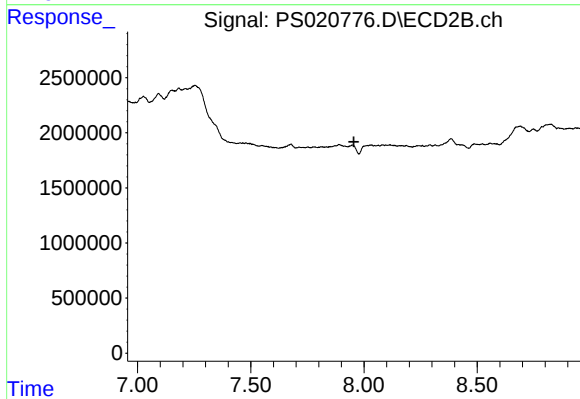

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.956 min
Response: 0
Conc: N.D.

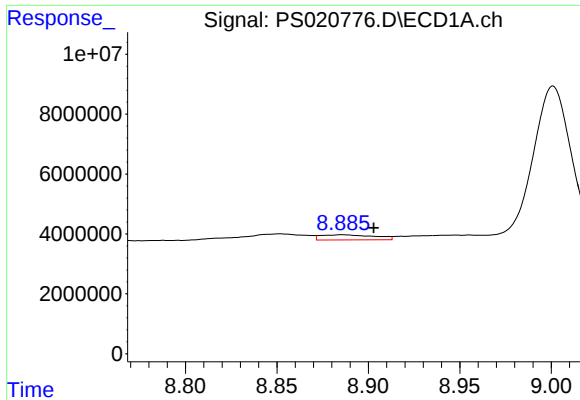

#13 2,4-DB


R.T.: 8.885 min
Delta R.T.: -0.017 min
Response: 3480938
Conc: 1.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

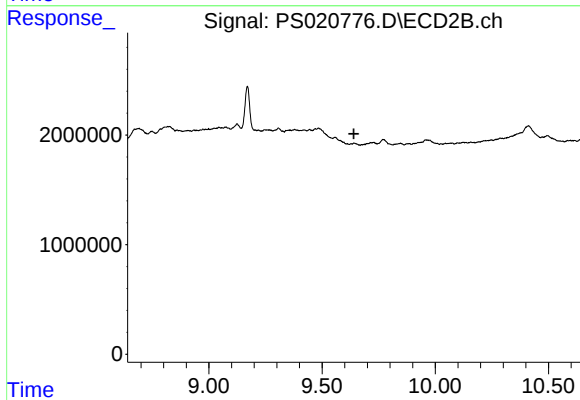


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.641 min
Response: 0
Conc: N.D.

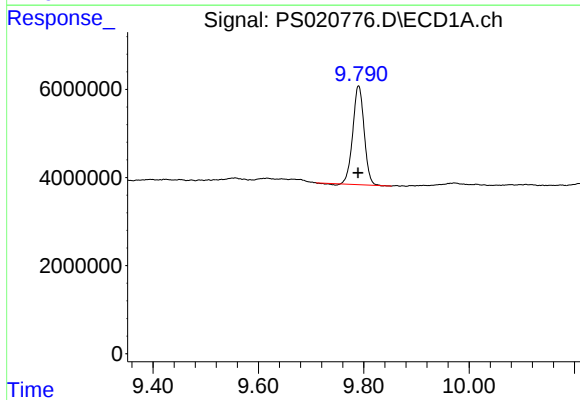


#15 Picloram

R.T.: 9.790 min
Delta R.T.: 0.001 min
Response: 33350524
Conc: 2.00 ng/ml

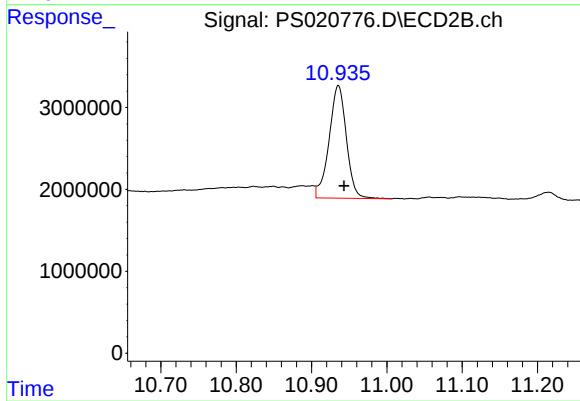

#15 Picloram


R.T.: 10.936 min
Delta R.T.: -0.008 min
Response: 21925492
Conc: 1.86 ng/ml

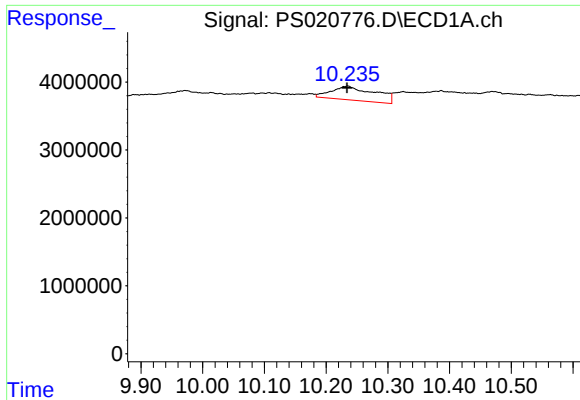

#16 DCPA

R.T.: 10.234 min
Delta R.T.: 0.000 min
Response: 10045458
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

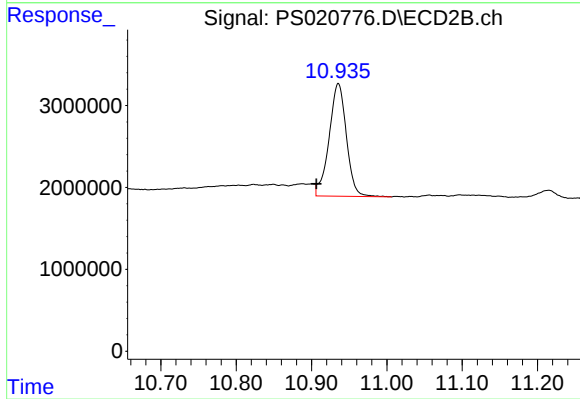

#16 DCPA

R.T.: 10.936 min
Delta R.T.: 0.029 min
Response: 21925492
Conc: 2.13 ng/ml