

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101222\
 Data File : PS020777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 09:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 00:33:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.419	6.863	920.6E6	652.2E6	487.986	487.113
Target Compounds							
1) T	Dalapon	2.502	0.000	382844	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.745f	0.000	2511653	0	<MDL	N.D. #
5) T	DICAMBA	6.562	0.000	575799	0	<MDL	N.D. #
6) T	MCP	6.715	0.000	584292	0	<MDL	N.D. #
7) T	MCPA	6.789f	0.000	3965133	0	<MDL	N.D. #
8) T	DICHLORPROP	7.216f	0.000	625434	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.127	0.000	660081	0	<MDL	N.D. #
12) T	2,4,5-T	8.386	9.170	793658	4462746	<MDL	<MDL #
13) T	2,4-DB	8.876	0.000	897410	0	<MDL	N.D. #
14) T	DINOSEB	9.966	0.000	315371	0	<MDL	N.D. #
15) T	Picloram	9.785	10.935	30201413	20335021	1.813	1.725
16) T	DCPA	10.229	10.935	349682	20335021	<MDL	1.979 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101222\
Data File : PS020777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 09:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 00:33:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

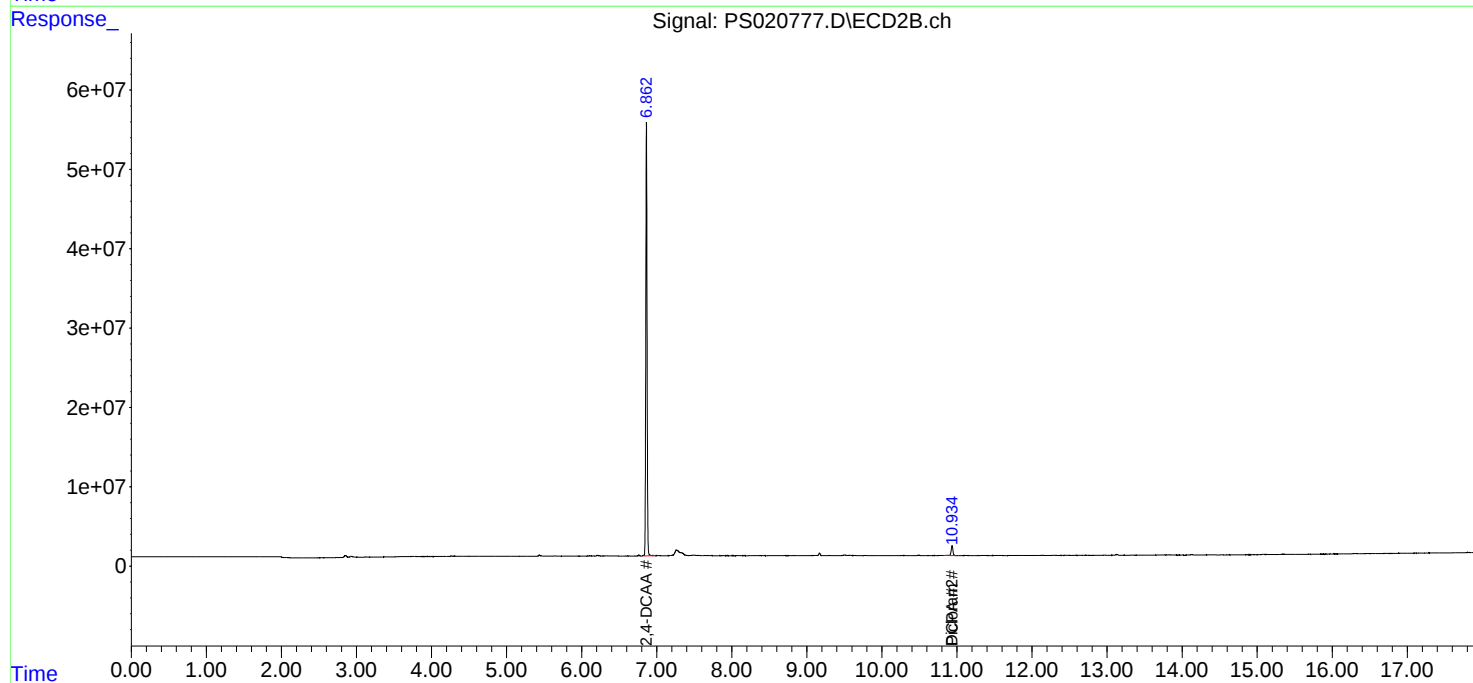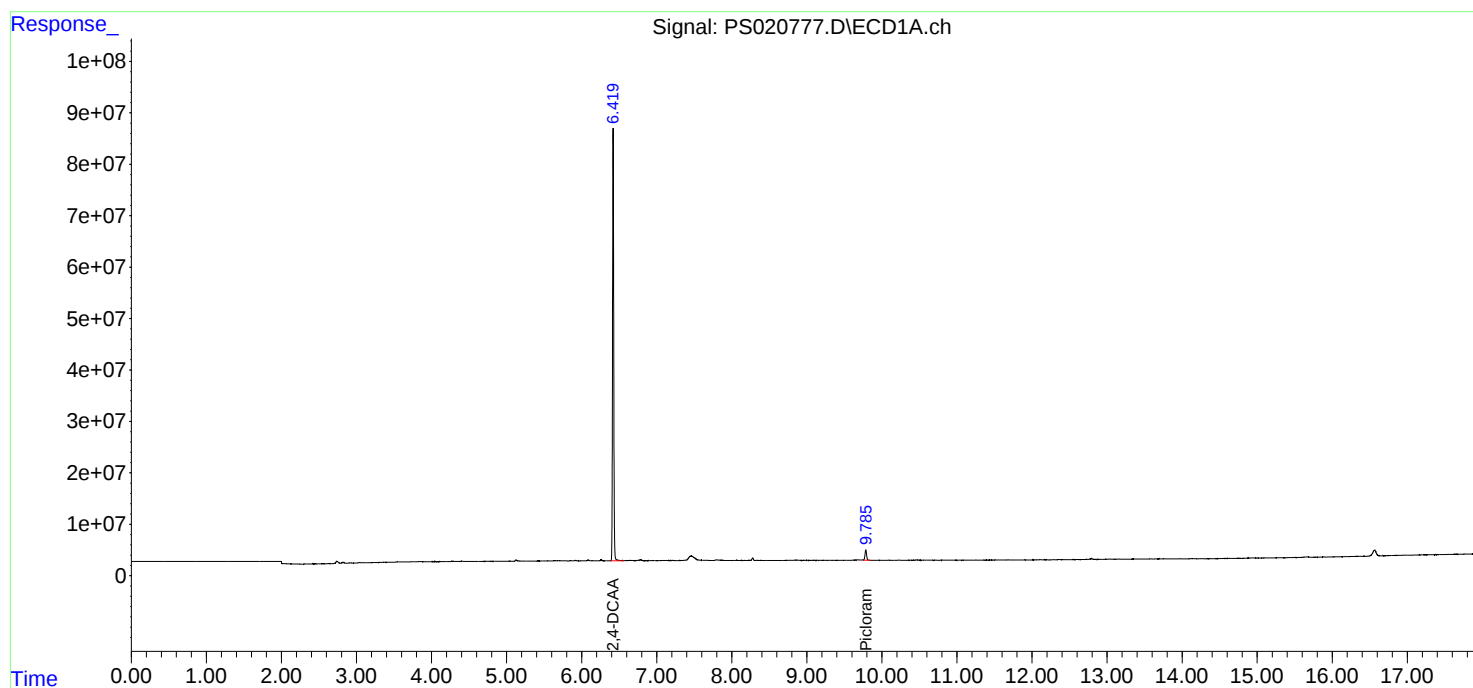


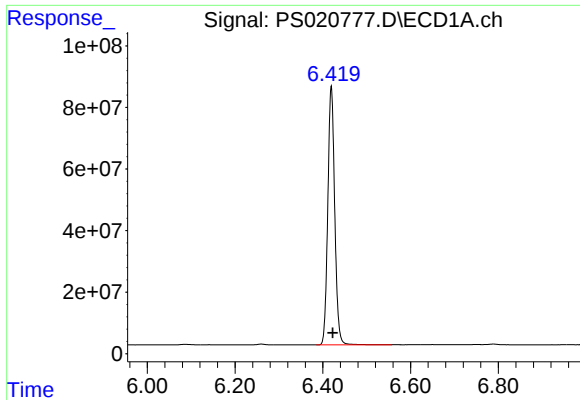

#4 2,4-DCAA


R.T.: 6.419 min
Delta R.T.: -0.003 min
Response: 920560548
Conc: 487.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

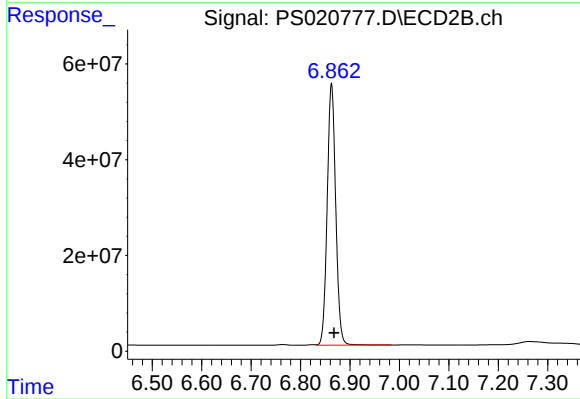


#4 2,4-DCAA

R.T.: 6.863 min
Delta R.T.: -0.005 min
Response: 652235190
Conc: 487.11 ng/ml

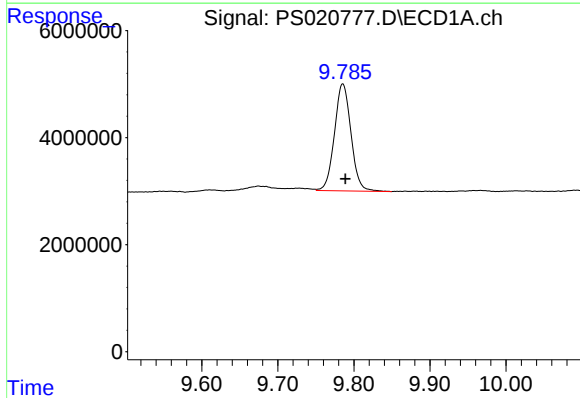


#15 Picloram

R.T.: 9.785 min
Delta R.T.: -0.004 min
Response: 30201413
Conc: 1.81 ng/ml

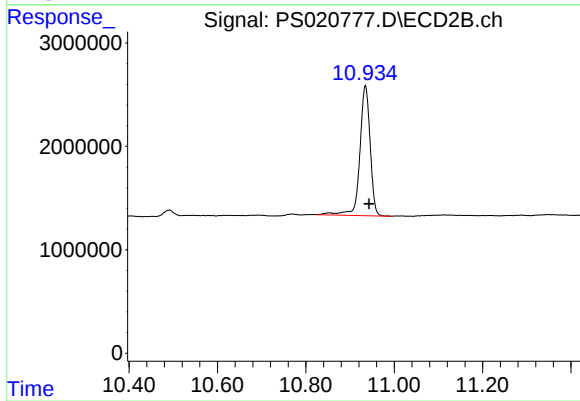

#15 Picloram


R.T.: 10.935 min
Delta R.T.: -0.009 min
Response: 20335021
Conc: 1.73 ng/ml

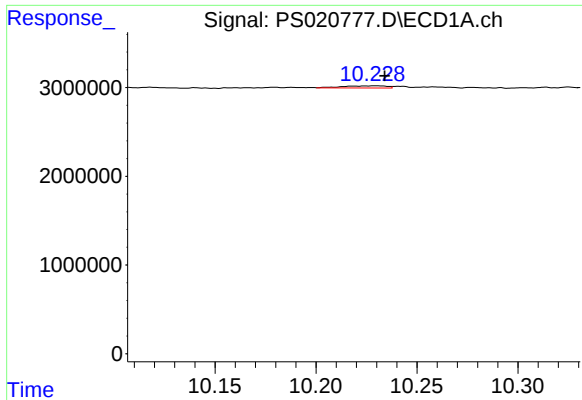

#16 DCPA

R.T.: 10.229 min
Delta R.T.: -0.005 min
Response: 349682
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

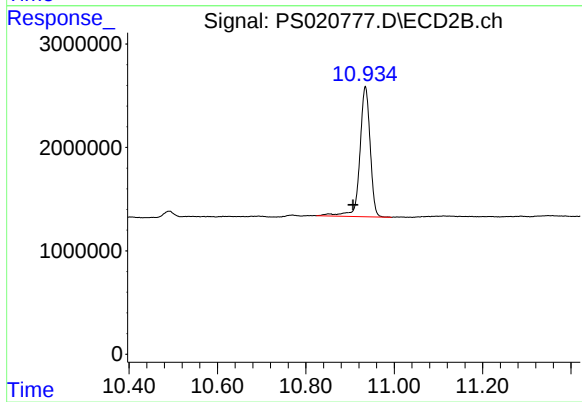

#16 DCPA

R.T.: 10.935 min
Delta R.T.: 0.028 min
Response: 20335021
Conc: 1.98 ng/ml