

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101222\
 Data File : PS020785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 18:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 00:37:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.423	6.862	940.5E6	661.5E6	498.551	494.012
Target Compounds							
1) T	Dalapon	2.512	0.000	1331682	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.807	6.016	1183897	1554980	<MDL	<MDL #
3) T	4-Nitroph...	6.260	6.509	5223732	3704654	N.D.	4.493
5) T	DICAMBA	6.620f	0.000	61660452	0	7.756	N.D. #
6) T	MCPD	6.750	0.000	26672209	0	4.539	N.D. #
7) T	MCPA	6.866	0.000	6803097	0	<MDL	N.D. #
8) T	DICHLORPROP	7.190	7.676	1091592	1253738	<MDL	<MDL #
9) T	2,4-D	7.366	8.000f	1268890	201524	<MDL	<MDL #
10) T	Pentachlo...	7.654f	8.380	14132	3382708	<MDL	<MDL #
11) T	2,4,5-TP ...	8.137	0.000	2786692	0	<MDL	N.D. #
12) T	2,4,5-T	8.409	0.000	5974371	0	<MDL	N.D. #
13) T	2,4-DB	8.911	0.000	586965	0	<MDL	N.D. #
14) T	DINOSEB	9.972	0.000	603114	0	<MDL	N.D. #
15) T	Picloram	9.791	10.930	993010	3238587	<MDL	<MDL #
16) T	DCPA	10.240	10.895	14052456	8488245	1.010	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101222\
Data File : PS020785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 18:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 00:37:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

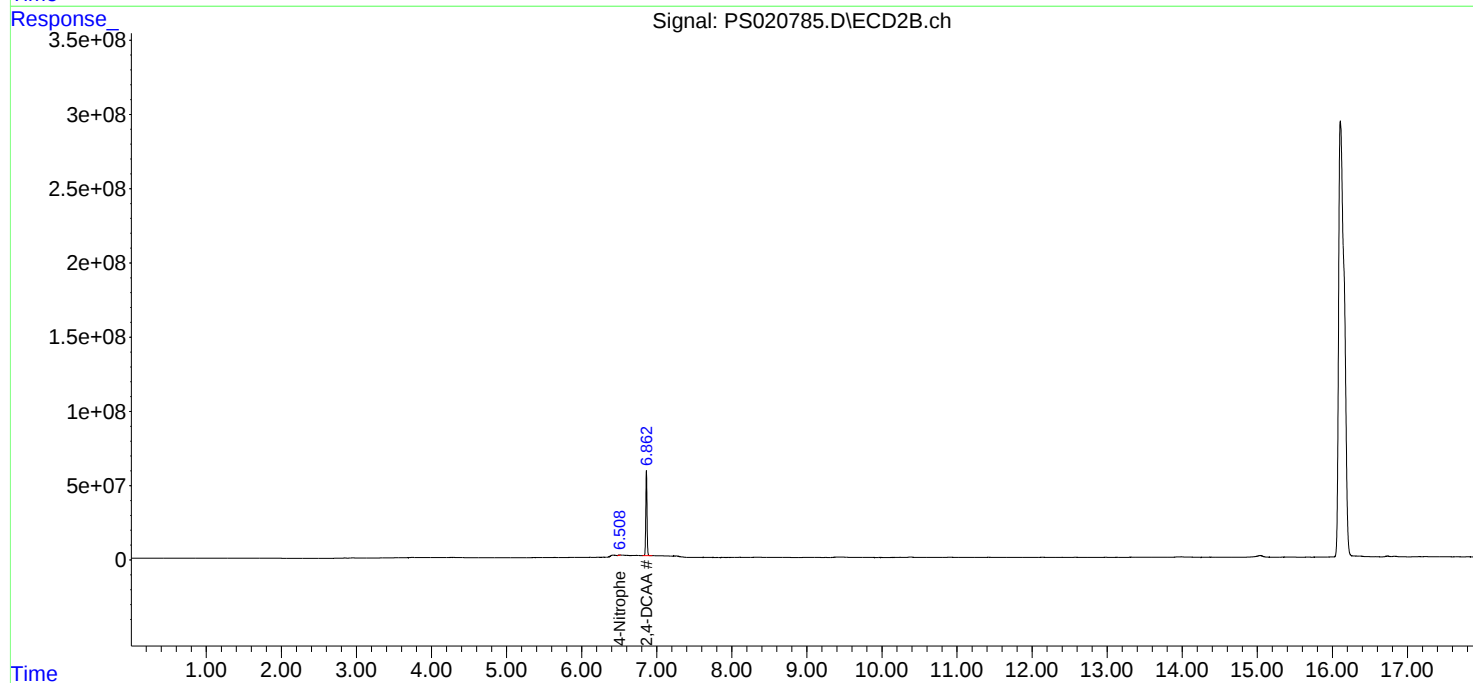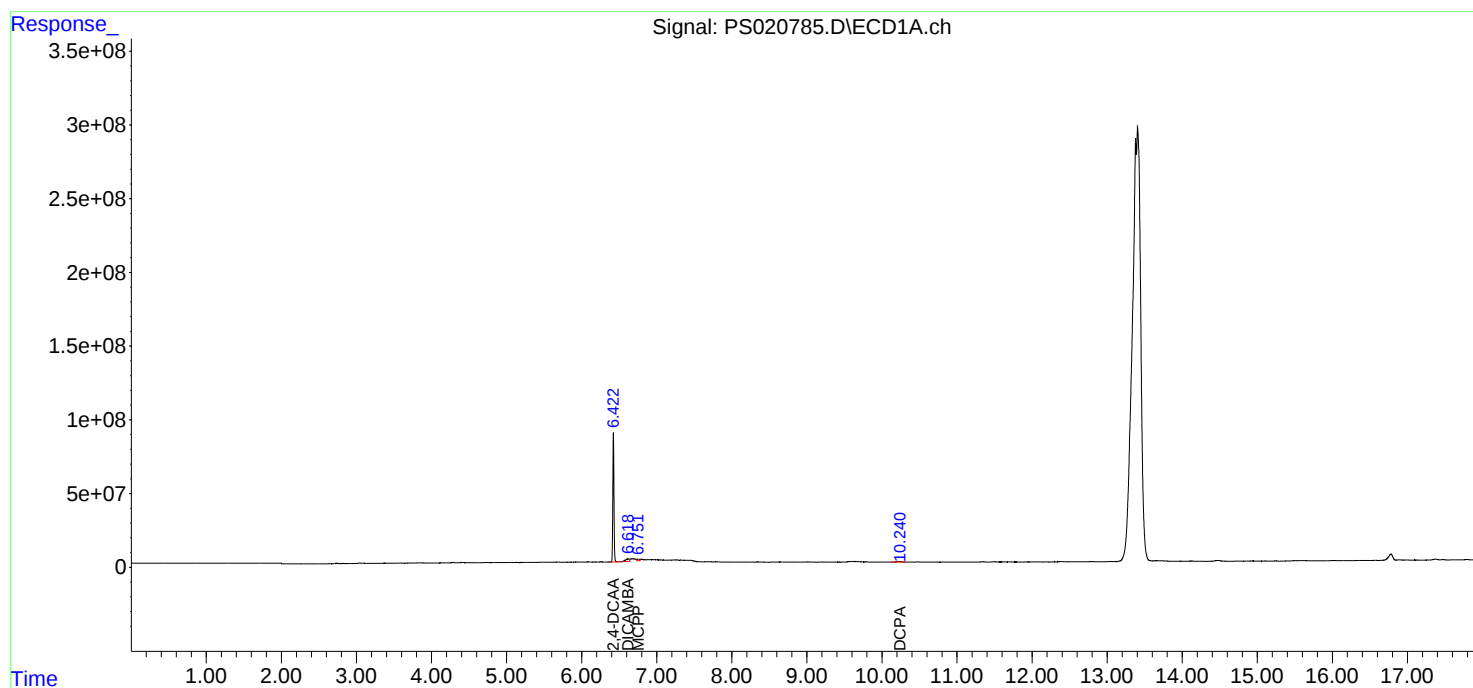


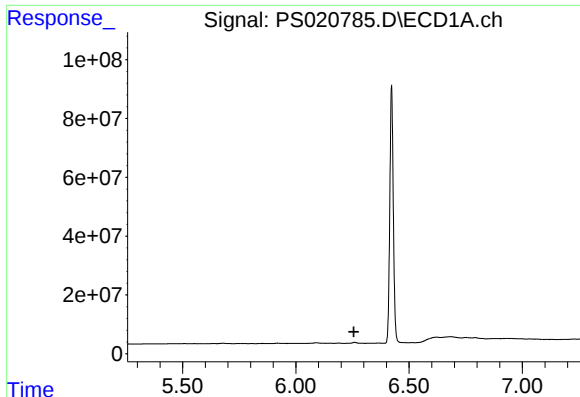

#3 4-Nitrophenol


R.T.: 6.260 min
Delta R.T.: 0.004 min
Response: 5223732
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

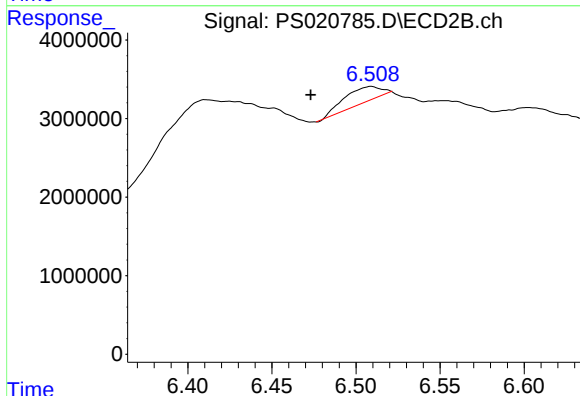


#3 4-Nitrophenol

R.T.: 6.509 min
Delta R.T.: 0.036 min
Response: 3704654
Conc: 4.49 ng/ml

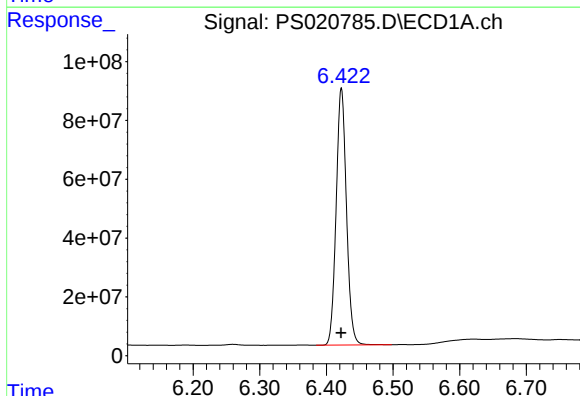


#4 2,4-DCAA

R.T.: 6.423 min
Delta R.T.: 0.000 min
Response: 940491403
Conc: 498.55 ng/ml

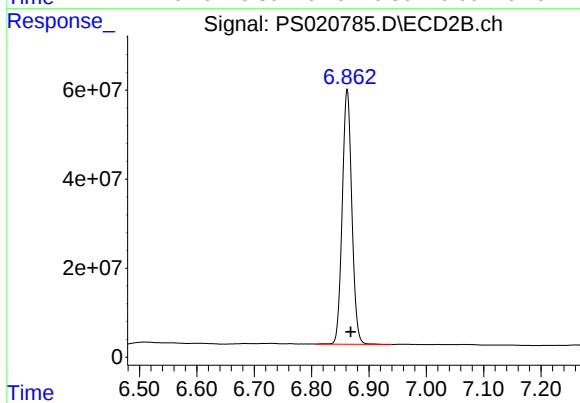

#4 2,4-DCAA


R.T.: 6.862 min
Delta R.T.: -0.006 min
Response: 661472912
Conc: 494.01 ng/ml

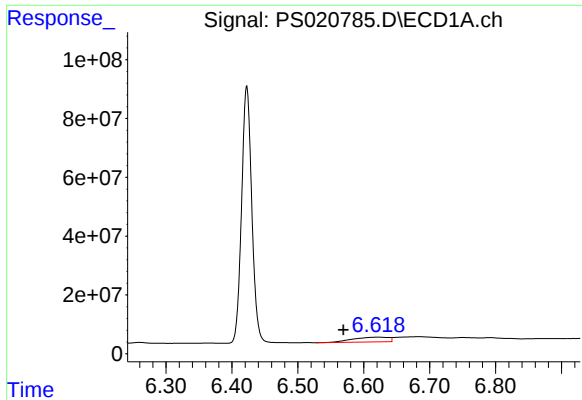

#5 DICAMBA


R.T.: 6.620 min
Delta R.T.: 0.051 min
Response: 61660452
Conc: 7.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

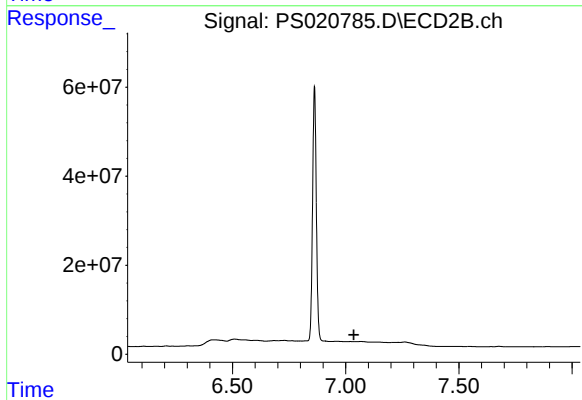


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.037 min
Response: 0
Conc: N.D.

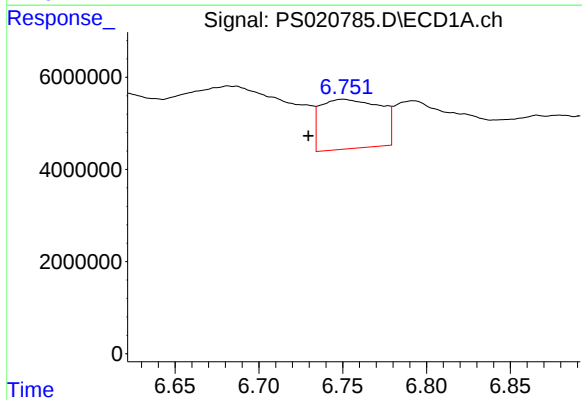


#6 MCP

R.T.: 6.750 min
Delta R.T.: 0.021 min
Response: 26672209
Conc: 4.54 ug/ml

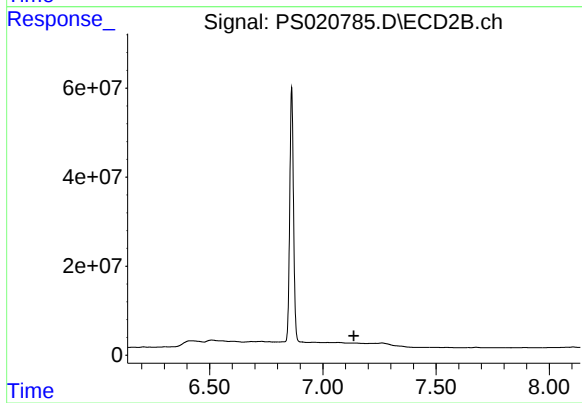

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.137 min
Response: 0
Conc: N.D.

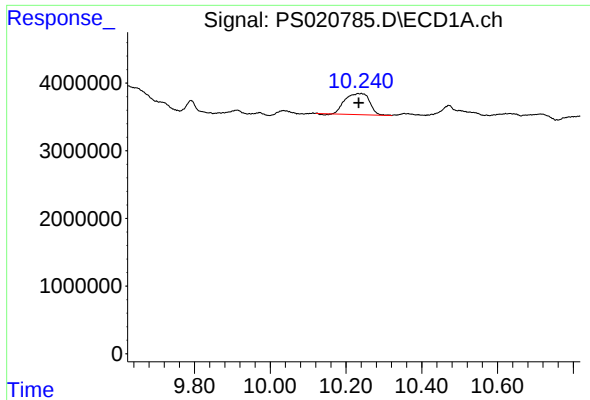

#16 DCPA

R.T.: 10.240 min
Delta R.T.: 0.006 min
Response: 14052456
Conc: 1.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

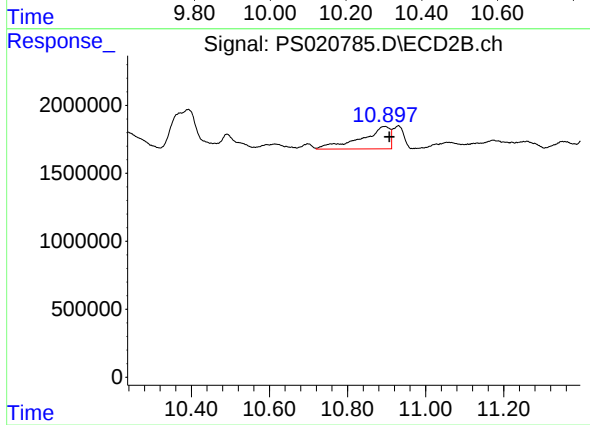

#16 DCPA

R.T.: 10.895 min
Delta R.T.: -0.012 min
Response: 8488245
Conc: N.D.