

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101322\
 Data File : PS020788.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2022 09:20
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 23:17:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.395	0.000	147488	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.546	0.000	837743	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.797	0.000	2506907	0	<MDL	N.D. #
3) T	4-Nitroph...	6.254	6.450	4453514	1092923	N.D.	1.326
5) T	DICAMBA	6.562	7.032	914721	509944	<MDL	<MDL #
6) T	MCPD	6.747	7.184f	3915492	1671874	<MDL	<MDL #
7) T	MCPA	6.880	0.000	1474005	0	<MDL	N.D. #
8) T	DICHLORPROP	7.187	7.674	1378309	1364092	<MDL	<MDL #
9) T	2,4-D	7.334	7.999f	835537	944812	<MDL	<MDL #
10) T	Pentachlo...	7.606	8.385	825629	999904	<MDL	<MDL #
11) T	2,4,5-TP ...	8.133	8.748	3398710	7541638	<MDL	<MDL #
12) T	2,4,5-T	8.395	9.126	2196368	1160904	<MDL	<MDL #
13) T	2,4-DB	8.926	0.000	4100365	0	1.795	N.D. #
14) T	DINOSEB	9.974	0.000	1066048	0	<MDL	N.D. #
15) T	Picloram	9.789	10.935	61808859	28894014	3.711	2.451 #
16) T	DCPA	10.233	10.897	1100650	3102649	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101322\
Data File : PS020788.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2022 09:20
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 23:17:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

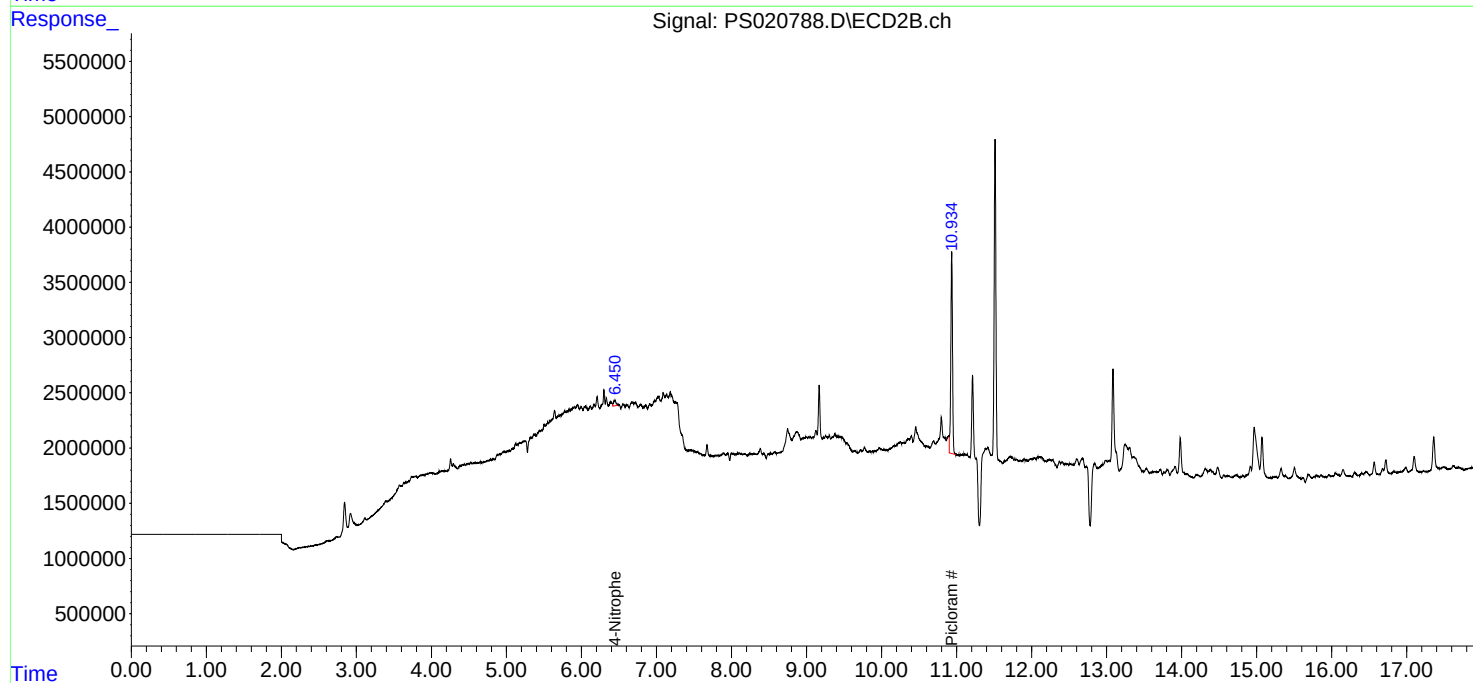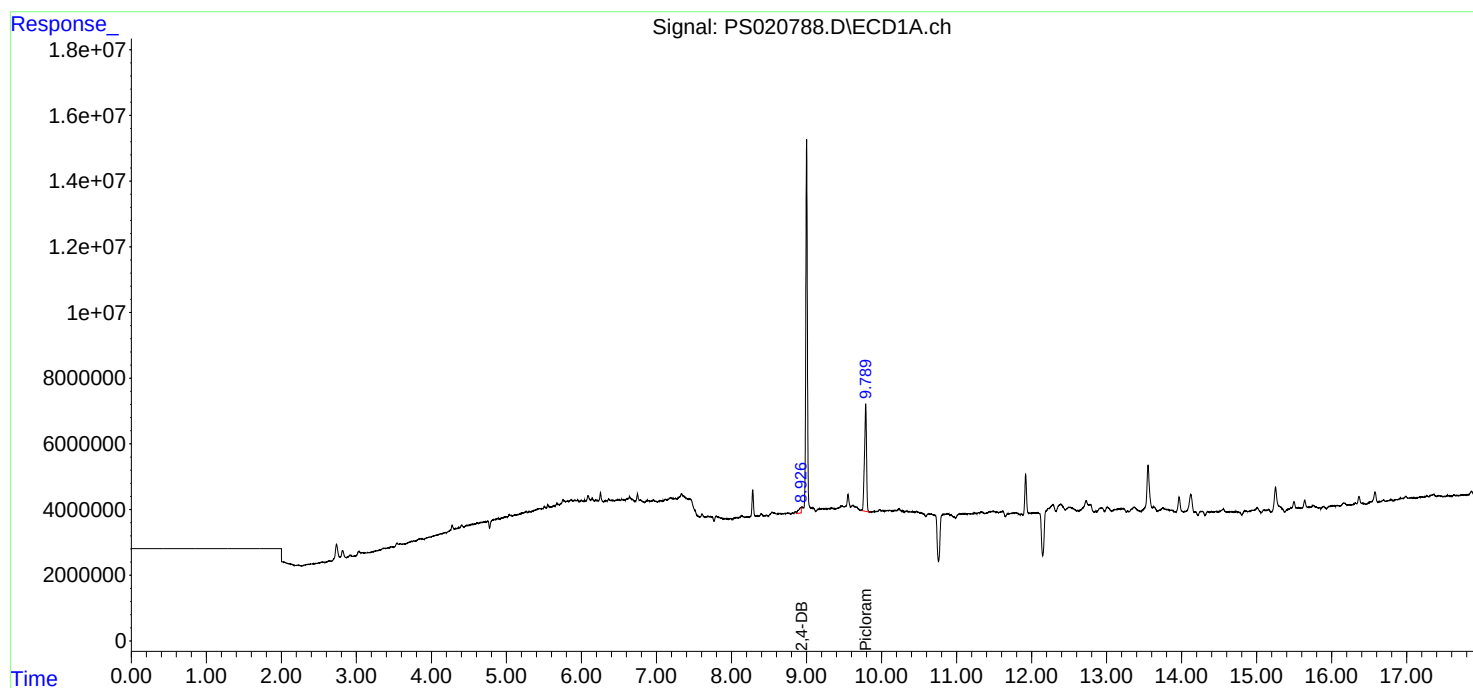


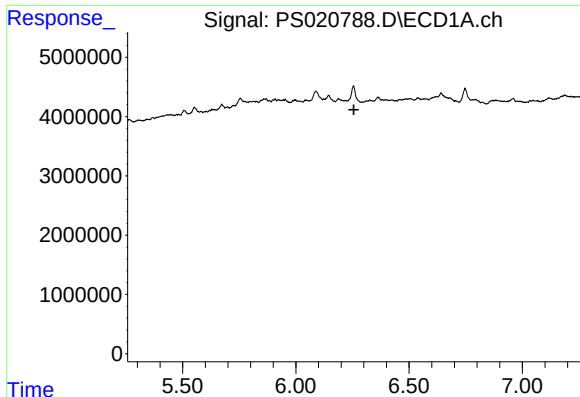

#3 4-Nitrophenol


R.T.: 6.254 min
Delta R.T.: -0.001 min
Response: 4453514
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

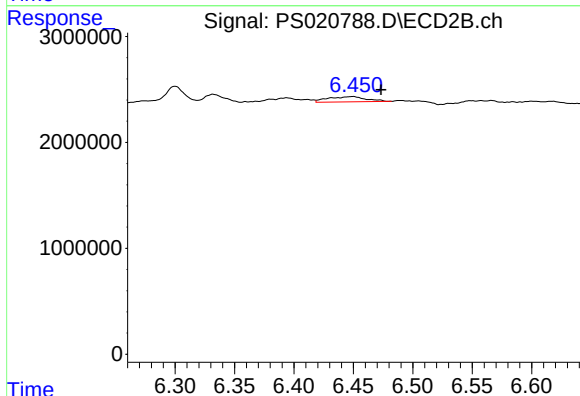


#3 4-Nitrophenol

R.T.: 6.450 min
Delta R.T.: -0.024 min
Response: 1092923
Conc: 1.33 ng/ml

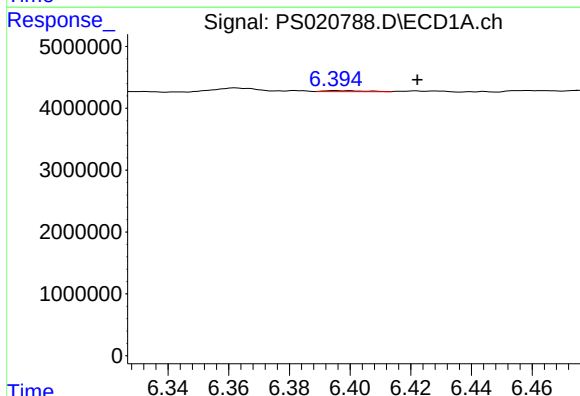


#4 2,4-DCAA

R.T.: 6.395 min
Delta R.T.: -0.027 min
Response: 147488
Conc: N.D.

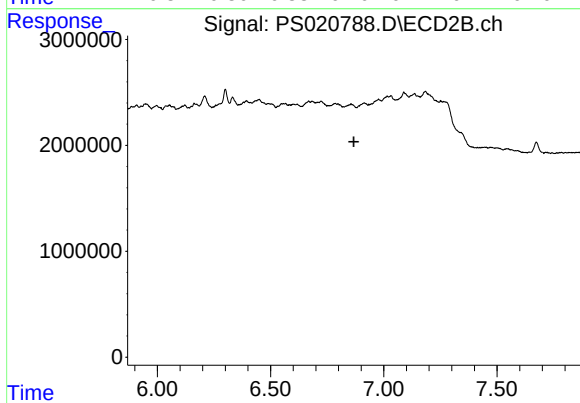

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.868 min
Response: 0
Conc: N.D.

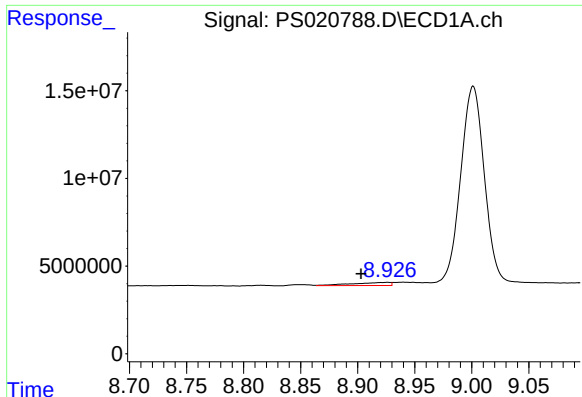

#13 2,4-DB


R.T.: 8.926 min
Delta R.T.: 0.023 min
Response: 4100365
Conc: 1.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

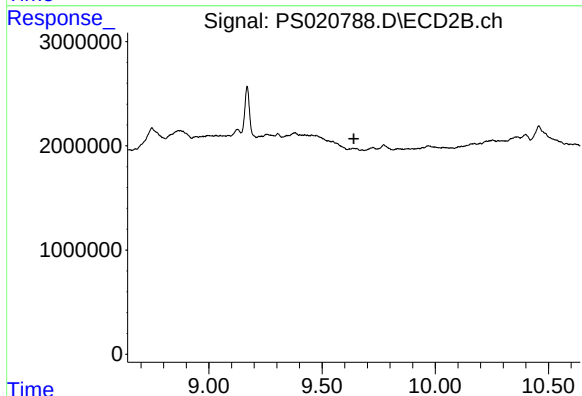


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.641 min
Response: 0
Conc: N.D.

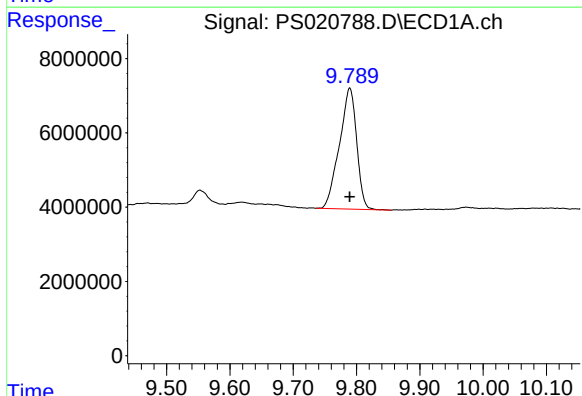

#15 Picloram

R.T.: 9.789 min
Delta R.T.: 0.000 min
Response: 61808859
Conc: 3.71 ng/ml

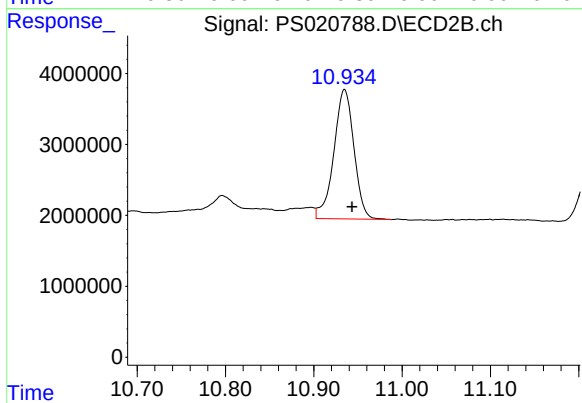

#15 Picloram

R.T.: 10.935 min
Delta R.T.: -0.008 min
Response: 28894014
Conc: 2.45 ng/ml