

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101322\
 Data File : PS020789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2022 09:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 23:17:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.419	6.862	954.9E6	681.1E6	506.203	508.698
Target Compounds							
1) T	Dalapon	2.550	0.000	845007	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.802	6.020	1102750	1534831	<MDL	<MDL #
3) T	4-Nitroph...	6.257	0.000	6061018	0	<MDL	N.D. #
5) T	DICAMBA	6.616f	7.016	2290732	1669447	<MDL	<MDL #
6) T	MCPD	6.749	0.000	4327257	0	<MDL	N.D. #
7) T	MCPA	6.787f	0.000	5779040	0	<MDL	N.D. #
8) T	DICHLORPROP	7.183	7.677	-66139	1072754	N.D.	<MDL
9) T	2,4-D	0.000	7.894f	0	2053397	N.D.	1.158
10) T	Pentachlo...	7.650f	0.000	1122153	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.112	0.000	1822762	0	<MDL	N.D. #
12) T	2,4,5-T	8.399	9.168	2690548	4927080	<MDL	<MDL #
13) T	2,4-DB	8.873	0.000	1028825	0	<MDL	N.D. #
14) T	DINOSEB	9.965	0.000	732685	0	<MDL	N.D. #
15) T	Picloram	9.785	10.933	36559302	24560349	2.195	2.084
16) T	DCPA	10.223	10.933	2697263	24560349	<MDL	2.391 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101322\
Data File : PS020789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2022 09:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 23:17:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

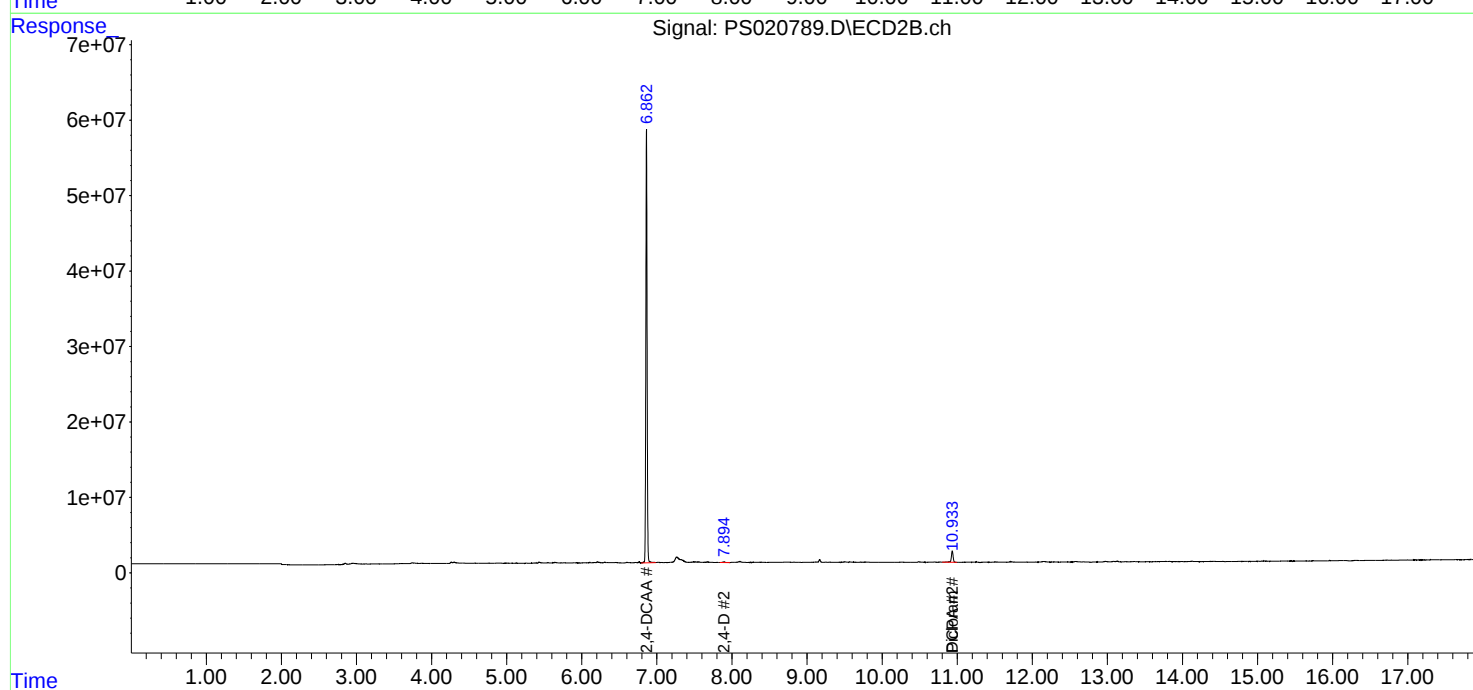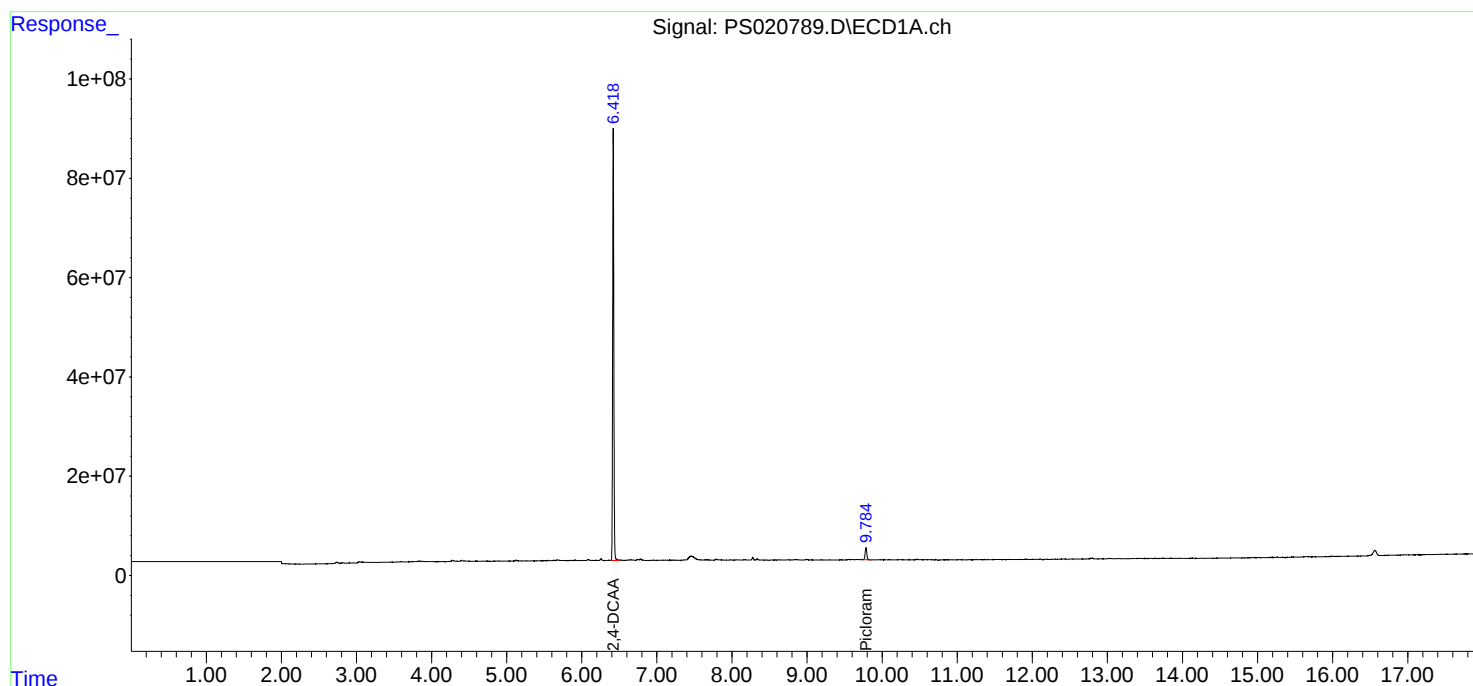


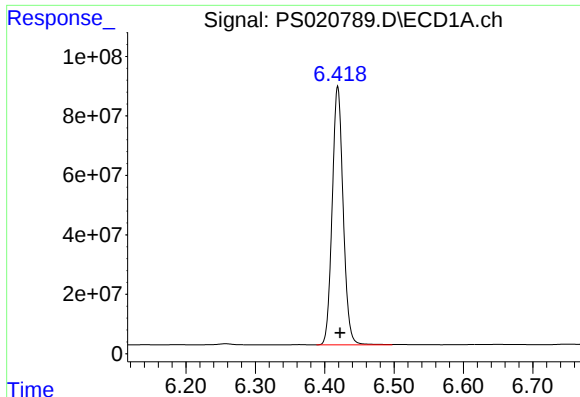

#4 2,4-DCAA


R.T.: 6.419 min
Delta R.T.: -0.003 min
Response: 954926119
Conc: 506.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

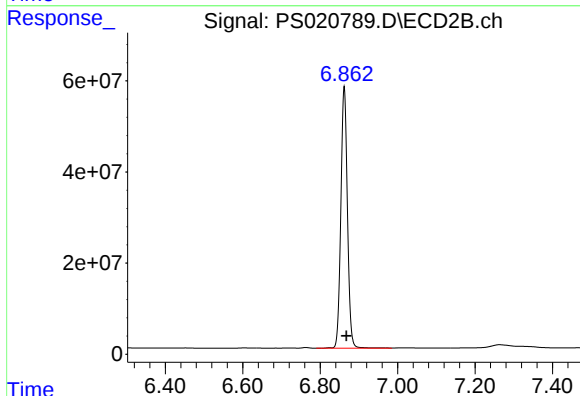


#4 2,4-DCAA

R.T.: 6.862 min
Delta R.T.: -0.006 min
Response: 681136375
Conc: 508.70 ng/ml

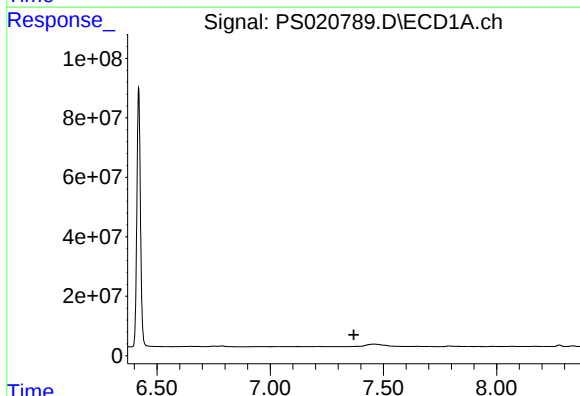


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.370 min
Response: 0
Conc: N.D.

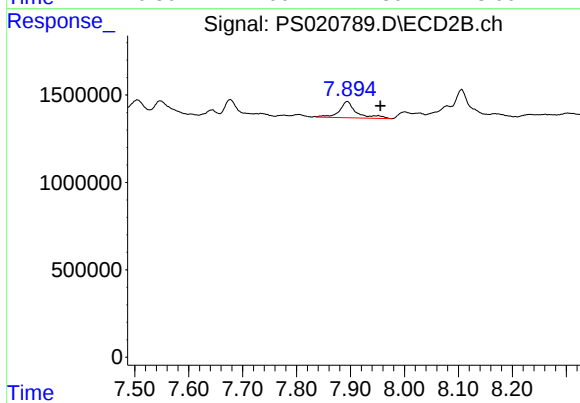

#9 2,4-D


R.T.: 7.894 min
Delta R.T.: -0.062 min
Response: 2053397
Conc: 1.16 ng/ml

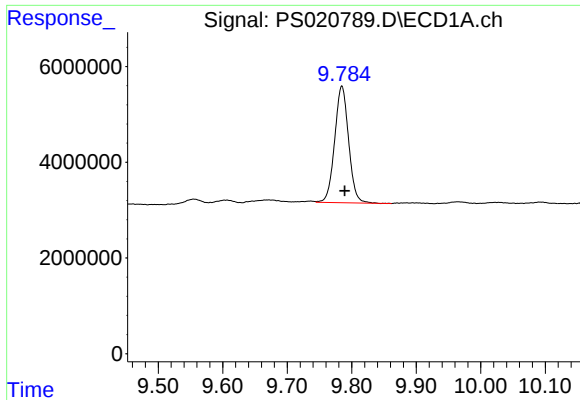

#15 Picloram


R.T.: 9.785 min
Delta R.T.: -0.004 min
Response: 36559302
Conc: 2.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

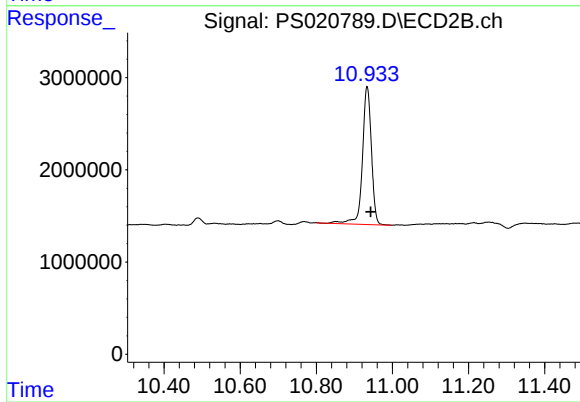


#15 Picloram

R.T.: 10.933 min
Delta R.T.: -0.010 min
Response: 24560349
Conc: 2.08 ng/ml

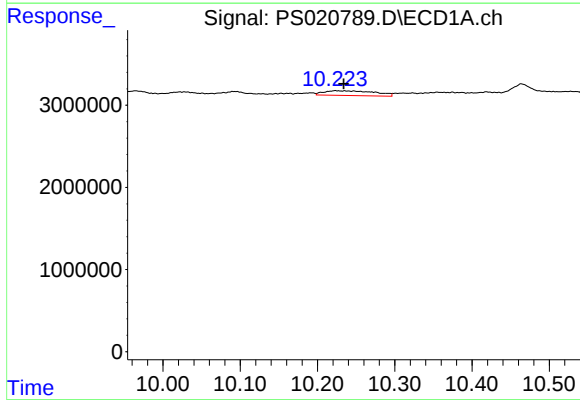

#16 DCPA

R.T.: 10.223 min
Delta R.T.: -0.011 min
Response: 2697263
Conc: N.D.

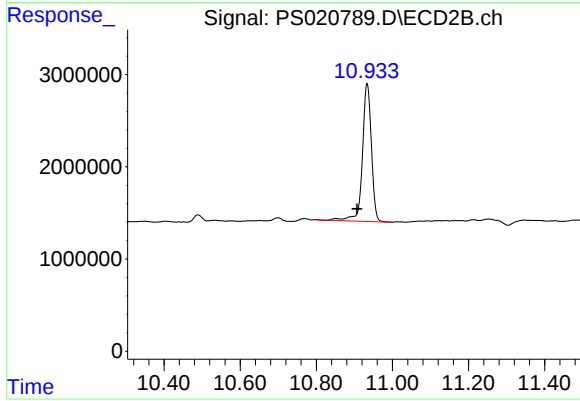

#16 DCPA

R.T.: 10.933 min
Delta R.T.: 0.027 min
Response: 24560349
Conc: 2.39 ng/ml