

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101322\
 Data File : PS020794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2022 12:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 23:20:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.419	6.862	965.5E6	685.1E6	511.798	511.695
Target Compounds							
1) T	Dalapon	2.542	0.000	1204578	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.799	0.000	1018816	0	<MDL	N.D. #
5) T	DICAMBA	6.615f	0.000	1065484	0	<MDL	N.D. #
6) T	MCP	6.747	0.000	3968491	0	<MDL	N.D. #
7) T	MCPA	6.865	0.000	378482	0	<MDL	N.D. #
8) T	DICHLORPROP	7.216f	7.676	832452	1119592	<MDL	<MDL #
10) T	Pentachlo...	7.649f	0.000	1105377	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.129	0.000	1747434	0	<MDL	N.D. #
12) T	2,4,5-T	8.389	9.168	2473126	3500285	<MDL	<MDL #
13) T	2,4-DB	8.876	0.000	997940	0	<MDL	N.D. #
14) T	DINOSEB	9.965	0.000	733949	0	<MDL	N.D. #
15) T	Picloram	9.785	10.933	19628326	14874967	1.179	1.262
16) T	DCPA	10.228	10.933	3320558	14874967	<MDL	1.448 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101322\
Data File : PS020794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2022 12:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 23:20:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

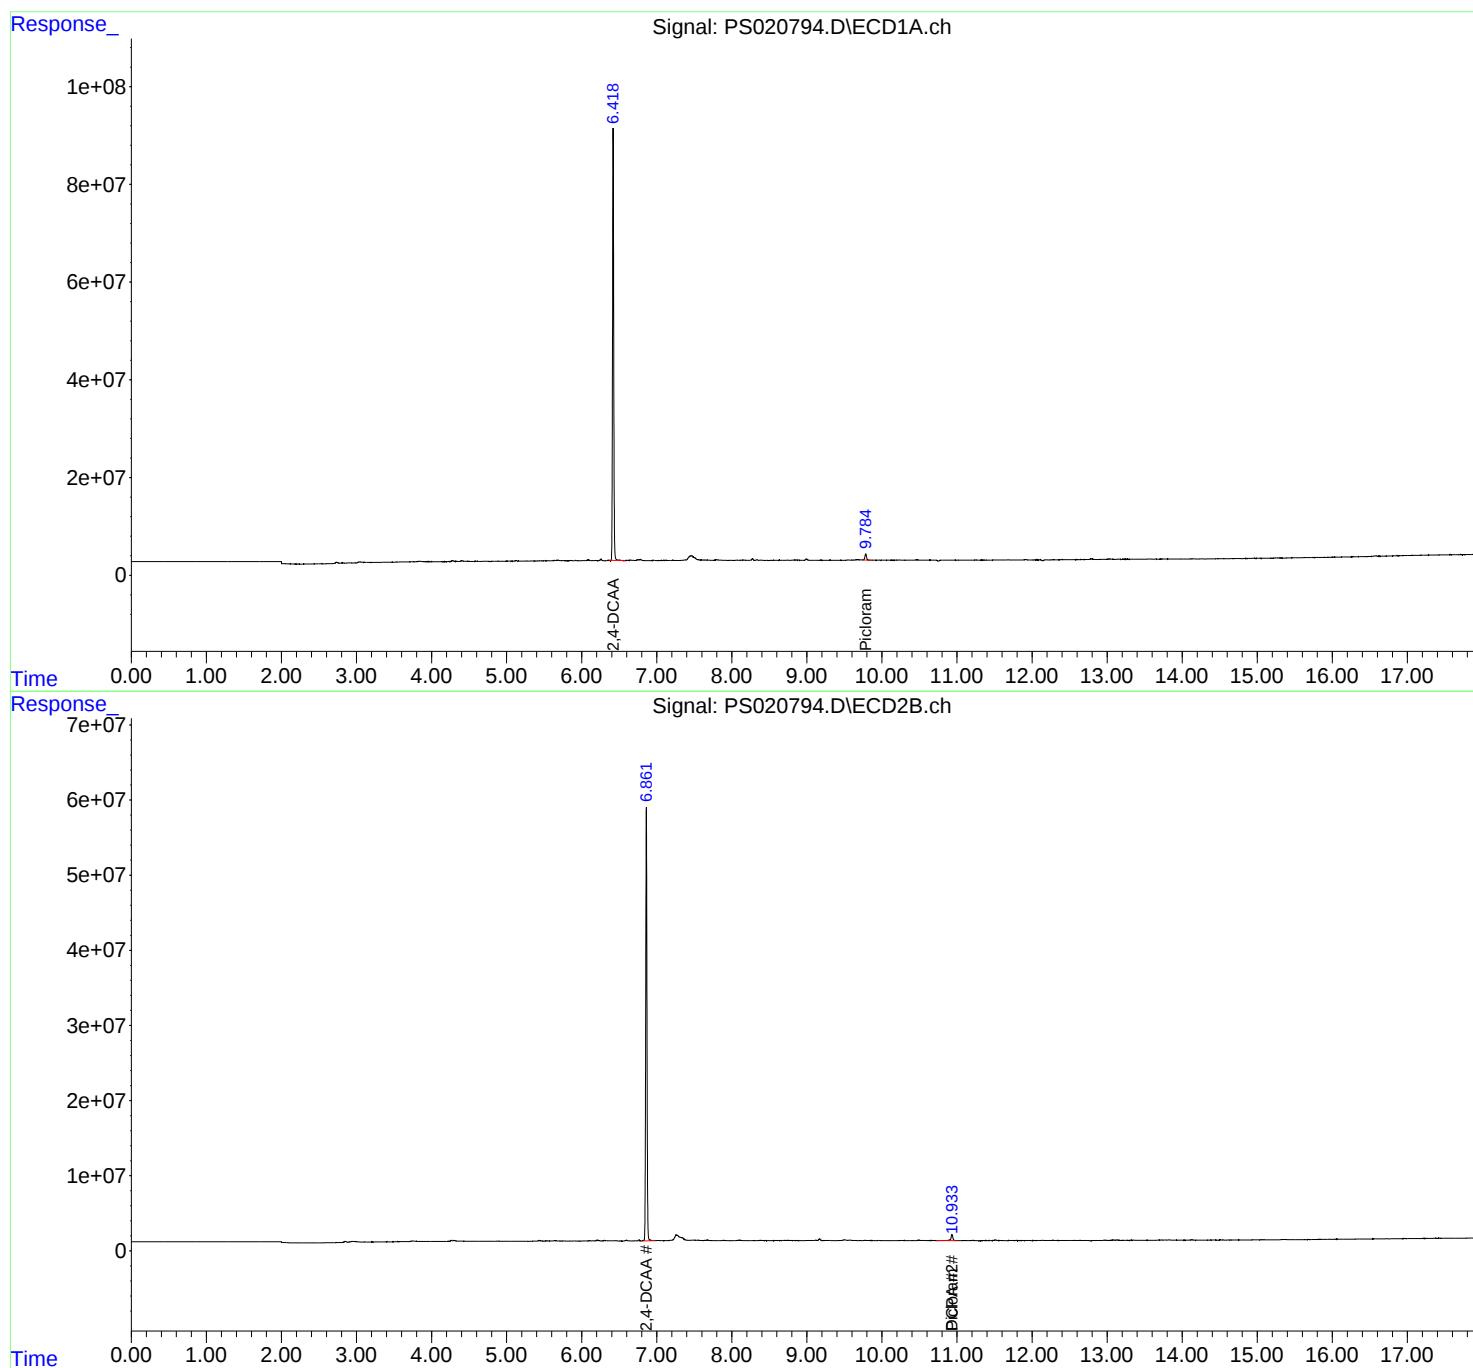


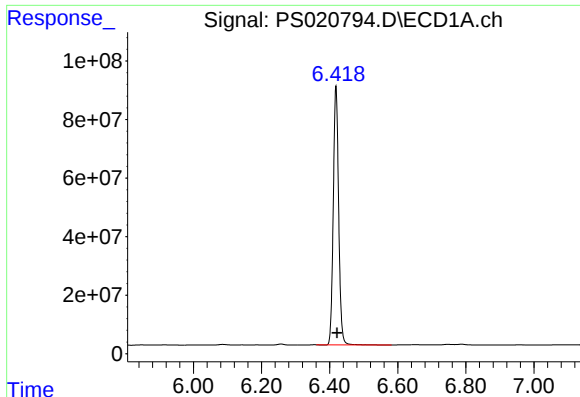

#4 2,4-DCAA


R.T.: 6.419 min
Delta R.T.: -0.004 min
Response: 965481855
Conc: 511.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

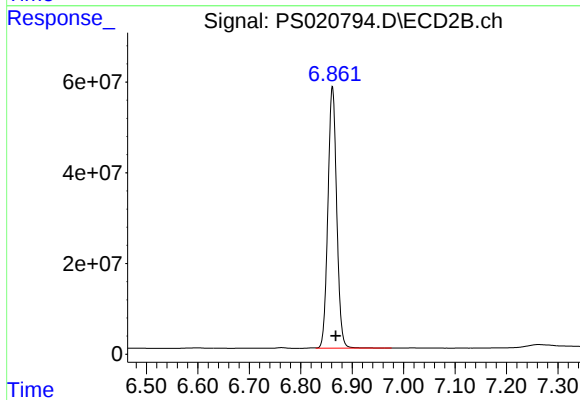


#4 2,4-DCAA

R.T.: 6.862 min
Delta R.T.: -0.006 min
Response: 685149673
Conc: 511.69 ng/ml

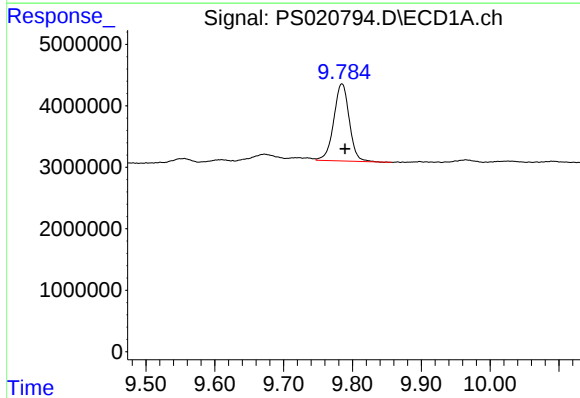


#15 Picloram

R.T.: 9.785 min
Delta R.T.: -0.005 min
Response: 19628326
Conc: 1.18 ng/ml

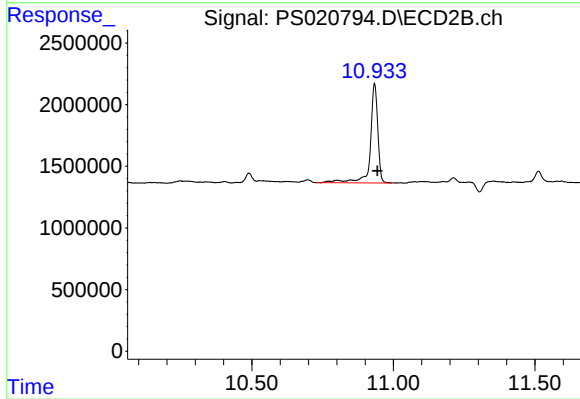

#15 Picloram


R.T.: 10.933 min
Delta R.T.: -0.010 min
Response: 14874967
Conc: 1.26 ng/ml

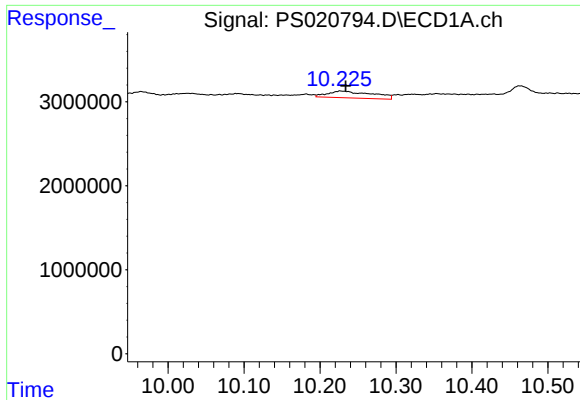

#16 DCPA

R.T.: 10.228 min
Delta R.T.: -0.006 min
Response: 3320558
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

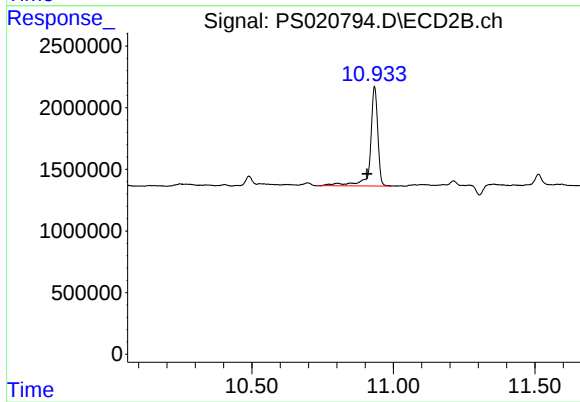

#16 DCPA

R.T.: 10.933 min
Delta R.T.: 0.027 min
Response: 14874967
Conc: 1.45 ng/ml