

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101323\
 Data File : PS024614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2023 15:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 00:22:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	6.781	1002.9E6	329.2E6	487.499	476.150
Target Compounds							
1) T	Dalapon	2.512	2.571	7710183	4014680	3.121	3.587
5) T	DICAMBA	0.000	6.985	0	29590422	N.D.	9.992
6) T	MCP	0.000	6.985f	0	29590422	N.D.	15.016
8) T	DICHLORPROP	0.000	7.571	0	1435923	N.D.	1.909
9) T	2,4-D	7.249	7.787f	329.8E6	692728	119.367	<MDL #
11) T	2,4,5-TP ...	0.000	8.621	0	560556	N.D.	<MDL
12) T	2,4,5-T	0.000	9.037	0	2734477	N.D.	<MDL
13) T	2,4-DB	0.000	9.491	0	896787	N.D.	1.760
15) T	Picloram	9.683	10.780	34179887	18844010	1.960	3.032 #
16) T	DCPA	0.000	10.780	0	18844010	N.D.	3.612



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101323\
Data File : PS024614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2023 15:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 00:22:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

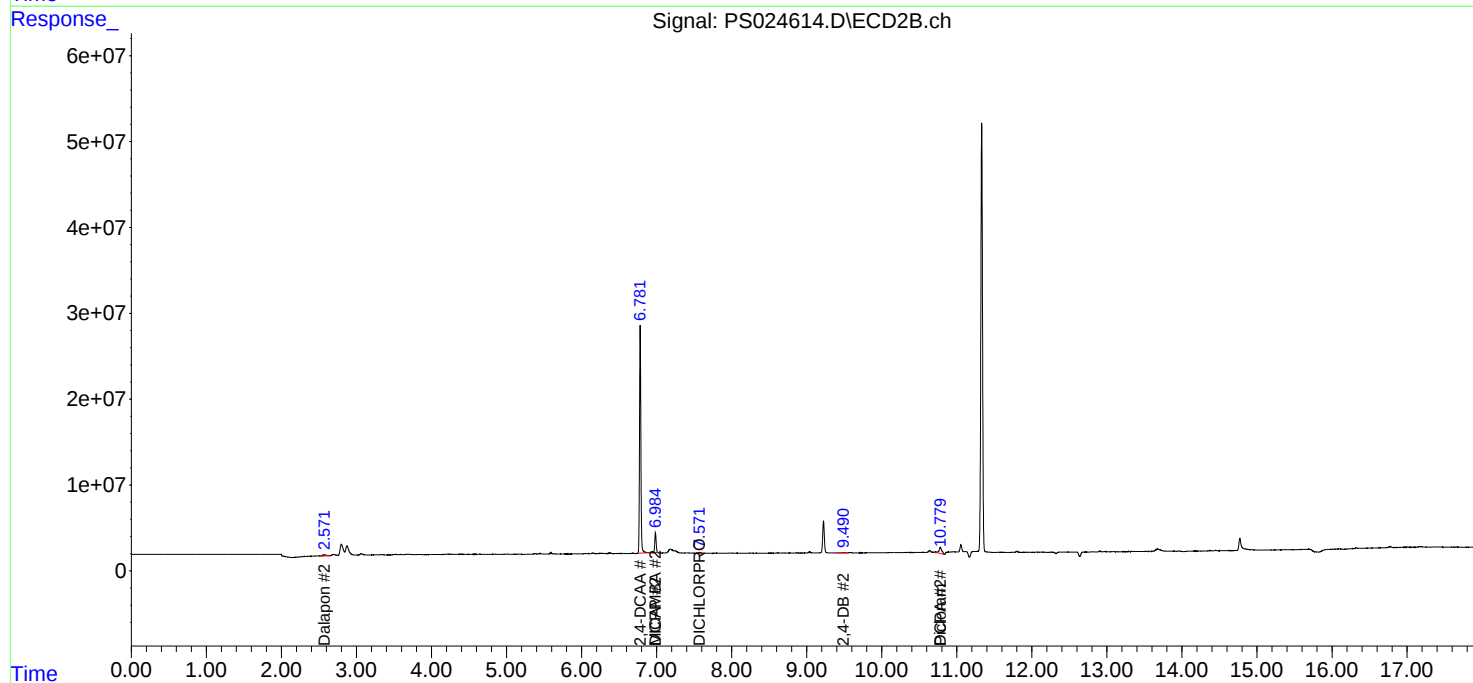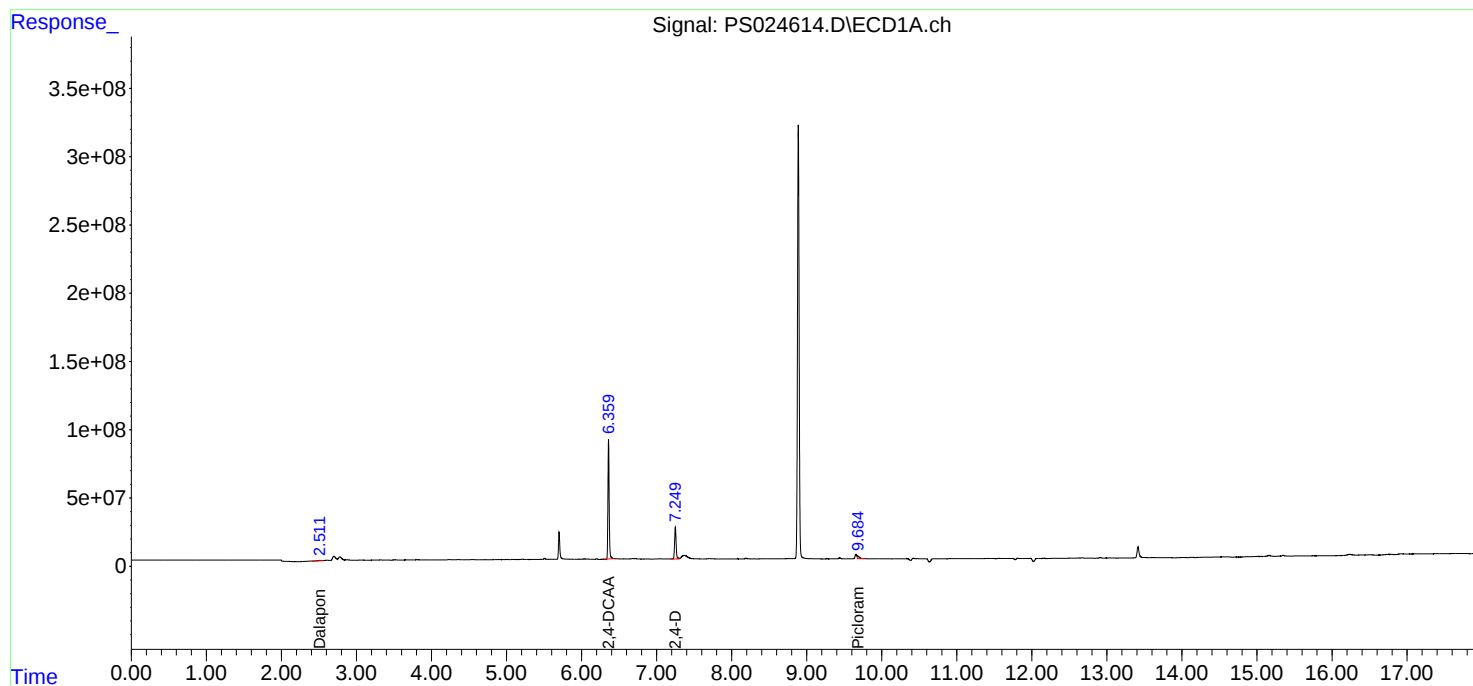


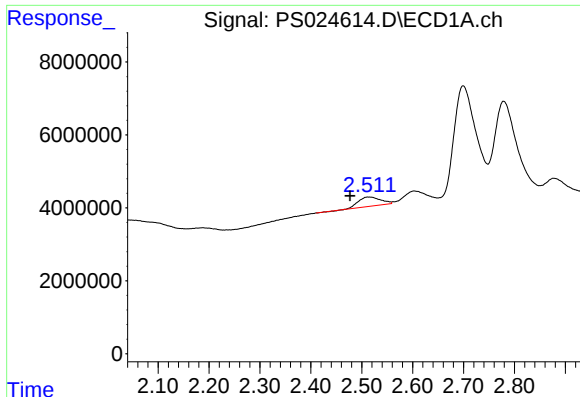

#1 Dalapon


R.T.: 2.512 min
Delta R.T.: 0.035 min
Response: 7710183
Conc: 3.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

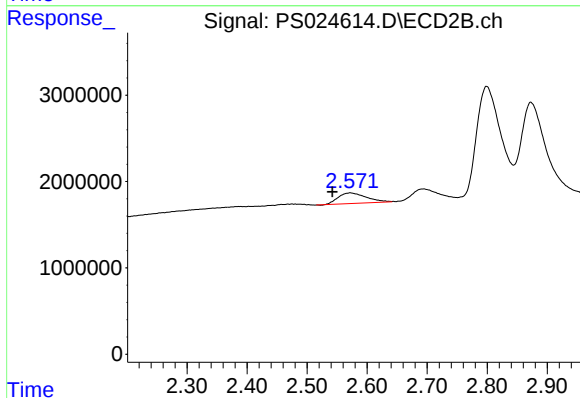


#1 Dalapon

R.T.: 2.571 min
Delta R.T.: 0.029 min
Response: 4014680
Conc: 3.59 ng/ml

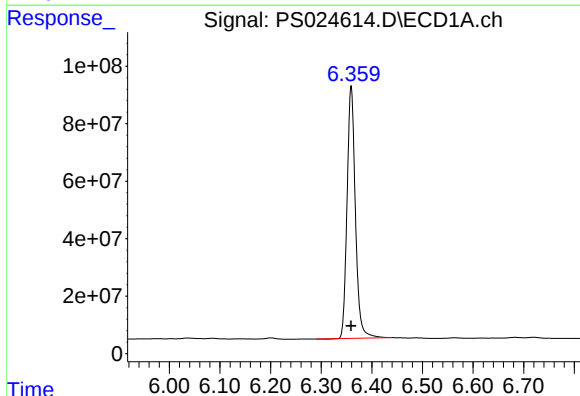


#4 2,4-DCAA

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 1002946227
Conc: 487.50 ng/ml

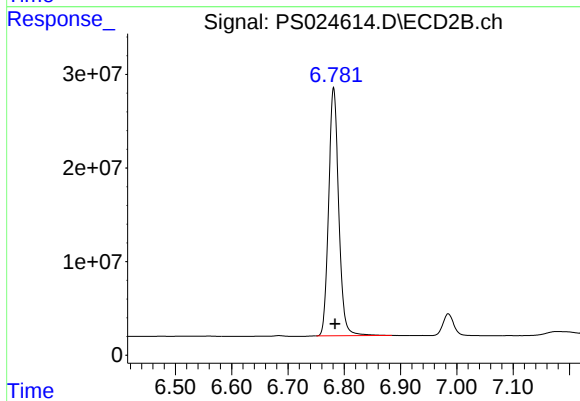

#4 2,4-DCAA


R.T.: 6.781 min
Delta R.T.: -0.002 min
Response: 329158234
Conc: 476.15 ng/ml

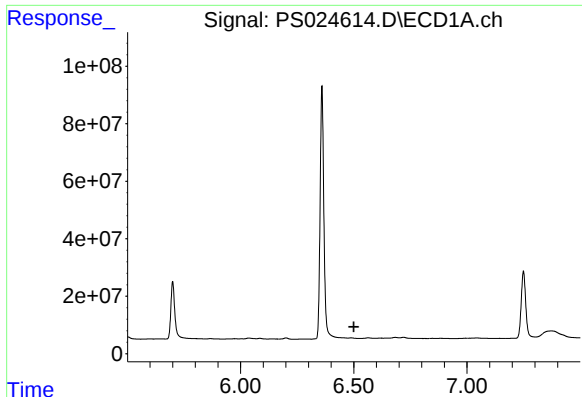

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

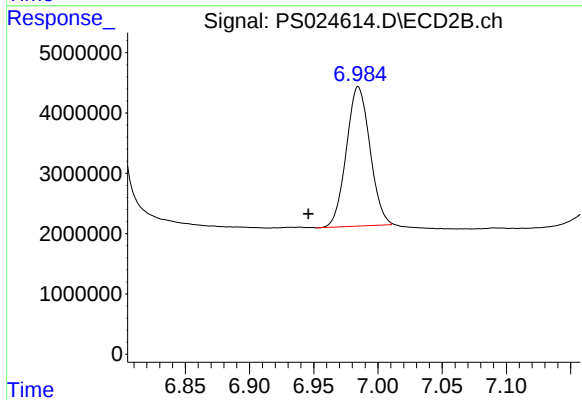


#5 DICAMBA

R.T.: 6.985 min
Delta R.T.: 0.039 min
Response: 29590422
Conc: 9.99 ng/ml

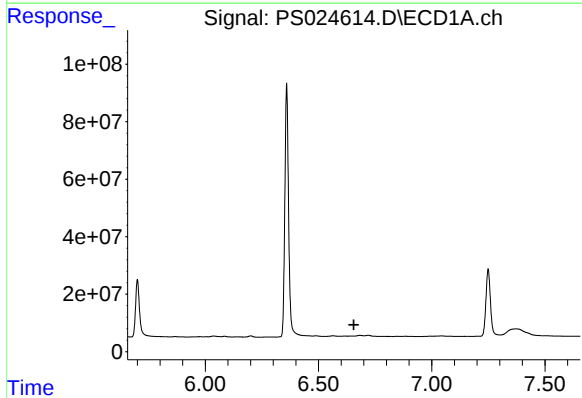


#6 MCP

R.T.: 0.000 min
Exp R.T.: 6.656 min
Response: 0
Conc: N.D.

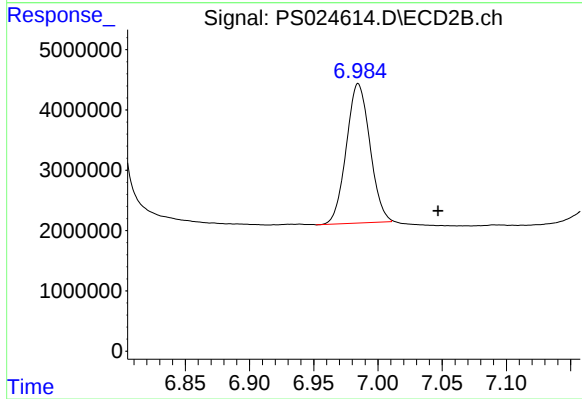

#6 MCP


R.T.: 6.985 min
Delta R.T.: -0.062 min
Response: 29590422
Conc: 15.02 ug/ml

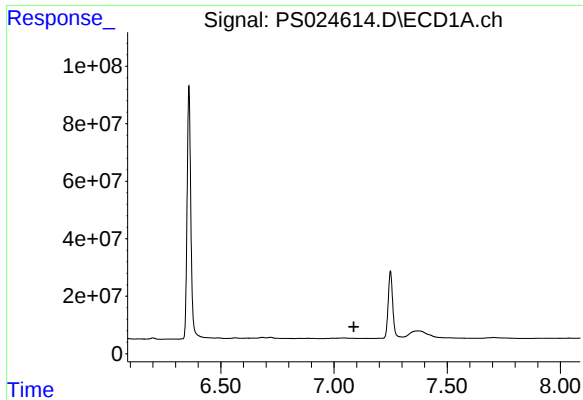

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

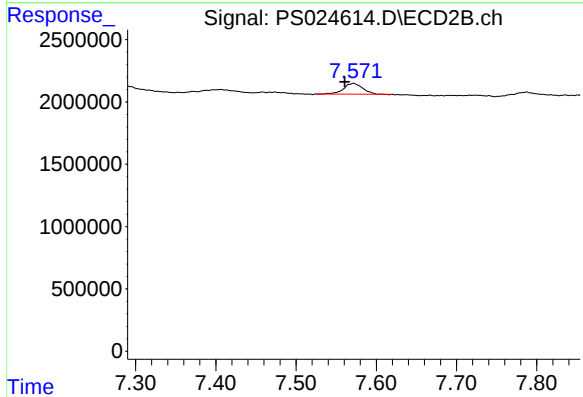


#8 DICHLORPROP

R.T.: 7.571 min
Delta R.T.: 0.010 min
Response: 1435923
Conc: 1.91 ng/ml

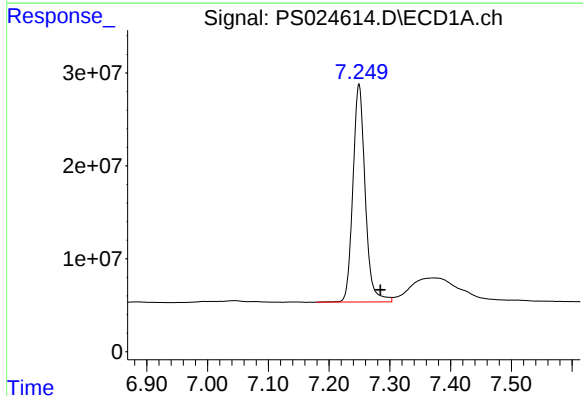


#9 2,4-D

R.T.: 7.249 min
Delta R.T.: -0.035 min
Response: 329811451
Conc: 119.37 ng/ml

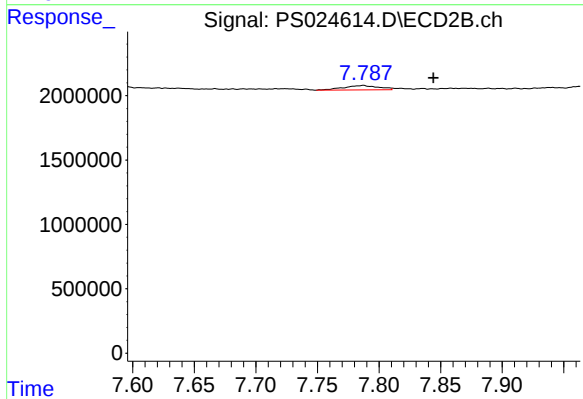

#9 2,4-D


R.T.: 7.787 min
Delta R.T.: -0.058 min
Response: 692728
Conc: N.D.

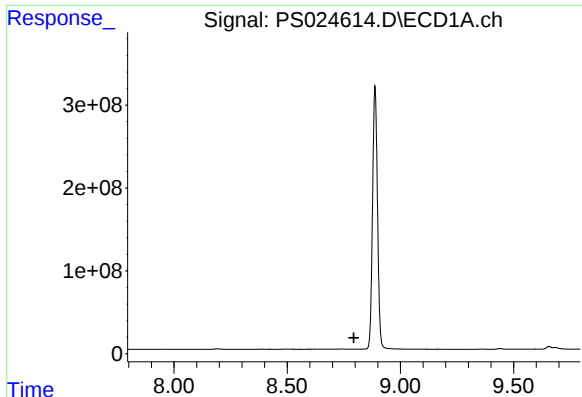

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

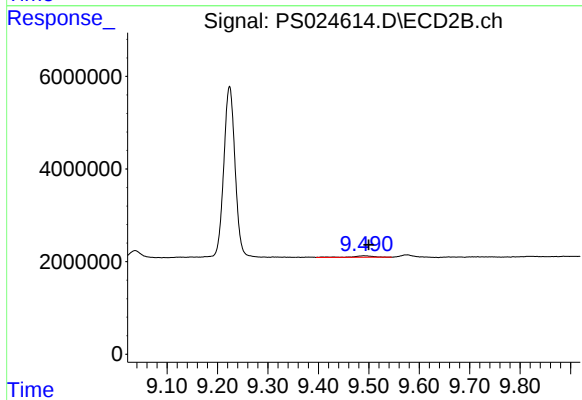


#13 2,4-DB

R.T.: 9.491 min
Delta R.T.: -0.009 min
Response: 896787
Conc: 1.76 ng/ml

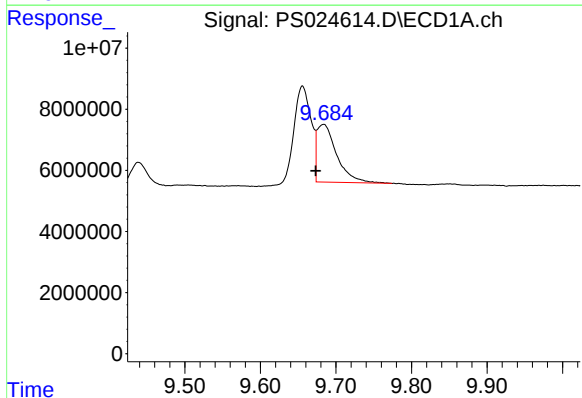


#15 Picloram

R.T.: 9.683 min
Delta R.T.: 0.010 min
Response: 34179887
Conc: 1.96 ng/ml

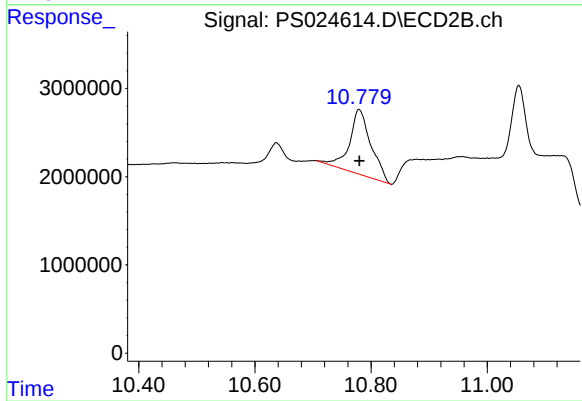

#15 Picloram


R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 18844010
Conc: 3.03 ng/ml

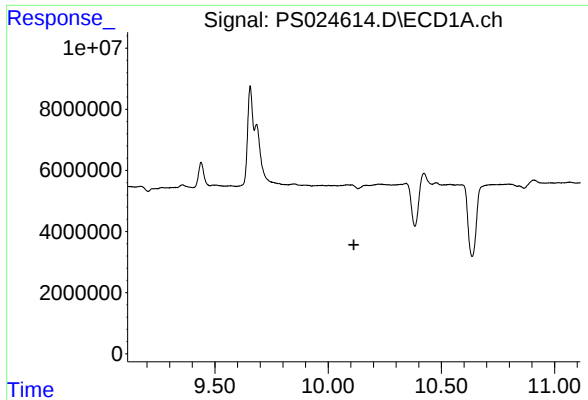

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

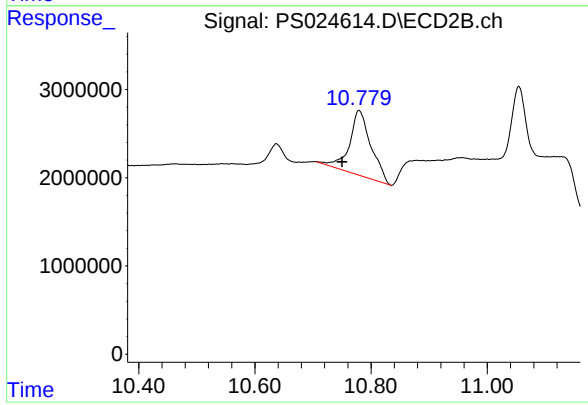

#16 DCPA

R.T.: 10.780 min
Delta R.T.: 0.029 min
Response: 18844010
Conc: 3.61 ng/ml