

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101323\
 Data File : PS024626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2023 20:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 00:31:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	6.780	995.9E6	327.1E6	484.050	473.172
Target Compounds							
1) T	Dalapon	0.000	2.564	0	3345693	N.D.	2.990
5) T	DICAMBA	0.000	6.985	0	31998527	N.D.	10.806
6) T	MCP	6.682	6.985f	3513739	31998527	<MDL	16.238 #
7) T	MCPA	0.000	7.241	0	8471632	N.D.	2.644
8) T	DICHLORPROP	0.000	7.569	0	3175149	N.D.	4.222
9) T	2,4-D	7.248	7.786f	356.3E6	499364	128.958	<MDL #
11) T	2,4,5-TP ...	0.000	8.619	0	543080	N.D.	<MDL
12) T	2,4,5-T	0.000	8.998	0	269491	N.D.	<MDL
13) T	2,4-DB	0.000	9.495	0	1018643	N.D.	1.999
15) T	Picloram	9.655	10.780	61532049	12140608	3.529	1.954 #
16) T	DCPA	0.000	10.780	0	12140608	N.D.	2.327



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101323\
Data File : PS024626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2023 20:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 00:31:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

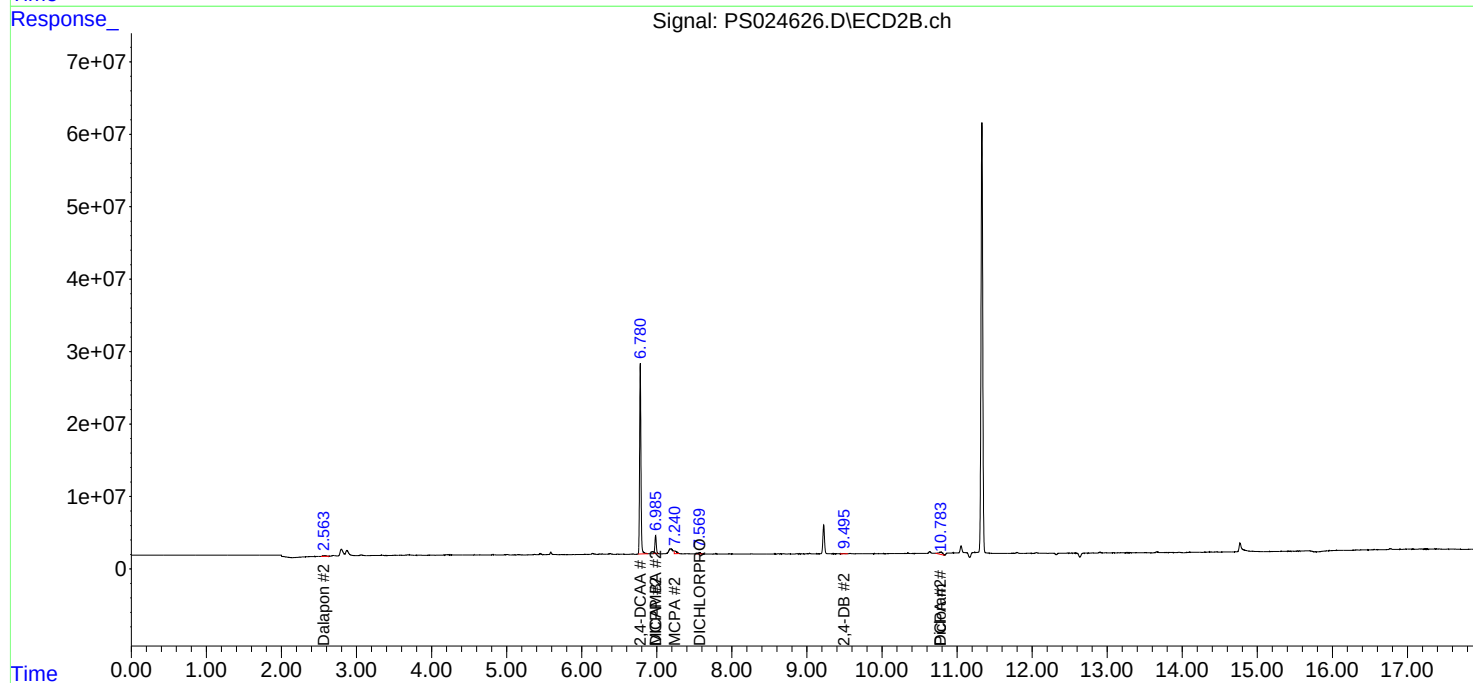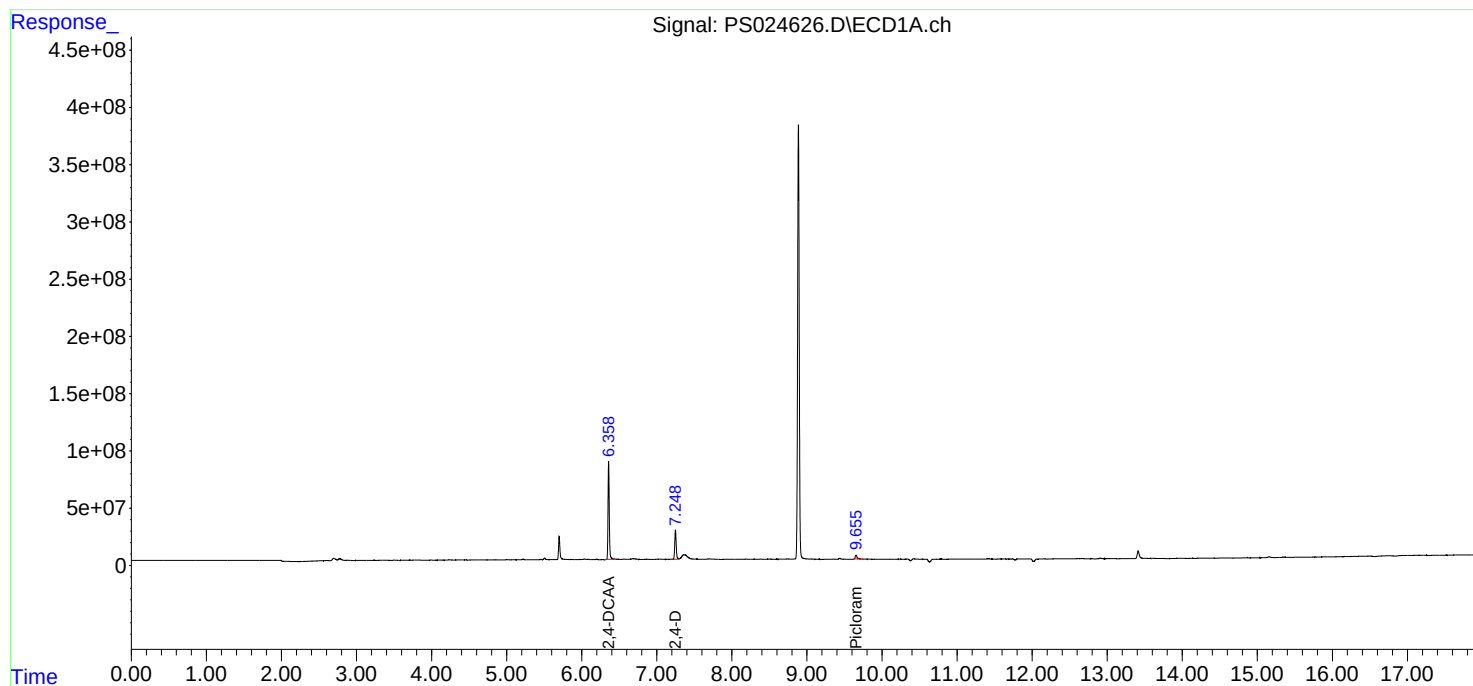


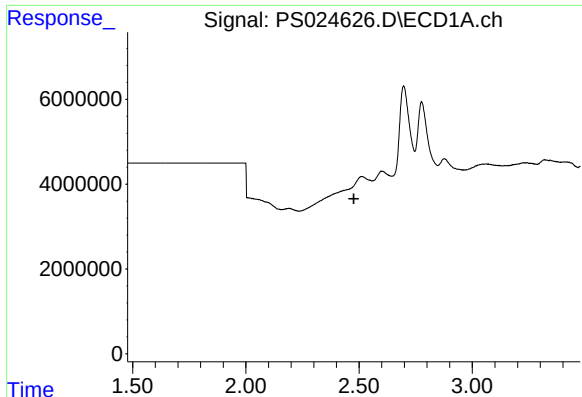

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

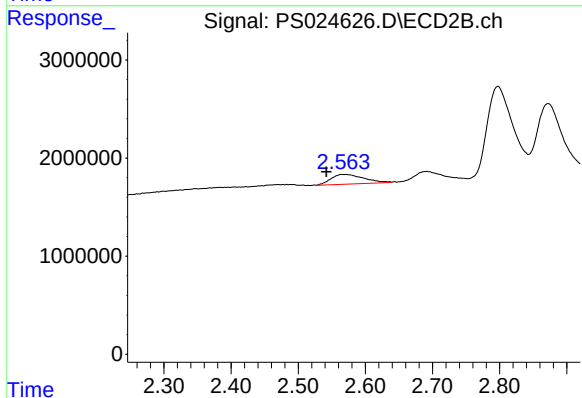


#1 Dalapon

R.T.: 2.564 min
Delta R.T.: 0.022 min
Response: 3345693
Conc: 2.99 ng/ml

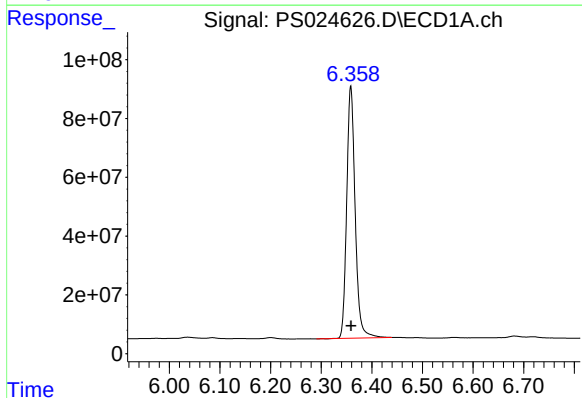


#4 2,4-DCAA

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 995850594
Conc: 484.05 ng/ml

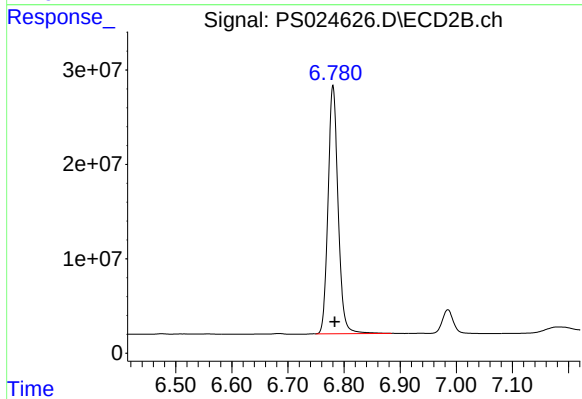

#4 2,4-DCAA


R.T.: 6.780 min
Delta R.T.: -0.003 min
Response: 327099059
Conc: 473.17 ng/ml

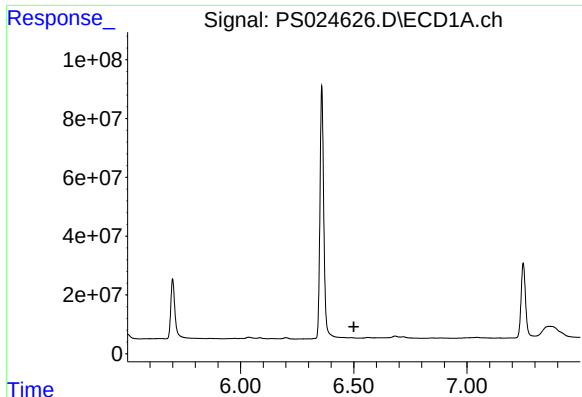

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

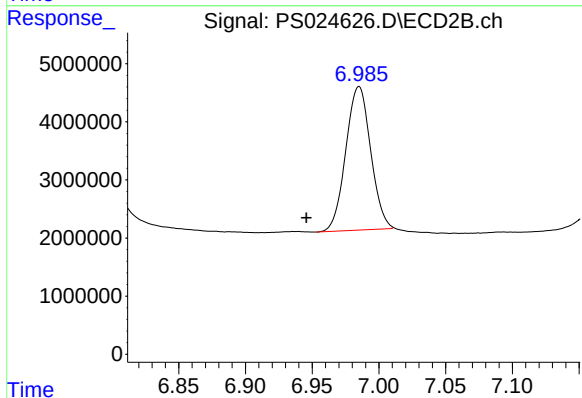


#5 DICAMBA

R.T.: 6.985 min
Delta R.T.: 0.039 min
Response: 31998527
Conc: 10.81 ng/ml

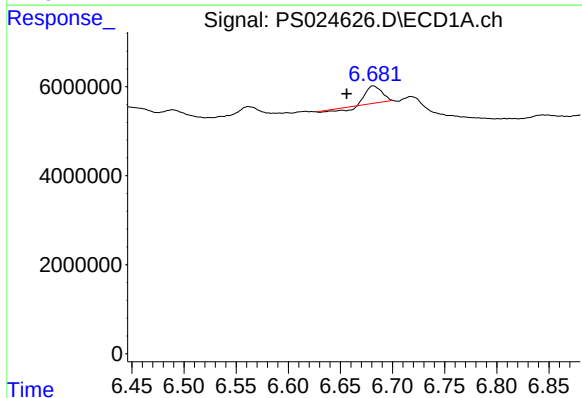


#6 MCP

R.T.: 6.682 min
Delta R.T.: 0.026 min
Response: 3513739
Conc: N.D.

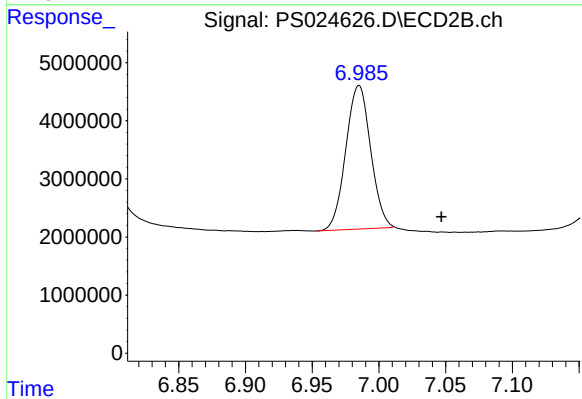

#6 MCP


R.T.: 6.985 min
Delta R.T.: -0.062 min
Response: 31998527
Conc: 16.24 ug/ml

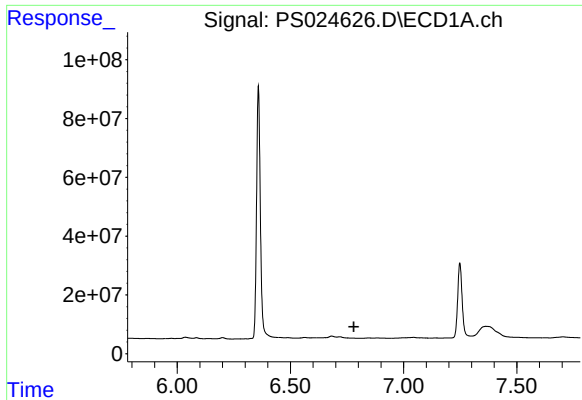

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

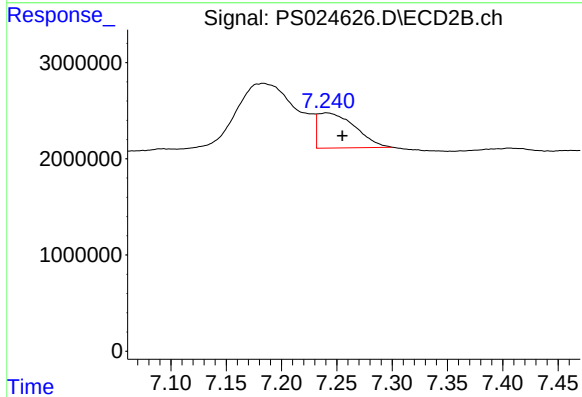


#7 MCPA

R.T.: 7.241 min
Delta R.T.: -0.014 min
Response: 8471632
Conc: 2.64 ug/ml

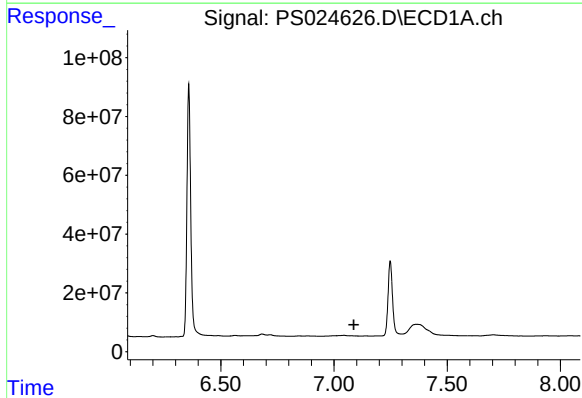


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

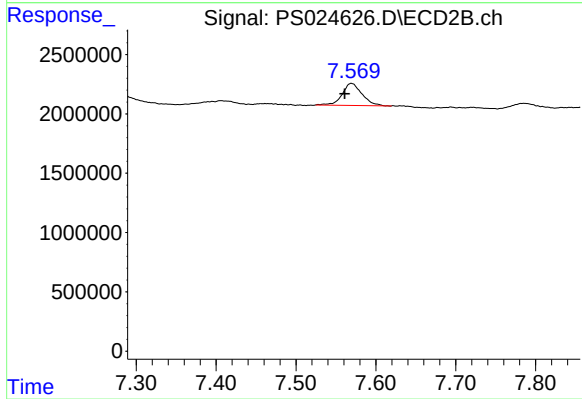

#8 DICHLORPROP


R.T.: 7.569 min
Delta R.T.: 0.009 min
Response: 3175149
Conc: 4.22 ng/ml

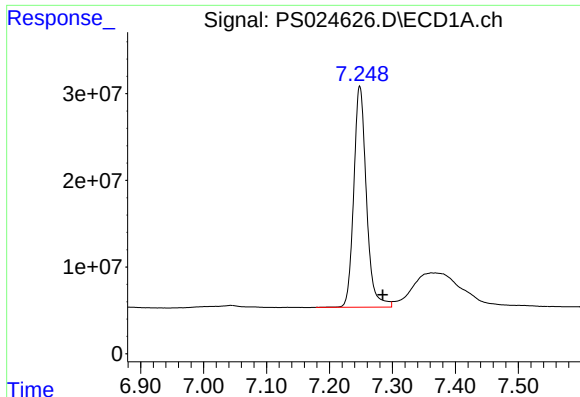

#9 2,4-D


R.T.: 7.248 min
Delta R.T.: -0.036 min
Response: 356310186
Conc: 128.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

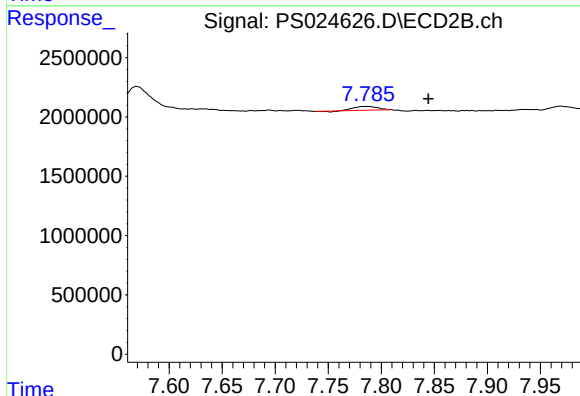


#9 2,4-D

R.T.: 7.786 min
Delta R.T.: -0.059 min
Response: 499364
Conc: N.D.

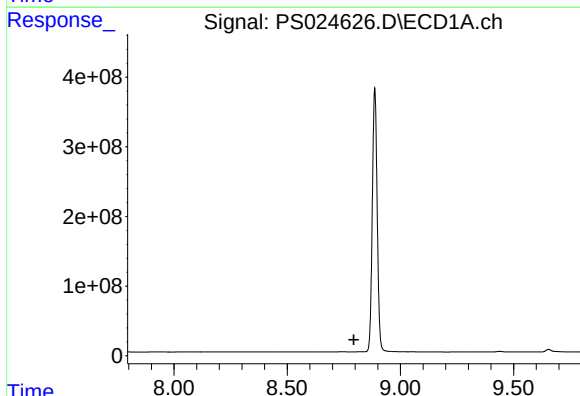


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.795 min
Response: 0
Conc: N.D.

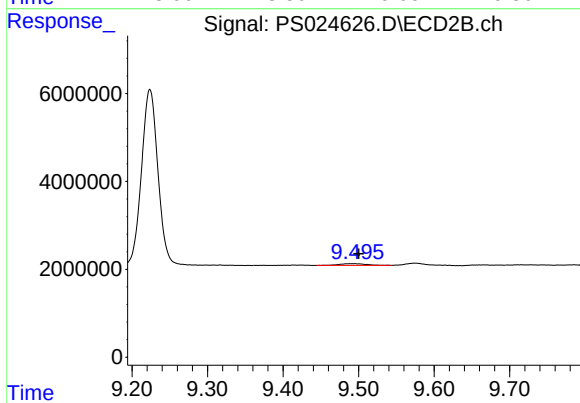

#13 2,4-DB


R.T.: 9.495 min
Delta R.T.: -0.006 min
Response: 1018643
Conc: 2.00 ng/ml

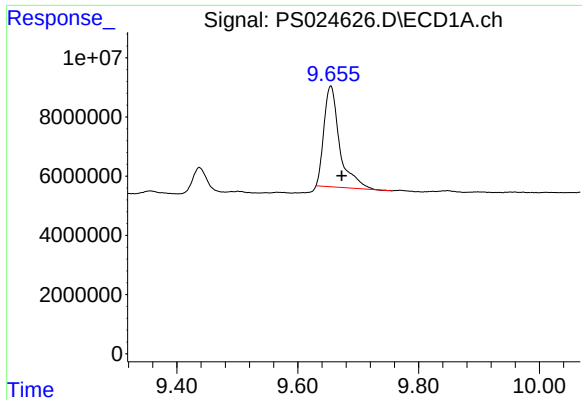

#15 Picloram


R.T.: 9.655 min
Delta R.T.: -0.019 min
Response: 61532049
Conc: 3.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

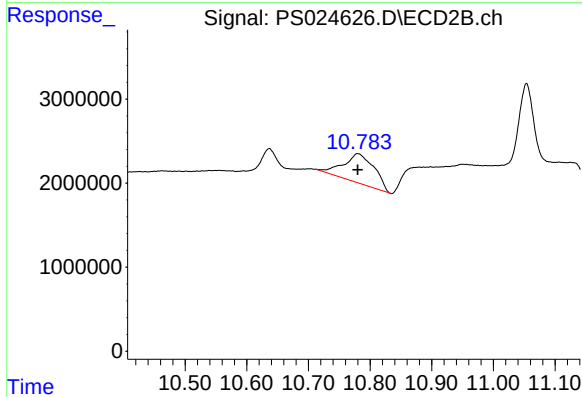


#15 Picloram

R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 12140608
Conc: 1.95 ng/ml

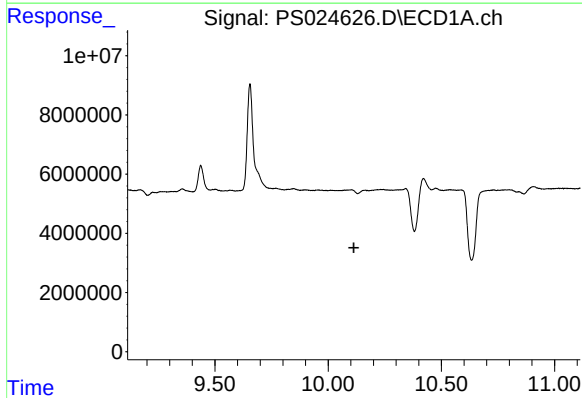

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.114 min
Response: 0
Conc: N.D.

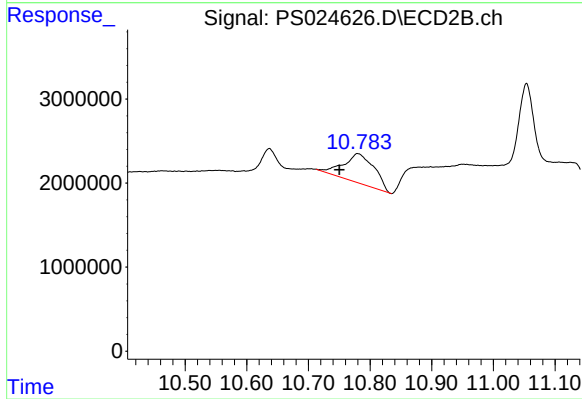

#16 DCPA

R.T.: 10.780 min
Delta R.T.: 0.030 min
Response: 12140608
Conc: 2.33 ng/ml